

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
 Data File : PL062504.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 21:49
 Operator : DD\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 16:26:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.413	3.952	85945121	143.7E6	49.966	48.894
28)	SA Decachlor...	8.127	8.989	68157999	96020320	42.485	45.878
Target Compounds							
2)	A alpha-BHC	3.845	4.338	127.5E6	218.1E6	50.019	49.094
3)	MA gamma-BHC...	4.124	4.620	113.6E6	200.6E6	49.050	48.032
4)	MA Heptachlor	4.421	5.126	104.2E6	184.6E6	48.569	46.281
5)	MB Aldrin	4.665	5.429	92699026	169.1E6	48.565	46.712
6)	B beta-BHC	4.373	4.792	46777672	85248112	48.972	45.272
7)	B delta-BHC	4.574	5.007	106.9E6	170.7E6	49.199	48.782
8)	B Heptachlo...	5.104	5.814	87471795	147.9E6	47.941	45.672
9)	A Endosulfan I	5.438	6.170	79286867	136.2E6	47.431	43.178
10)	B gamma-Chl...	5.329	6.048	84493432	146.4E6	46.900	43.485
11)	B alpha-Chl...	5.386	6.121	84427589	146.5E6	46.703	43.497
12)	B 4,4'-DDE	5.551	6.279	78263751	140.4E6	47.305	43.585
13)	MA Dieldrin	5.679	6.427	82831714	138.3E6	46.878	43.222
14)	MA Endrin	5.934	6.643	77577640	122.7E6	46.627	43.950
15)	B Endosulfa...	6.206	6.852	74606815	118.3E6	45.253	41.378
16)	A 4,4'-DDD	6.063	6.768	71691994	119.4E6	50.684	46.637
17)	MA 4,4'-DDT	6.302	7.067	53147511	87680456	39.824	39.051
18)	B Endrin al...	6.373	6.977	64583734	96945868	44.477	42.509
19)	B Endosulfa...	6.585	7.199	73096241	107.3E6	44.294	44.712
20)	A Methoxychlor	6.846	7.525	34719164	51142573	40.310	41.394
21)	B Endrin ke...	7.071	7.668	79701612	110.3E6	44.205	46.543
22)	Mirex	7.257	8.121	59636229	75789137	42.066	44.475
23)	Chlordane-1	4.298f	0.000	2193644	0	42.554	N.D. #
24)	Chlordane-2	0.000	5.429f	0	169.1E6	N.D.	1550.632 #
25)	Chlordane-3	5.329	6.048	84493432	146.4E6	551.780	362.399 #
26)	Chlordane-4	5.386	6.121	84427589	146.5E6	648.143	302.584 #
27)	Chlordane-5	6.206	0.000	74606815	0	1546.395	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
Data File : PL062504.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 21:49
Operator : DD\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 16:26:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

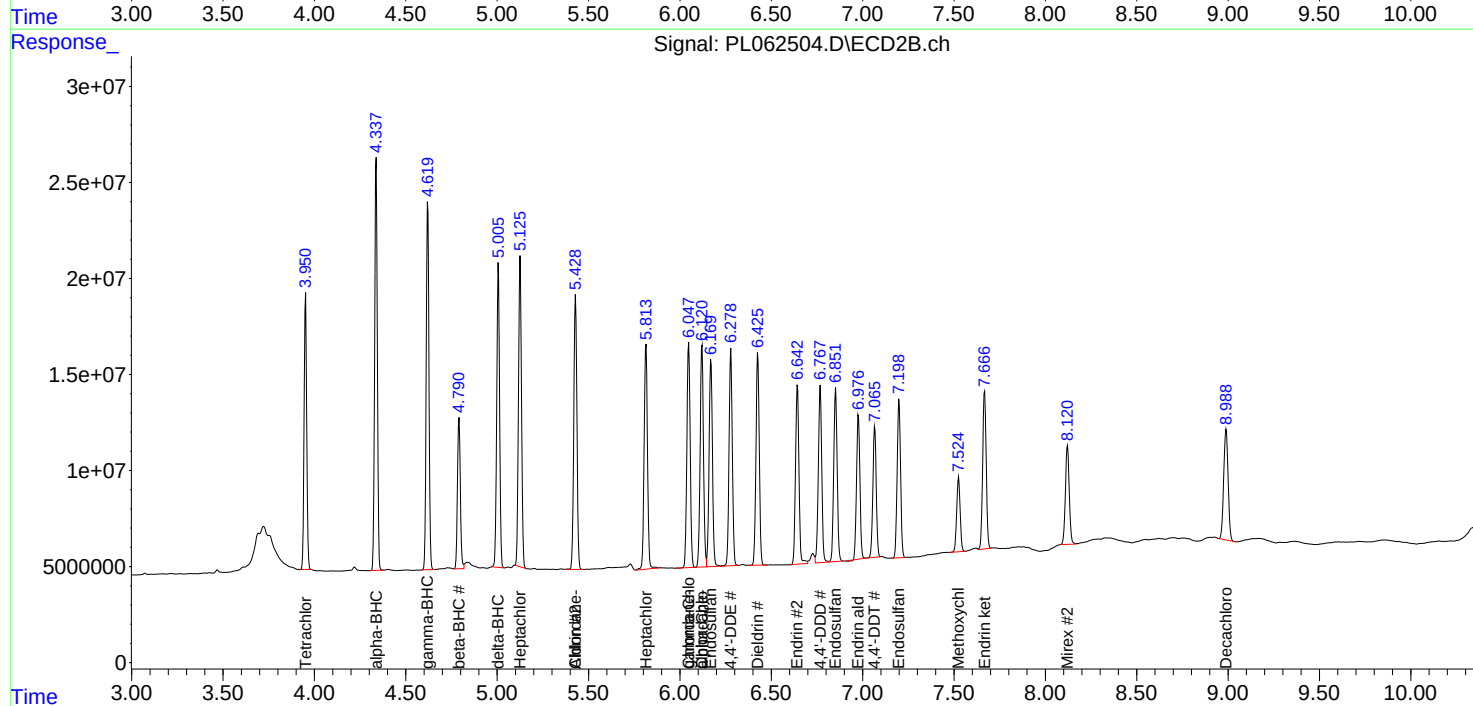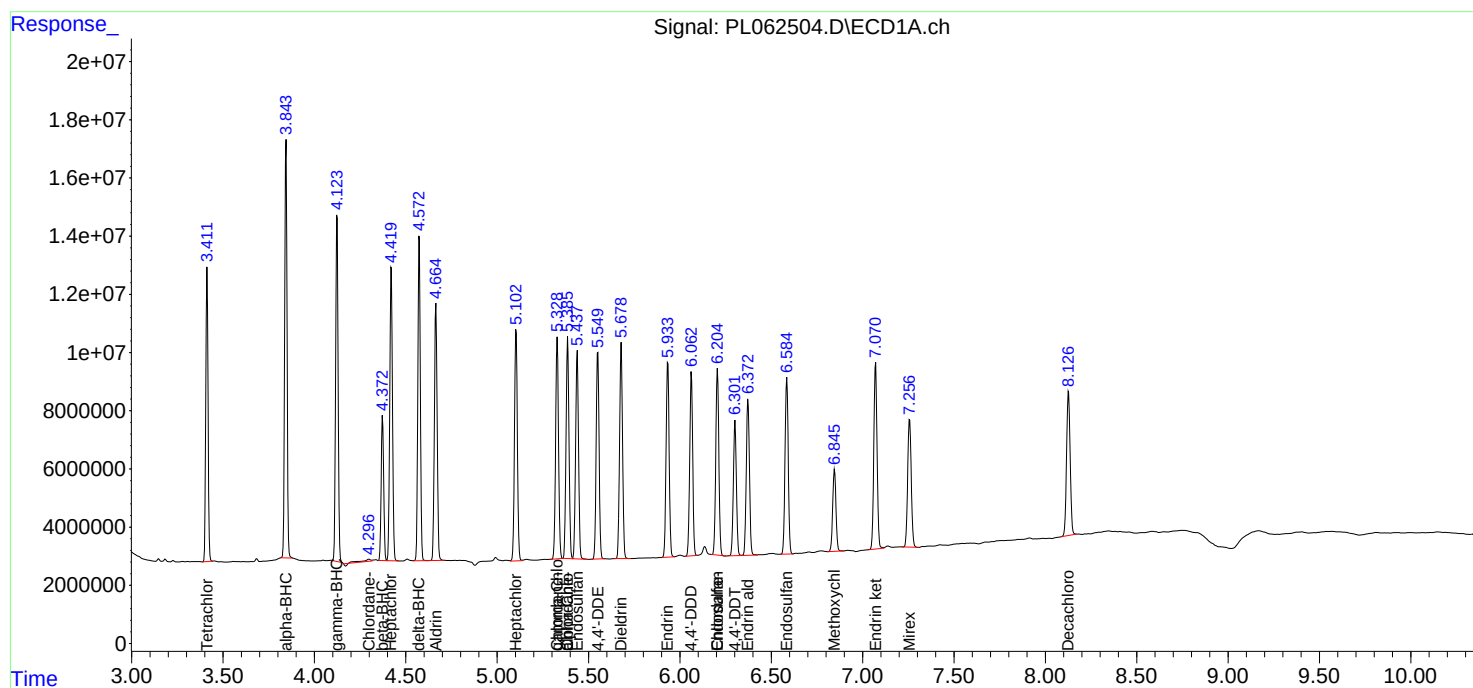


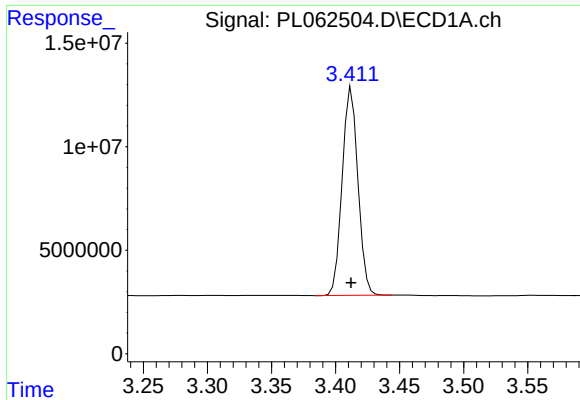

#1 Tetrachloro-m-xylene


R.T.: 3.413 min
Delta R.T.: 0.000 min
Response: 85945121
Conc: 49.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

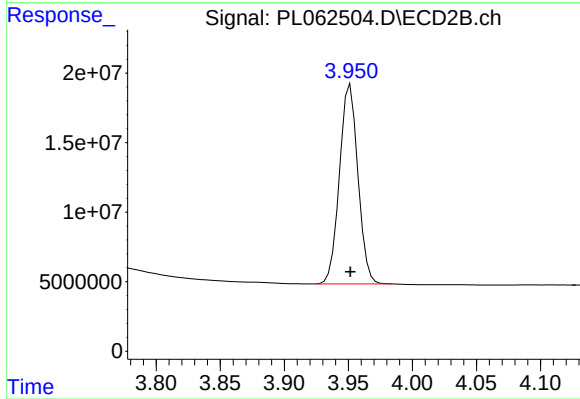


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 143686611
Conc: 48.89 ng/ml

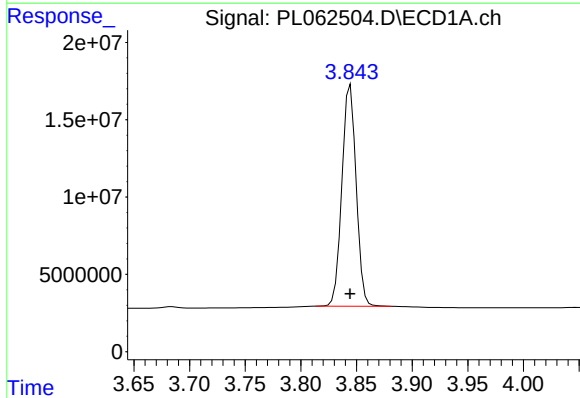


#2 alpha-BHC

R.T.: 3.845 min
Delta R.T.: 0.000 min
Response: 127534326
Conc: 50.02 ng/ml

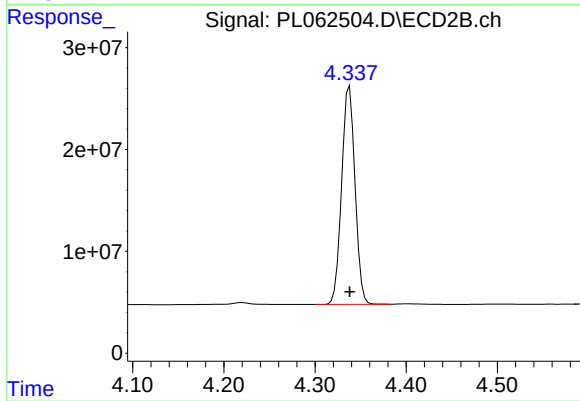

#2 alpha-BHC


R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 218136796
Conc: 49.09 ng/ml

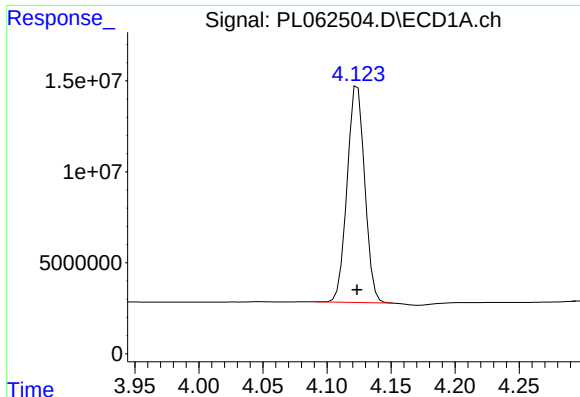

#3 gamma-BHC (Lindane)


R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 113633373
Conc: 49.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

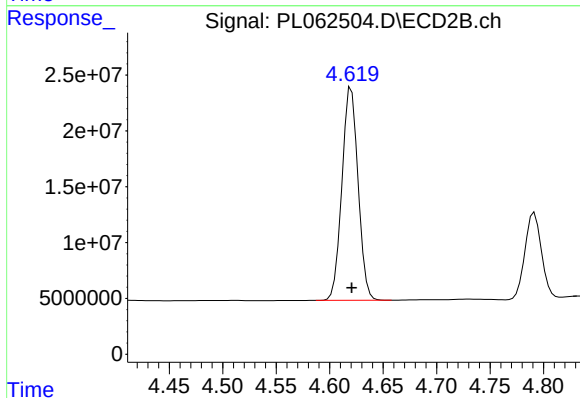


#3 gamma-BHC (Lindane)

R.T.: 4.620 min
Delta R.T.: 0.000 min
Response: 200569696
Conc: 48.03 ng/ml

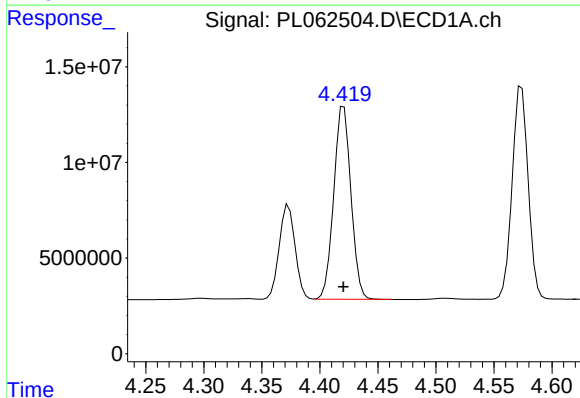


#4 Heptachlor

R.T.: 4.421 min
Delta R.T.: 0.000 min
Response: 104218230
Conc: 48.57 ng/ml

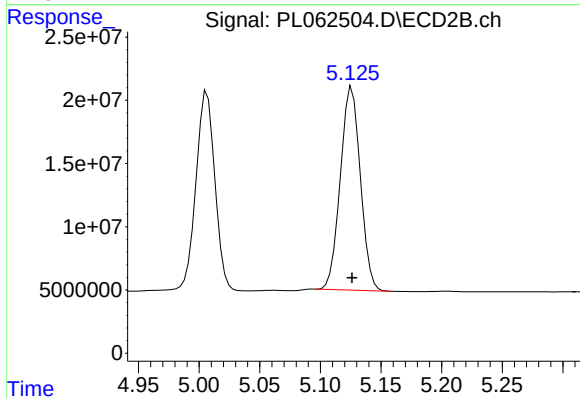

#4 Heptachlor


R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 184563246
Conc: 46.28 ng/ml

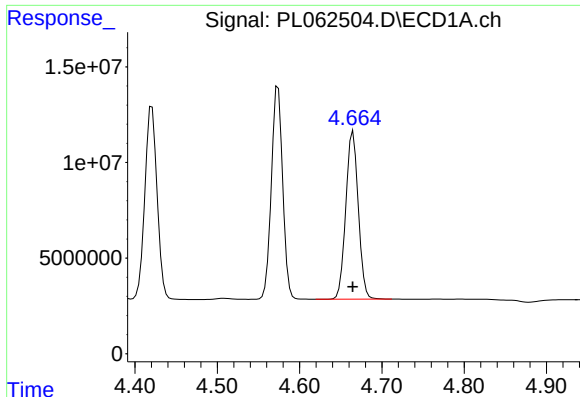

#5 Aldrin


R.T.: 4.665 min
Delta R.T.: 0.000 min
Response: 92699026
Conc: 48.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

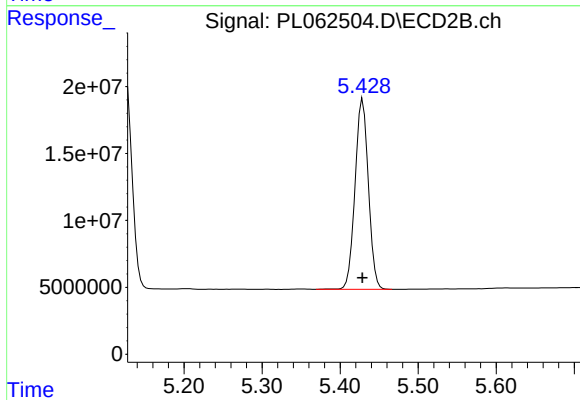


#5 Aldrin

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 169074650
Conc: 46.71 ng/ml

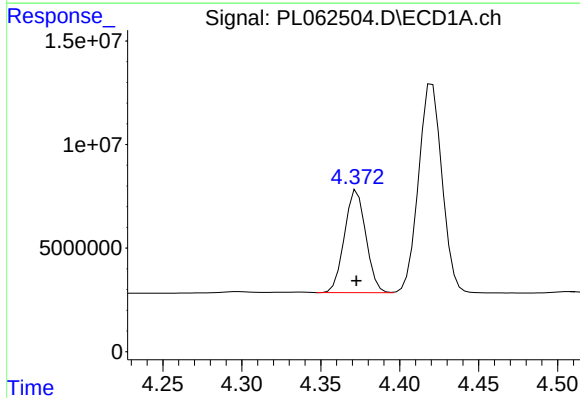


#6 beta-BHC

R.T.: 4.373 min
Delta R.T.: 0.000 min
Response: 46777672
Conc: 48.97 ng/ml

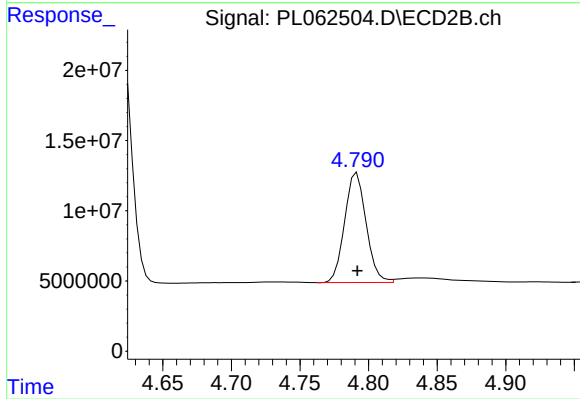

#6 beta-BHC


R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 85248112
Conc: 45.27 ng/ml

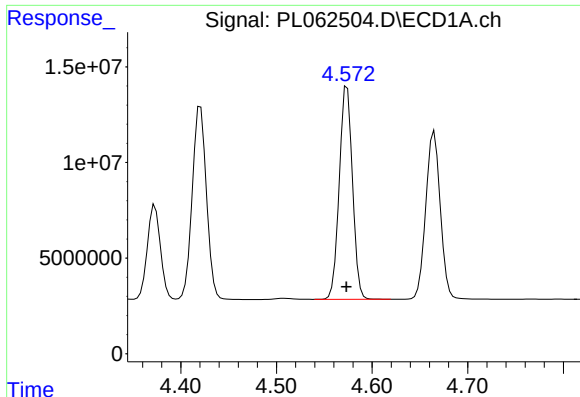

#7 delta-BHC


R.T.: 4.574 min
Delta R.T.: 0.000 min
Response: 106920023
Conc: 49.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

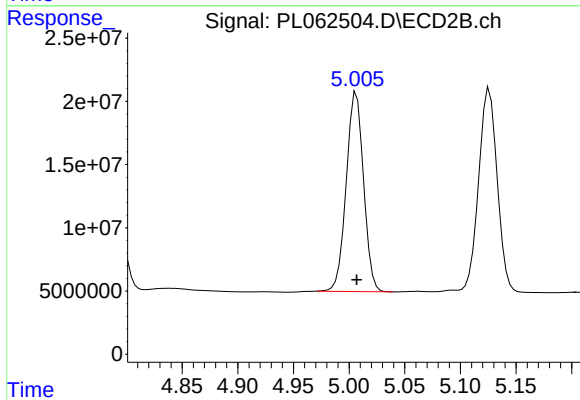


#7 delta-BHC

R.T.: 5.007 min
Delta R.T.: 0.000 min
Response: 170709648
Conc: 48.78 ng/ml

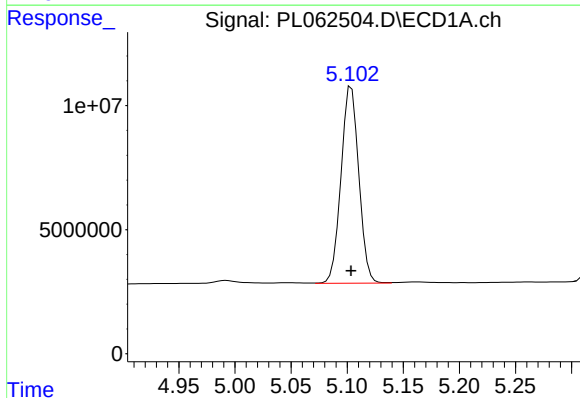


#8 Heptachlor epoxide

R.T.: 5.104 min
Delta R.T.: 0.000 min
Response: 87471795
Conc: 47.94 ng/ml

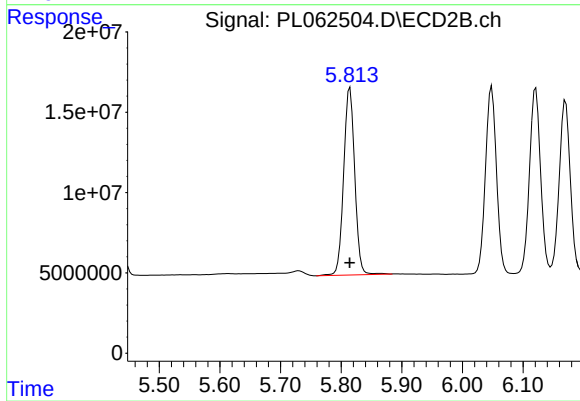

#8 Heptachlor epoxide


R.T.: 5.814 min
Delta R.T.: 0.000 min
Response: 147914134
Conc: 45.67 ng/ml

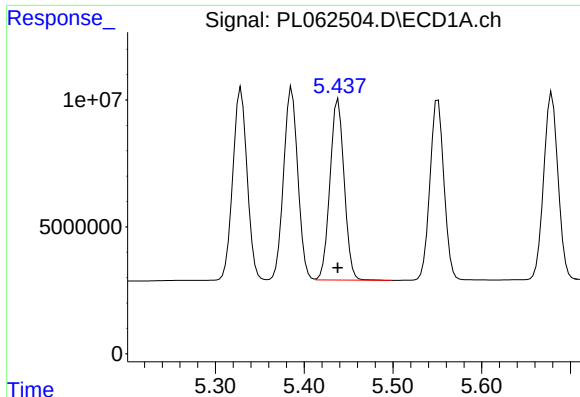

#9 Endosulfan I


R.T.: 5.438 min
Delta R.T.: 0.000 min
Response: 79286867
Conc: 47.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

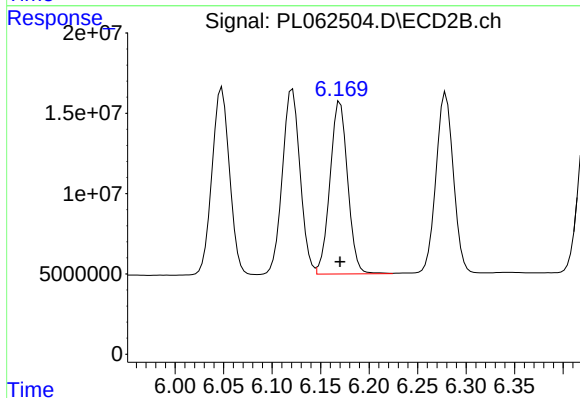


#9 Endosulfan I

R.T.: 6.170 min
Delta R.T.: 0.000 min
Response: 136175683
Conc: 43.18 ng/ml

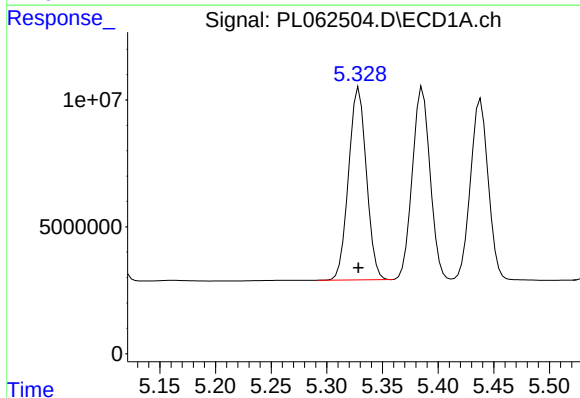


#10 gamma-Chlordane

R.T.: 5.329 min
Delta R.T.: 0.000 min
Response: 84493432
Conc: 46.90 ng/ml

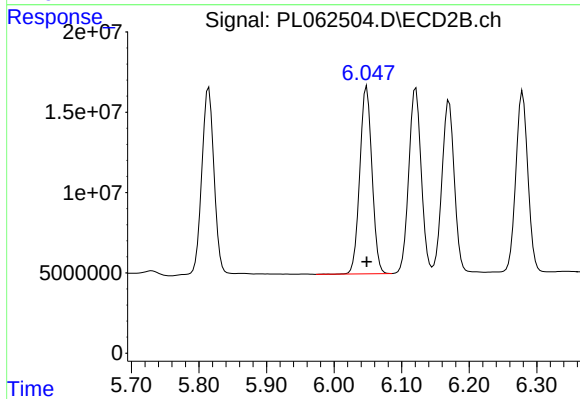

#10 gamma-Chlordane


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 146387647
Conc: 43.49 ng/ml

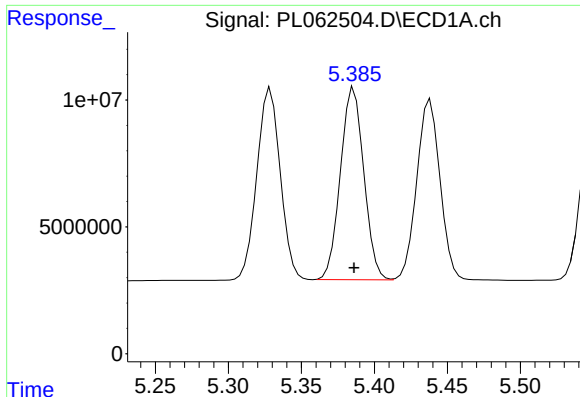

#11 alpha-Chlordane


R.T.: 5.386 min
Delta R.T.: 0.000 min
Response: 84427589
Conc: 46.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

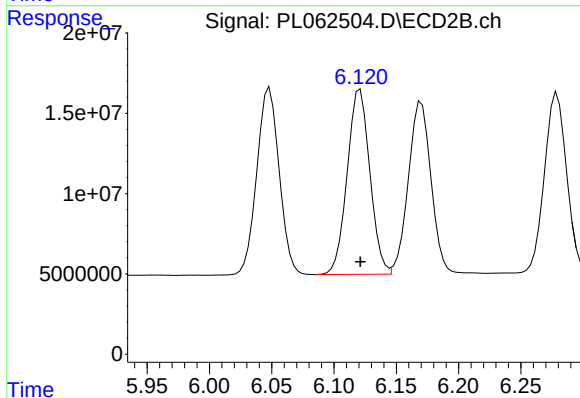


#11 alpha-Chlordane

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 146537418
Conc: 43.50 ng/ml

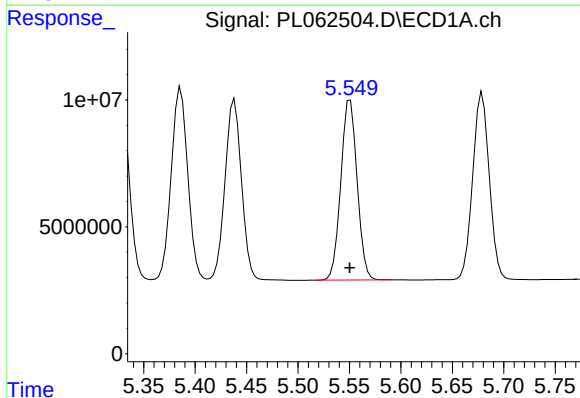


#12 4,4'-DDE

R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 78263751
Conc: 47.31 ng/ml

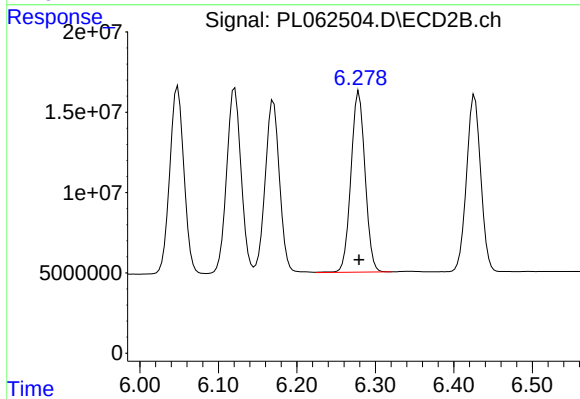

#12 4,4'-DDE


R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 140431469
Conc: 43.58 ng/ml

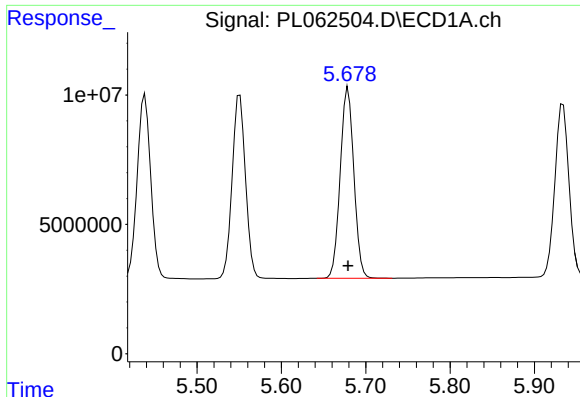

#13 Dieldrin


R.T.: 5.679 min
Delta R.T.: 0.000 min
Response: 82831714
Conc: 46.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

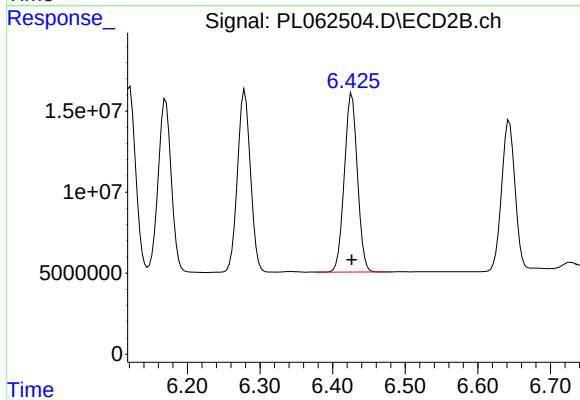


#13 Dieldrin

R.T.: 6.427 min
Delta R.T.: 0.000 min
Response: 138347712
Conc: 43.22 ng/ml

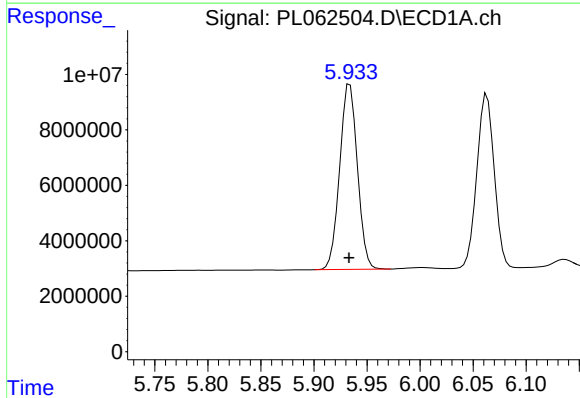


#14 Endrin

R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 77577640
Conc: 46.63 ng/ml

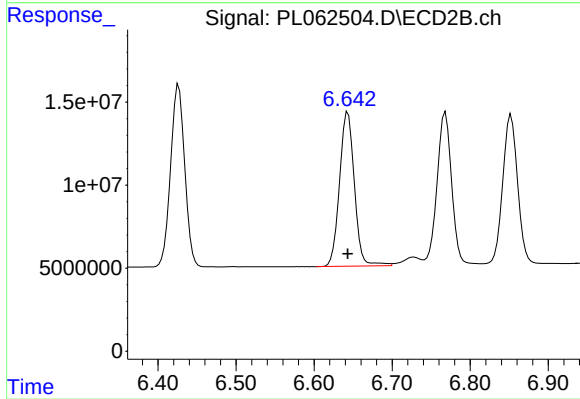

#14 Endrin


R.T.: 6.643 min
Delta R.T.: 0.000 min
Response: 122669347
Conc: 43.95 ng/ml

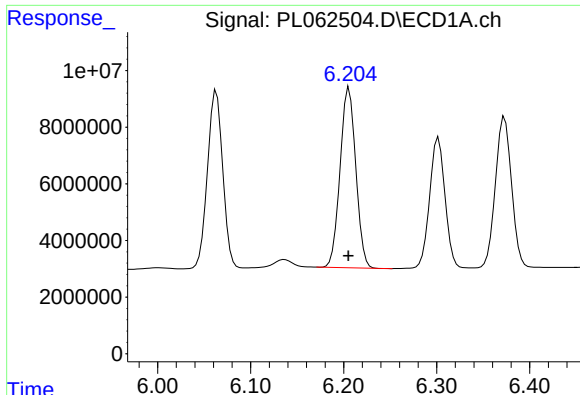

#15 Endosulfan II


R.T.: 6.206 min
Delta R.T.: 0.000 min
Response: 74606815
Conc: 45.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

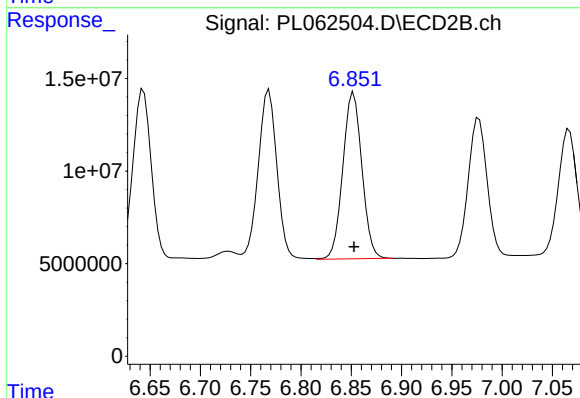


#15 Endosulfan II

R.T.: 6.852 min
Delta R.T.: 0.000 min
Response: 118285457
Conc: 41.38 ng/ml

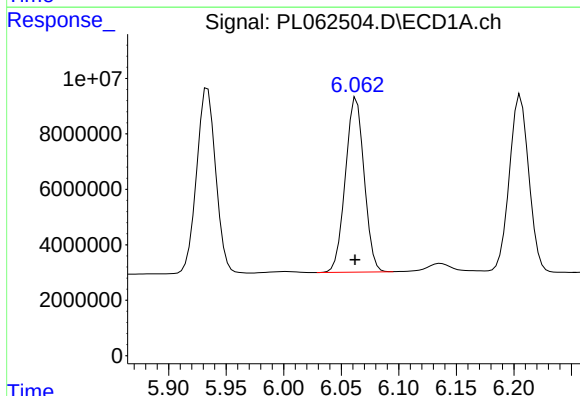


#16 4,4'-DDD

R.T.: 6.063 min
Delta R.T.: 0.001 min
Response: 71691994
Conc: 50.68 ng/ml

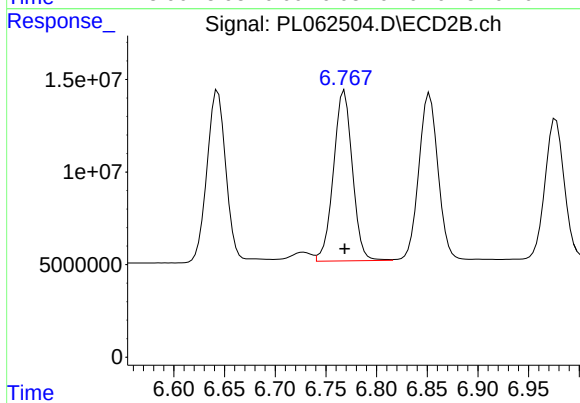

#16 4,4'-DDD


R.T.: 6.768 min
Delta R.T.: 0.000 min
Response: 119389308
Conc: 46.64 ng/ml

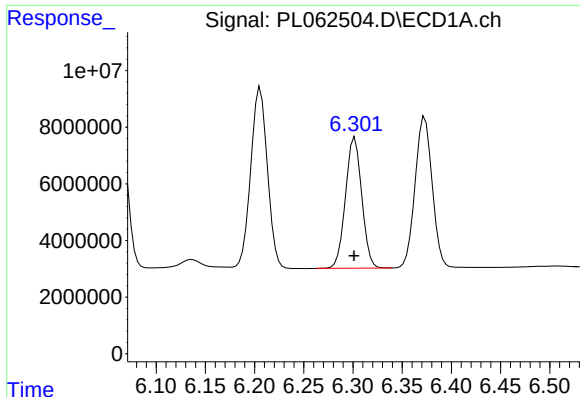

#17 4,4'-DDT


R.T.: 6.302 min
Delta R.T.: 0.000 min
Response: 53147511
Conc: 39.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

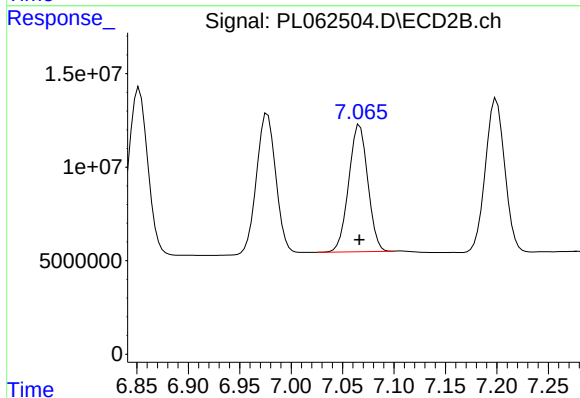


#17 4,4'-DDT

R.T.: 7.067 min
Delta R.T.: 0.000 min
Response: 87680456
Conc: 39.05 ng/ml

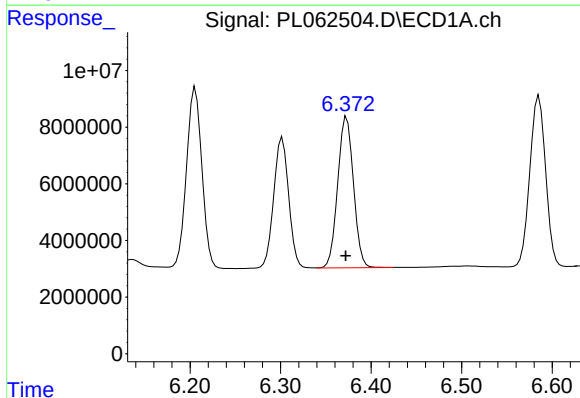


#18 Endrin aldehyde

R.T.: 6.373 min
Delta R.T.: 0.001 min
Response: 64583734
Conc: 44.48 ng/ml

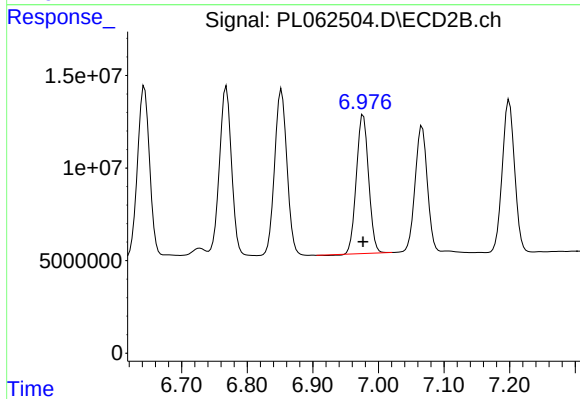

#18 Endrin aldehyde


R.T.: 6.977 min
Delta R.T.: 0.000 min
Response: 96945868
Conc: 42.51 ng/ml

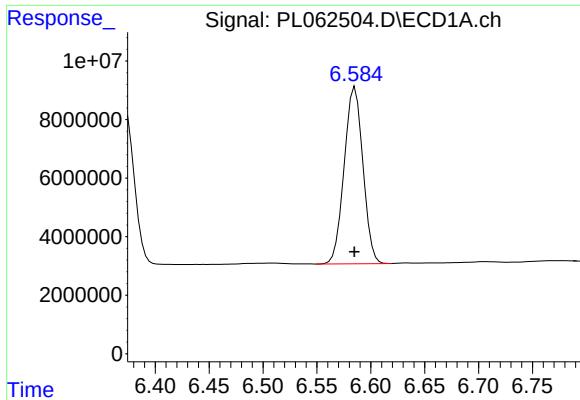

#19 Endosulfan Sulfate


R.T.: 6.585 min
Delta R.T.: 0.000 min
Response: 73096241
Conc: 44.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

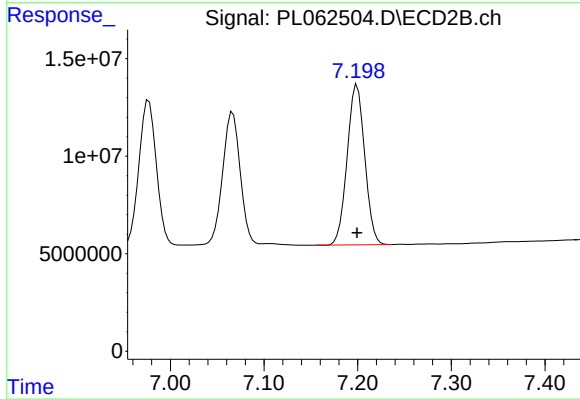


#19 Endosulfan Sulfate

R.T.: 7.199 min
Delta R.T.: 0.000 min
Response: 107273663
Conc: 44.71 ng/ml

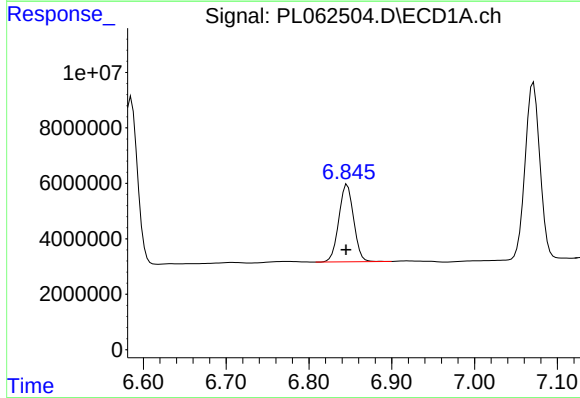


#20 Methoxychlor

R.T.: 6.846 min
Delta R.T.: 0.001 min
Response: 34719164
Conc: 40.31 ng/ml

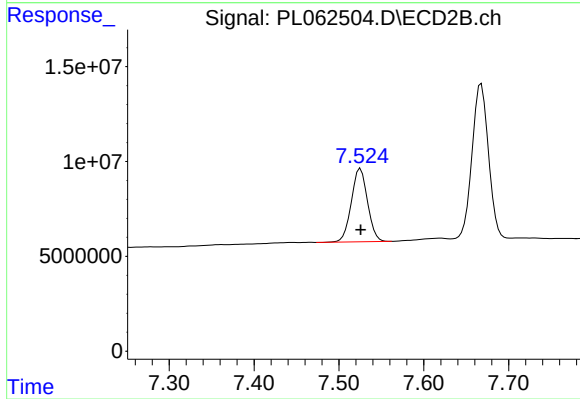

#20 Methoxychlor


R.T.: 7.525 min
Delta R.T.: 0.000 min
Response: 51142573
Conc: 41.39 ng/ml

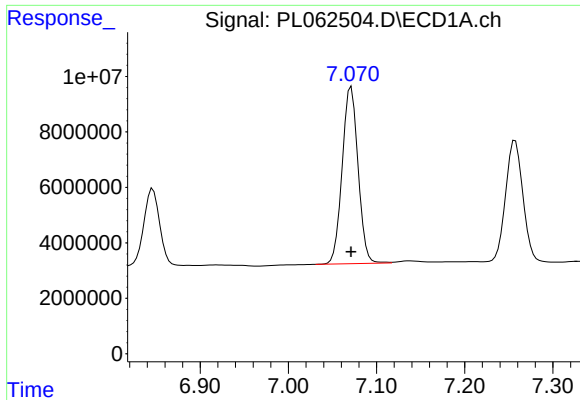

#21 Endrin ketone


R.T.: 7.071 min
Delta R.T.: 0.000 min
Response: 79701612
Conc: 44.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

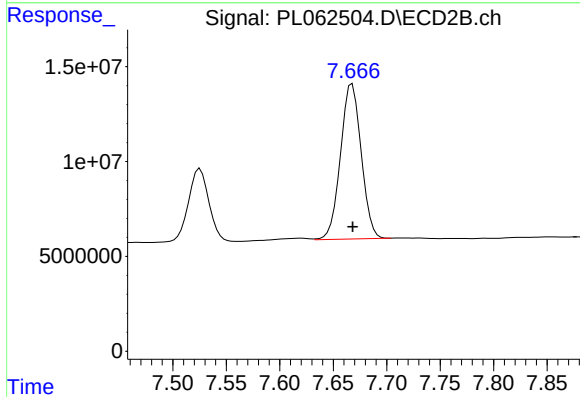


#21 Endrin ketone

R.T.: 7.668 min
Delta R.T.: 0.000 min
Response: 110298159
Conc: 46.54 ng/ml

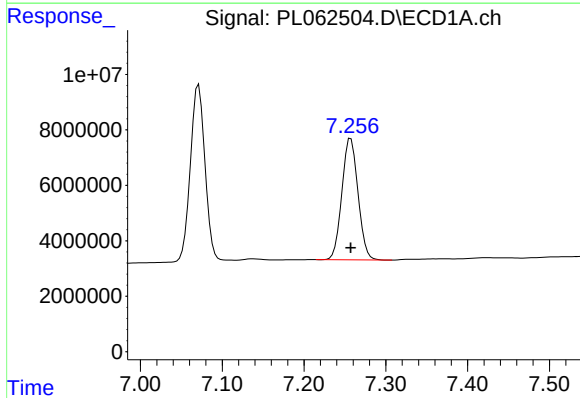


#22 Mirex

R.T.: 7.257 min
Delta R.T.: 0.000 min
Response: 59636229
Conc: 42.07 ng/ml

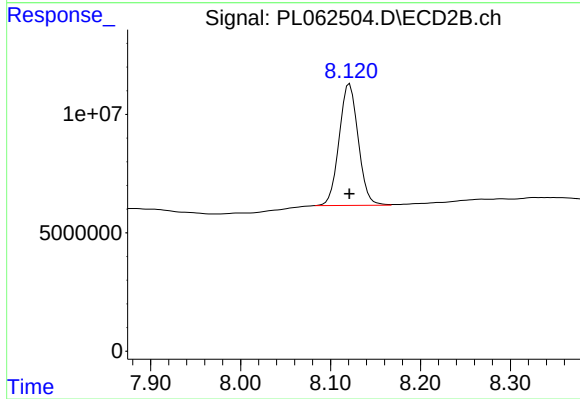

#22 Mirex


R.T.: 8.121 min
Delta R.T.: 0.000 min
Response: 75789137
Conc: 44.48 ng/ml

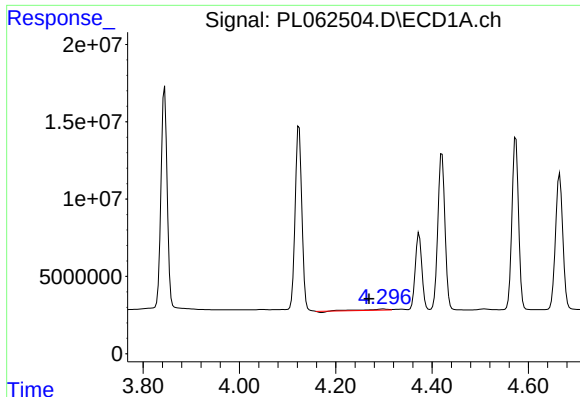

#23 Chlordane-1


R.T.: 4.298 min
Delta R.T.: 0.029 min
Response: 2193644
Conc: 42.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

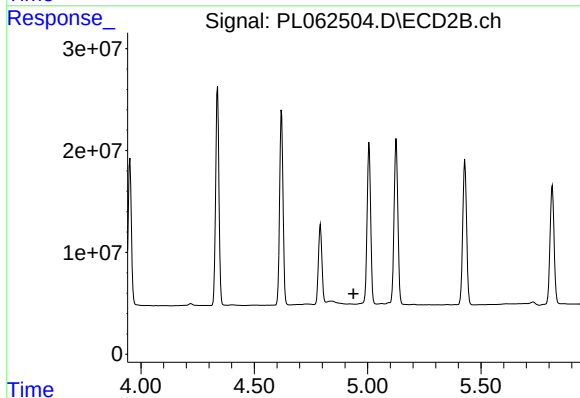


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

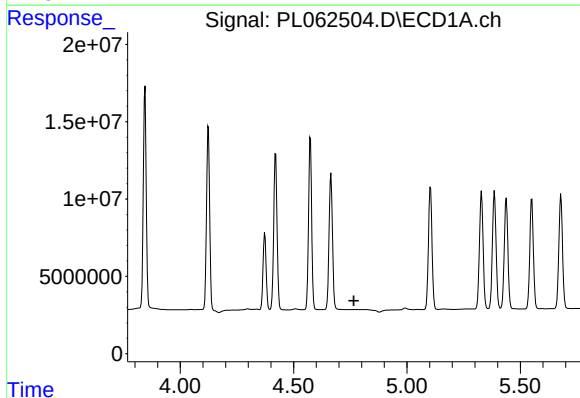


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.765 min
Response: 0
Conc: N.D.

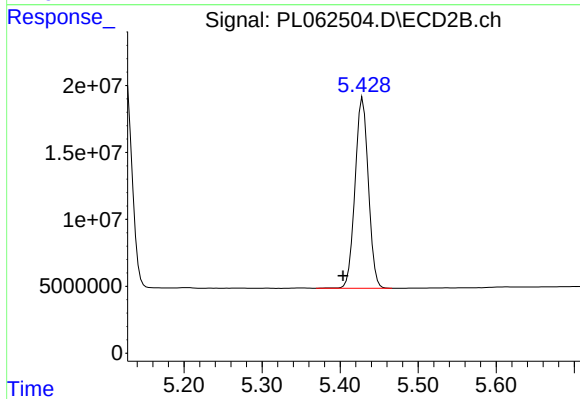

#24 Chlordane-2


R.T.: 5.429 min
Delta R.T.: 0.025 min
Response: 169074650
Conc: 1550.63 ng/ml

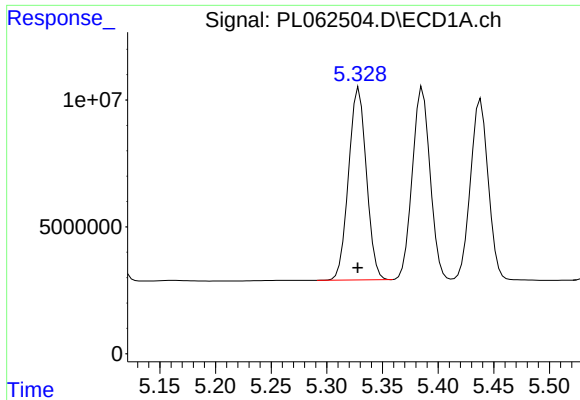

#25 Chlordane-3


R.T.: 5.329 min
Delta R.T.: 0.001 min
Response: 84493432
Conc: 551.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

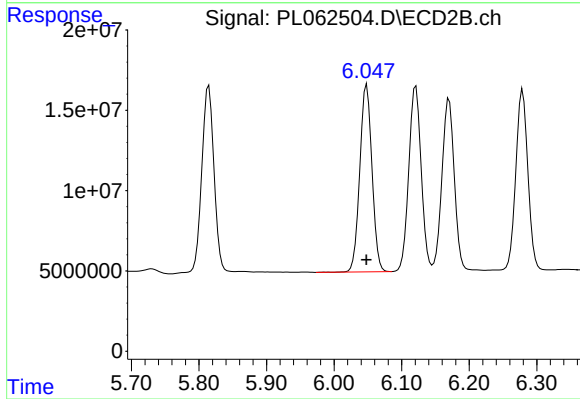


#25 Chlordane-3

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 146387647
Conc: 362.40 ng/ml

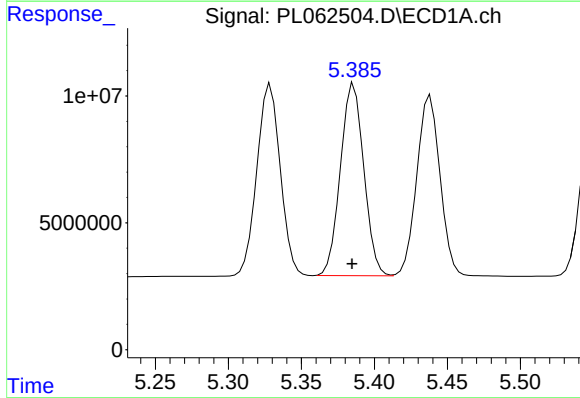


#26 Chlordane-4

R.T.: 5.386 min
Delta R.T.: 0.001 min
Response: 84427589
Conc: 648.14 ng/ml

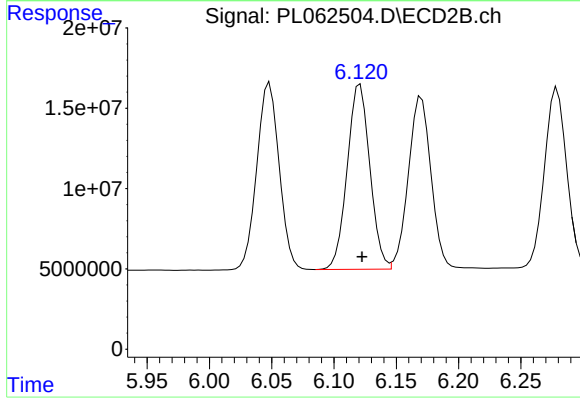

#26 Chlordane-4


R.T.: 6.121 min
Delta R.T.: -0.002 min
Response: 146537418
Conc: 302.58 ng/ml

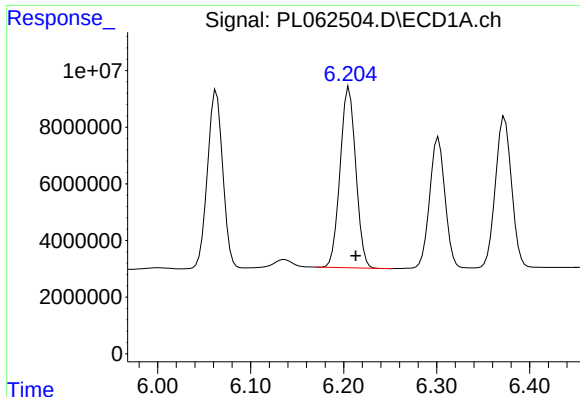

#27 Chlordane-5


R.T.: 6.206 min
Delta R.T.: -0.007 min
Response: 74606815
Conc: 1546.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

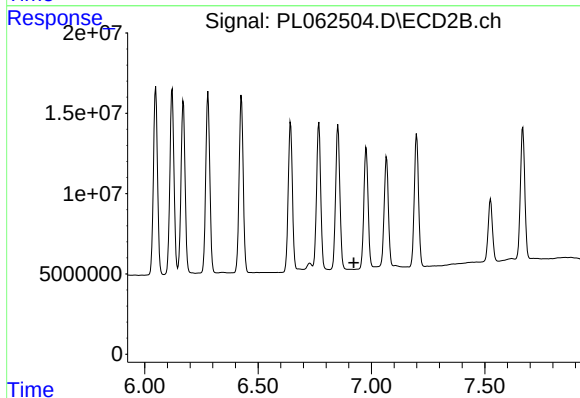


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.923 min
Response: 0
Conc: N.D.

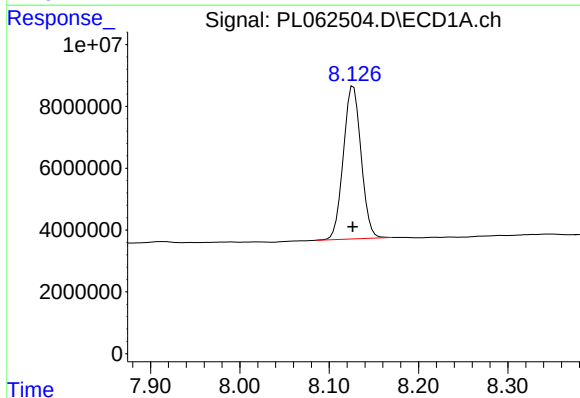

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 68157999
Conc: 42.48 ng/ml

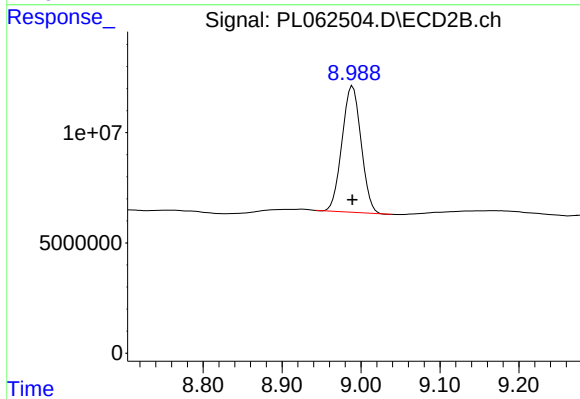

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 96020320
Conc: 45.88 ng/ml