

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
 Data File : PL062499.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 20:38
 Operator : DD\AJ
 Sample : L4455-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HP-627

Manual Integrations
 APPROVED

Ankita
 10/22/2020 5:34:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 09:16:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.952	101.7E6	40332080	59.140	13.724 #
28)	SA Decachlor...	8.128	8.989	34078752	56816802	21.242	27.147m#
Target Compounds							
12)	B 4,4'-DDE	5.549	6.279	9725796	17103126	5.879m	5.308

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
Data File : PL062499.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 20:38
Operator : DD\AJ
Sample : L4455-03
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HP-627


Manual Integrations
APPROVED

Ankita
10/22/2020 5:34:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 09:16:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

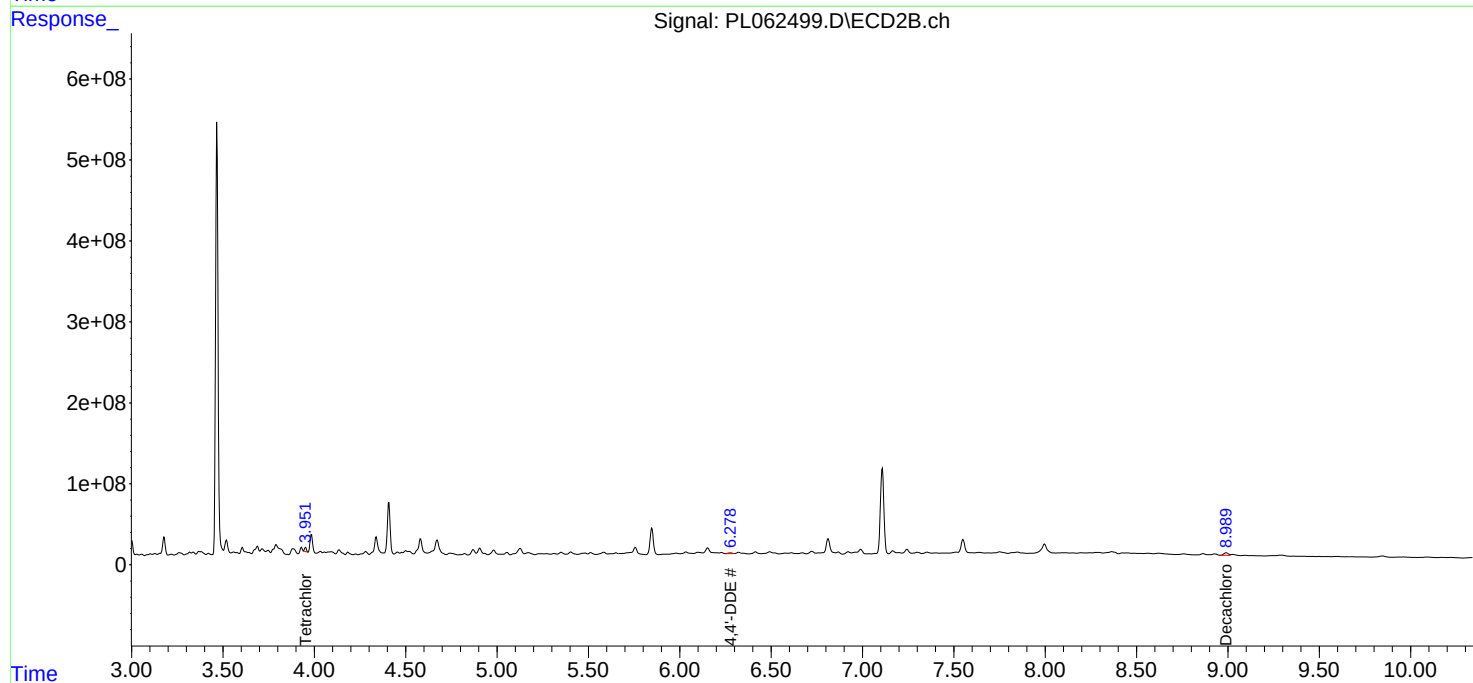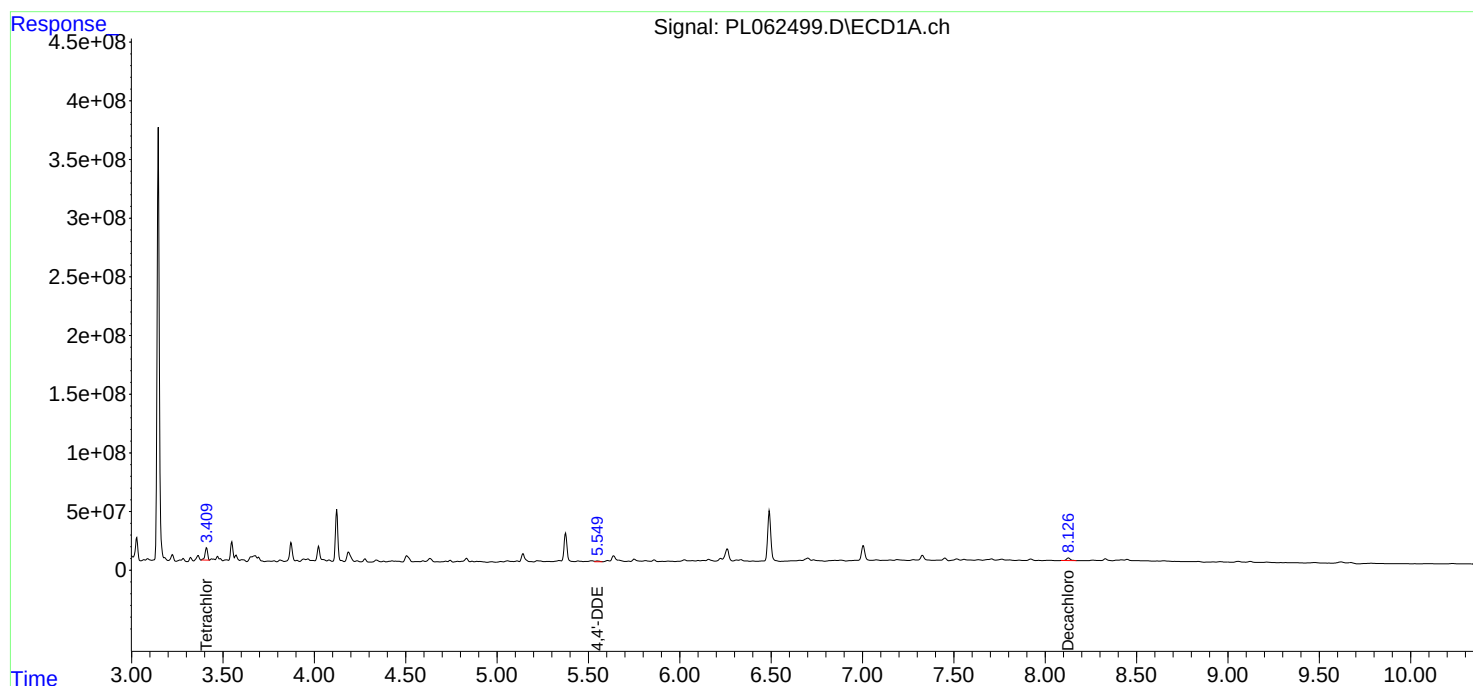

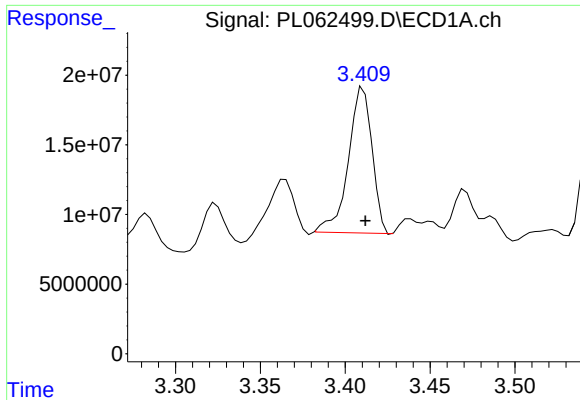


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: -0.001 min
Response: 101724828
Conc: 59.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
HP-627


Manual Integrations
APPROVED

Ankita
10/22/2020 5:34:51 PM

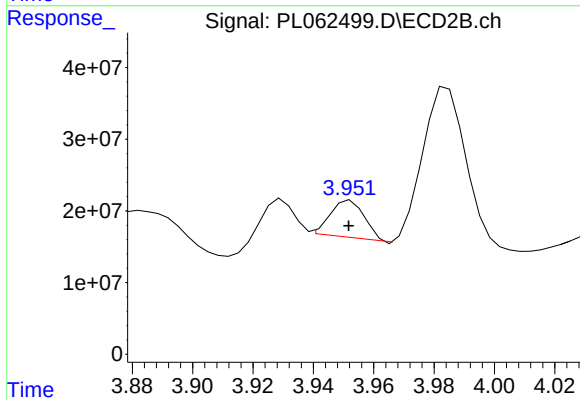


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 40332080
Conc: 13.72 ng/ml

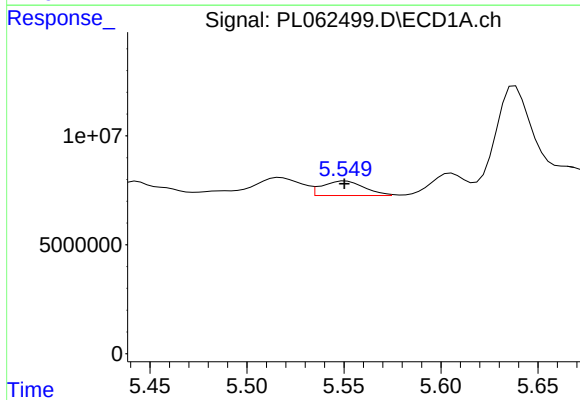


#12 4,4'-DDE

R.T.: 5.549 min
Delta R.T.: 0.000 min
Response: 9725796
Conc: 5.88 ng/ml m

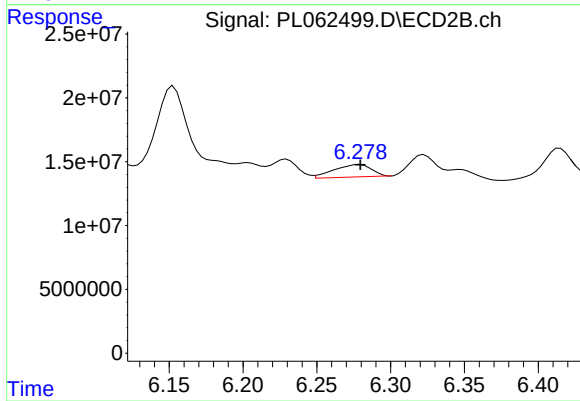

#12 4,4'-DDE

R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 17103126
Conc: 5.31 ng/ml

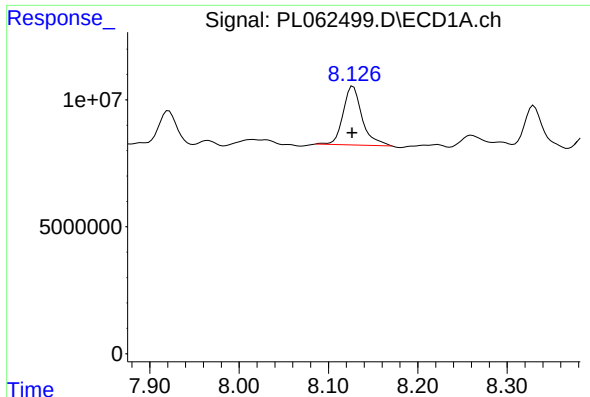


#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.001 min
Response: 34078752
Conc: 21.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
HP-627

Manual Integrations
APPROVED

Ankita
10/22/2020 5:34:51 PM

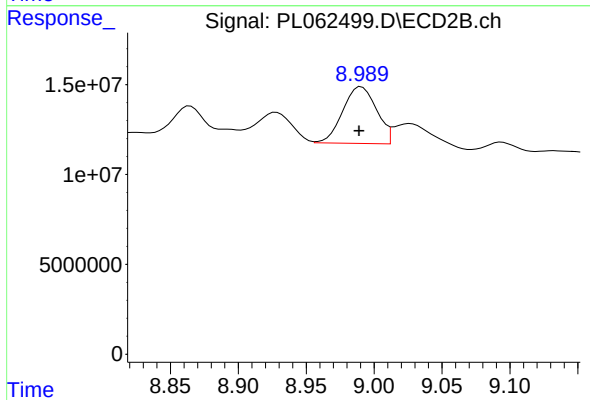

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 56816802
Conc: 27.15 ng/ml m