

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
 Data File : PL062501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 21:06
 Operator : DD\AJ
 Sample : L4455-03RE
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HP-627RE

Manual Integrations
 APPROVED

Ankita
 10/22/2020 5:34:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 09:16:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.943	100.7E6	61455304	58.517	20.912 #
28)	SA Decachlor...	8.127	9.002	32380576	47648904	20.184	22.766m
Target Compounds							
12)	B 4,4'-DDE	5.549	6.293	7877629	17817928	4.761m	5.530

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
Data File : PL062501.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 21:06
Operator : DD\AJ
Sample : L4455-03RE
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HP-627RE


Manual Integrations
APPROVED

Ankita
10/22/2020 5:34:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 09:16:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

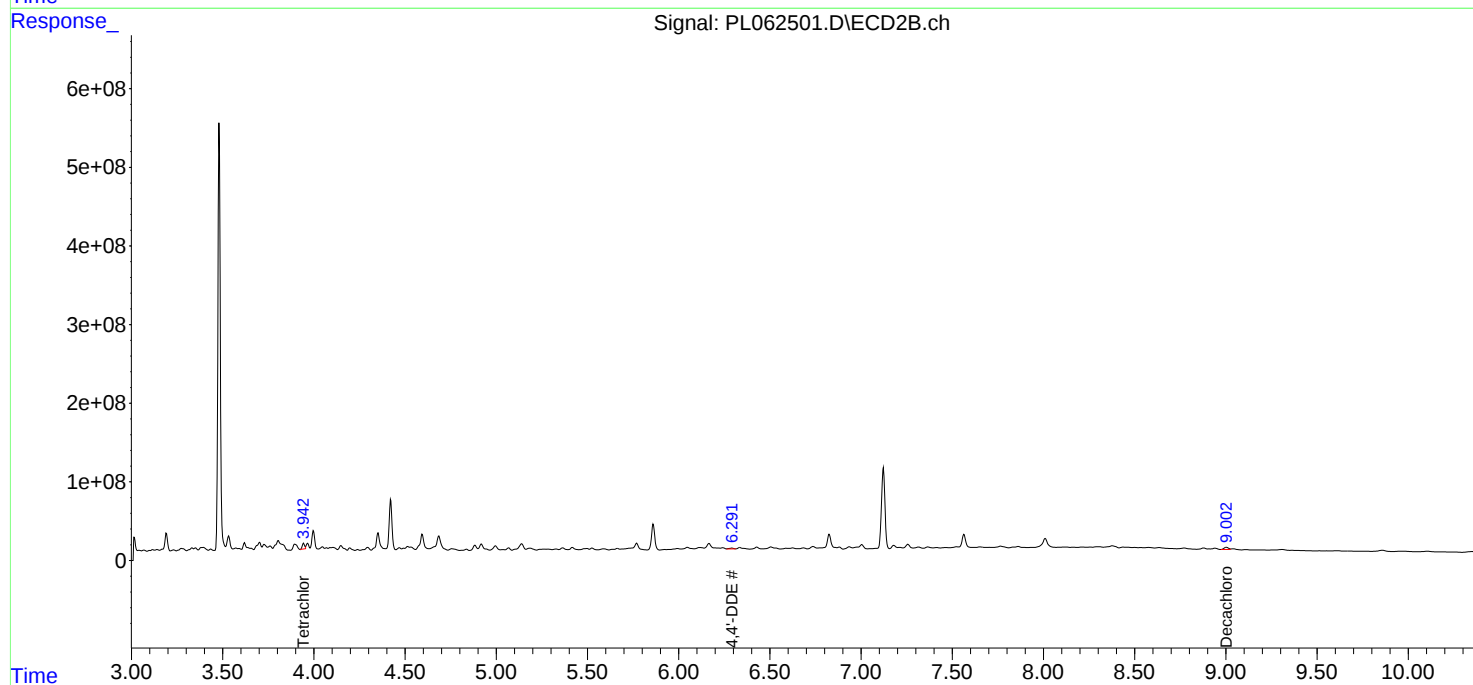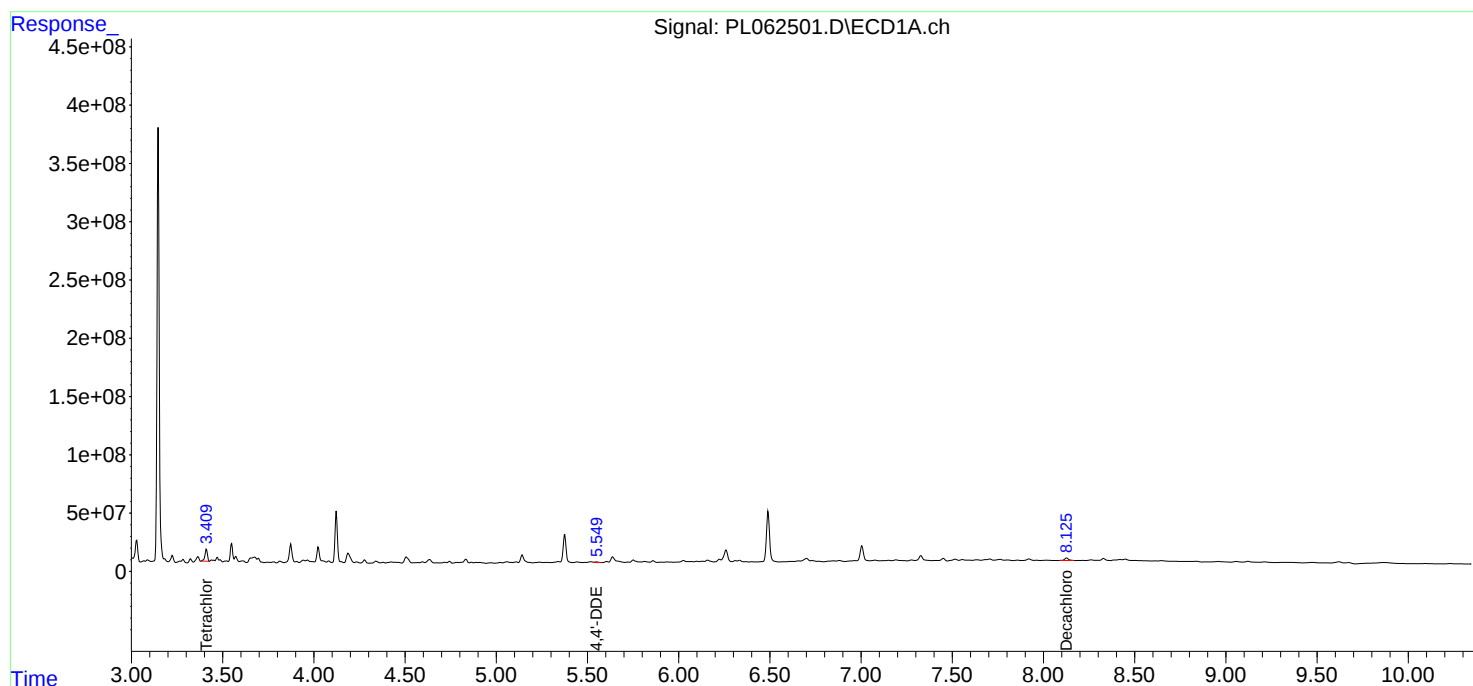

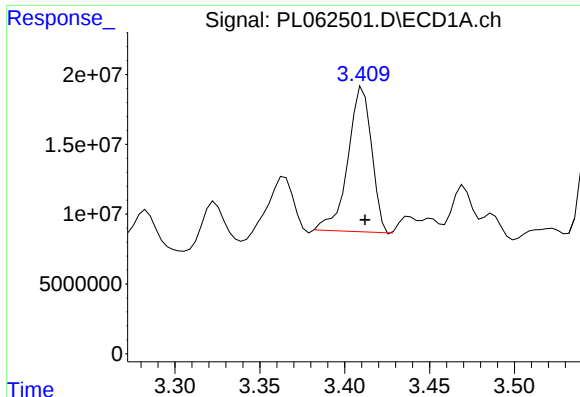


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: -0.001 min
Response: 100653766
Conc: 58.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
HP-627RE


Manual Integrations
APPROVED

Ankita
10/22/2020 5:34:54 PM

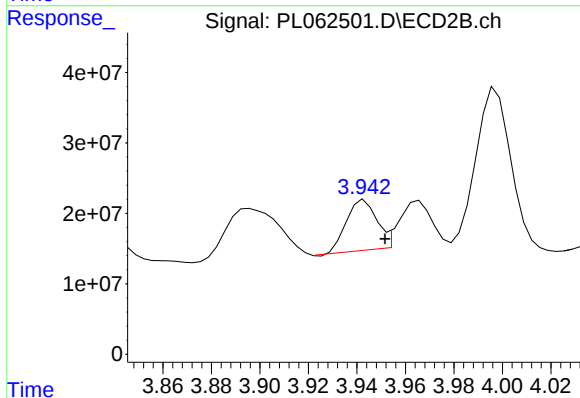


#1 Tetrachloro-m-xylene

R.T.: 3.943 min
Delta R.T.: -0.009 min
Response: 61455304
Conc: 20.91 ng/ml

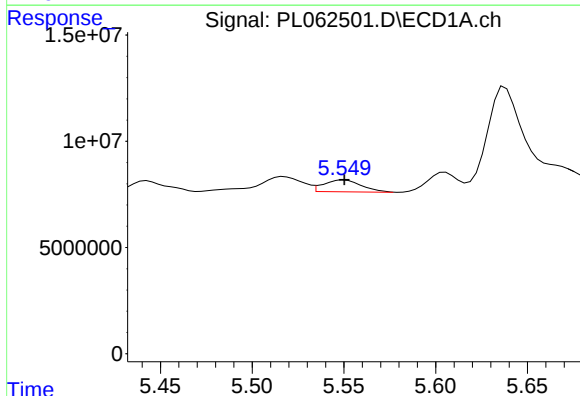


#12 4,4'-DDE

R.T.: 5.549 min
Delta R.T.: -0.001 min
Response: 7877629
Conc: 4.76 ng/ml m

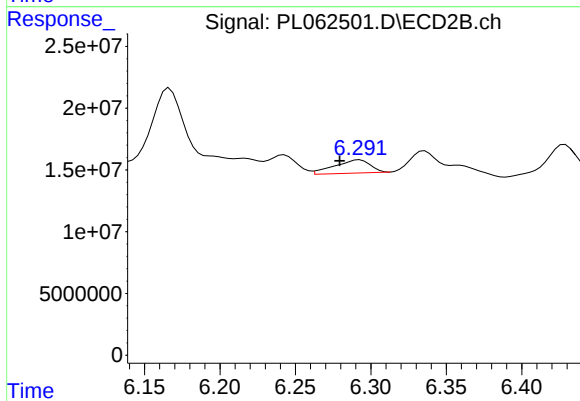

#12 4,4'-DDE

R.T.: 6.293 min
Delta R.T.: 0.013 min
Response: 17817928
Conc: 5.53 ng/ml

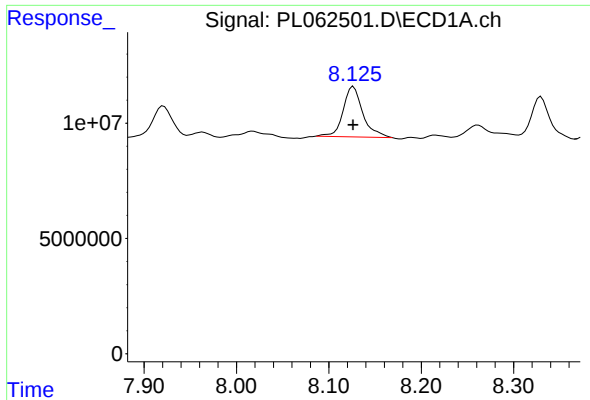

#28 Decachlorobiphenyl

R.T.: 8.127 min

Delta R.T.: 0.000 min


Response: 32380576

Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
HP-627RE

Manual Integrations
APPROVED

Ankita
10/22/2020 5:34:54 PM

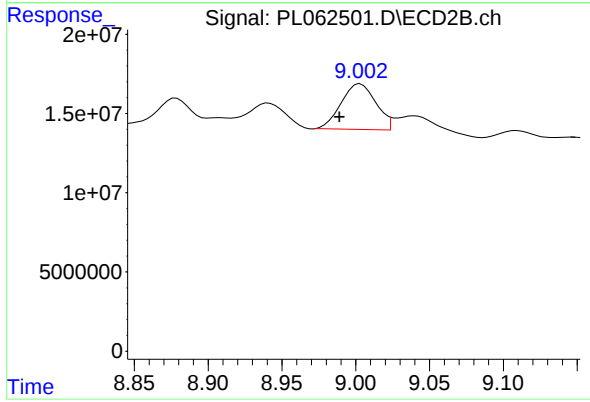

#28 Decachlorobiphenyl

R.T.: 9.002 min

Delta R.T.: 0.013 min

Response: 47648904

Conc: 22.77 ng/ml m