

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
 Data File : PL062502.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 21:21
 Operator : DD\AJ
 Sample : L4456-03RE
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HP-640RE

Manual Integrations
 APPROVED

Ankita
 10/22/2020 5:34:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 09:16:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.952	53793896	45064686	31.274m	15.335 #
28)	SA Decachlor...	8.127	8.989	31363462	35691870	19.550m	17.053

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
Data File : PL062502.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 21:21
Operator : DD\AJ
Sample : L4456-03RE
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HP-640RE


Manual Integrations
APPROVED

Ankita
10/22/2020 5:34:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 09:16:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

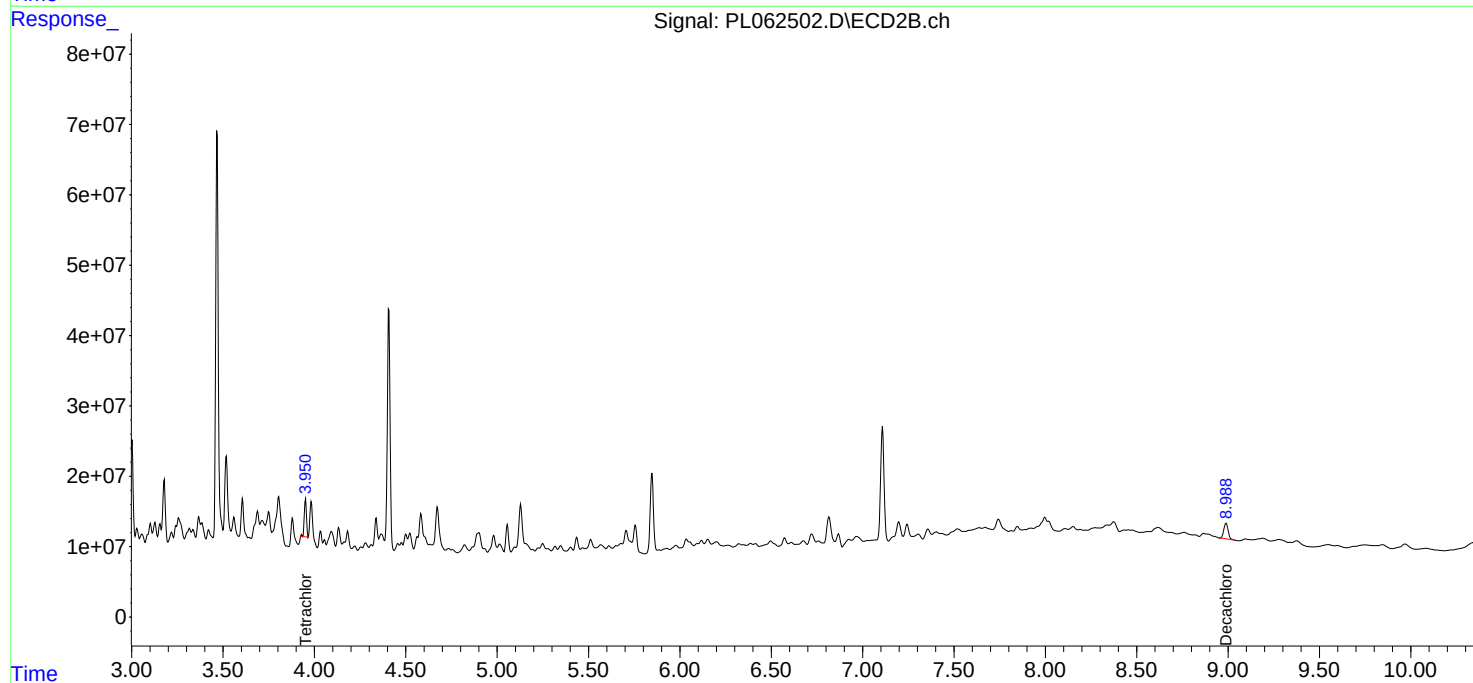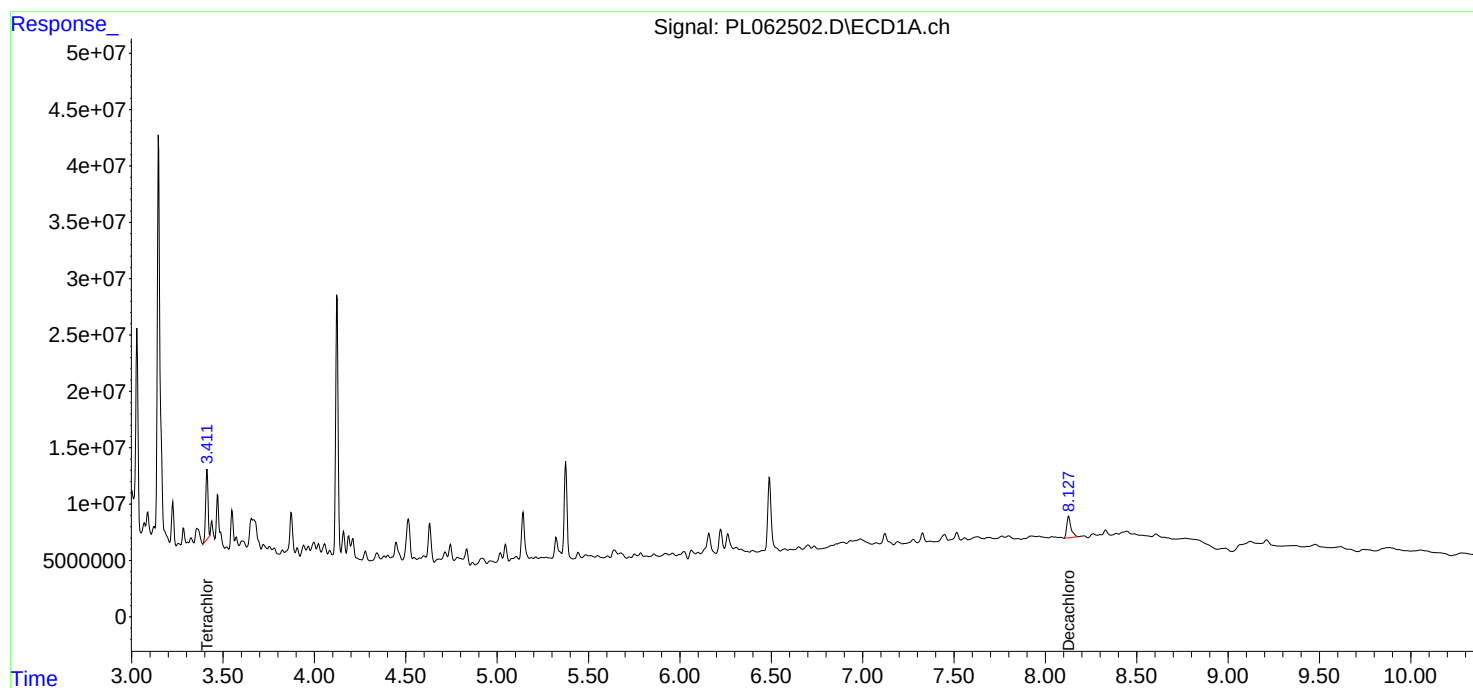

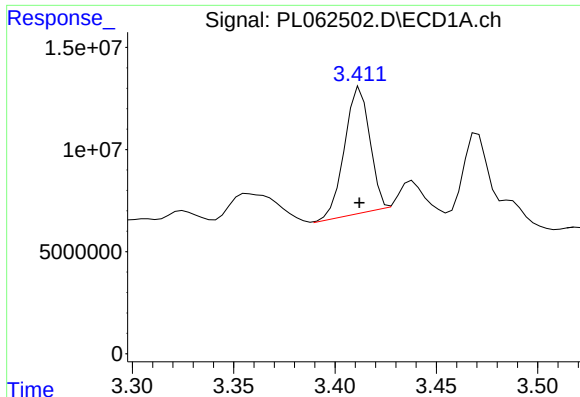

#1 Tetrachloro-m-xylene

R.T.: 3.411 min

Delta R.T.: -0.001 min


Response: 53793896

Conc: 31.27 ng/ml m

Instrument :
ECD_L
ClientSampleId :
HP-640RE

Manual Integrations
APPROVED

Ankita
10/22/2020 5:34:57 PM

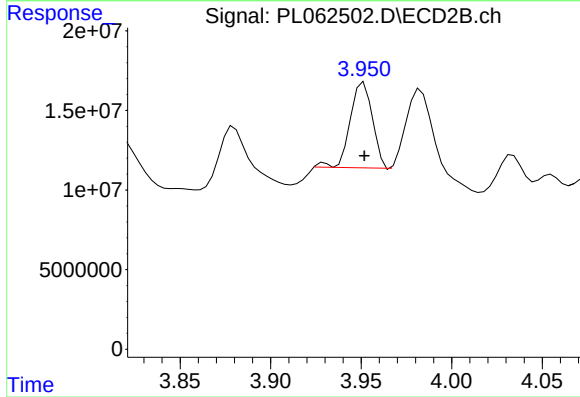


#1 Tetrachloro-m-xylene

R.T.: 3.952 min

Delta R.T.: 0.000 min

Response: 45064686

Conc: 15.33 ng/ml

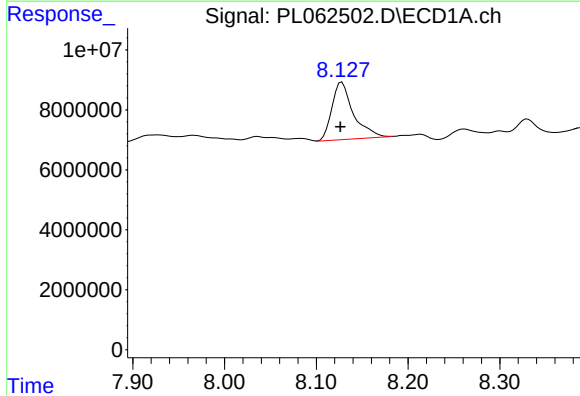


#28 Decachlorobiphenyl

R.T.: 8.127 min

Delta R.T.: 0.000 min

Response: 31363462

Conc: 19.55 ng/ml m

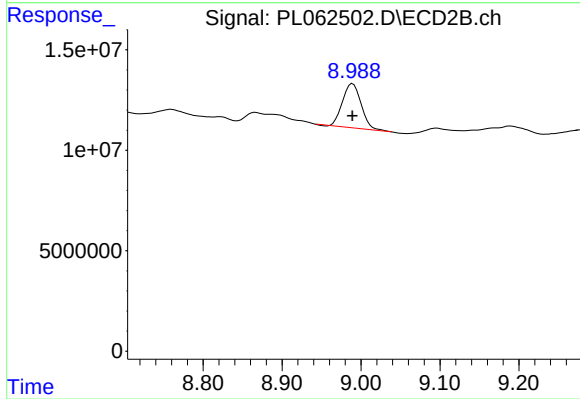

#28 Decachlorobiphenyl

R.T.: 8.989 min

Delta R.T.: 0.000 min

Response: 35691870

Conc: 17.05 ng/ml