

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102121\
 Data File : PL070452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2021 15:06
 Operator : AR\AJ
 Sample : M4290-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:53:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.564	7346413	17758015	14.681	13.426
28)	SA Decachlor...	10.400	11.495	9129723	15628025	13.194	12.914
Target Compounds							
2)	A alpha-BHC	0.000	6.129f	0	2149176	N.D.	1.099 #
11)	B alpha-Chl...	0.000	8.381	0	655420	N.D.	0.416 #
14)	MA Endrin	0.000	8.996f	0	529369	N.D.	0.421 #
15)	B Endosulfa...	0.000	9.209	0	1962127	N.D.	1.642 #
16)	A 4,4'-DDD	0.000	9.106	0	1585113	N.D.	1.342 #
17)	MA 4,4'-DDT	8.477	9.429	997244	1279767	1.630	0.979 #
18)	B Endrin al...	0.000	9.342	0	1202786	N.D.	1.247 #
20)	A Methoxychlor	9.049f	0.000	602233	0	1.613	N.D. #
26)	Chlordane-4	0.000	8.381	0	655420	N.D.	2.579 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102121\
Data File : PL070452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2021 15:06
Operator : AR\AJ
Sample : M4290-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:53:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

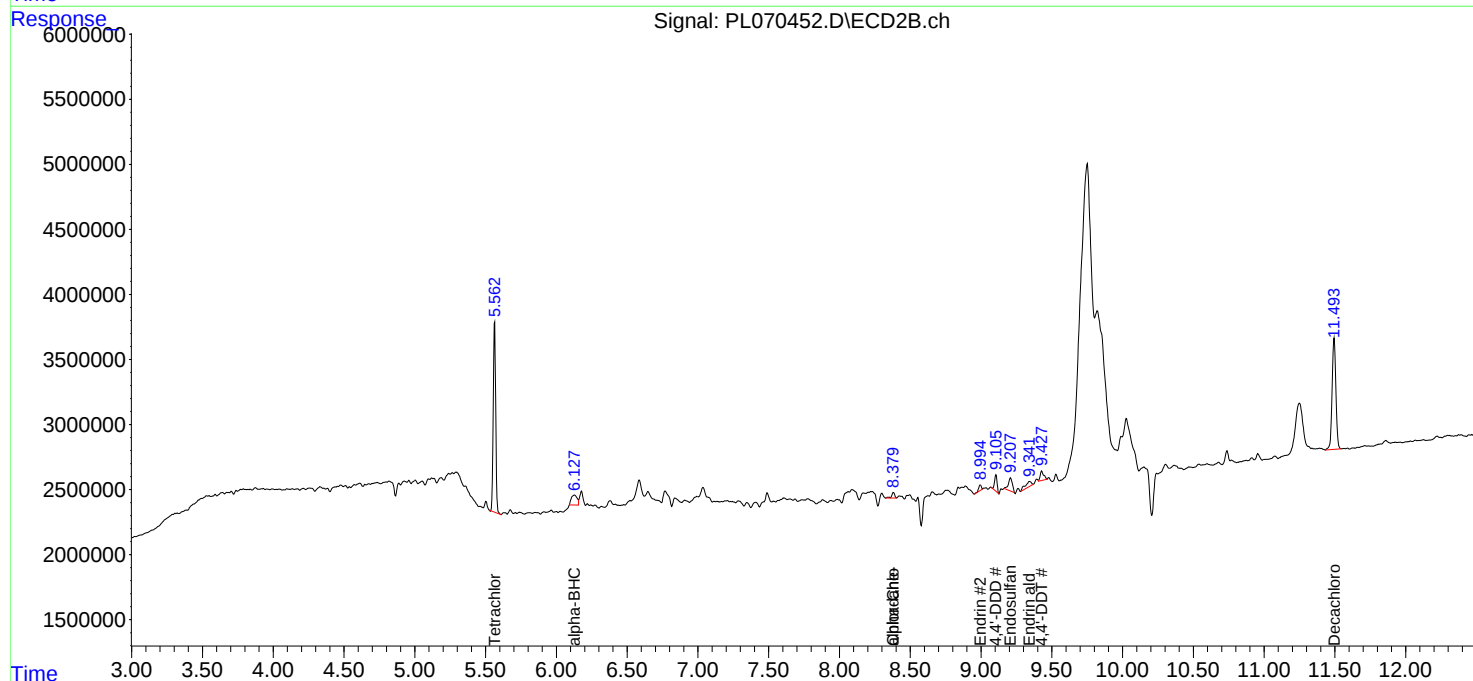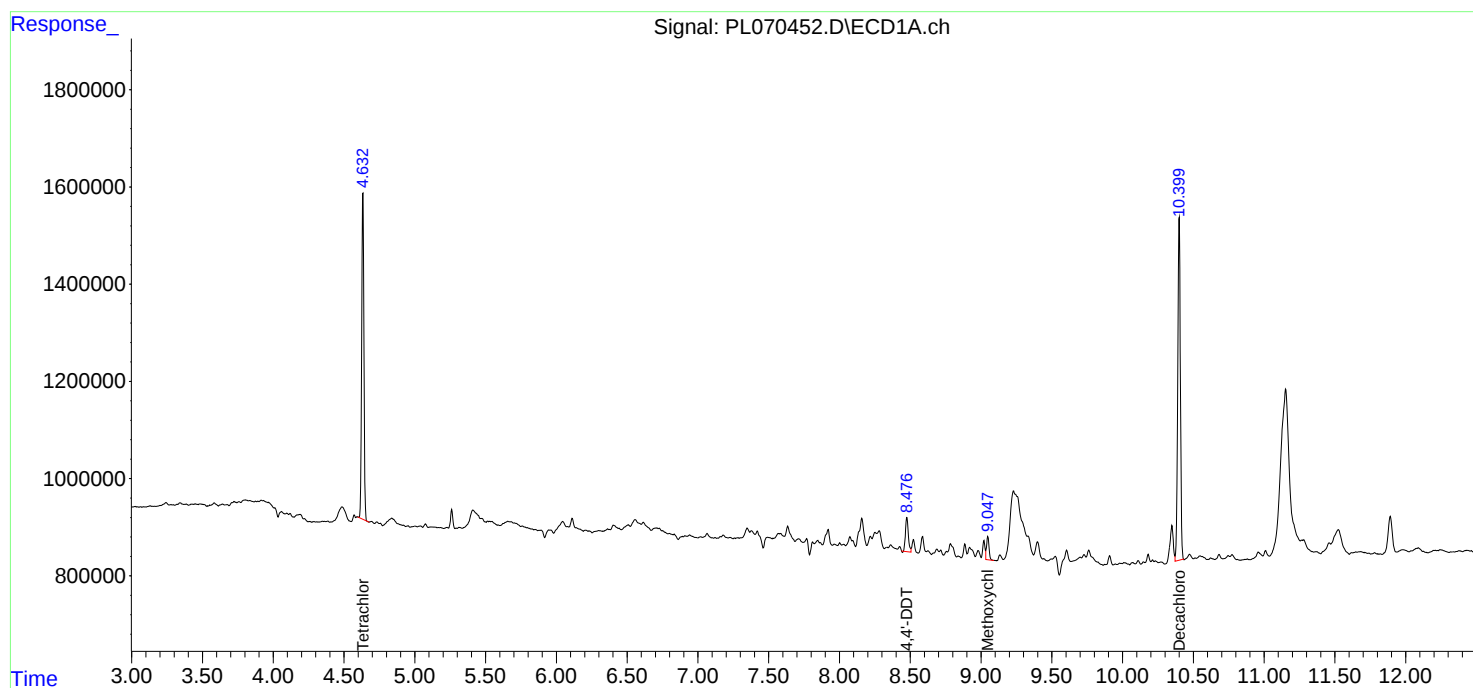


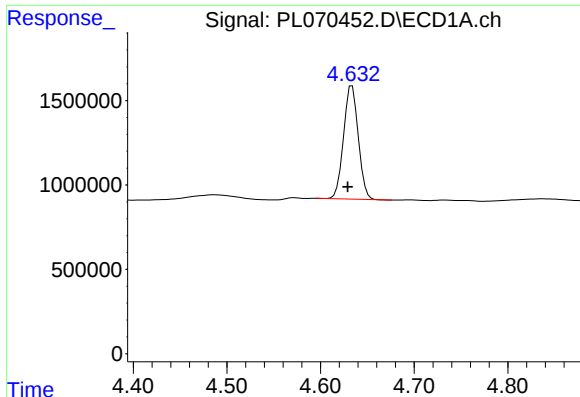

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: 0.005 min
Response: 7346413
Conc: 14.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

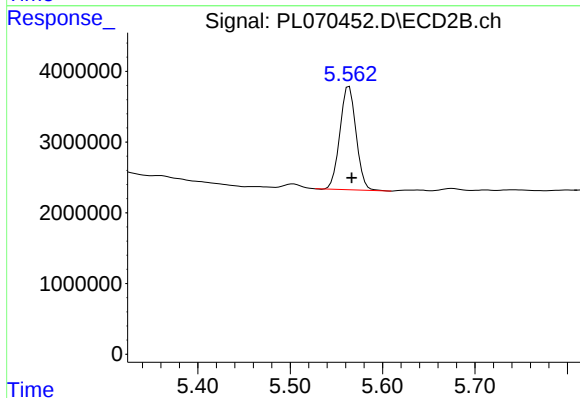


#1 Tetrachloro-m-xylene

R.T.: 5.564 min
Delta R.T.: -0.003 min
Response: 17758015
Conc: 13.43 ng/ml

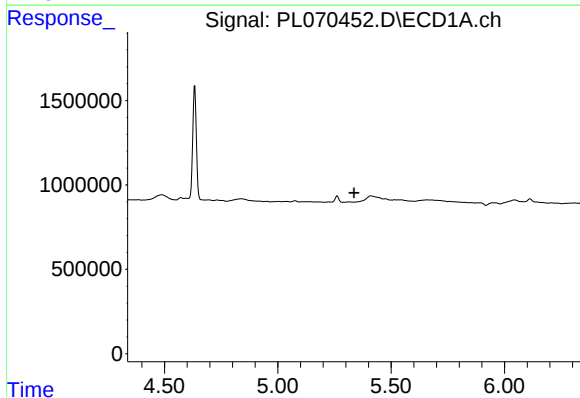


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.336 min
Response: 0
Conc: N.D.

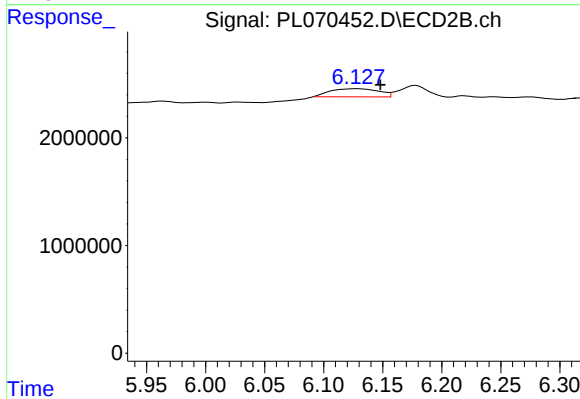

#2 alpha-BHC


R.T.: 6.129 min
Delta R.T.: -0.019 min
Response: 2149176
Conc: 1.10 ng/ml

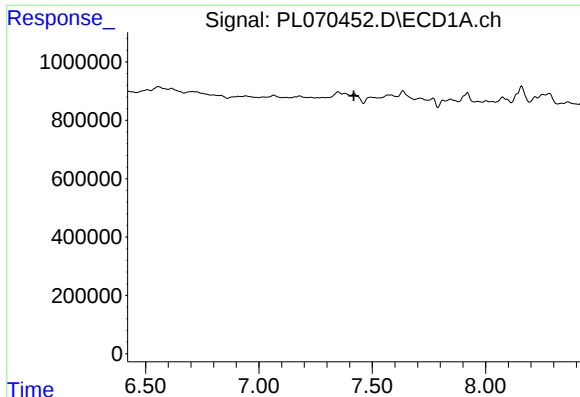

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

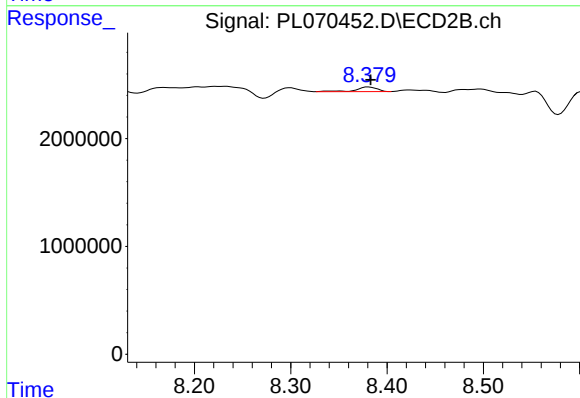


#11 alpha-Chlordane

R.T.: 8.381 min
Delta R.T.: -0.002 min
Response: 655420
Conc: 0.42 ng/ml

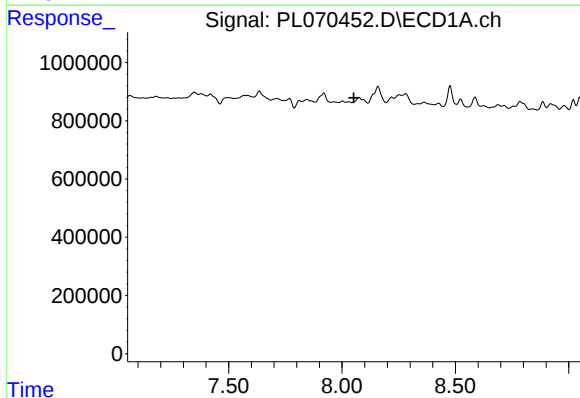


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 8.052 min
Response: 0
Conc: N.D.

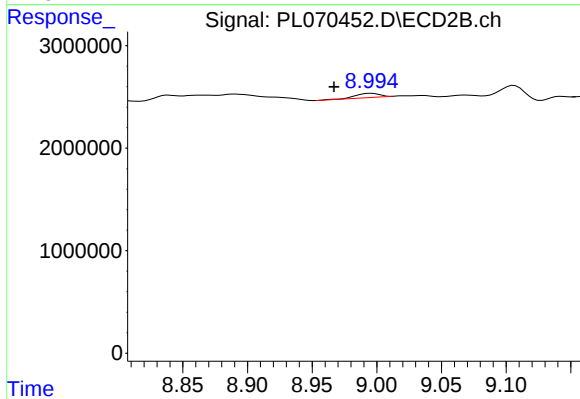

#14 Endrin


R.T.: 8.996 min
Delta R.T.: 0.029 min
Response: 529369
Conc: 0.42 ng/ml

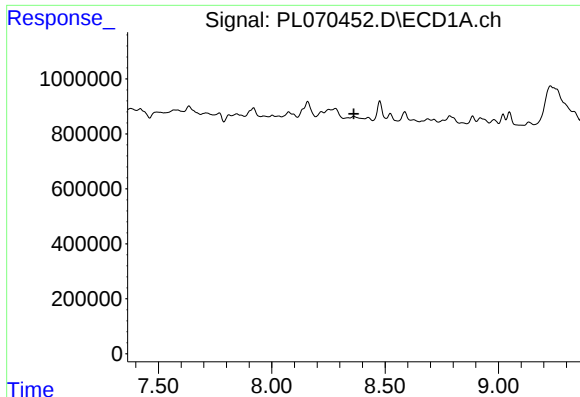

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

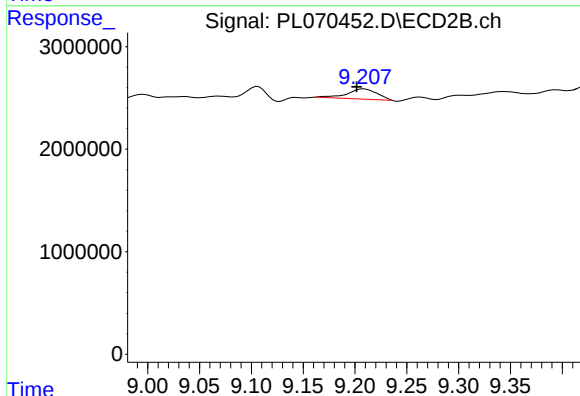


#15 Endosulfan II

R.T.: 9.209 min
Delta R.T.: 0.007 min
Response: 1962127
Conc: 1.64 ng/ml

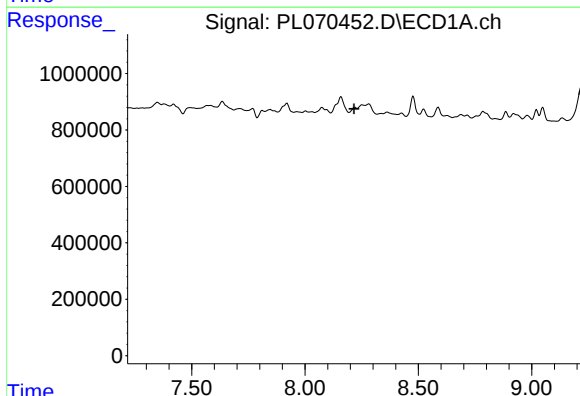


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.217 min
Response: 0
Conc: N.D.

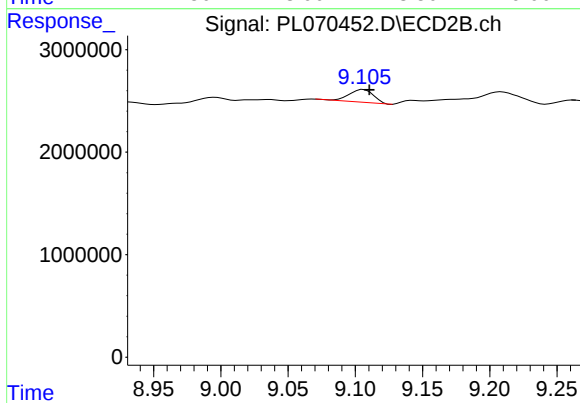

#16 4,4'-DDD


R.T.: 9.106 min
Delta R.T.: -0.004 min
Response: 1585113
Conc: 1.34 ng/ml

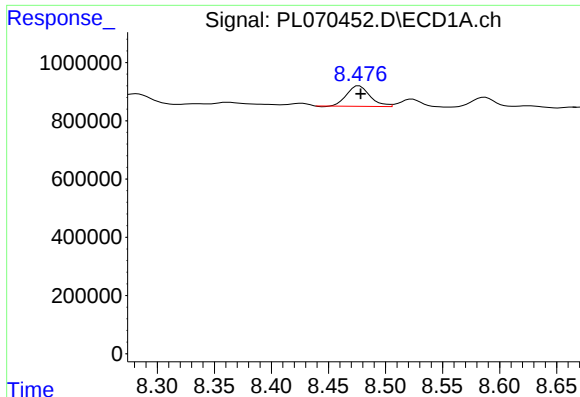

#17 4,4'-DDT


R.T.: 8.477 min
Delta R.T.: -0.001 min
Response: 997244
Conc: 1.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

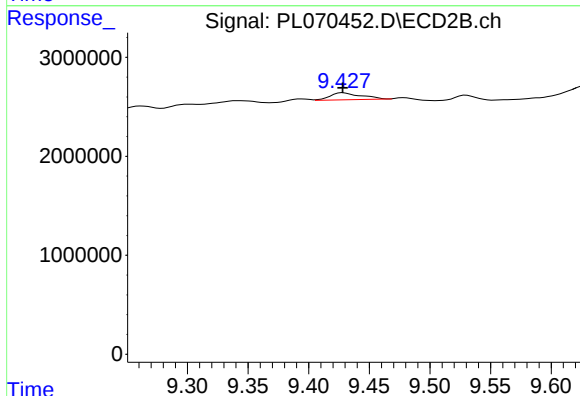


#17 4,4'-DDT

R.T.: 9.429 min
Delta R.T.: 0.000 min
Response: 1279767
Conc: 0.98 ng/ml

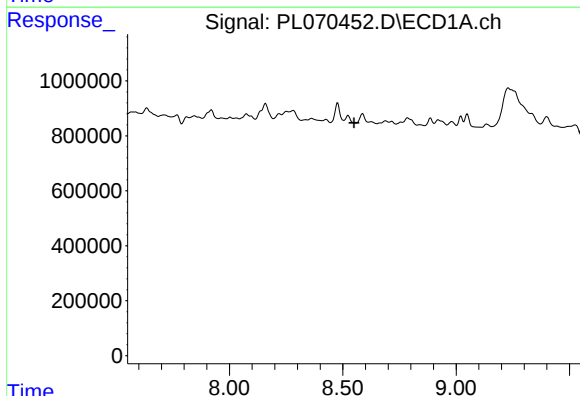


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 8.551 min
Response: 0
Conc: N.D.

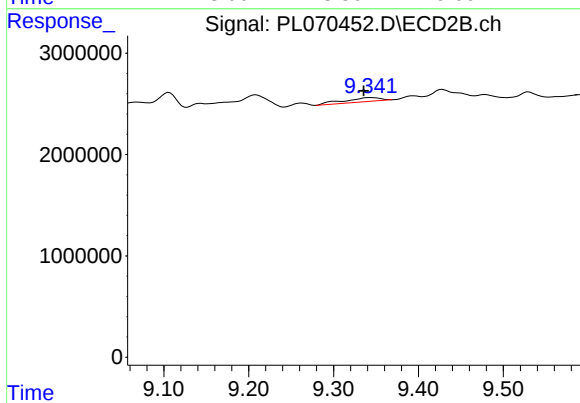

#18 Endrin aldehyde


R.T.: 9.342 min
Delta R.T.: 0.007 min
Response: 1202786
Conc: 1.25 ng/ml

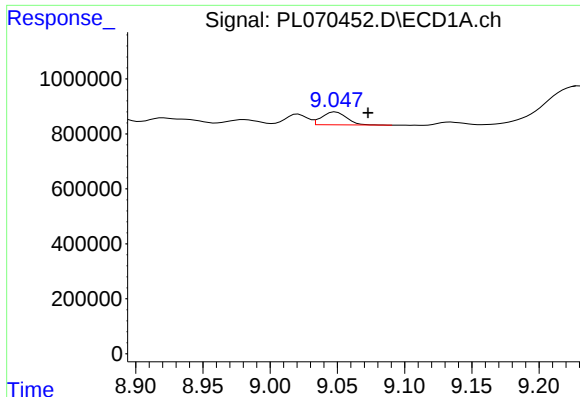

#20 Methoxychlor


R.T.: 9.049 min
Delta R.T.: -0.024 min
Response: 602233
Conc: 1.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

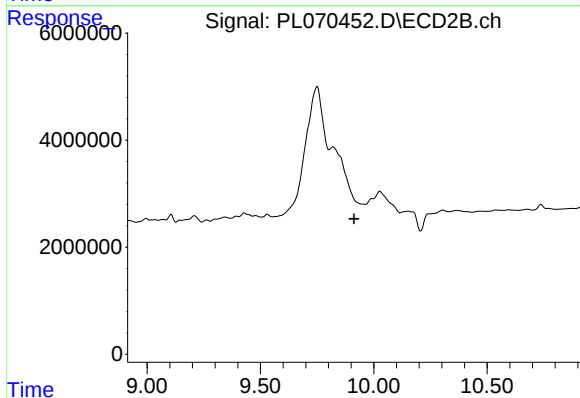


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.913 min
Response: 0
Conc: N.D.

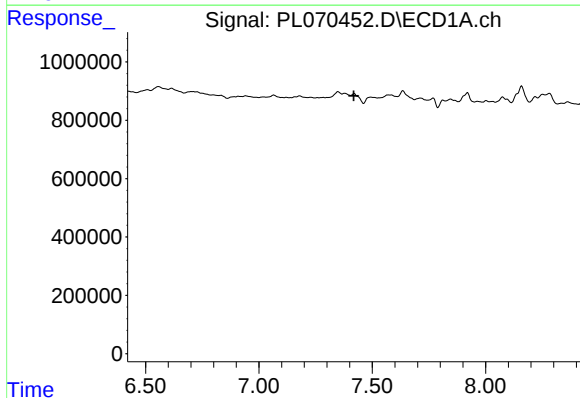


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.418 min
Response: 0
Conc: N.D.

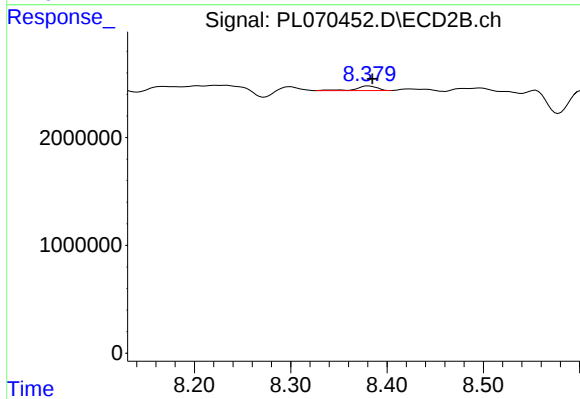

#26 Chlordane-4


R.T.: 8.381 min
Delta R.T.: -0.004 min
Response: 655420
Conc: 2.58 ng/ml

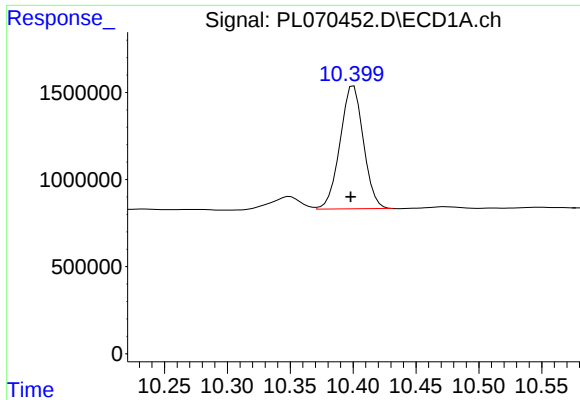

#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: 0.002 min
Response: 9129723
Conc: 13.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

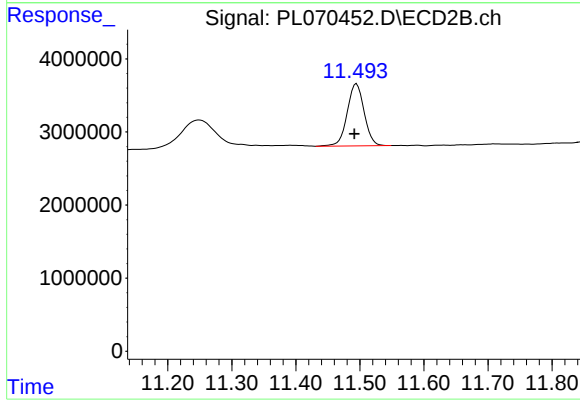

#28 Decachlorobiphenyl

R.T.: 11.495 min
Delta R.T.: 0.003 min
Response: 15628025
Conc: 12.91 ng/ml