

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102121\
 Data File : PL070453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2021 15:23
 Operator : AR\AJ
 Sample : M4290-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:53:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.626	5.564	7975312	19653913	15.938	14.860
28)	SA Decachlor...	10.395	11.491	9813127	16013663	14.181	13.233
Target Compounds							
10)	B gamma-Chl...	7.345	8.300	574275	1590601	0.793	0.994 #
11)	B alpha-Chl...	7.413	8.382	725042	2492360	0.995	1.580 #
17)	MA 4,4'-DDT	8.469	0.000	594397	0	0.972	N.D. #
19)	B Endosulfa...	8.780	0.000	376080	0	0.570	N.D. #
20)	A Methoxychlor	9.044f	0.000	1326797	0	3.553	N.D. #
21)	B Endrin ke...	9.315	0.000	3490091	0	4.567	N.D. #
25)	Chlordane-3	7.345	8.300	574275	1590601	8.394	7.510
26)	Chlordane-4	7.413	8.382	725042	2492360	9.921	9.806



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102121\
Data File : PL070453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2021 15:23
Operator : AR\AJ
Sample : M4290-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:53:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

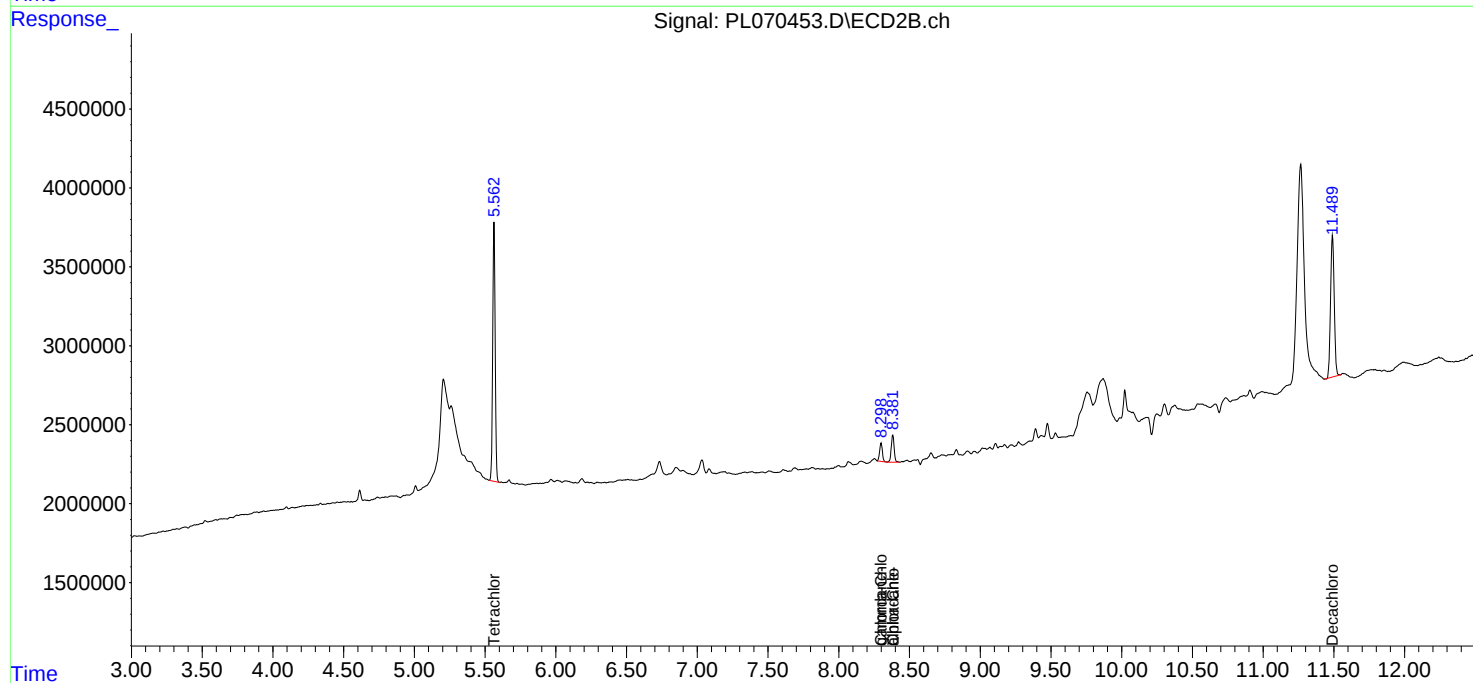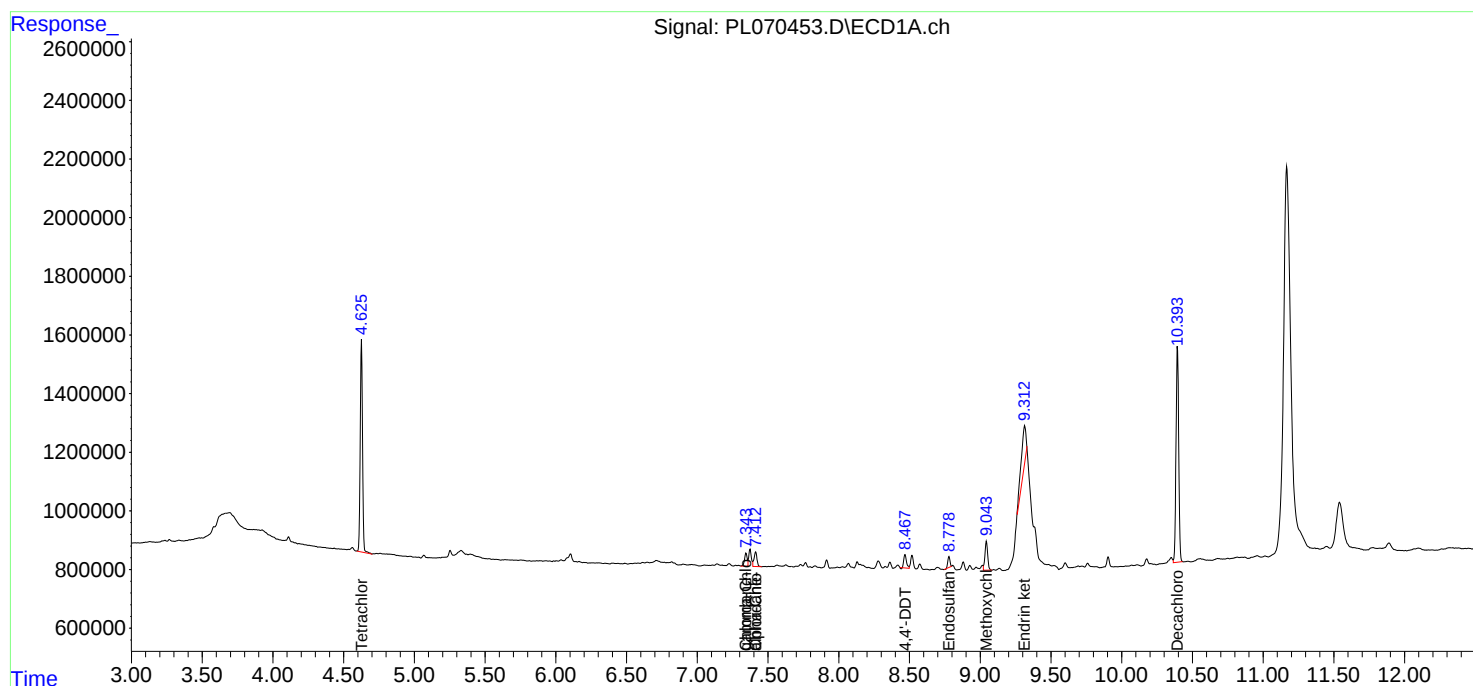


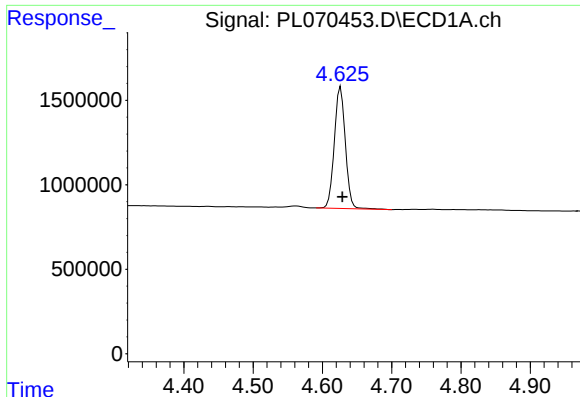

#1 Tetrachloro-m-xylene


R.T.: 4.626 min
Delta R.T.: -0.003 min
Response: 7975312
Conc: 15.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

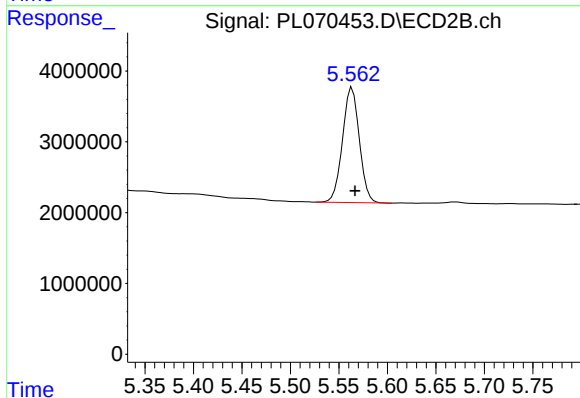


#1 Tetrachloro-m-xylene

R.T.: 5.564 min
Delta R.T.: -0.003 min
Response: 19653913
Conc: 14.86 ng/ml

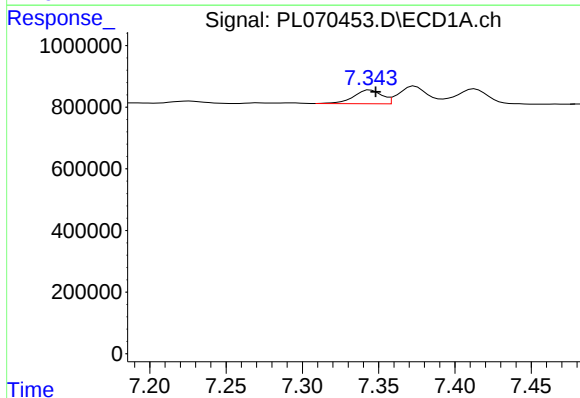


#10 gamma-Chlordane

R.T.: 7.345 min
Delta R.T.: -0.004 min
Response: 574275
Conc: 0.79 ng/ml

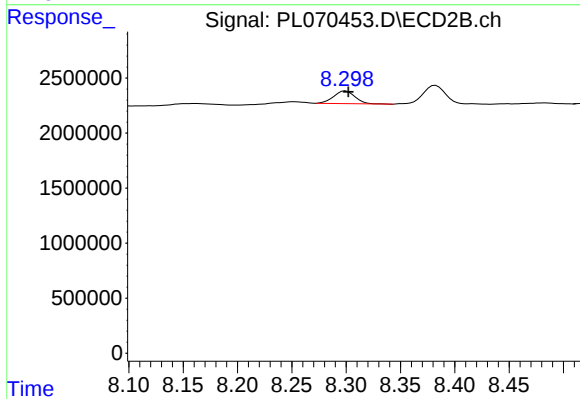

#10 gamma-Chlordane


R.T.: 8.300 min
Delta R.T.: -0.002 min
Response: 1590601
Conc: 0.99 ng/ml

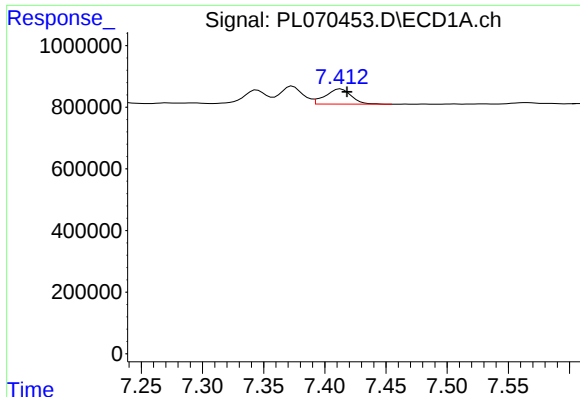

#11 alpha-Chlordane


R.T.: 7.413 min
Delta R.T.: -0.005 min
Response: 725042
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

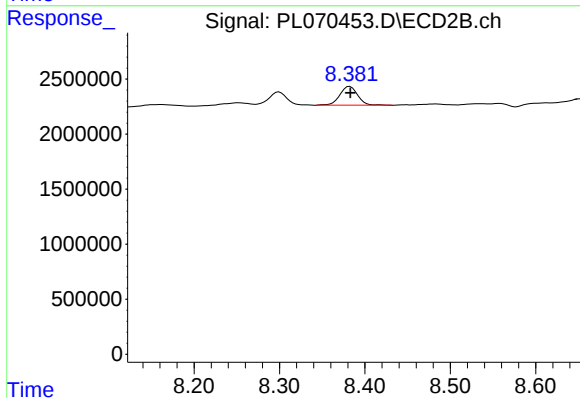


#11 alpha-Chlordane

R.T.: 8.382 min
Delta R.T.: 0.000 min
Response: 2492360
Conc: 1.58 ng/ml

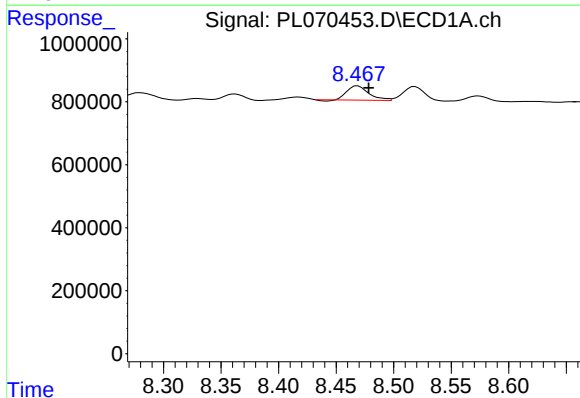


#17 4,4'-DDT

R.T.: 8.469 min
Delta R.T.: -0.009 min
Response: 594397
Conc: 0.97 ng/ml

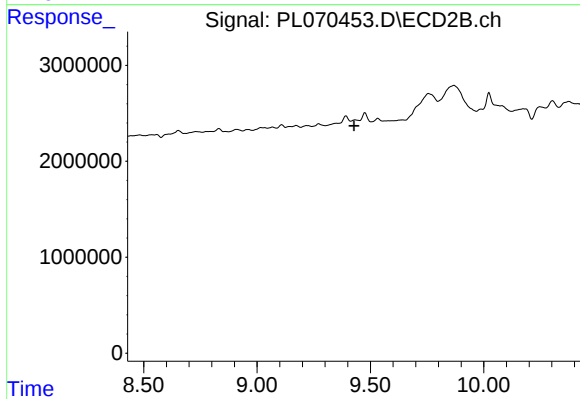

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.428 min
Response: 0
Conc: N.D.

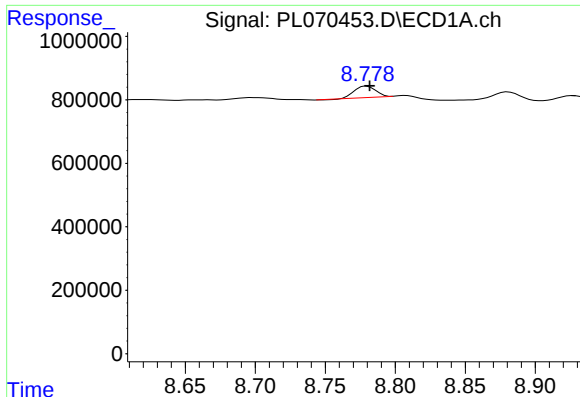

#19 Endosulfan Sulfate


R.T.: 8.780 min
Delta R.T.: -0.002 min
Response: 376080
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

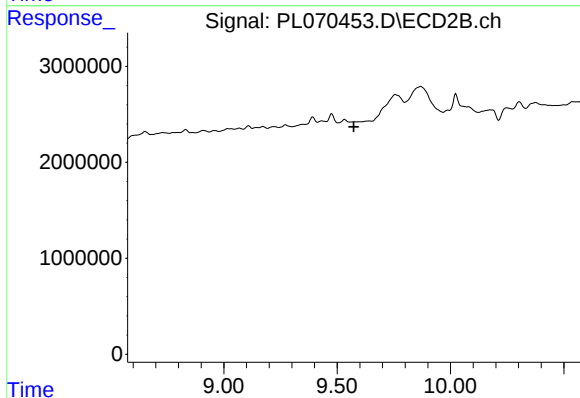


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.573 min
Response: 0
Conc: N.D.

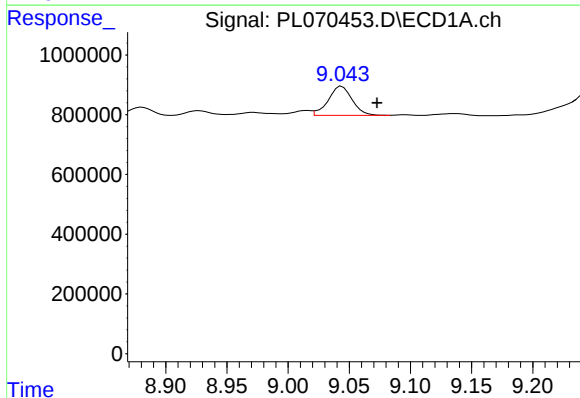


#20 Methoxychlor

R.T.: 9.044 min
Delta R.T.: -0.029 min
Response: 1326797
Conc: 3.55 ng/ml

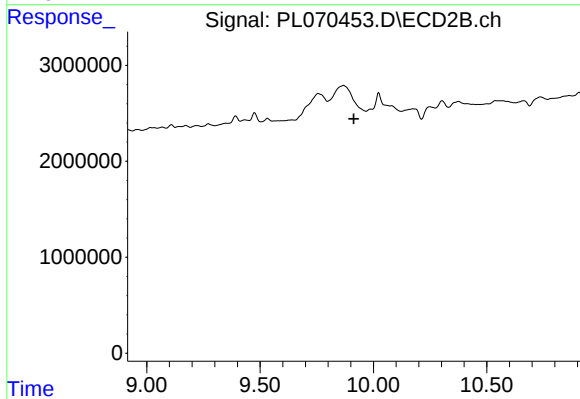

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 9.913 min
Response: 0
Conc: N.D.

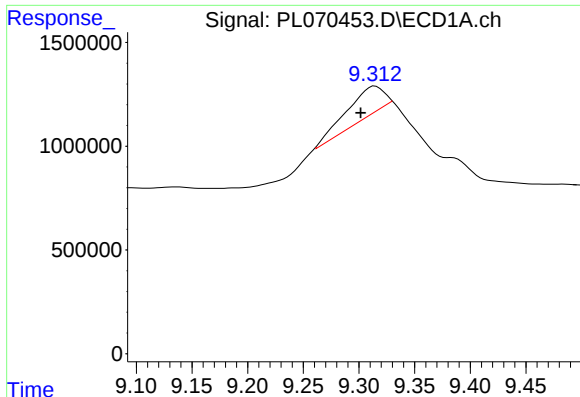

#21 Endrin ketone


R.T.: 9.315 min
Delta R.T.: 0.013 min
Response: 3490091
Conc: 4.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

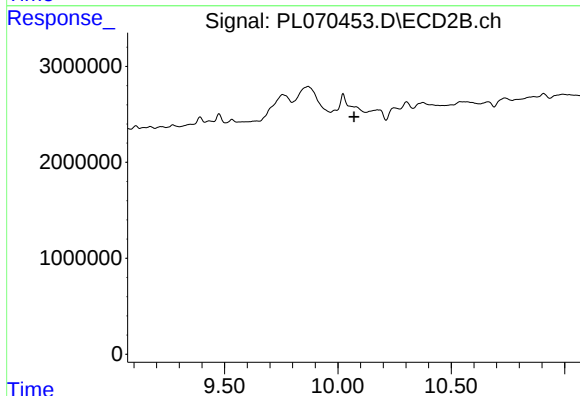


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 10.072 min
Response: 0
Conc: N.D.

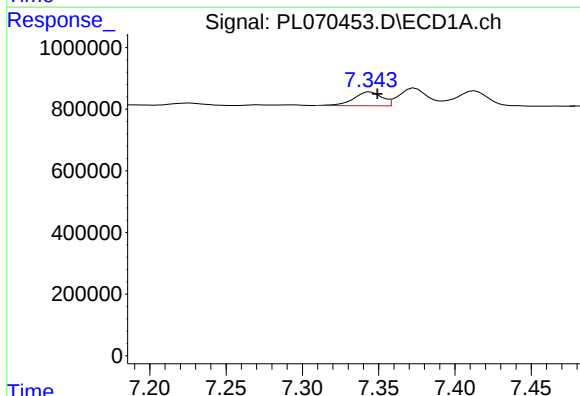


#25 Chlordane-3

R.T.: 7.345 min
Delta R.T.: -0.005 min
Response: 574275
Conc: 8.39 ng/ml

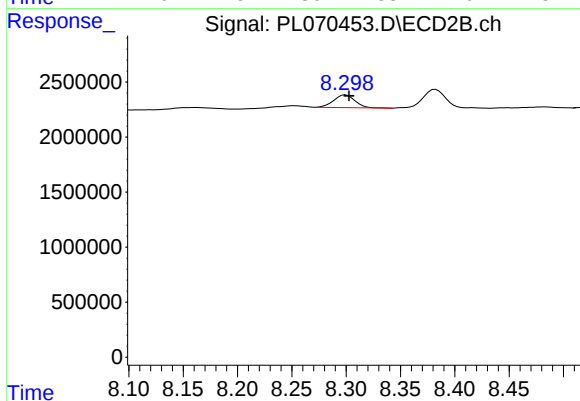

#25 Chlordane-3


R.T.: 8.300 min
Delta R.T.: -0.003 min
Response: 1590601
Conc: 7.51 ng/ml

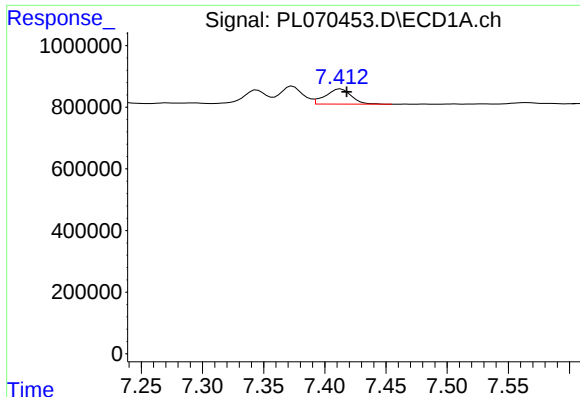

#26 Chlordane-4


R.T.: 7.413 min
Delta R.T.: -0.005 min
Response: 725042
Conc: 9.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

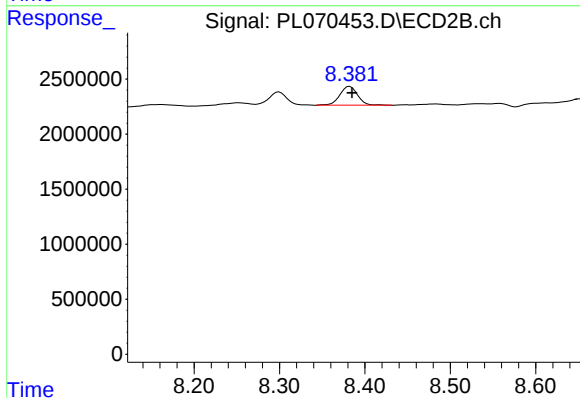


#26 Chlordane-4

R.T.: 8.382 min
Delta R.T.: -0.002 min
Response: 2492360
Conc: 9.81 ng/ml

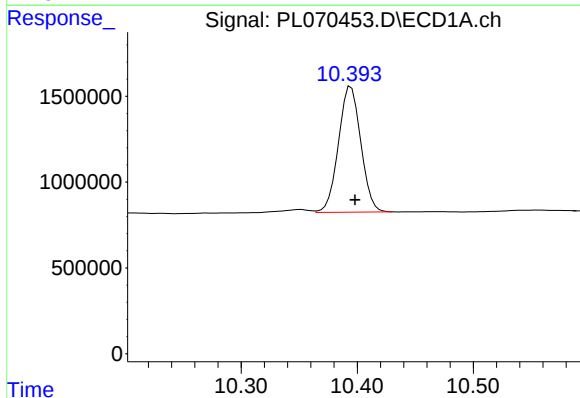

#28 Decachlorobiphenyl

R.T.: 10.395 min
Delta R.T.: -0.003 min
Response: 9813127
Conc: 14.18 ng/ml

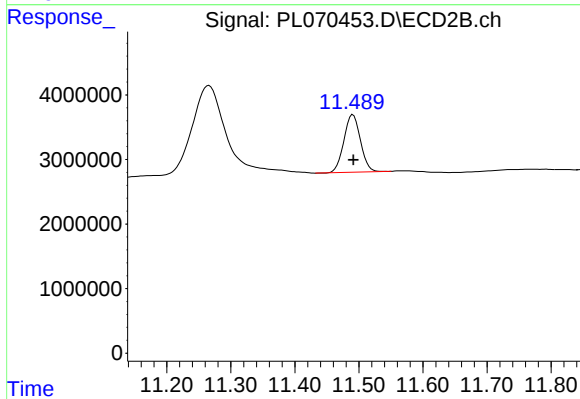

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: -0.001 min
Response: 16013663
Conc: 13.23 ng/ml