

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102121\
 Data File : PL070464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2021 19:15
 Operator : AR\AJ
 Sample : M4294-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:56:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.623	5.561	7026266	18170386	14.042	13.738
28)	SA Decachlor...	10.389	11.483	9198172	15432843	13.293	12.753
Target Compounds							
7)	B delta-BHC	0.000	7.080	0	697762	N.D.	0.360 #
10)	B gamma-Chl...	0.000	8.296	0	1137096	N.D.	0.711 #
11)	B alpha-Chl...	0.000	8.377	0	978161	N.D.	0.620 #
25)	Chlordane-3	0.000	8.296	0	1137096	N.D.	5.369 #
26)	Chlordane-4	0.000	8.377	0	978161	N.D.	3.849 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102121\
Data File : PL070464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2021 19:15
Operator : AR\AJ
Sample : M4294-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:56:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

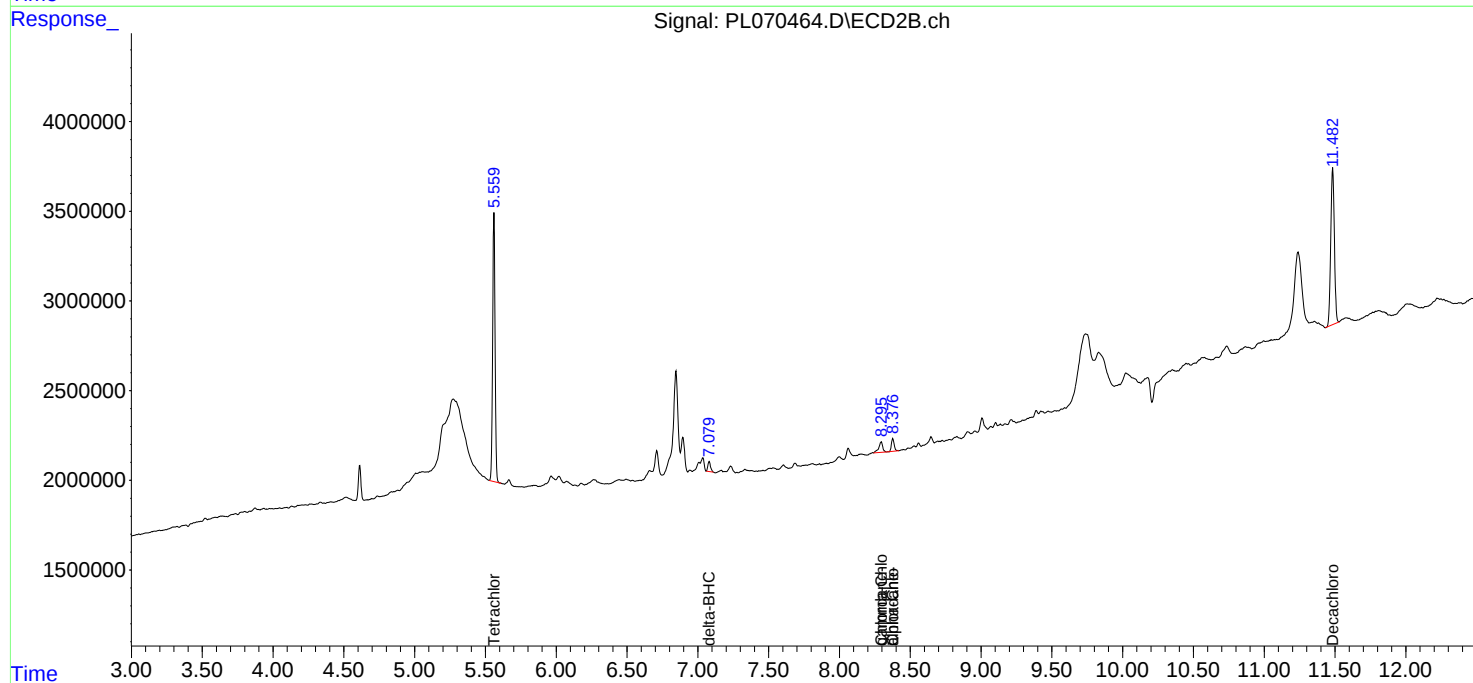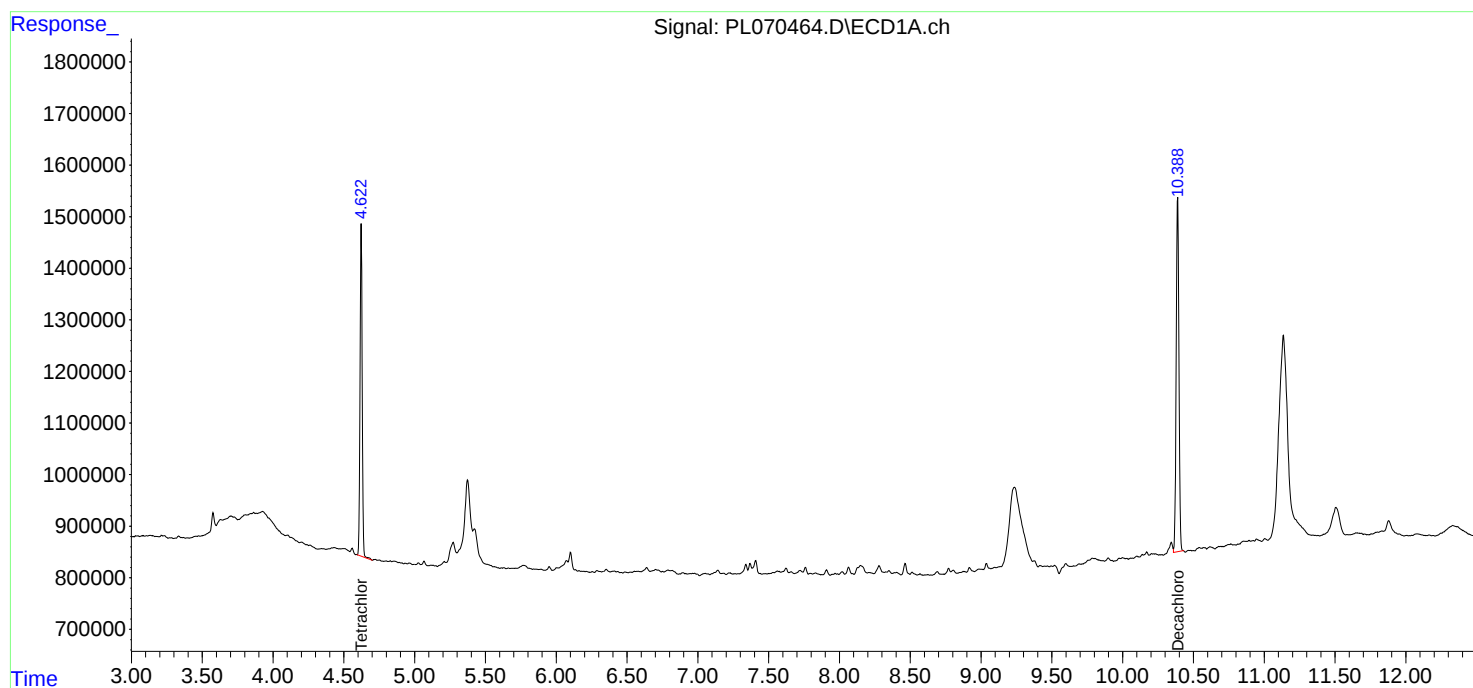


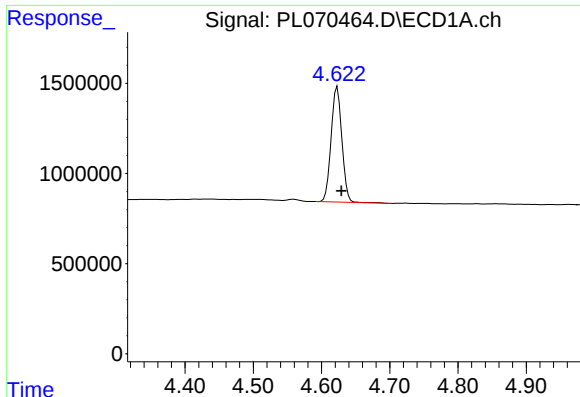

#1 Tetrachloro-m-xylene


R.T.: 4.623 min
Delta R.T.: -0.006 min
Response: 7026266
Conc: 14.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

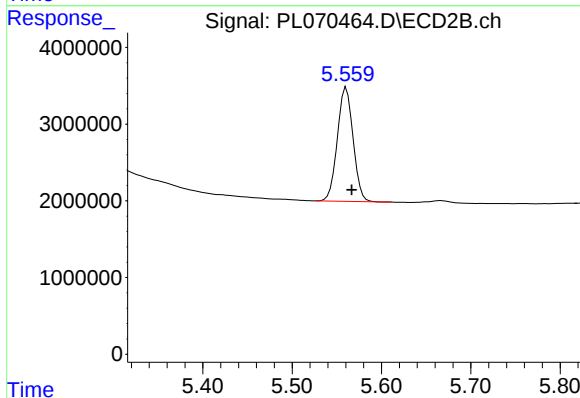


#1 Tetrachloro-m-xylene

R.T.: 5.561 min
Delta R.T.: -0.006 min
Response: 18170386
Conc: 13.74 ng/ml

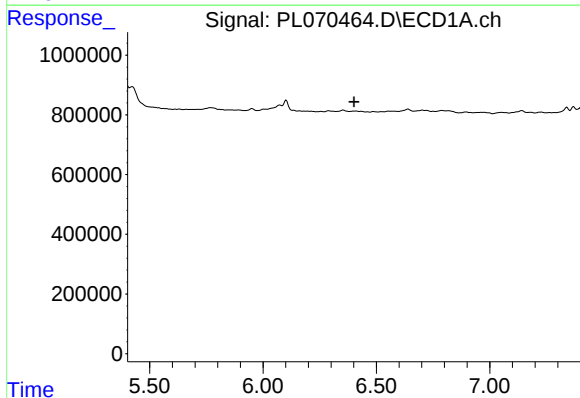


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.401 min
Response: 0
Conc: N.D.

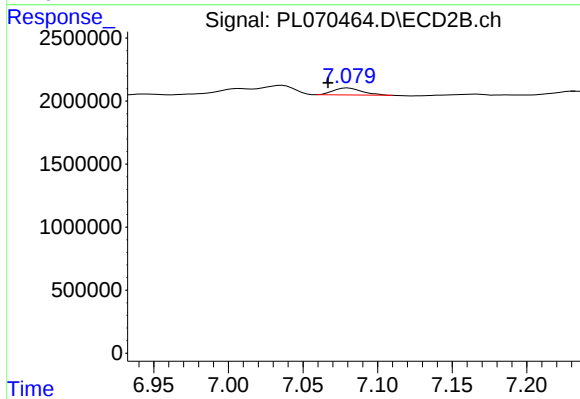

#7 delta-BHC


R.T.: 7.080 min
Delta R.T.: 0.013 min
Response: 697762
Conc: 0.36 ng/ml

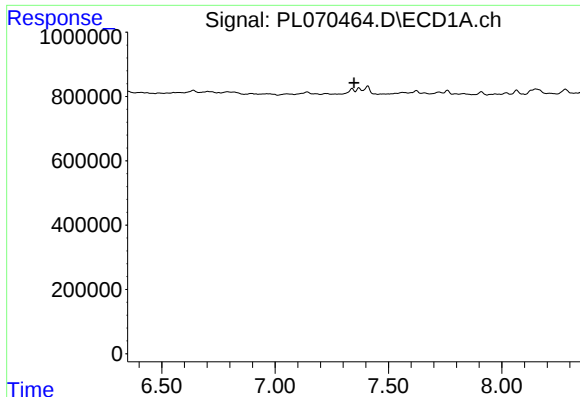

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.348 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

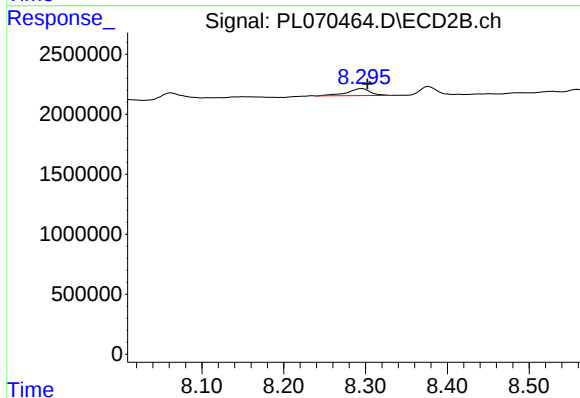


#10 gamma-Chlordane

R.T.: 8.296 min
Delta R.T.: -0.006 min
Response: 1137096
Conc: 0.71 ng/ml

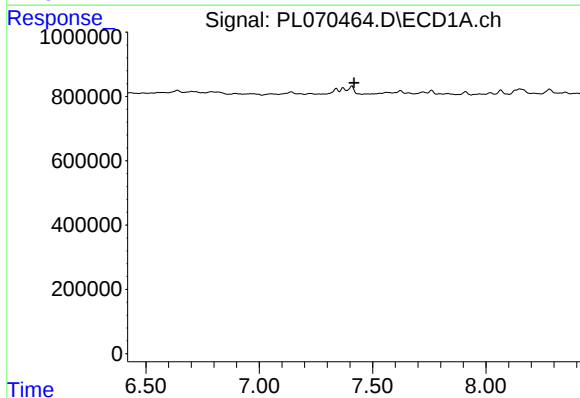


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.418 min
Response: 0
Conc: N.D.

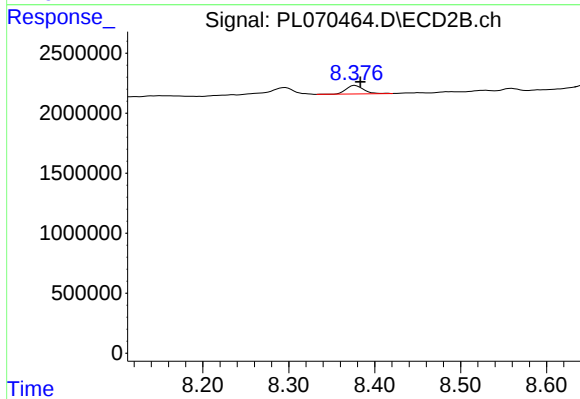

#11 alpha-Chlordane


R.T.: 8.377 min
Delta R.T.: -0.006 min
Response: 978161
Conc: 0.62 ng/ml

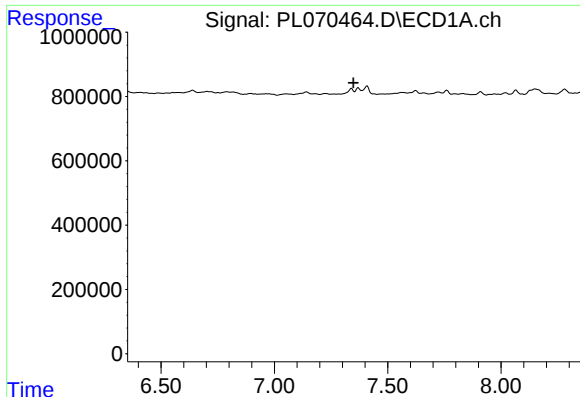

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

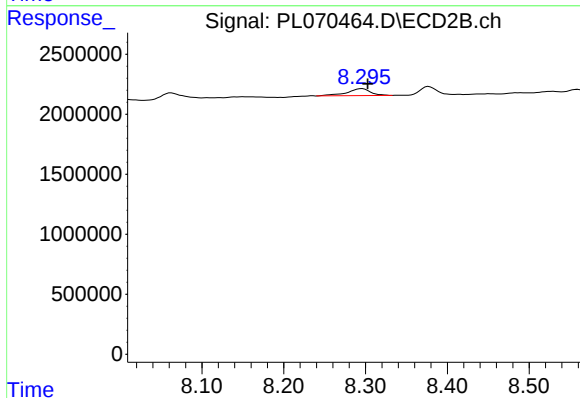


#25 Chlordane-3

R.T.: 8.296 min
Delta R.T.: -0.007 min
Response: 1137096
Conc: 5.37 ng/ml

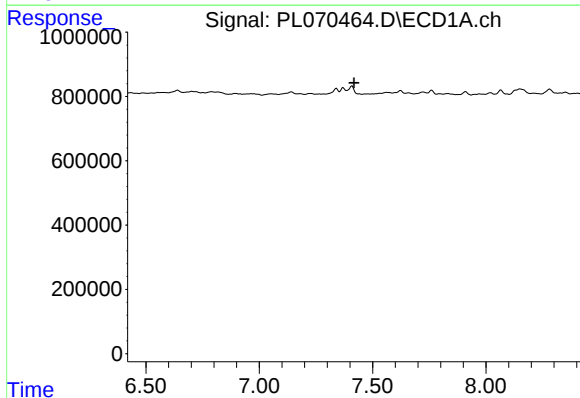


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.418 min
Response: 0
Conc: N.D.

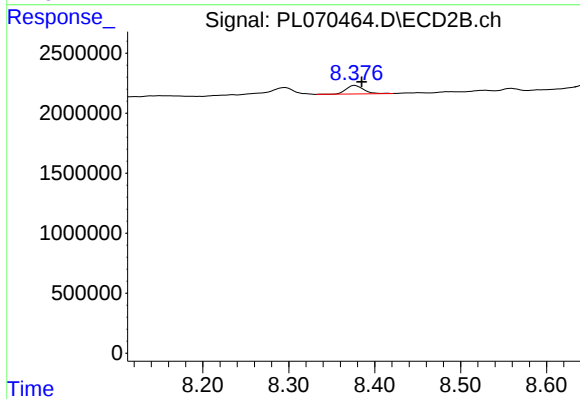

#26 Chlordane-4


R.T.: 8.377 min
Delta R.T.: -0.008 min
Response: 978161
Conc: 3.85 ng/ml

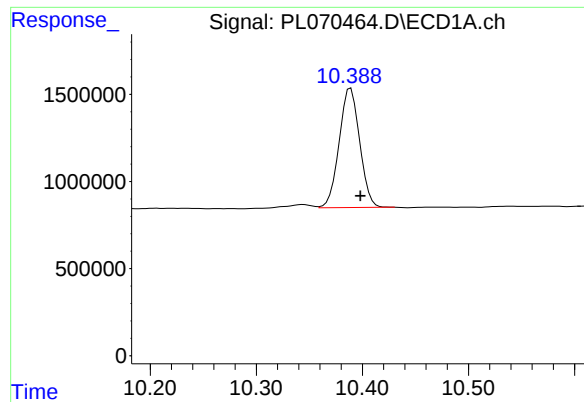

#28 Decachlorobiphenyl

R.T.: 10.389 min
Delta R.T.: -0.009 min
Response: 9198172
Conc: 13.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

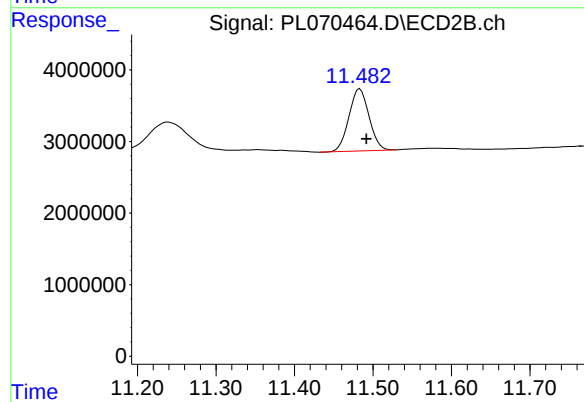

#28 Decachlorobiphenyl

R.T.: 11.483 min
Delta R.T.: -0.008 min
Response: 15432843
Conc: 12.75 ng/ml