

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102121\
 Data File : PL070470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2021 20:55
 Operator : AR\AJ
 Sample : M4300-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:58:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.623	5.561	8078334	20104537	16.144	15.200
28)	SA Decachlor...	10.389	11.483	10358838	17141113	14.970	14.164
Target Compounds							
6)	B beta-BHC	0.000	6.795	0	745148	N.D.	0.867 #
10)	B gamma-Chl...	7.340	8.295	699243	2740295	0.966	1.713 #
11)	B alpha-Chl...	7.409	8.378	1537972	4956806	2.112	3.143 #
12)	B 4,4'-DDE	7.623	8.560	1295157	1883937	2.035	1.216 #
14)	MA Endrin	8.056	8.995f	2065786	598325	3.269	0.476 #
17)	MA 4,4'-DDT	8.469	9.422	1439646	1747021	2.353	1.337 #
25)	Chlordane-3	7.340	8.295	699243	2740295	10.220	12.939 #
26)	Chlordane-4	7.409	8.378	1537972	4956806	21.044	19.503


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102121\
Data File : PL070470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2021 20:55
Operator : AR\AJ
Sample : M4300-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:58:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

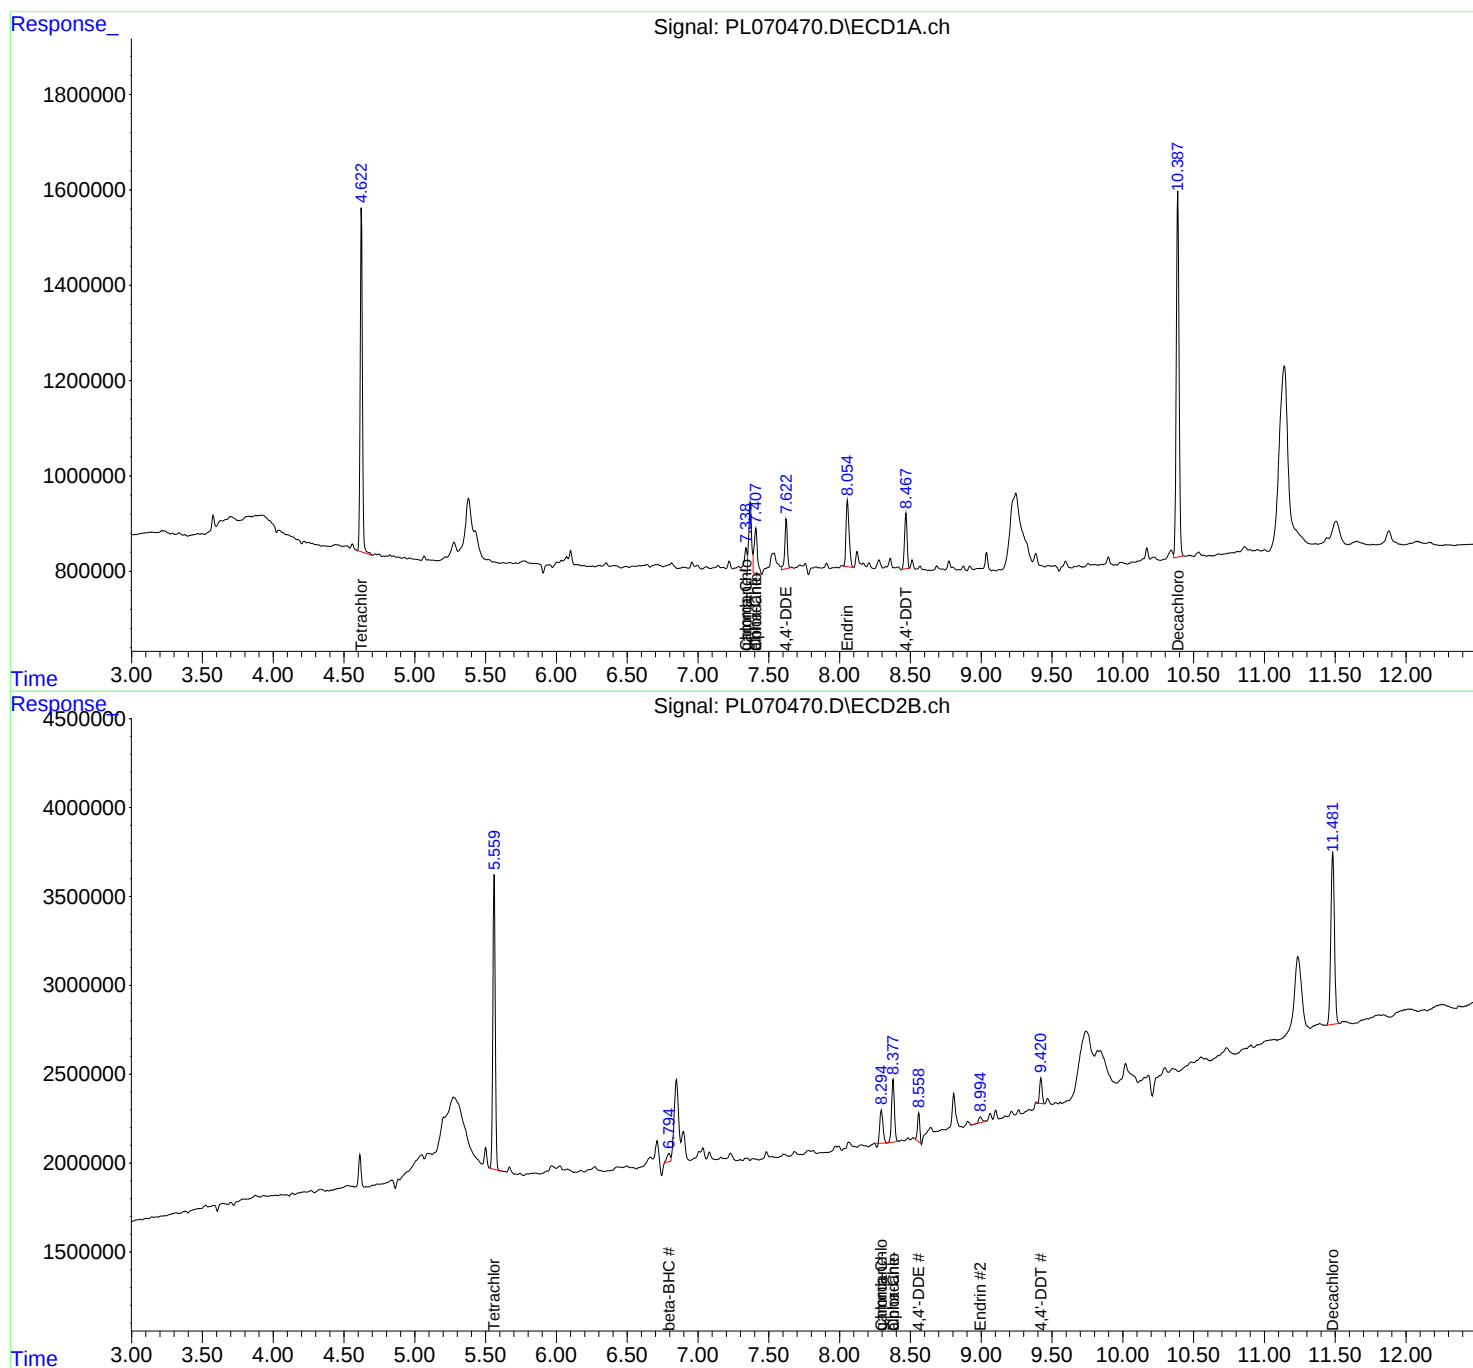


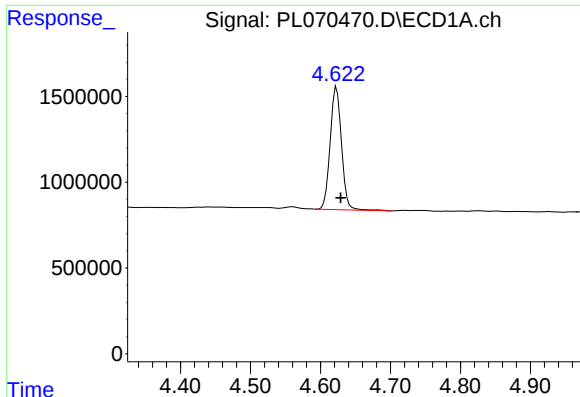

#1 Tetrachloro-m-xylene


R.T.: 4.623 min
Delta R.T.: -0.006 min
Response: 8078334
Conc: 16.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

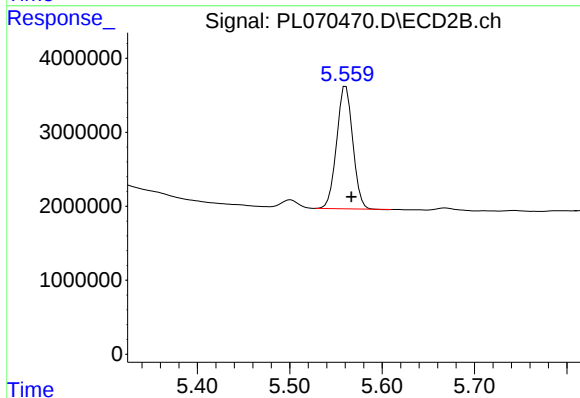


#1 Tetrachloro-m-xylene

R.T.: 5.561 min
Delta R.T.: -0.006 min
Response: 20104537
Conc: 15.20 ng/ml

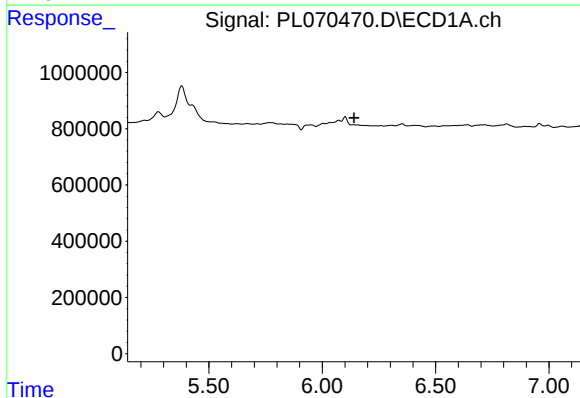


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.140 min
Response: 0
Conc: N.D.

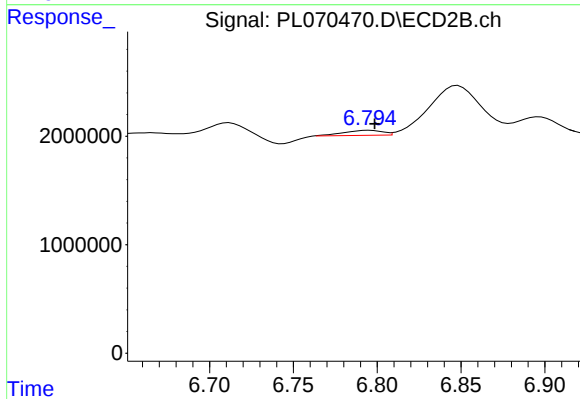

#6 beta-BHC


R.T.: 6.795 min
Delta R.T.: -0.003 min
Response: 745148
Conc: 0.87 ng/ml

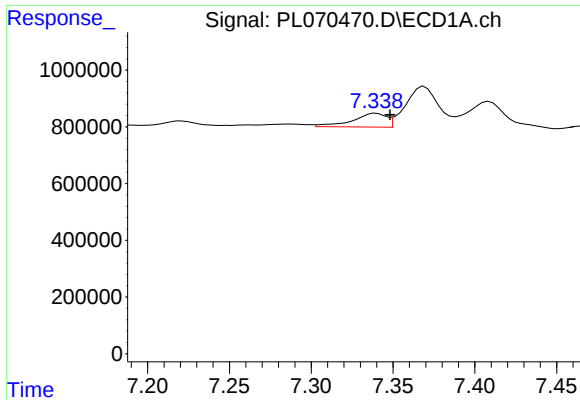

#10 gamma-Chlordane


R.T.: 7.340 min
Delta R.T.: -0.008 min
Response: 699243
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

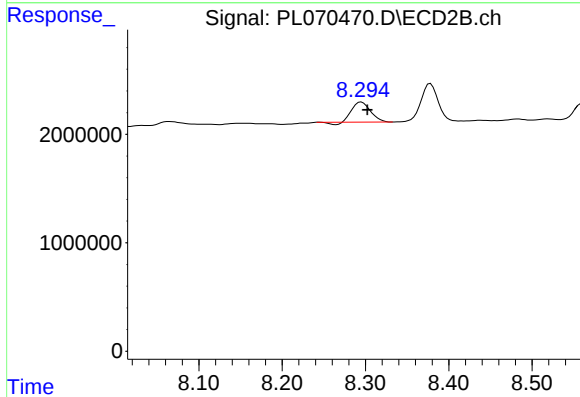


#10 gamma-Chlordane

R.T.: 8.295 min
Delta R.T.: -0.007 min
Response: 2740295
Conc: 1.71 ng/ml

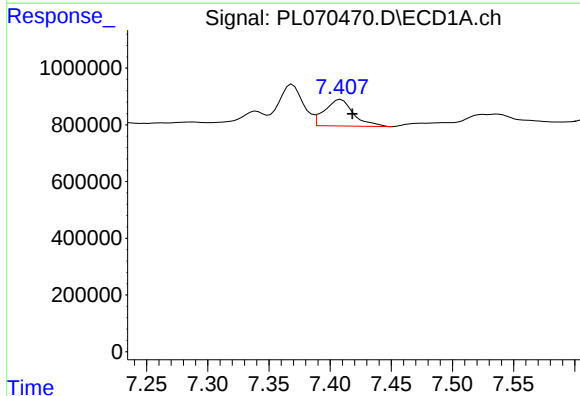


#11 alpha-Chlordane

R.T.: 7.409 min
Delta R.T.: -0.009 min
Response: 1537972
Conc: 2.11 ng/ml

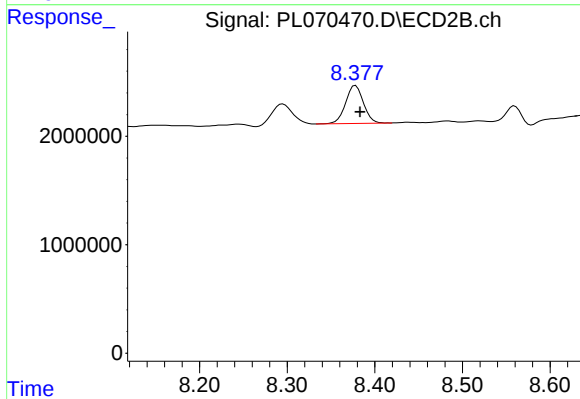

#11 alpha-Chlordane


R.T.: 8.378 min
Delta R.T.: -0.005 min
Response: 4956806
Conc: 3.14 ng/ml

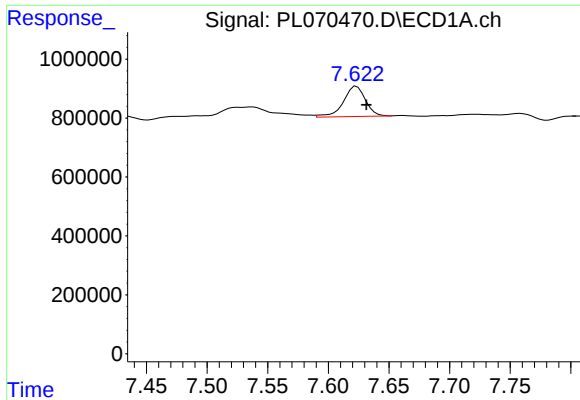

#12 4,4'-DDE


R.T.: 7.623 min
Delta R.T.: -0.008 min
Response: 1295157
Conc: 2.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

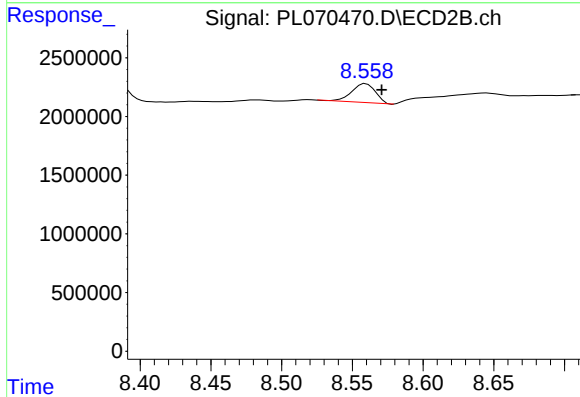


#12 4,4'-DDE

R.T.: 8.560 min
Delta R.T.: -0.011 min
Response: 1883937
Conc: 1.22 ng/ml

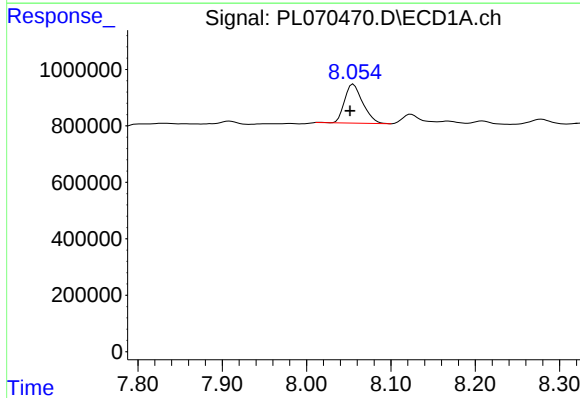


#14 Endrin

R.T.: 8.056 min
Delta R.T.: 0.004 min
Response: 2065786
Conc: 3.27 ng/ml

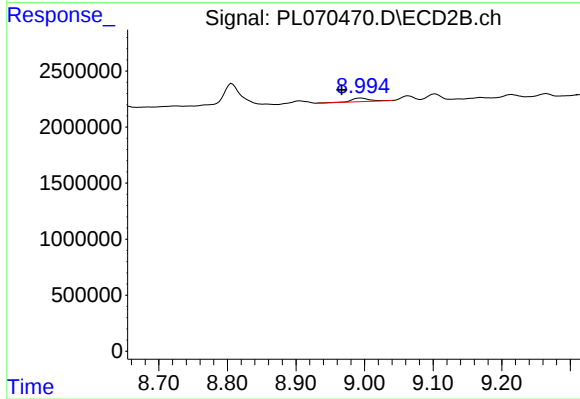

#14 Endrin


R.T.: 8.995 min
Delta R.T.: 0.028 min
Response: 598325
Conc: 0.48 ng/ml

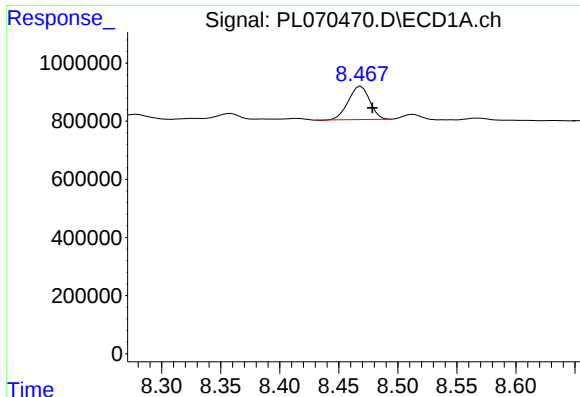

#17 4,4'-DDT


R.T.: 8.469 min
Delta R.T.: -0.009 min
Response: 1439646
Conc: 2.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

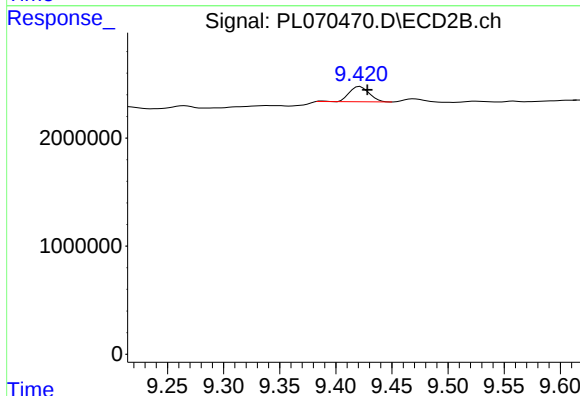


#17 4,4'-DDT

R.T.: 9.422 min
Delta R.T.: -0.007 min
Response: 1747021
Conc: 1.34 ng/ml

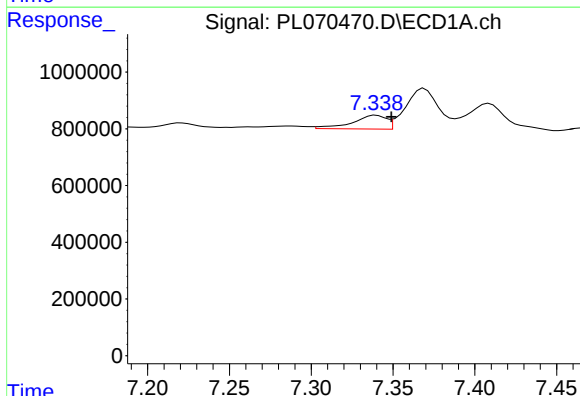


#25 Chlordane-3

R.T.: 7.340 min
Delta R.T.: -0.009 min
Response: 699243
Conc: 10.22 ng/ml

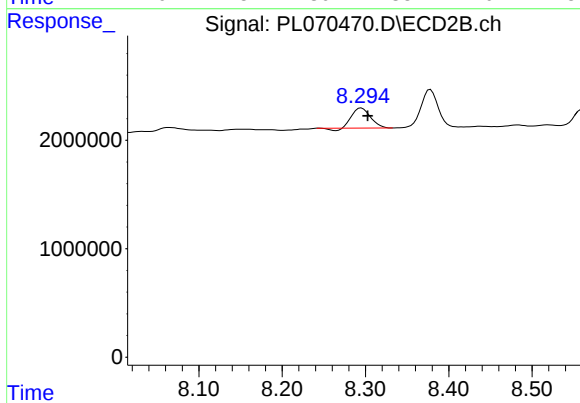

#25 Chlordane-3


R.T.: 8.295 min
Delta R.T.: -0.007 min
Response: 2740295
Conc: 12.94 ng/ml

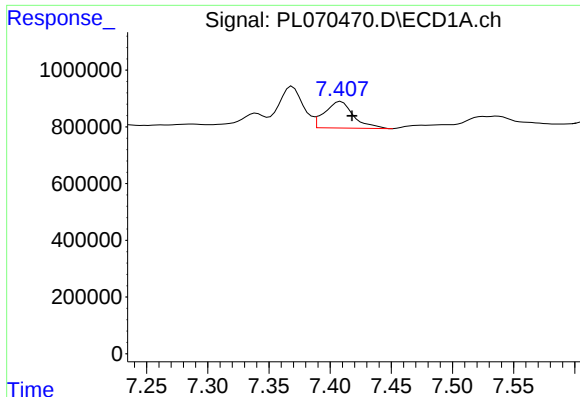

#26 Chlordane-4


R.T.: 7.409 min
Delta R.T.: -0.009 min
Response: 1537972
Conc: 21.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

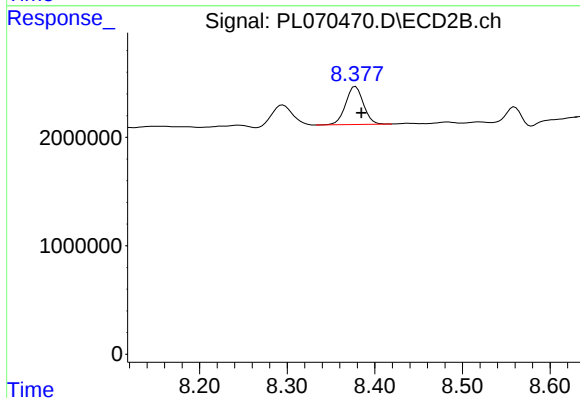


#26 Chlordane-4

R.T.: 8.378 min
Delta R.T.: -0.007 min
Response: 4956806
Conc: 19.50 ng/ml

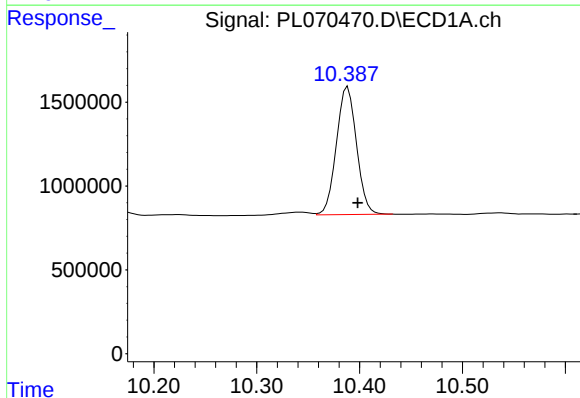

#28 Decachlorobiphenyl

R.T.: 10.389 min
Delta R.T.: -0.010 min
Response: 10358838
Conc: 14.97 ng/ml

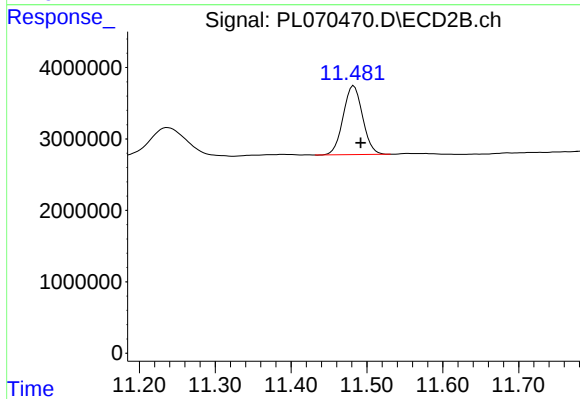

#28 Decachlorobiphenyl

R.T.: 11.483 min
Delta R.T.: -0.009 min
Response: 17141113
Conc: 14.16 ng/ml