

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102121\
 Data File : PL070472.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2021 21:28
 Operator : AR\AJ
 Sample : M4300-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:58:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.623	5.561	9780639	25629804	19.546	19.378
28)	SA Decachlor...	10.389	11.483	10536798	18831878	15.227	15.561
Target Compounds							
3)	MA gamma-BHC...	5.746	0.000	622645	0	0.892	N.D. #
9)	A Endosulfan I	7.492f	0.000	591672	0	0.885	N.D. #
10)	B gamma-Chl...	7.370f	8.293	291208	832417	0.402	0.520 #
11)	B alpha-Chl...	0.000	8.379	0	934181	N.D.	0.592 #
13)	MA Dieldrin	7.761	0.000	387813	0	0.564	N.D. #
17)	MA 4,4'-DDT	8.470	9.421	519416	1040751	0.849	0.796
20)	A Methoxychlor	9.088f	0.000	362954	0	0.972	N.D. #
25)	Chlordane-3	7.370f	8.293	291208	832417	4.256	3.930
26)	Chlordane-4	0.000	8.379	0	934181	N.D.	3.676 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102121\
Data File : PL070472.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2021 21:28
Operator : AR\AJ
Sample : M4300-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:58:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

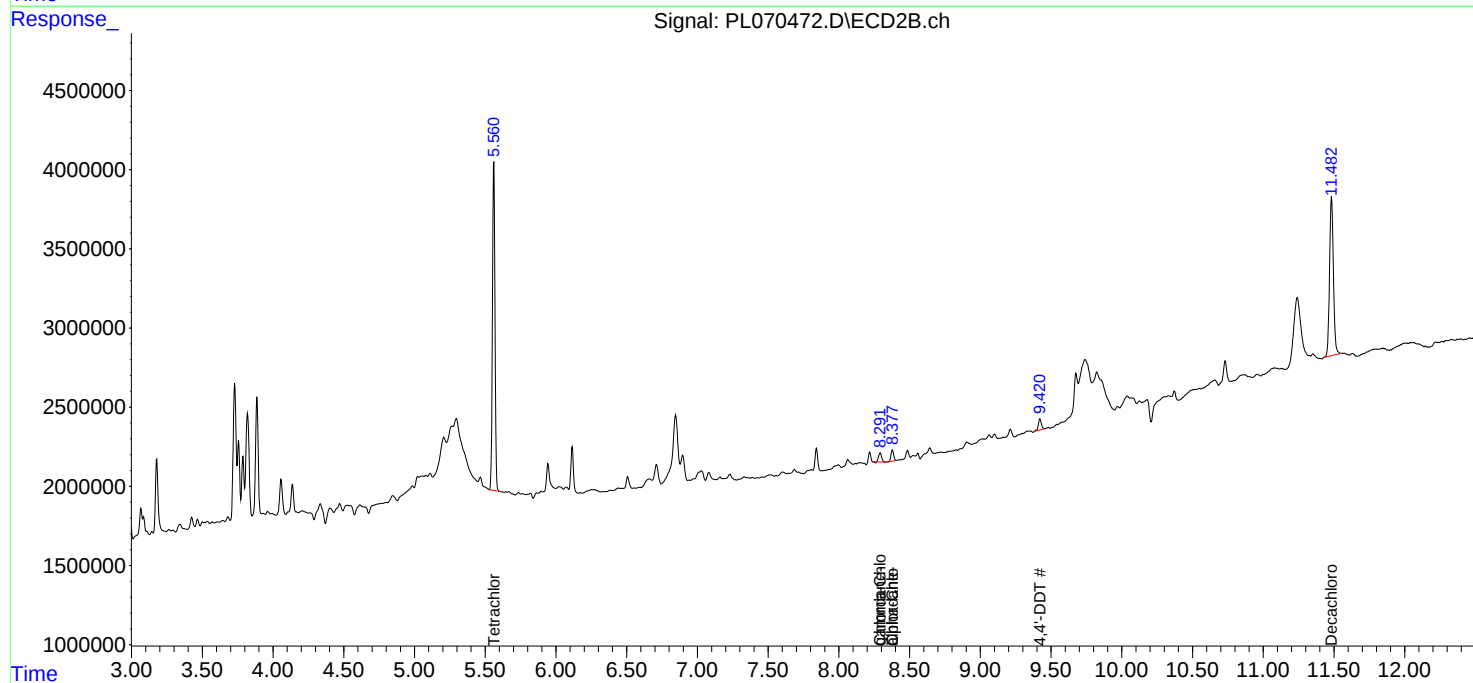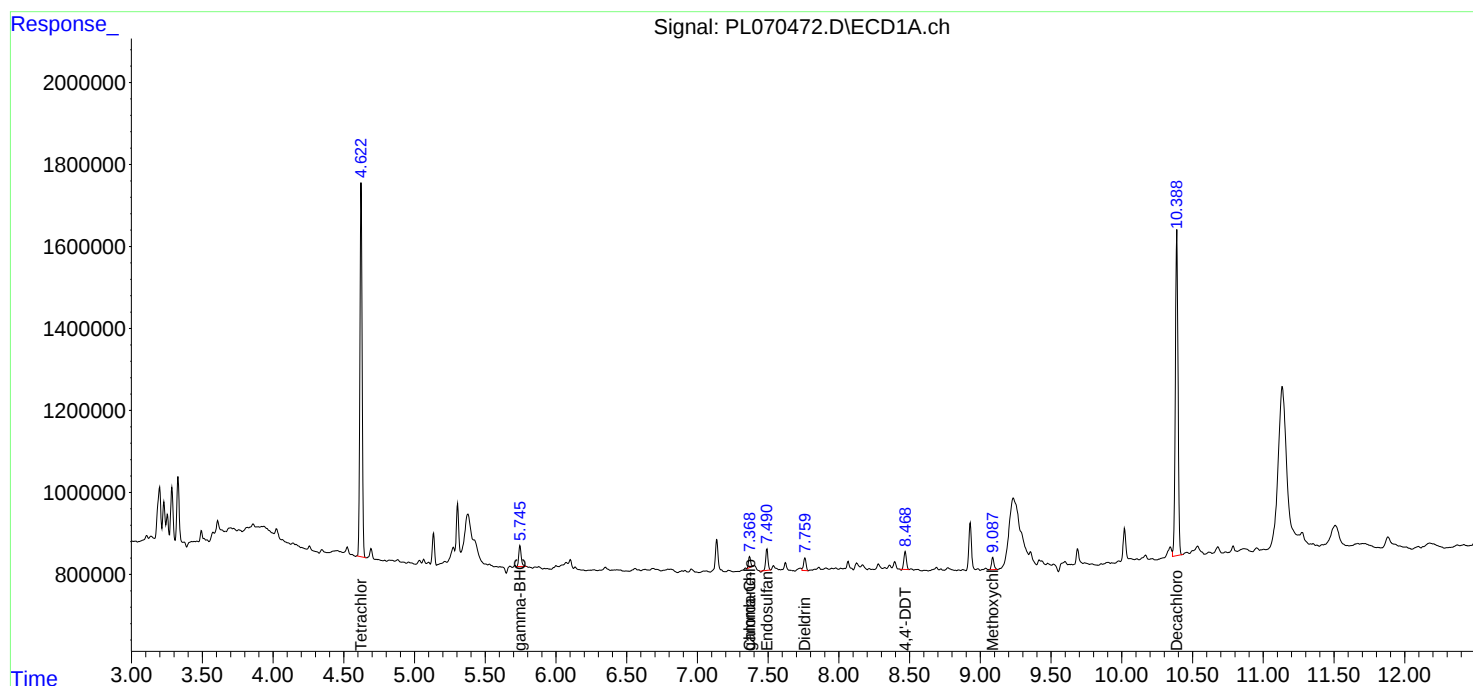


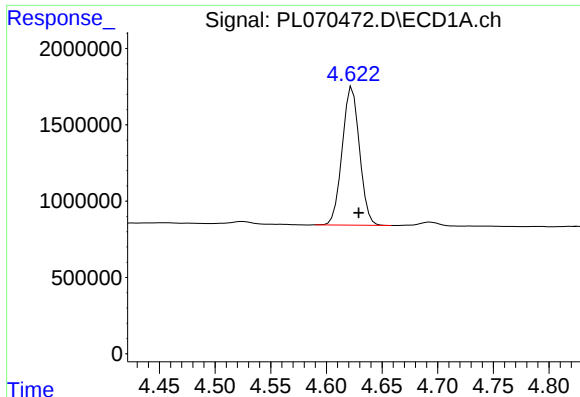

#1 Tetrachloro-m-xylene


R.T.: 4.623 min
Delta R.T.: -0.006 min
Response: 9780639
Conc: 19.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

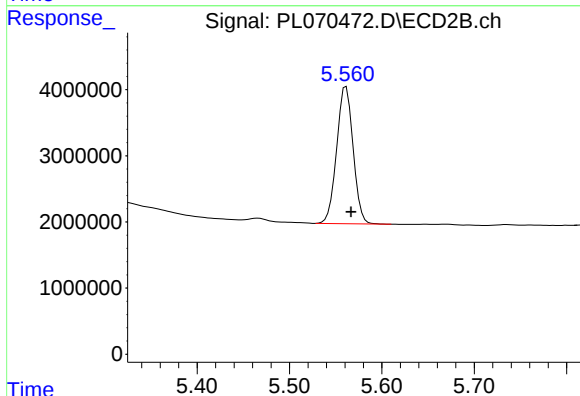


#1 Tetrachloro-m-xylene

R.T.: 5.561 min
Delta R.T.: -0.005 min
Response: 25629804
Conc: 19.38 ng/ml

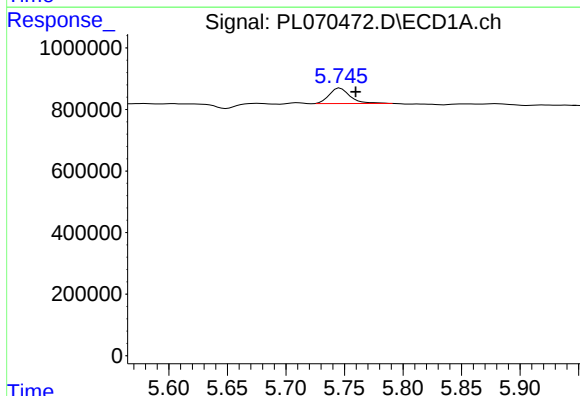


#3 gamma-BHC (Lindane)

R.T.: 5.746 min
Delta R.T.: -0.013 min
Response: 622645
Conc: 0.89 ng/ml

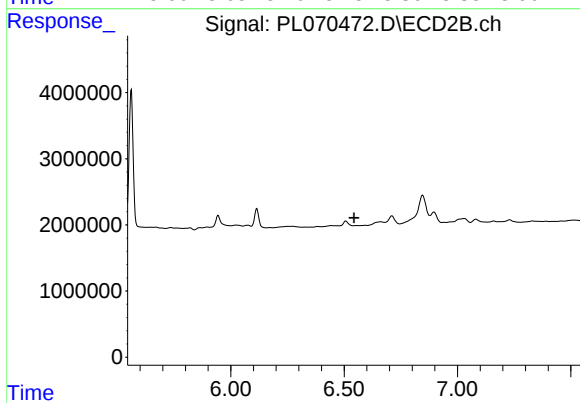

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.545 min
Response: 0
Conc: N.D.

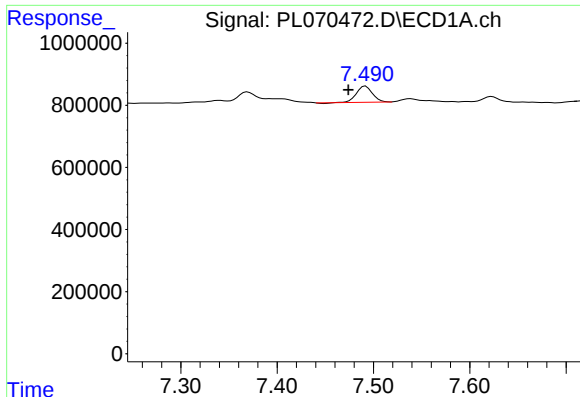

#9 Endosulfan I


R.T.: 7.492 min
Delta R.T.: 0.018 min
Response: 591672
Conc: 0.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

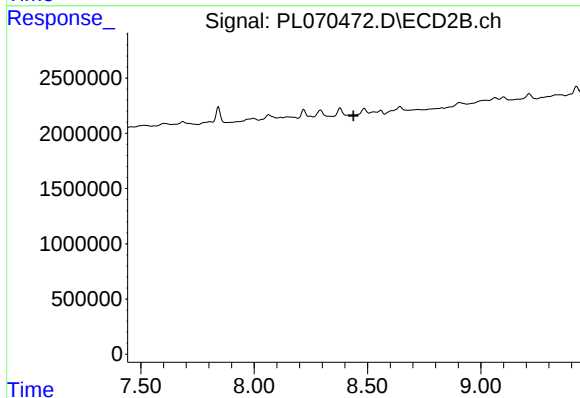


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.439 min
Response: 0
Conc: N.D.

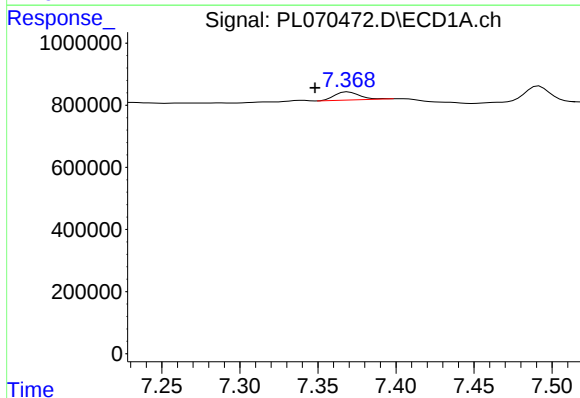


#10 gamma-Chlordane

R.T.: 7.370 min
Delta R.T.: 0.021 min
Response: 291208
Conc: 0.40 ng/ml

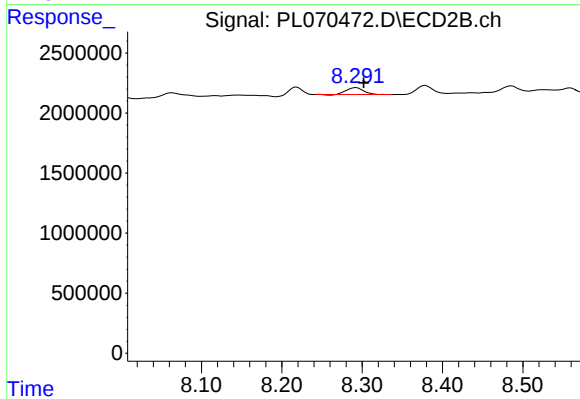

#10 gamma-Chlordane


R.T.: 8.293 min
Delta R.T.: -0.010 min
Response: 832417
Conc: 0.52 ng/ml

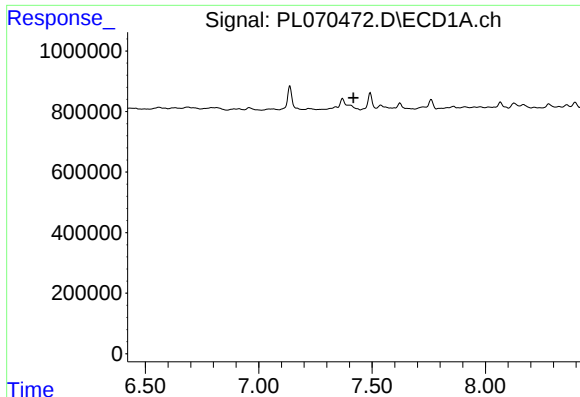

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

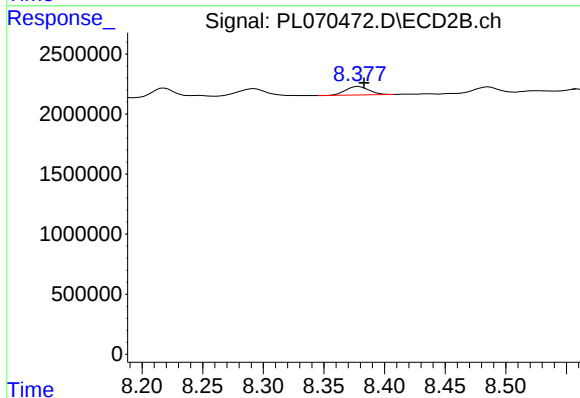


#11 alpha-Chlordane

R.T.: 8.379 min
Delta R.T.: -0.005 min
Response: 934181
Conc: 0.59 ng/ml

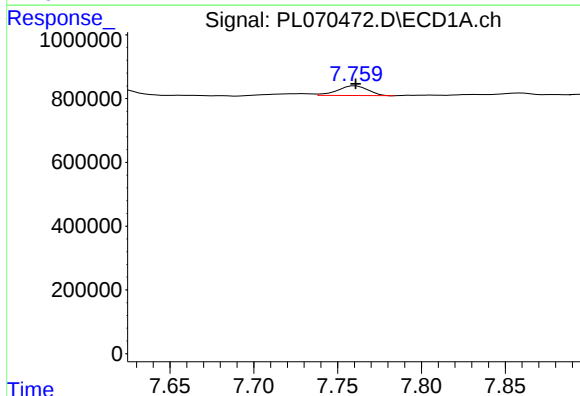


#13 Dieldrin

R.T.: 7.761 min
Delta R.T.: 0.000 min
Response: 387813
Conc: 0.56 ng/ml

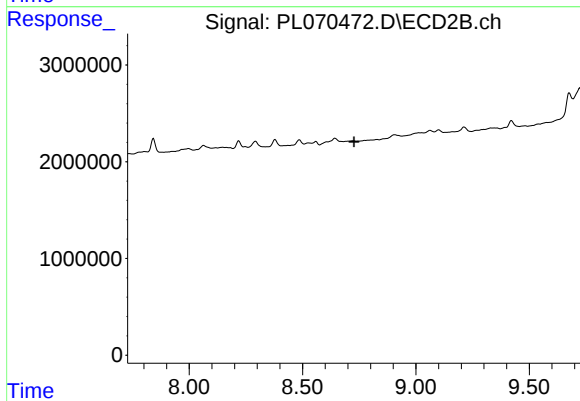

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.728 min
Response: 0
Conc: N.D.

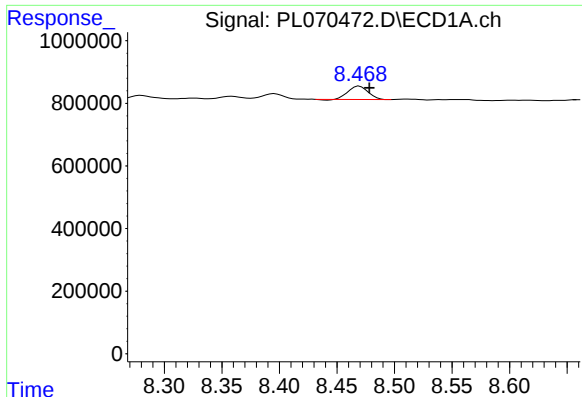

#17 4,4'-DDT


R.T.: 8.470 min
Delta R.T.: -0.009 min
Response: 519416
Conc: 0.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

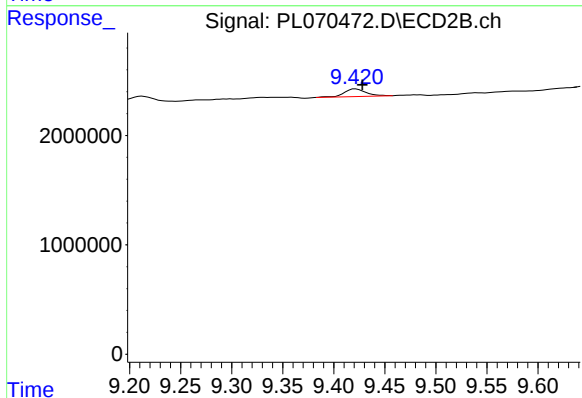


#17 4,4'-DDT

R.T.: 9.421 min
Delta R.T.: -0.007 min
Response: 1040751
Conc: 0.80 ng/ml

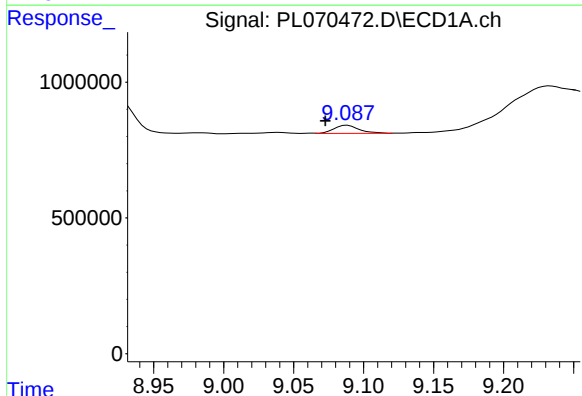


#20 Methoxychlor

R.T.: 9.088 min
Delta R.T.: 0.016 min
Response: 362954
Conc: 0.97 ng/ml

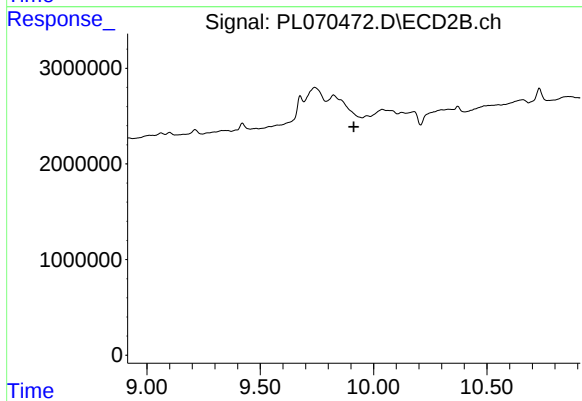

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.913 min
Response: 0
Conc: N.D.

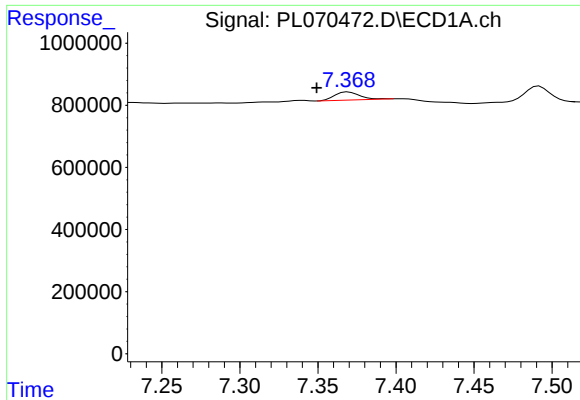

#25 Chlordane-3


R.T.: 7.370 min
Delta R.T.: 0.020 min
Response: 291208
Conc: 4.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

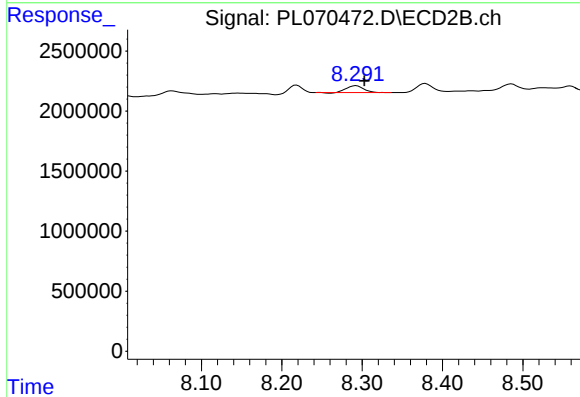


#25 Chlordane-3

R.T.: 8.293 min
Delta R.T.: -0.010 min
Response: 832417
Conc: 3.93 ng/ml

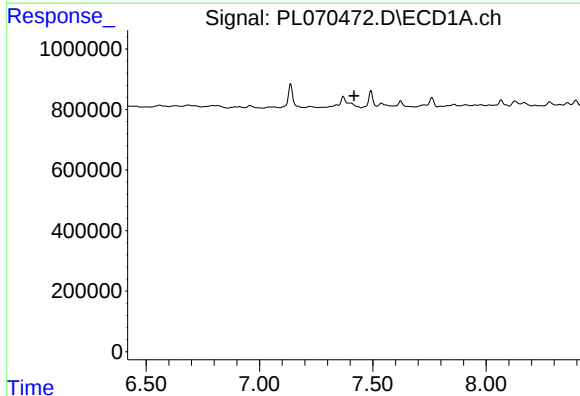


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.418 min
Response: 0
Conc: N.D.

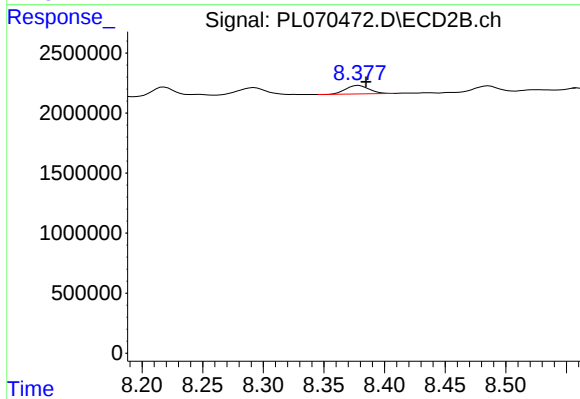

#26 Chlordane-4


R.T.: 8.379 min
Delta R.T.: -0.006 min
Response: 934181
Conc: 3.68 ng/ml

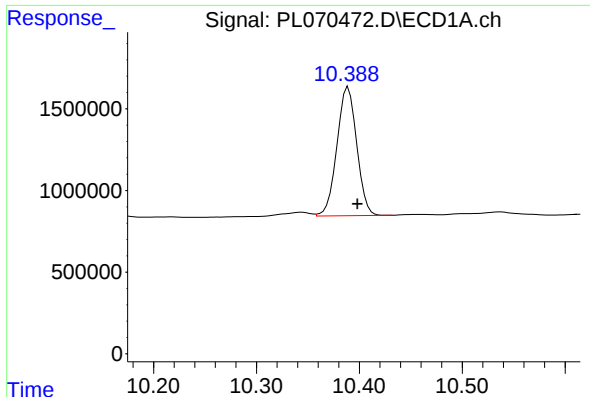

#28 Decachlorobiphenyl

R.T.: 10.389 min
Delta R.T.: -0.009 min
Response: 10536798
Conc: 15.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

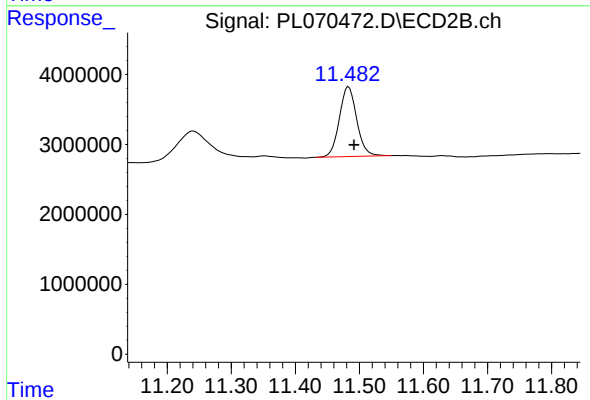

#28 Decachlorobiphenyl

R.T.: 11.483 min
Delta R.T.: -0.008 min
Response: 18831878
Conc: 15.56 ng/ml