

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102122\
 Data File : PL078439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2022 23:21
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 06:55:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 06:53:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	2.571	187.9E6	291.8E6	94.271	90.617
28)	SA Decachlor...	8.777	7.645	141.3E6	169.7E6	91.776	88.831
Target Compounds							
23)	Chlordane-1	4.472	3.538	74738458	91706630	936.499	906.291
24)	Chlordane-2	5.005	4.105	75773578	94317724	901.228	880.275
25)	Chlordane-3	5.715	4.725	332.1E6	285.9E6	959.908	920.853
26)	Chlordane-4	5.793	4.785	401.2E6	301.6E6	952.520	915.814
27)	Chlordane-5	6.649	5.447	64423849	76242587	940.739	910.351



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102122\
Data File : PL078439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2022 23:21
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 06:55:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 06:53:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

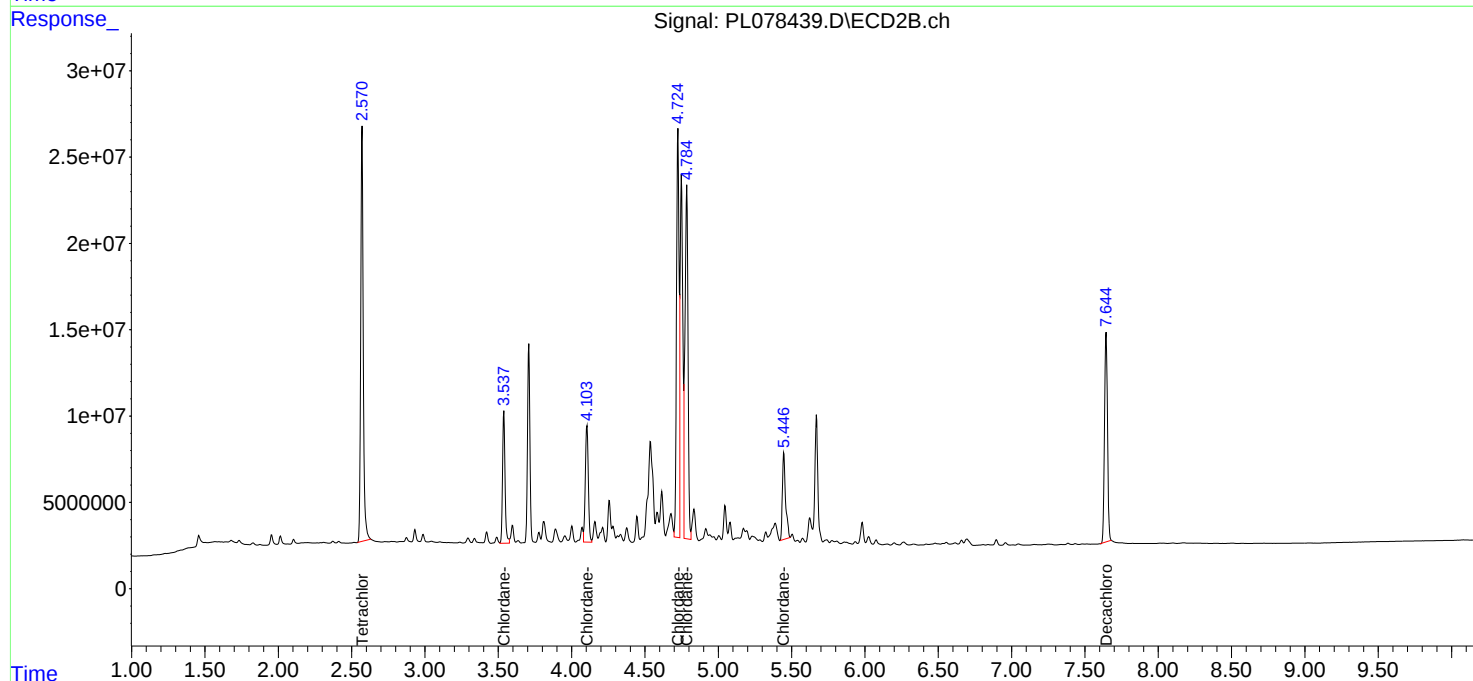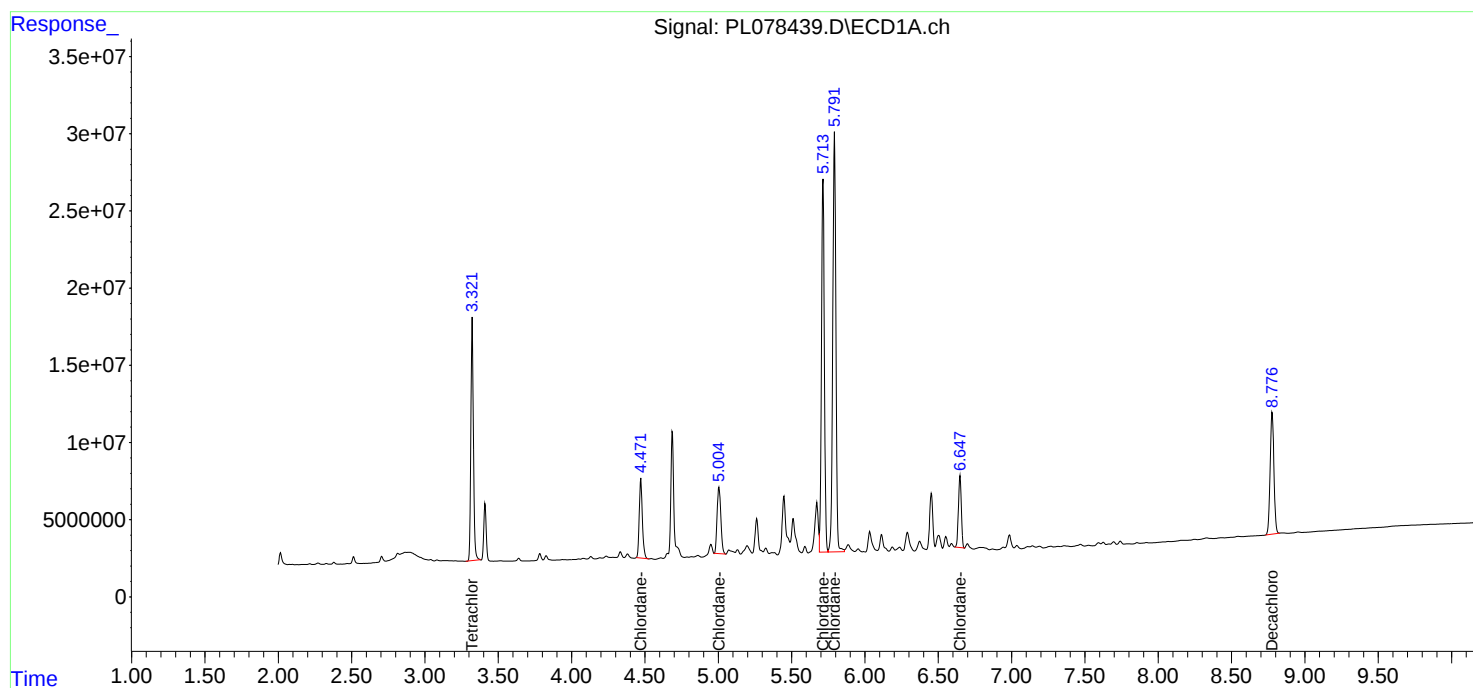


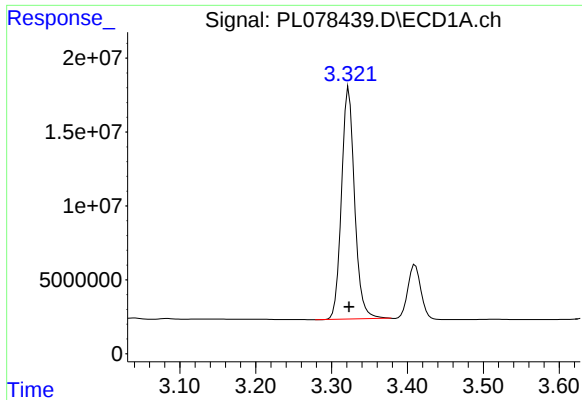

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 187935579
Conc: 94.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

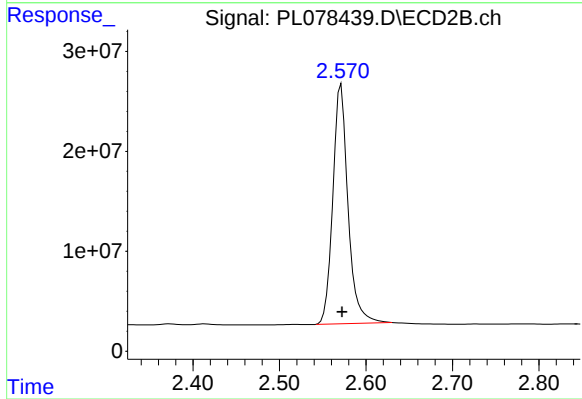


#1 Tetrachloro-m-xylene

R.T.: 2.571 min
Delta R.T.: -0.001 min
Response: 291788308
Conc: 90.62 ng/ml

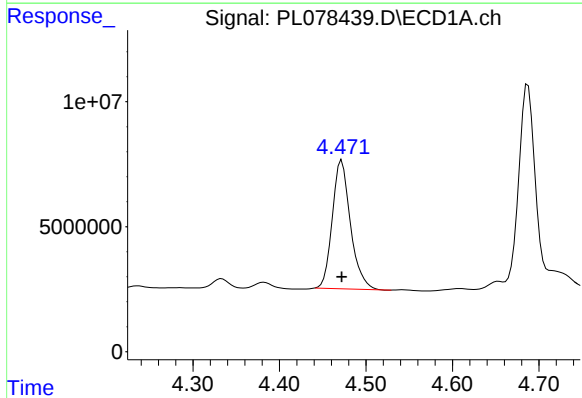


#23 Chlordane-1

R.T.: 4.472 min
Delta R.T.: 0.000 min
Response: 74738458
Conc: 936.50 ng/ml

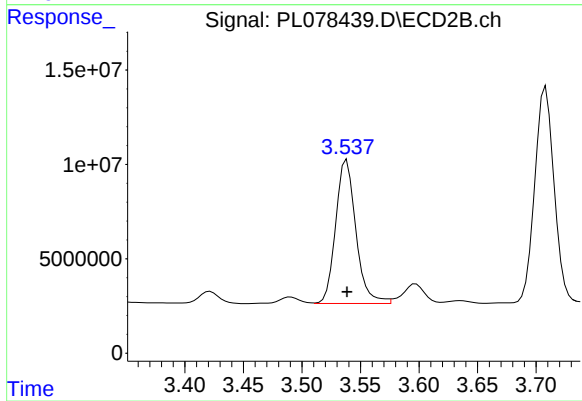

#23 Chlordane-1


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 91706630
Conc: 906.29 ng/ml

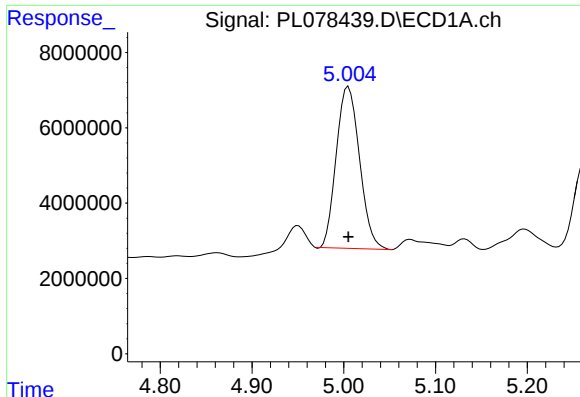

#24 Chlordane-2


R.T.: 5.005 min
Delta R.T.: 0.000 min
Response: 75773578
Conc: 901.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

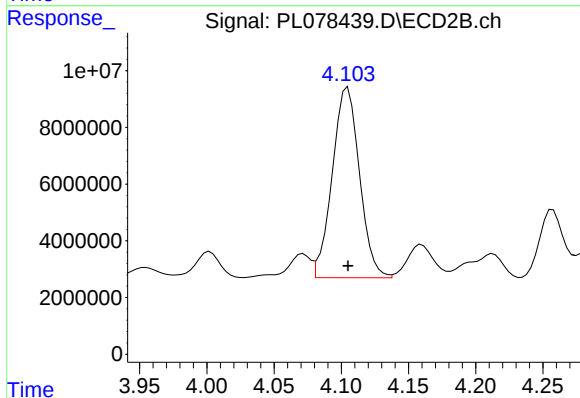


#24 Chlordane-2

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 94317724
Conc: 880.28 ng/ml

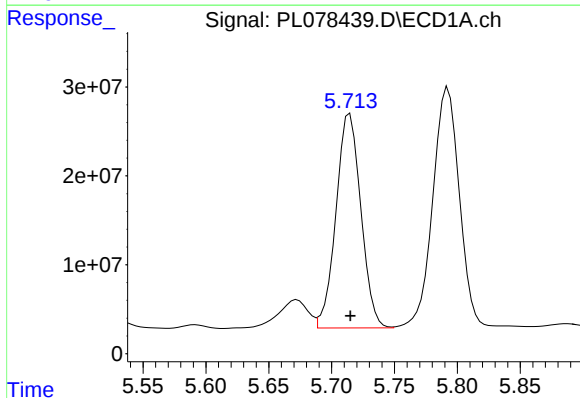


#25 Chlordane-3

R.T.: 5.715 min
Delta R.T.: 0.000 min
Response: 332085347
Conc: 959.91 ng/ml

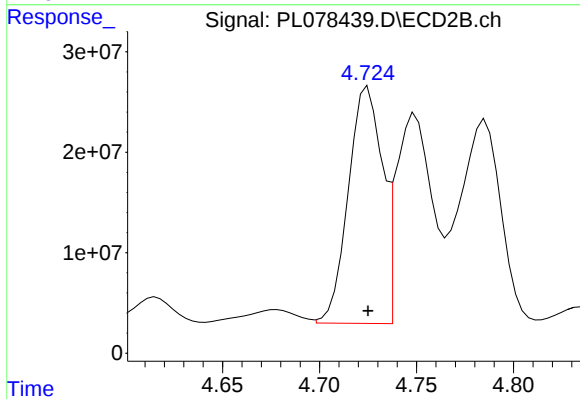

#25 Chlordane-3


R.T.: 4.725 min
Delta R.T.: 0.000 min
Response: 285922111
Conc: 920.85 ng/ml

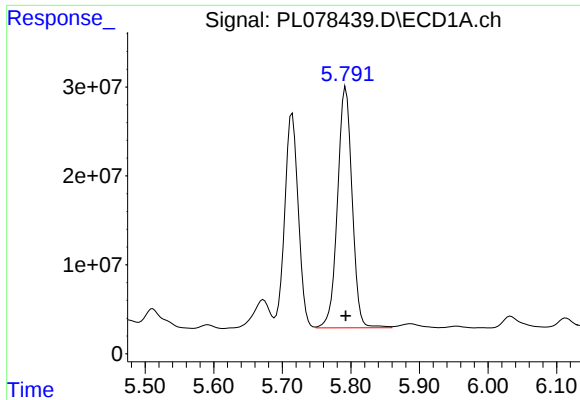

#26 Chlordane-4


R.T.: 5.793 min
Delta R.T.: 0.000 min
Response: 401247042
Conc: 952.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

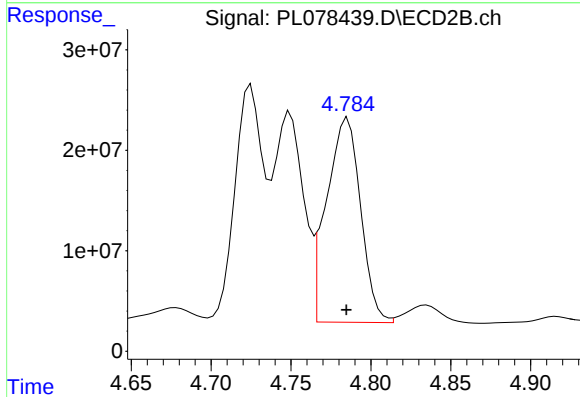


#26 Chlordane-4

R.T.: 4.785 min
Delta R.T.: 0.000 min
Response: 301554165
Conc: 915.81 ng/ml

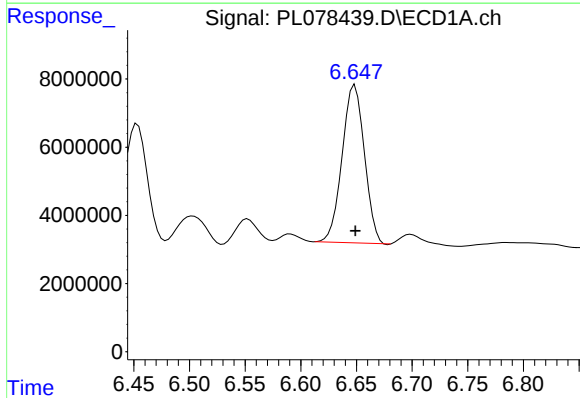


#27 Chlordane-5

R.T.: 6.649 min
Delta R.T.: 0.000 min
Response: 64423849
Conc: 940.74 ng/ml

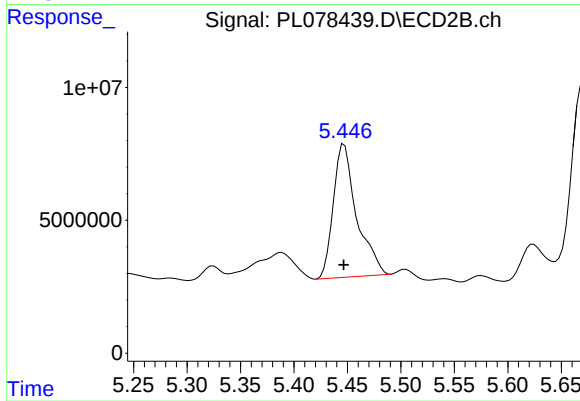

#27 Chlordane-5


R.T.: 5.447 min
Delta R.T.: 0.000 min
Response: 76242587
Conc: 910.35 ng/ml

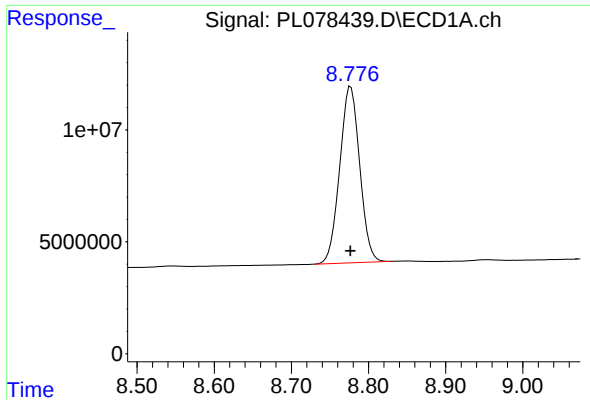

#28 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: 0.000 min
Response: 141342914
Conc: 91.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

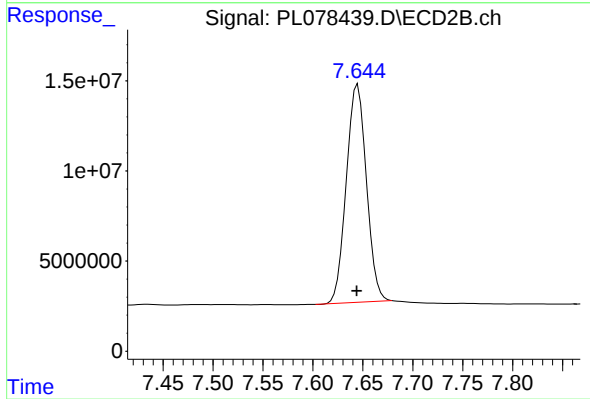

#28 Decachlorobiphenyl

R.T.: 7.645 min
Delta R.T.: 0.001 min
Response: 169721898
Conc: 88.83 ng/ml