

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102122\
 Data File : PL078441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2022 23:48
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 06:56:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 06:53:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	2.573	99678471	161.0E6	50.000	50.000
28)	SA Decachlor...	8.777	7.644	77004044	95530497	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.472	3.539	39903114	50594447	500.000	500.000
24)	Chlordane-2	5.005	4.105	42039065	53572863	500.000	500.000
25)	Chlordane-3	5.715	4.725	173.0E6	155.2E6	500.000	500.000
26)	Chlordane-4	5.793	4.785	210.6E6	164.6E6	500.000	500.000
27)	Chlordane-5	6.649	5.446	34241070	41875362	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102122\
Data File : PL078441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2022 23:48
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 06:56:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 06:53:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

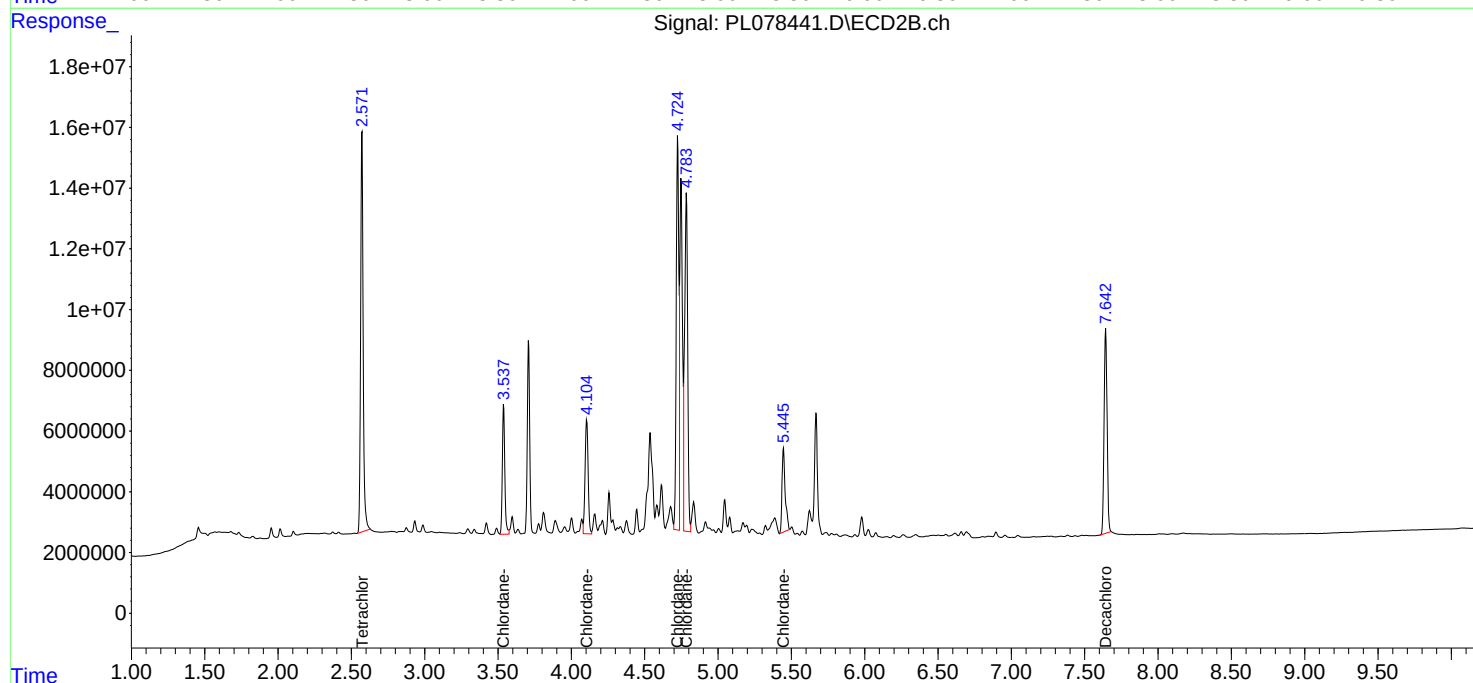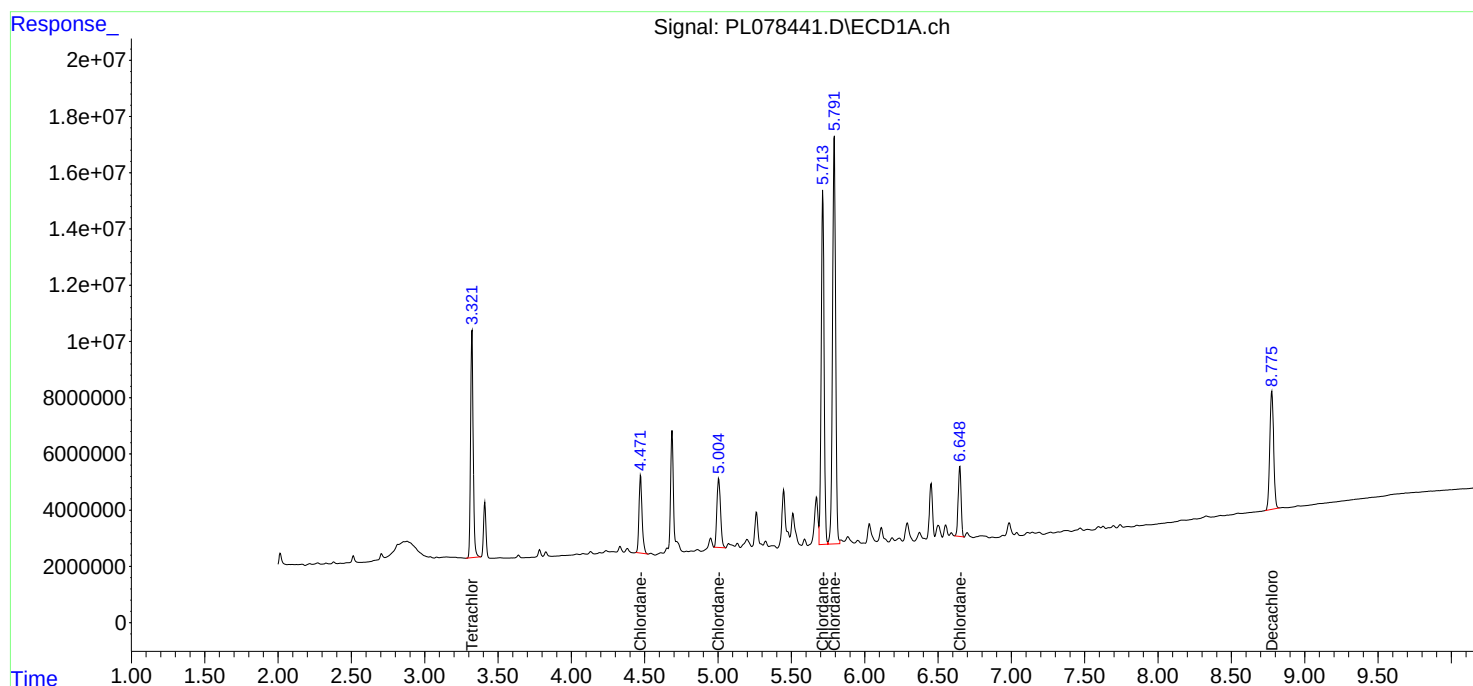


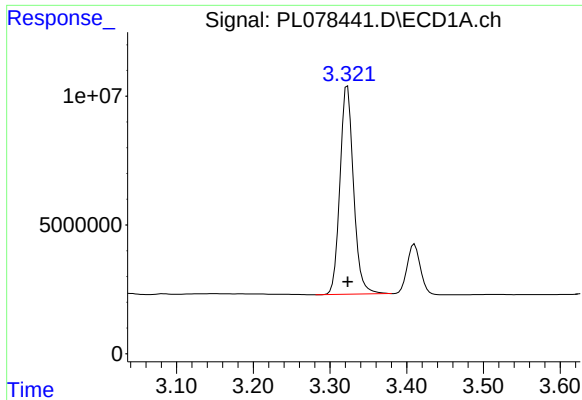

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 99678471
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

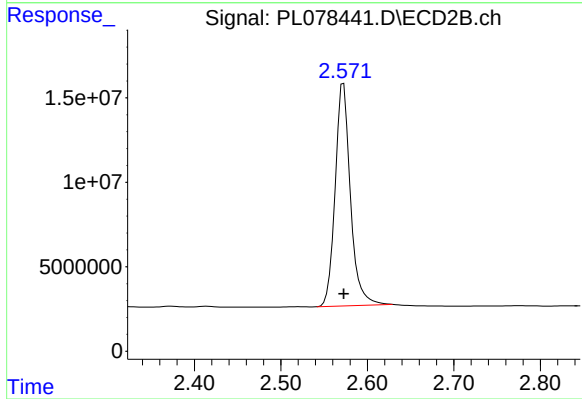


#1 Tetrachloro-m-xylene

R.T.: 2.573 min
Delta R.T.: 0.000 min
Response: 161000263
Conc: 50.00 ng/ml

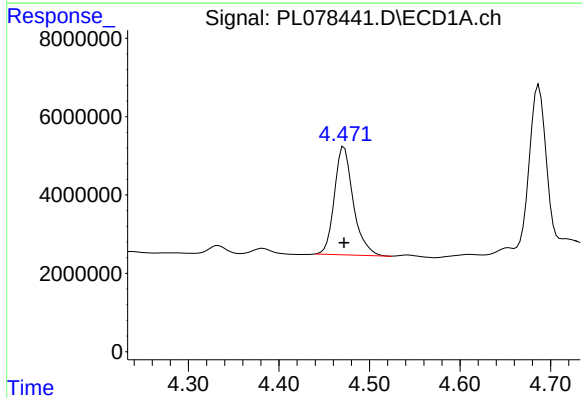


#23 Chlordane-1

R.T.: 4.472 min
Delta R.T.: 0.000 min
Response: 39903114
Conc: 500.00 ng/ml

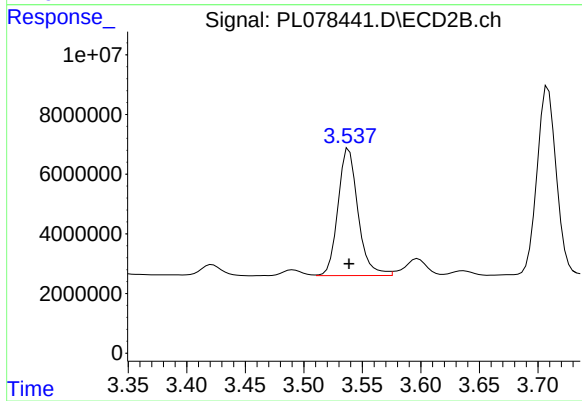

#23 Chlordane-1


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 50594447
Conc: 500.00 ng/ml

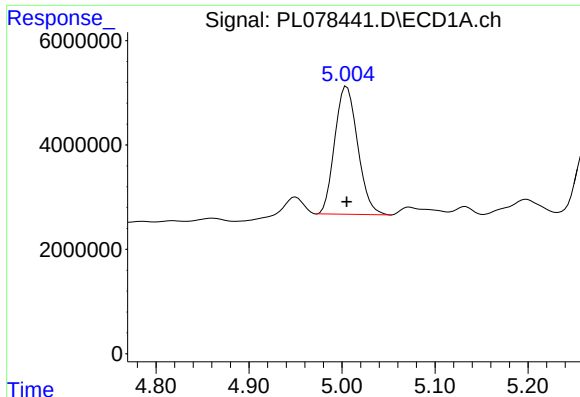

#24 Chlordane-2


R.T.: 5.005 min
Delta R.T.: 0.000 min
Response: 42039065
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

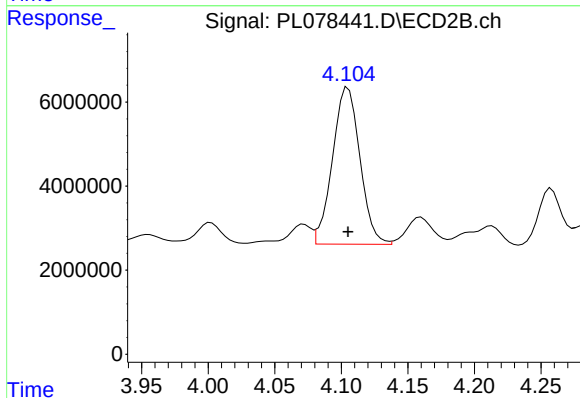


#24 Chlordane-2

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 53572863
Conc: 500.00 ng/ml

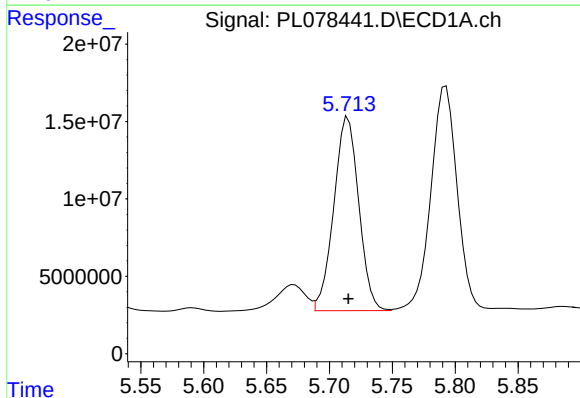


#25 Chlordane-3

R.T.: 5.715 min
Delta R.T.: 0.000 min
Response: 172977748
Conc: 500.00 ng/ml

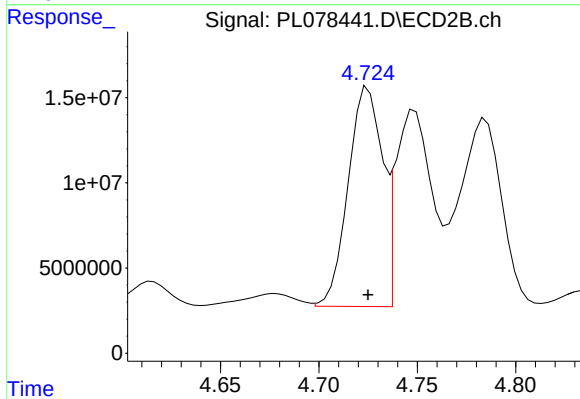

#25 Chlordane-3


R.T.: 4.725 min
Delta R.T.: 0.000 min
Response: 155248553
Conc: 500.00 ng/ml

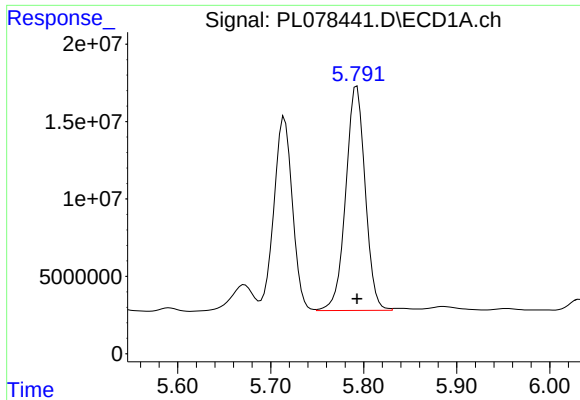

#26 Chlordane-4


R.T.: 5.793 min
Delta R.T.: 0.000 min
Response: 210623935
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

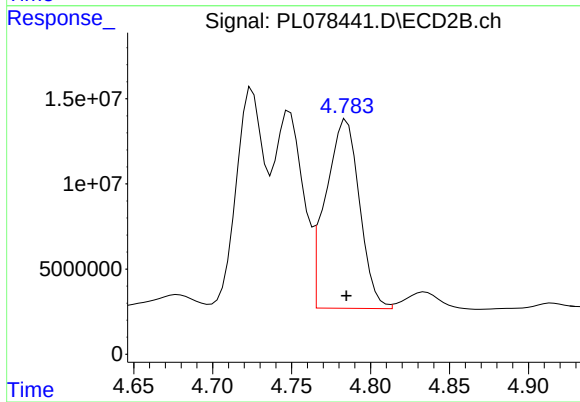


#26 Chlordane-4

R.T.: 4.785 min
Delta R.T.: 0.000 min
Response: 164637152
Conc: 500.00 ng/ml

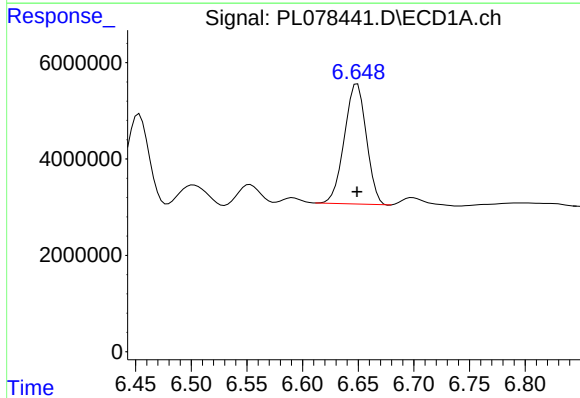


#27 Chlordane-5

R.T.: 6.649 min
Delta R.T.: 0.000 min
Response: 34241070
Conc: 500.00 ng/ml

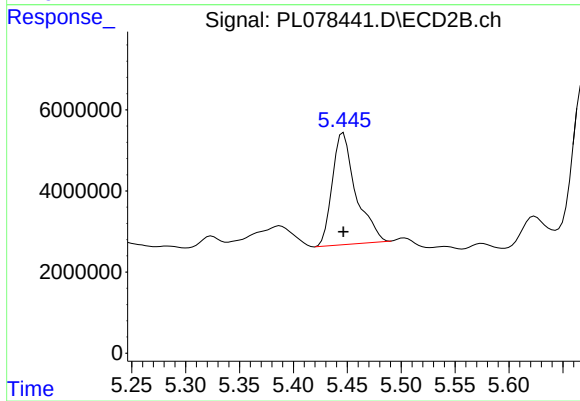

#27 Chlordane-5


R.T.: 5.446 min
Delta R.T.: 0.000 min
Response: 41875362
Conc: 500.00 ng/ml

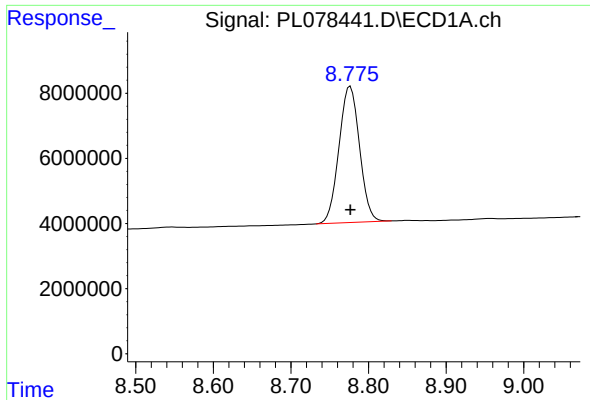

#28 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: 0.000 min
Response: 77004044
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

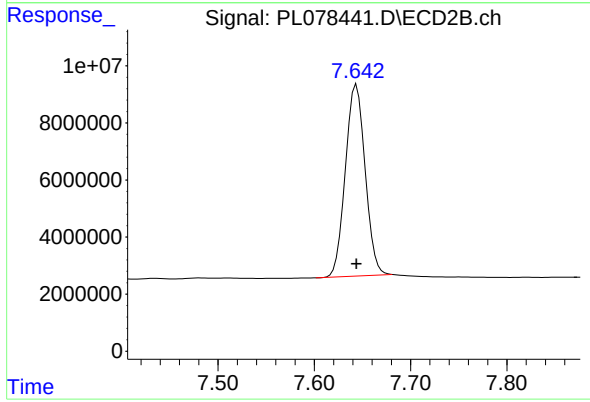

#28 Decachlorobiphenyl

R.T.: 7.644 min
Delta R.T.: 0.000 min
Response: 95530497
Conc: 50.00 ng/ml