

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102122\
 Data File : PL078442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2022 00:02
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 06:56:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 06:53:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	2.572	47752026	77744845	23.953	24.144
28)	SA Decachlor...	8.776	7.645	38092680	48456539	24.734	25.362
Target Compounds							
23)	Chlordane-1	4.472	3.538	19082236	24956231	239.107	246.630
24)	Chlordane-2	5.005	4.105	20574530	27525875	244.707	256.901
25)	Chlordane-3	5.715	4.725	80582842	74892365	232.928	241.201
26)	Chlordane-4	5.793	4.785	100.1E6	81050119	237.658	246.148
27)	Chlordane-5	6.649	5.447	15772871	20584558	230.321	245.784



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102122\
Data File : PL078442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2022 00:02
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 06:56:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 06:53:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

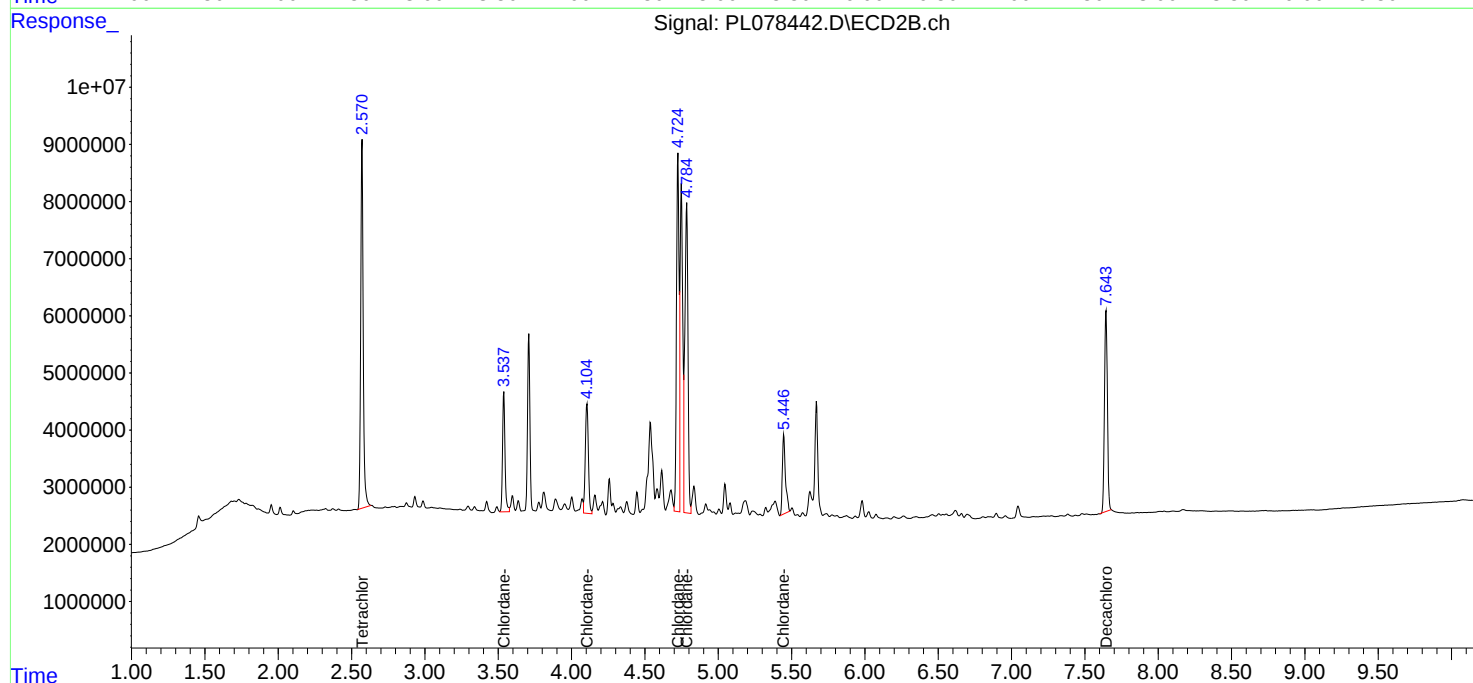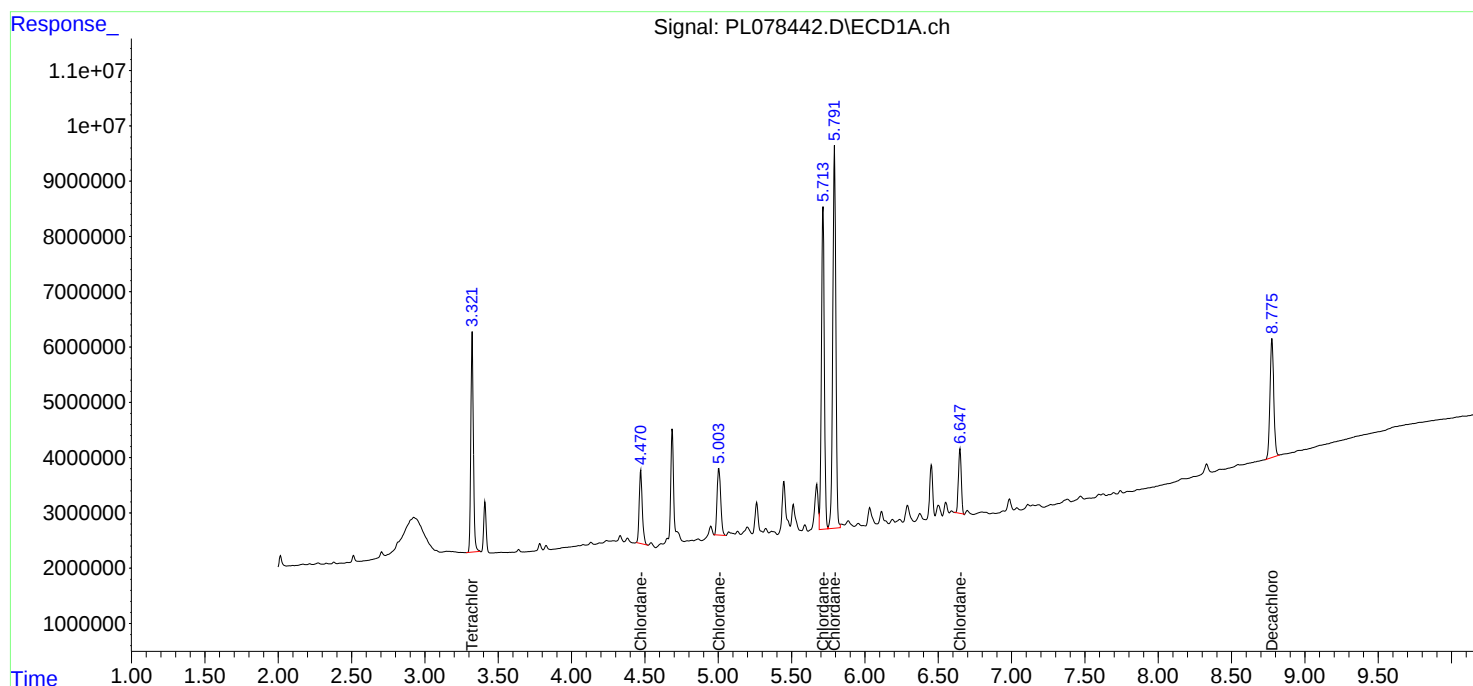


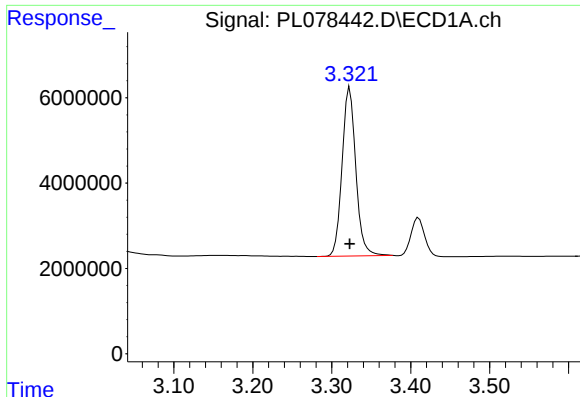

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 47752026
Conc: 23.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

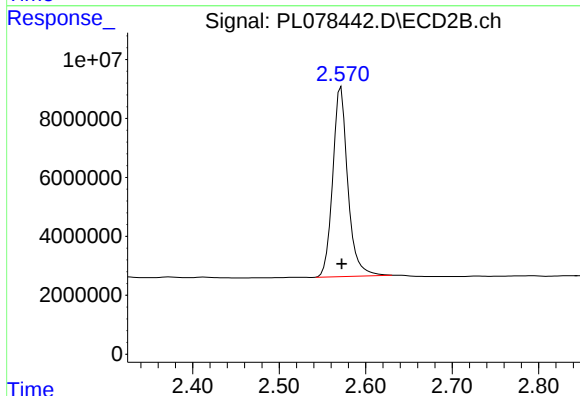


#1 Tetrachloro-m-xylene

R.T.: 2.572 min
Delta R.T.: 0.000 min
Response: 77744845
Conc: 24.14 ng/ml

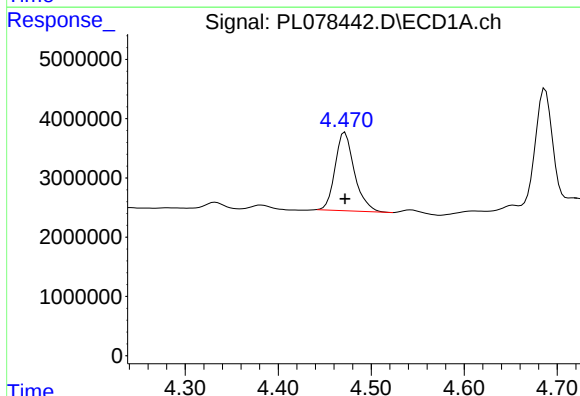


#23 Chlordane-1

R.T.: 4.472 min
Delta R.T.: 0.000 min
Response: 19082236
Conc: 239.11 ng/ml

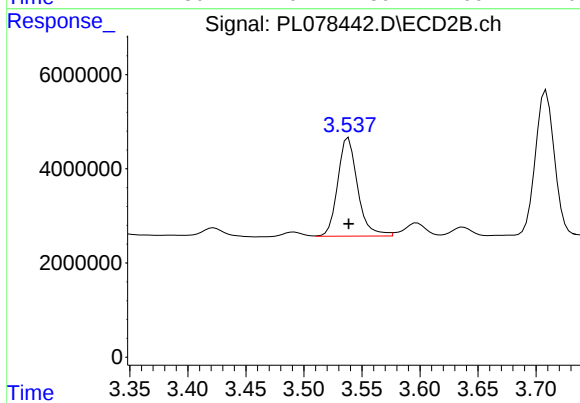

#23 Chlordane-1


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 24956231
Conc: 246.63 ng/ml

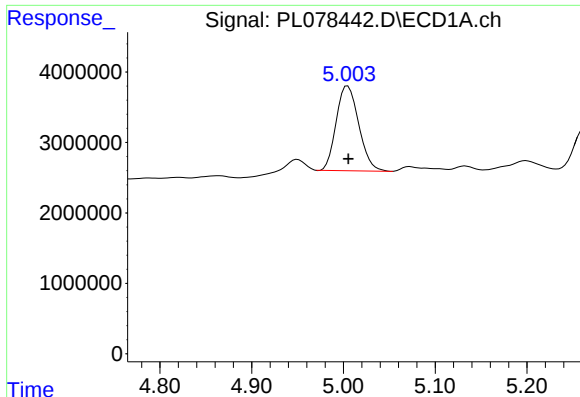

#24 Chlordane-2


R.T.: 5.005 min
Delta R.T.: 0.000 min
Response: 20574530
Conc: 244.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

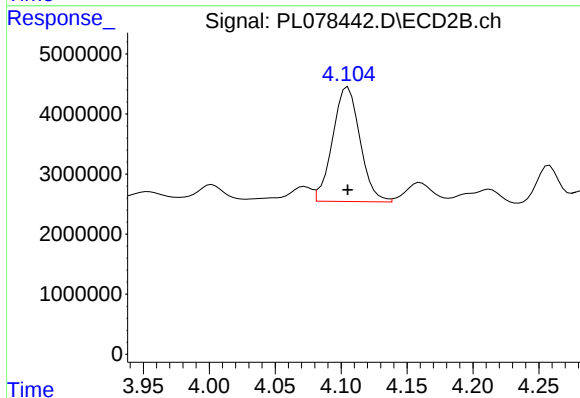


#24 Chlordane-2

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 27525875
Conc: 256.90 ng/ml

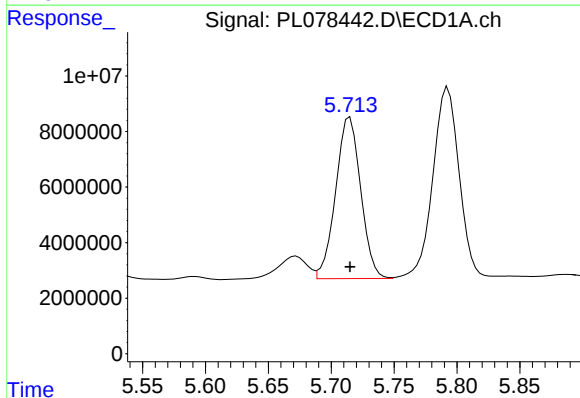


#25 Chlordane-3

R.T.: 5.715 min
Delta R.T.: 0.000 min
Response: 80582842
Conc: 232.93 ng/ml

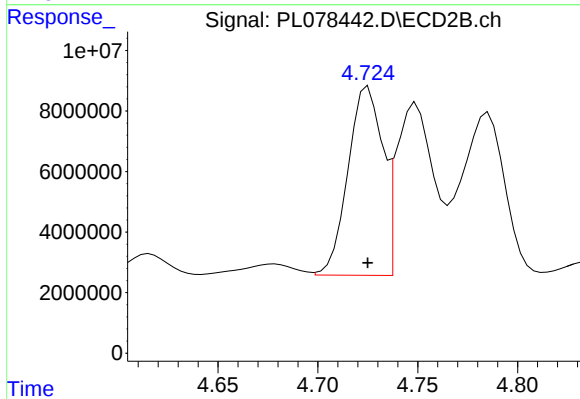

#25 Chlordane-3


R.T.: 4.725 min
Delta R.T.: 0.000 min
Response: 74892365
Conc: 241.20 ng/ml

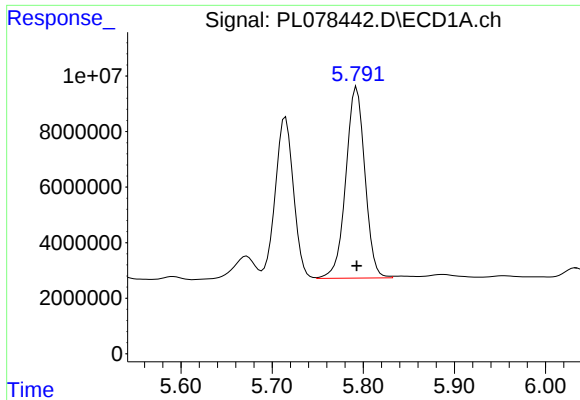

#26 Chlordane-4


R.T.: 5.793 min
Delta R.T.: 0.000 min
Response: 100112932
Conc: 237.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

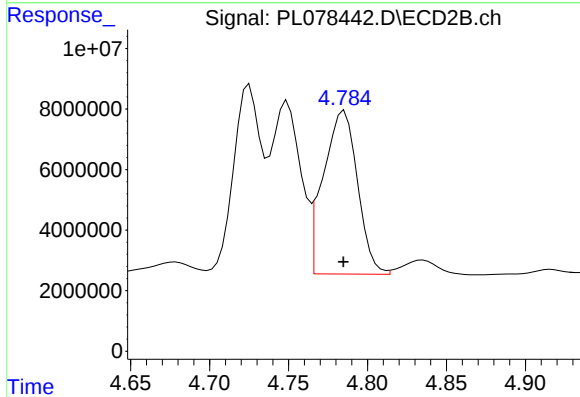


#26 Chlordane-4

R.T.: 4.785 min
Delta R.T.: 0.000 min
Response: 81050119
Conc: 246.15 ng/ml

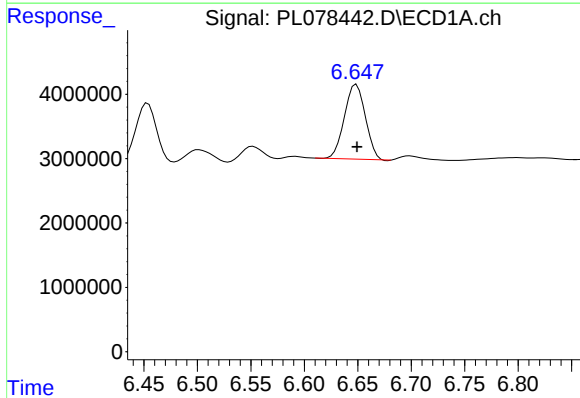


#27 Chlordane-5

R.T.: 6.649 min
Delta R.T.: 0.000 min
Response: 15772871
Conc: 230.32 ng/ml

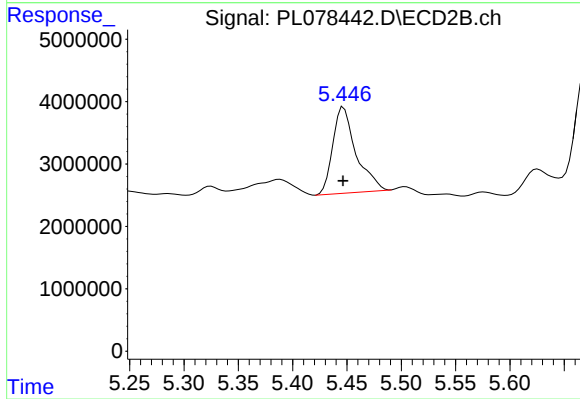

#27 Chlordane-5


R.T.: 5.447 min
Delta R.T.: 0.000 min
Response: 20584558
Conc: 245.78 ng/ml

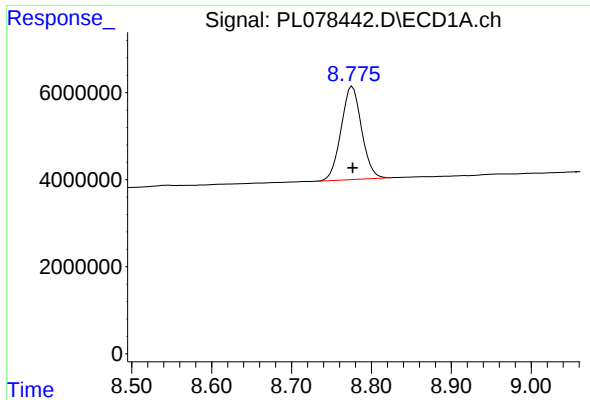

#28 Decachlorobiphenyl

R.T.: 8.776 min
Delta R.T.: 0.000 min
Response: 38092680
Conc: 24.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

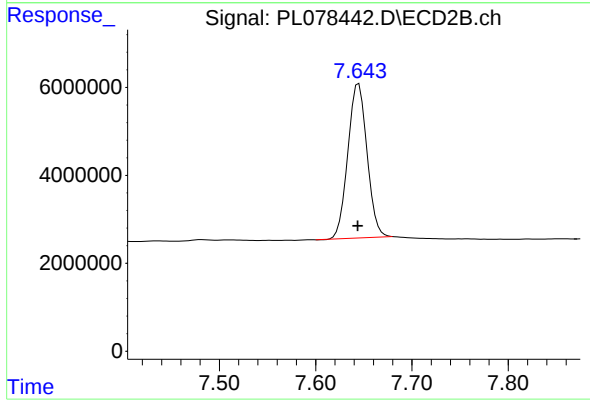

#28 Decachlorobiphenyl

R.T.: 7.645 min
Delta R.T.: 0.000 min
Response: 48456539
Conc: 25.36 ng/ml