

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102122\
 Data File : PL078450.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2022 01:53
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL102122CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 06:57:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 06:53:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	2.572	103.5E6	154.9E6	51.941	48.106
28)	SA Decachlor...	8.777	7.645	80375187	94719934	52.189	49.576
Target Compounds							
23)	Chlordane-1	4.472	3.539	41665851	50050091	522.088	494.620
24)	Chlordane-2	5.005	4.106	43240461	53154161	514.289	496.092
25)	Chlordane-3	5.715	4.727	179.6E6	152.0E6	519.263	489.648
26)	Chlordane-4	5.793	4.787	217.7E6	163.2E6	516.704	495.604
27)	Chlordane-5	6.649	5.448	35429788	41820213	517.358	499.342



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102122\
Data File : PL078450.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2022 01:53
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL102122CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 06:57:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 06:53:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

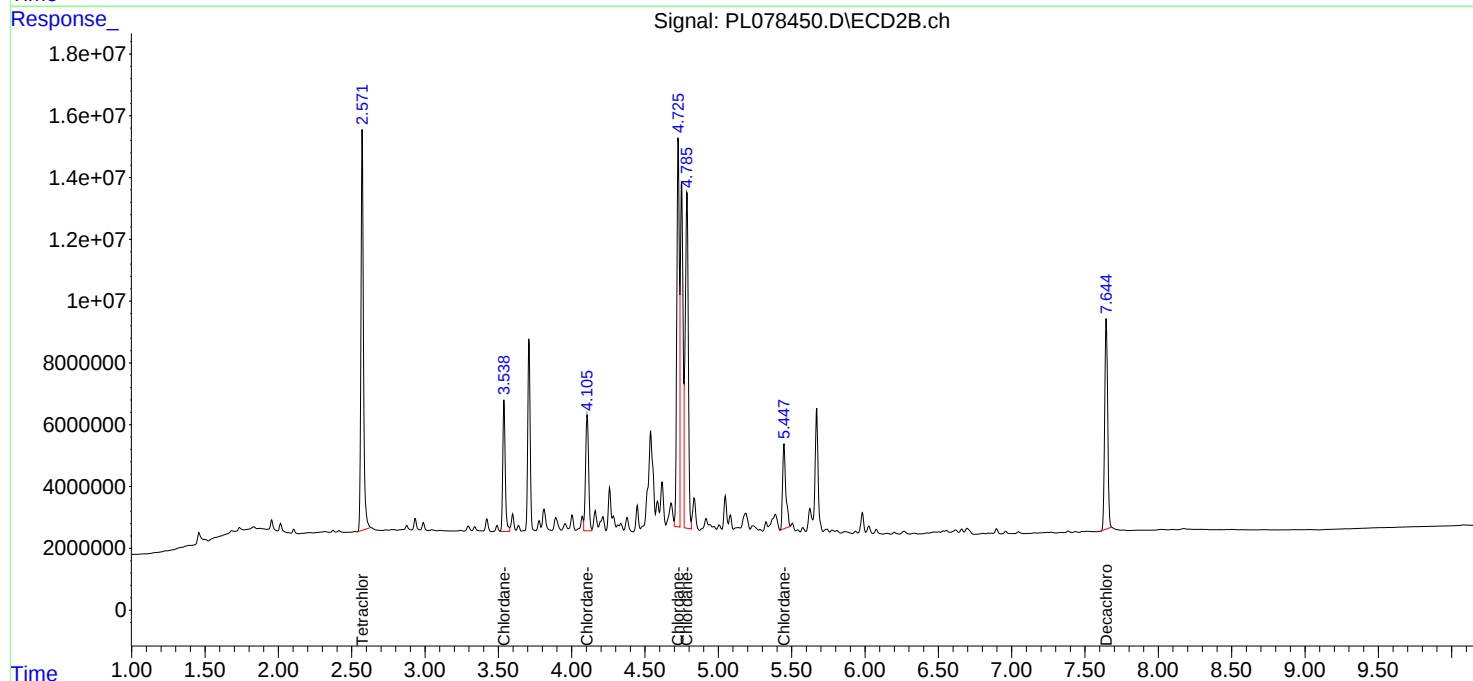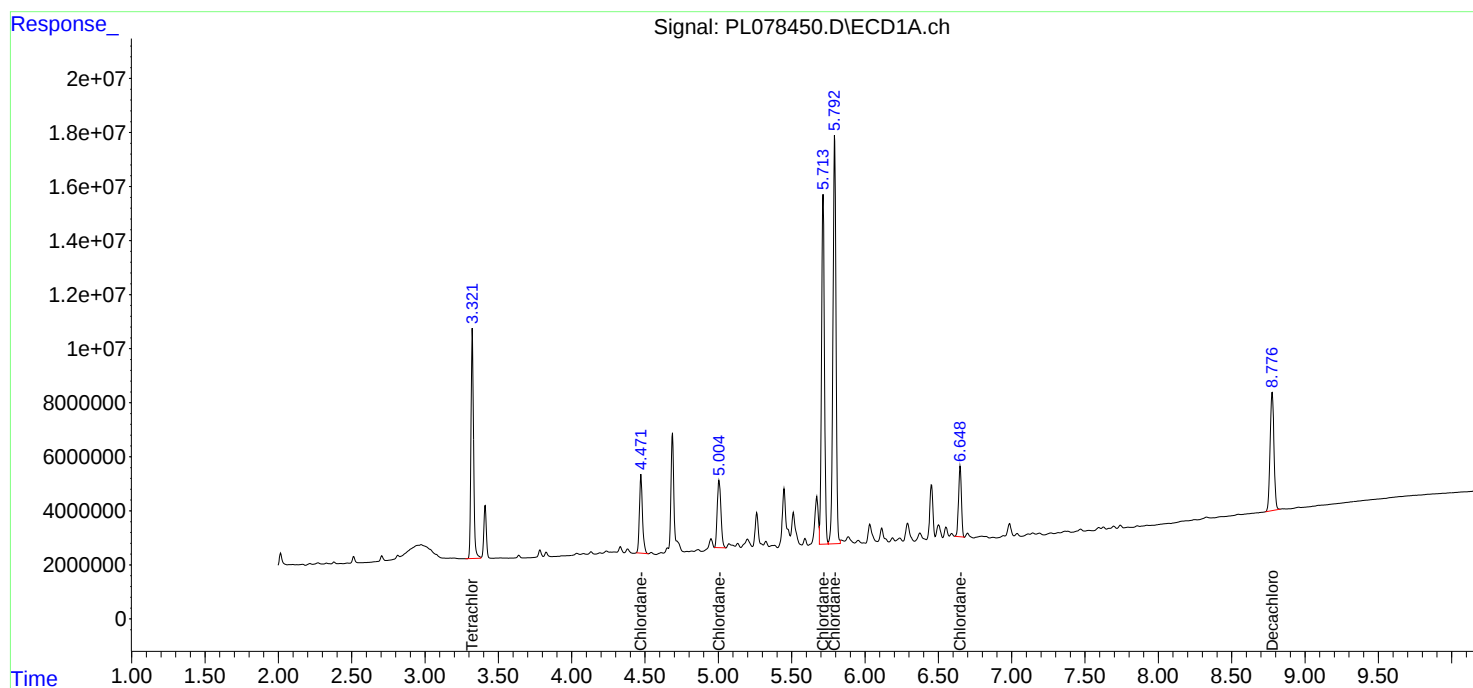


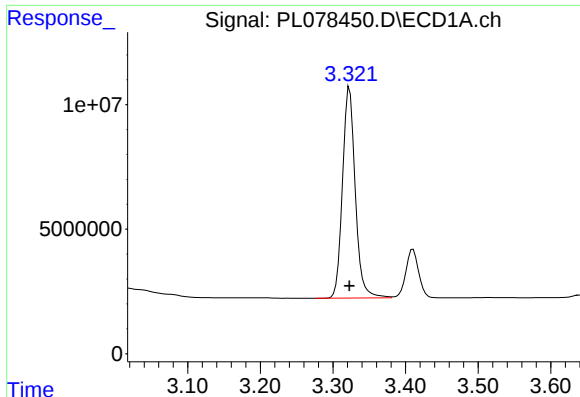

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 103548263
Conc: 51.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL102122CHLOR

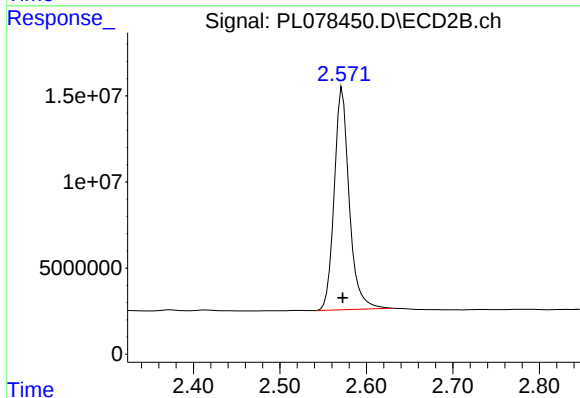


#1 Tetrachloro-m-xylene

R.T.: 2.572 min
Delta R.T.: 0.000 min
Response: 154902143
Conc: 48.11 ng/ml

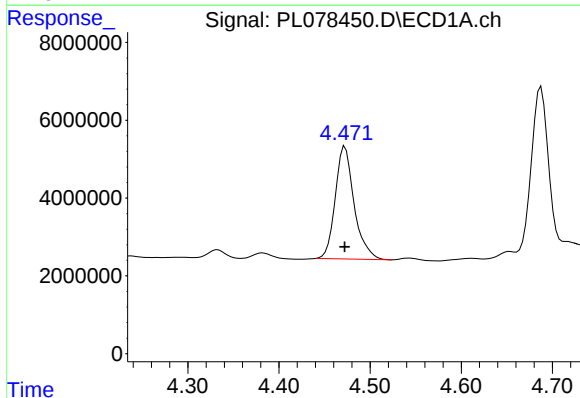


#23 Chlordane-1

R.T.: 4.472 min
Delta R.T.: 0.000 min
Response: 41665851
Conc: 522.09 ng/ml

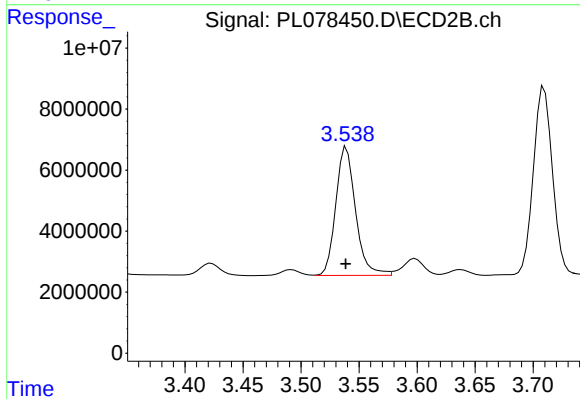

#23 Chlordane-1


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 50050091
Conc: 494.62 ng/ml

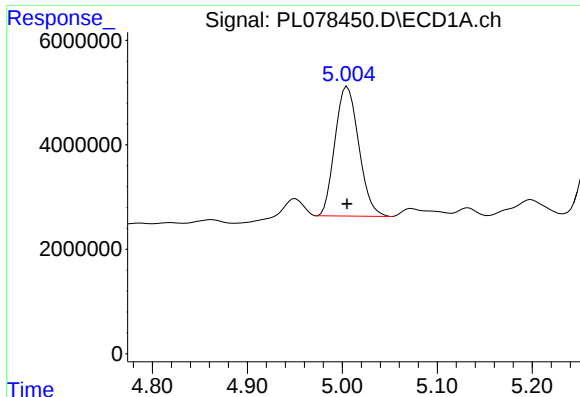

#24 Chlordane-2


R.T.: 5.005 min
Delta R.T.: 0.000 min
Response: 43240461
Conc: 514.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL102122CHLOR

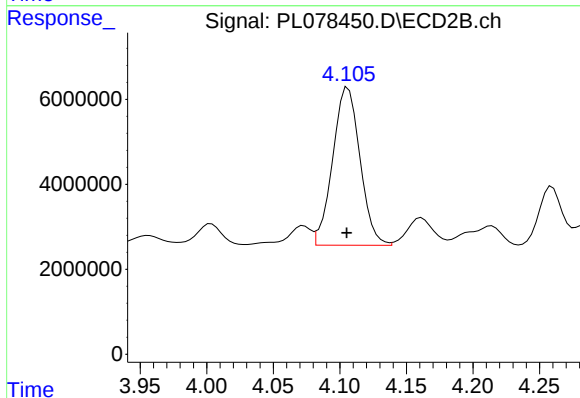


#24 Chlordane-2

R.T.: 4.106 min
Delta R.T.: 0.001 min
Response: 53154161
Conc: 496.09 ng/ml

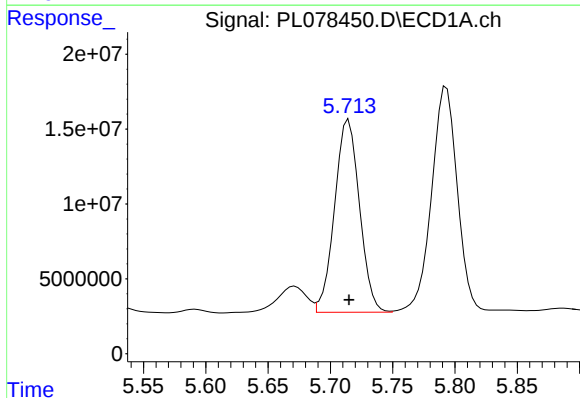


#25 Chlordane-3

R.T.: 5.715 min
Delta R.T.: 0.000 min
Response: 179641772
Conc: 519.26 ng/ml

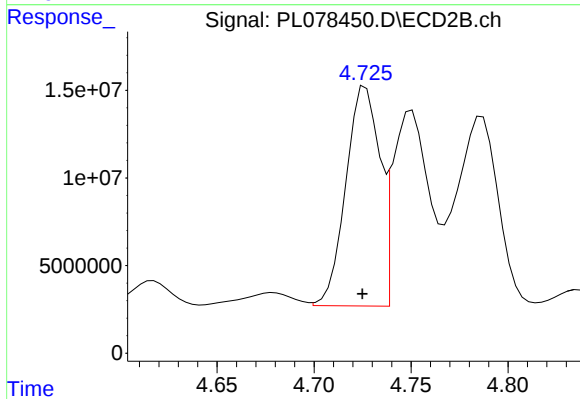

#25 Chlordane-3


R.T.: 4.727 min
Delta R.T.: 0.002 min
Response: 152034133
Conc: 489.65 ng/ml

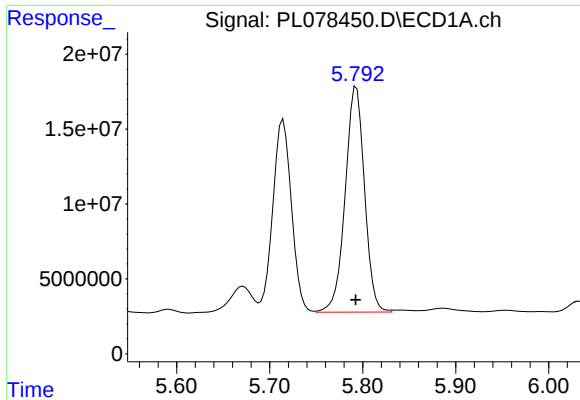

#26 Chlordane-4


R.T.: 5.793 min
Delta R.T.: 0.000 min
Response: 217660654
Conc: 516.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL102122CHLOR

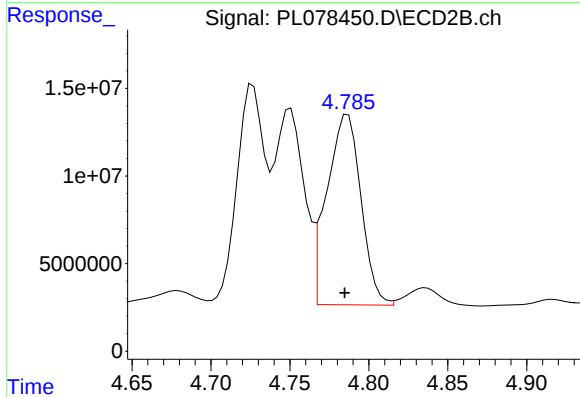


#26 Chlordane-4

R.T.: 4.787 min
Delta R.T.: 0.002 min
Response: 163189578
Conc: 495.60 ng/ml

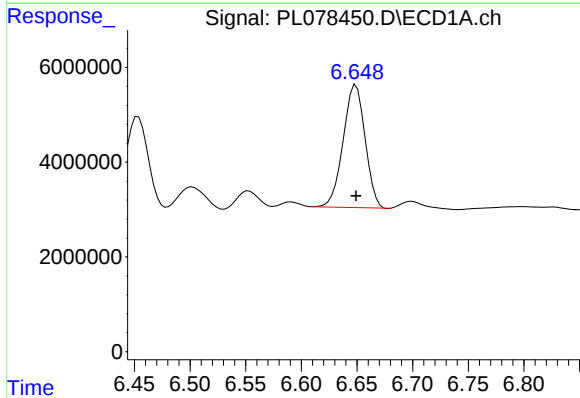


#27 Chlordane-5

R.T.: 6.649 min
Delta R.T.: 0.000 min
Response: 35429788
Conc: 517.36 ng/ml

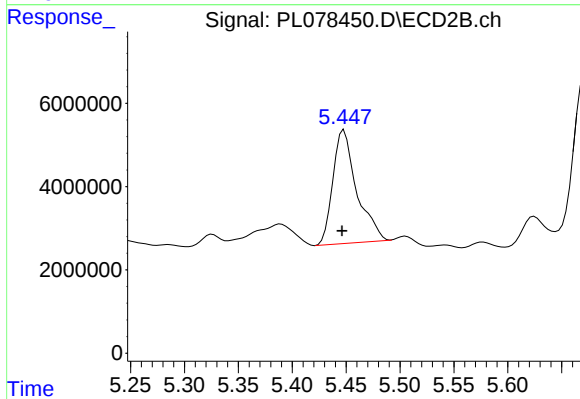

#27 Chlordane-5


R.T.: 5.448 min
Delta R.T.: 0.002 min
Response: 41820213
Conc: 499.34 ng/ml

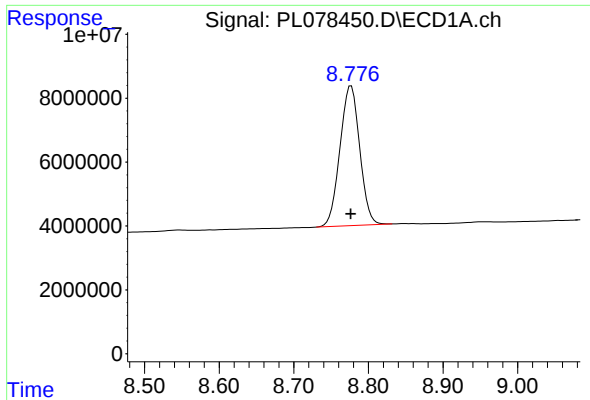

#28 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: 0.000 min
Response: 80375187
Conc: 52.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL102122CHLOR

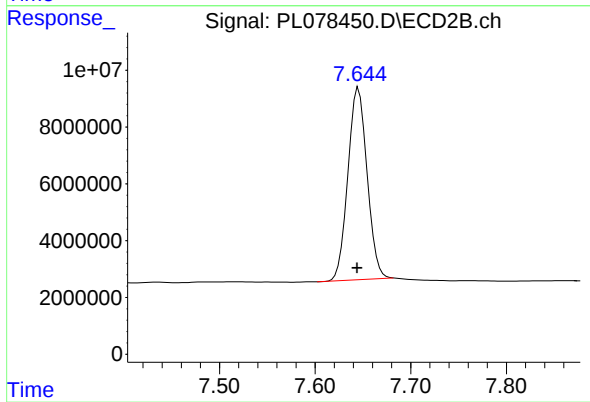

#28 Decachlorobiphenyl

R.T.: 7.645 min
Delta R.T.: 0.002 min
Response: 94719934
Conc: 49.58 ng/ml