

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102122\
 Data File : PL078440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2022 23:34
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 07:00:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:00:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	2.573	143.8E6	230.6E6	74.500	75.092
28)	SA Decachlor...	8.776	7.644	109.3E6	133.3E6	74.362	74.273
Target Compounds							
23)	Chlordane-1	4.472	3.539	57421872	71453337	745.393	743.875
24)	Chlordane-2	5.006	4.105	58557925	73744855	738.346	737.965
25)	Chlordane-3	5.715	4.725	251.4E6	219.5E6	744.410	740.695
26)	Chlordane-4	5.793	4.785	306.2E6	234.6E6	746.317	745.945
27)	Chlordane-5	6.649	5.446	49303784	59235932	744.604	743.626



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102122\
Data File : PL078440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2022 23:34
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 07:00:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:00:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

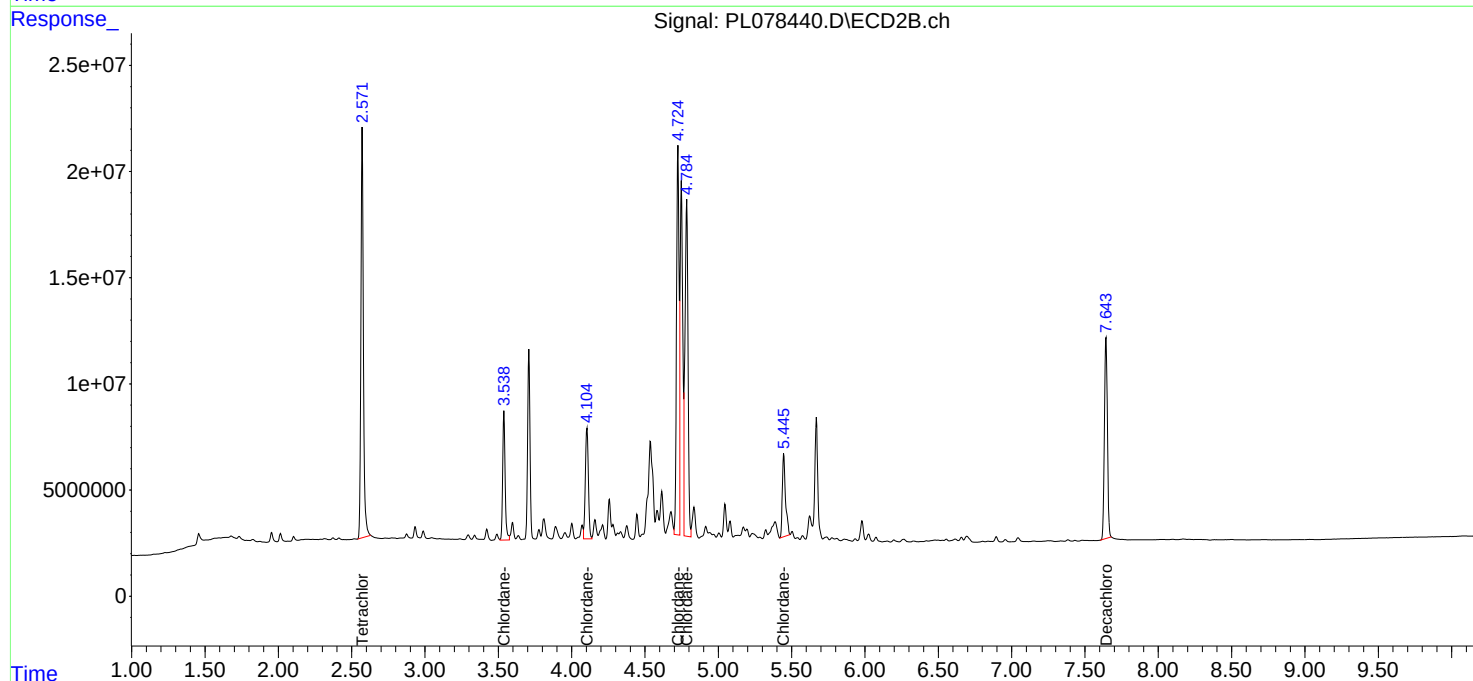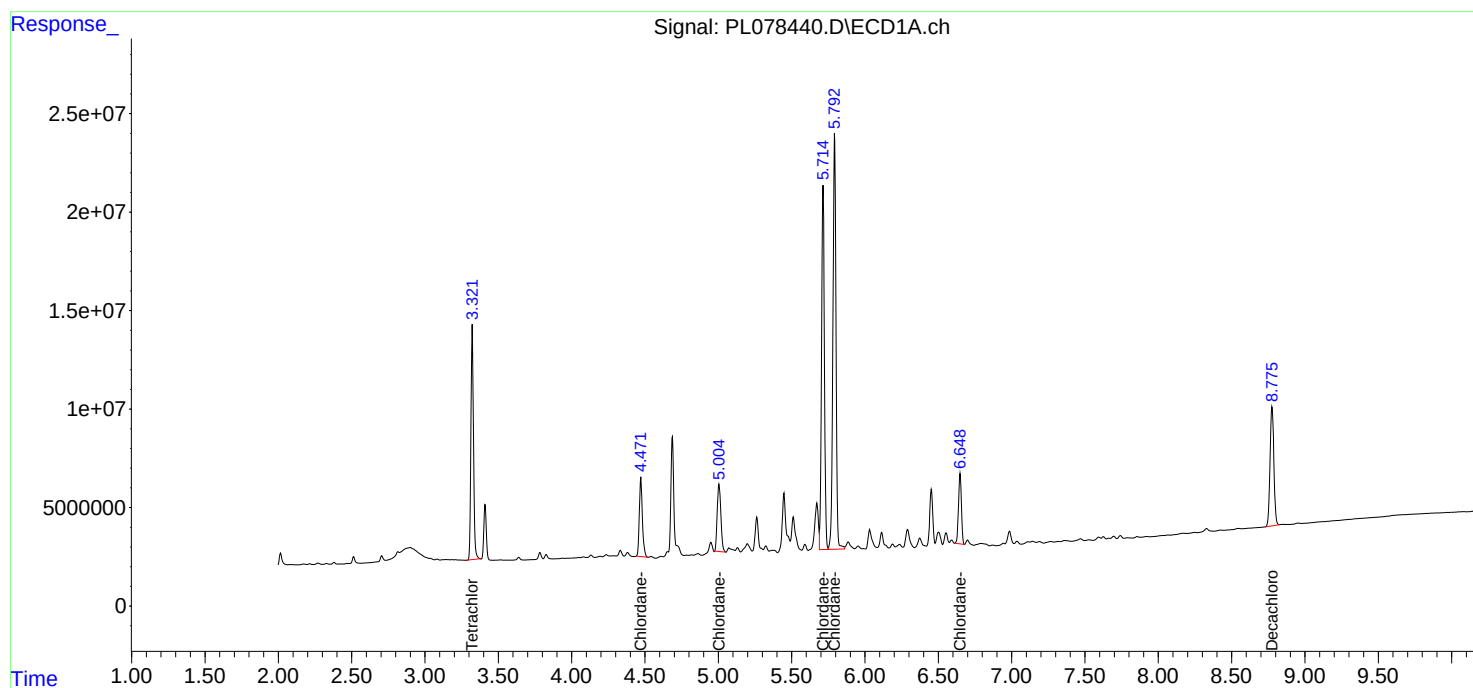


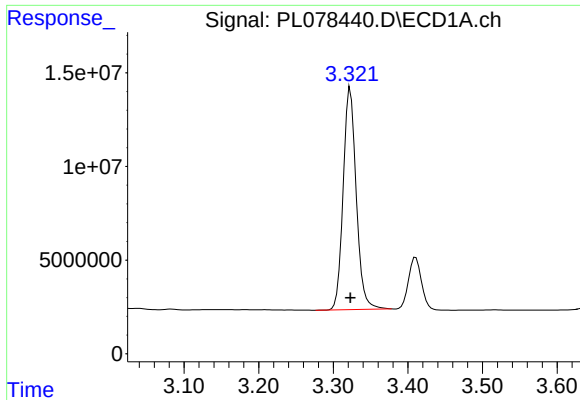

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 143788478
Conc: 74.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

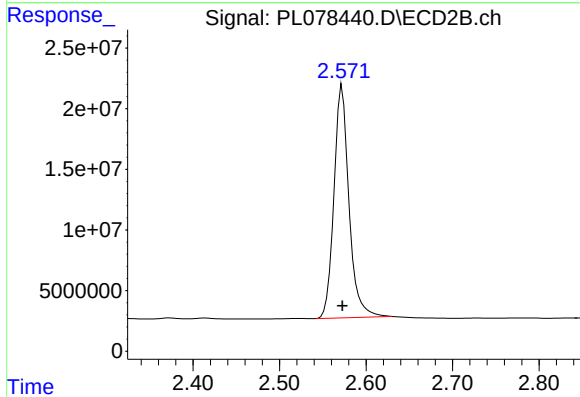


#1 Tetrachloro-m-xylene

R.T.: 2.573 min
Delta R.T.: 0.000 min
Response: 230595451
Conc: 75.09 ng/ml

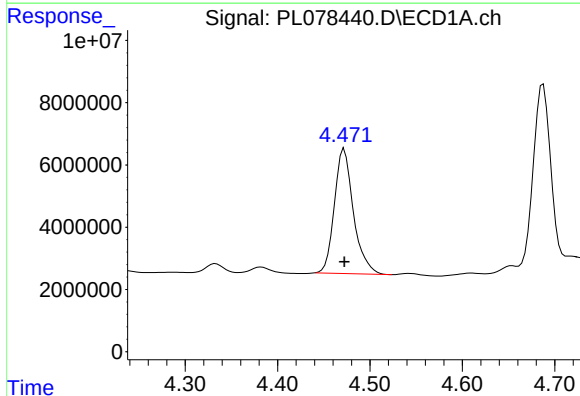


#23 Chlordane-1

R.T.: 4.472 min
Delta R.T.: 0.000 min
Response: 57421872
Conc: 745.39 ng/ml

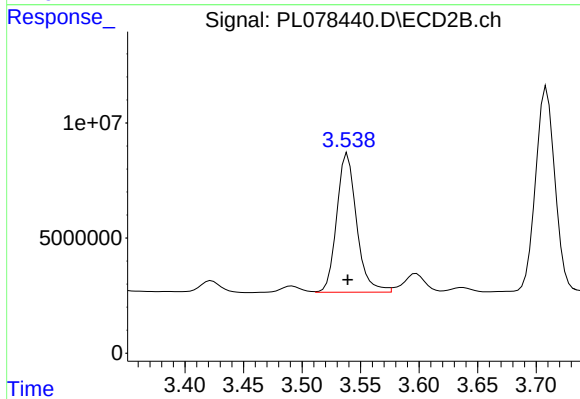

#23 Chlordane-1


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 71453337
Conc: 743.88 ng/ml

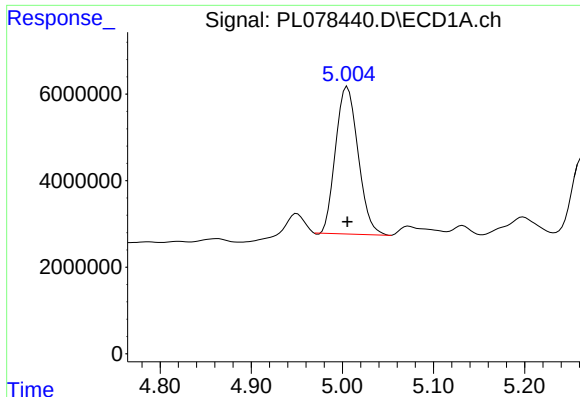

#24 Chlordane-2


R.T.: 5.006 min
Delta R.T.: 0.000 min
Response: 58557925
Conc: 738.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

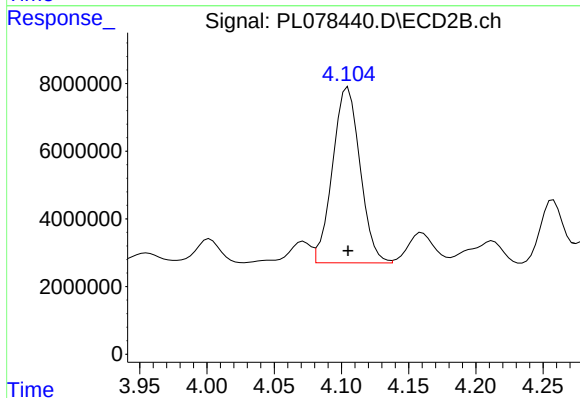


#24 Chlordane-2

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 73744855
Conc: 737.97 ng/ml

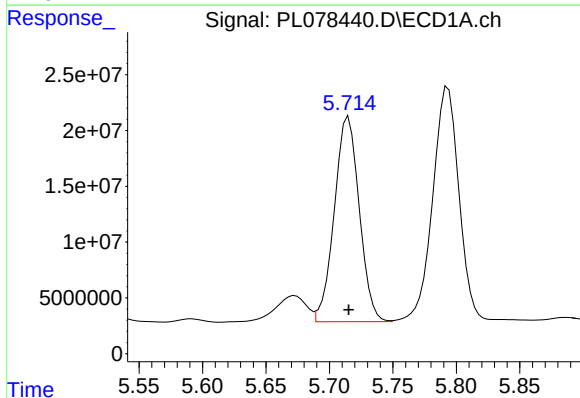


#25 Chlordane-3

R.T.: 5.715 min
Delta R.T.: 0.000 min
Response: 251432946
Conc: 744.41 ng/ml

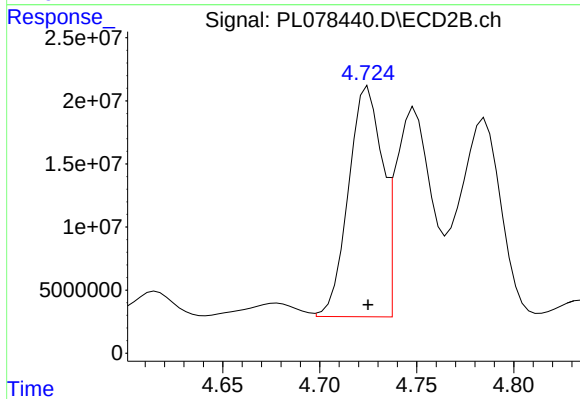

#25 Chlordane-3


R.T.: 4.725 min
Delta R.T.: 0.000 min
Response: 219520814
Conc: 740.70 ng/ml

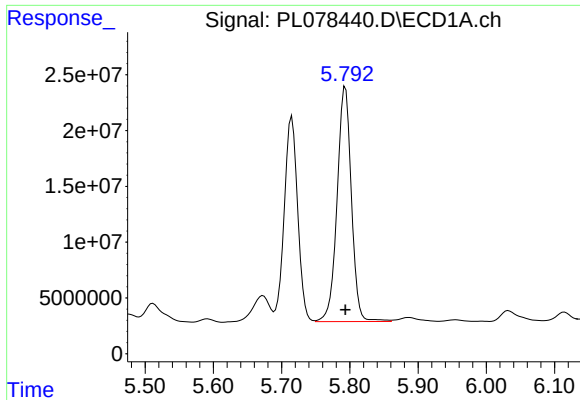

#26 Chlordane-4


R.T.: 5.793 min
Delta R.T.: 0.000 min
Response: 306169432
Conc: 746.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

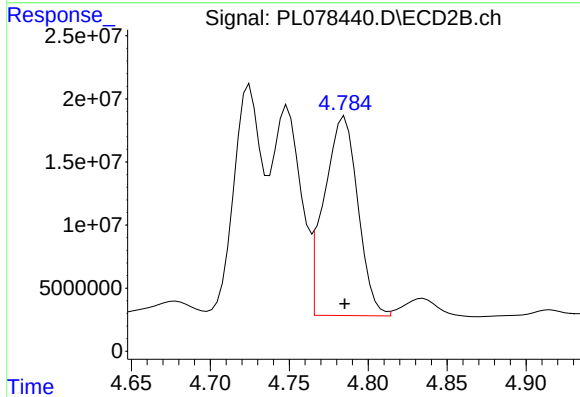


#26 Chlordane-4

R.T.: 4.785 min
Delta R.T.: 0.000 min
Response: 234647336
Conc: 745.94 ng/ml

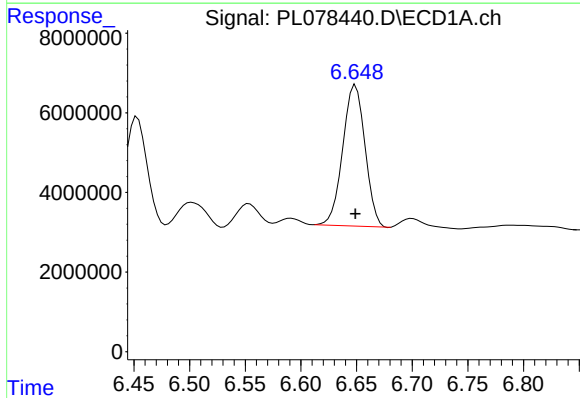


#27 Chlordane-5

R.T.: 6.649 min
Delta R.T.: 0.000 min
Response: 49303784
Conc: 744.60 ng/ml

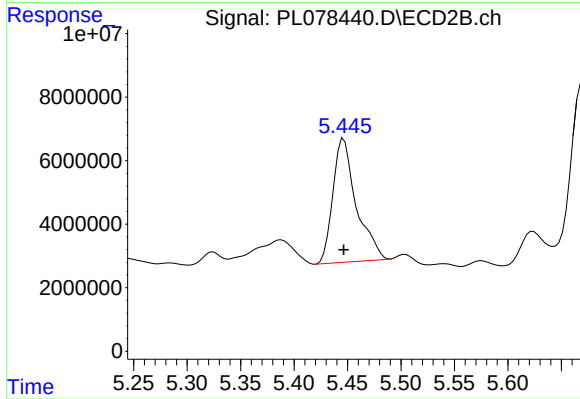

#27 Chlordane-5


R.T.: 5.446 min
Delta R.T.: 0.000 min
Response: 59235932
Conc: 743.63 ng/ml

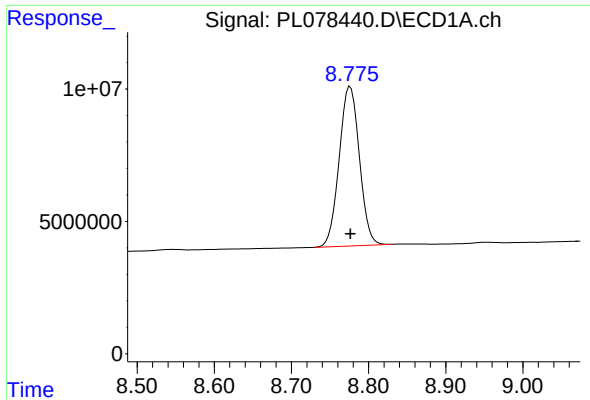

#28 Decachlorobiphenyl

R.T.: 8.776 min
Delta R.T.: 0.000 min
Response: 109348783
Conc: 74.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

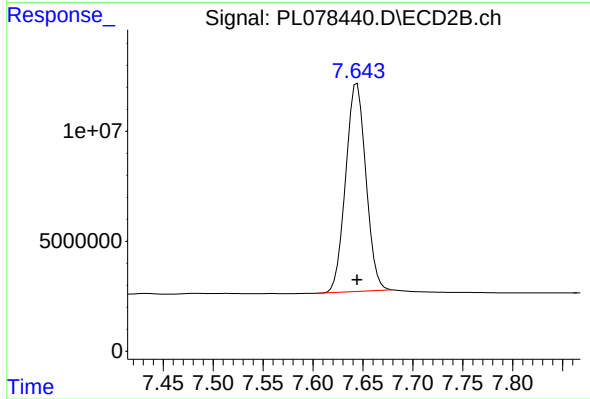

#28 Decachlorobiphenyl

R.T.: 7.644 min
Delta R.T.: 0.000 min
Response: 133337188
Conc: 74.27 ng/ml