

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102124\
 Data File : PL092502.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2024 14:07
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 16:00:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 21 15:58:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.776	250.4E6	329.6E6	96.728	99.974
28)	SA Decachlor...	9.055	7.918	187.9E6	259.2E6	95.992	97.871
Target Compounds							
23)	Chlordane-1	4.701	3.775	125.1E6	115.3E6	950.971	989.514
24)	Chlordane-2	5.231	4.352	117.1E6	128.0E6	886.230	891.198
25)	Chlordane-3	5.941	4.982	441.2E6	382.9E6	952.711	995.396
26)	Chlordane-4	6.022	5.045	526.3E6	377.1E6	949.489	1011.396
27)	Chlordane-5	6.872	5.941	106.6E6	139.5E6	935.128	949.313



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102124\
Data File : PL092502.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2024 14:07
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 16:00:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
Quant Title : GC Extractables
QLast Update : Mon Oct 21 15:58:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

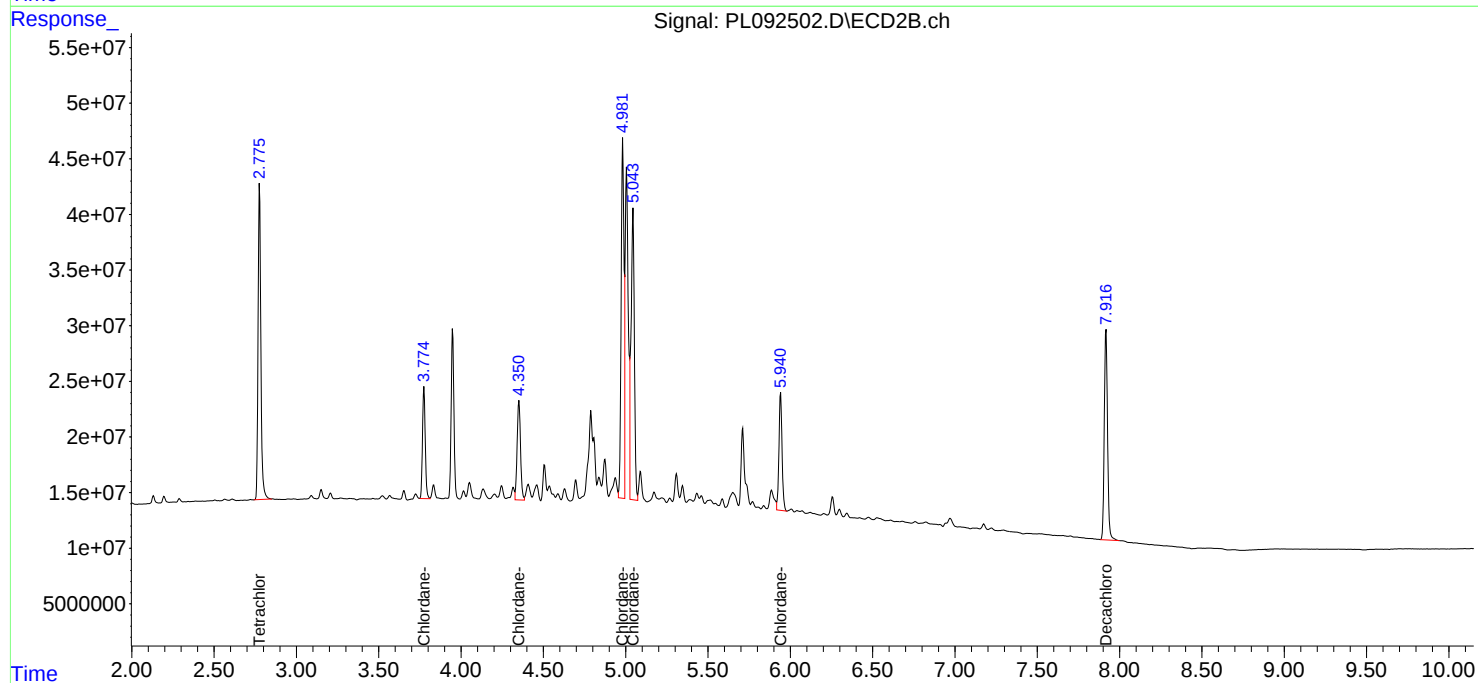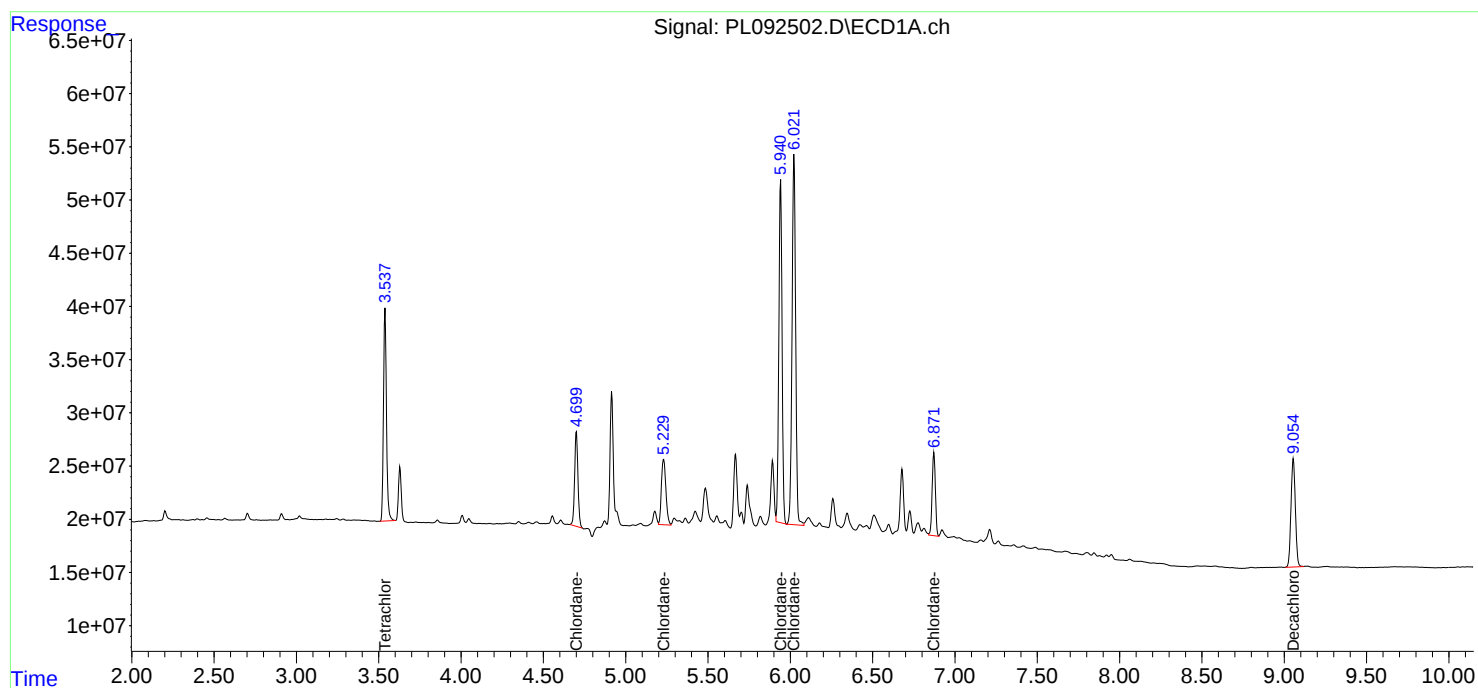


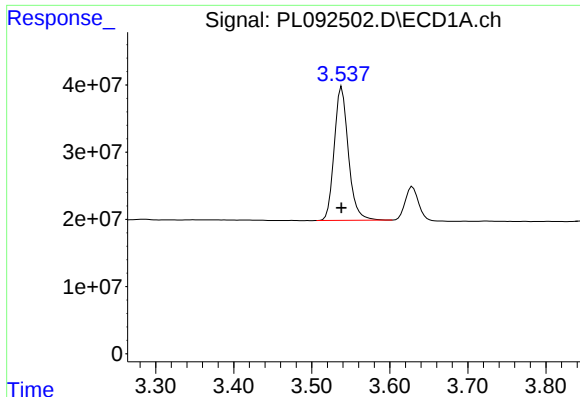

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 250426056
Conc: 96.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

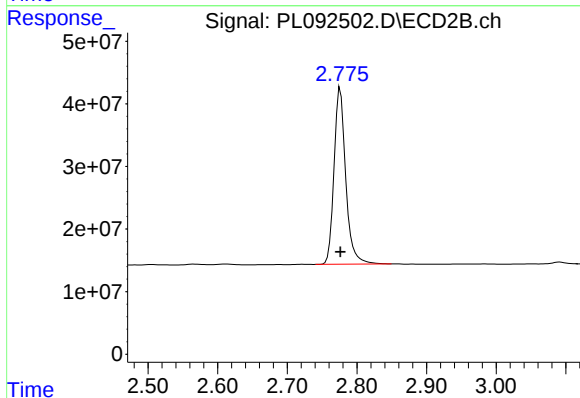


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 329581747
Conc: 99.97 ng/ml

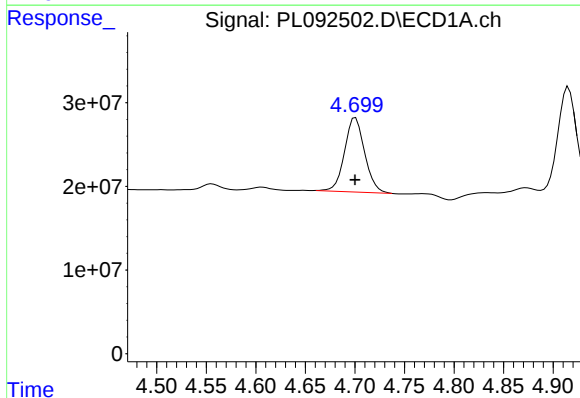


#23 Chlordane-1

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 125122533
Conc: 950.97 ng/ml

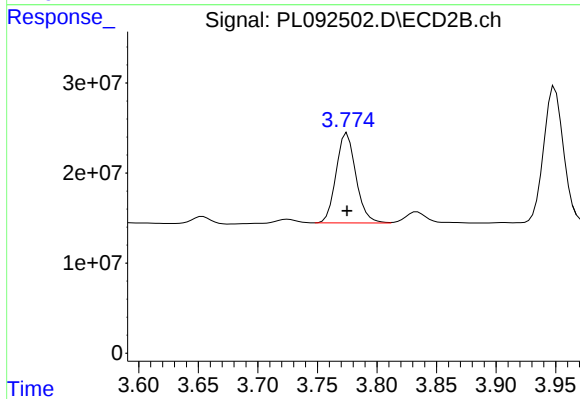

#23 Chlordane-1


R.T.: 3.775 min
Delta R.T.: 0.000 min
Response: 115300553
Conc: 989.51 ng/ml

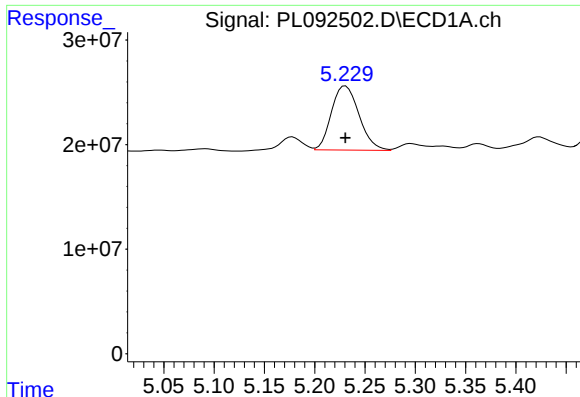

#24 Chlordane-2


R.T.: 5.231 min
Delta R.T.: 0.000 min
Response: 117130289
Conc: 886.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

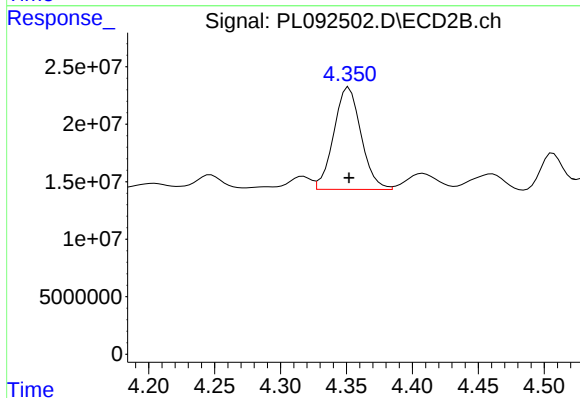


#24 Chlordane-2

R.T.: 4.352 min
Delta R.T.: 0.000 min
Response: 127958347
Conc: 891.20 ng/ml

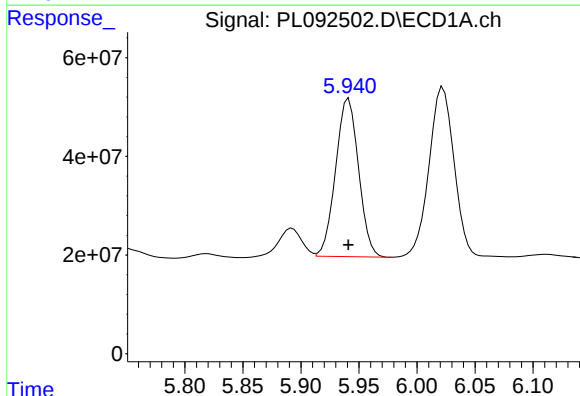


#25 Chlordane-3

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 441184432
Conc: 952.71 ng/ml

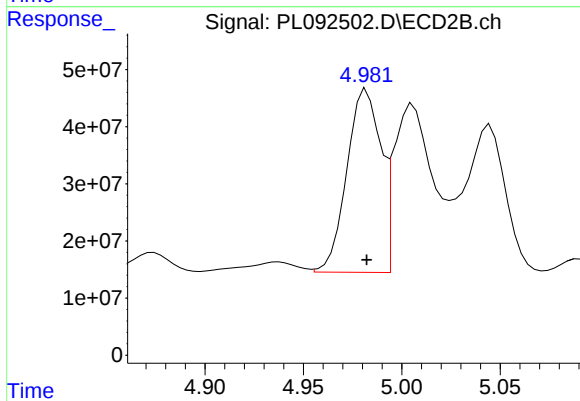

#25 Chlordane-3


R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 382861420
Conc: 995.40 ng/ml

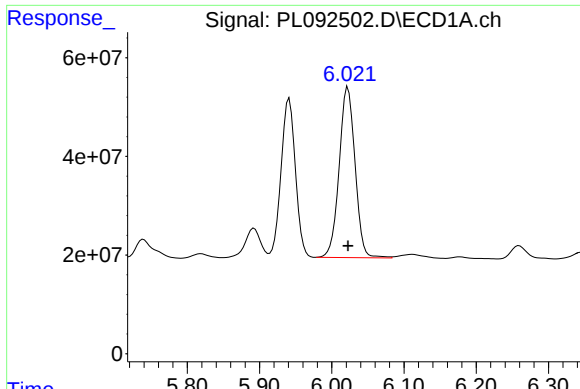

#26 Chlordane-4


R.T.: 6.022 min
Delta R.T.: 0.000 min
Response: 526263121
Conc: 949.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

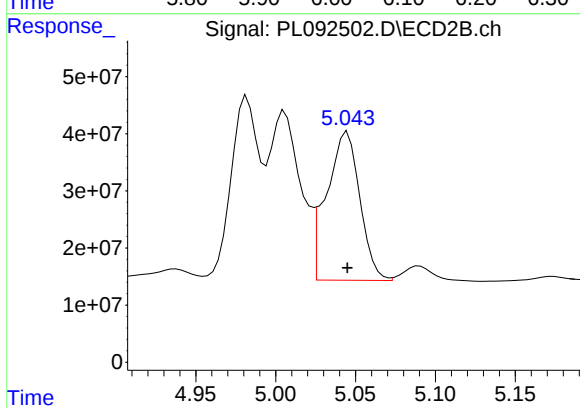


#26 Chlordane-4

R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 377099575
Conc: 1011.40 ng/ml

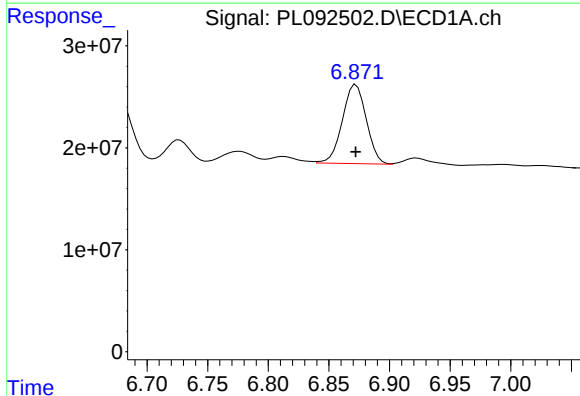


#27 Chlordane-5

R.T.: 6.872 min
Delta R.T.: 0.000 min
Response: 106551811
Conc: 935.13 ng/ml

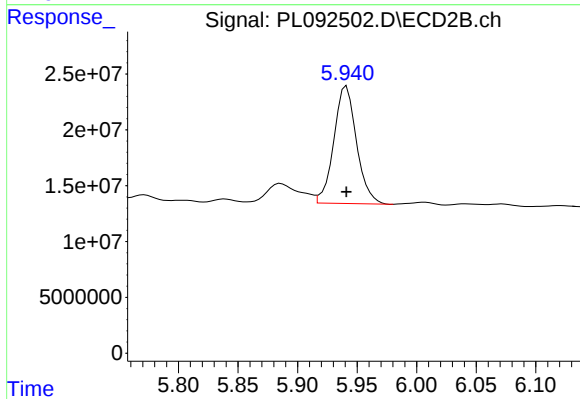

#27 Chlordane-5


R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 139513128
Conc: 949.31 ng/ml

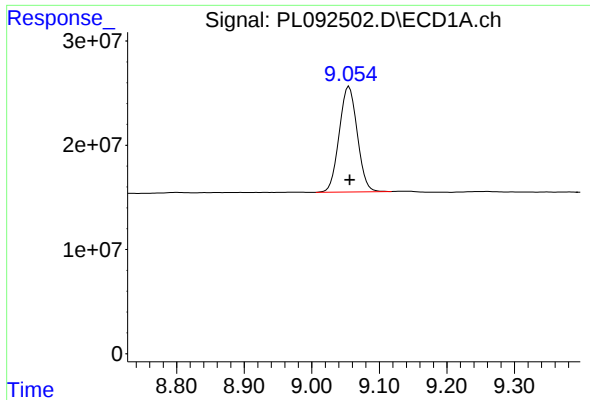

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: -0.001 min
Response: 187947173
Conc: 95.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

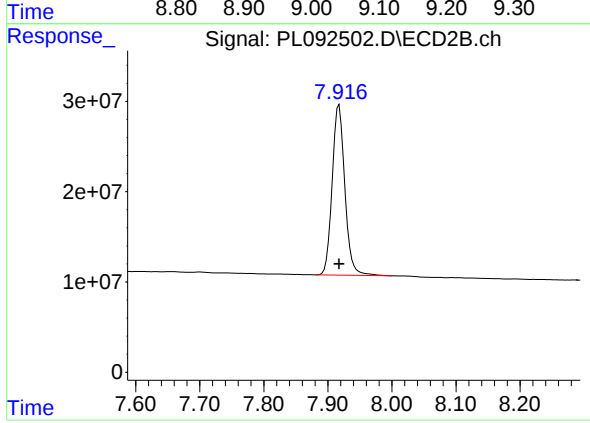

#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: 0.000 min
Response: 259160809
Conc: 97.87 ng/ml