

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102124\
 Data File : PL092503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2024 14:20
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 16:04:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 21 16:04:37 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.776	189.6E6	246.9E6	74.640	74.936
28)	SA Decachlor...	9.056	7.917	142.6E6	195.6E6	74.560	74.781
Target Compounds							
23)	Chlordane-1	4.701	3.775	94578470	86066685	741.209	744.997
24)	Chlordane-2	5.231	4.352	88509890	96706683	722.903	724.429
25)	Chlordane-3	5.941	4.982	336.0E6	287.4E6	745.459	749.299
26)	Chlordane-4	6.023	5.045	401.3E6	280.5E6	745.131	748.743
27)	Chlordane-5	6.873	5.941	81780426	104.5E6	744.505	736.367



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102124\
Data File : PL092503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2024 14:20
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 16:04:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
Quant Title : GC Extractables
QLast Update : Mon Oct 21 16:04:37 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

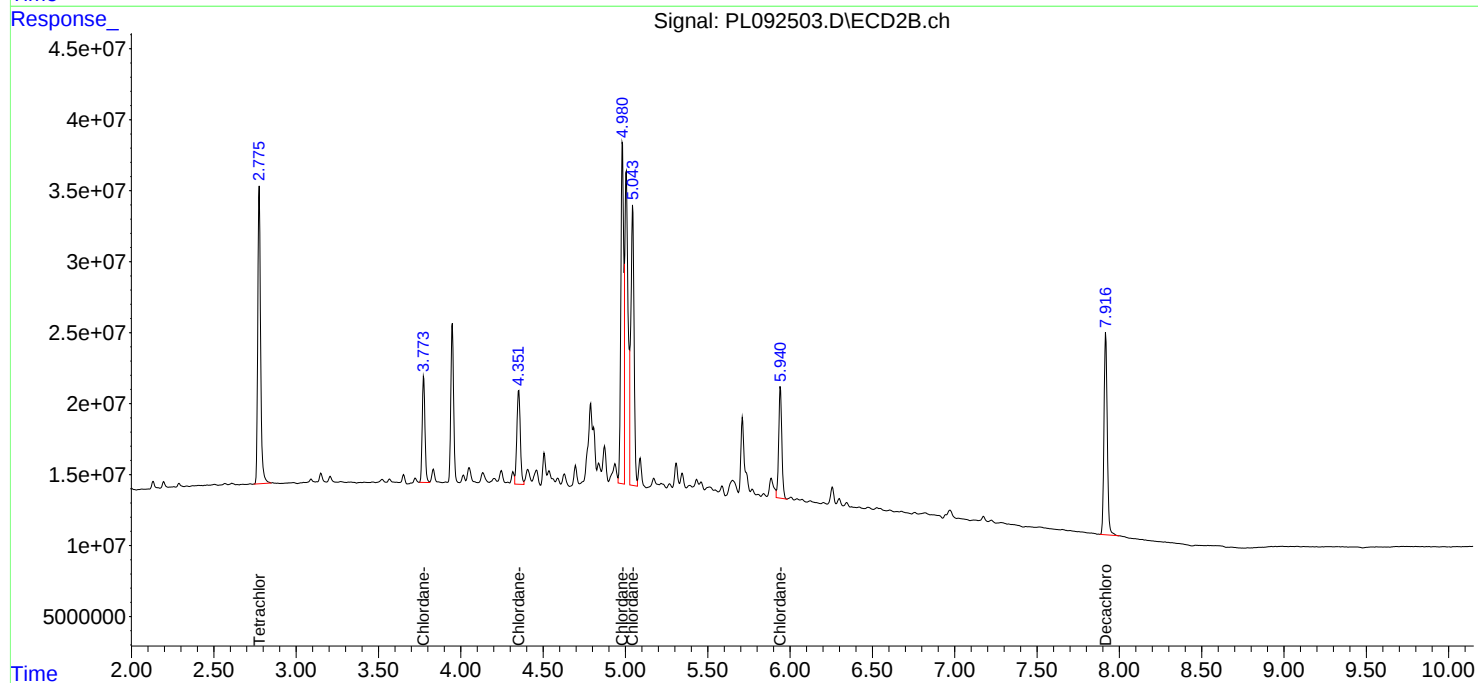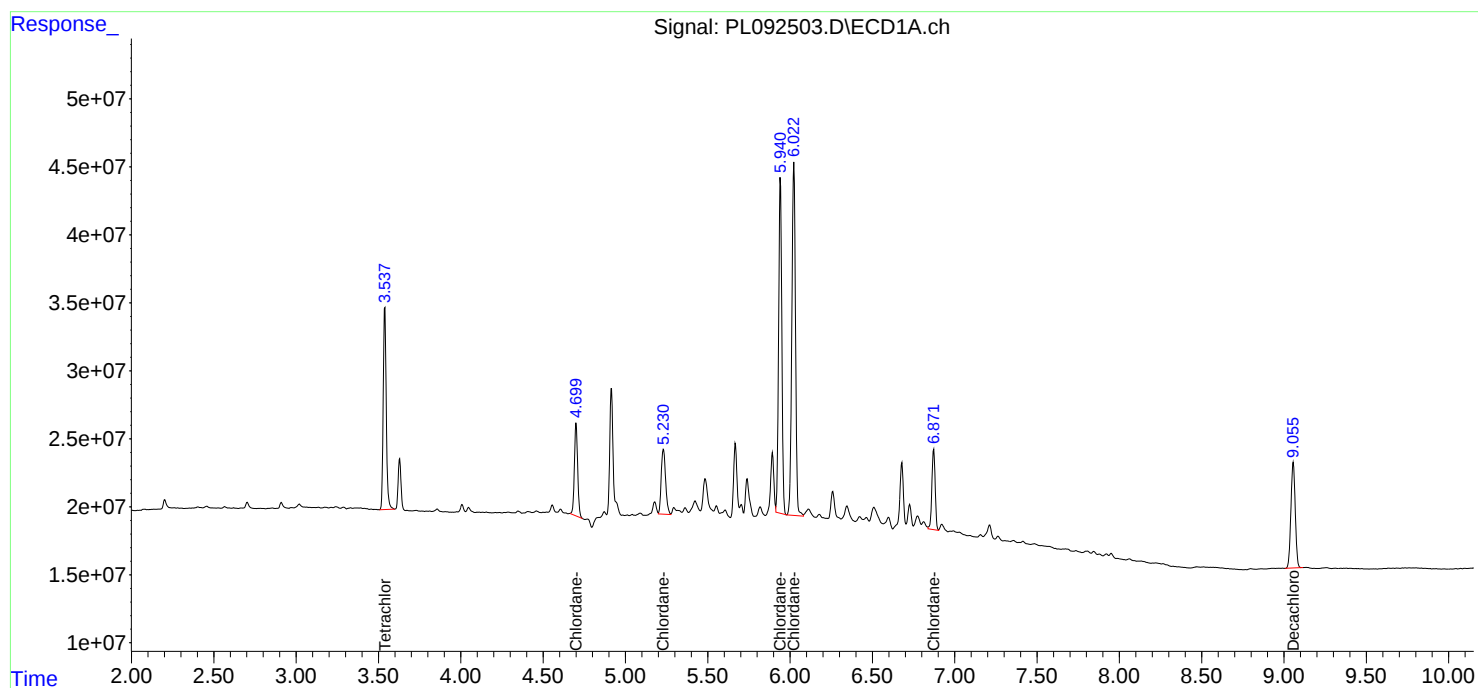


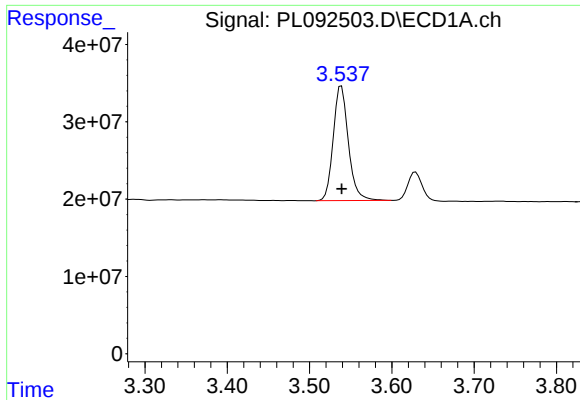

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 189623675
Conc: 74.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

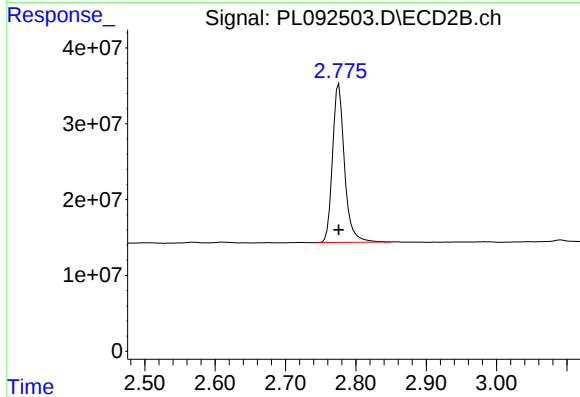


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 246904350
Conc: 74.94 ng/ml

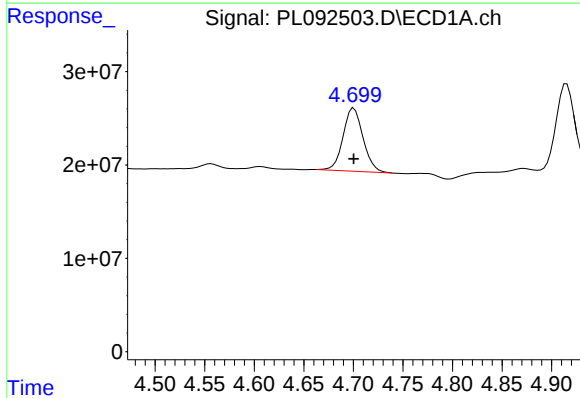


#23 Chlordane-1

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 94578470
Conc: 741.21 ng/ml

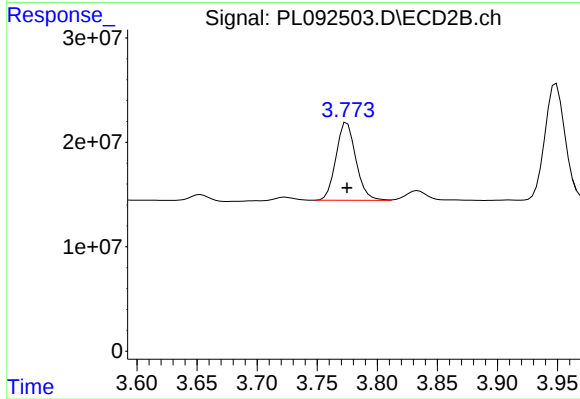

#23 Chlordane-1


R.T.: 3.775 min
Delta R.T.: 0.000 min
Response: 86066685
Conc: 745.00 ng/ml

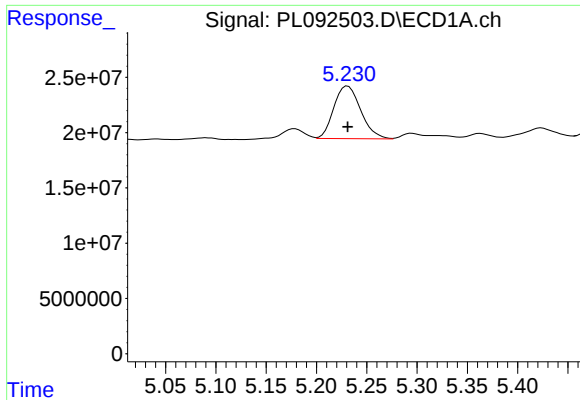

#24 Chlordane-2


R.T.: 5.231 min
Delta R.T.: 0.000 min
Response: 88509890
Conc: 722.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

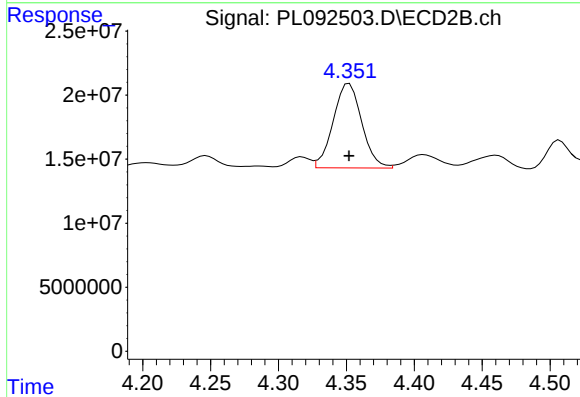


#24 Chlordane-2

R.T.: 4.352 min
Delta R.T.: 0.000 min
Response: 96706683
Conc: 724.43 ng/ml

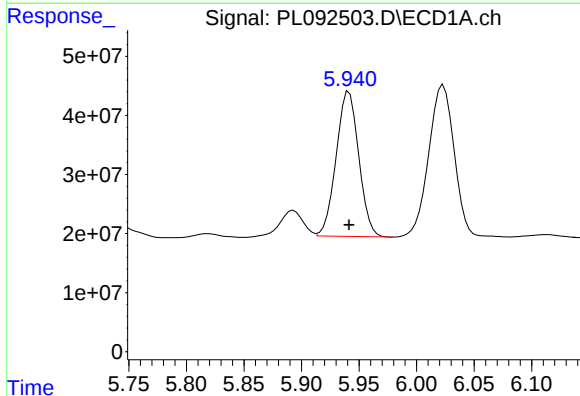


#25 Chlordane-3

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 336029869
Conc: 745.46 ng/ml

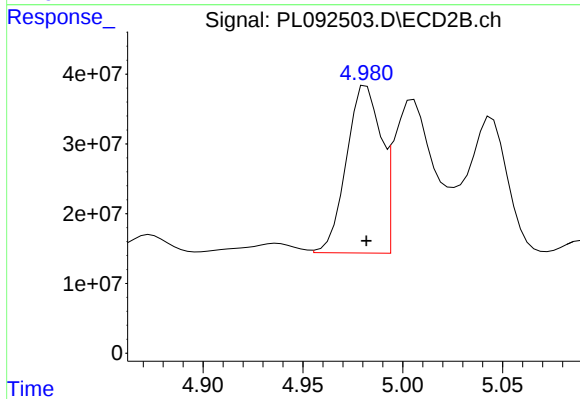

#25 Chlordane-3


R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 287406978
Conc: 749.30 ng/ml

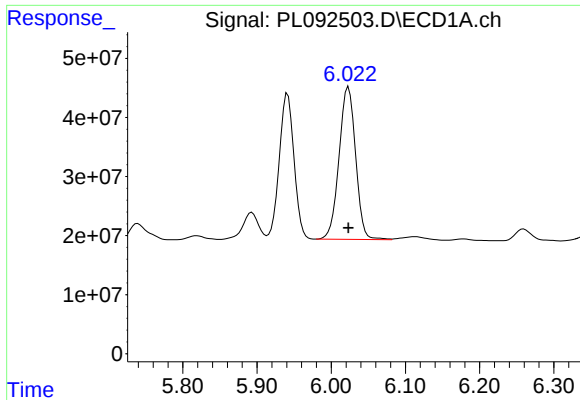

#26 Chlordane-4


R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 401262852
Conc: 745.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

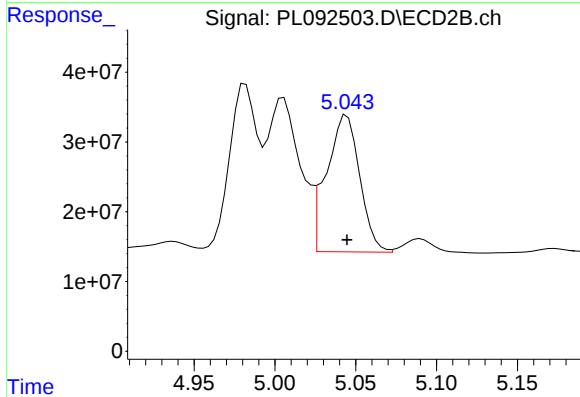


#26 Chlordane-4

R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 280524796
Conc: 748.74 ng/ml

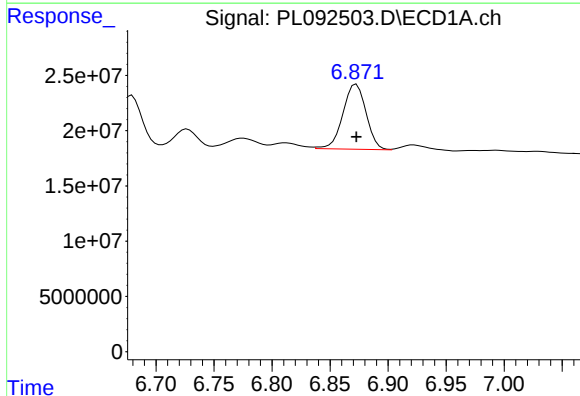


#27 Chlordane-5

R.T.: 6.873 min
Delta R.T.: 0.000 min
Response: 81780426
Conc: 744.51 ng/ml

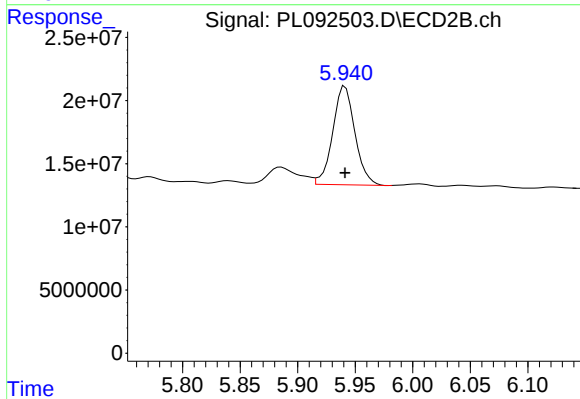

#27 Chlordane-5


R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 104525594
Conc: 736.37 ng/ml

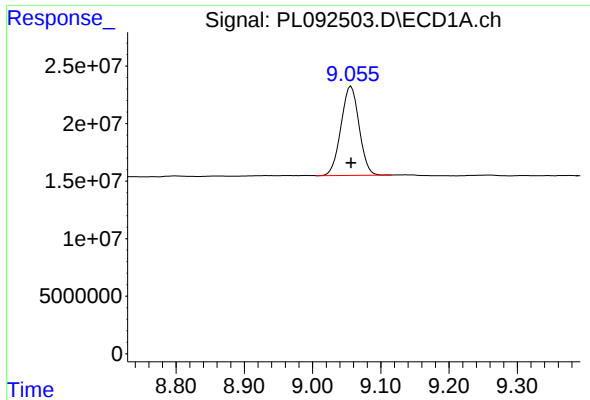

#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.000 min
Response: 142641293
Conc: 74.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

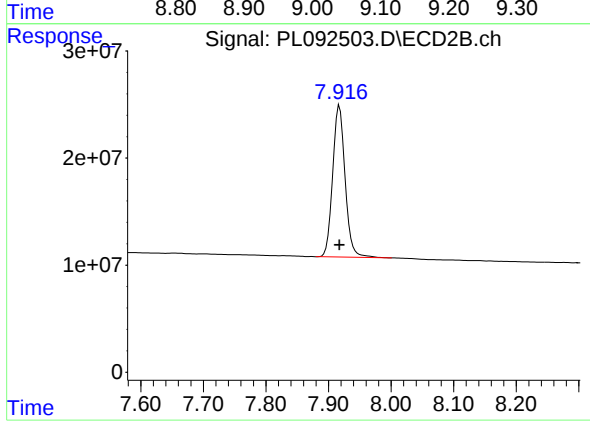

#28 Decachlorobiphenyl

R.T.: 7.917 min
Delta R.T.: 0.000 min
Response: 195625220
Conc: 74.78 ng/ml