

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102124\
 Data File : PL092504.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2024 14:33
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 15:59:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 21 15:58:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.776	129.4E6	164.8E6	50.000	50.000
28)	SA Decachlor...	9.056	7.918	97897038	132.4E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.700	3.775	65786710	58261206	500.000	500.000
24)	Chlordane-2	5.231	4.352	66083445	71790067	500.000	500.000
25)	Chlordane-3	5.941	4.982	231.5E6	192.3E6	500.000	500.000
26)	Chlordane-4	6.023	5.045	277.1E6	186.4E6	500.000	500.000
27)	Chlordane-5	6.872	5.941	56971777	73481136	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102124\
Data File : PL092504.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2024 14:33
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 15:59:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
Quant Title : GC Extractables
QLast Update : Mon Oct 21 15:58:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

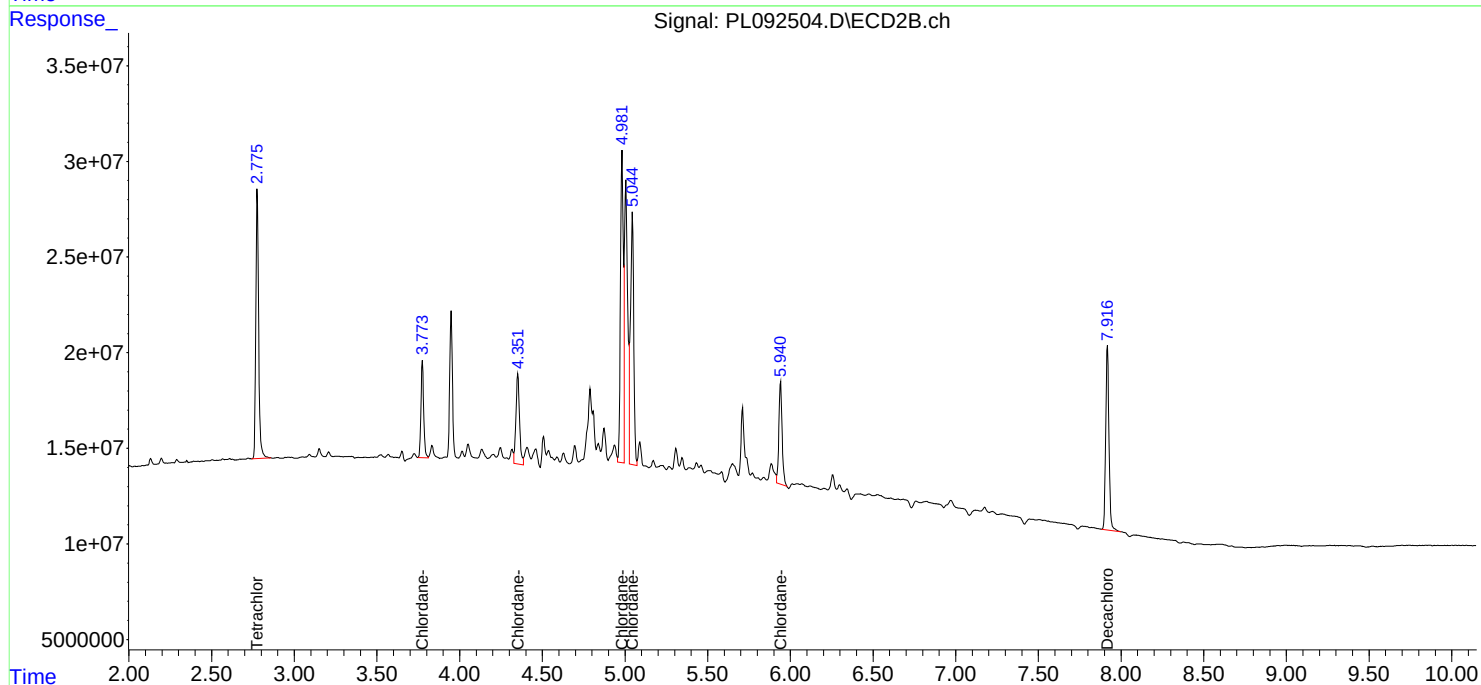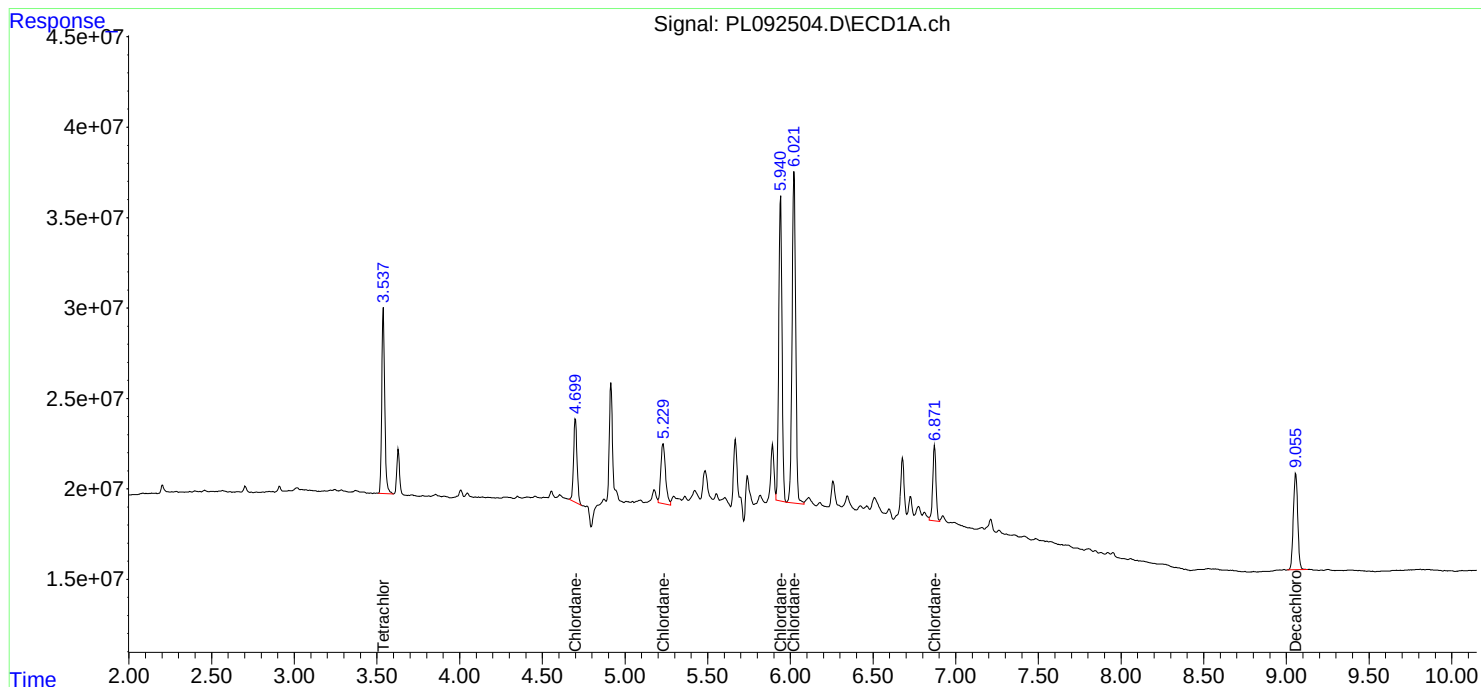


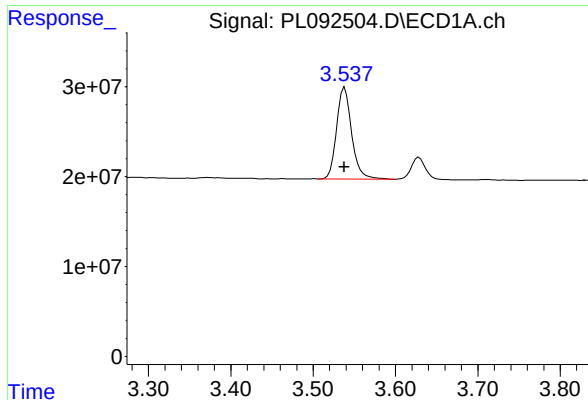

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 129448927
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

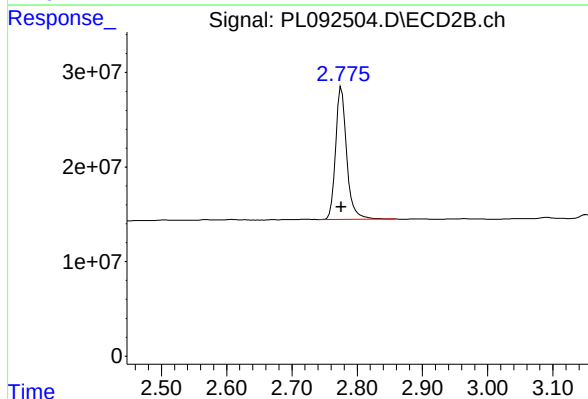


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 164833808
Conc: 50.00 ng/ml

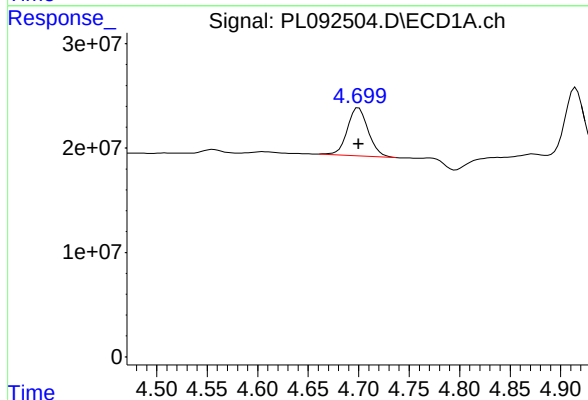


#23 Chlordane-1

R.T.: 4.700 min
Delta R.T.: 0.000 min
Response: 65786710
Conc: 500.00 ng/ml

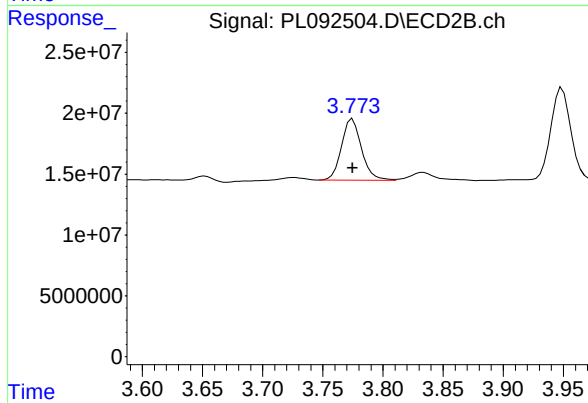

#23 Chlordane-1


R.T.: 3.775 min
Delta R.T.: 0.000 min
Response: 58261206
Conc: 500.00 ng/ml

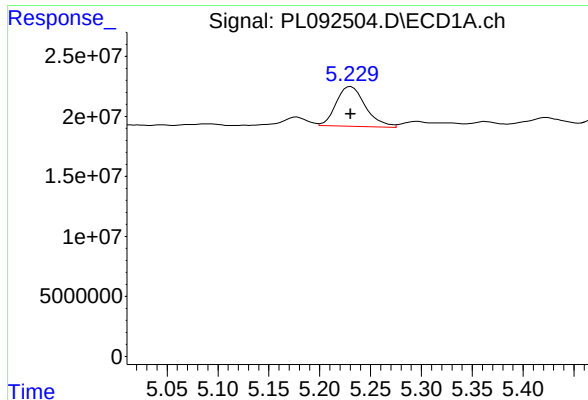

#24 Chlordane-2


R.T.: 5.231 min
Delta R.T.: 0.000 min
Response: 66083445
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

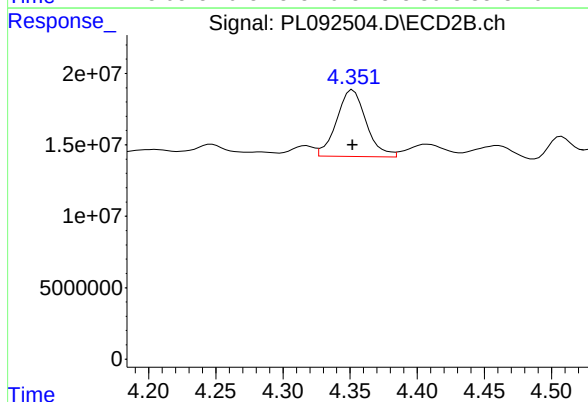


#24 Chlordane-2

R.T.: 4.352 min
Delta R.T.: 0.000 min
Response: 71790067
Conc: 500.00 ng/ml

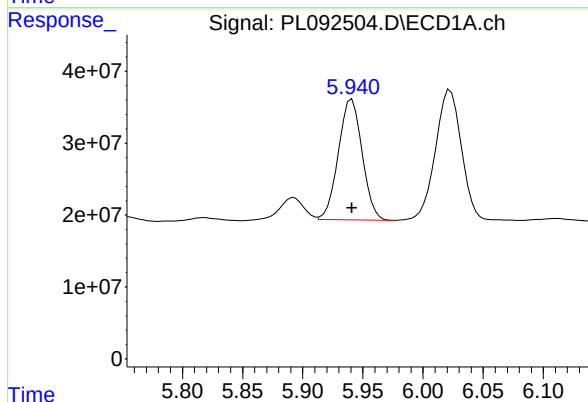


#25 Chlordane-3

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 231541583
Conc: 500.00 ng/ml

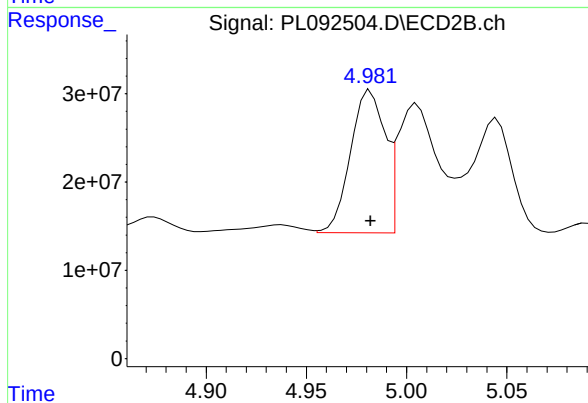

#25 Chlordane-3


R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 192316183
Conc: 500.00 ng/ml

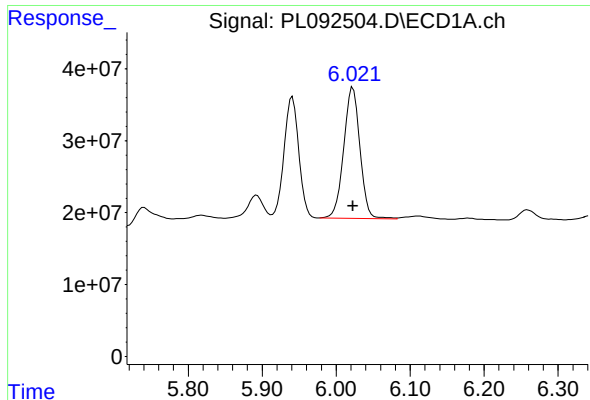

#26 Chlordane-4


R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 277129769
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

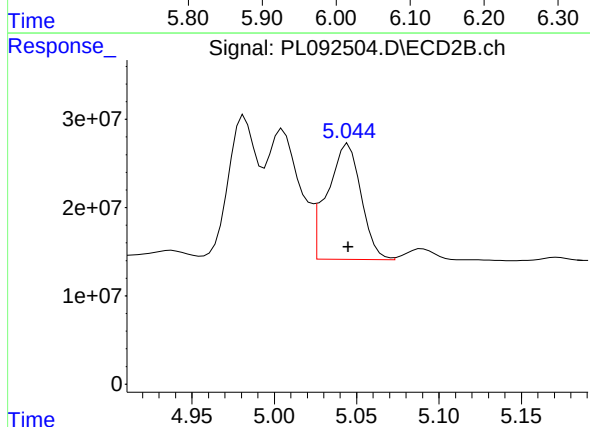


#26 Chlordane-4

R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 186425212
Conc: 500.00 ng/ml

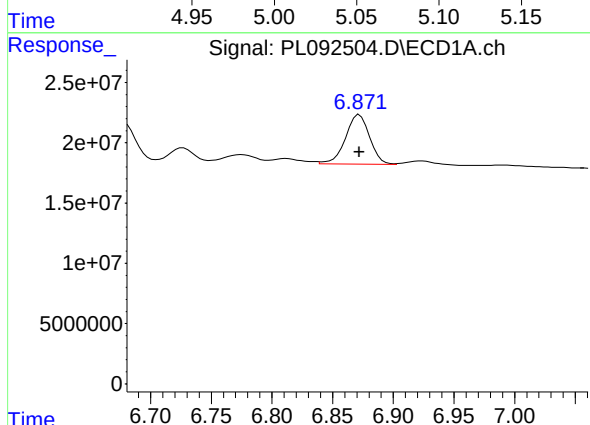


#27 Chlordane-5

R.T.: 6.872 min
Delta R.T.: 0.000 min
Response: 56971777
Conc: 500.00 ng/ml

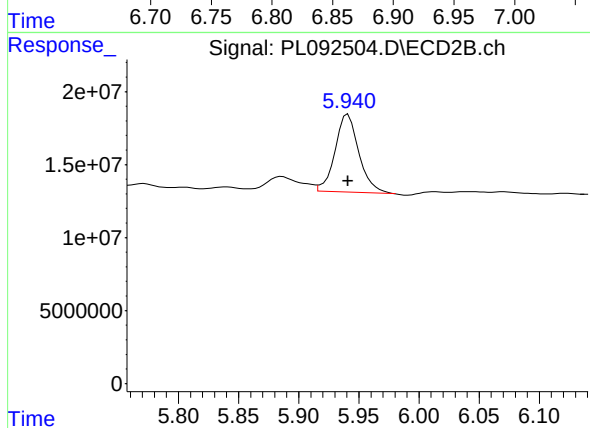

#27 Chlordane-5


R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 73481136
Conc: 500.00 ng/ml

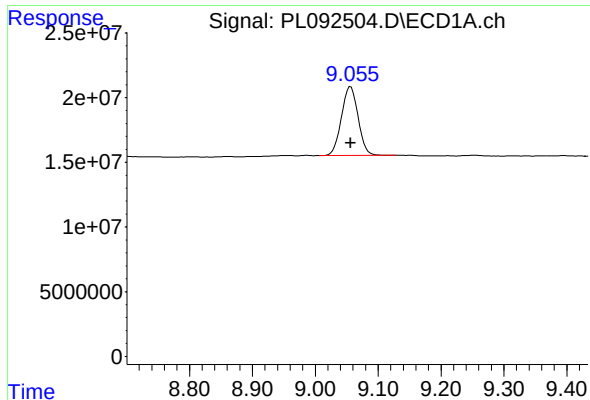

#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.000 min
Response: 97897038
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

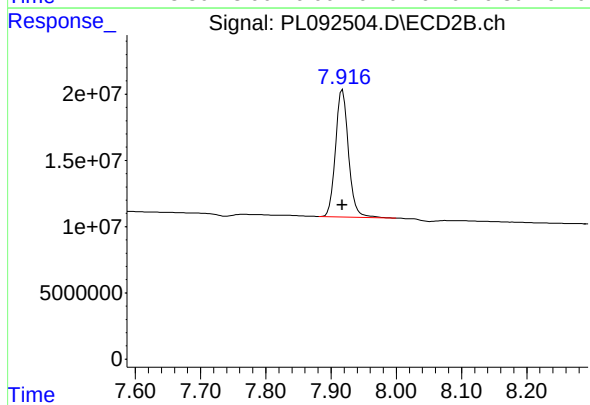

#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: 0.000 min
Response: 132398681
Conc: 50.00 ng/ml