

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102124\
 Data File : PL092520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2024 19:48
 Operator : AR\AJ
 Sample : P4455-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SU-4-101824

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/22/2024
 Supervised By :Ankita Jodhani 10/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:46:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 21 17:09:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.539	2.776	28958806	33202496	10.750	11.954m
28) SA Decachlor...	9.054	7.917	21245397	29656969	10.460m	11.255

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102124\
Data File : PL092520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2024 19:48
Operator : AR\AJ
Sample : P4455-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SU-4-101824


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/22/2024
Supervised By : Ankita Jodhani 10/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:46:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
Quant Title : GC Extractables
QLast Update : Mon Oct 21 17:09:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

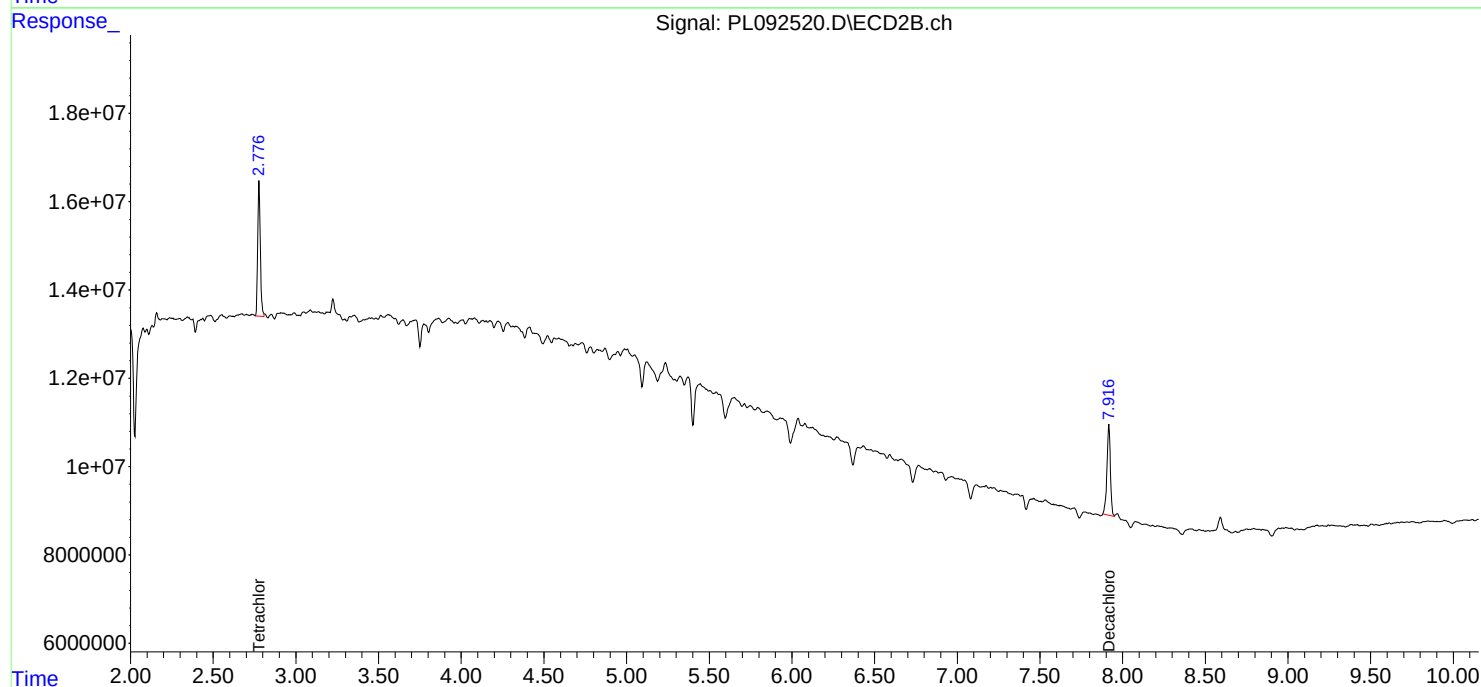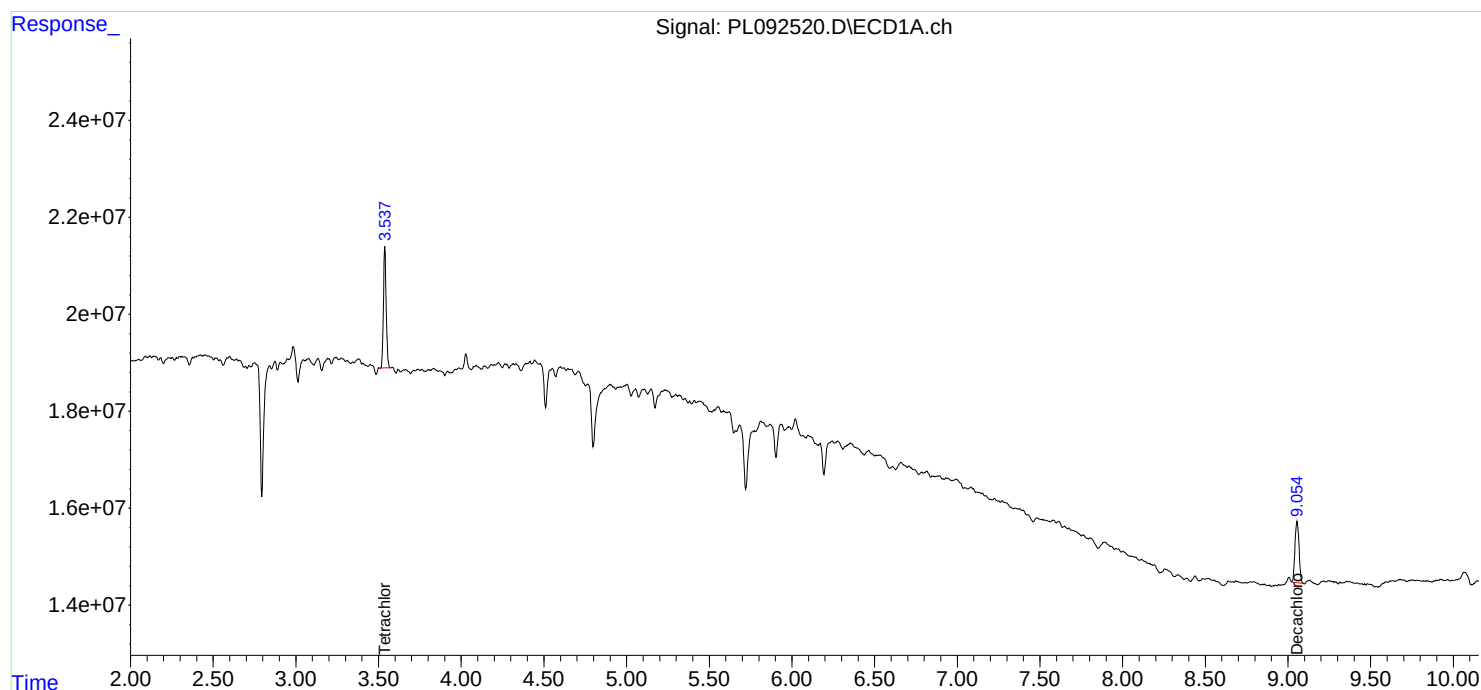

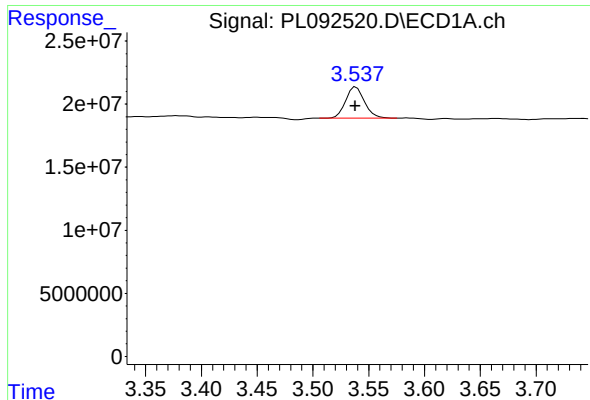


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 28958806
Conc: 10.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-4-101824


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/22/2024
Supervised By :Ankita Jodhani 10/22/2024

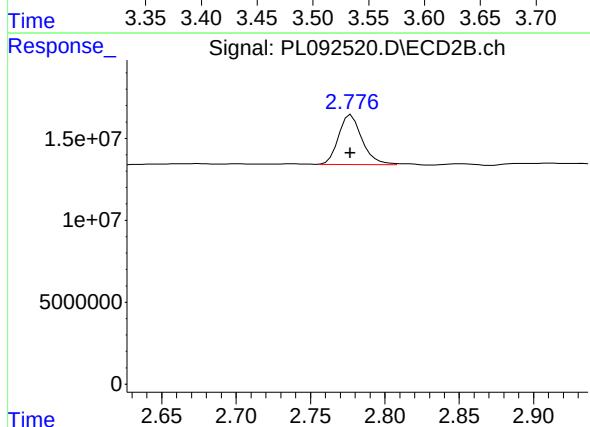


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 33202496
Conc: 11.95 ng/ml m

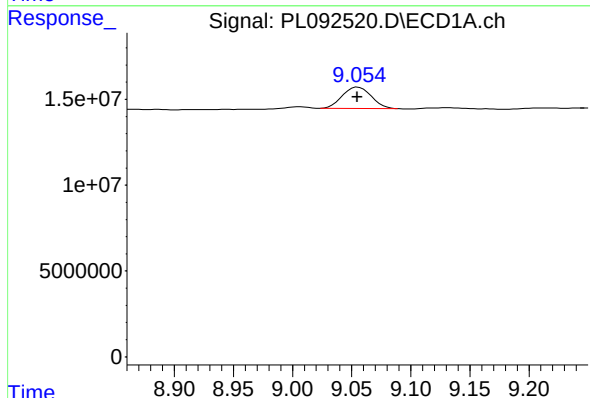

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: -0.001 min
Response: 21245397
Conc: 10.46 ng/ml m

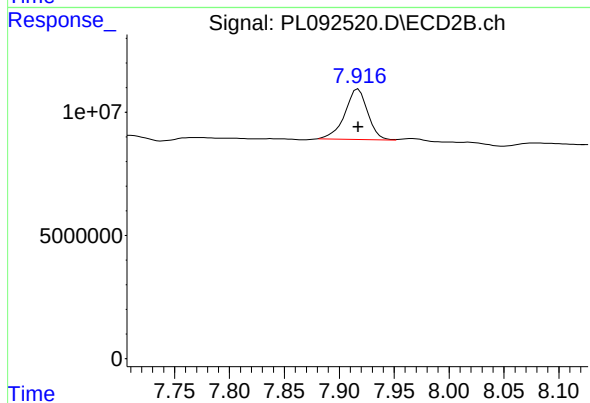

#28 Decachlorobiphenyl

R.T.: 7.917 min
Delta R.T.: 0.000 min
Response: 29656969
Conc: 11.26 ng/ml