

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102218\
 Data File : PL041220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2018 12:44
 Operator : AJ\SJ
 Sample : J5577-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 01:10:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.102	56183792	29836907	10.251	10.701
28)	SA Decachlor...	8.222	9.232	79329745	32631242	15.257	12.619
Target Compounds							
2)	A alpha-BHC	3.910	0.000	3322026	0	0.419	N.D. #
6)	B beta-BHC	0.000	4.996f	0	1988542	N.D.	1.241 #
9)	A Endosulfan I	5.471f	6.309f	2046450	1379750	0.342	0.539 #
10)	B gamma-Chl...	5.434	0.000	3712894	0	0.565	N.D. #
11)	B alpha-Chl...	5.471	6.309	2046450	1379750	0.315	0.497 #
12)	B 4,4'-DDE	5.638	6.461	6215224	3277867	1.093	1.239
16)	A 4,4'-DDD	6.232f	0.000	3012050	0	0.667	N.D. #
17)	MA 4,4'-DDT	6.391	0.000	1494318	0	0.328	N.D. #
24)	Chlordane-2	4.852	0.000	1426015	0	5.284	N.D. #
25)	Chlordane-3	5.434	0.000	3712894	0	4.851	N.D. #
26)	Chlordane-4	5.471	6.309	2046450	1379750	3.052	2.907


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102218\
Data File : PL041220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2018 12:44
Operator : AJ\SJ
Sample : J5577-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 01:10:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

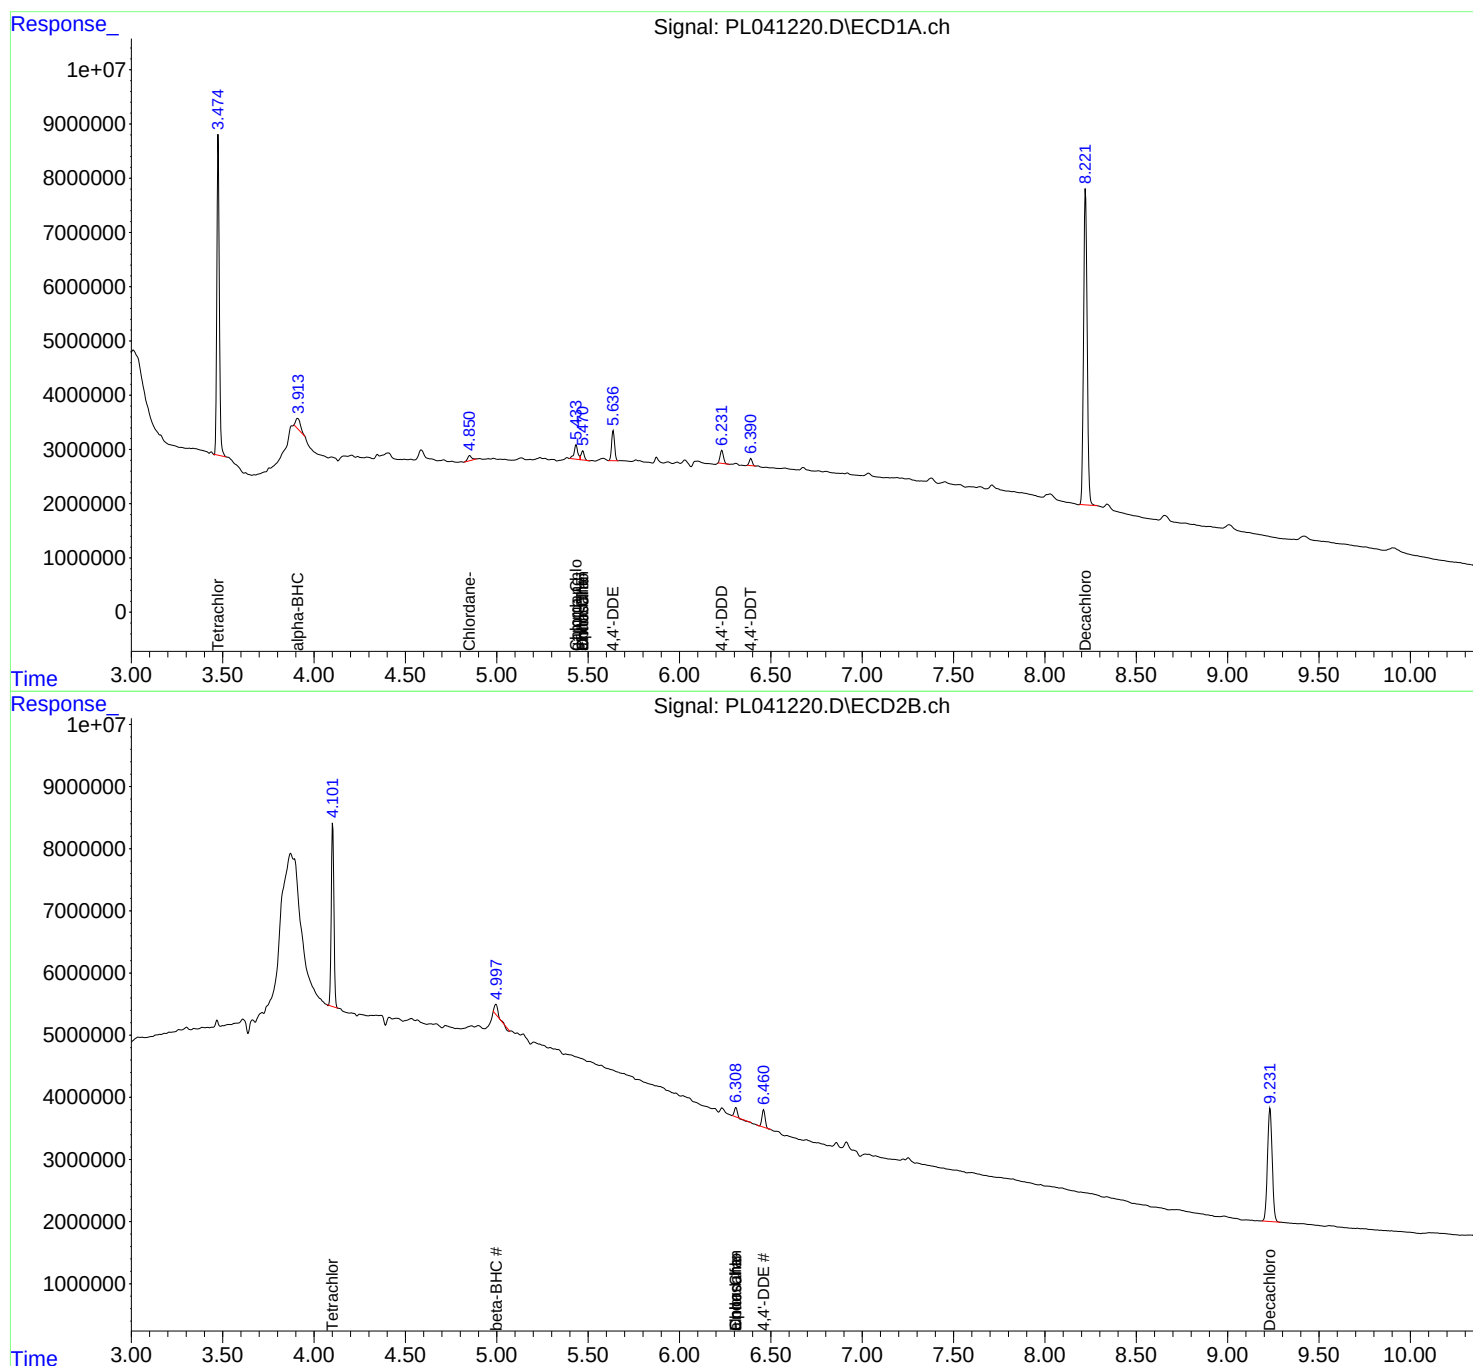


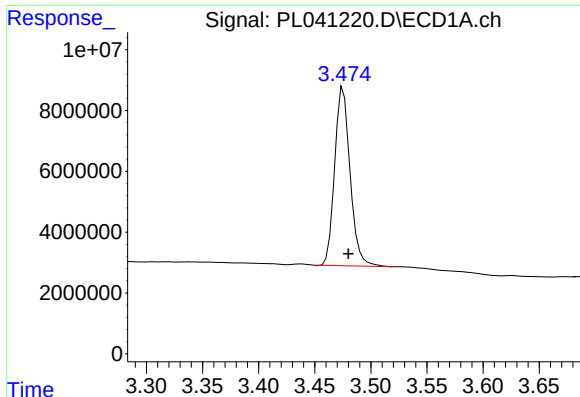

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: -0.004 min
Response: 56183792
Conc: 10.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

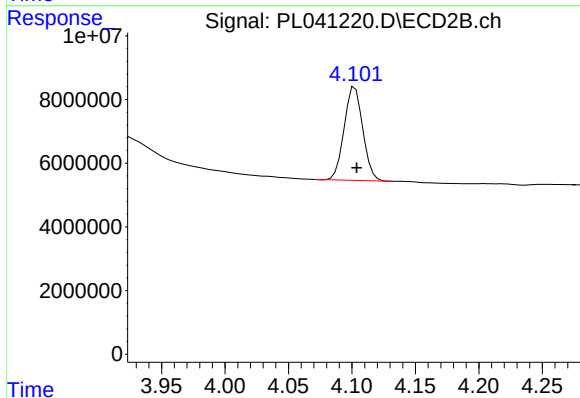


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: -0.001 min
Response: 29836907
Conc: 10.70 ng/ml

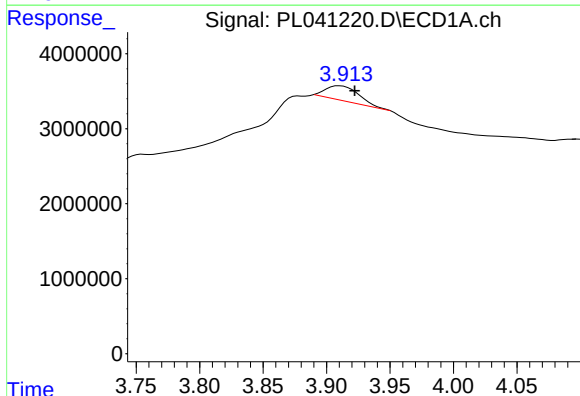


#2 alpha-BHC

R.T.: 3.910 min
Delta R.T.: -0.012 min
Response: 3322026
Conc: 0.42 ng/ml

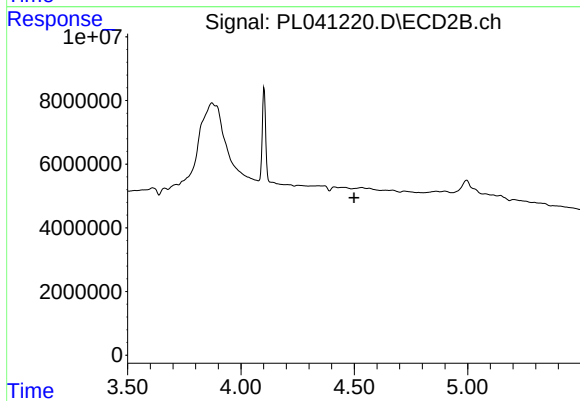

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.499 min
Response: 0
Conc: N.D.

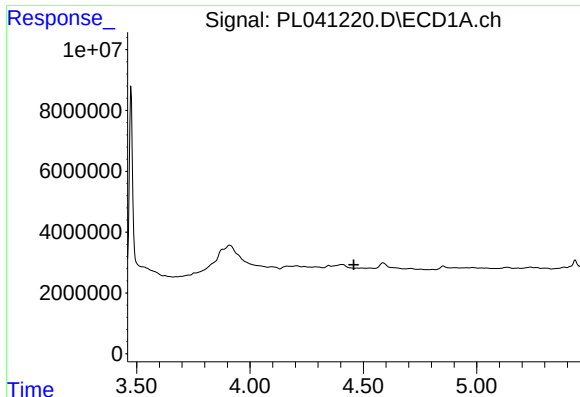

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

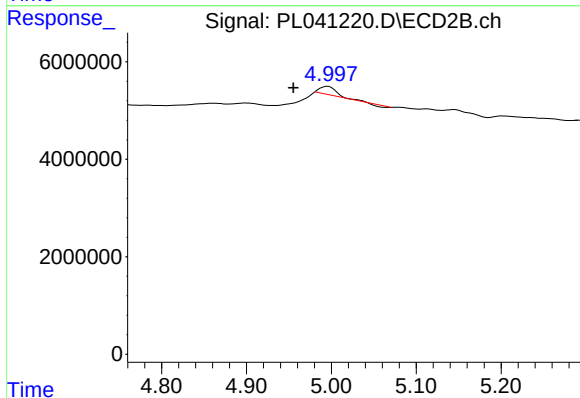


#6 beta-BHC

R.T.: 4.996 min
Delta R.T.: 0.041 min
Response: 1988542
Conc: 1.24 ng/ml

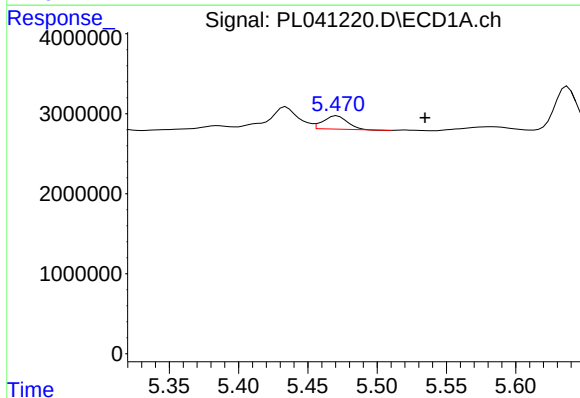


#9 Endosulfan I

R.T.: 5.471 min
Delta R.T.: -0.063 min
Response: 2046450
Conc: 0.34 ng/ml

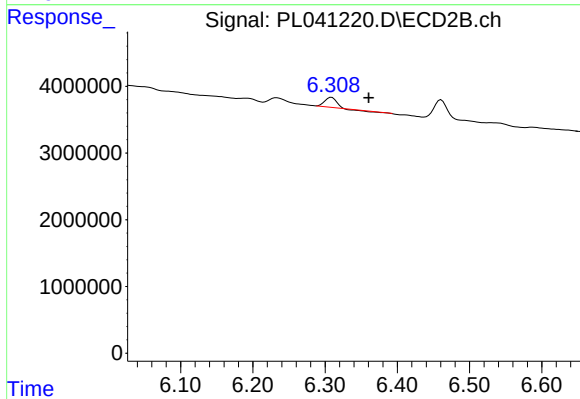

#9 Endosulfan I


R.T.: 6.309 min
Delta R.T.: -0.051 min
Response: 1379750
Conc: 0.54 ng/ml

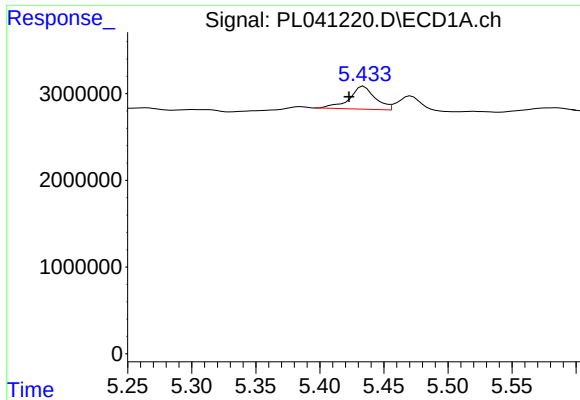

#10 gamma-Chlordane


R.T.: 5.434 min
Delta R.T.: 0.012 min
Response: 3712894
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

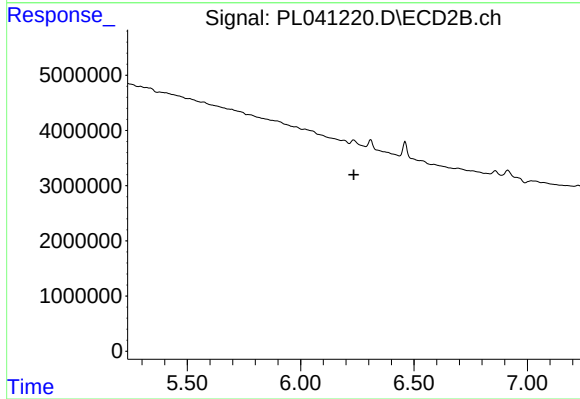


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.235 min
Response: 0
Conc: N.D.

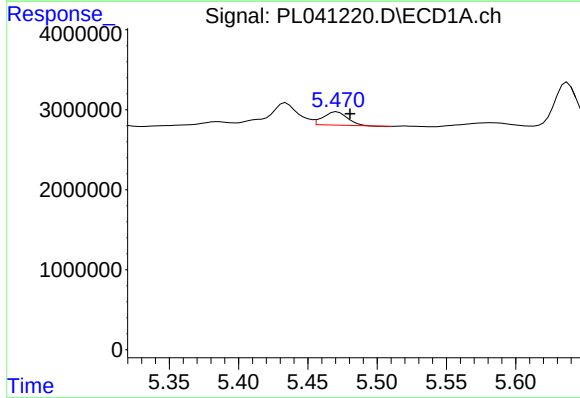


#11 alpha-Chlordane

R.T.: 5.471 min
Delta R.T.: -0.009 min
Response: 2046450
Conc: 0.31 ng/ml

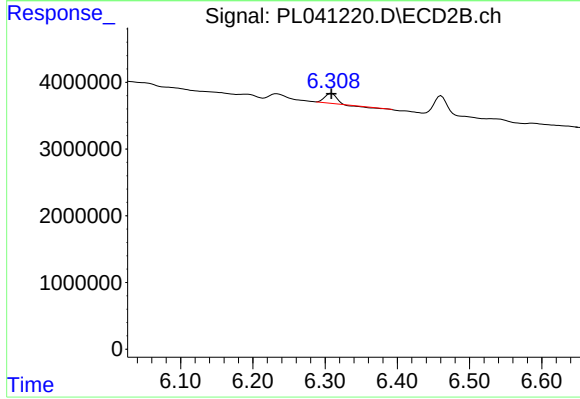

#11 alpha-Chlordane


R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 1379750
Conc: 0.50 ng/ml

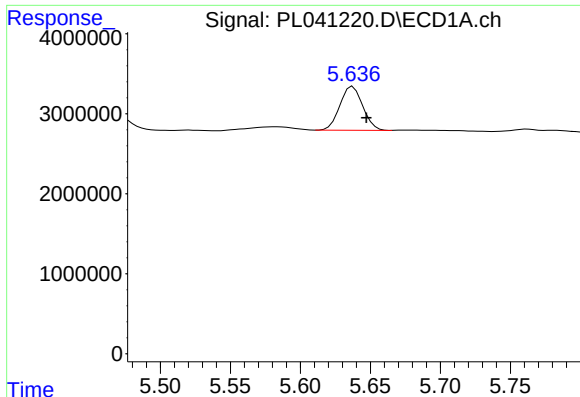

#12 4,4'-DDE


R.T.: 5.638 min
Delta R.T.: -0.010 min
Response: 6215224
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

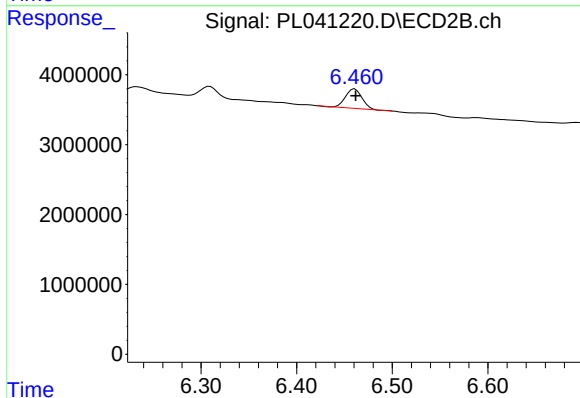


#12 4,4'-DDE

R.T.: 6.461 min
Delta R.T.: -0.001 min
Response: 3277867
Conc: 1.24 ng/ml

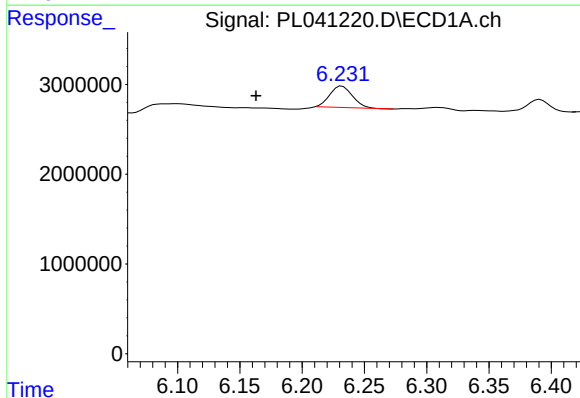


#16 4,4'-DDD

R.T.: 6.232 min
Delta R.T.: 0.069 min
Response: 3012050
Conc: 0.67 ng/ml

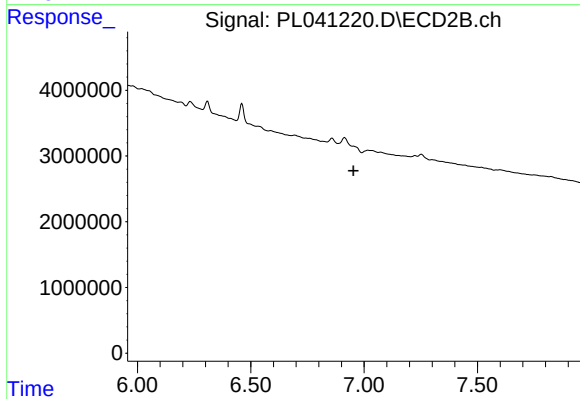

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.954 min
Response: 0
Conc: N.D.

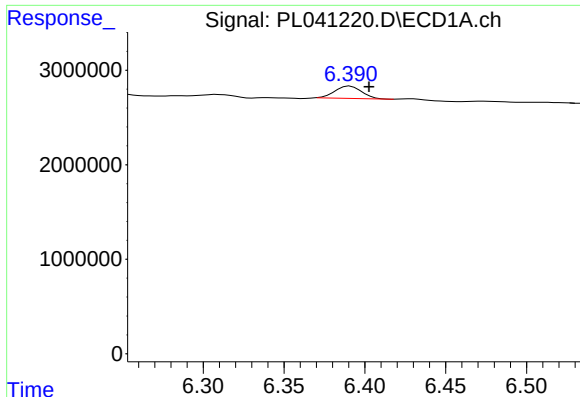

#17 4,4'-DDT


R.T.: 6.391 min
Delta R.T.: -0.012 min
Response: 1494318
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

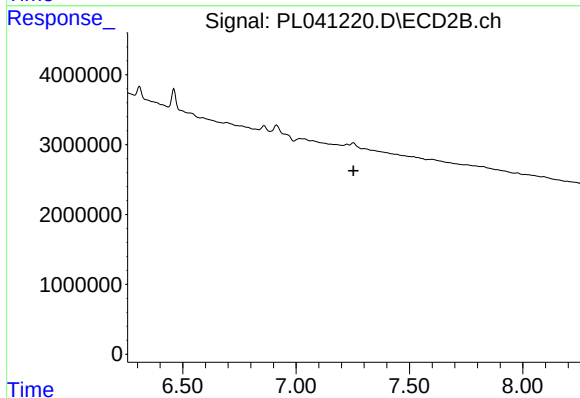


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.254 min
Response: 0
Conc: N.D.

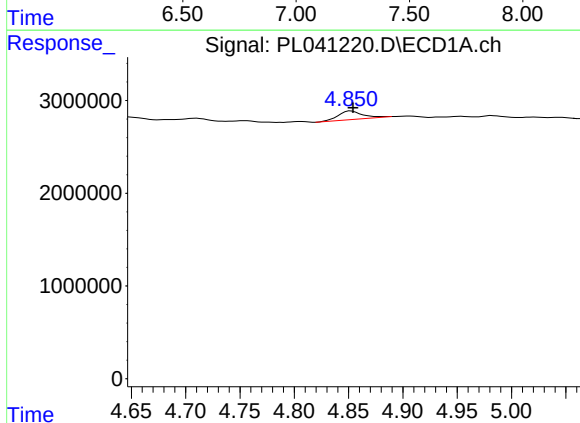


#24 Chlordane-2

R.T.: 4.852 min
Delta R.T.: -0.002 min
Response: 1426015
Conc: 5.28 ng/ml

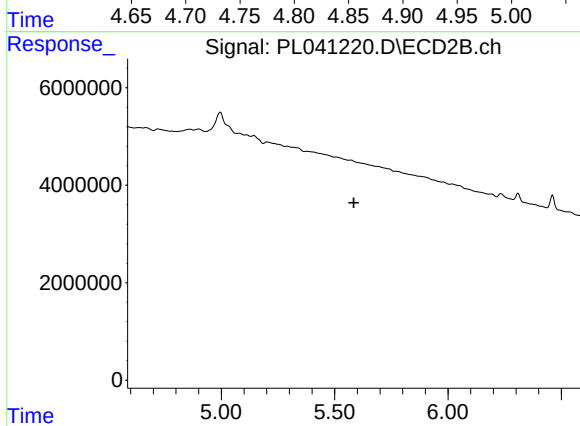

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.584 min
Response: 0
Conc: N.D.

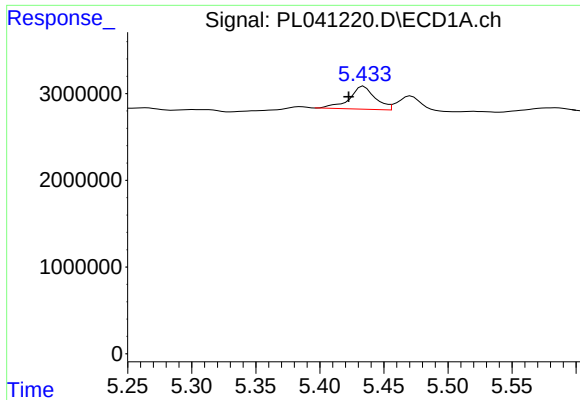

#25 Chlordane-3


R.T.: 5.434 min
Delta R.T.: 0.012 min
Response: 3712894
Conc: 4.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

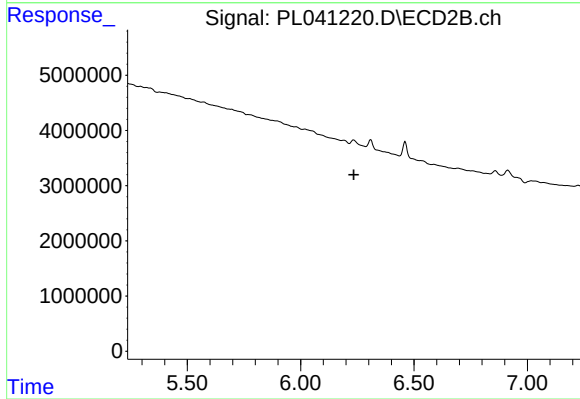


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.235 min
Response: 0
Conc: N.D.

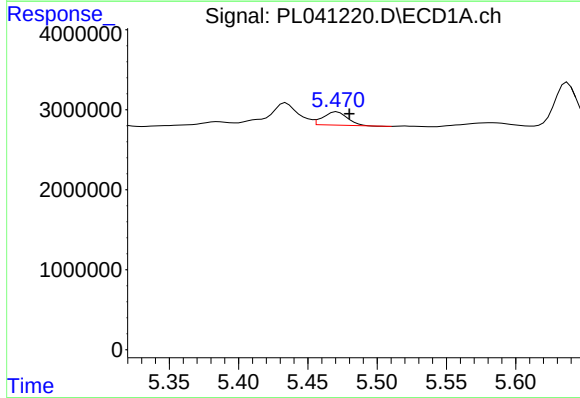


#26 Chlordane-4

R.T.: 5.471 min
Delta R.T.: -0.009 min
Response: 2046450
Conc: 3.05 ng/ml

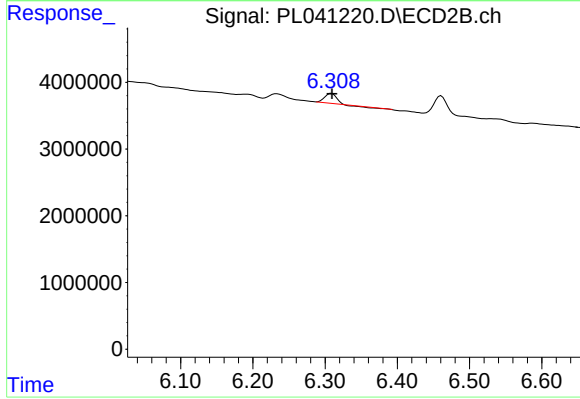

#26 Chlordane-4


R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 1379750
Conc: 2.91 ng/ml

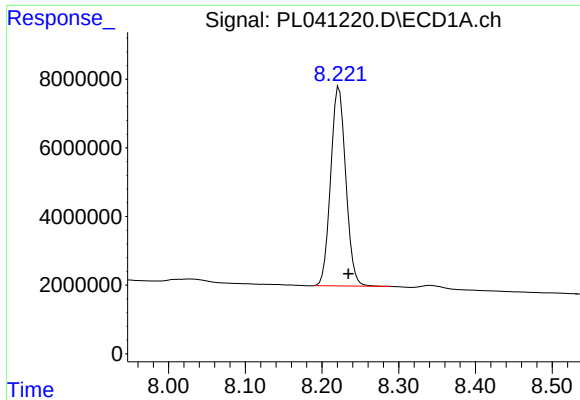

#28 Decachlorobiphenyl

R.T.: 8.222 min
Delta R.T.: -0.012 min
Response: 79329745
Conc: 15.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

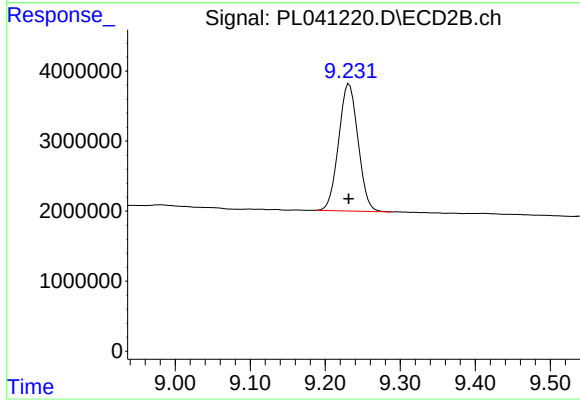

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 32631242
Conc: 12.62 ng/ml