

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102218\
 Data File : PL041234.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2018 18:01
 Operator : AJ\SJ
 Sample : J5605-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 01:12:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.103	64464648	34194775	11.762	12.264
28)	SA Decachlor...	8.221	9.233	52456742	22688250	10.089	8.774
Target Compounds							
10)	B gamma-Chl...	5.434	0.000	2487618	0	0.378	N.D. #
11)	B alpha-Chl...	5.434f	0.000	2487618	0	0.382	N.D. #
12)	B 4,4'-DDE	5.636	0.000	1880865	0	0.331	N.D. #
16)	A 4,4'-DDD	6.230f	0.000	2399600	0	0.531	N.D. #
17)	MA 4,4'-DDT	6.388	0.000	2788175	0	0.612	N.D. #
23)	Chlordane-1	4.407	0.000	3044721	0	11.930	N.D. #
24)	Chlordane-2	4.826	0.000	2551927	0	9.455	N.D. #
25)	Chlordane-3	5.434	0.000	2487618	0	3.250	N.D. #
26)	Chlordane-4	5.434	0.000	2487618	0	3.710	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102218\
Data File : PL041234.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2018 18:01
Operator : AJ\SJ
Sample : J5605-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 01:12:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

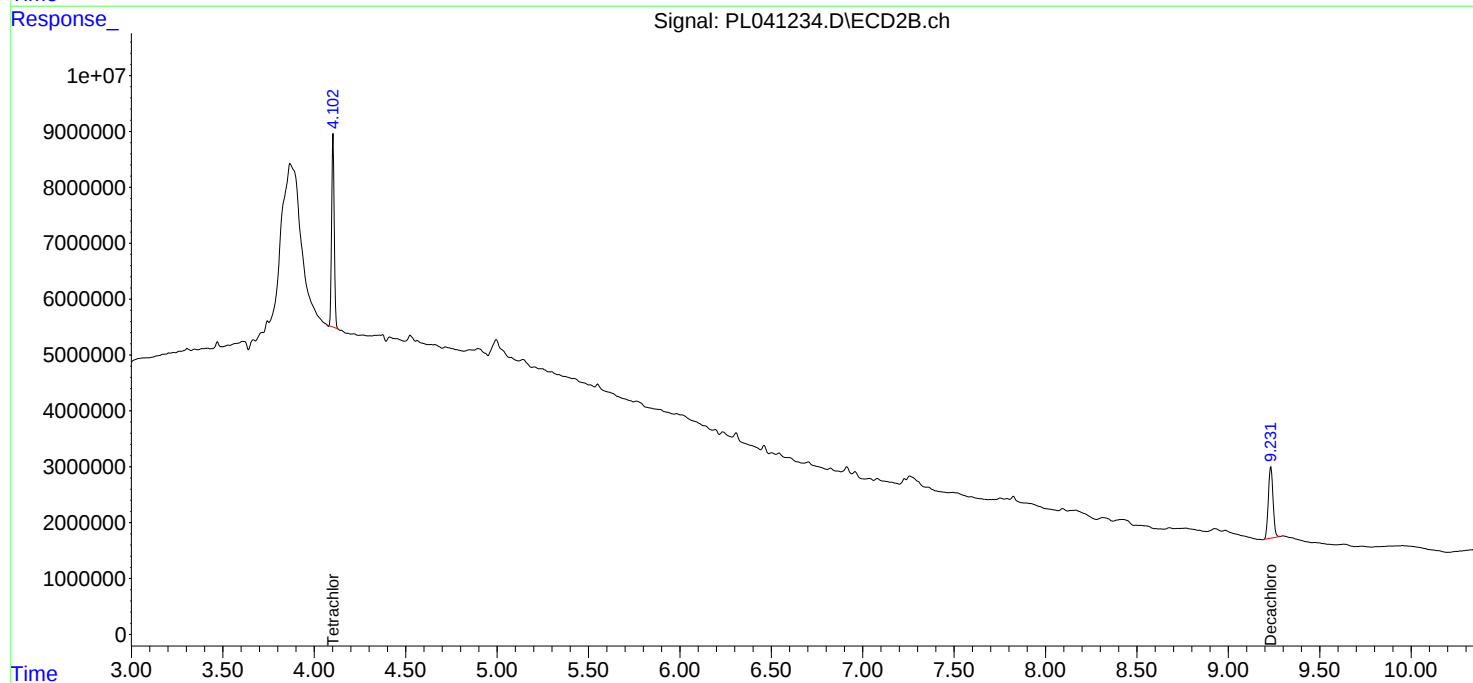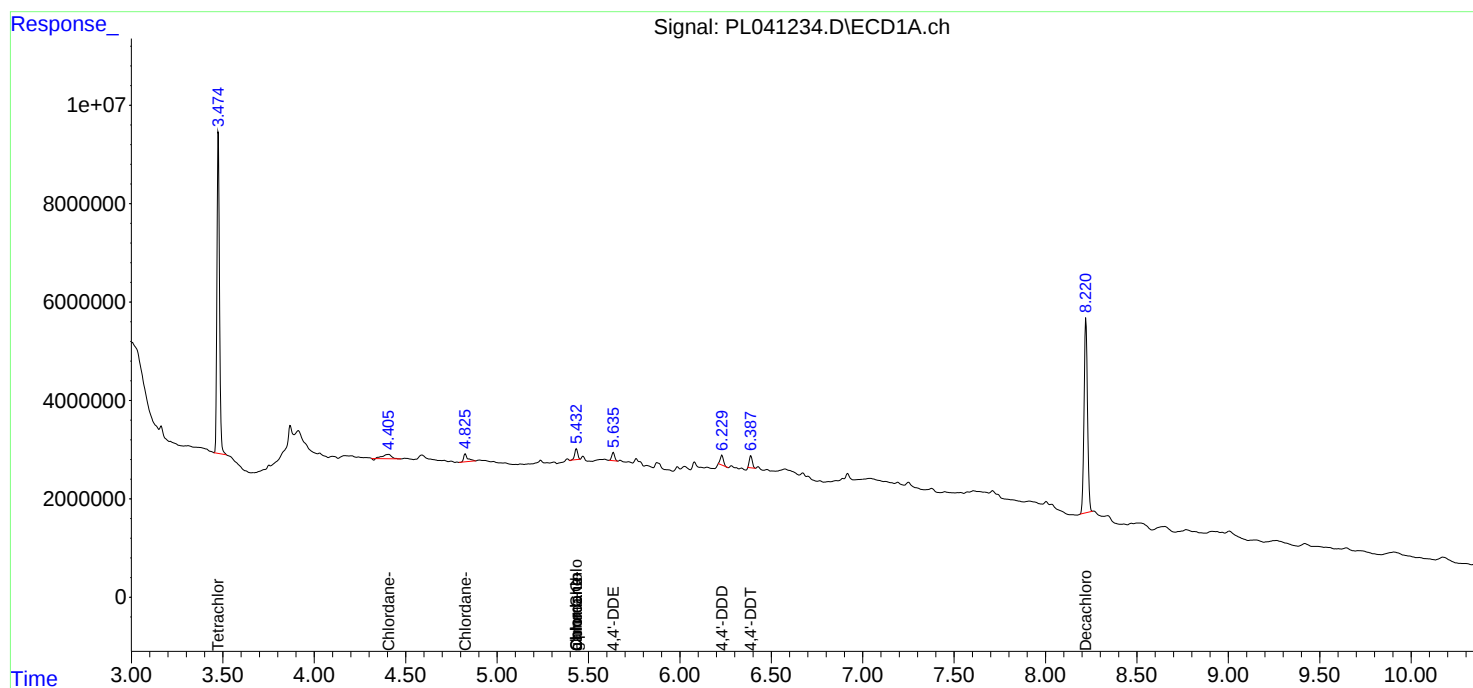


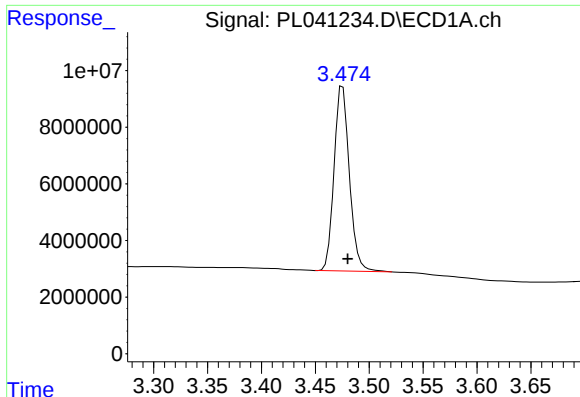

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: -0.005 min
Response: 64464648
Conc: 11.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

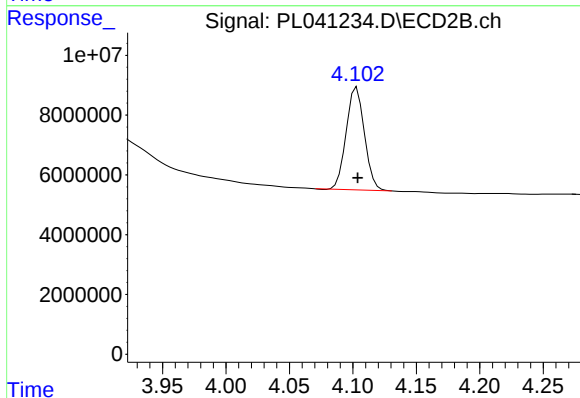


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.000 min
Response: 34194775
Conc: 12.26 ng/ml

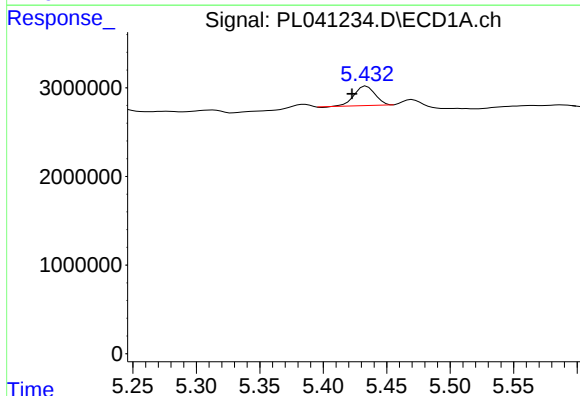


#10 gamma-Chlordane

R.T.: 5.434 min
Delta R.T.: 0.011 min
Response: 2487618
Conc: 0.38 ng/ml

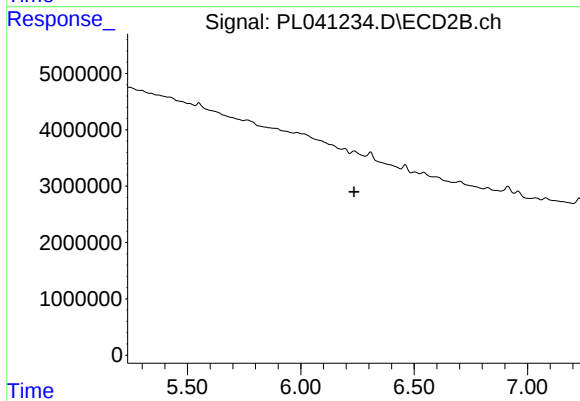

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.235 min
Response: 0
Conc: N.D.

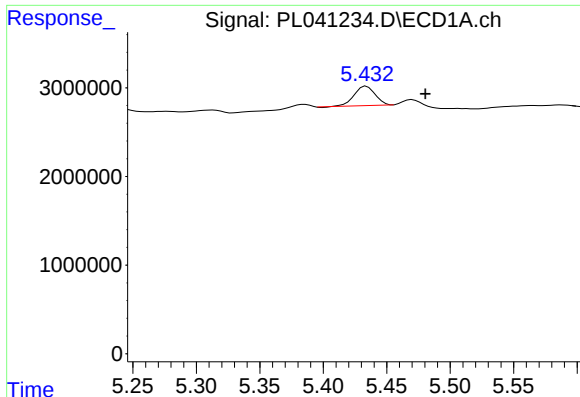

#11 alpha-Chlordane


R.T.: 5.434 min
Delta R.T.: -0.046 min
Response: 2487618
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

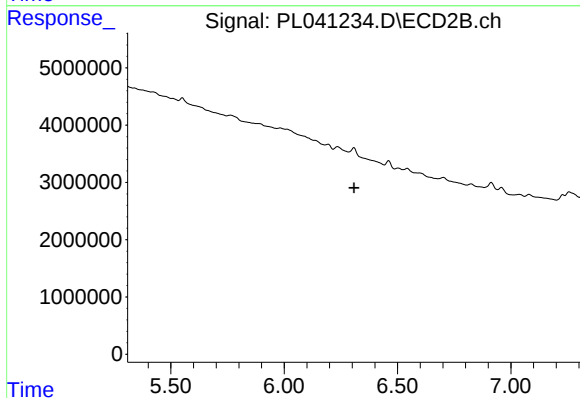


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.309 min
Response: 0
Conc: N.D.

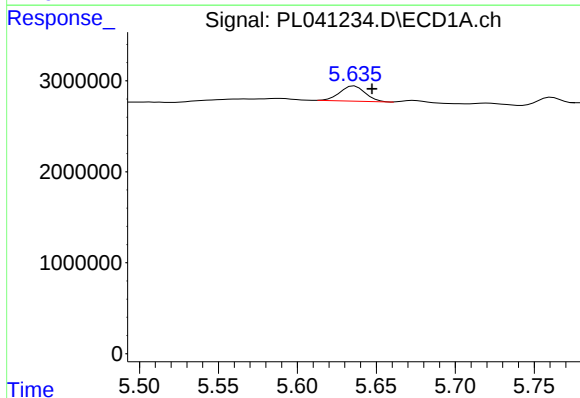


#12 4,4'-DDE

R.T.: 5.636 min
Delta R.T.: -0.011 min
Response: 1880865
Conc: 0.33 ng/ml

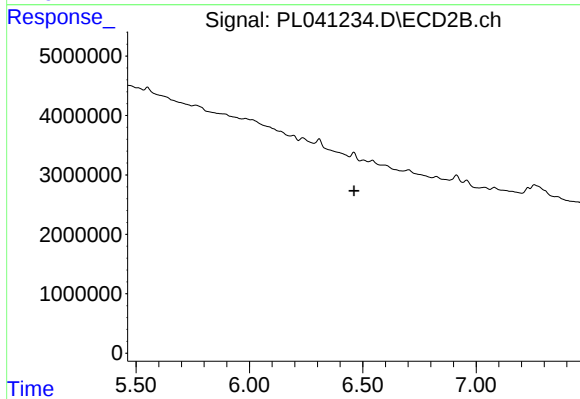

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.462 min
Response: 0
Conc: N.D.

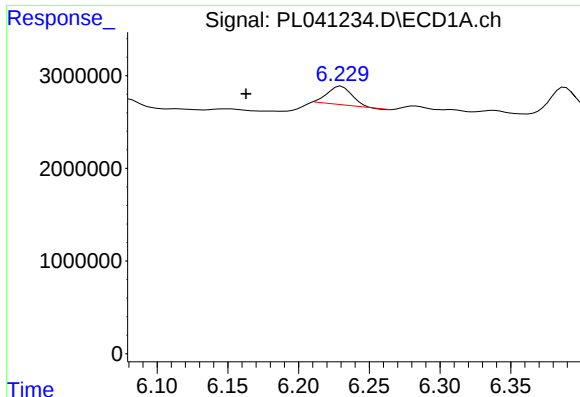

#16 4,4'-DDD


R.T.: 6.230 min
Delta R.T.: 0.067 min
Response: 2399600
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

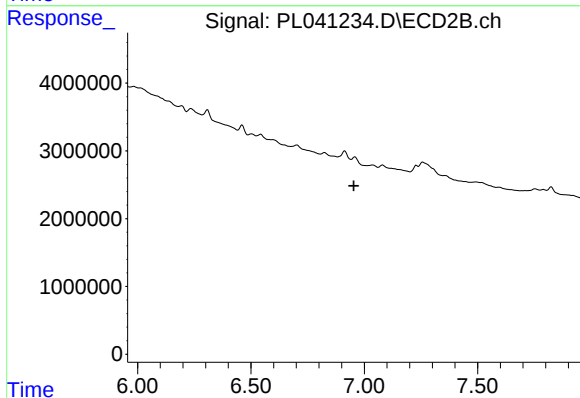


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.954 min
Response: 0
Conc: N.D.

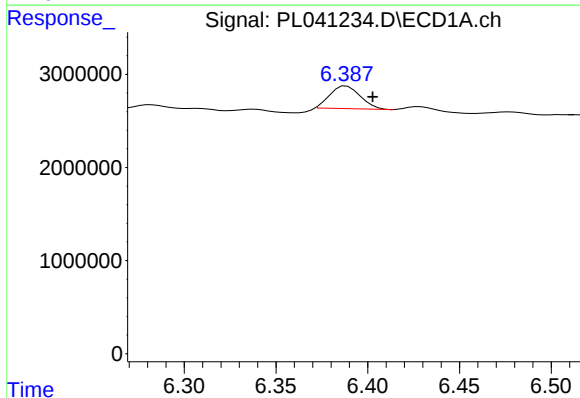


#17 4,4'-DDT

R.T.: 6.388 min
Delta R.T.: -0.014 min
Response: 2788175
Conc: 0.61 ng/ml

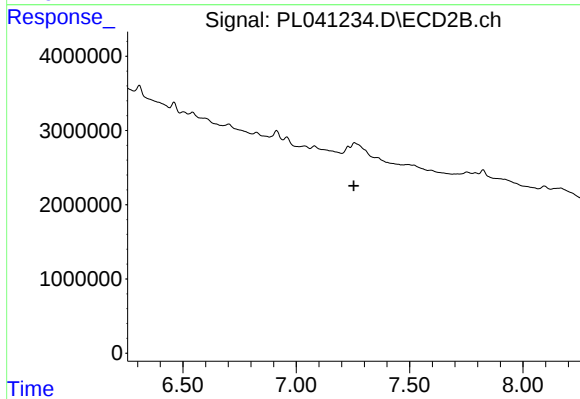

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.254 min
Response: 0
Conc: N.D.

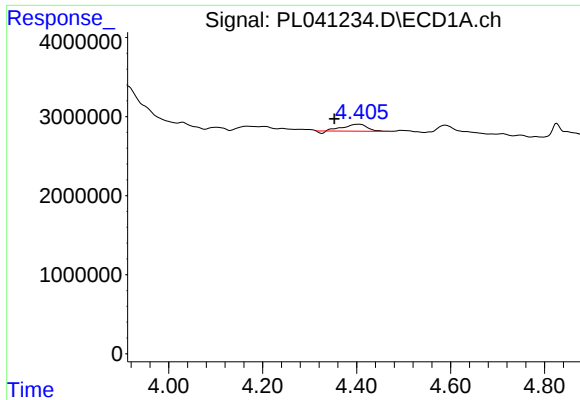

#23 Chlordane-1


R.T.: 4.407 min
Delta R.T.: 0.054 min
Response: 3044721
Conc: 11.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

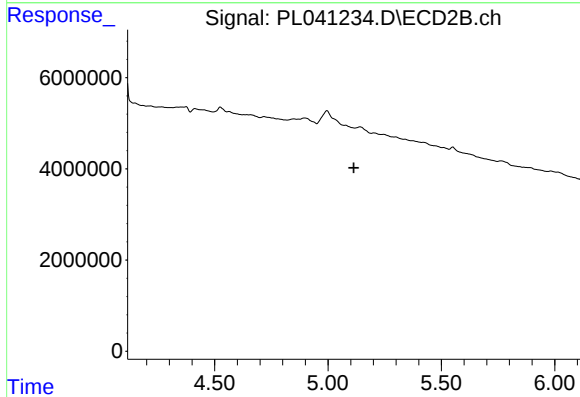


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

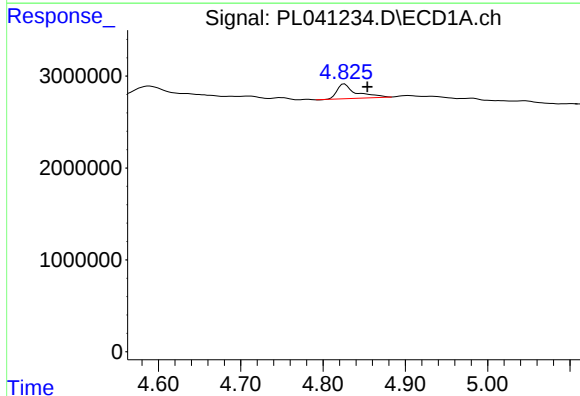


#24 Chlordane-2

R.T.: 4.826 min
Delta R.T.: -0.028 min
Response: 2551927
Conc: 9.46 ng/ml

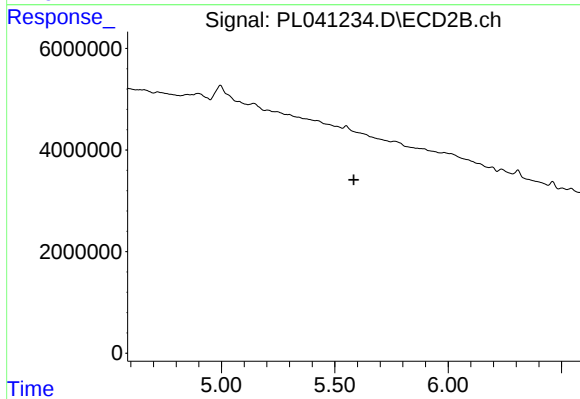

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.584 min
Response: 0
Conc: N.D.

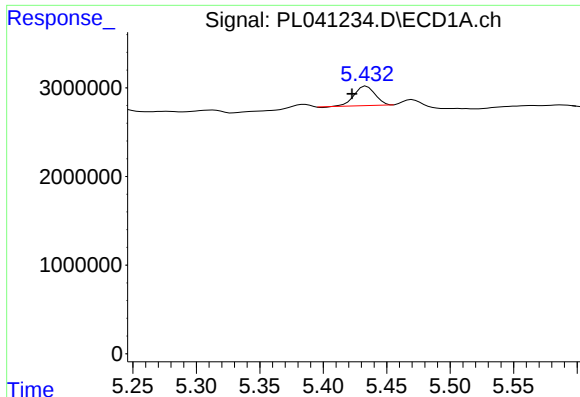

#25 Chlordane-3


R.T.: 5.434 min
Delta R.T.: 0.011 min
Response: 2487618
Conc: 3.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

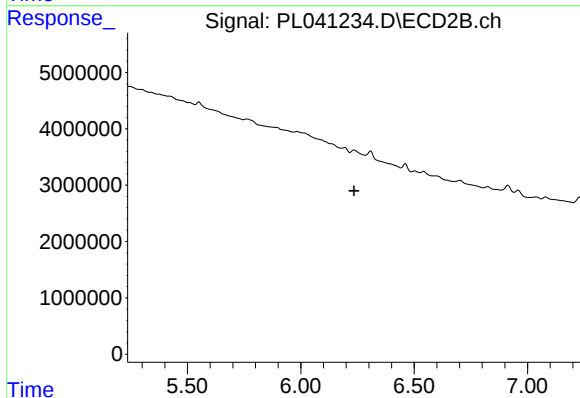


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.235 min
Response: 0
Conc: N.D.

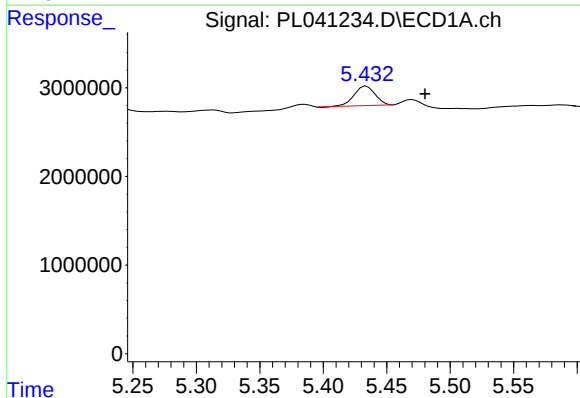


#26 Chlordane-4

R.T.: 5.434 min
Delta R.T.: -0.046 min
Response: 2487618
Conc: 3.71 ng/ml

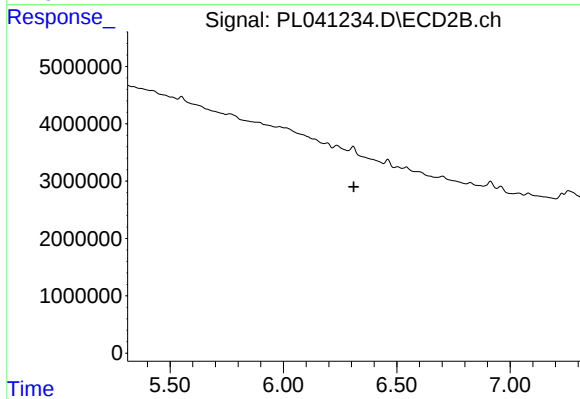

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.310 min
Response: 0
Conc: N.D.

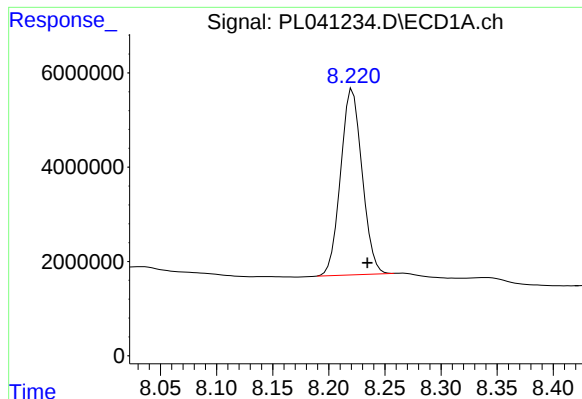

#28 Decachlorobiphenyl

R.T.: 8.221 min
Delta R.T.: -0.013 min
Response: 52456742
Conc: 10.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

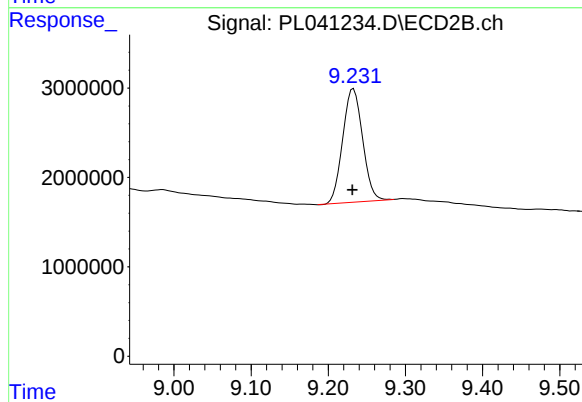

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.001 min
Response: 22688250
Conc: 8.77 ng/ml