

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102218\
 Data File : PL041220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2018 12:44
 Operator : AJ\SJ
 Sample : J5577-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SSSI-1016-S-DH-22

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 01:10:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.102	56183792	29836907	10.251	10.701
28)	SA Decachlor...	8.222	9.232	79329745	32631242	15.257	12.619
Target Compounds							
12)	B 4,4'-DDE	5.638	6.461	6215224	3277867	1.093	1.239



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102218\
Data File : PL041220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2018 12:44
Operator : AJ\SJ
Sample : J5577-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SSSI-1016-S-DH-22

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 01:10:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

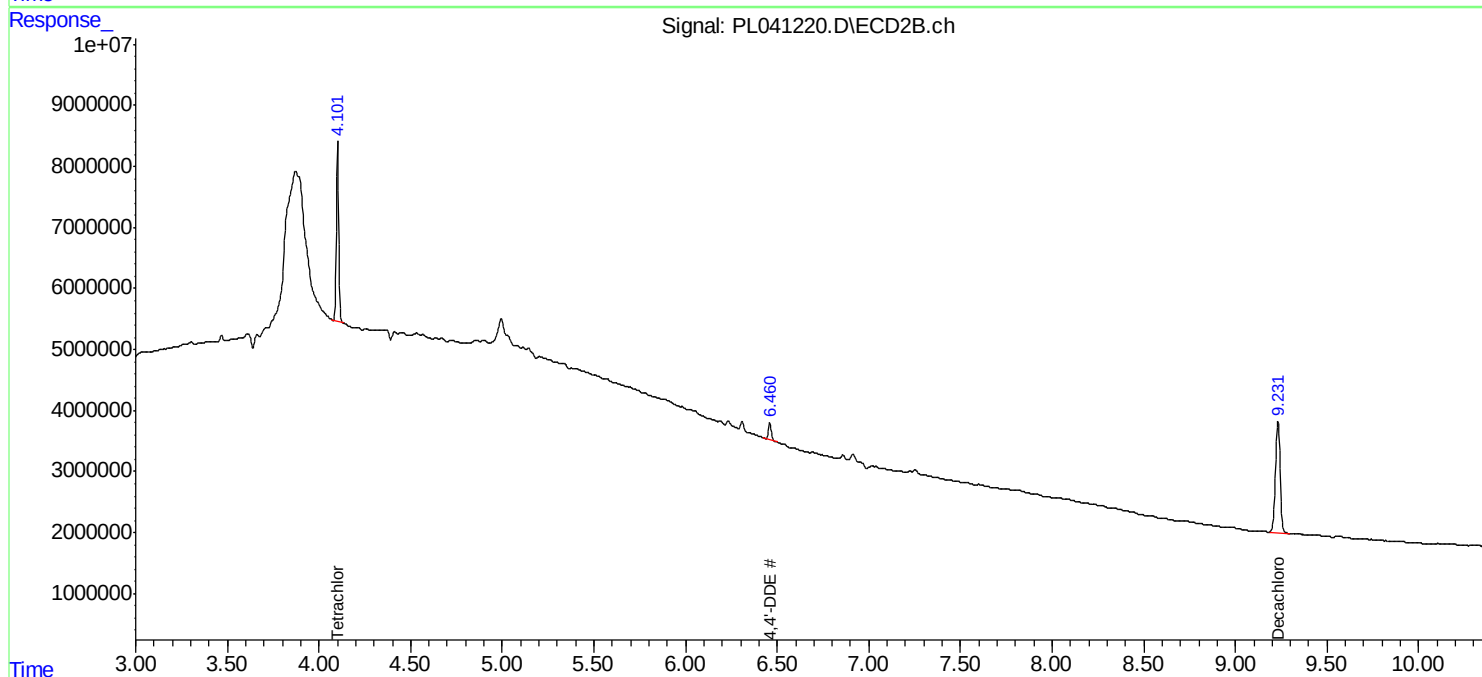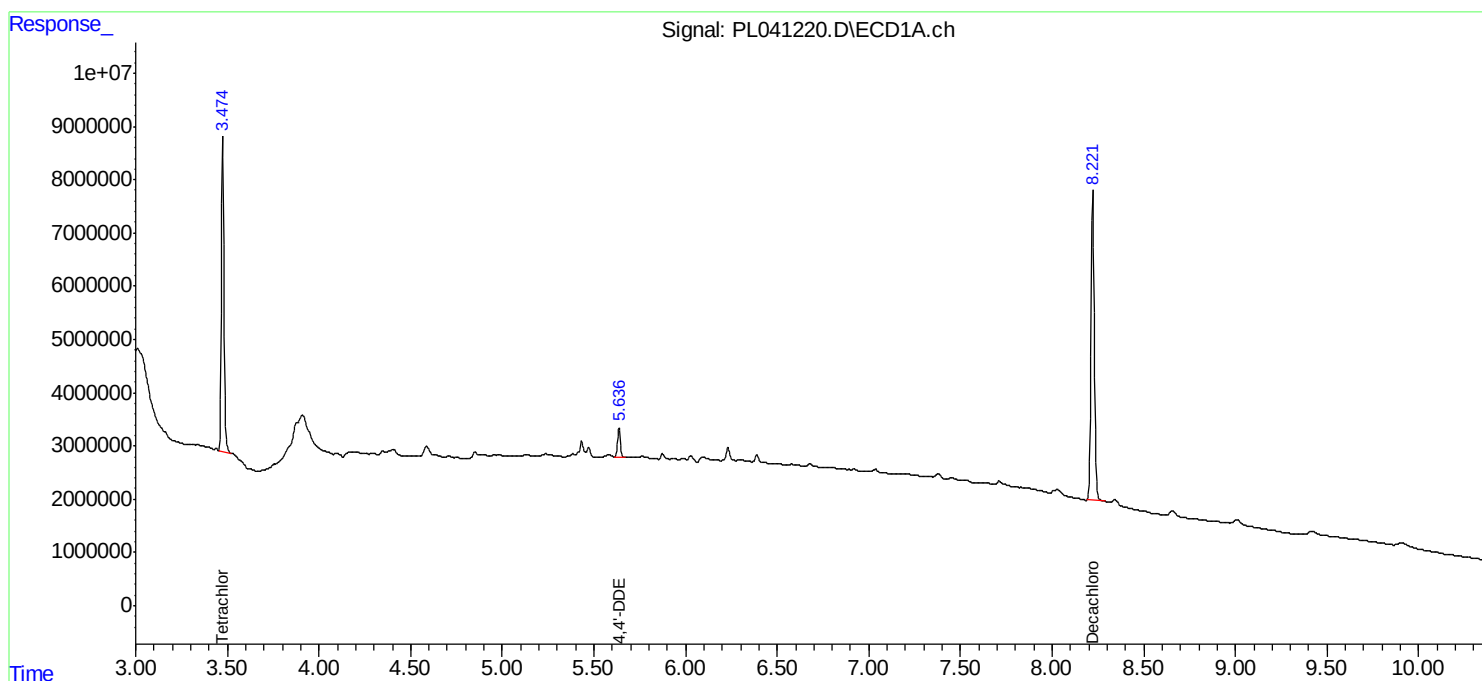


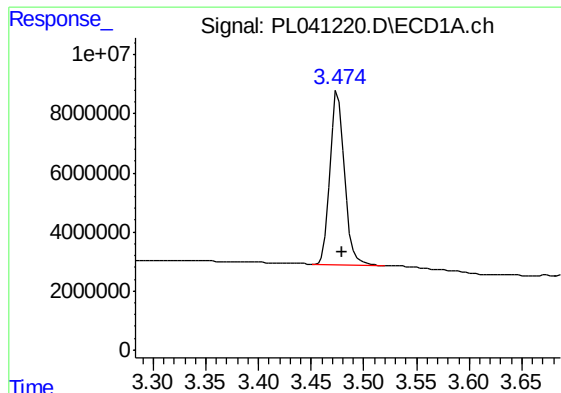

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: -0.004 min
Response: 56183792
Conc: 10.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1016-S-DH-22

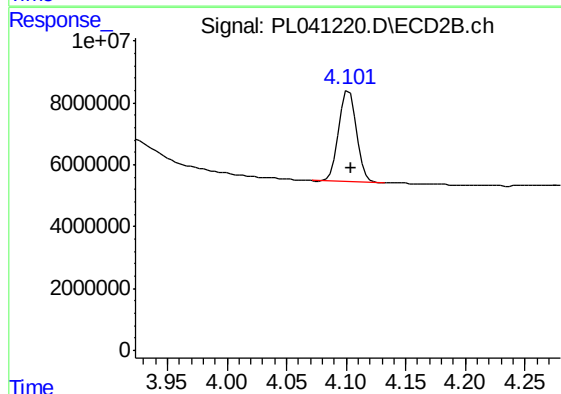


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: -0.001 min
Response: 29836907
Conc: 10.70 ng/ml

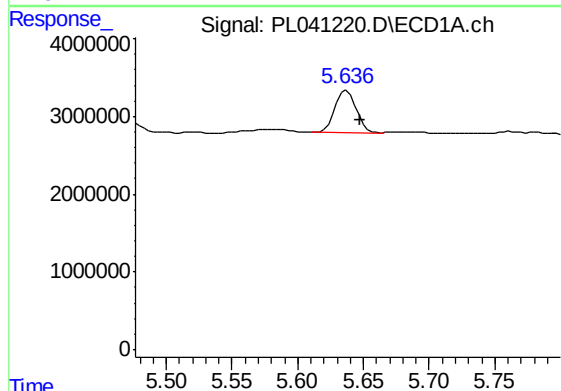


#12 4,4'-DDE

R.T.: 5.638 min
Delta R.T.: -0.010 min
Response: 6215224
Conc: 1.09 ng/ml

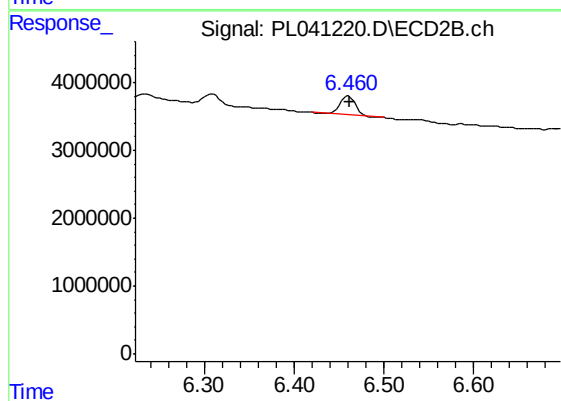

#12 4,4'-DDE


R.T.: 6.461 min
Delta R.T.: -0.001 min
Response: 3277867
Conc: 1.24 ng/ml

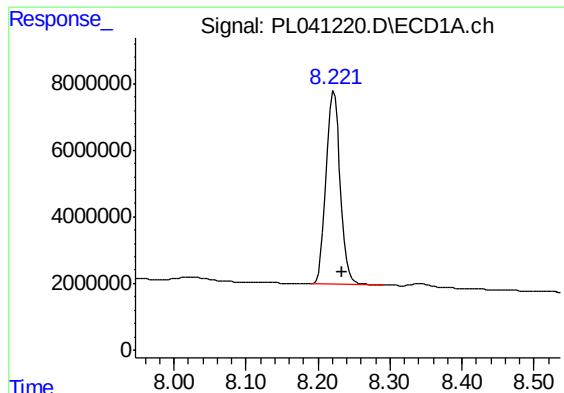

#28 Decachlorobiphenyl

R.T.: 8.222 min
Delta R.T.: -0.012 min
Response: 79329745
Conc: 15.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1016-S-DH-22

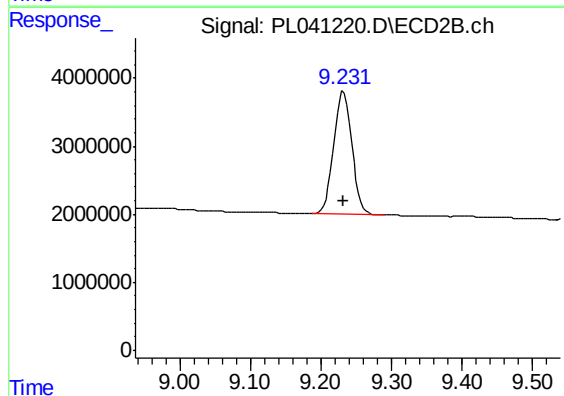

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 32631242
Conc: 12.62 ng/ml