

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102219\
 Data File : PL053563.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2019 09:31
 Operator : SG\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 01:27:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	4.045	613.2E6	113.1E6	56.569	45.182
28)	SA Decachlor...	8.332	9.123	410.7E6	118.7E6	41.862	42.138
Target Compounds							
23)	Chlordane-1	4.428	5.043	181.7E6	40012513	512.357	477.097
24)	Chlordane-2	4.934	5.510	195.0E6	46272030	506.047	471.099
25)	Chlordane-3	5.509	6.157	578.6E6	162.6E6	501.954	445.139
26)	Chlordane-4	5.567	6.231	479.5E6	207.5E6	511.497	462.234
27)	Chlordane-5	6.409	7.036	160.6E6	36493771	439.271	477.366



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102219\
Data File : PL053563.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2019 09:31
Operator : SG\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 01:27:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

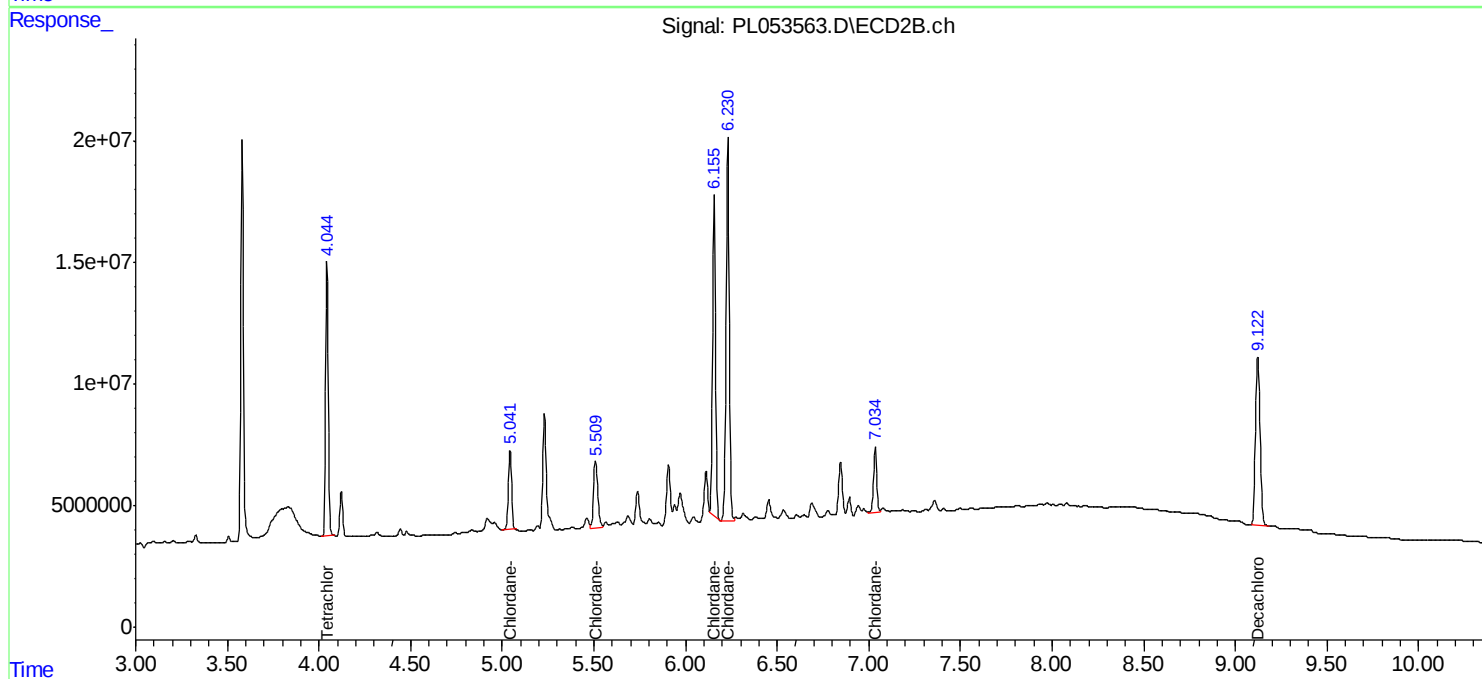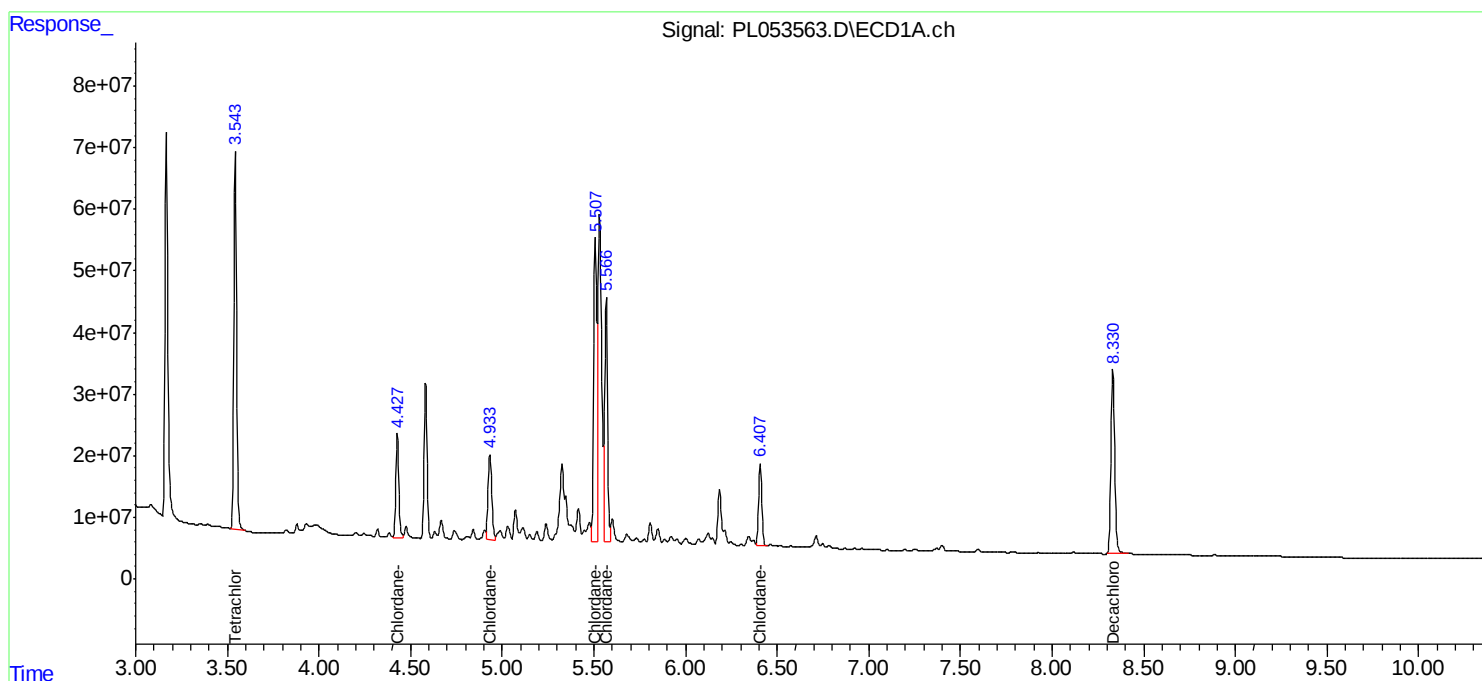


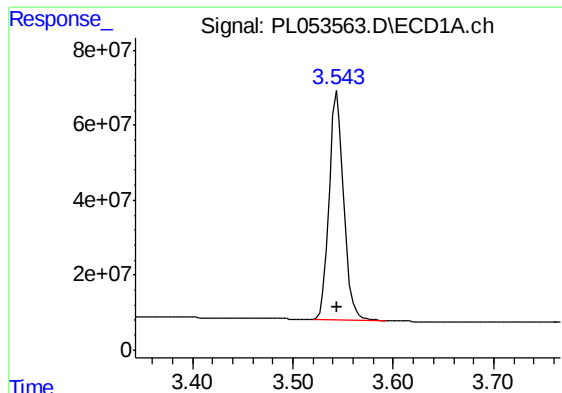

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 613172981
Conc: 56.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

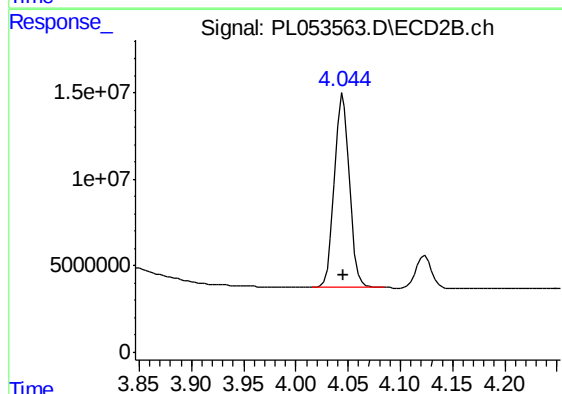


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 113062468
Conc: 45.18 ng/ml

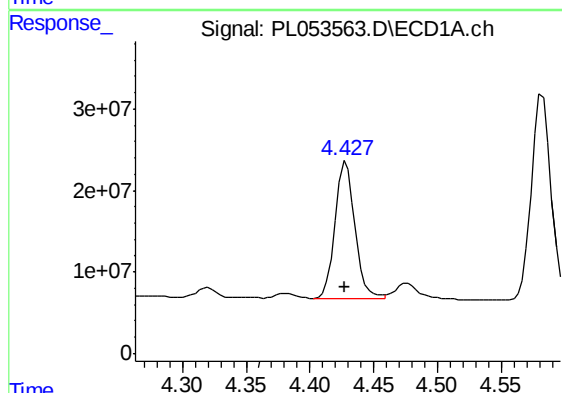


#23 Chlordane-1

R.T.: 4.428 min
Delta R.T.: 0.000 min
Response: 181718394
Conc: 512.36 ng/ml

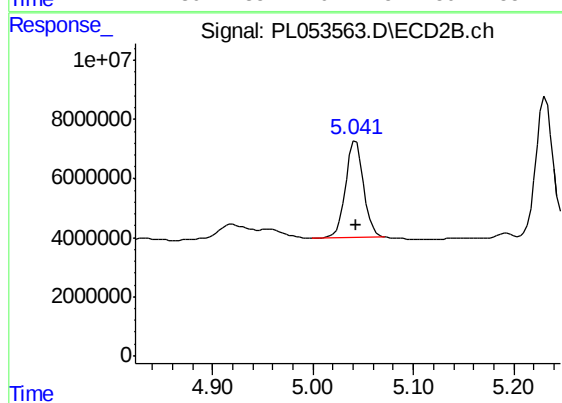

#23 Chlordane-1


R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 40012513
Conc: 477.10 ng/ml

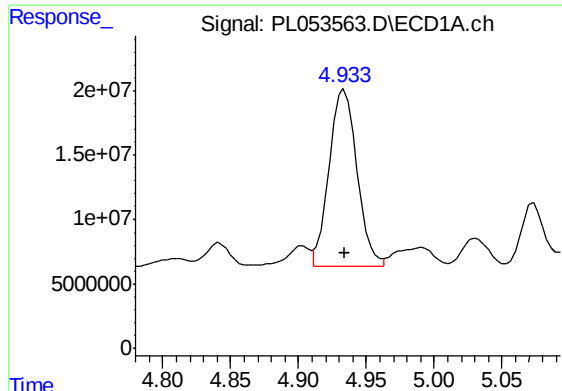

#24 Chlordane-2


R.T.: 4.934 min
Delta R.T.: 0.000 min
Response: 194987838
Conc: 506.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

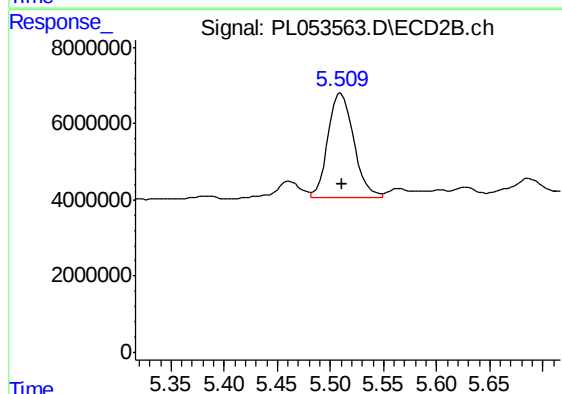


#24 Chlordane-2

R.T.: 5.510 min
Delta R.T.: 0.000 min
Response: 46272030
Conc: 471.10 ng/ml

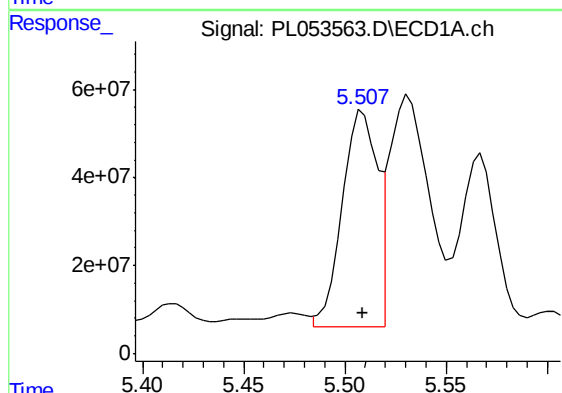


#25 Chlordane-3

R.T.: 5.509 min
Delta R.T.: 0.000 min
Response: 578595609
Conc: 501.95 ng/ml

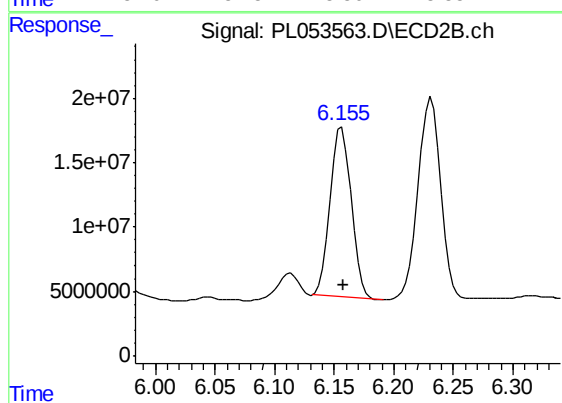

#25 Chlordane-3


R.T.: 6.157 min
Delta R.T.: -0.002 min
Response: 162578353
Conc: 445.14 ng/ml

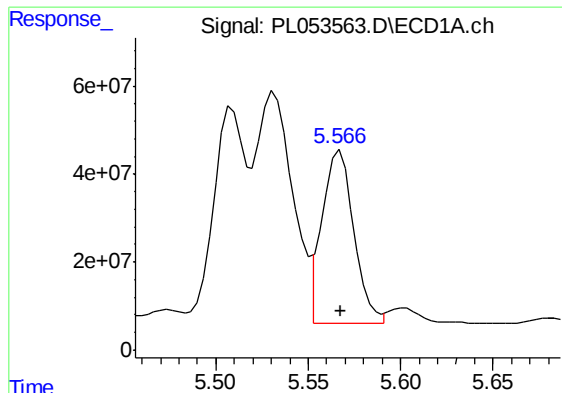

#26 Chlordane-4


R.T.: 5.567 min
Delta R.T.: 0.000 min
Response: 479504079
Conc: 511.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

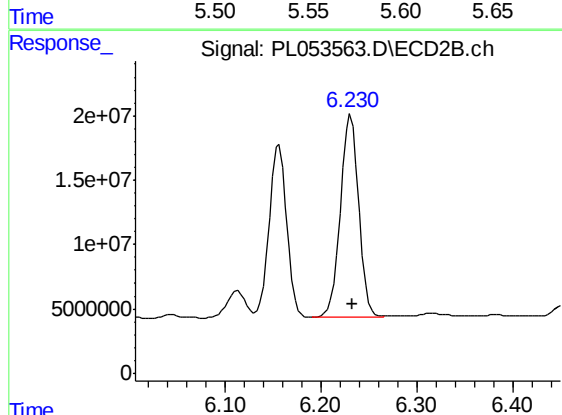


#26 Chlordane-4

R.T.: 6.231 min
Delta R.T.: 0.000 min
Response: 207514013
Conc: 462.23 ng/ml

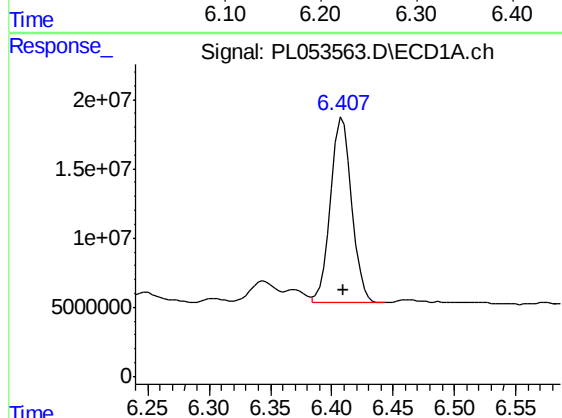


#27 Chlordane-5

R.T.: 6.409 min
Delta R.T.: 0.000 min
Response: 160572955
Conc: 439.27 ng/ml

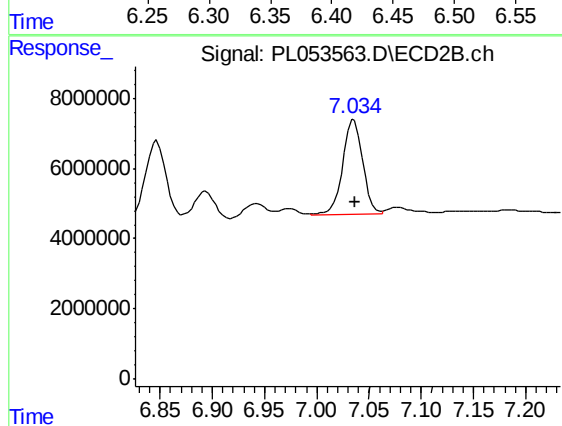

#27 Chlordane-5


R.T.: 7.036 min
Delta R.T.: -0.001 min
Response: 36493771
Conc: 477.37 ng/ml

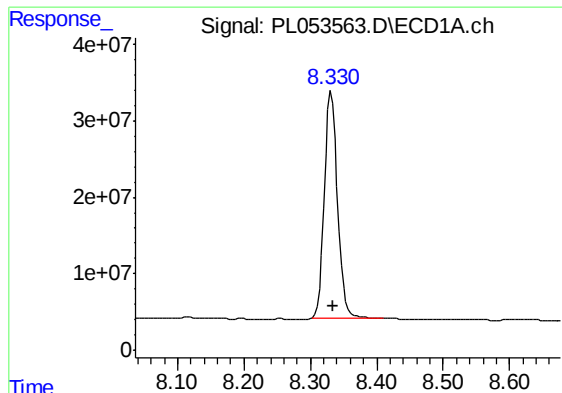

#28 Decachlorobiphenyl

R.T.: 8.332 min
Delta R.T.: -0.002 min
Response: 410729039
Conc: 41.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

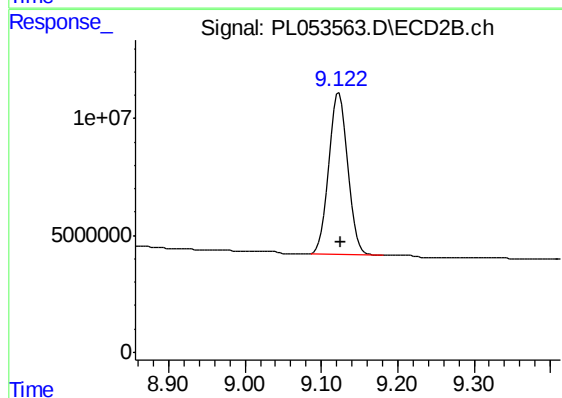

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.003 min
Response: 118660944
Conc: 42.14 ng/ml