

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102219\
 Data File : PL053575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2019 12:45
 Operator : SG\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 03:25:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	4.045	597.6E6	115.8E6	55.137	46.287
28)	SA Decachlor...	8.330	9.123	415.3E6	122.8E6	42.324	43.600
Target Compounds							
23)	Chlordane-1	4.426	5.042	175.9E6	41063900	495.955	489.633
24)	Chlordane-2	4.932	5.510	161.6E6	47359796	419.322	482.174
25)	Chlordane-3	5.507	6.157	588.4E6	170.1E6	510.447	465.625
26)	Chlordane-4	5.565	6.231	475.1E6	217.4E6	506.781	484.262
27)	Chlordane-5	6.407	7.035	170.0E6	38663316	465.188	505.745



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102219\
Data File : PL053575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2019 12:45
Operator : SG\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 03:25:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

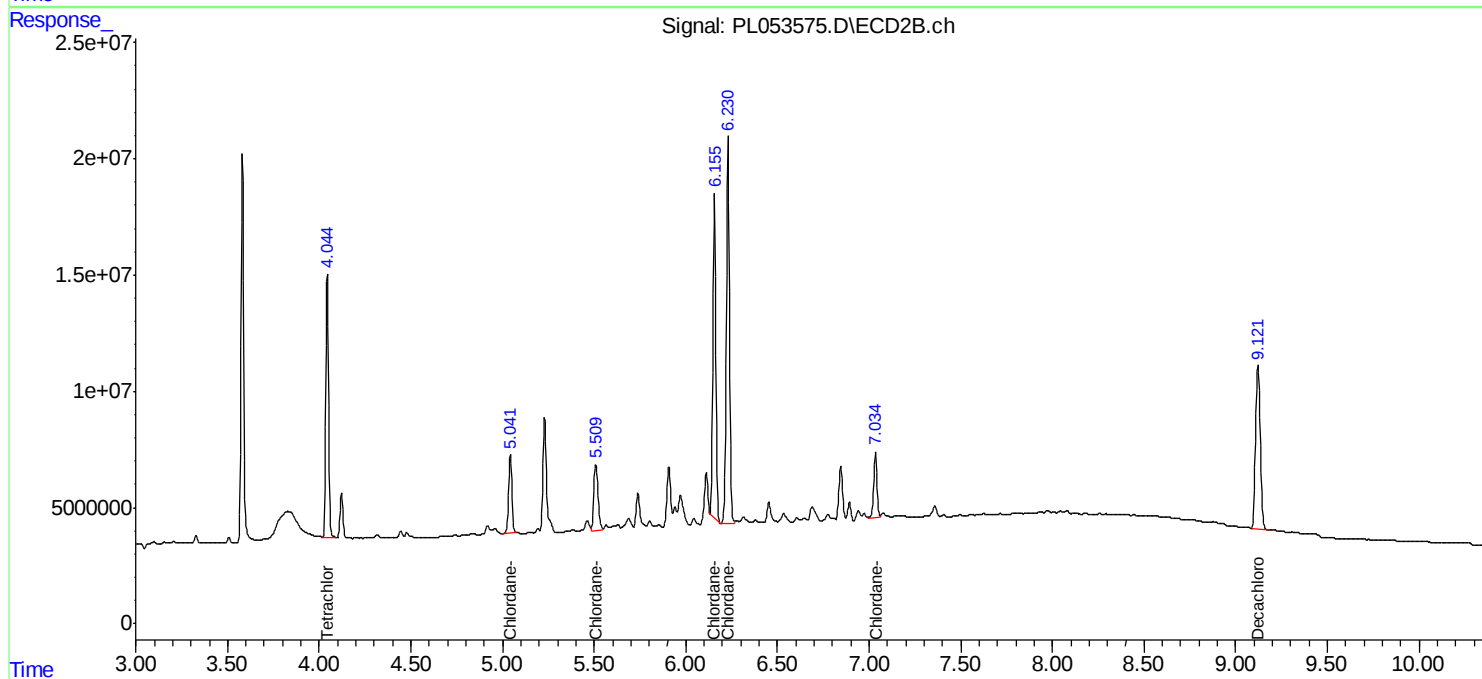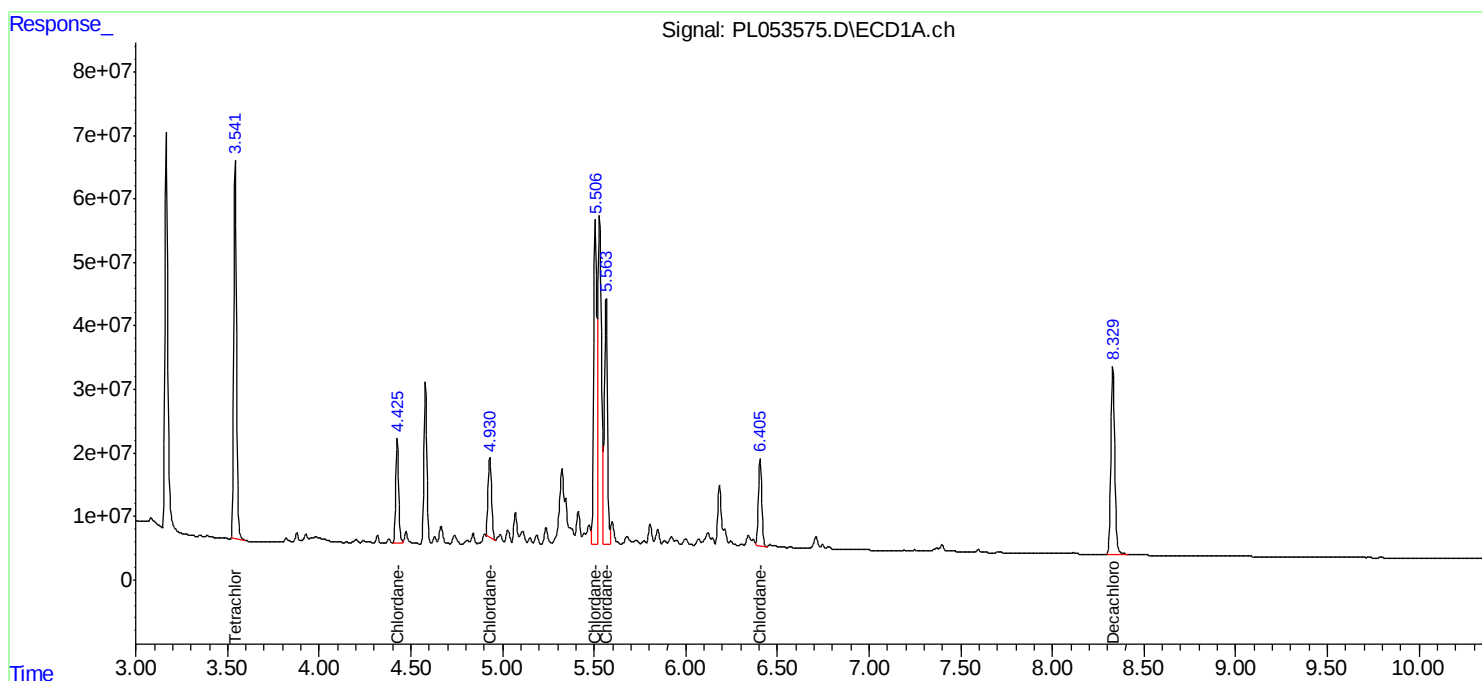


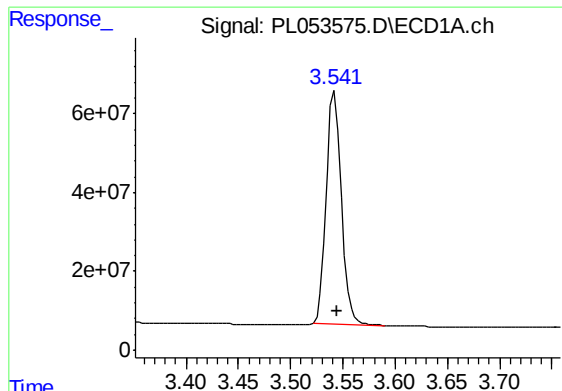

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 597645888
Conc: 55.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

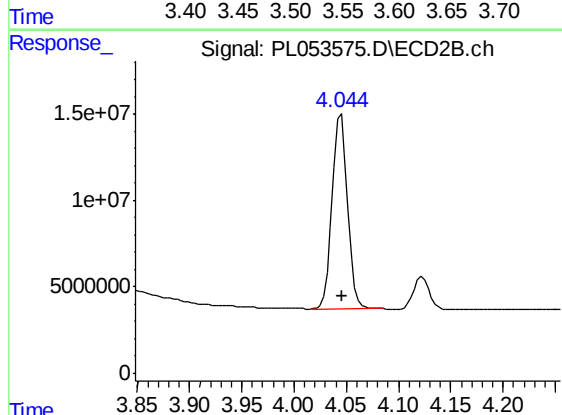


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 115826605
Conc: 46.29 ng/ml

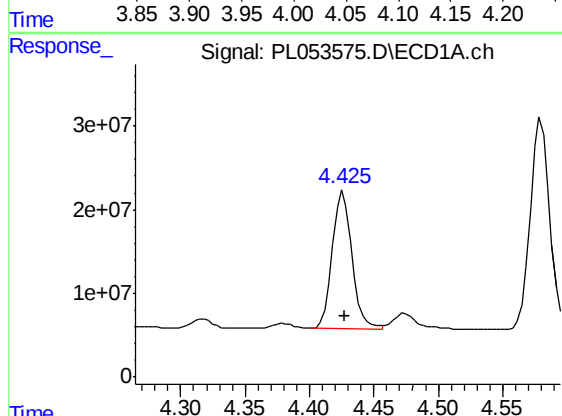


#23 Chlordane-1

R.T.: 4.426 min
Delta R.T.: -0.001 min
Response: 175901101
Conc: 495.96 ng/ml

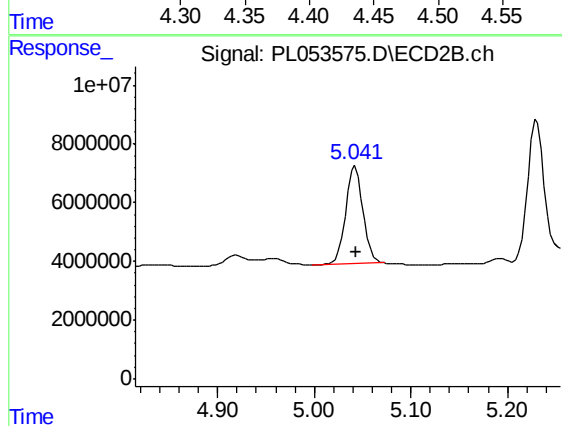

#23 Chlordane-1


R.T.: 5.042 min
Delta R.T.: -0.001 min
Response: 41063900
Conc: 489.63 ng/ml

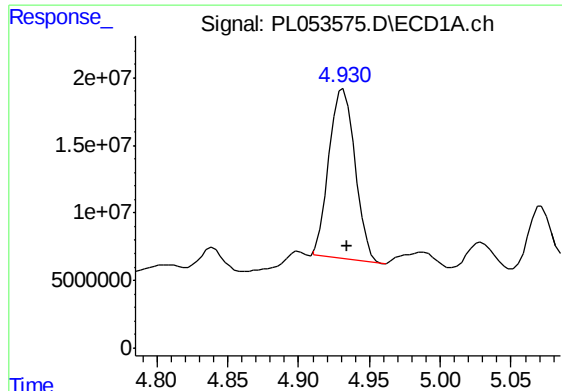

#24 Chlordane-2


R.T.: 4.932 min
Delta R.T.: -0.002 min
Response: 161571275
Conc: 419.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

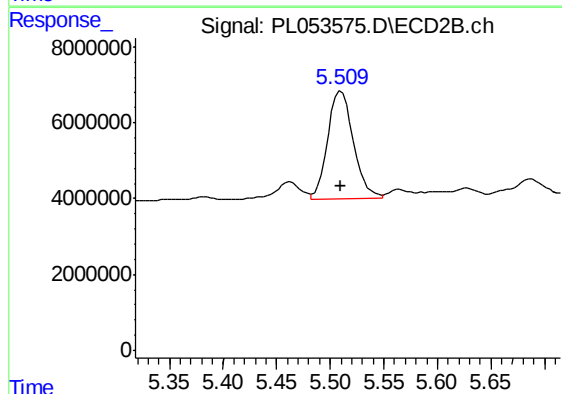


#24 Chlordane-2

R.T.: 5.510 min
Delta R.T.: 0.000 min
Response: 47359796
Conc: 482.17 ng/ml

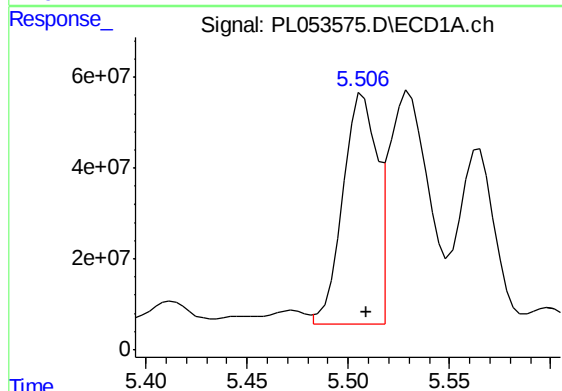


#25 Chlordane-3

R.T.: 5.507 min
Delta R.T.: -0.002 min
Response: 588385853
Conc: 510.45 ng/ml

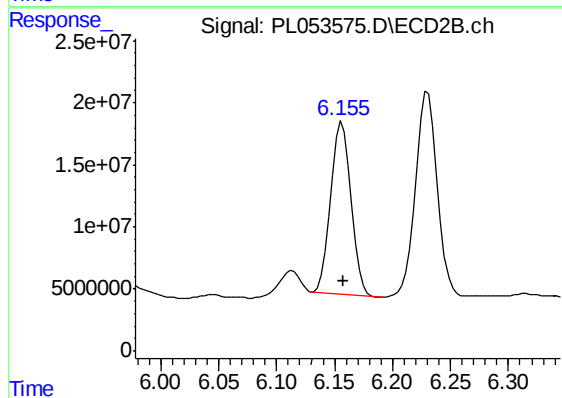

#25 Chlordane-3


R.T.: 6.157 min
Delta R.T.: -0.002 min
Response: 170060306
Conc: 465.62 ng/ml

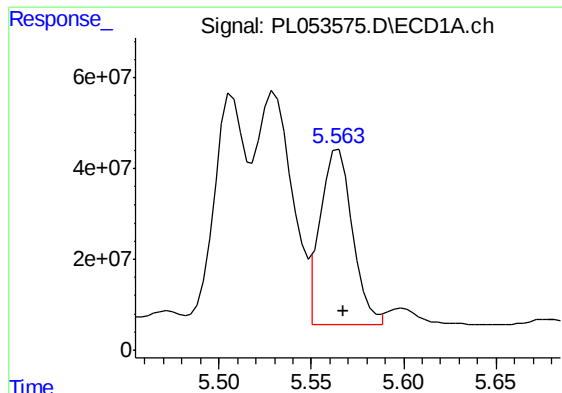

#26 Chlordane-4


R.T.: 5.565 min
Delta R.T.: -0.003 min
Response: 475082920
Conc: 506.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

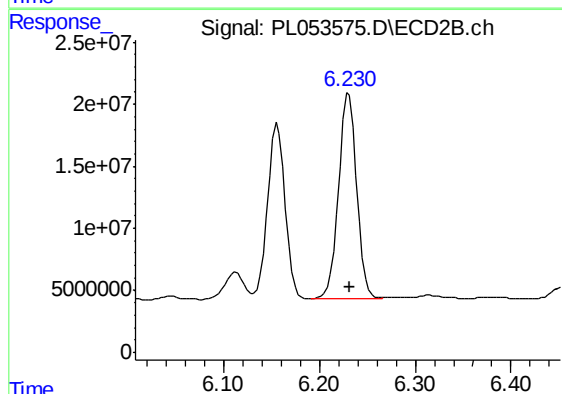


#26 Chlordane-4

R.T.: 6.231 min
Delta R.T.: -0.001 min
Response: 217403260
Conc: 484.26 ng/ml

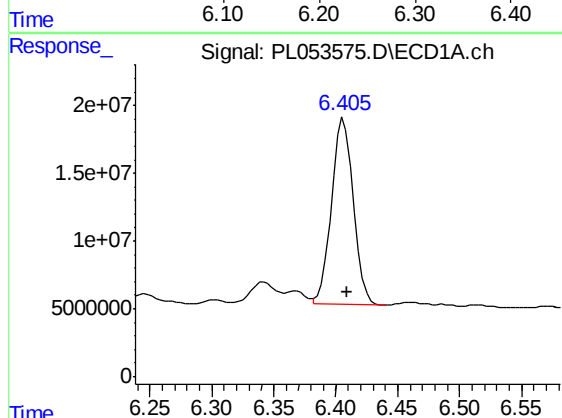


#27 Chlordane-5

R.T.: 6.407 min
Delta R.T.: -0.003 min
Response: 170046663
Conc: 465.19 ng/ml

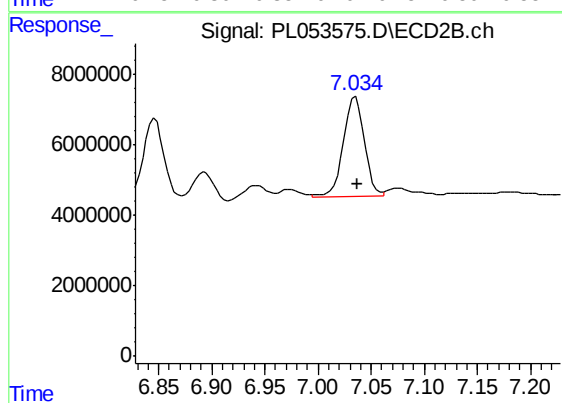

#27 Chlordane-5


R.T.: 7.035 min
Delta R.T.: -0.002 min
Response: 38663316
Conc: 505.75 ng/ml

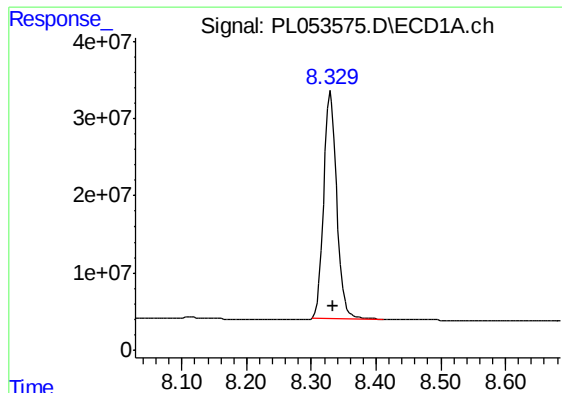

#28 Decachlorobiphenyl

R.T.: 8.330 min
Delta R.T.: -0.004 min
Response: 415267685
Conc: 42.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

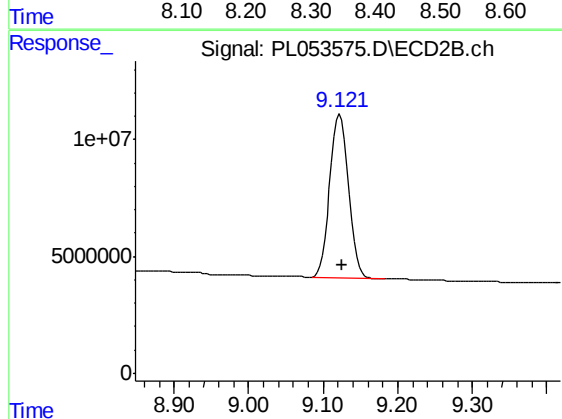

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.003 min
Response: 122778311
Conc: 43.60 ng/ml