

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102220\
 Data File : PL062505.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2020 08:34
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 15:32:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) MB Aldrin	4.651	0.000	452481	0	0.237	N.D. #
8) B Heptachlo...	5.103	5.812	12145493	28532493	6.657	8.810 #
10) B gamma-Chl...	0.000	6.040	0	2903231	N.D.	0.862 #
12) B 4,4'-DDE	5.580f	0.000	1064664	0	0.644	N.D. #
14) MA Endrin	5.947	0.000	580062	0	0.349	N.D. #
23) Chlordane-1	4.269	0.000	508752	0	9.869	N.D. #
24) Chlordane-2	4.757	0.000	21213603	0	368.038	N.D. #
25) Chlordane-3	0.000	6.040	0	2903231	N.D.	7.187 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102220\
Data File : PL062505.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2020 08:34
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 15:32:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

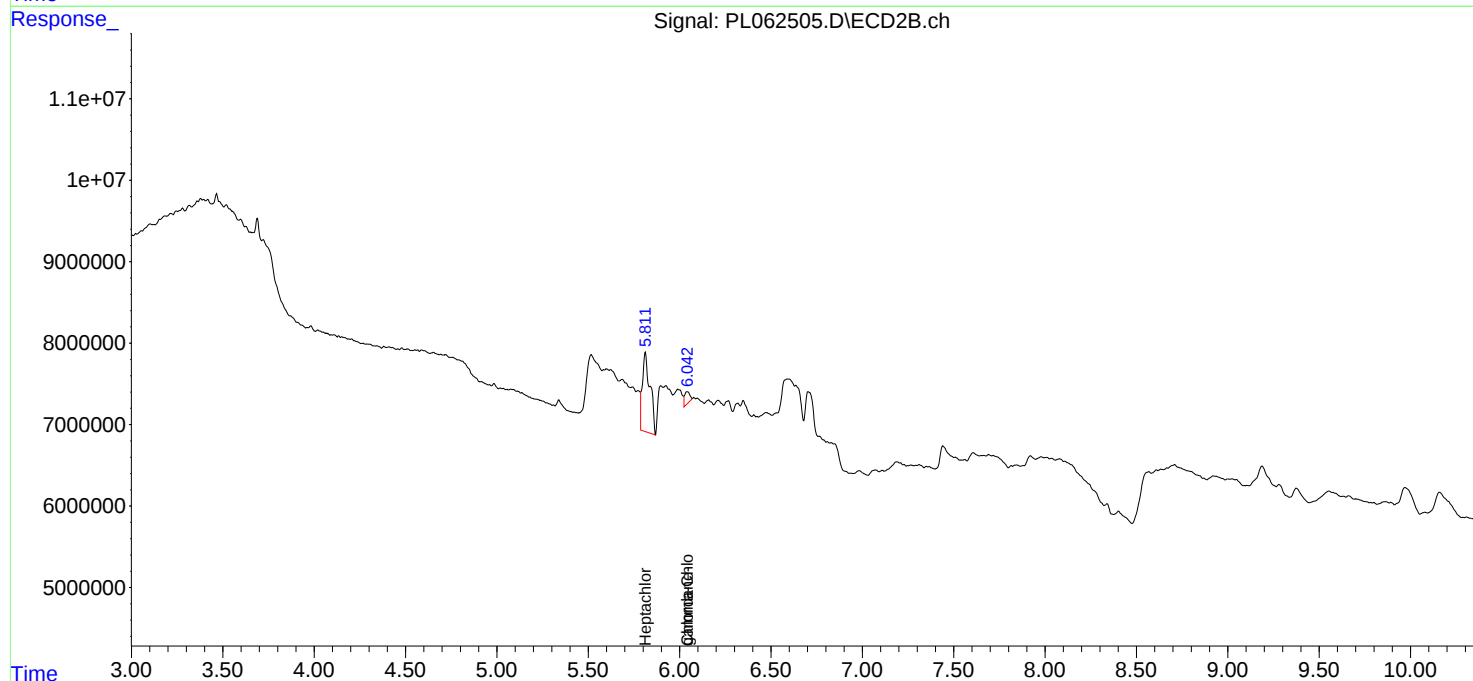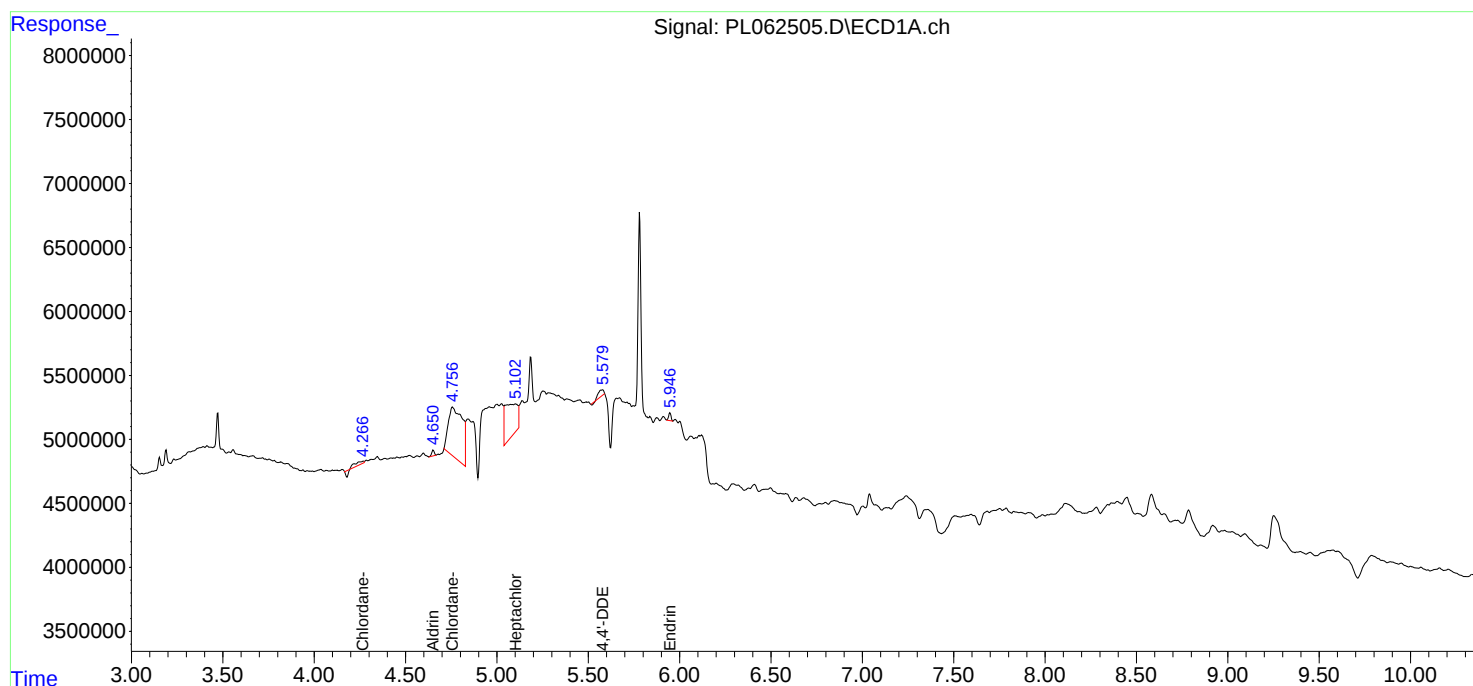


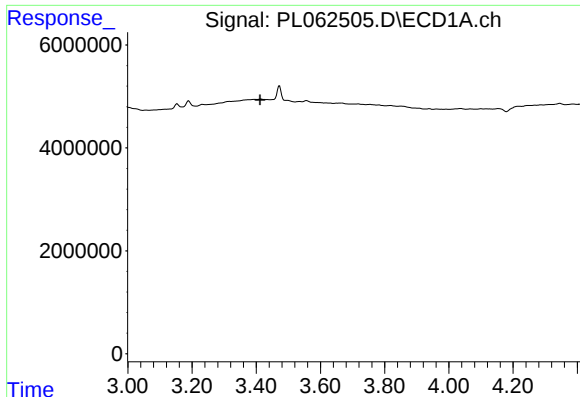

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

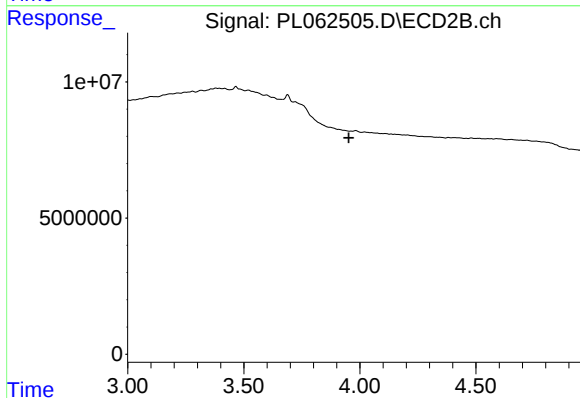


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.952 min
Response: 0
Conc: N.D.

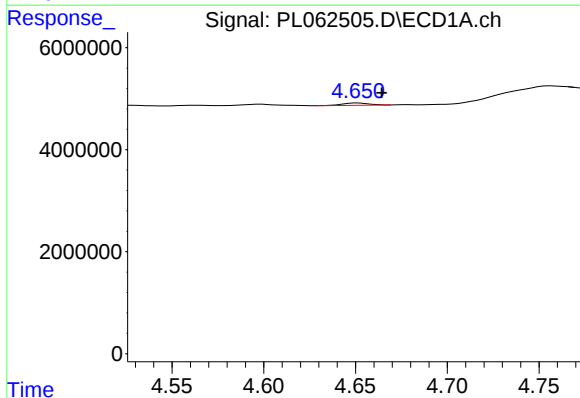


#5 Aldrin

R.T.: 4.651 min
Delta R.T.: -0.013 min
Response: 452481
Conc: 0.24 ng/ml

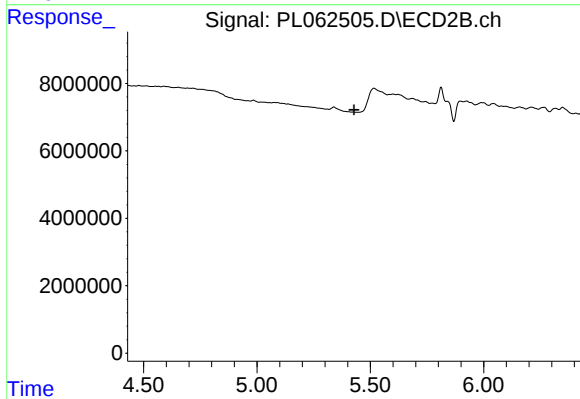

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.429 min
Response: 0
Conc: N.D.

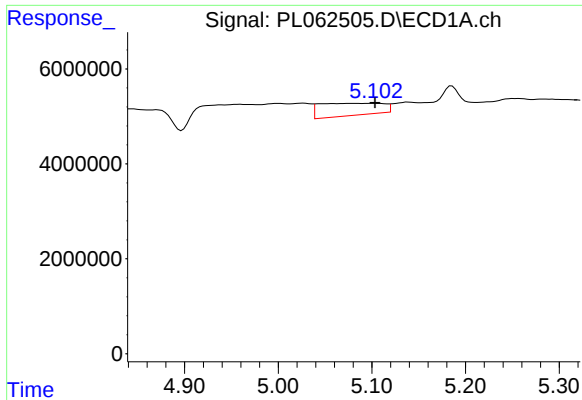

#8 Heptachlor epoxide


R.T.: 5.103 min
Delta R.T.: 0.000 min
Response: 12145493
Conc: 6.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

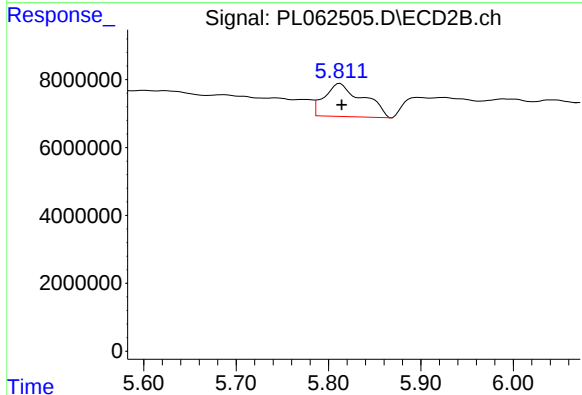


#8 Heptachlor epoxide

R.T.: 5.812 min
Delta R.T.: -0.002 min
Response: 28532493
Conc: 8.81 ng/ml

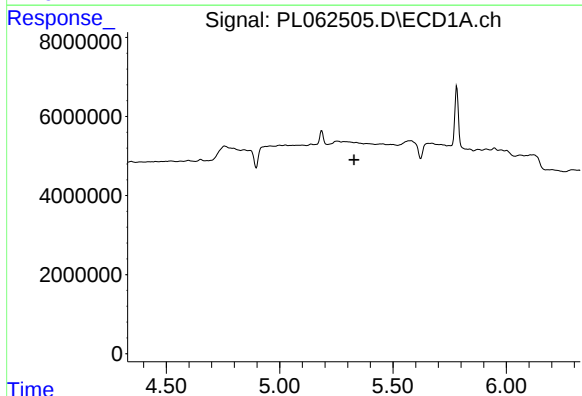


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

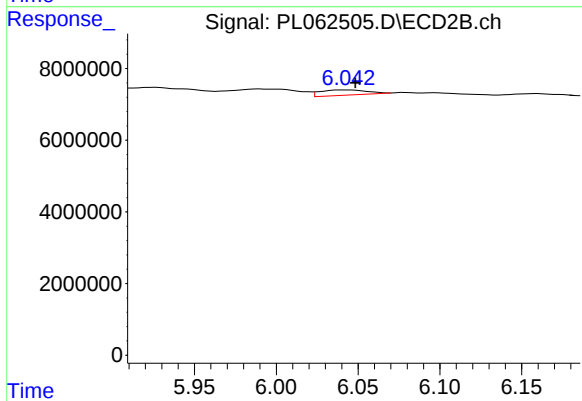

#10 gamma-Chlordane


R.T.: 6.040 min
Delta R.T.: -0.009 min
Response: 2903231
Conc: 0.86 ng/ml

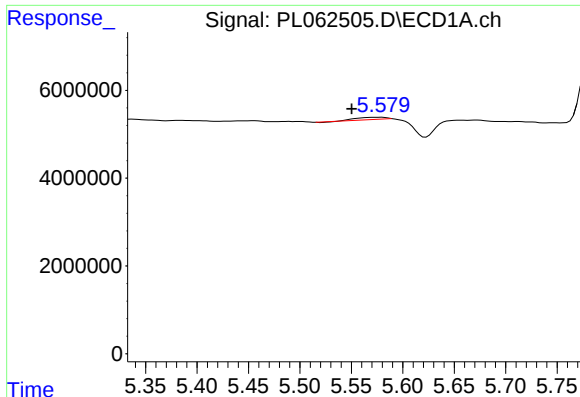

#12 4,4'-DDE


R.T.: 5.580 min
Delta R.T.: 0.029 min
Response: 1064664
Conc: 0.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

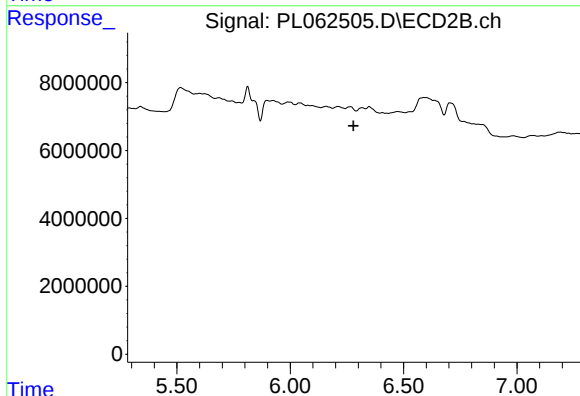


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.279 min
Response: 0
Conc: N.D.

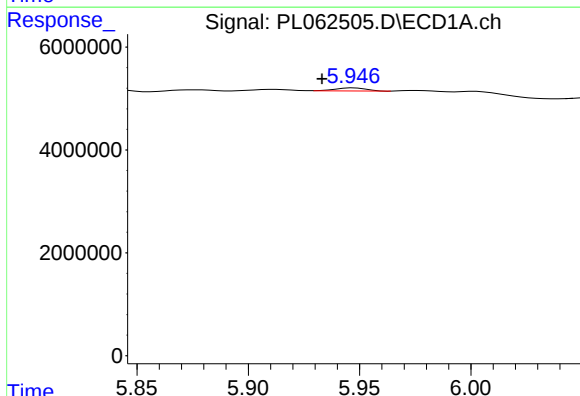


#14 Endrin

R.T.: 5.947 min
Delta R.T.: 0.014 min
Response: 580062
Conc: 0.35 ng/ml

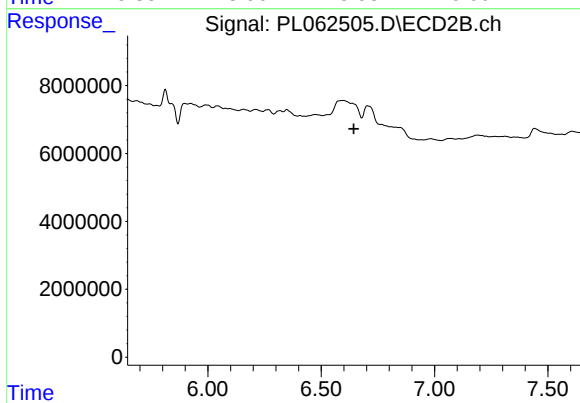

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.643 min
Response: 0
Conc: N.D.

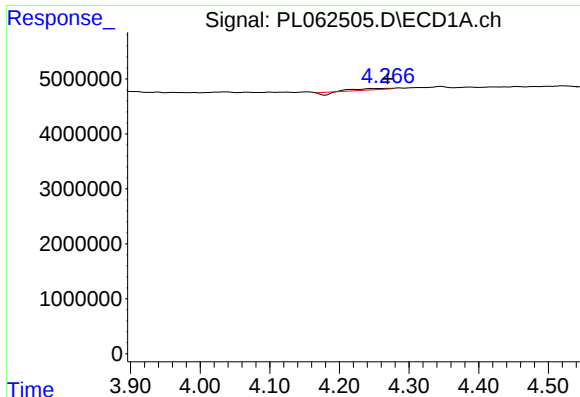

#23 Chlordane-1


R.T.: 4.269 min
Delta R.T.: 0.000 min
Response: 508752
Conc: 9.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

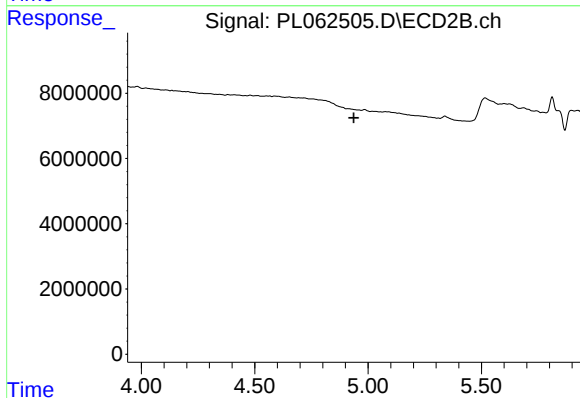


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

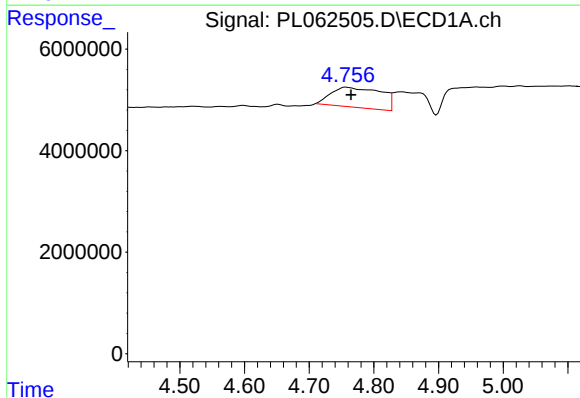


#24 Chlordane-2

R.T.: 4.757 min
Delta R.T.: -0.008 min
Response: 21213603
Conc: 368.04 ng/ml

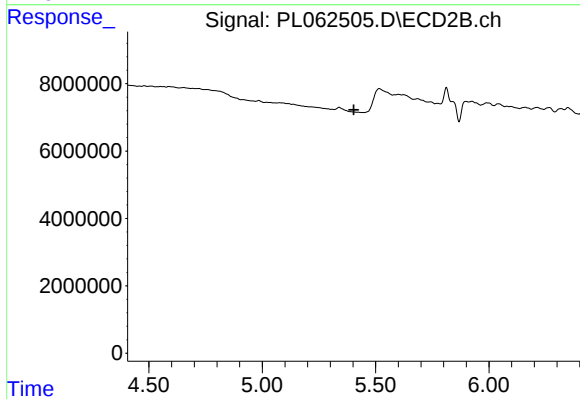

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.404 min
Response: 0
Conc: N.D.

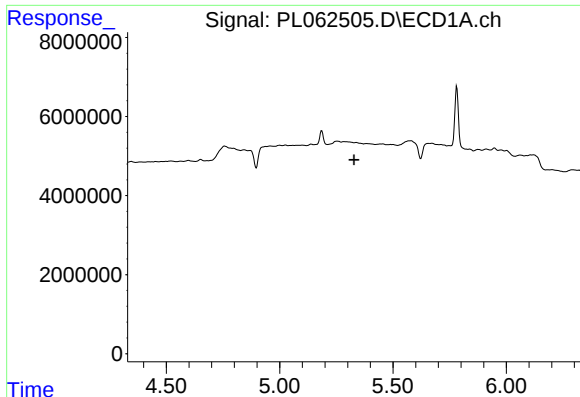

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

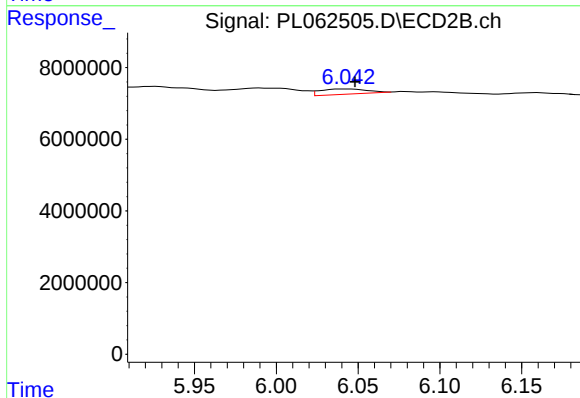


#25 Chlordane-3

R.T.: 6.040 min
Delta R.T.: -0.008 min
Response: 2903231
Conc: 7.19 ng/ml

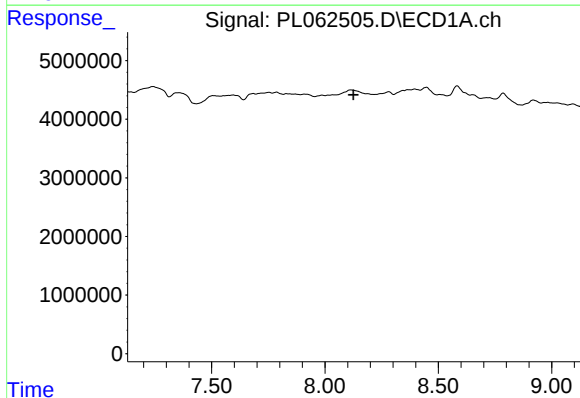

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.126 min
Response: 0
Conc: N.D.

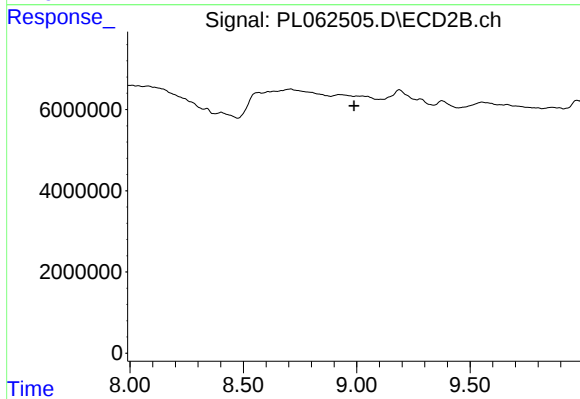

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.989 min
Response: 0
Conc: N.D.