

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102220\
 Data File : PL062514.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2020 13:09
 Operator : DD\AJ
 Sample : PB132579BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 15:34:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.950	34658069	58526264	20.149	19.916
28)	SA Decachlor...	8.127	8.988	29133454	38425464	18.160	18.359
Target Compounds							
23)	Chlordane-1	4.298f	0.000	250863	0	4.866	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102220\
Data File : PL062514.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2020 13:09
Operator : DD\AJ
Sample : PB132579BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 15:34:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

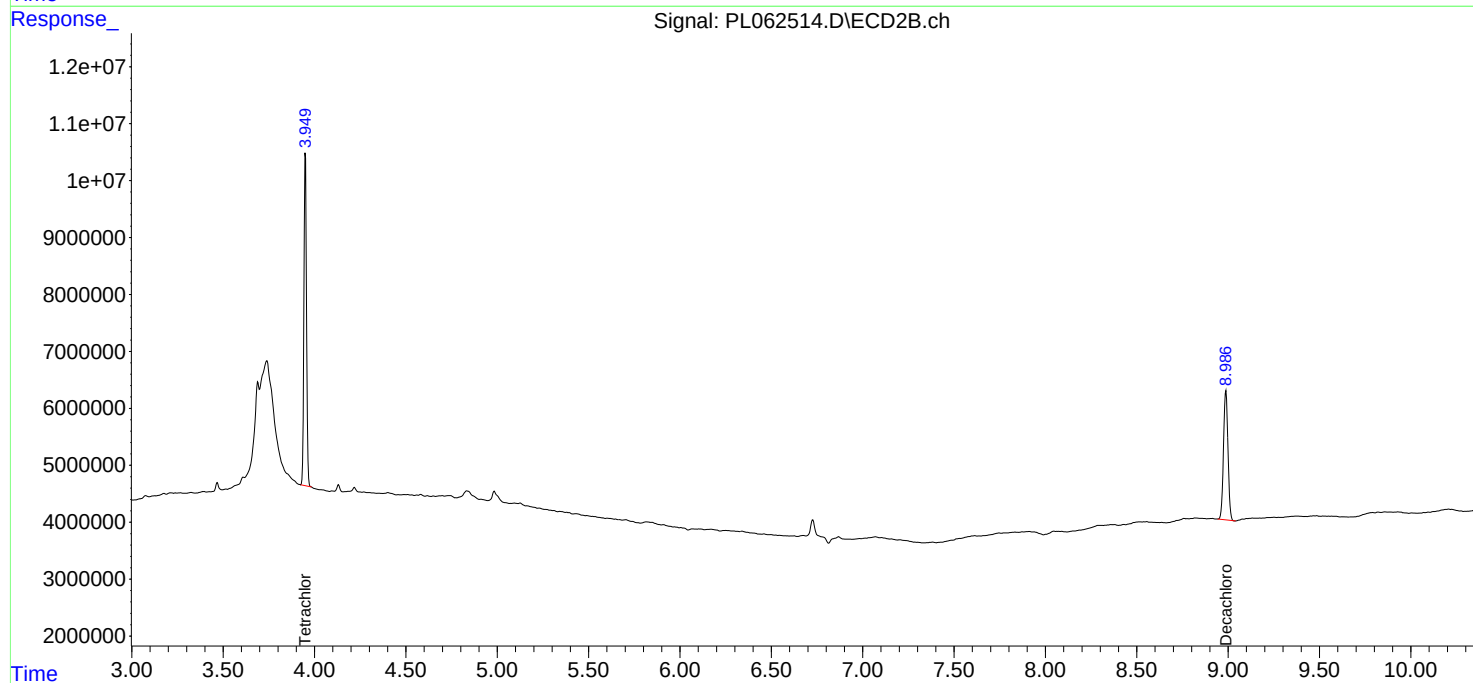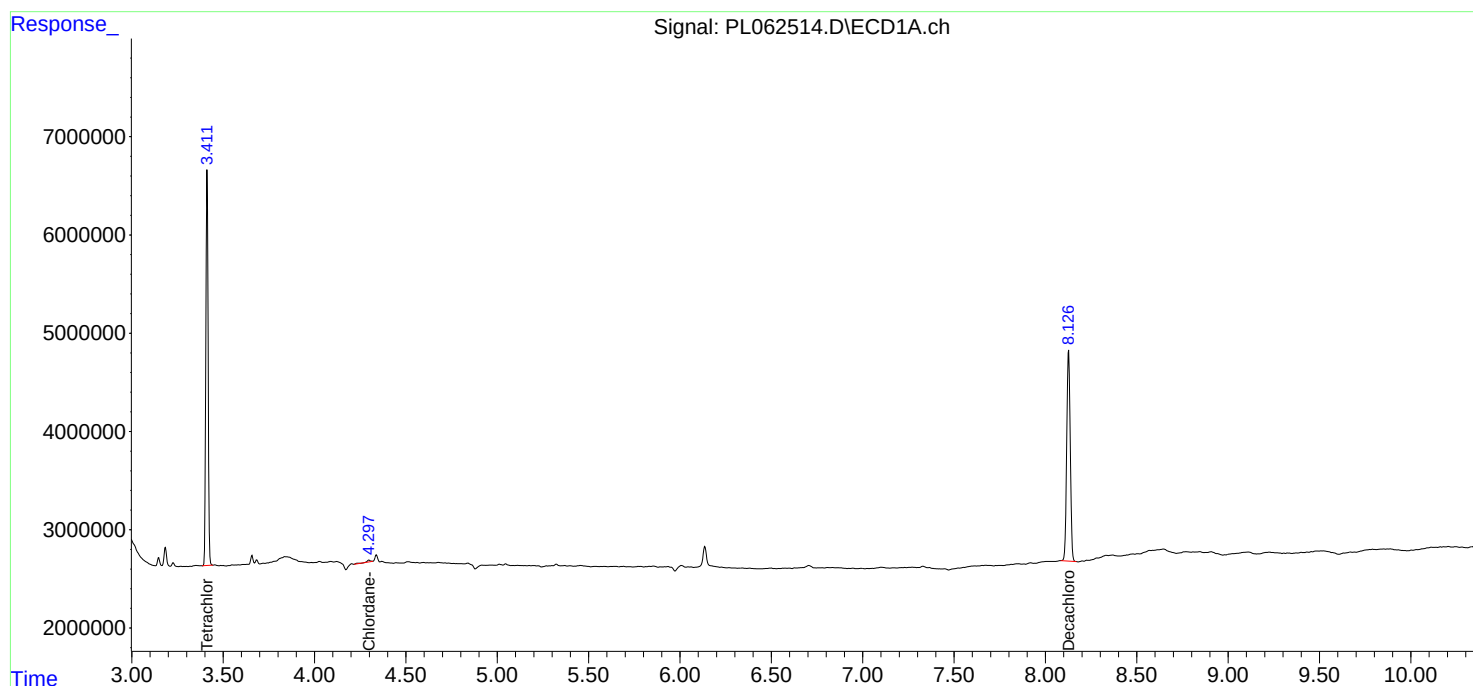


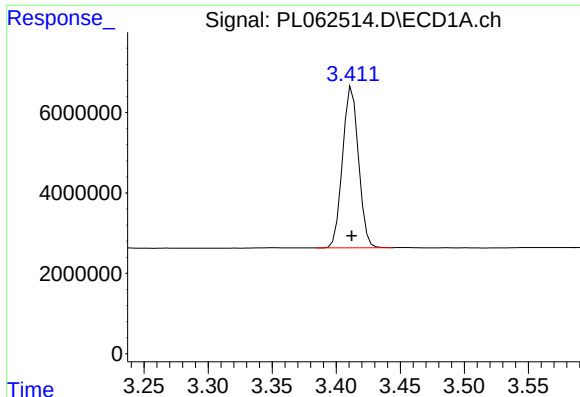

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 34658069
Conc: 20.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

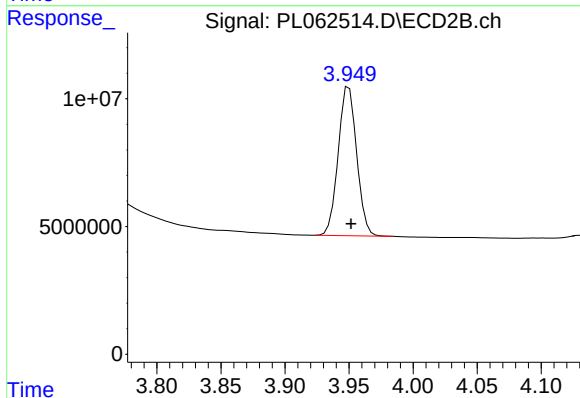


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 58526264
Conc: 19.92 ng/ml

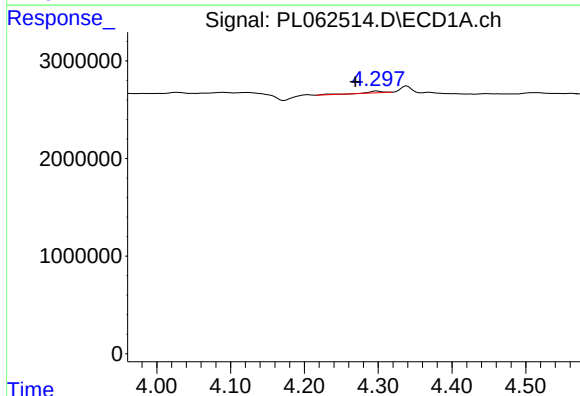


#23 Chlordane-1

R.T.: 4.298 min
Delta R.T.: 0.029 min
Response: 250863
Conc: 4.87 ng/ml

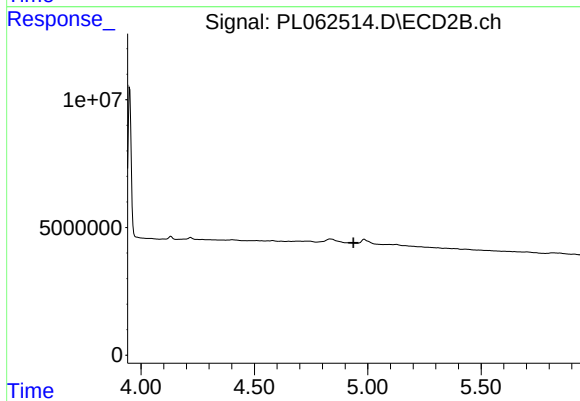

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.938 min
Response: 0
Conc: N.D.

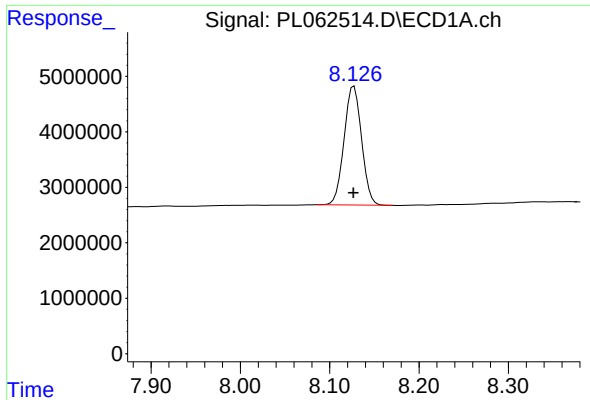

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 29133454
Conc: 18.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

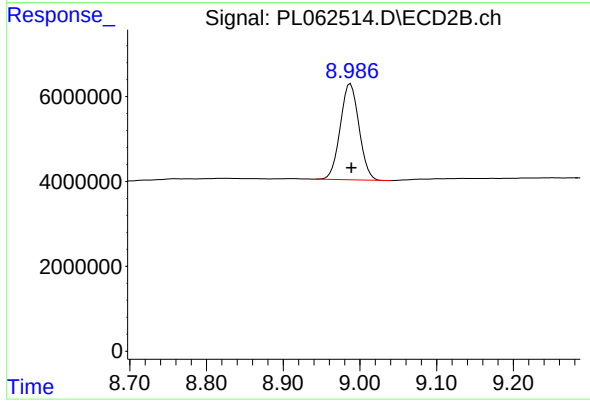

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: -0.001 min
Response: 38425464
Conc: 18.36 ng/ml