

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102220\
 Data File : PL062534.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2020 19:25
 Operator : DD\AJ
 Sample : L4484-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 04:51:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.413	3.952	33279359	58723807	19.348	19.983
28)	SA Decachlor...	8.127	8.990	32318177	44221007	20.145	21.128
Target Compounds							
2)	A alpha-BHC	0.000	4.309f	0	7096428	N.D.	1.597 #
3)	MA gamma-BHC...	4.128	0.000	950293	0	0.410	N.D. #
7)	B delta-BHC	0.000	4.983f	0	2609820	N.D.	0.746 #
8)	B Heptachlo...	5.114	0.000	2346474	0	1.286	N.D. #
9)	A Endosulfan I	5.460f	0.000	1588629	0	0.950	N.D. #
10)	B gamma-Chl...	0.000	6.032f	0	4826371	N.D.	1.434 #
13)	MA Dieldrin	5.651f	0.000	1840352	0	1.042	N.D. #
15)	B Endosulfa...	0.000	6.871f	0	4904639	N.D.	1.716 #
23)	Chlordane-1	4.276	0.000	801793	0	15.554	N.D. #
25)	Chlordane-3	0.000	6.032f	0	4826371	N.D.	11.948 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102220\
Data File : PL062534.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2020 19:25
Operator : DD\AJ
Sample : L4484-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 04:51:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

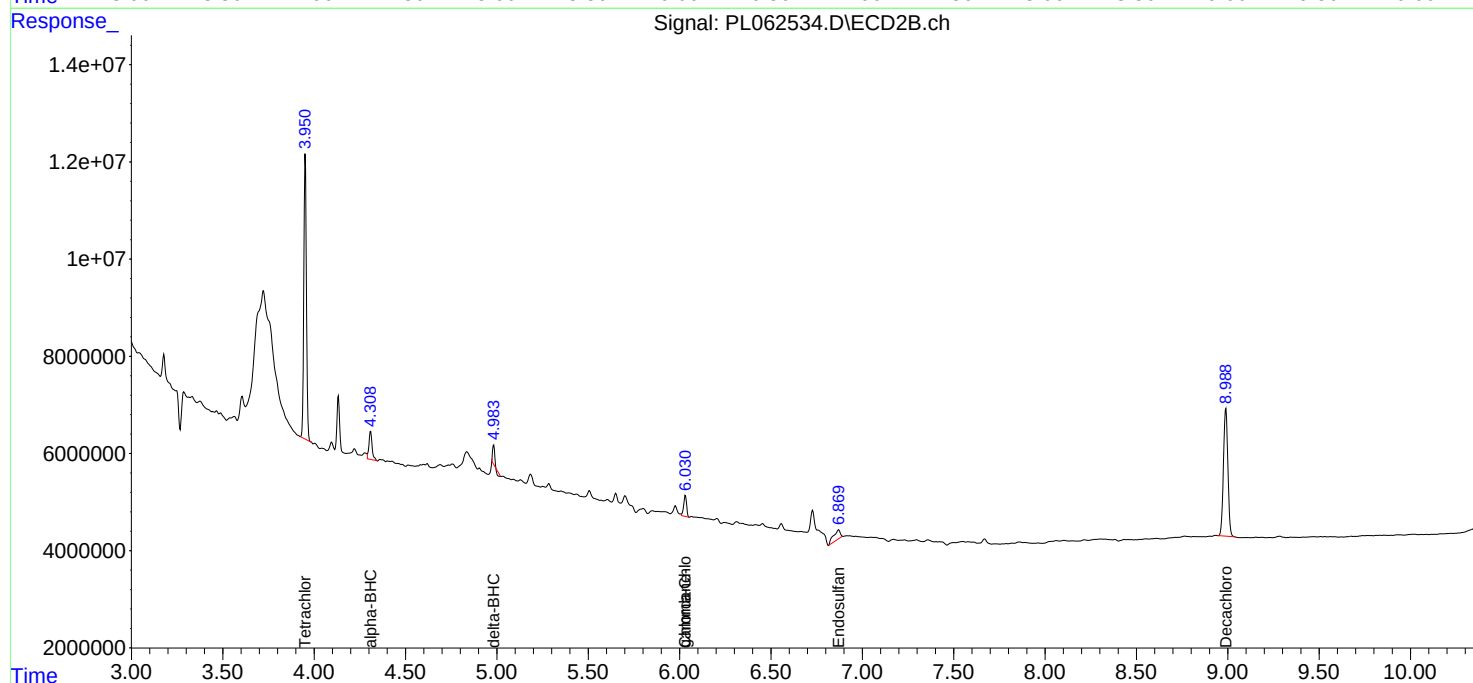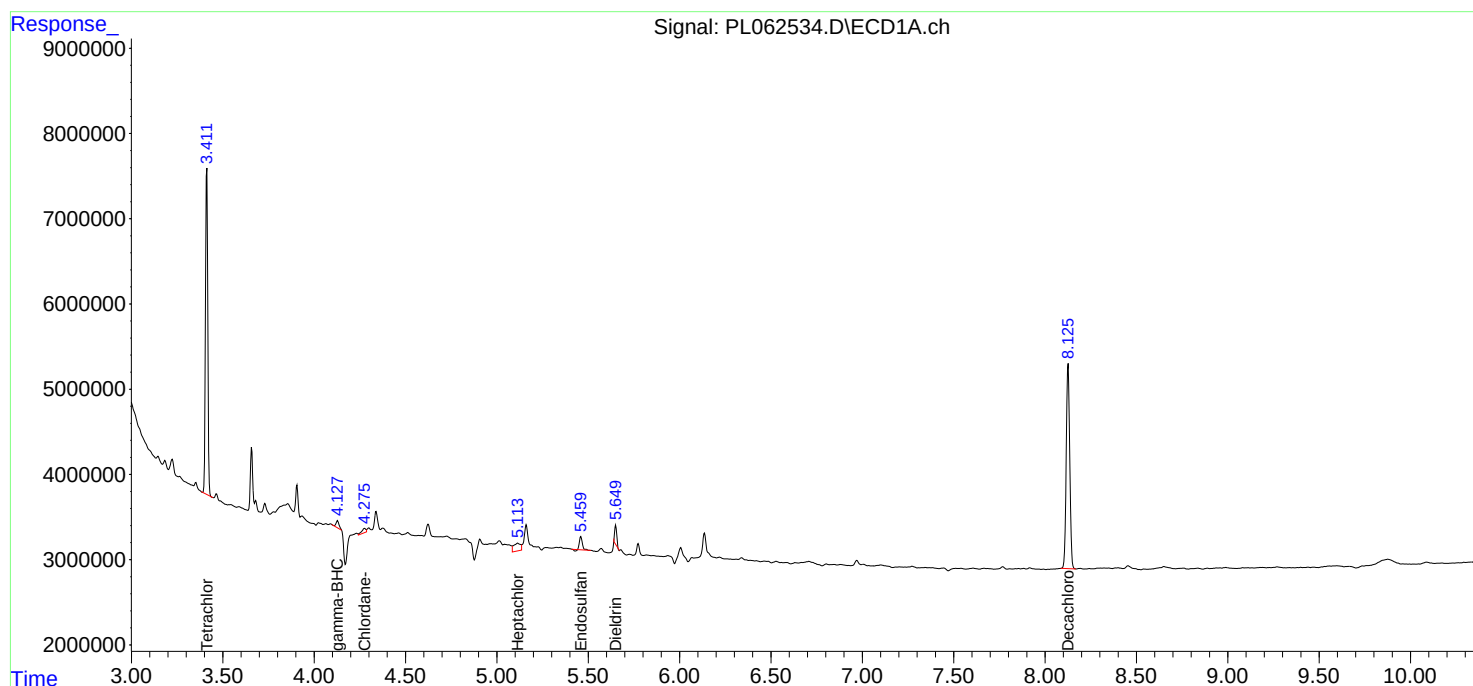


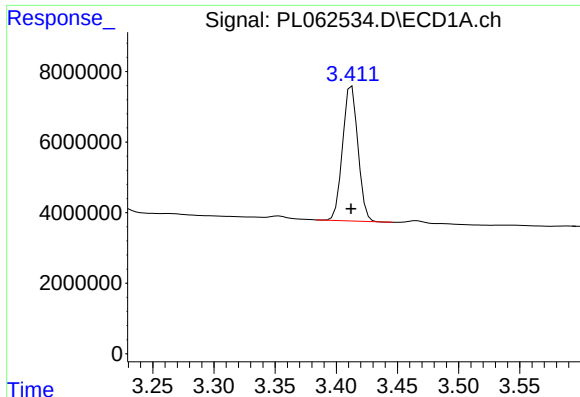

#1 Tetrachloro-m-xylene


R.T.: 3.413 min
Delta R.T.: 0.000 min
Response: 33279359
Conc: 19.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

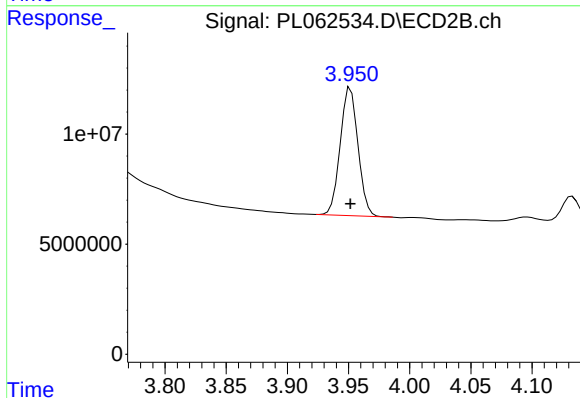


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 58723807
Conc: 19.98 ng/ml

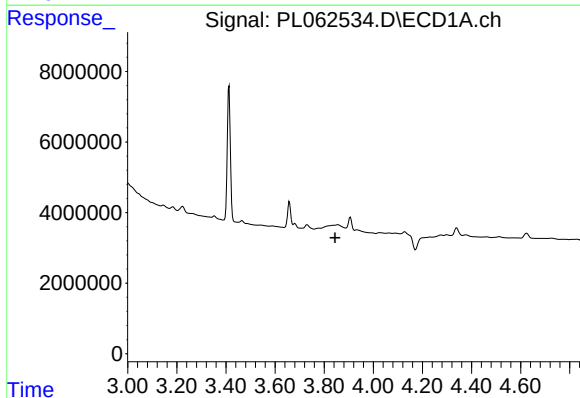


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.844 min
Response: 0
Conc: N.D.

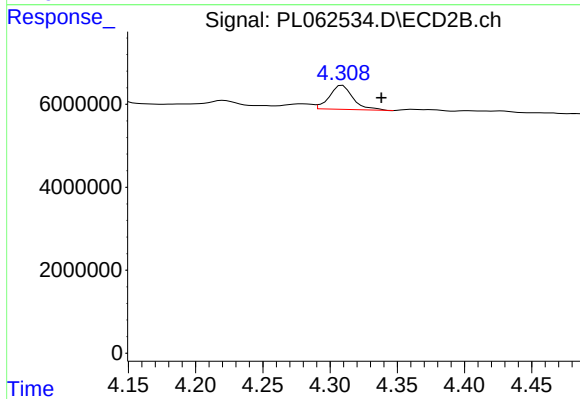

#2 alpha-BHC


R.T.: 4.309 min
Delta R.T.: -0.029 min
Response: 7096428
Conc: 1.60 ng/ml

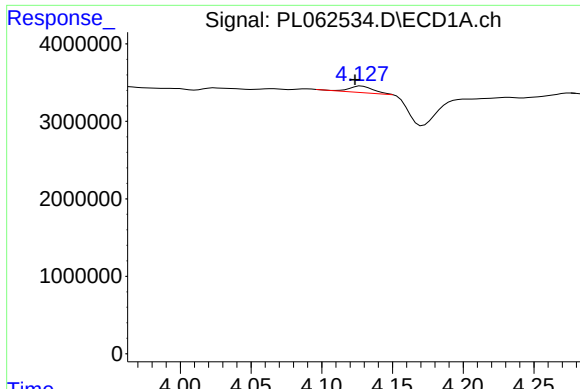

#3 gamma-BHC (Lindane)


R.T.: 4.128 min
Delta R.T.: 0.004 min
Response: 950293
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

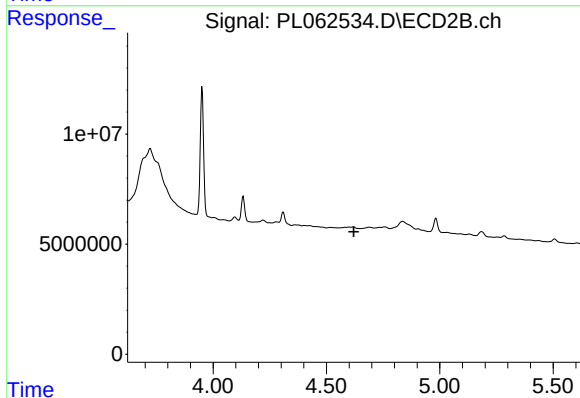


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.621 min
Response: 0
Conc: N.D.

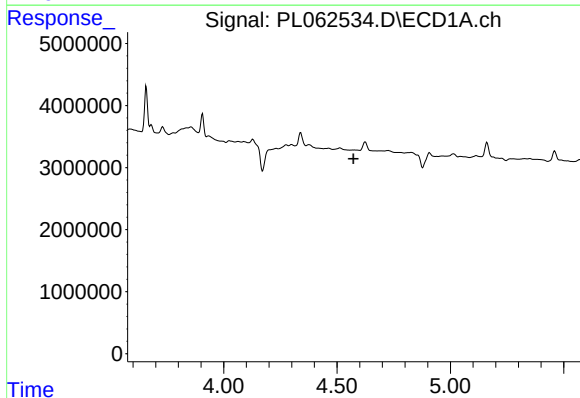


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

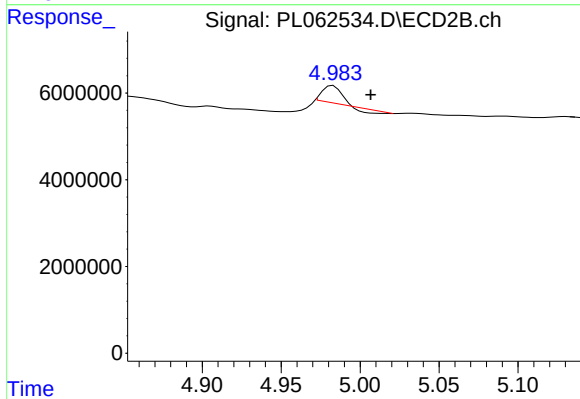

#7 delta-BHC


R.T.: 4.983 min
Delta R.T.: -0.024 min
Response: 2609820
Conc: 0.75 ng/ml

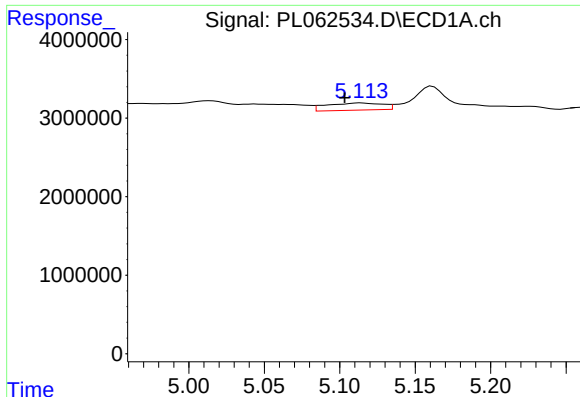

#8 Heptachlor epoxide


R.T.: 5.114 min
Delta R.T.: 0.011 min
Response: 2346474
Conc: 1.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

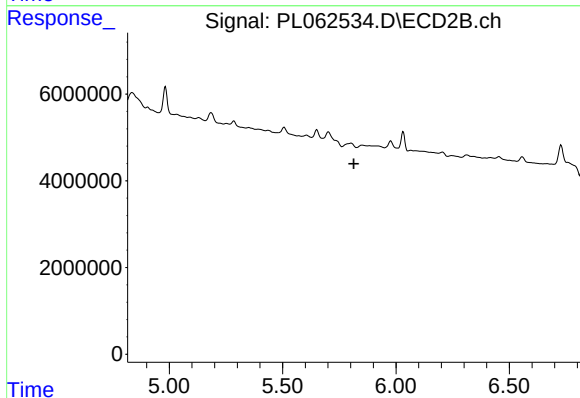


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.815 min
Response: 0
Conc: N.D.

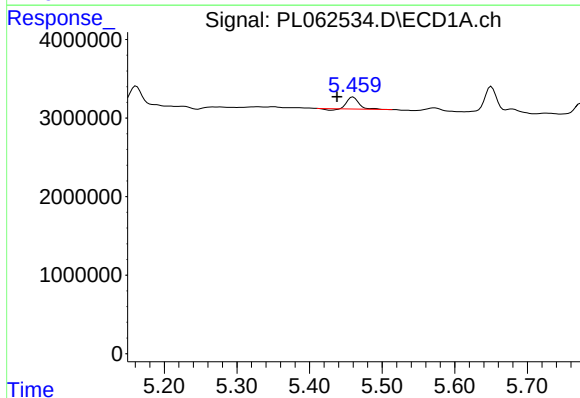


#9 Endosulfan I

R.T.: 5.460 min
Delta R.T.: 0.022 min
Response: 1588629
Conc: 0.95 ng/ml

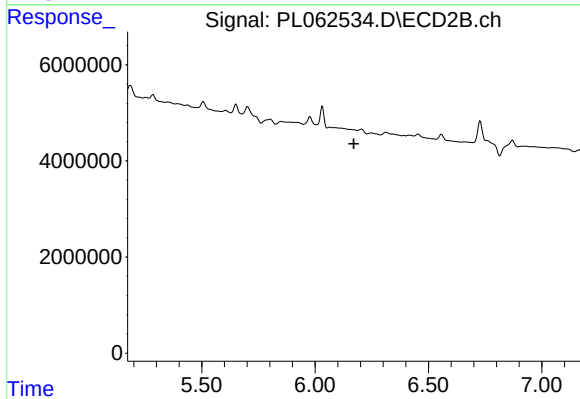

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

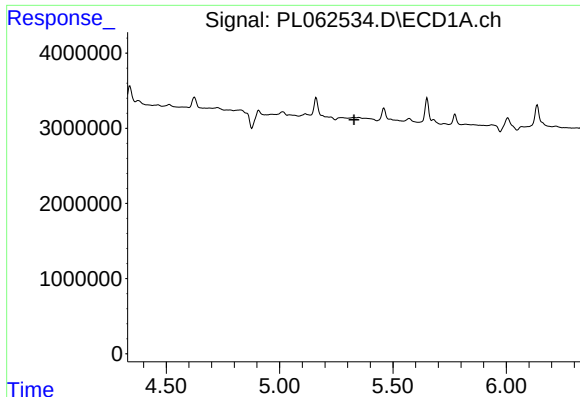

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

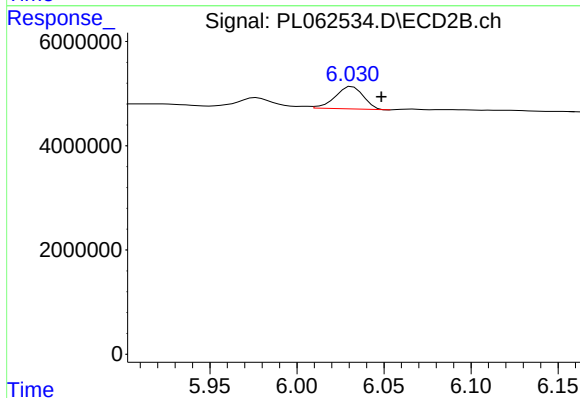


#10 gamma-Chlordane

R.T.: 6.032 min
Delta R.T.: -0.017 min
Response: 4826371
Conc: 1.43 ng/ml

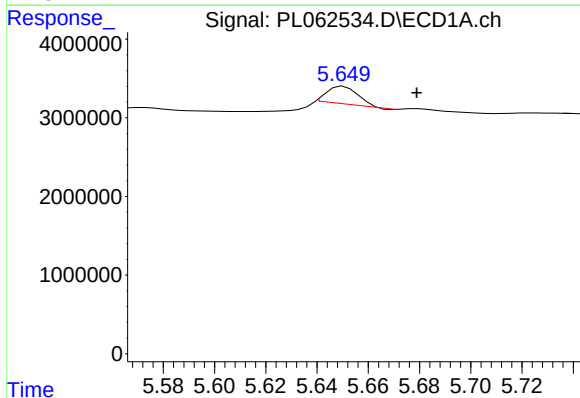


#13 Dieldrin

R.T.: 5.651 min
Delta R.T.: -0.028 min
Response: 1840352
Conc: 1.04 ng/ml

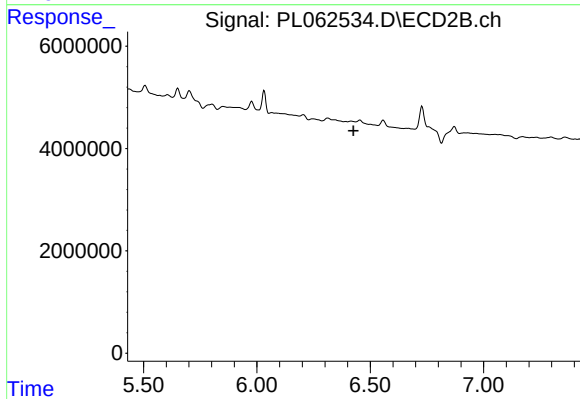

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.426 min
Response: 0
Conc: N.D.

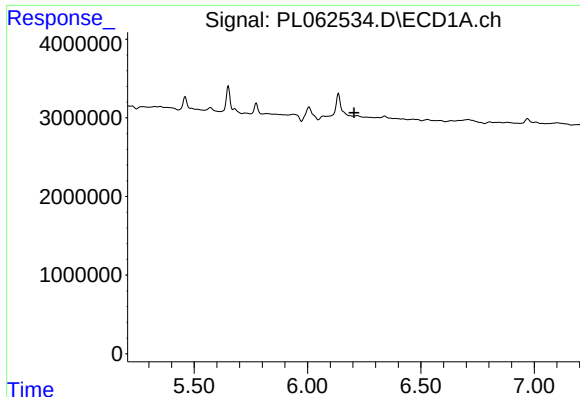

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

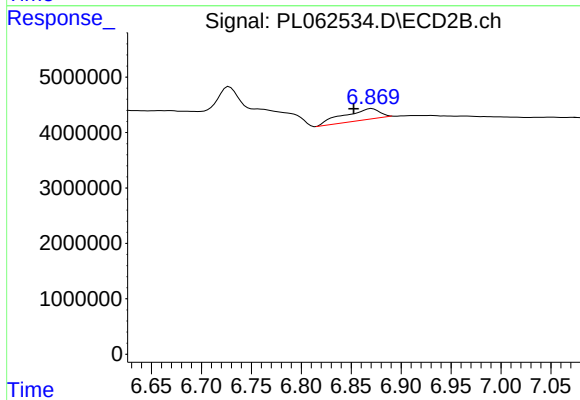


#15 Endosulfan II

R.T.: 6.871 min
Delta R.T.: 0.018 min
Response: 4904639
Conc: 1.72 ng/ml

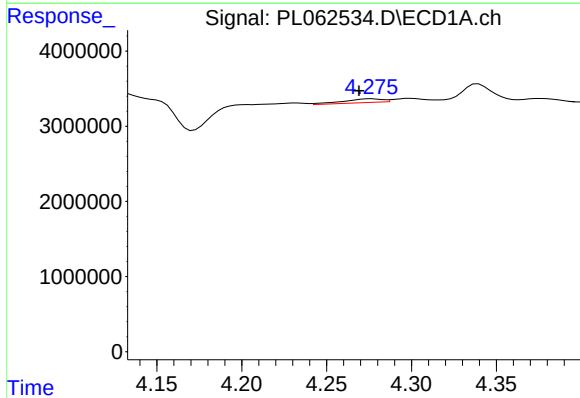


#23 Chlordane-1

R.T.: 4.276 min
Delta R.T.: 0.007 min
Response: 801793
Conc: 15.55 ng/ml

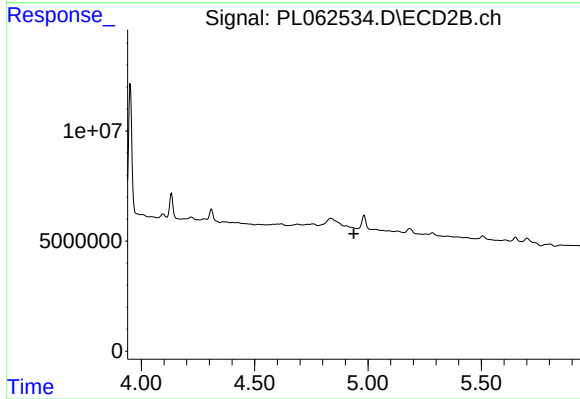

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.938 min
Response: 0
Conc: N.D.

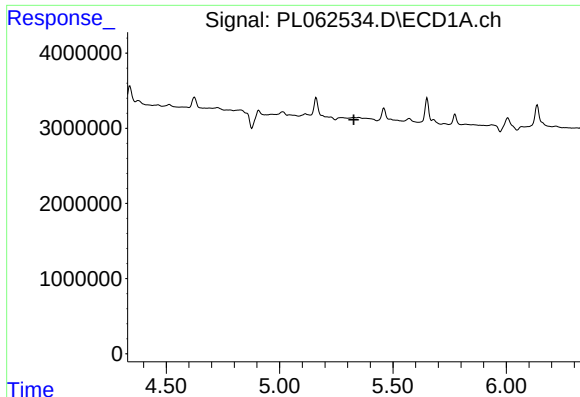

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

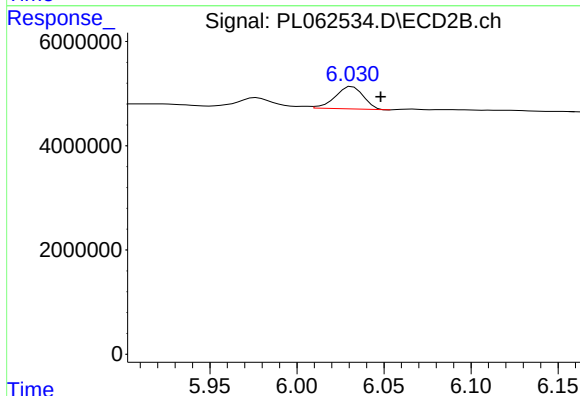


#25 Chlordane-3

R.T.: 6.032 min
Delta R.T.: -0.016 min
Response: 4826371
Conc: 11.95 ng/ml

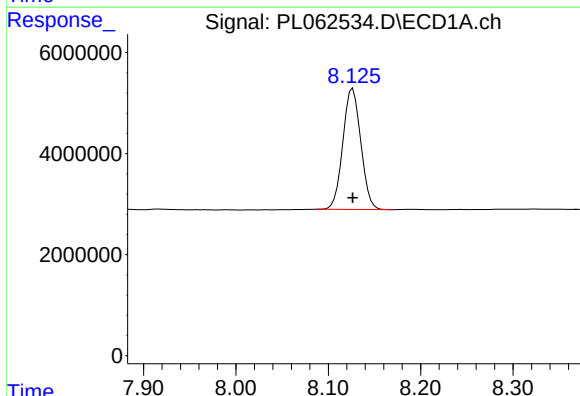

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 32318177
Conc: 20.14 ng/ml

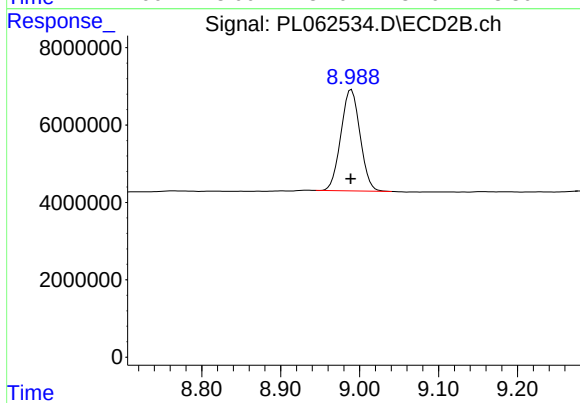

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 44221007
Conc: 21.13 ng/ml