

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102220\
 Data File : PL062535.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2020 19:39
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 04:51:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.413	3.952	39083863	67991045	22.722	23.136
28)	SA Decachlor...	8.126	8.989	34650920	47777773	21.599	22.828
Target Compounds							
8)	B Heptachlo...	0.000	5.810	0	8557447	N.D.	2.642 #
23)	Chlordane-1	4.299f	0.000	276810	0	5.370	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102220\
Data File : PL062535.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2020 19:39
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 04:51:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

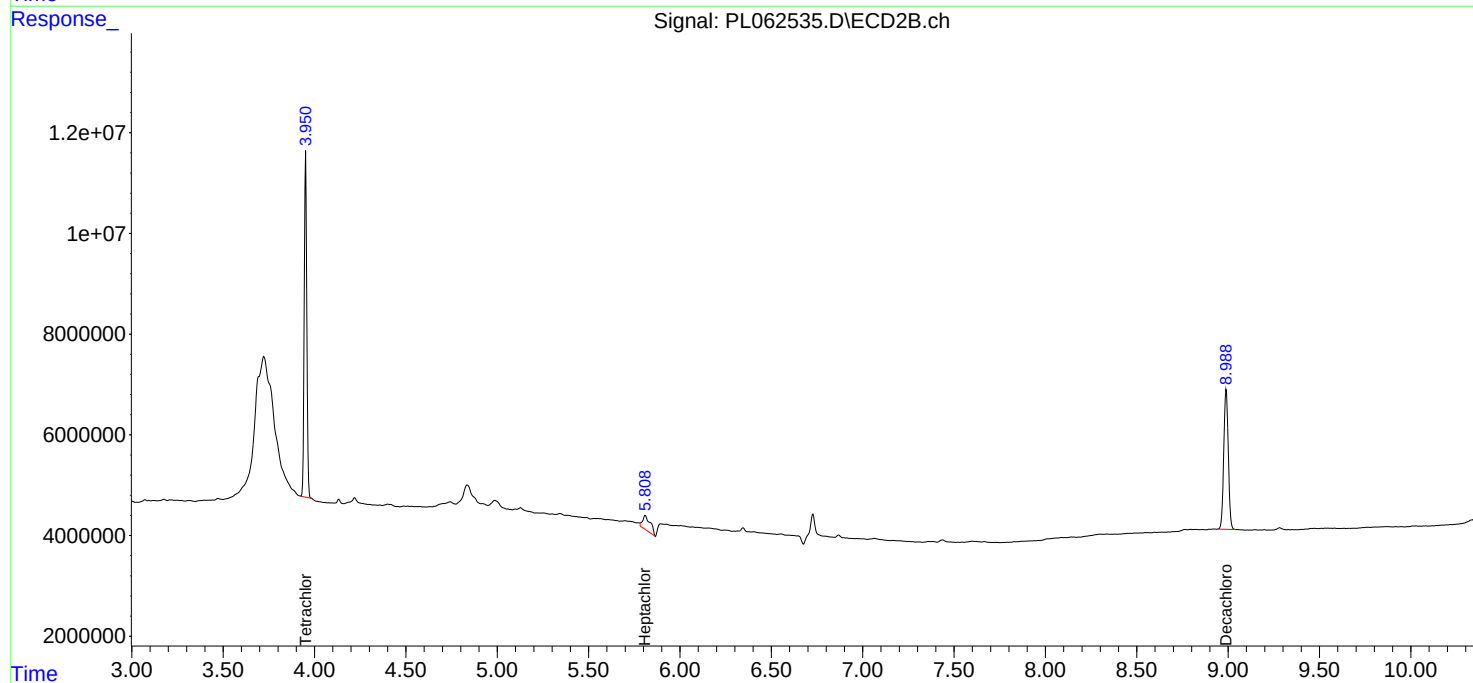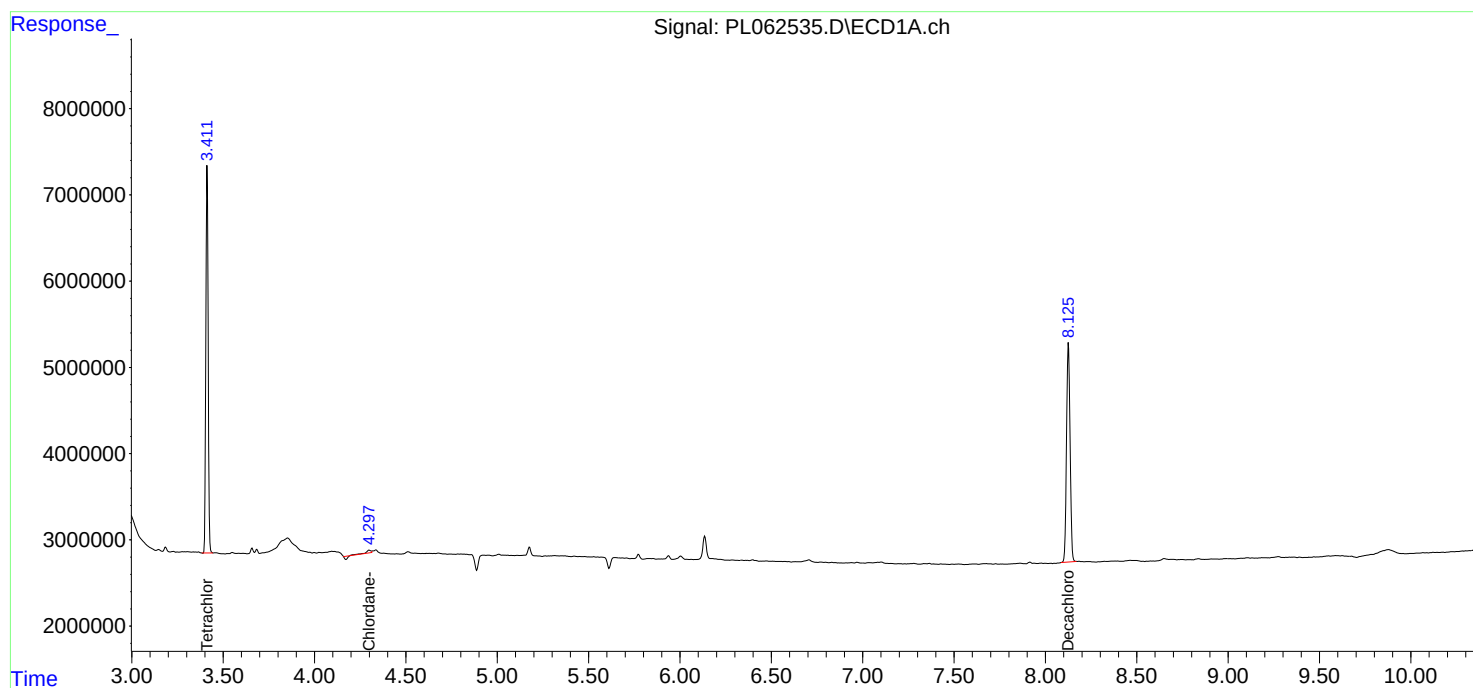


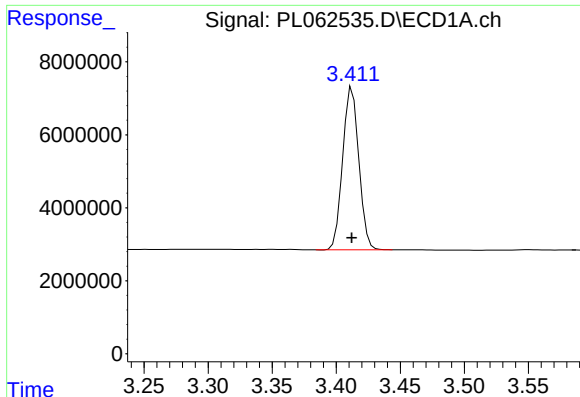

#1 Tetrachloro-m-xylene


R.T.: 3.413 min
Delta R.T.: 0.000 min
Response: 39083863
Conc: 22.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

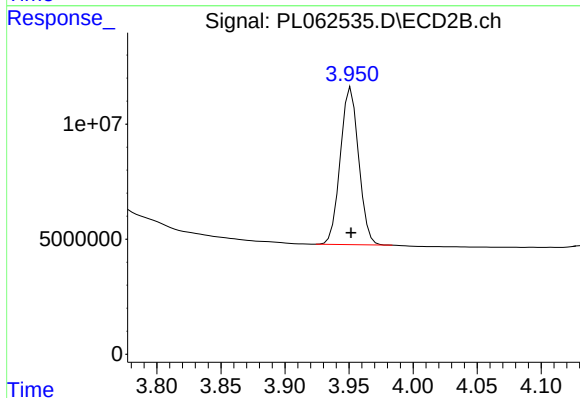


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 67991045
Conc: 23.14 ng/ml

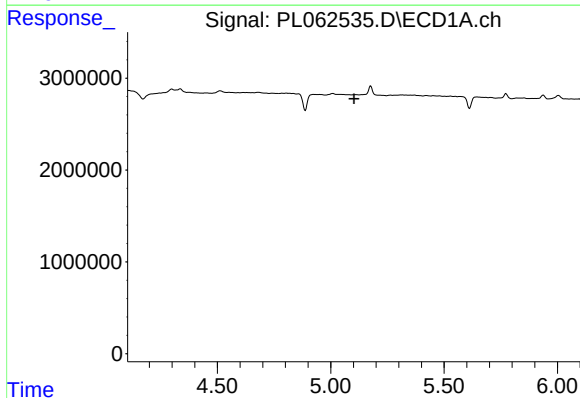


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.103 min
Response: 0
Conc: N.D.

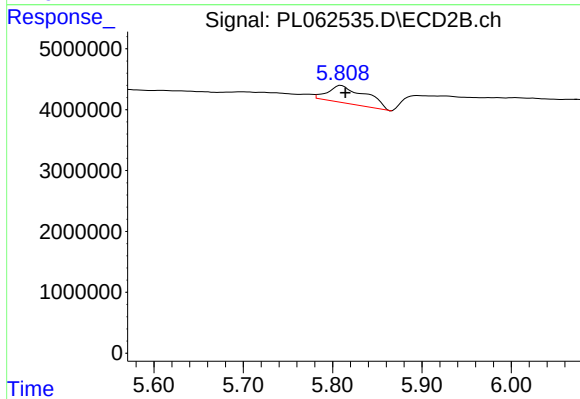

#8 Heptachlor epoxide


R.T.: 5.810 min
Delta R.T.: -0.005 min
Response: 8557447
Conc: 2.64 ng/ml

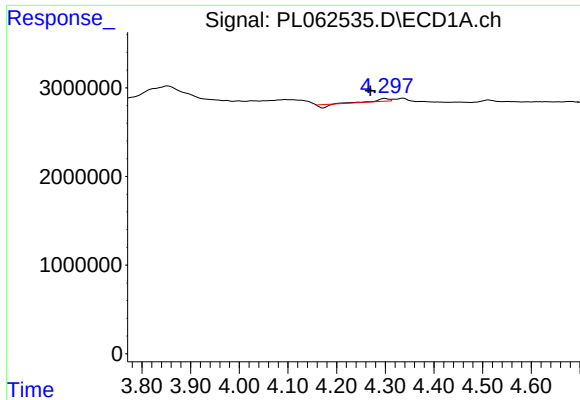

#23 Chlordane-1


R.T.: 4.299 min
Delta R.T.: 0.030 min
Response: 276810
Conc: 5.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

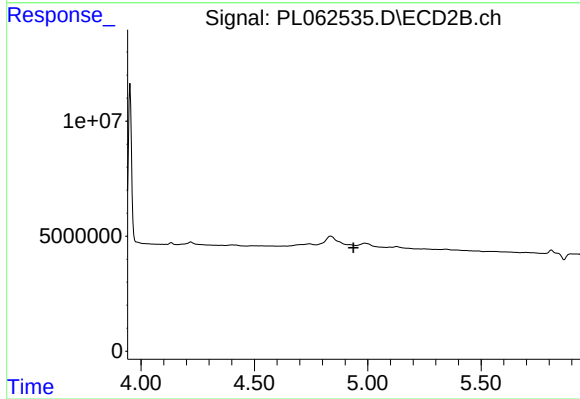


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

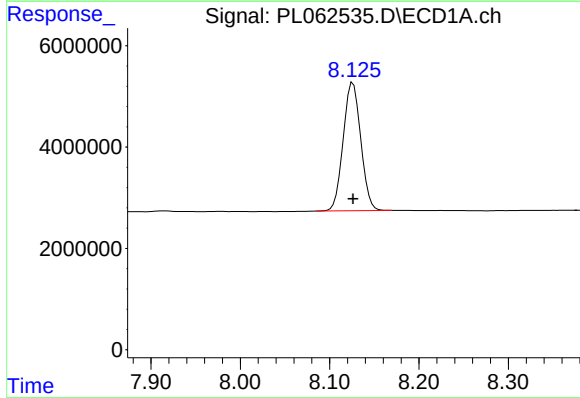

#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 34650920
Conc: 21.60 ng/ml

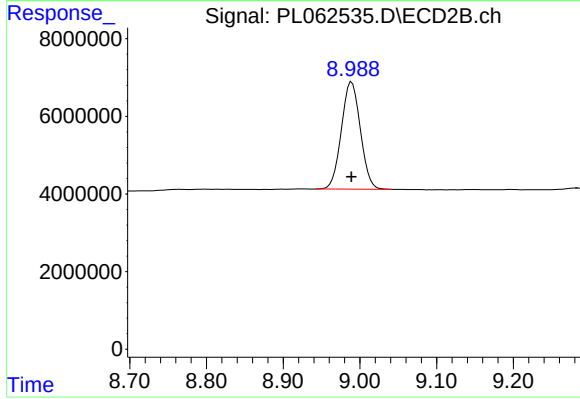

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 47777773
Conc: 22.83 ng/ml