

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102220\
 Data File : PL062518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2020 15:06
 Operator : DD\AJ
 Sample : L4484-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 72-11998

Manual Integrations
 APPROVED

Ankita
 10/23/2020 4:49:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 17:51:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.412	3.950	25716757	41187172	14.951	14.015
28) SA Decachlor...	8.127	8.988	20632952	26134978	12.861	12.487
Target Compounds						
11) B alpha-Chl...	5.384	6.121	967515	2574696	0.535m	0.764m#
14) MA Endrin	5.930	6.637	1337710	2718142	0.804m	0.974

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102220\
Data File : PL062518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2020 15:06
Operator : DD\AJ
Sample : L4484-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
72-11998


Manual Integrations
APPROVED

Ankita
10/23/2020 4:49:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 17:51:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

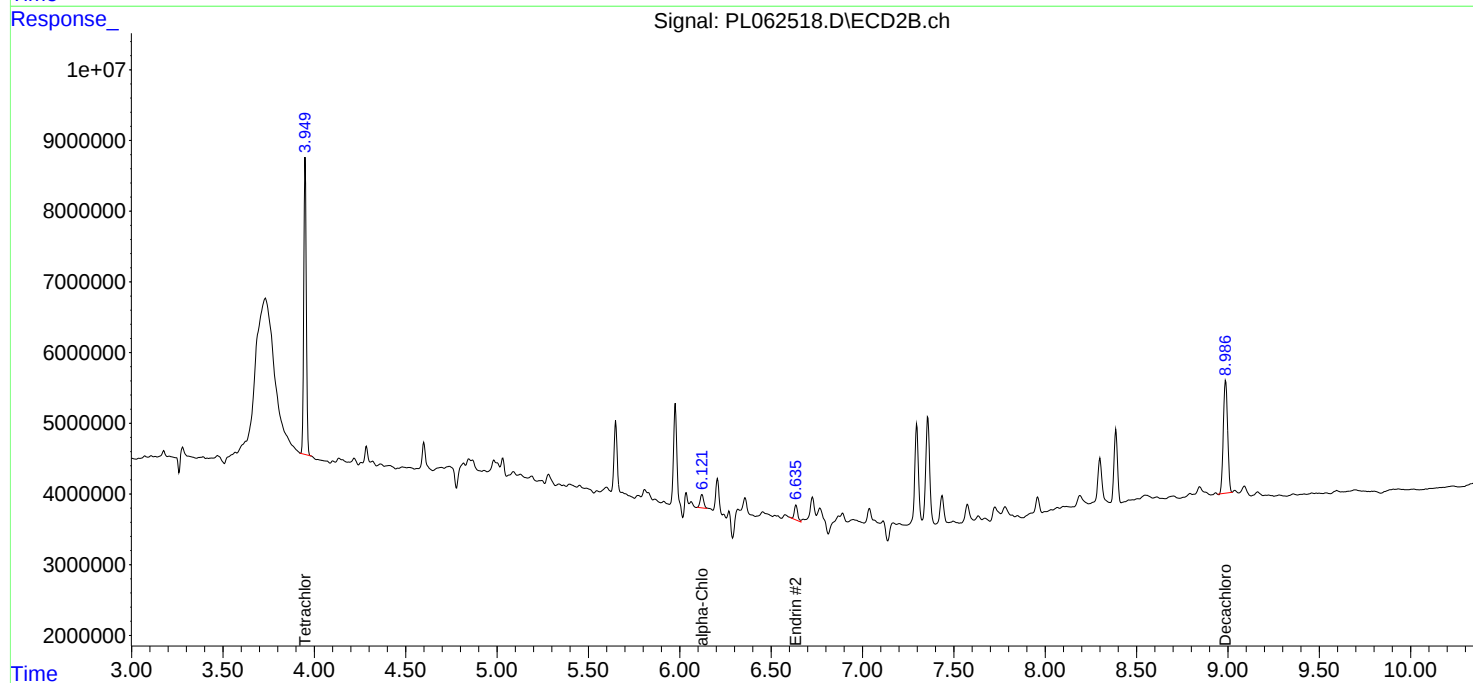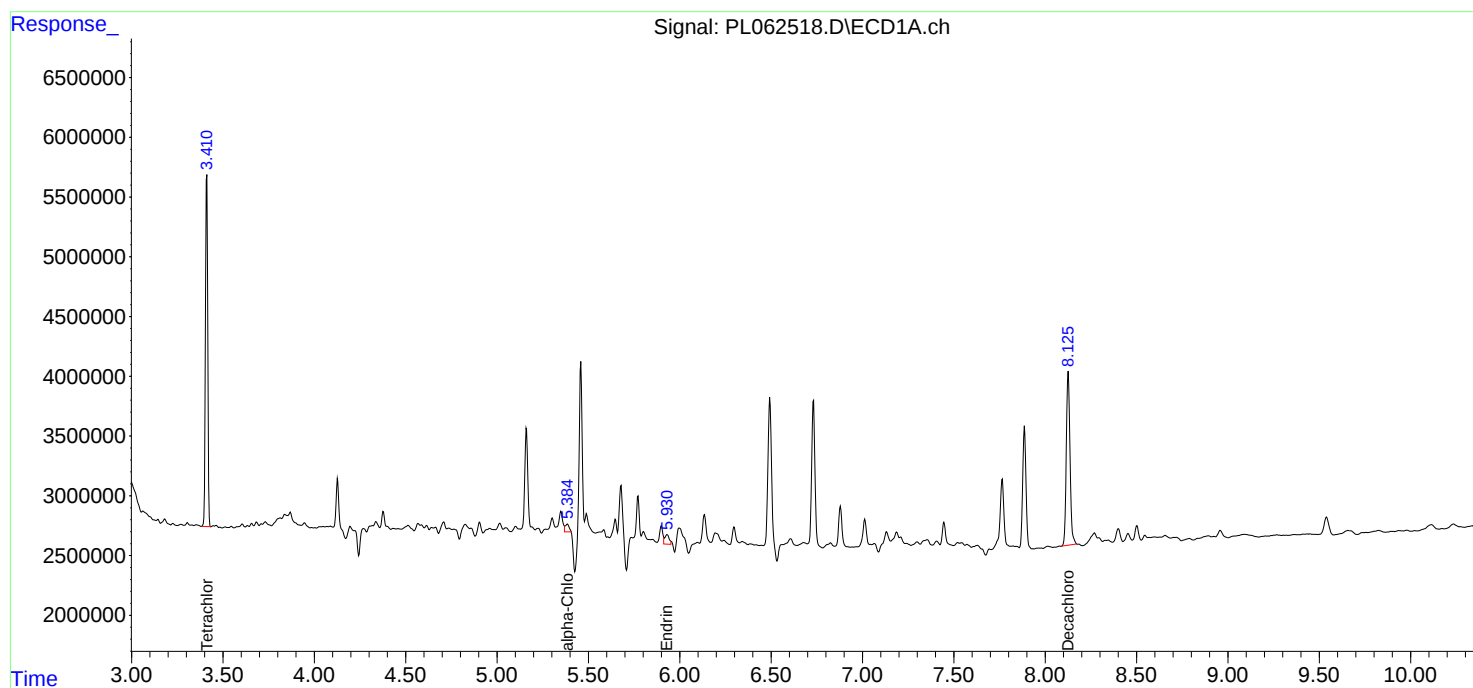

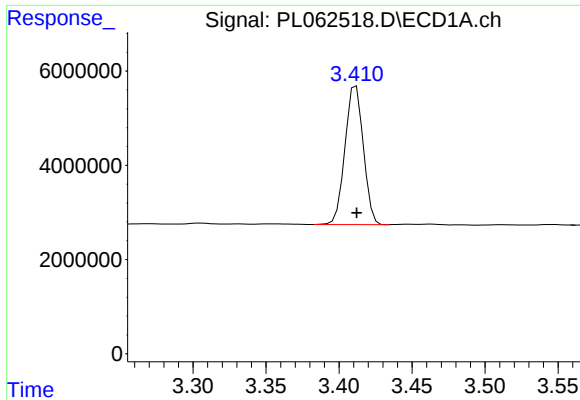


#1 Tetrachloro-m-xylene

R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 25716757
Conc: 14.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
72-11998


Manual Integrations
APPROVED

Ankita
10/23/2020 4:49:07 PM

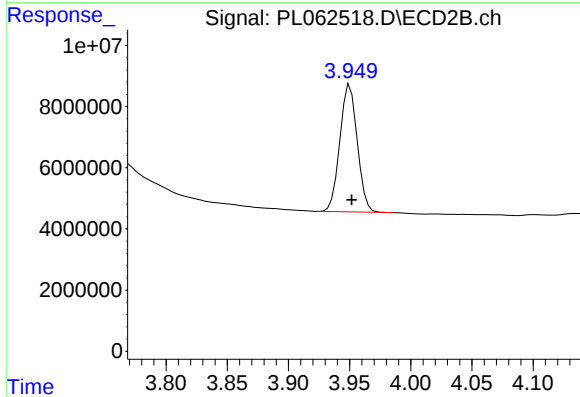


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.001 min
Response: 41187172
Conc: 14.02 ng/ml

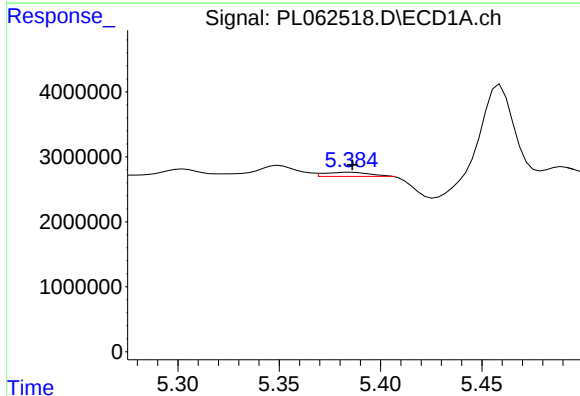


#11 alpha-Chlordane

R.T.: 5.384 min
Delta R.T.: -0.002 min
Response: 967515
Conc: 0.54 ng/ml m

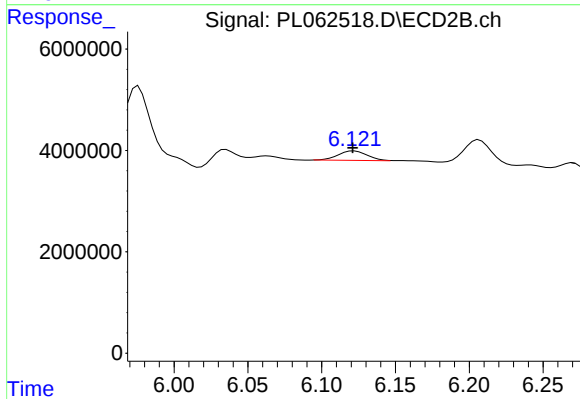

#11 alpha-Chlordane

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 2574696
Conc: 0.76 ng/ml m

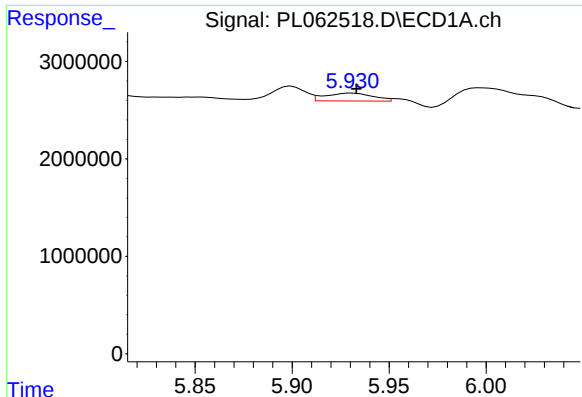


#14 Endrin

R.T.: 5.930 min
Delta R.T.: -0.003 min
Response: 1337710
Conc: 0.80 ng/ml m

Instrument :
ECD_L
ClientSampleId :
72-11998


Manual Integrations
APPROVED

Ankita
10/23/2020 4:49:07 PM

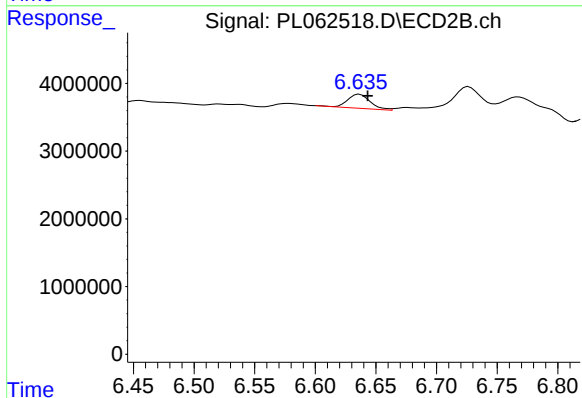


#14 Endrin

R.T.: 6.637 min
Delta R.T.: -0.007 min
Response: 2718142
Conc: 0.97 ng/ml

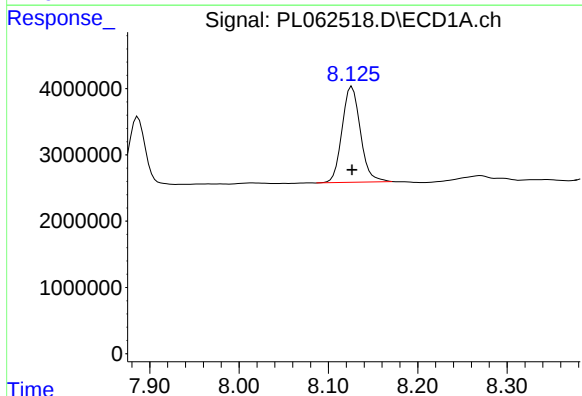

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 20632952
Conc: 12.86 ng/ml

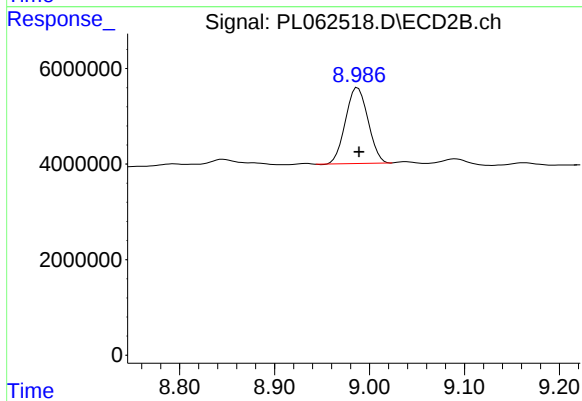

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: -0.001 min
Response: 26134978
Conc: 12.49 ng/ml