

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102222\
 Data File : PL078466.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2022 13:57
 Operator : AR\AJ
 Sample : N5218-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:55:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.322	2.572	38562170	54083174	20.221	21.183
2) SA Decachlor...	8.776	7.643	28377560	36386167	18.864	19.210
Target Compounds						
10) B gamma-Chl...	5.714	4.724	19612225	26087075	8.689	8.513
11) B alpha-Chl...	5.792	4.786	21418604	26186239	9.257	8.786



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102222\
Data File : PL078466.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2022 13:57
Operator : AR\AJ
Sample : N5218-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:55:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

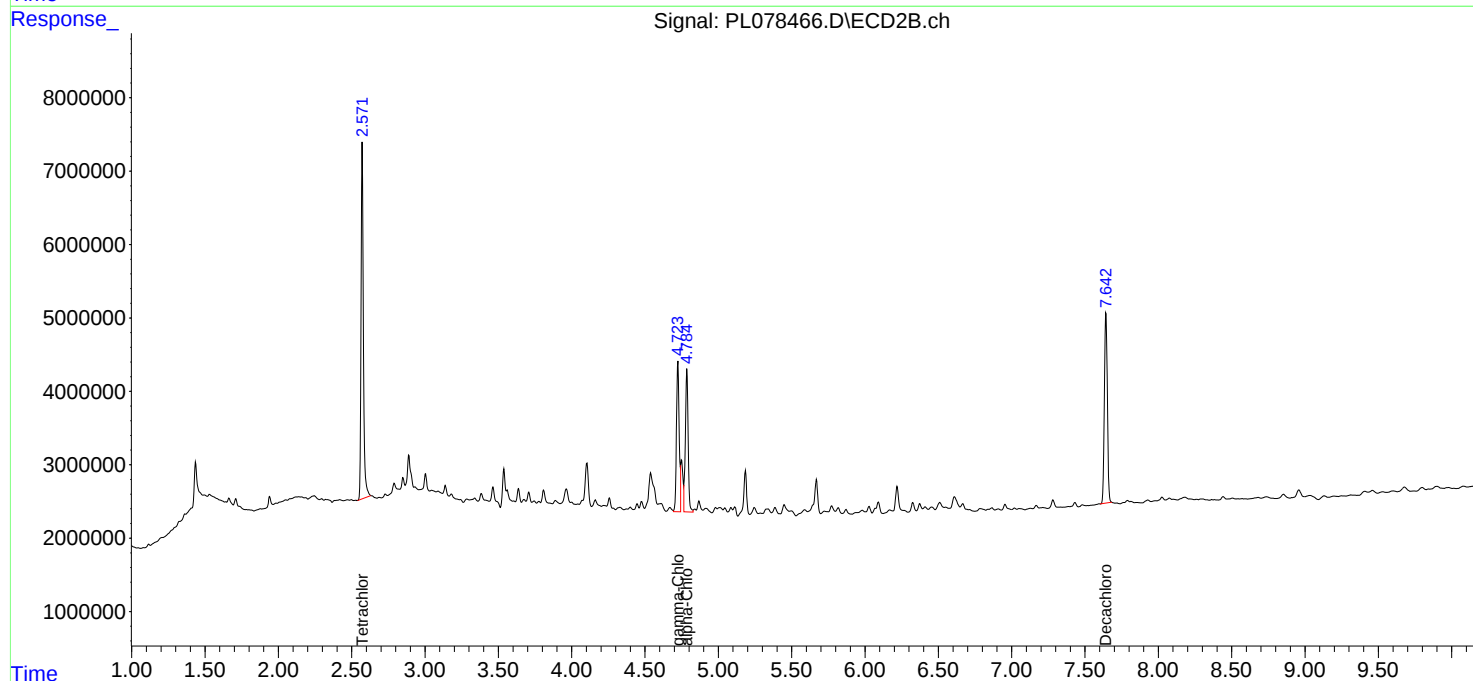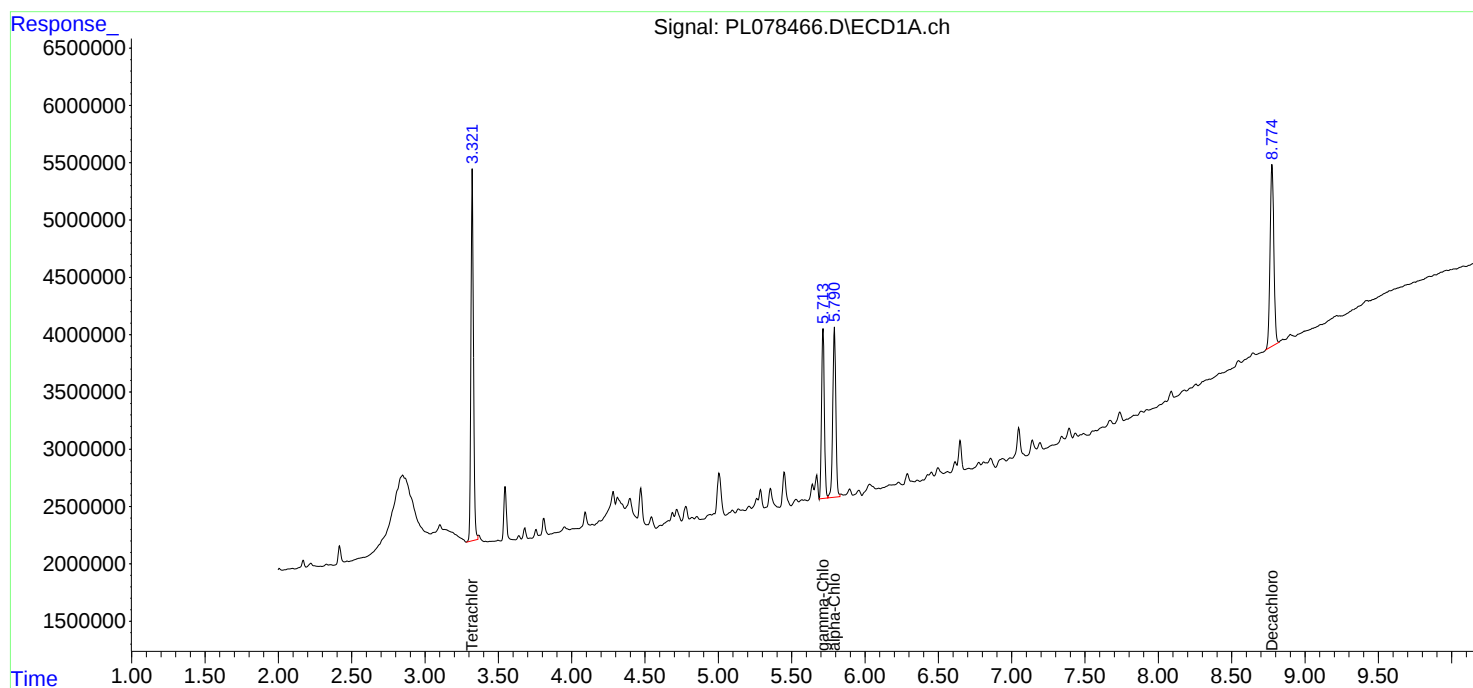


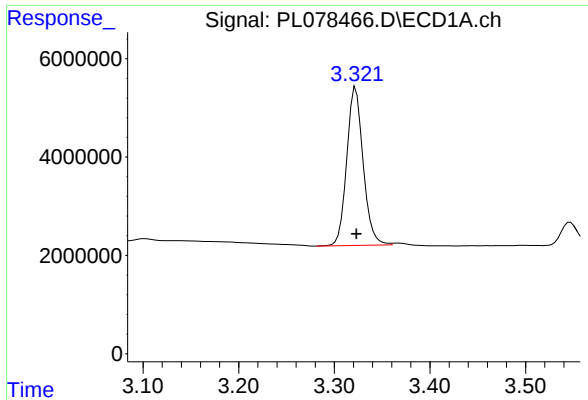

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: 0.000 min
Response: 38562170
Conc: 20.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-1

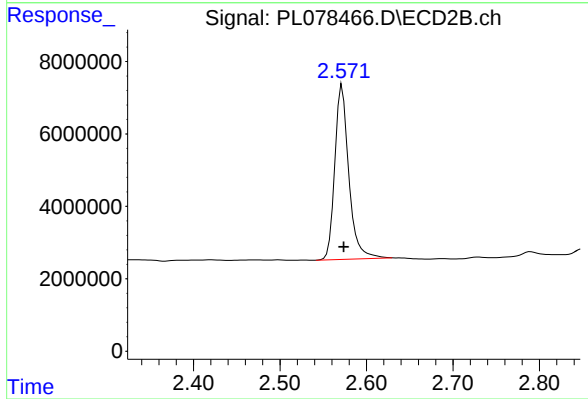


#1 Tetrachloro-m-xylene

R.T.: 2.572 min
Delta R.T.: -0.002 min
Response: 54083174
Conc: 21.18 ng/ml

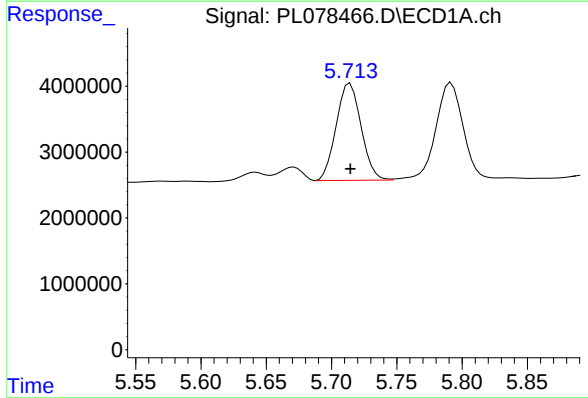


#10 gamma-Chlordane

R.T.: 5.714 min
Delta R.T.: 0.000 min
Response: 19612225
Conc: 8.69 ng/ml

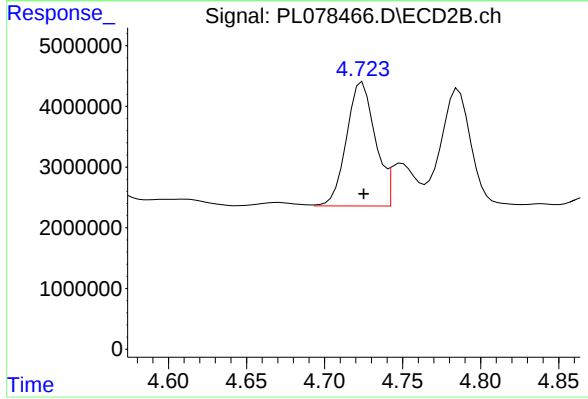

#10 gamma-Chlordane


R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 26087075
Conc: 8.51 ng/ml

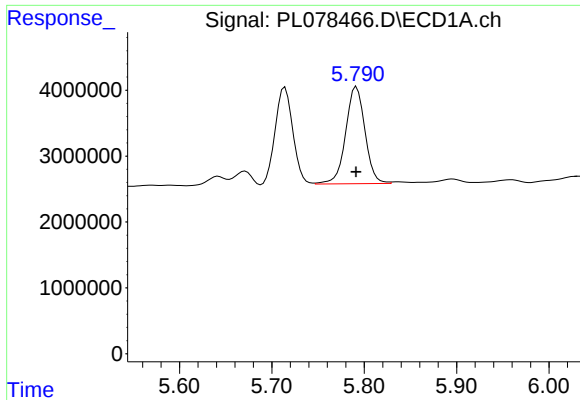

#11 alpha-Chlordane


R.T.: 5.792 min
Delta R.T.: 0.000 min
Response: 21418604
Conc: 9.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-1

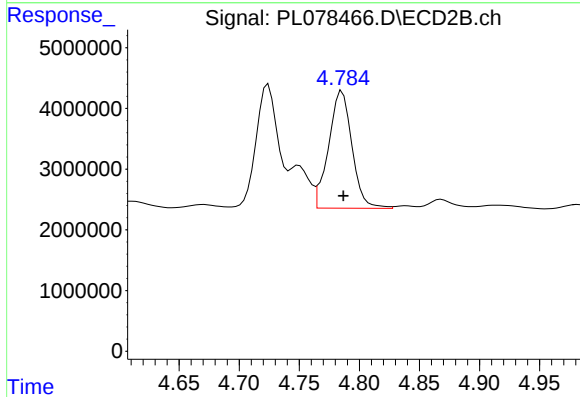


#11 alpha-Chlordane

R.T.: 4.786 min
Delta R.T.: -0.001 min
Response: 26186239
Conc: 8.79 ng/ml

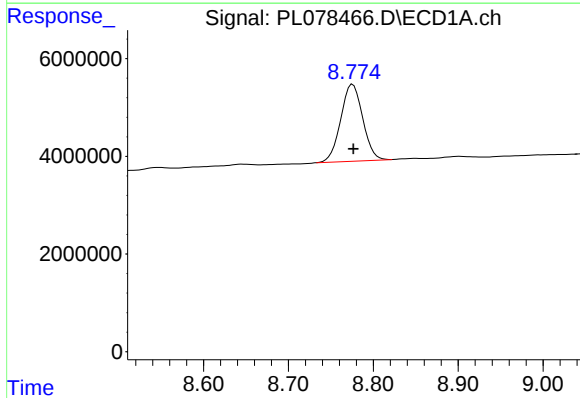

#28 Decachlorobiphenyl

R.T.: 8.776 min
Delta R.T.: 0.000 min
Response: 28377560
Conc: 18.86 ng/ml

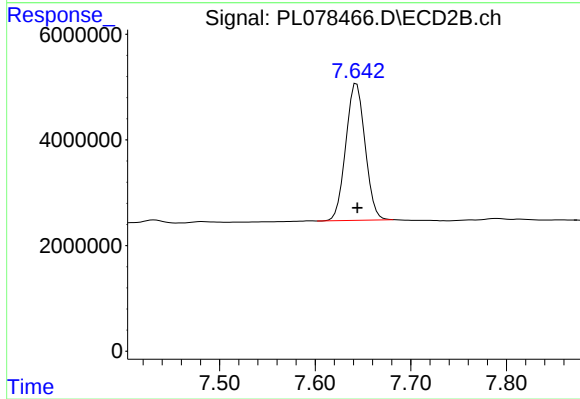

#28 Decachlorobiphenyl

R.T.: 7.643 min
Delta R.T.: -0.001 min
Response: 36386167
Conc: 19.21 ng/ml