

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102222\
 Data File : PL078468.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2022 14:24
 Operator : AR\AJ
 Sample : N5218-21
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:57:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	2.573	39659924	55290420	20.797	21.655
28)	SA Decachlor...	8.779	7.645	28979458	37305523	19.264	19.696
Target Compounds							
10)	B gamma-Chl...	5.716	4.725	3276854	4765003	1.452	1.555
11)	B alpha-Chl...	5.793	4.787	3396915	4462319	1.468	1.497



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102222\
Data File : PL078468.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2022 14:24
Operator : AR\AJ
Sample : N5218-21
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:57:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

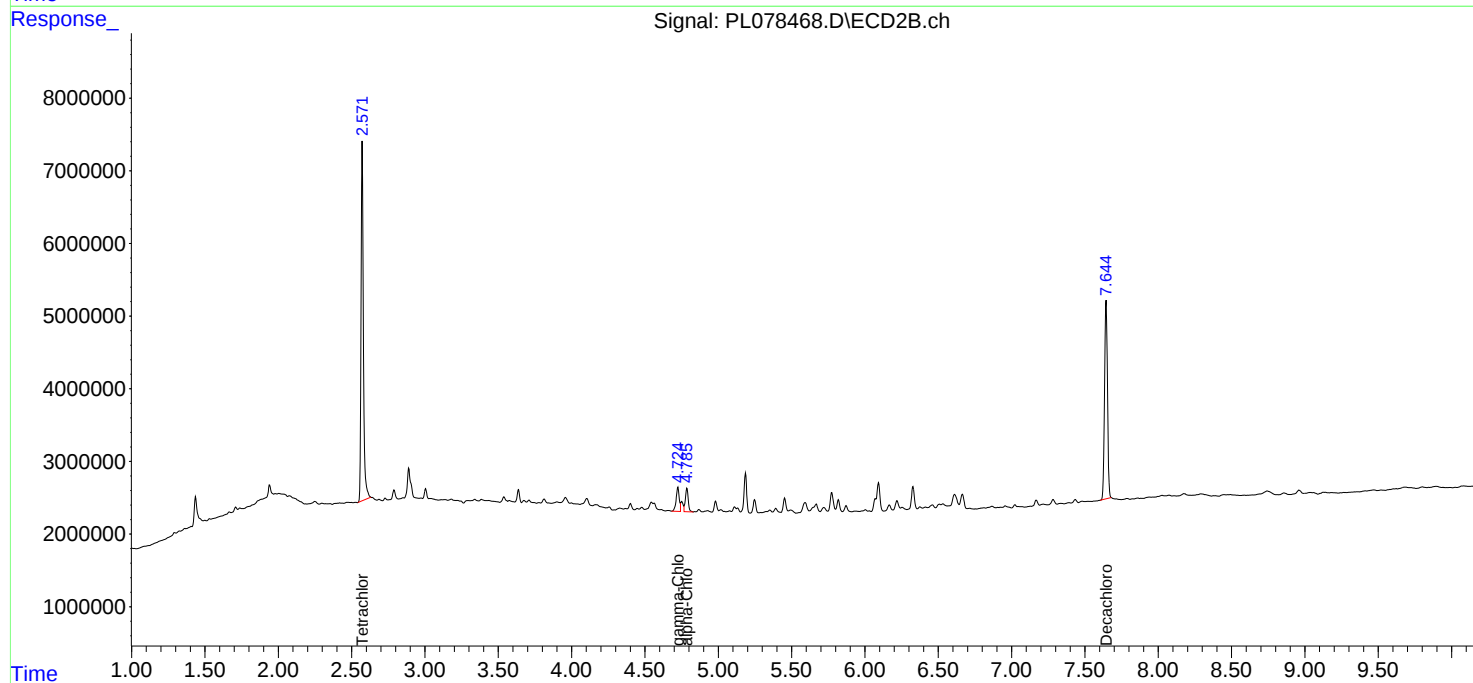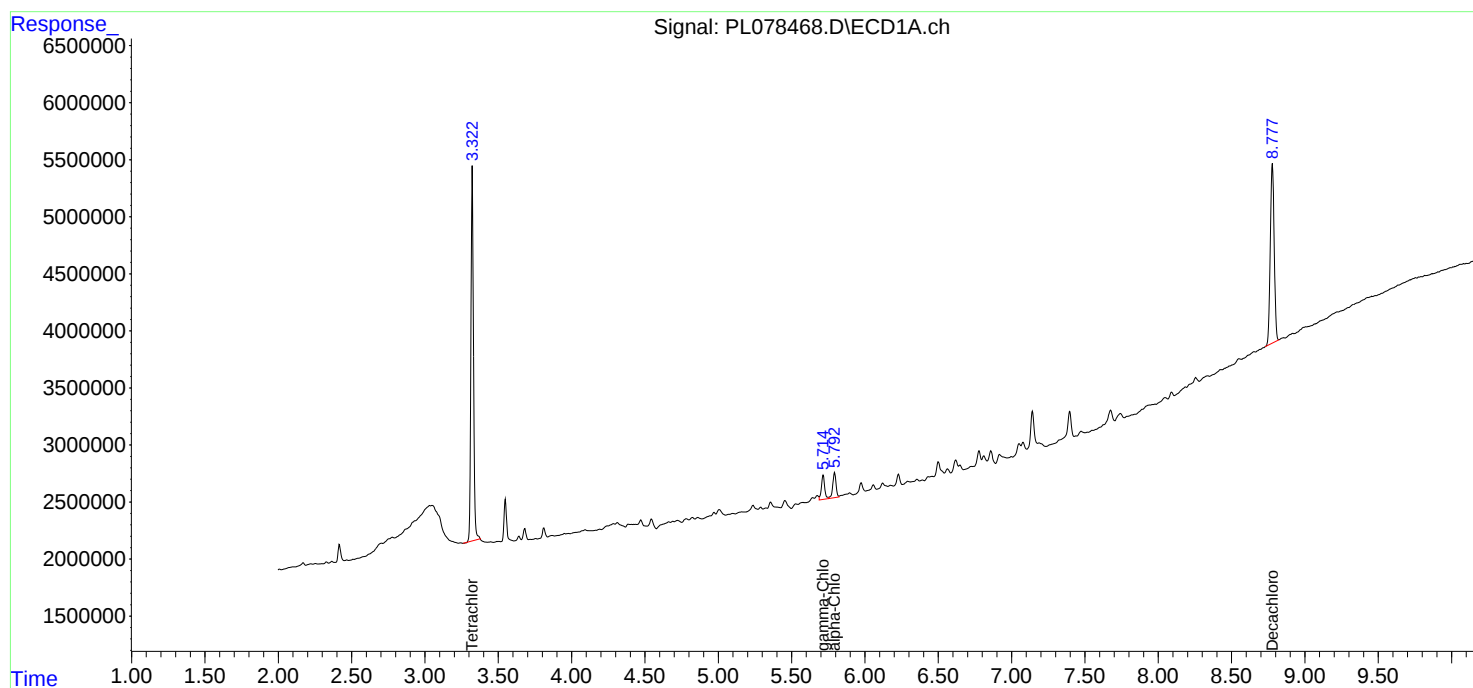


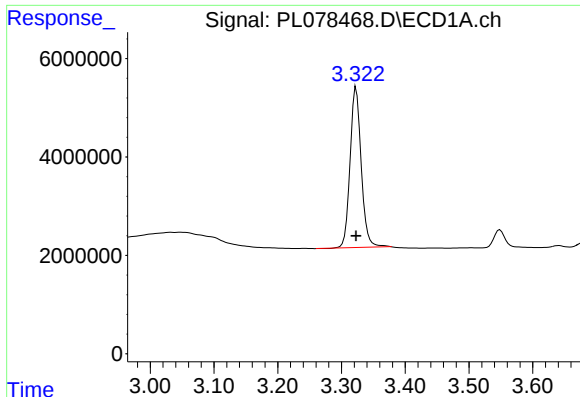

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 39659924
Conc: 20.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-3

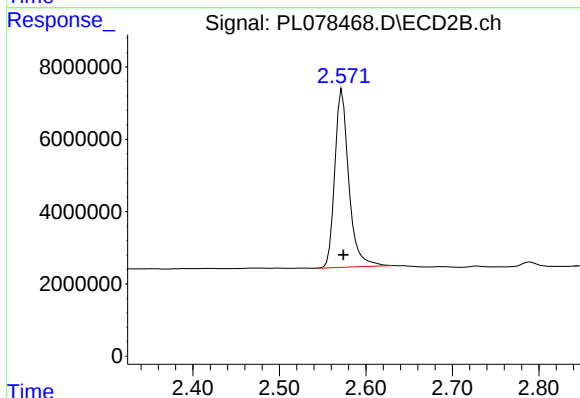


#1 Tetrachloro-m-xylene

R.T.: 2.573 min
Delta R.T.: -0.001 min
Response: 55290420
Conc: 21.66 ng/ml

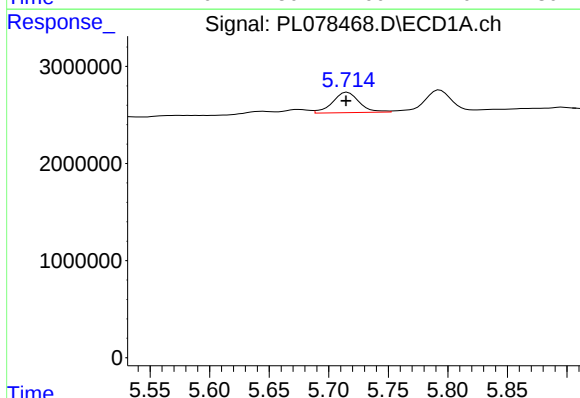


#10 gamma-Chlordane

R.T.: 5.716 min
Delta R.T.: 0.001 min
Response: 3276854
Conc: 1.45 ng/ml

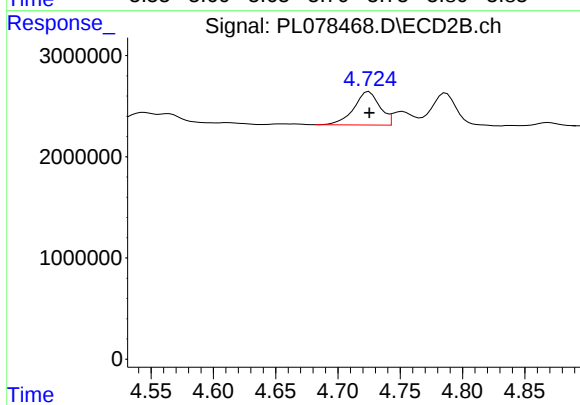

#10 gamma-Chlordane


R.T.: 4.725 min
Delta R.T.: 0.000 min
Response: 4765003
Conc: 1.55 ng/ml

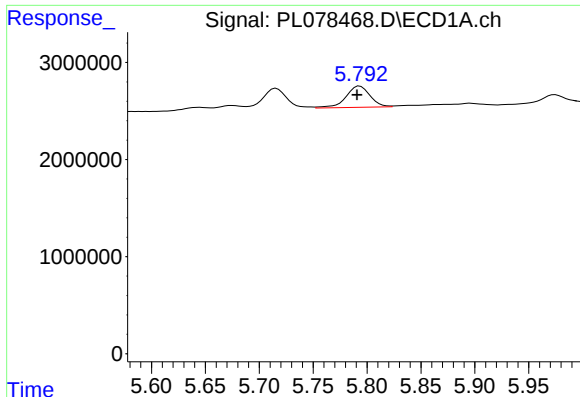

#11 alpha-Chlordane


R.T.: 5.793 min
Delta R.T.: 0.002 min
Response: 3396915
Conc: 1.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-3

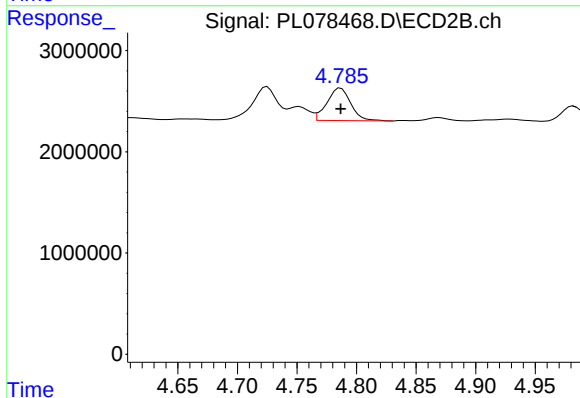


#11 alpha-Chlordane

R.T.: 4.787 min
Delta R.T.: 0.000 min
Response: 4462319
Conc: 1.50 ng/ml

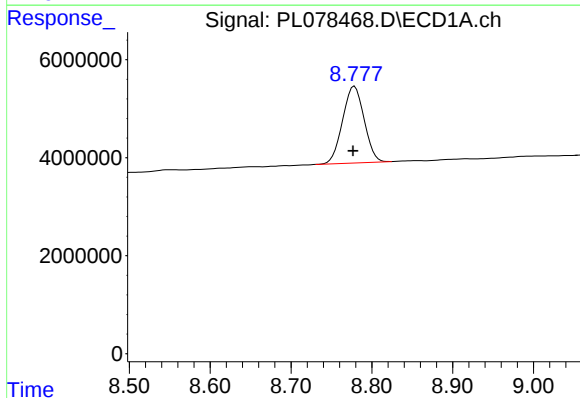

#28 Decachlorobiphenyl

R.T.: 8.779 min
Delta R.T.: 0.002 min
Response: 28979458
Conc: 19.26 ng/ml

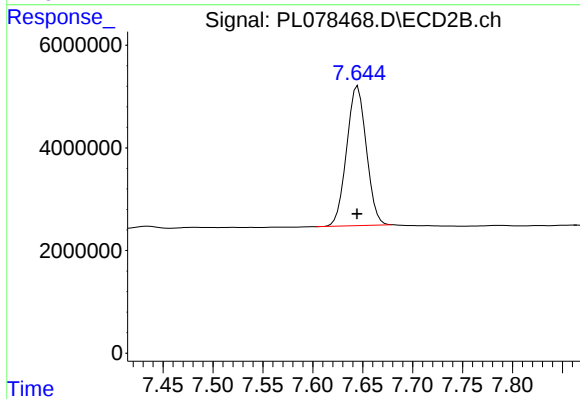

#28 Decachlorobiphenyl

R.T.: 7.645 min
Delta R.T.: 0.000 min
Response: 37305523
Conc: 19.70 ng/ml