

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102318\
 Data File : PL041235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2018 12:37
 Operator : AJ\SJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 14:19:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102318CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 23 14:18:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.103	64846942	33460696	9.948	10.103
27)	SA Decachlor...	8.221	9.234	135.5E6	56323561	21.101	20.863
Target Compounds							
2)	A alpha-BHC	3.916	4.499	90814926	46094924	9.476	9.839
3)	MA gamma-BHC...	4.199	4.787	84274295	43421815	9.466	9.904
4)	MA Heptachlor	4.496	5.303	90962362	43406980	9.784	10.011
9)	A Endosulfan I	5.524	6.360	74548568	33016798	9.895	10.154
13)	MA Dieldrin	5.769	6.618	162.5E6	67794794	19.141	19.909
14)	MA Endrin	6.025	6.838	138.2E6	54062486	19.237	20.051
16)	A 4,4'-DDD	6.153	6.954	114.7E6	49872587	19.062	19.789
17)	MA 4,4'-DDT	6.392	7.254	120.0E6	53221100	18.872	19.994
20)	A Methoxychlor	6.940	7.710	349.8E6	143.2E6	99.365	102.153

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102318\
Data File : PL041235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2018 12:37
Operator : AJ\SJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 14:19:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102318CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 23 14:18:26 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

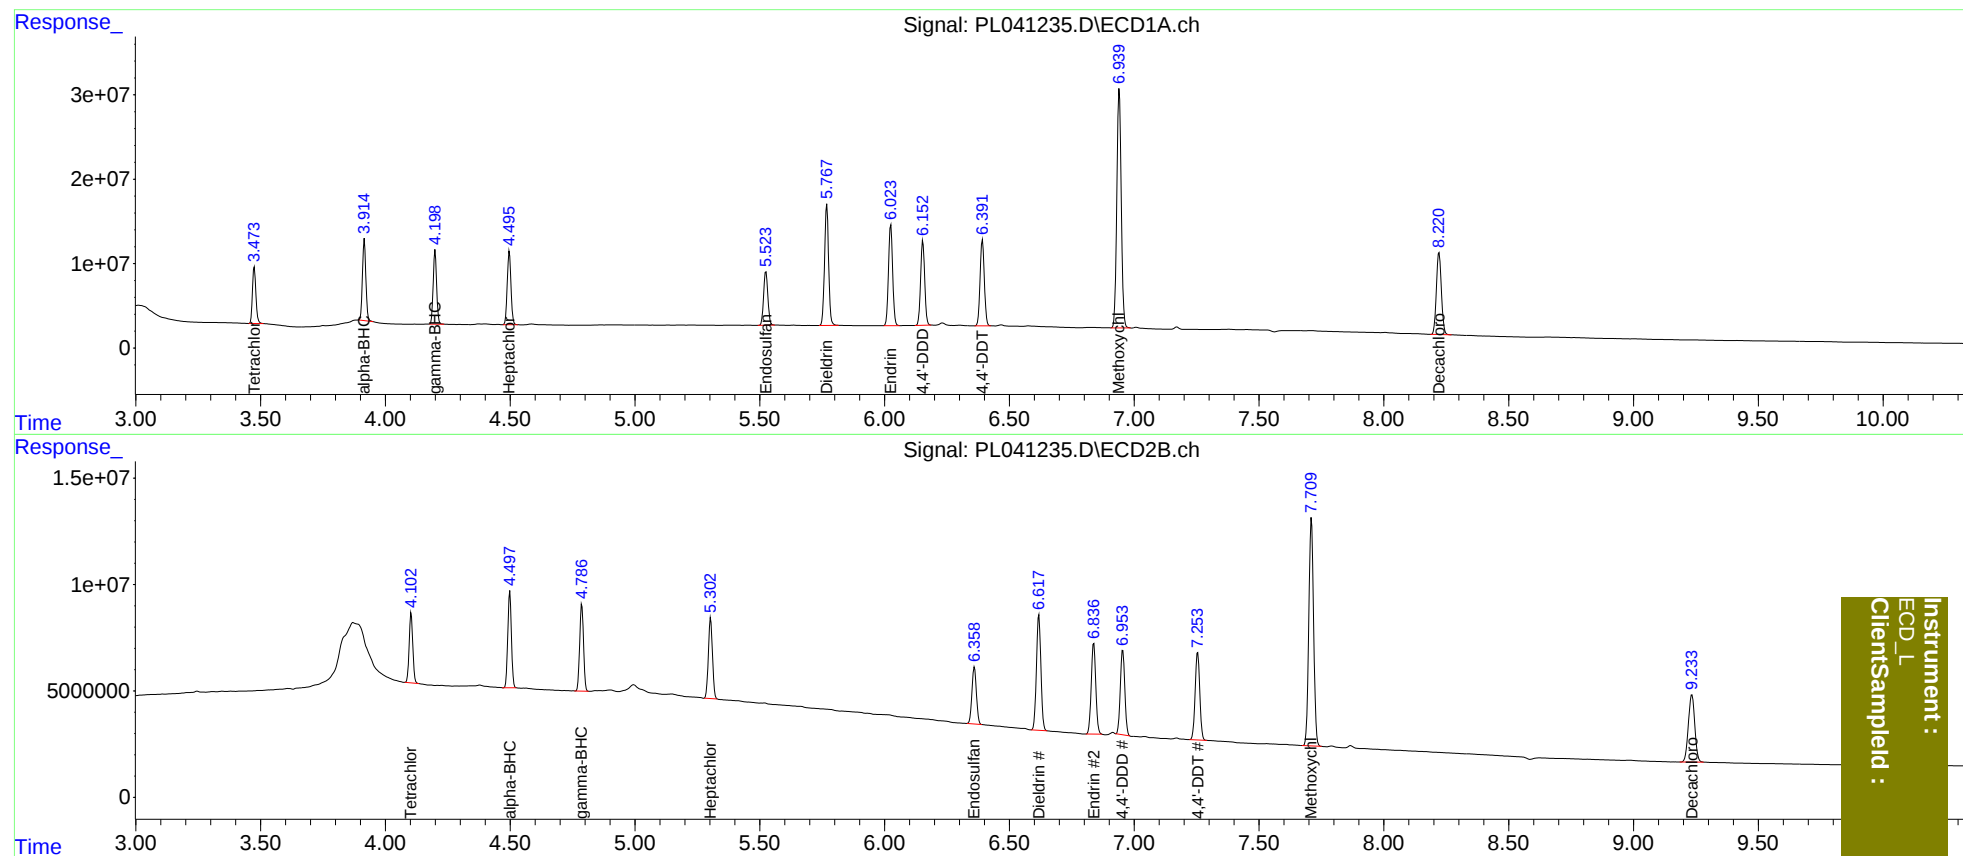


Instrument :
ECD_L
ClientSampled :

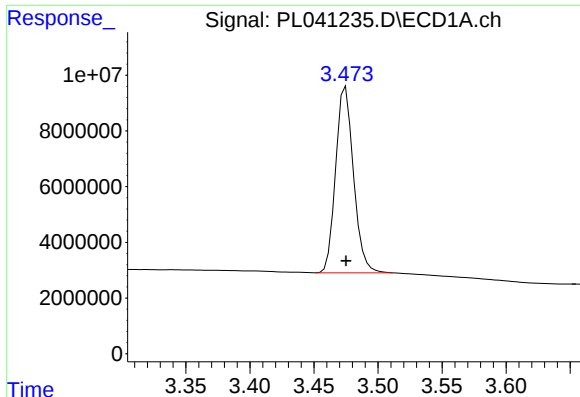

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: 0.000 min
Response: 64846942
Conc: 9.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

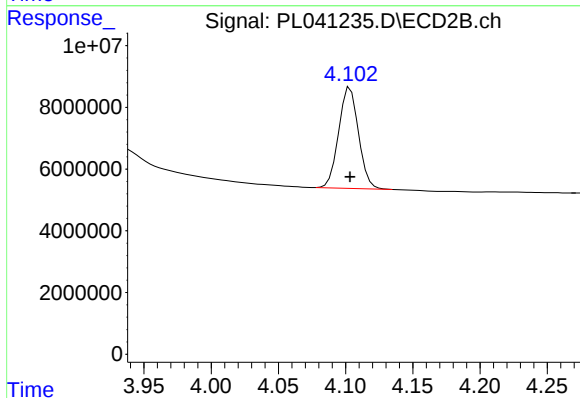


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.000 min
Response: 33460696
Conc: 10.10 ng/ml

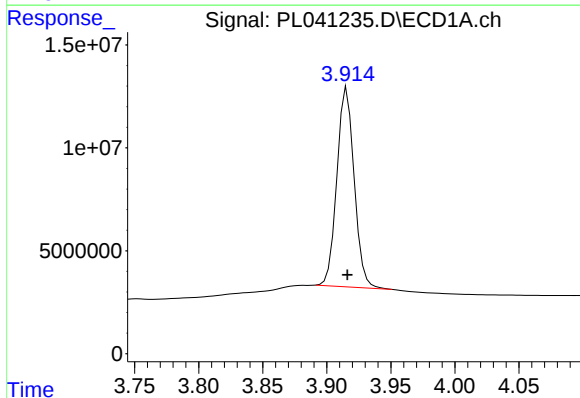


#2 alpha-BHC

R.T.: 3.916 min
Delta R.T.: 0.000 min
Response: 90814926
Conc: 9.48 ng/ml

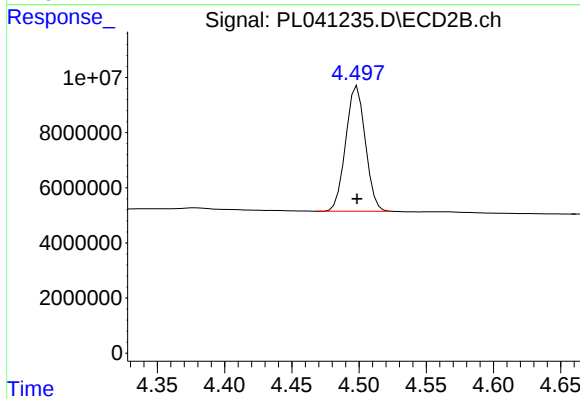

#2 alpha-BHC


R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 46094924
Conc: 9.84 ng/ml

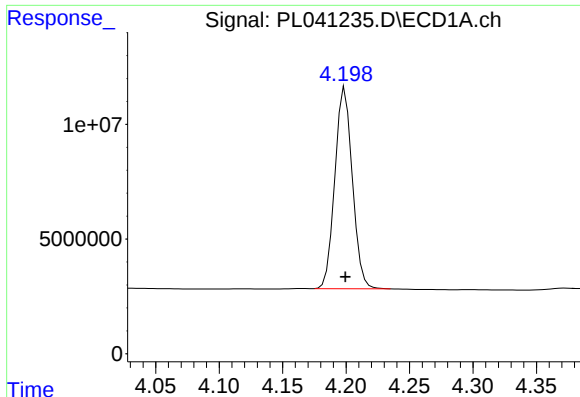

#3 gamma-BHC (Lindane)


R.T.: 4.199 min
Delta R.T.: 0.000 min
Response: 84274295
Conc: 9.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

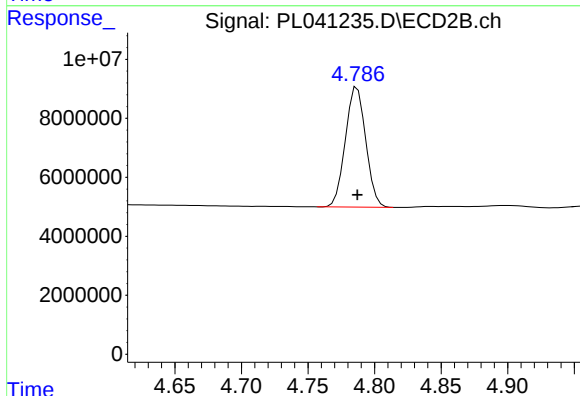


#3 gamma-BHC (Lindane)

R.T.: 4.787 min
Delta R.T.: 0.000 min
Response: 43421815
Conc: 9.90 ng/ml

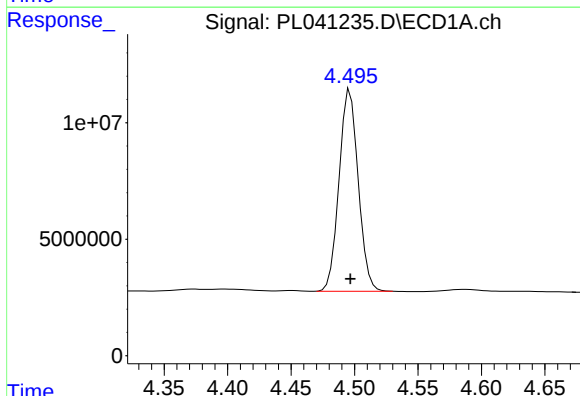


#4 Heptachlor

R.T.: 4.496 min
Delta R.T.: 0.000 min
Response: 90962362
Conc: 9.78 ng/ml

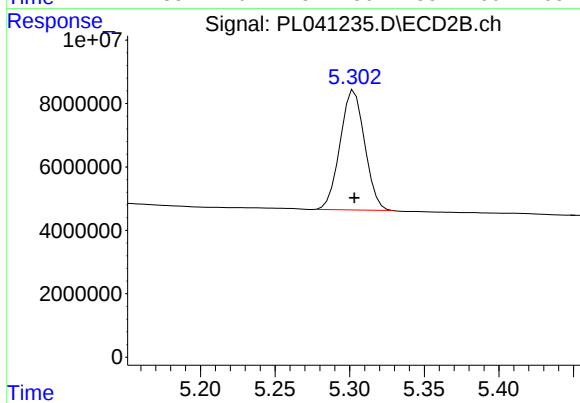

#4 Heptachlor


R.T.: 5.303 min
Delta R.T.: 0.000 min
Response: 43406980
Conc: 10.01 ng/ml

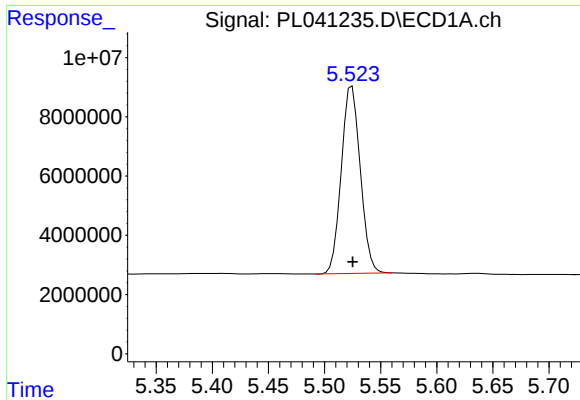

#9 Endosulfan I


R.T.: 5.524 min
Delta R.T.: 0.000 min
Response: 74548568
Conc: 9.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

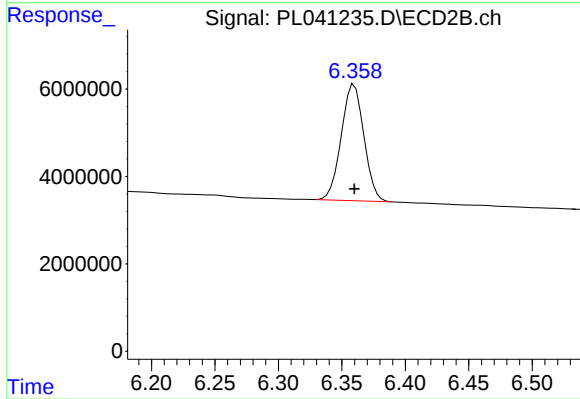


#9 Endosulfan I

R.T.: 6.360 min
Delta R.T.: 0.000 min
Response: 33016798
Conc: 10.15 ng/ml

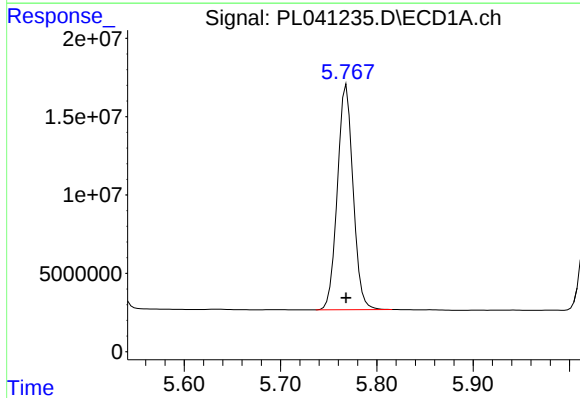


#13 Dieldrin

R.T.: 5.769 min
Delta R.T.: 0.000 min
Response: 162548628
Conc: 19.14 ng/ml

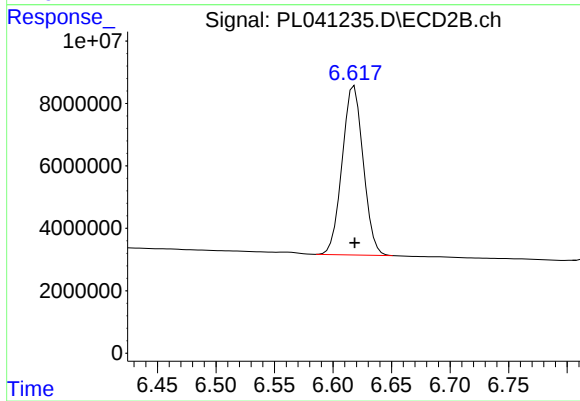

#13 Dieldrin


R.T.: 6.618 min
Delta R.T.: 0.000 min
Response: 67794794
Conc: 19.91 ng/ml

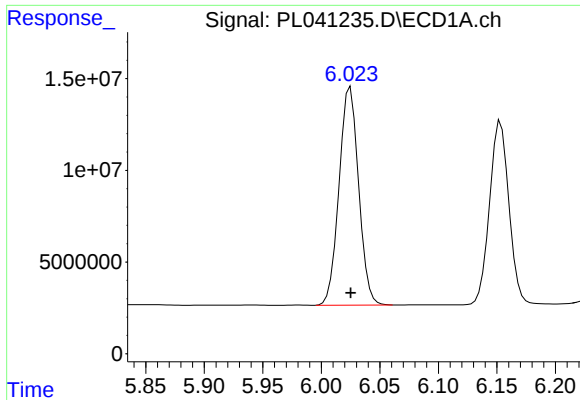

#14 Endrin


R.T.: 6.025 min
Delta R.T.: 0.000 min
Response: 138241253
Conc: 19.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

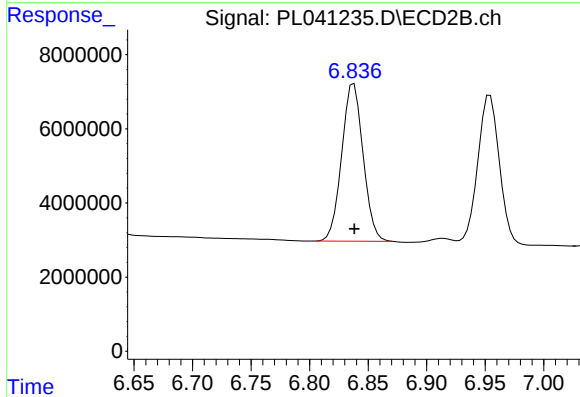


#14 Endrin

R.T.: 6.838 min
Delta R.T.: 0.000 min
Response: 54062486
Conc: 20.05 ng/ml

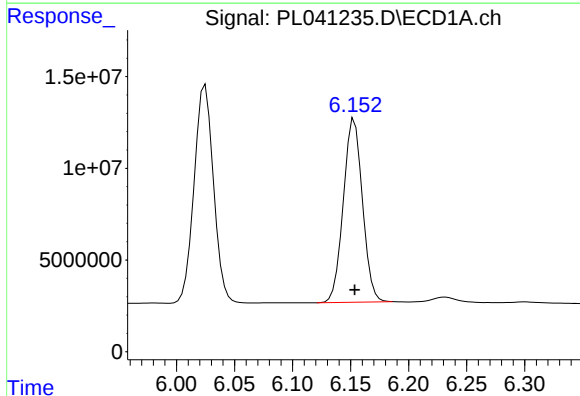


#16 4,4'-DDD

R.T.: 6.153 min
Delta R.T.: 0.000 min
Response: 114667206
Conc: 19.06 ng/ml

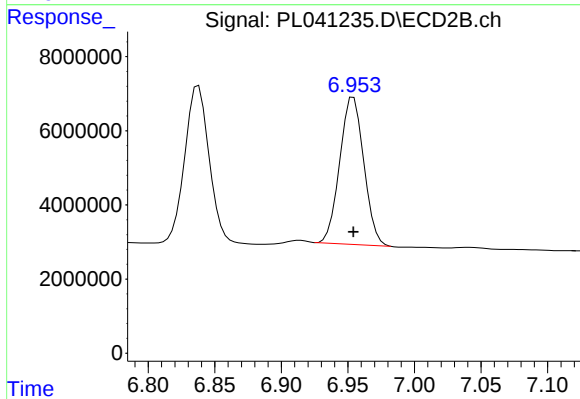

#16 4,4'-DDD


R.T.: 6.954 min
Delta R.T.: 0.000 min
Response: 49872587
Conc: 19.79 ng/ml

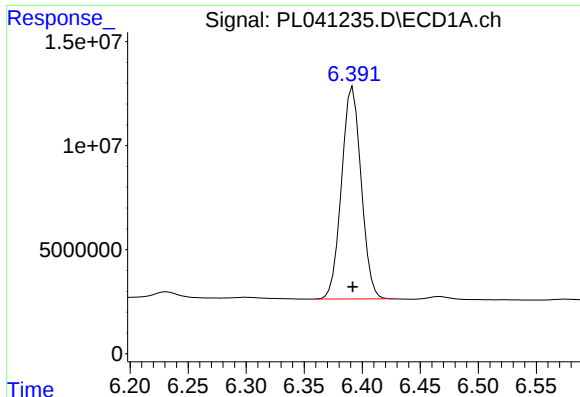

#17 4,4'-DDT


R.T.: 6.392 min
Delta R.T.: 0.000 min
Response: 119966247
Conc: 18.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

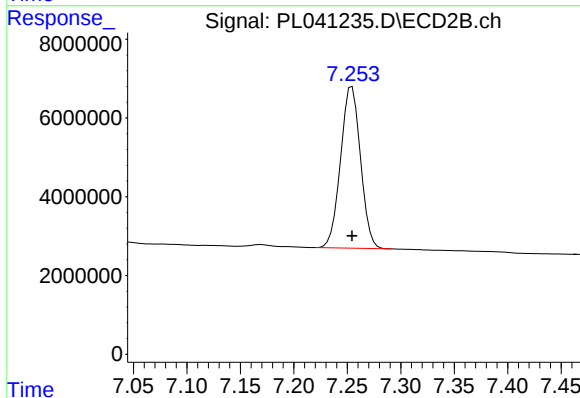


#17 4,4'-DDT

R.T.: 7.254 min
Delta R.T.: 0.000 min
Response: 53221100
Conc: 19.99 ng/ml

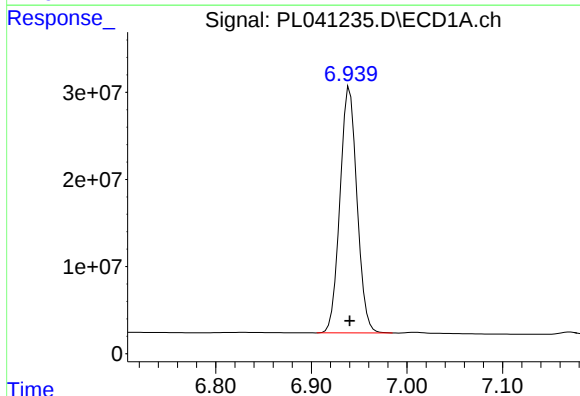


#20 Methoxychlor

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 349780774
Conc: 99.36 ng/ml

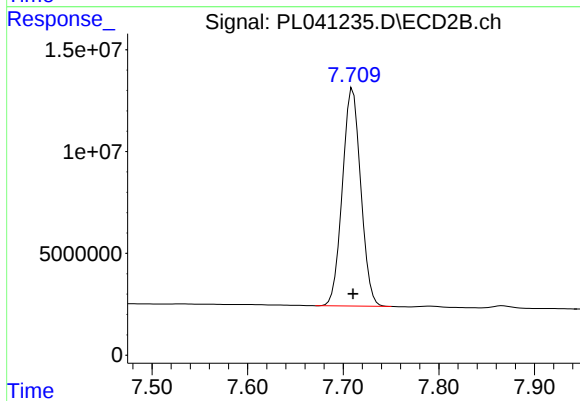

#20 Methoxychlor

R.T.: 7.710 min
Delta R.T.: 0.000 min
Response: 143239904
Conc: 102.15 ng/ml

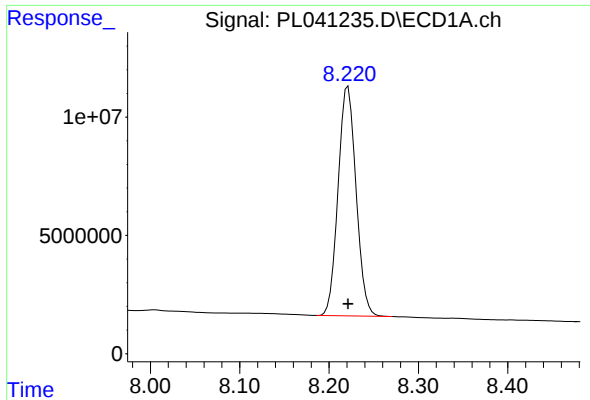

#27 Decachlorobiphenyl


R.T.: 8.221 min

Delta R.T.: 0.000 min

Response: 135484413

Conc: 21.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

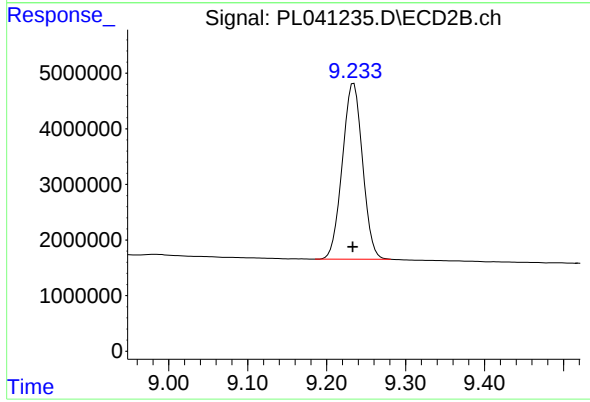

#27 Decachlorobiphenyl

R.T.: 9.234 min

Delta R.T.: 0.001 min

Response: 56323561

Conc: 20.86 ng/ml