

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102318\
 Data File : PL041241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2018 14:02
 Operator : AJ\SJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 14:19:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102318CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 23 14:18:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.103	503.3E6	246.9E6	77.213	74.558
27)	SA Decachlor...	8.222	9.234	937.8E6	391.4E6	146.058	144.993
Target Compounds							
2)	A alpha-BHC	3.916	4.498	793.1E6	371.6E6	82.757	79.315
3)	MA gamma-BHC...	4.200	4.787	734.6E6	342.0E6	82.506	78.011
4)	MA Heptachlor	4.496	5.303	740.6E6	331.8E6	79.661	76.527
9)	A Endosulfan I	5.526	6.360	597.6E6	248.0E6	79.323	76.270
13)	MA Dieldrin	5.769	6.618	1371.2E6	537.6E6	161.464	157.861
14)	MA Endrin	6.025	6.837	1166.1E6	427.2E6	162.273	158.443
16)	A 4,4'-DDD	6.154	6.954	993.4E6	403.4E6	165.141	160.071
17)	MA 4,4'-DDT	6.392	7.254	1069.2E6	420.9E6	168.194	158.121
20)	A Methoxychlor	6.941	7.710	2695.6E6	1036.5E6	765.757	739.165


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102318\
Data File : PL041241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2018 14:02
Operator : AJ\SJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 14:19:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102318CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 23 14:18:26 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

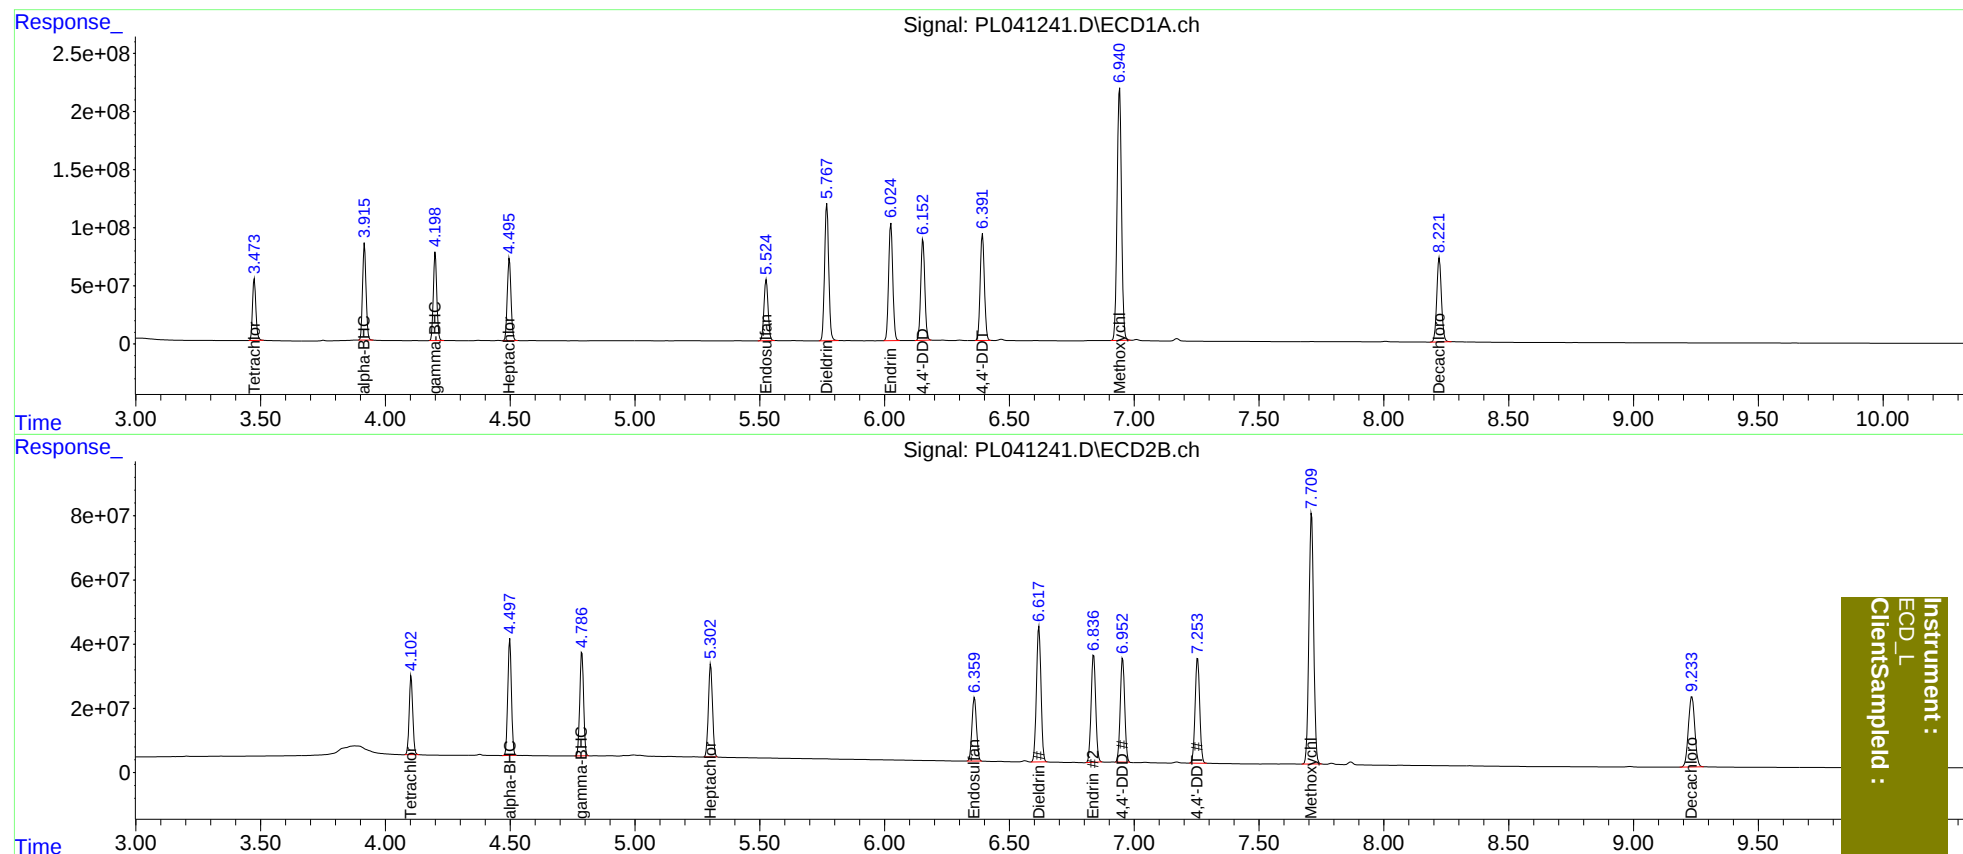


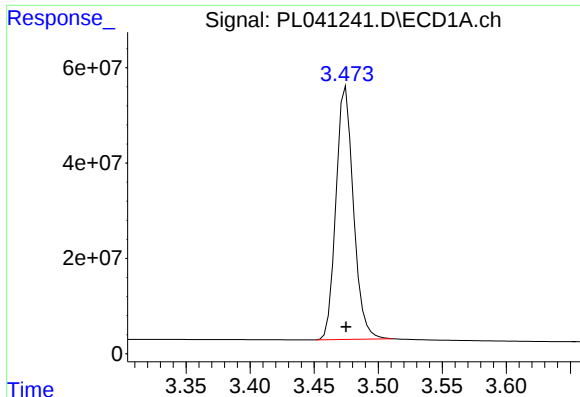

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: 0.000 min
Response: 503342819
Conc: 77.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

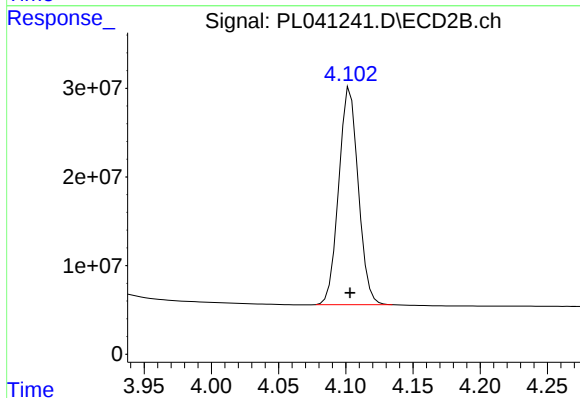


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.000 min
Response: 246940868
Conc: 74.56 ng/ml

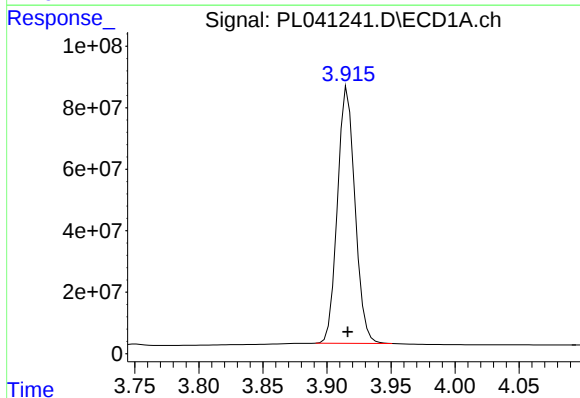


#2 alpha-BHC

R.T.: 3.916 min
Delta R.T.: 0.000 min
Response: 793143450
Conc: 82.76 ng/ml

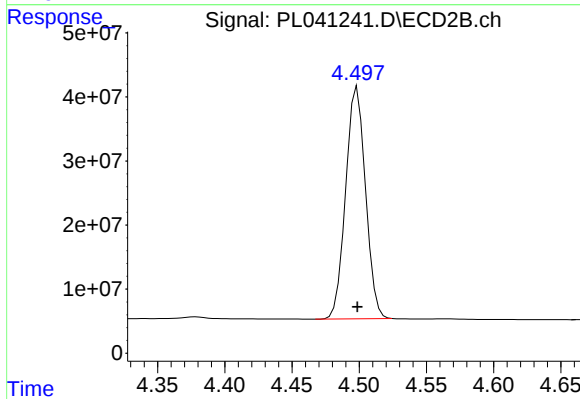

#2 alpha-BHC


R.T.: 4.498 min
Delta R.T.: 0.000 min
Response: 371601626
Conc: 79.32 ng/ml

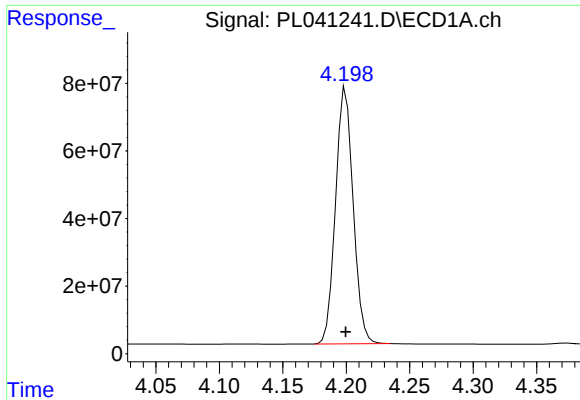

#3 gamma-BHC (Lindane)


R.T.: 4.200 min
Delta R.T.: 0.000 min
Response: 734570884
Conc: 82.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

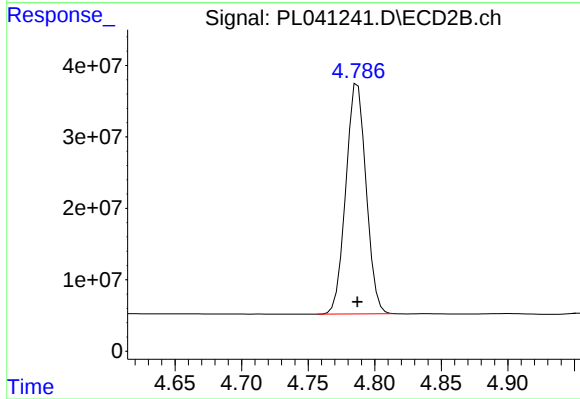


#3 gamma-BHC (Lindane)

R.T.: 4.787 min
Delta R.T.: 0.000 min
Response: 342010407
Conc: 78.01 ng/ml

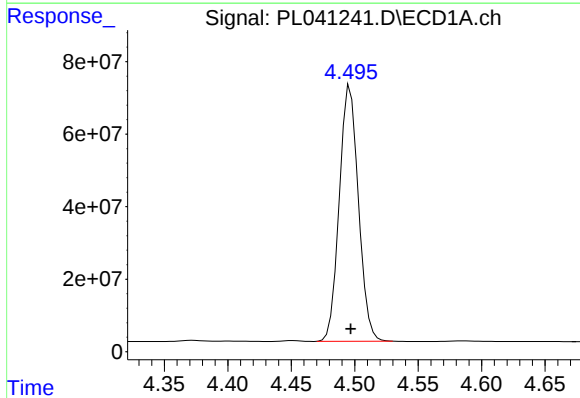


#4 Heptachlor

R.T.: 4.496 min
Delta R.T.: 0.000 min
Response: 740580978
Conc: 79.66 ng/ml

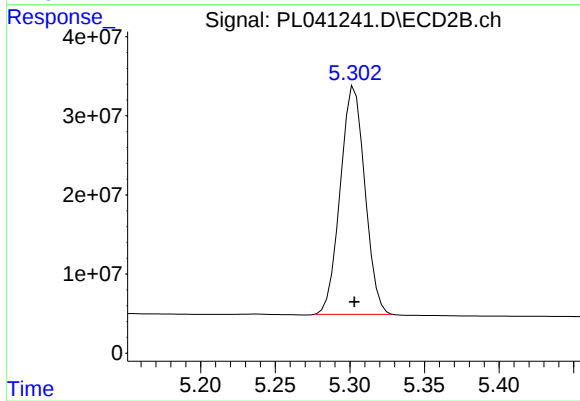

#4 Heptachlor


R.T.: 5.303 min
Delta R.T.: 0.000 min
Response: 331811154
Conc: 76.53 ng/ml

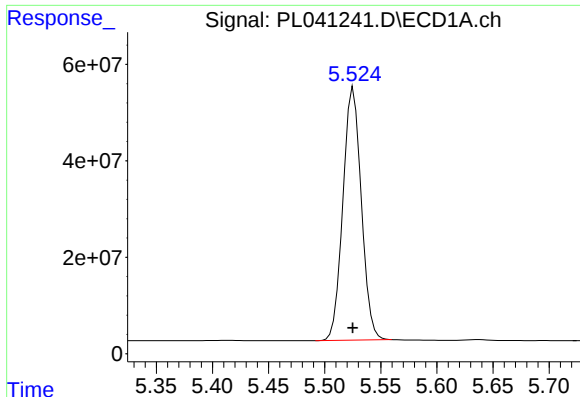

#9 Endosulfan I


R.T.: 5.526 min
Delta R.T.: 0.000 min
Response: 597638871
Conc: 79.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

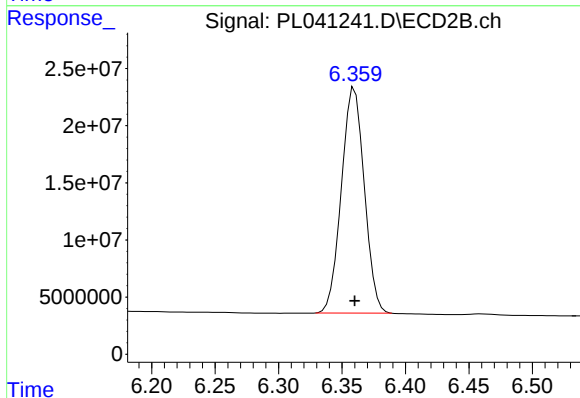


#9 Endosulfan I

R.T.: 6.360 min
Delta R.T.: 0.000 min
Response: 248008569
Conc: 76.27 ng/ml

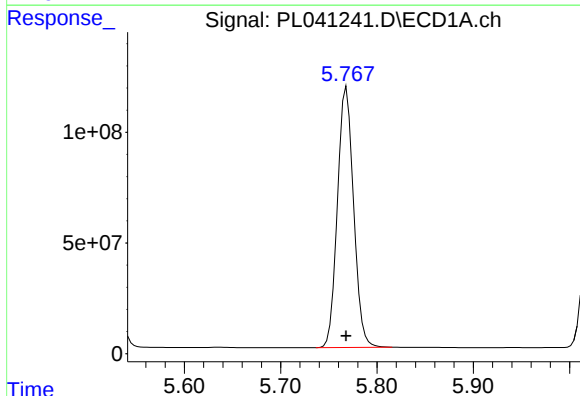


#13 Dieldrin

R.T.: 5.769 min
Delta R.T.: 0.000 min
Response: 1371188831
Conc: 161.46 ng/ml

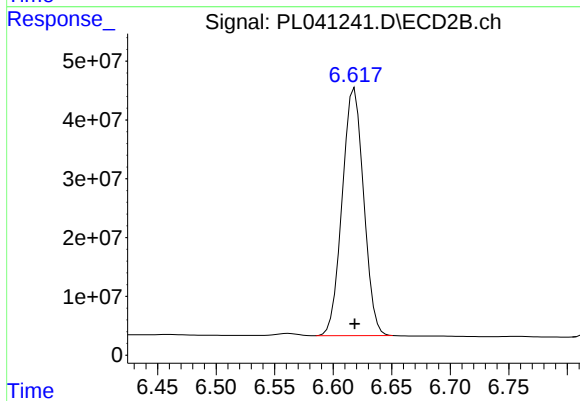

#13 Dieldrin


R.T.: 6.618 min
Delta R.T.: 0.000 min
Response: 537553584
Conc: 157.86 ng/ml

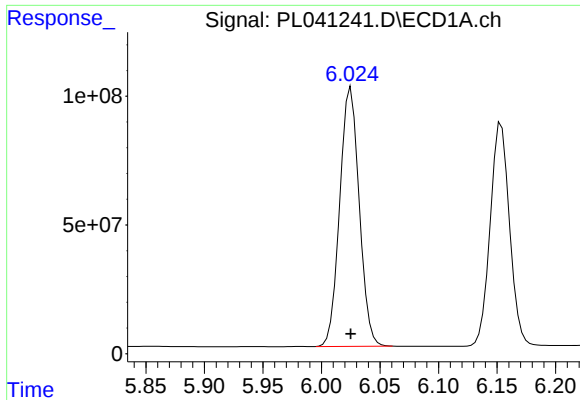

#14 Endrin


R.T.: 6.025 min
Delta R.T.: 0.000 min
Response: 1166122904
Conc: 162.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

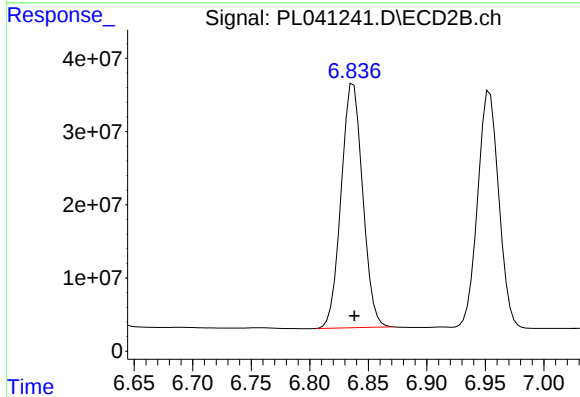


#14 Endrin

R.T.: 6.837 min
Delta R.T.: -0.001 min
Response: 427209593
Conc: 158.44 ng/ml

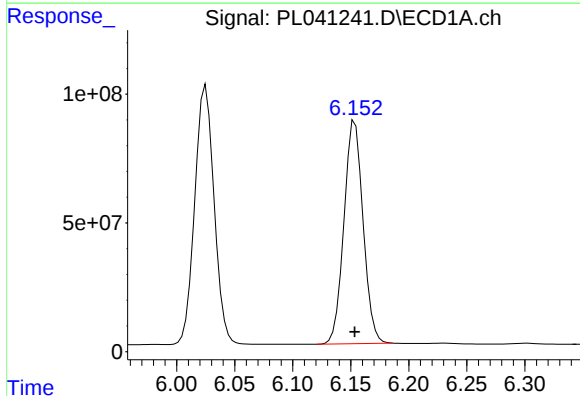


#16 4,4'-DDD

R.T.: 6.154 min
Delta R.T.: 0.000 min
Response: 993413195
Conc: 165.14 ng/ml

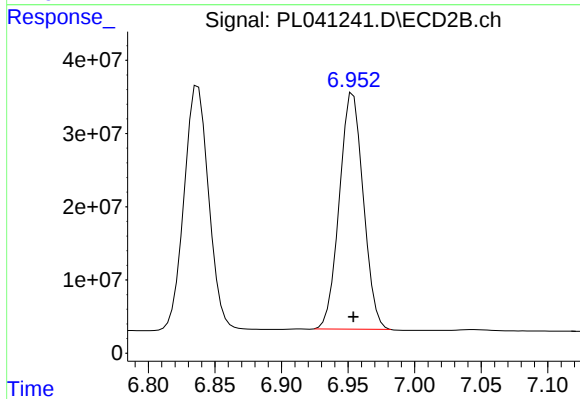

#16 4,4'-DDD


R.T.: 6.954 min
Delta R.T.: 0.000 min
Response: 403403779
Conc: 160.07 ng/ml

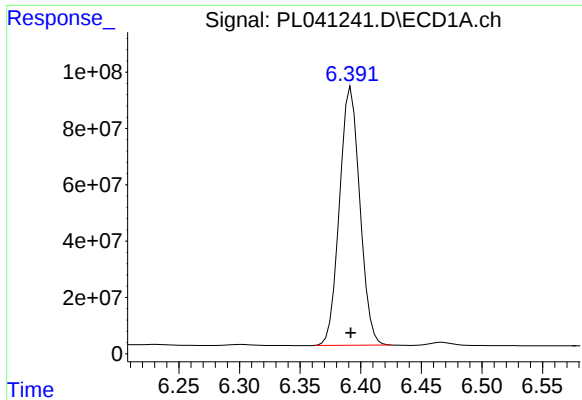

#17 4,4'-DDT


R.T.: 6.392 min
Delta R.T.: 0.000 min
Response: 1069164603
Conc: 168.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

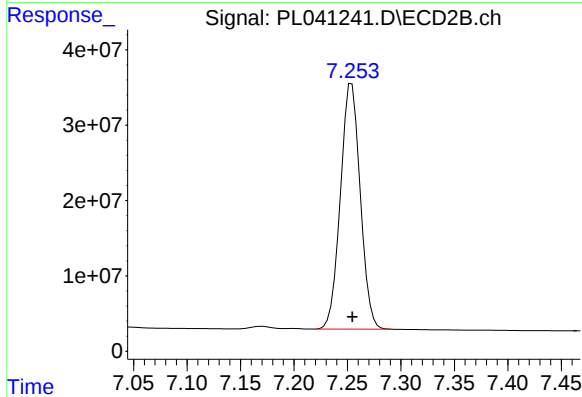


#17 4,4'-DDT

R.T.: 7.254 min
Delta R.T.: 0.000 min
Response: 420896620
Conc: 158.12 ng/ml

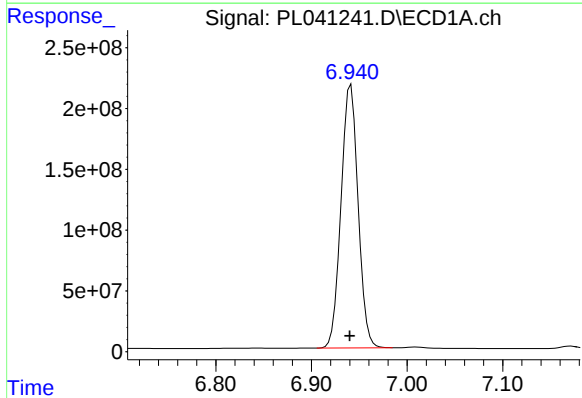


#20 Methoxychlor

R.T.: 6.941 min
Delta R.T.: 0.000 min
Response: 2695599820
Conc: 765.76 ng/ml

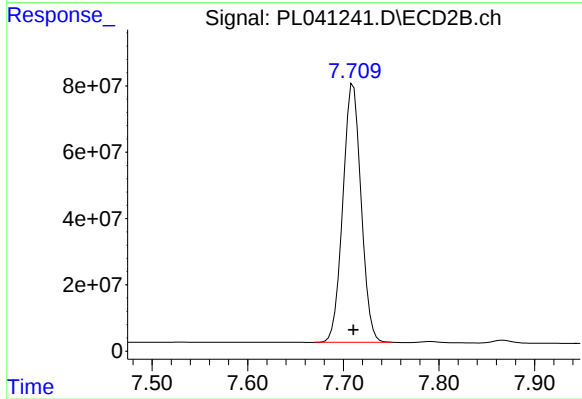

#20 Methoxychlor


R.T.: 7.710 min
Delta R.T.: 0.000 min
Response: 1036467828
Conc: 739.17 ng/ml

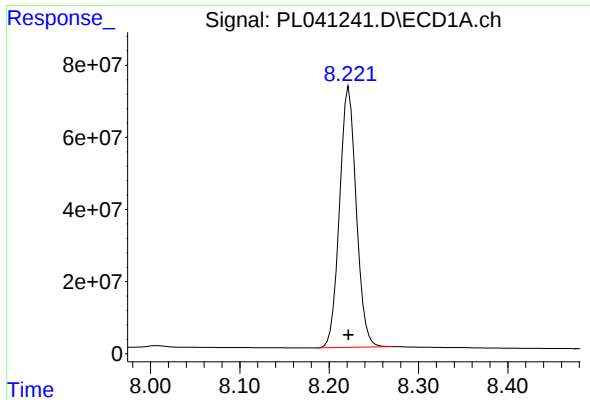

#27 Decachlorobiphenyl

R.T.: 8.222 min
Delta R.T.: 0.000 min
Response: 937812526
Conc: 146.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

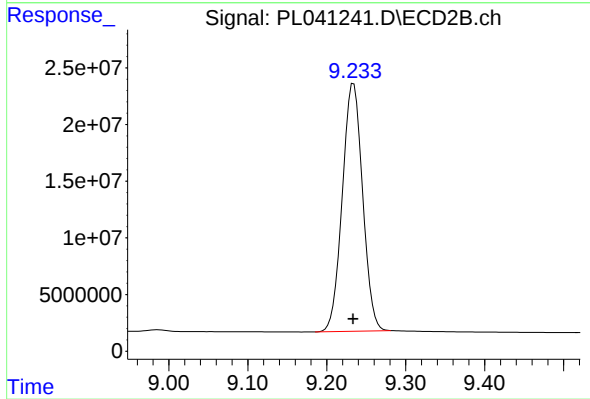

#27 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.000 min
Response: 391441559
Conc: 144.99 ng/ml