


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102318\
Data File : PL041226.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2018 10:31
Operator : AJ\SJ
Sample : RESC51
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESC51

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 01:07:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102318CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 24 01:06:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

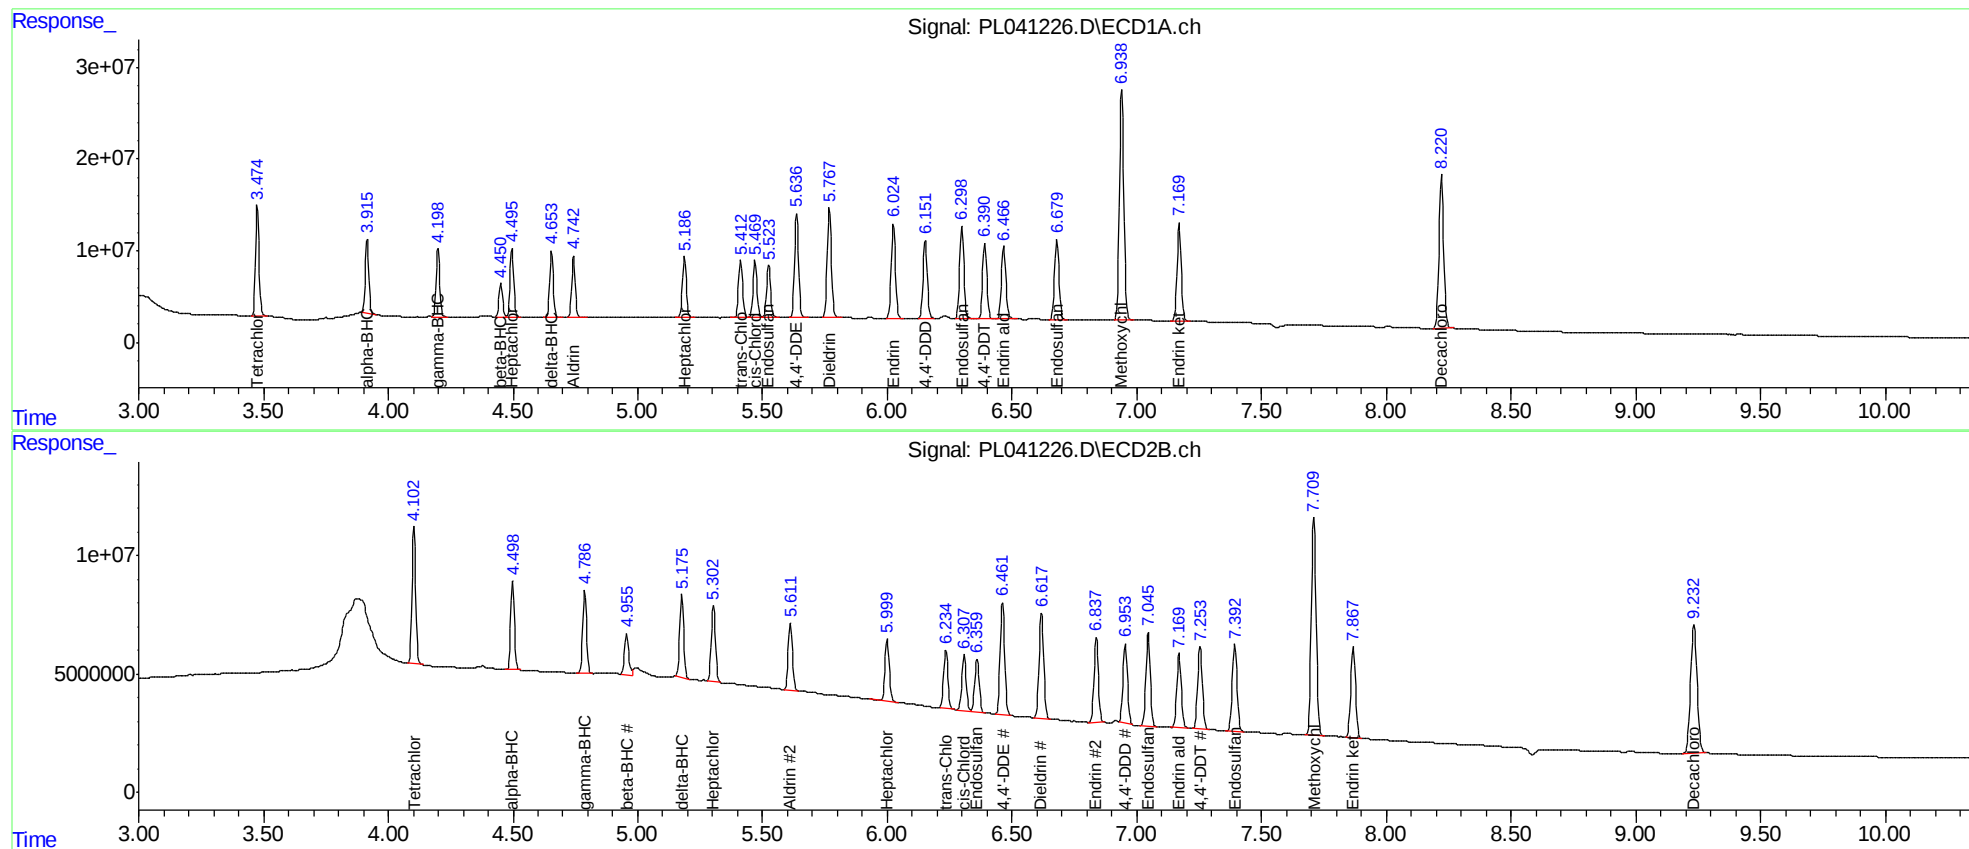

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102318\
 Data File : PL041226.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2018 10:31
 Operator : AJ\SJ
 Sample : RESC51
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESC51

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 01:07:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102318CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 24 01:06:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.104	116.6E6	58495889	18.249	18.102
27)	SA Decachlor...	8.221	9.234	227.1E6	96449956	35.394	35.965
Target Compounds							
2)	A alpha-BHC	3.916	4.499	77590967	38836041	8.276	8.428
3)	MA gamma-BHC...	4.199	4.787	72169419	36990524	8.304	8.569
4)	MA Heptachlor	4.496	5.304	79035211	37041604	8.648	8.680
5)	MB Aldrin	4.743	5.612	71204628	33776583	9.088	9.231
6)	B beta-BHC	4.452	4.956	36978139	19975558	9.748	9.917
7)	B delta-BHC	4.655	5.177	71597212	37795914	8.975	9.289
8)	B Heptachlo...	5.187	6.000	74830128	32155400	9.612	9.340
9)	A Endosulfan I	5.525	6.360	66480385	27731721	8.912	8.611
10)	B trans-Chl...	5.413	6.235	72957894	29995198	9.459	9.257
11)	B cis-Chlor...	5.471	6.309	71739429	30026688	9.439	9.484
12)	B 4,4'-DDE	5.637	6.463	126.6E6	59265017	18.297	18.507
13)	MA Dieldrin	5.768	6.618	139.1E6	56187819	16.803	16.671
14)	MA Endrin	6.025	6.838	118.5E6	45006686	16.819	16.773
15)	B Endosulfa...	6.299	7.046	120.4E6	50122797	18.044	18.672
16)	A 4,4'-DDD	6.153	6.954	97406251	41670899	16.543	16.761
17)	MA 4,4'-DDT	6.392	7.255	99967771	44970964	16.019	17.033
18)	B Endrin al...	6.467	7.170	98102684	41052239	18.827	18.450
19)	B Endosulfa...	6.680	7.393	109.2E6	48230765	17.655	19.046
20)	A Methoxychlor	6.940	7.710	305.9E6	123.1E6	88.637	88.814
21)	B Endrin ke...	7.171	7.868	130.5E6	50734993	20.168	19.412

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.