

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102318\
 Data File : PL041247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2018 15:27
 Operator : AJ\SJ
 Sample : MDL-S-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-S-02

Manual Integrations
 APPROVED

Sohil
 10/25/2018 8:36:15 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 07:54:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102318CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 24 01:06:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.104	109.1E6	57270400	17.067	17.723
27)	SA Decachlor...	8.222	9.234	240.4E6	103.2E6	37.469	38.492
Target Compounds							
2)	A alpha-BHC	3.915	4.499	8165598	3358353	0.871	0.729
3)	MA gamma-BHC...	4.199	4.787	5810979	3444968	0.669	0.798
4)	MA Heptachlor	4.496	5.303	6797323	3781256	0.744	0.886
5)	MB Aldrin	4.743	5.612	5543113	3256260	0.707	0.890 #
6)	B beta-BHC	4.452	4.957	2744920	2554279	0.724	1.268 #
7)	B delta-BHC	4.653	5.175	5046608	2362725	0.633m	0.581
8)	B Heptachlo...	5.185	5.999	6894429	3286227	0.886m	0.955m
9)	A Endosulfan I	5.524	6.359	6132742	2507814	0.822m	0.779
10)	B trans-Chl...	5.411	6.235	6736190	2796369	0.873m	0.863
11)	B cis-Chlor...	5.471	6.308	6965975	2809689	0.916	0.887
12)	B 4,4'-DDE	5.637	6.462	4801048	2758834	0.694	0.862
13)	MA Dieldrin	5.766	6.618	5769253	2931496	0.697m	0.870
14)	MA Endrin	6.025	6.838	6096573	2455291	0.865	0.915
15)	B Endosulfa...	6.299	7.045	6060847	2850054	0.909	1.062
16)	A 4,4'-DDD	6.151	6.953	4106617	2548579	0.697m	1.025m#
17)	MA 4,4'-DDT	6.391	7.254	4003244	2361866	0.641	0.895 #
18)	B Endrin al...	6.468	7.170	4772245	2138242	0.916	0.961
19)	B Endosulfa...	6.680	7.392	5719568	2442232	0.925	0.964
20)	A Methoxychlor	6.939	7.710	2877872	1283714	0.834	0.926
21)	B Endrin ke...	7.170	7.868	5481212	2576007	0.847	0.986

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102318\
Data File : PL041247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2018 15:27
Operator : AJ\SJ
Sample : MDL-S-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 07:54:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102318CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 24 01:06:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

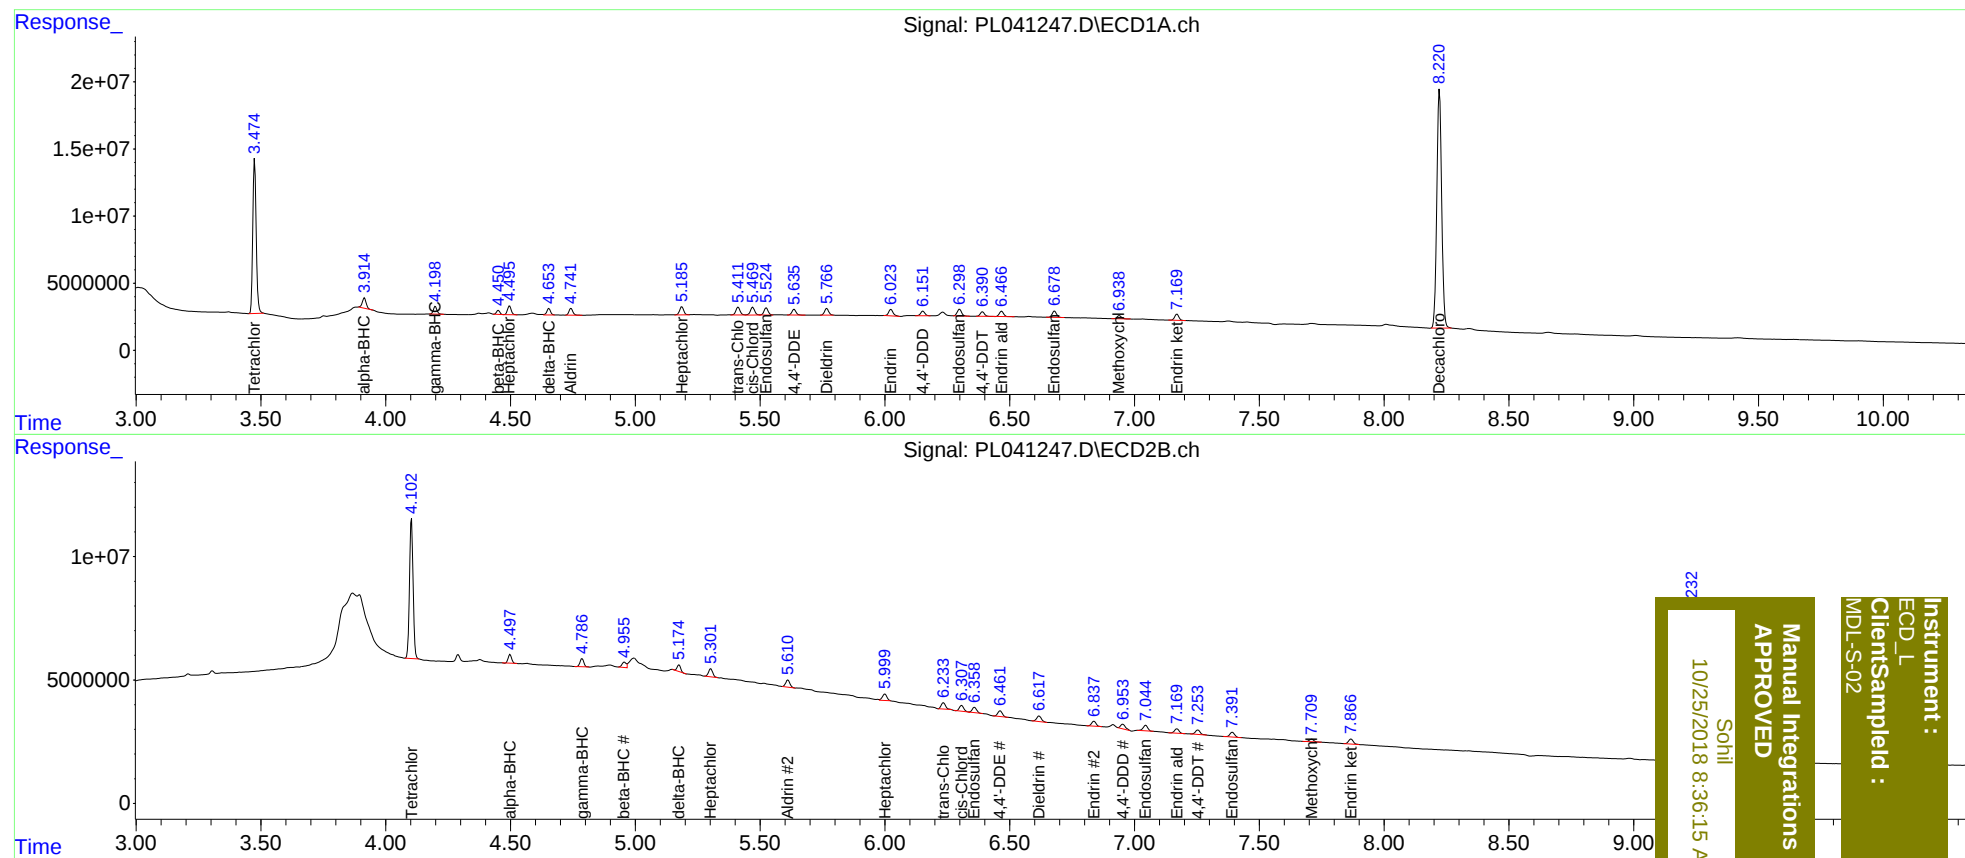

232
10/25/2018 8:36:15 AM

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sample :
MDL-S-02