

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102318\
 Data File : PL041248.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2018 15:41
 Operator : AJ\SJ
 Sample : MDL-S-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-S-03

Manual Integrations
 APPROVED

Sohil
 10/25/2018 8:36:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 07:54:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102318CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 24 01:06:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.103	108.7E6	57103280	17.015	17.671
27)	SA Decachlor...	8.222	9.234	239.3E6	102.5E6	37.294	38.235
Target Compounds							
2)	A alpha-BHC	3.916	4.499	7449526	3249943	0.795	0.705
3)	MA gamma-BHC...	4.200	4.787	5633725	3336746	0.648	0.773
4)	MA Heptachlor	4.496	5.303	6284962	3316370	0.688m	0.777
5)	MB Aldrin	4.744	5.612	5238251	2878428	0.669	0.787
6)	B beta-BHC	4.452	4.956	2464119	2515215	0.650	1.249 #
7)	B delta-BHC	4.655	5.174	5070004	2563108	0.636	0.630m
8)	B Heptachlo...	5.186	5.999	6424038	3353260	0.825m	0.974m
9)	A Endosulfan I	5.525	6.359	5539785	3010176	0.743m	0.935 #
10)	B trans-Chl...	5.412	6.235	6323803	2574868	0.820m	0.795
11)	B cis-Chlor...	5.472	6.309	6592467	3255822	0.867	1.028
12)	B 4,4'-DDE	5.636	6.462	4719490	2791314	0.682m	0.872 #
13)	MA Dieldrin	5.767	6.618	5482922	2932985	0.662m	0.870 #
14)	MA Endrin	6.024	6.838	5208786	2495007	0.739m	0.930 #
15)	B Endosulfa...	6.300	7.046	6747191	2726071	1.012	1.016
16)	A 4,4'-DDD	6.151	6.953	4004293	2355971	0.680m	0.948m#
17)	MA 4,4'-DDT	6.392	7.255	3869626	2235760	0.620	0.847 #
18)	B Endrin al...	6.468	7.172	4601562	1663043	0.883	0.747
19)	B Endosulfa...	6.680	7.393	6387140	2422812	1.033	0.957
20)	A Methoxychlor	6.940	7.710	2707499	1231525	0.784	0.889
21)	B Endrin ke...	7.171	7.868	5119383	2605224	0.791	0.997 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102318\
Data File : PL041248.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2018 15:41
Operator : AJ\SJ
Sample : MDL-S-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 07:54:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102318CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 24 01:06:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

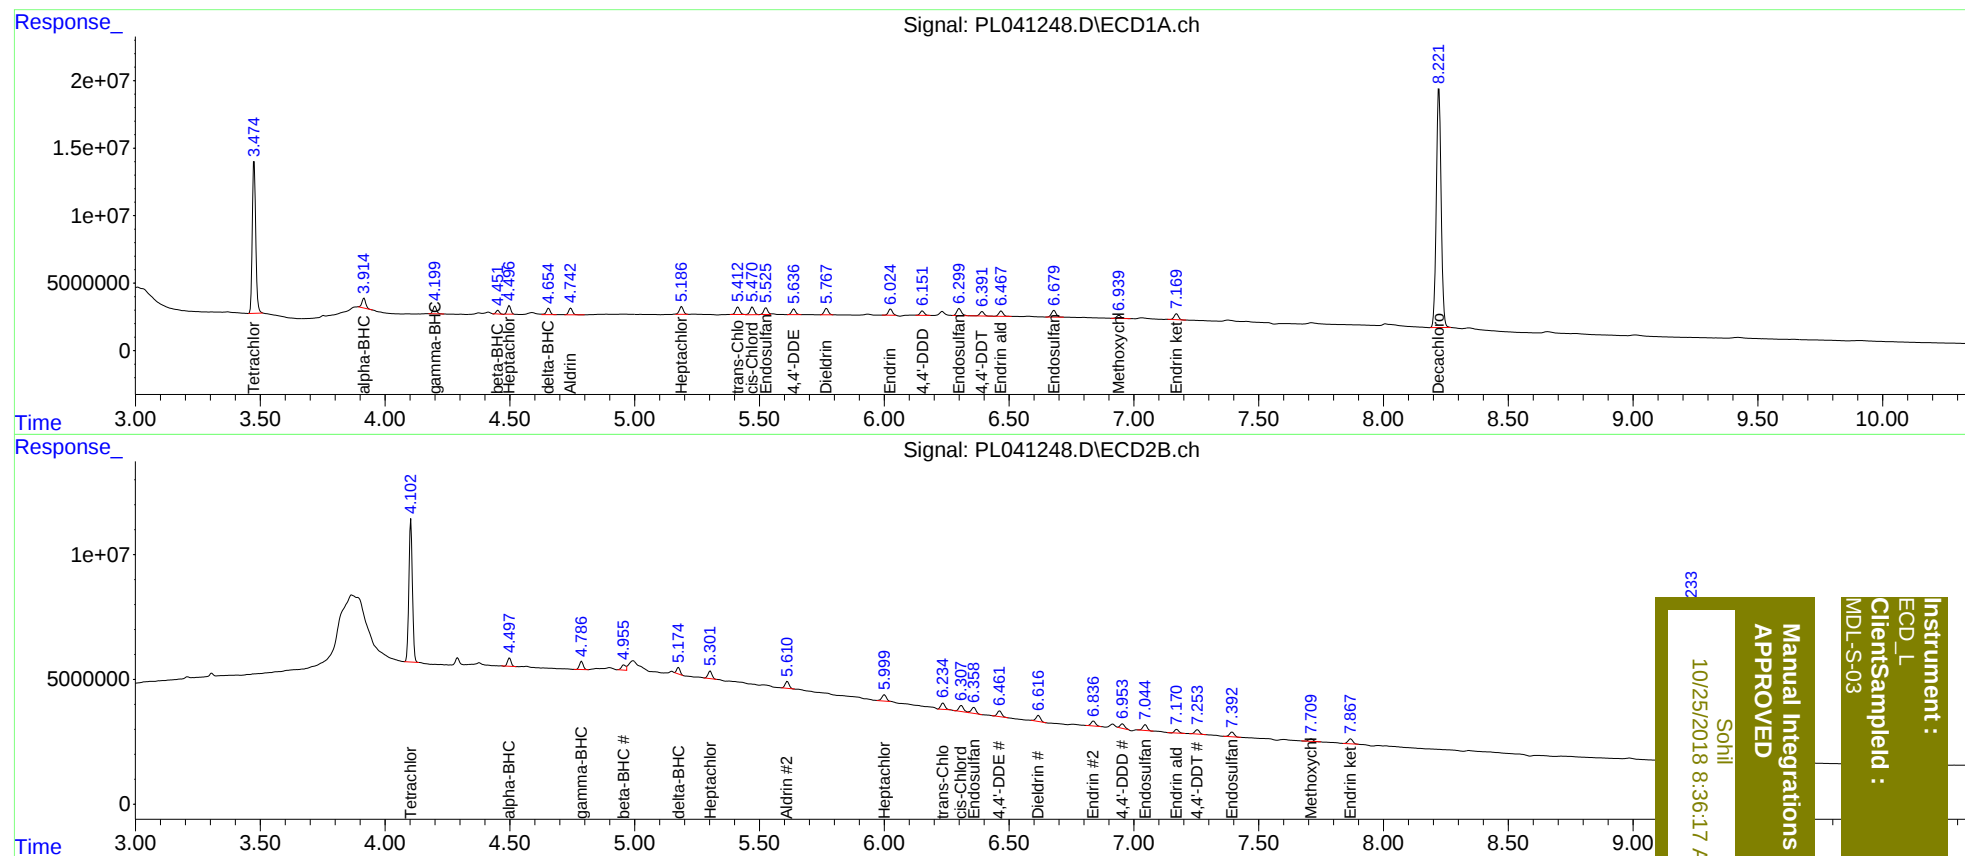

232
10/25/2018 8:36:17 AM

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sampled :
MDL-S-03