

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
 Data File : PL053602.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2019 14:37
 Operator : SG\AJ
 Sample : K5489-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 22:36:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.045	215.1E6	52142542	19.847	20.837
28)	SA Decachlor...	8.331	9.123	158.3E6	49276705	16.135	17.499
Target Compounds							
15)	B Endosulfa...	6.405	6.976	13283571	9394370	1.188	3.678 #
16)	A 4,4'-DDD	6.247	0.000	1589161	0	0.179	N.D. #
17)	MA 4,4'-DDT	6.485	7.148f	3705951	10561618	0.374	4.567 #
19)	B Endosulfa...	6.794	0.000	36387119	0	3.577	N.D. #
23)	Chlordane-1	4.449f	0.000	3680132	0	10.376	N.D. #
27)	Chlordane-5	6.405	0.000	13283571	0	36.339	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
Data File : PL053602.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2019 14:37
Operator : SG\AJ
Sample : K5489-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 22:36:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

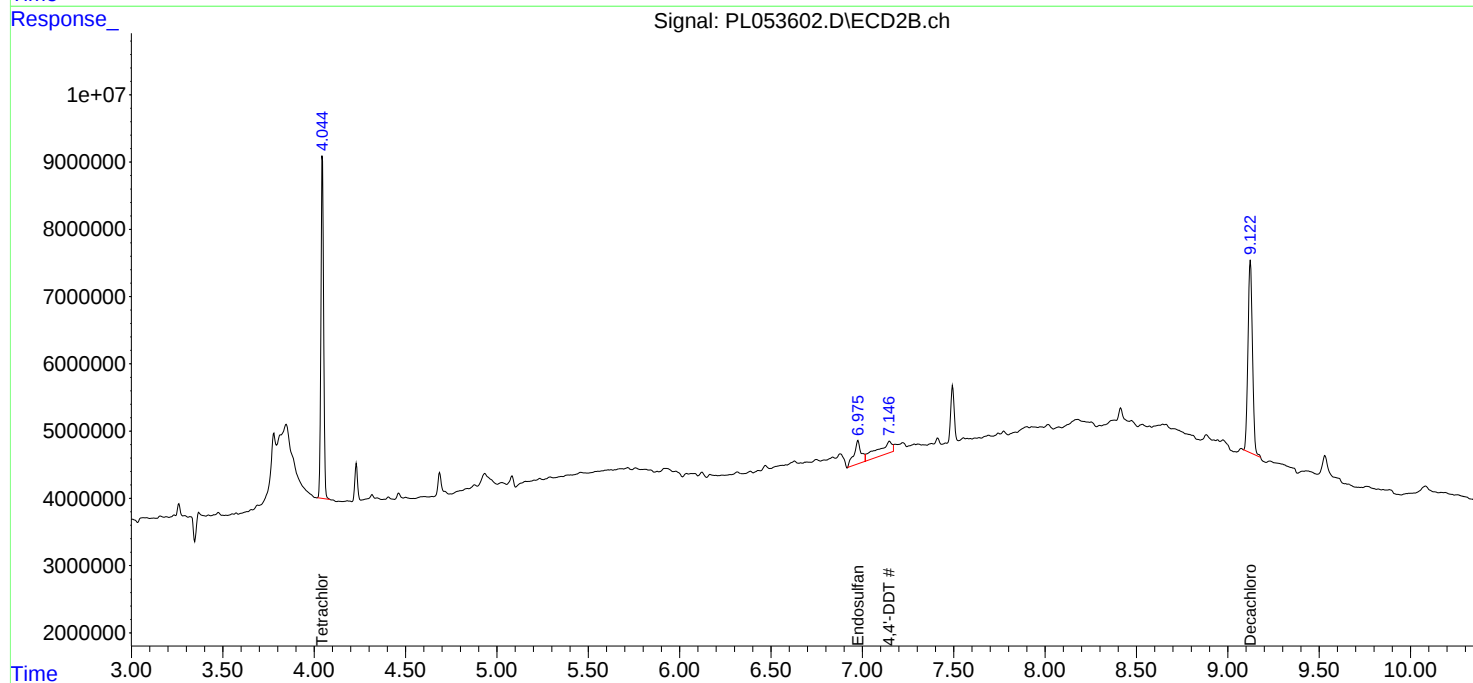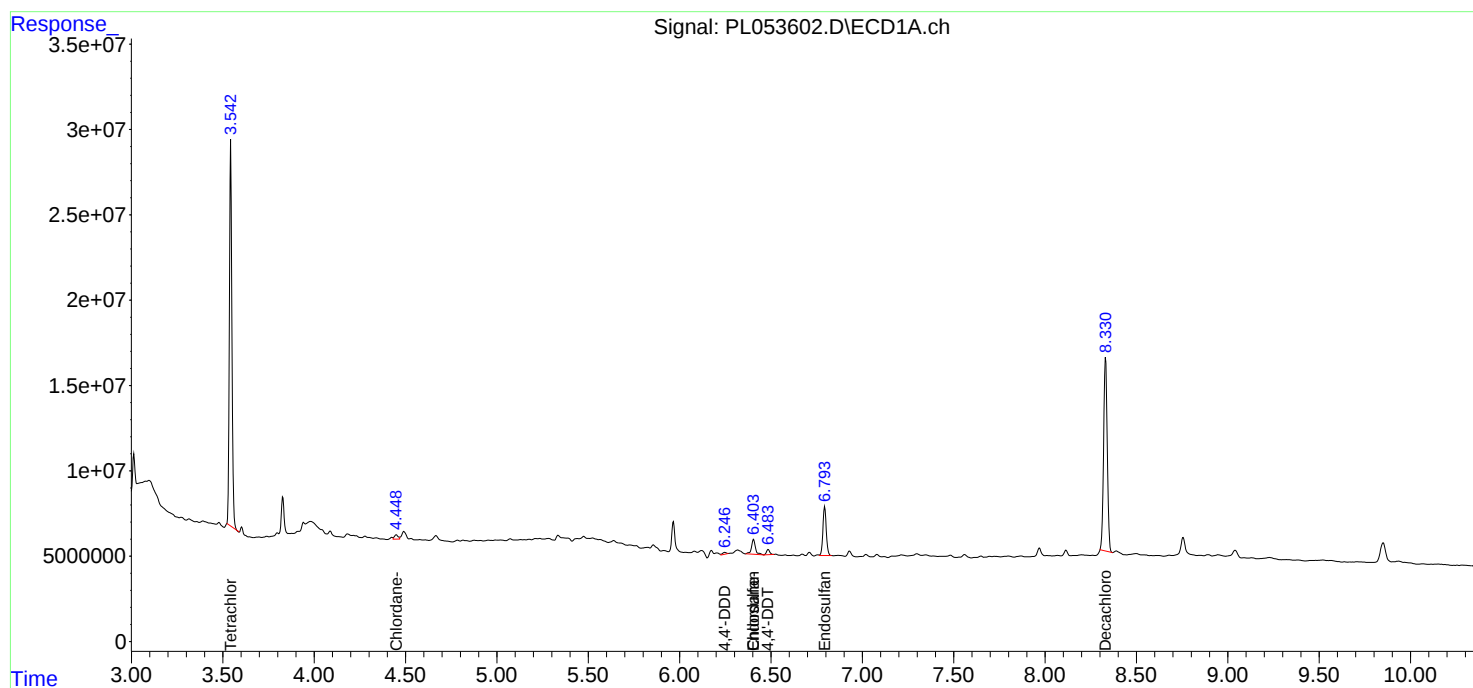


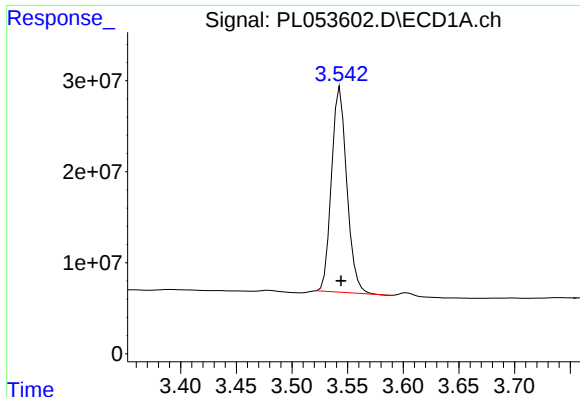

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 215126129
Conc: 19.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

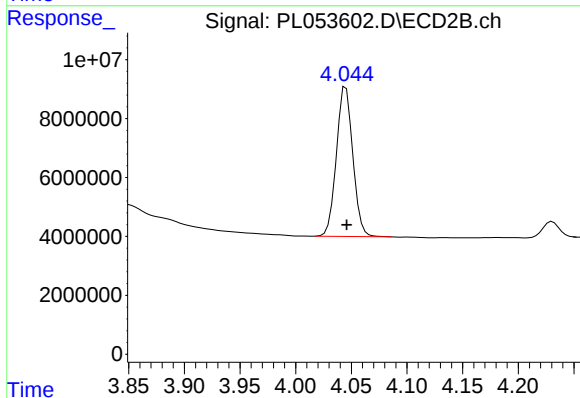


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 52142542
Conc: 20.84 ng/ml

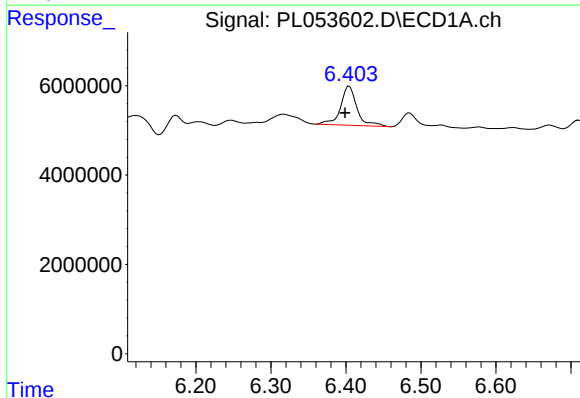


#15 Endosulfan II

R.T.: 6.405 min
Delta R.T.: 0.006 min
Response: 13283571
Conc: 1.19 ng/ml

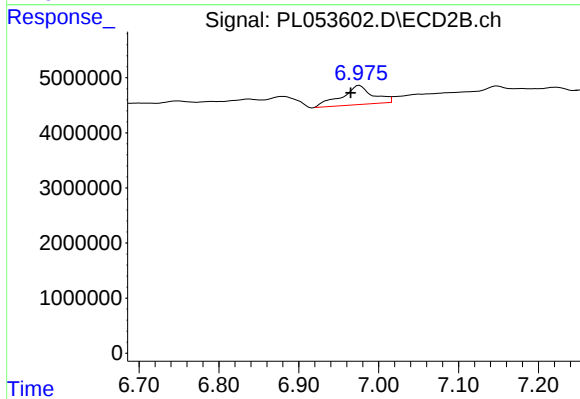

#15 Endosulfan II


R.T.: 6.976 min
Delta R.T.: 0.011 min
Response: 9394370
Conc: 3.68 ng/ml

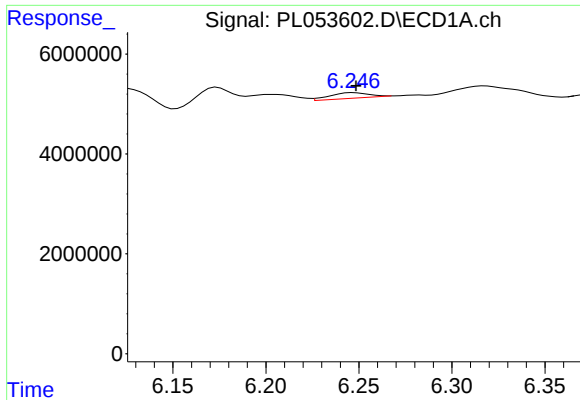

#16 4,4'-DDD


R.T.: 6.247 min
Delta R.T.: -0.001 min
Response: 1589161
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

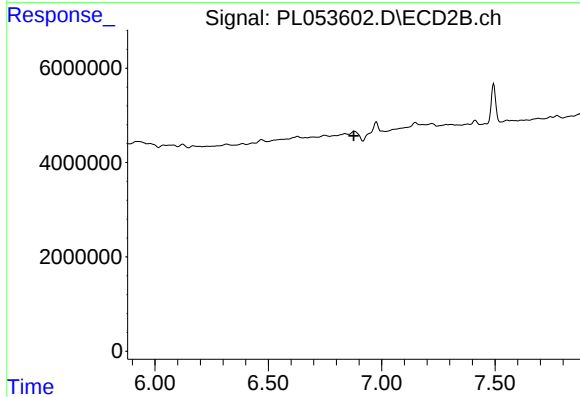


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.877 min
Response: 0
Conc: N.D.

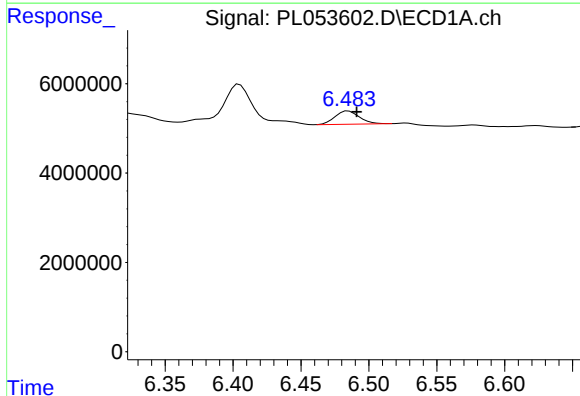


#17 4,4'-DDT

R.T.: 6.485 min
Delta R.T.: -0.006 min
Response: 3705951
Conc: 0.37 ng/ml

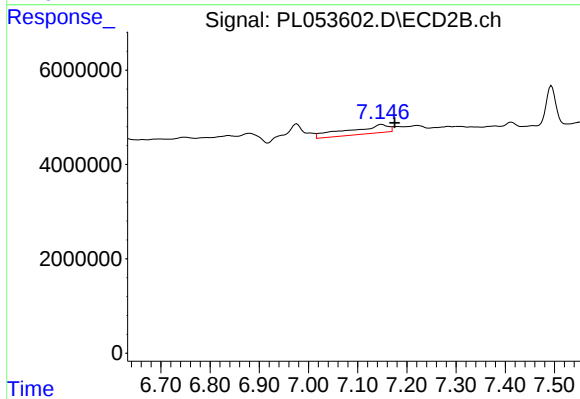

#17 4,4'-DDT


R.T.: 7.148 min
Delta R.T.: -0.027 min
Response: 10561618
Conc: 4.57 ng/ml

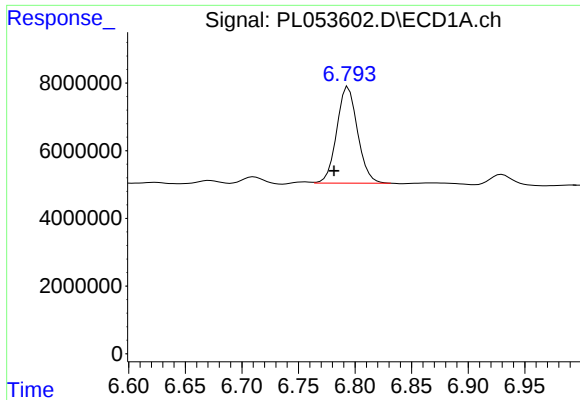

#19 Endosulfan Sulfate


R.T.: 6.794 min
Delta R.T.: 0.013 min
Response: 36387119
Conc: 3.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

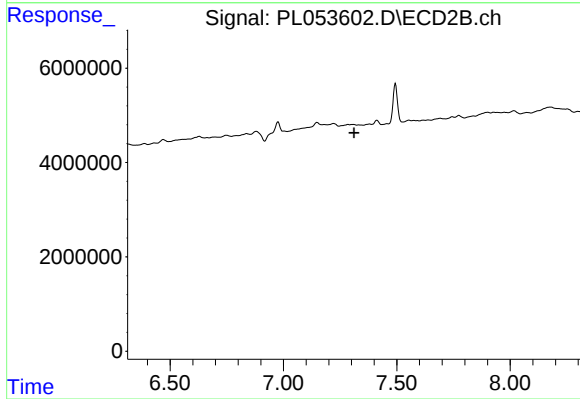


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.312 min
Response: 0
Conc: N.D.

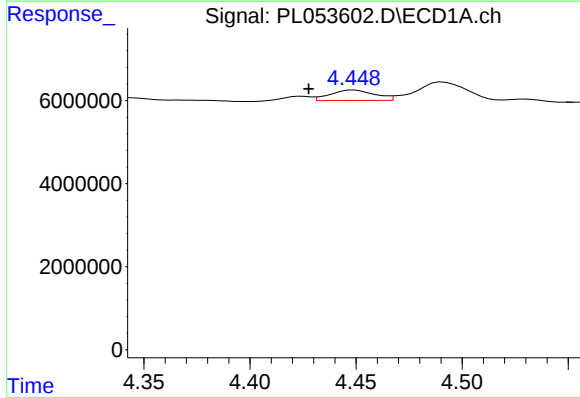


#23 Chlordane-1

R.T.: 4.449 min
Delta R.T.: 0.021 min
Response: 3680132
Conc: 10.38 ng/ml

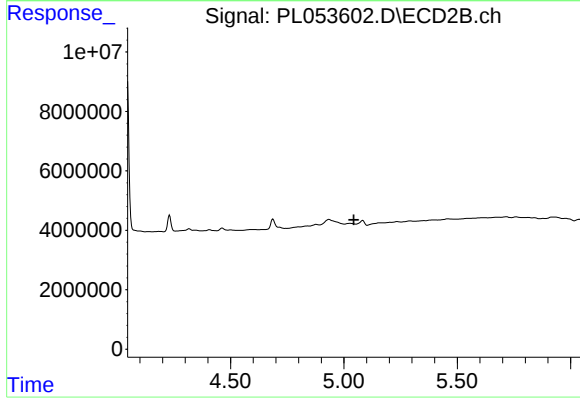

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.043 min
Response: 0
Conc: N.D.

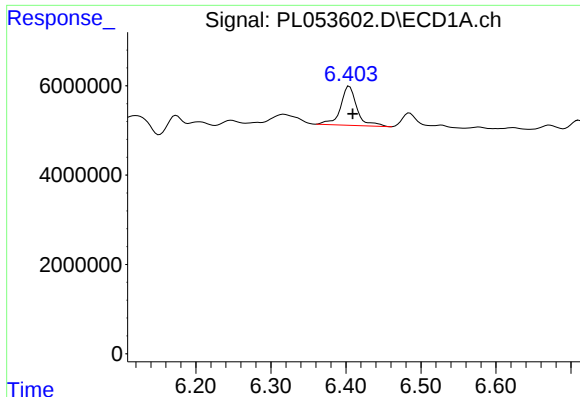

#27 Chlordane-5


R.T.: 6.405 min
Delta R.T.: -0.004 min
Response: 13283571
Conc: 36.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

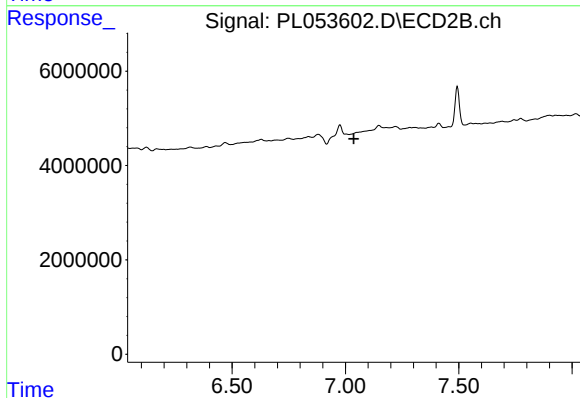


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.037 min
Response: 0
Conc: N.D.

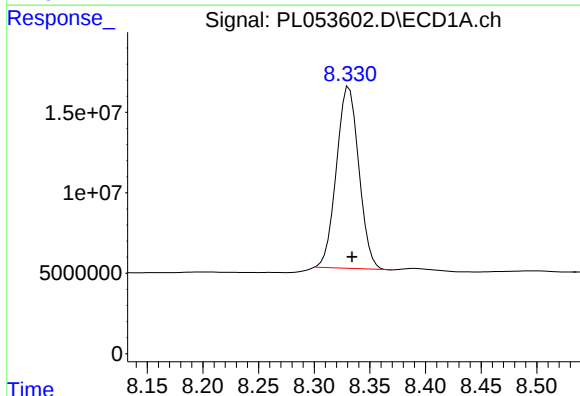

#28 Decachlorobiphenyl

R.T.: 8.331 min
Delta R.T.: -0.003 min
Response: 158307429
Conc: 16.13 ng/ml

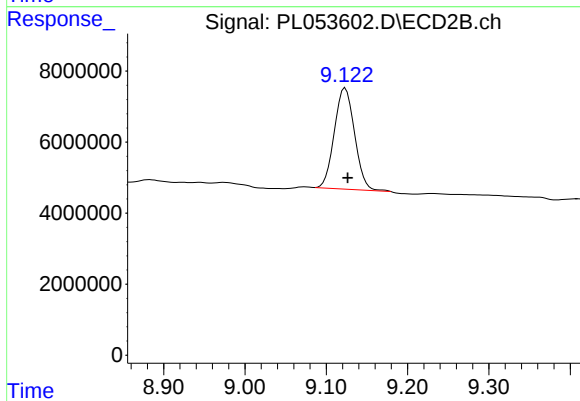

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.003 min
Response: 49276705
Conc: 17.50 ng/ml