

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
 Data File : PL053620.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2019 18:49
 Operator : SG\AJ
 Sample : K5494-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 22:39:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.045	136.1E6	33098095	12.552	13.227
28)	SA Decachlor...	8.329	9.123	101.8E6	32311059	10.377	11.474
Target Compounds							
10)	B gamma-Chl...	0.000	6.167	0	3045015	N.D.	1.044 #
11)	B alpha-Chl...	0.000	6.232	0	6234660	N.D.	2.136 #
12)	B 4,4'-DDE	5.727	6.382	2805518	3623304	0.236	1.287 #
14)	MA Endrin	6.119	0.000	5072745	0	0.438	N.D. #
16)	A 4,4'-DDD	0.000	6.878	0	1041009	N.D.	0.500 #
17)	MA 4,4'-DDT	6.486	7.174	7377181	1790663	0.745	0.774
20)	A Methoxychlor	7.019f	0.000	3900994	0	0.791	N.D. #
25)	Chlordane-3	0.000	6.167	0	3045015	N.D.	8.337 #
26)	Chlordane-4	0.000	6.232	0	6234660	N.D.	13.888 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
Data File : PL053620.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2019 18:49
Operator : SG\AJ
Sample : K5494-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 22:39:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

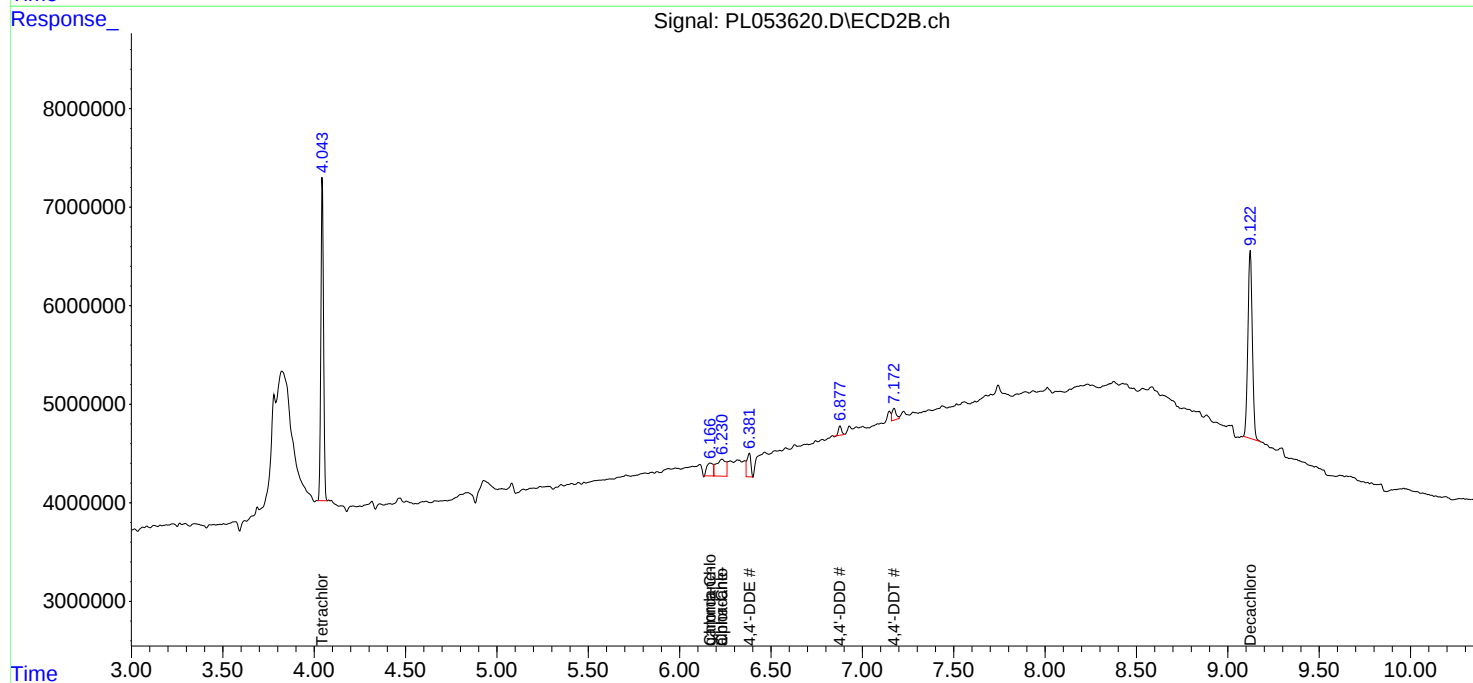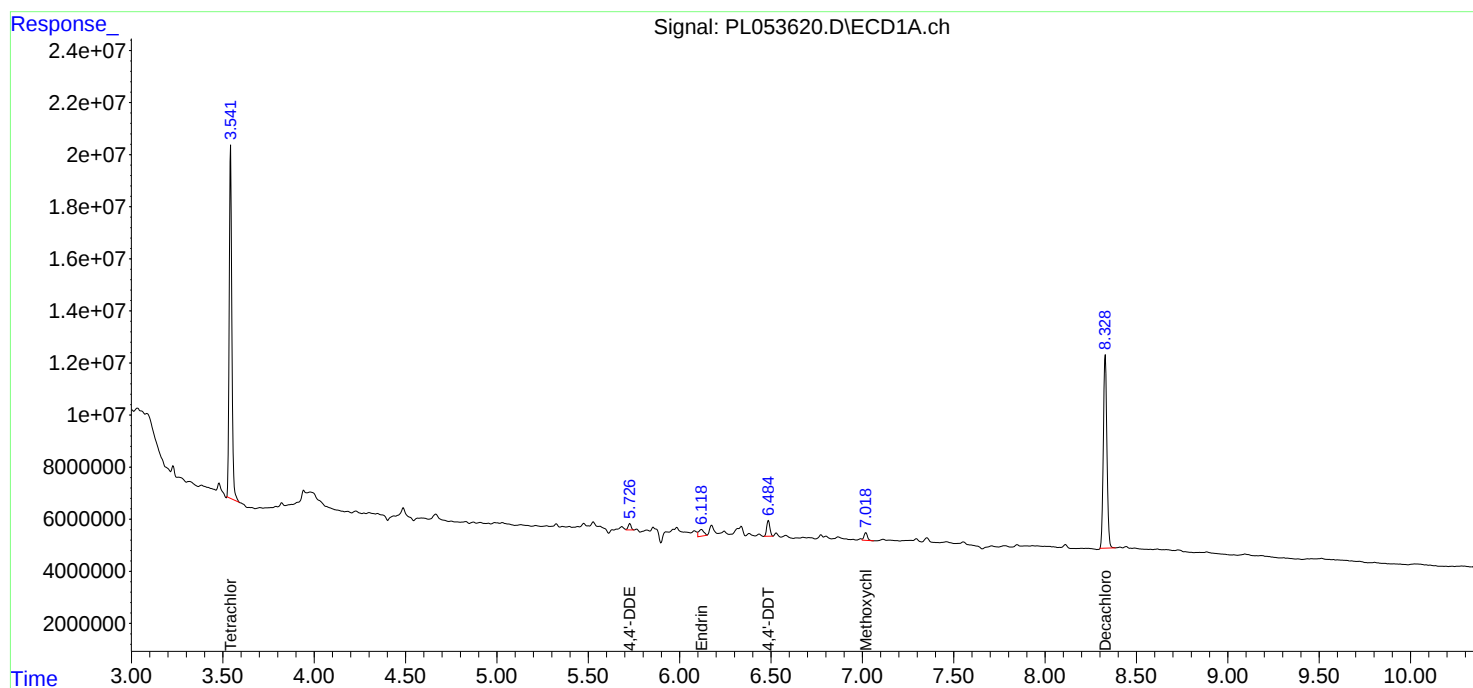


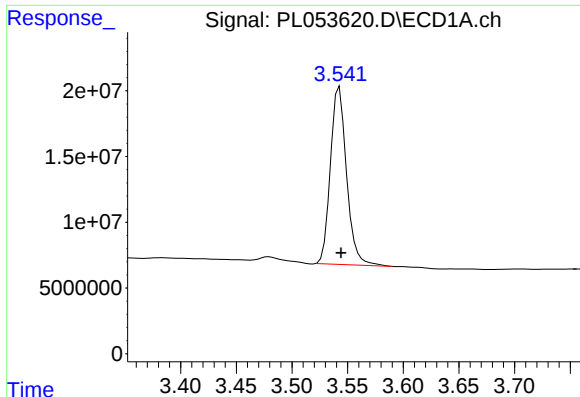

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 136060737
Conc: 12.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

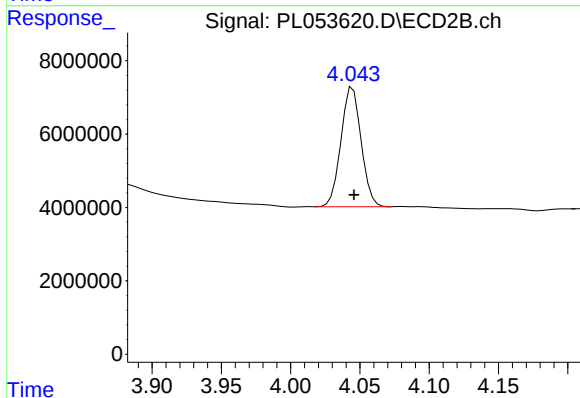


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: -0.001 min
Response: 33098095
Conc: 13.23 ng/ml

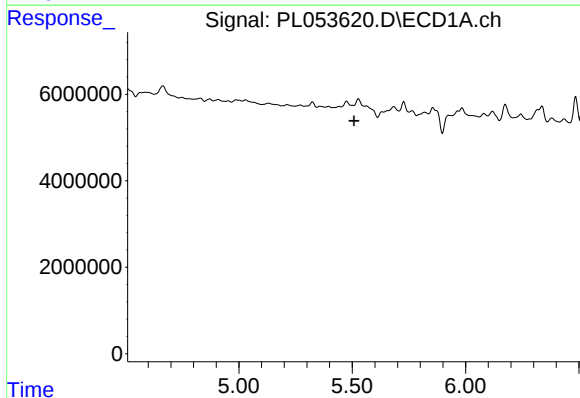


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.509 min
Response: 0
Conc: N.D.

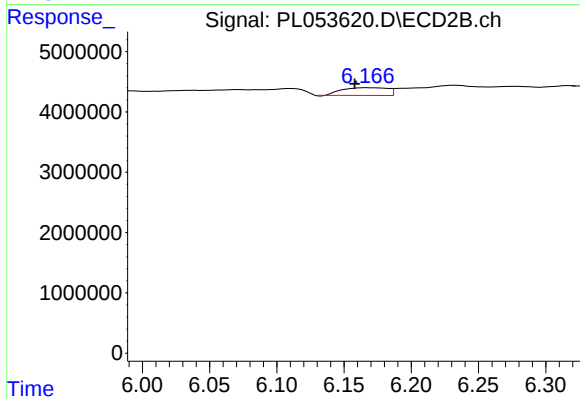

#10 gamma-Chlordane


R.T.: 6.167 min
Delta R.T.: 0.009 min
Response: 3045015
Conc: 1.04 ng/ml

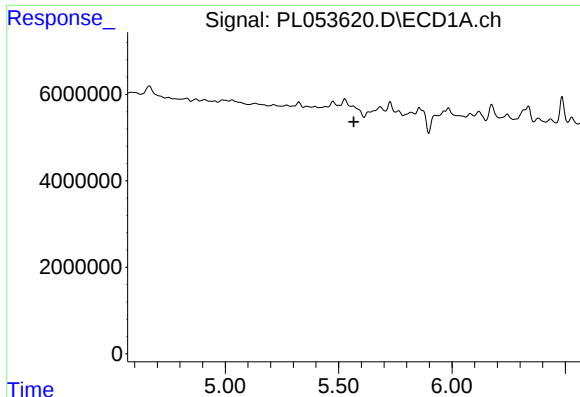

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.568 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

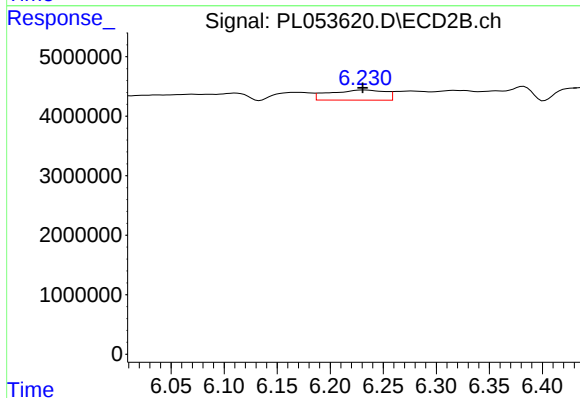


#11 alpha-Chlordane

R.T.: 6.232 min
Delta R.T.: 0.000 min
Response: 6234660
Conc: 2.14 ng/ml

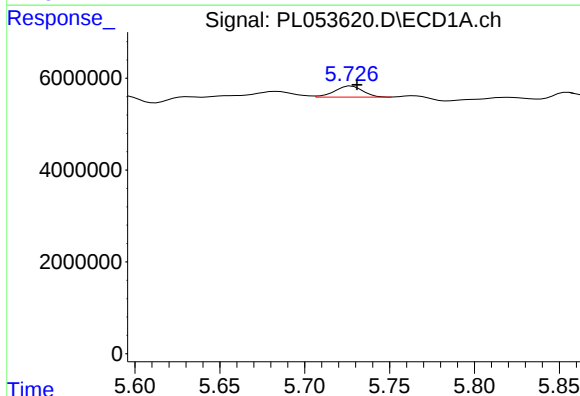


#12 4,4'-DDE

R.T.: 5.727 min
Delta R.T.: -0.003 min
Response: 2805518
Conc: 0.24 ng/ml

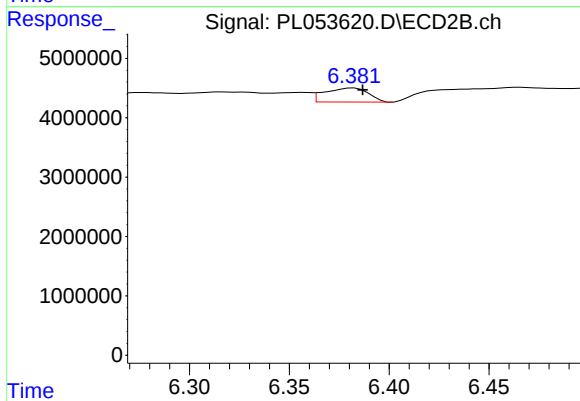

#12 4,4'-DDE


R.T.: 6.382 min
Delta R.T.: -0.004 min
Response: 3623304
Conc: 1.29 ng/ml

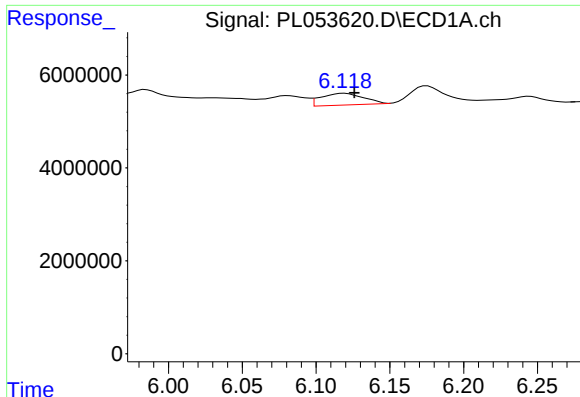

#14 Endrin


R.T.: 6.119 min
Delta R.T.: -0.007 min
Response: 5072745
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

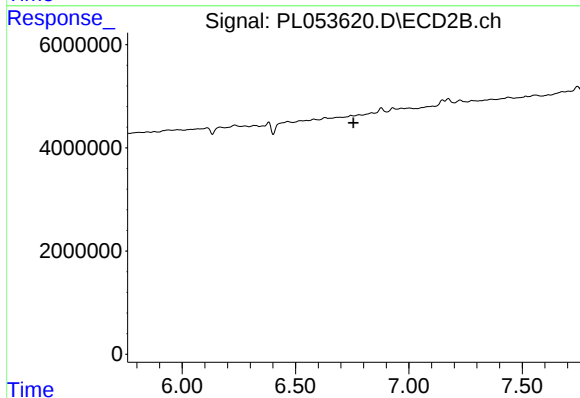


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.756 min
Response: 0
Conc: N.D.

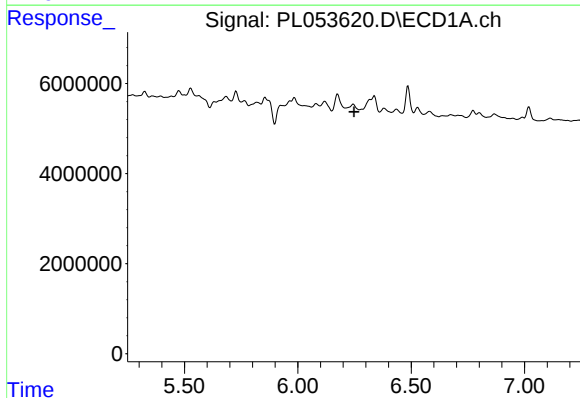


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.248 min
Response: 0
Conc: N.D.

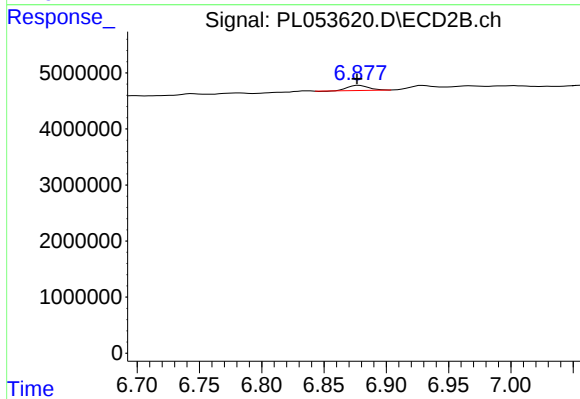

#16 4,4'-DDD


R.T.: 6.878 min
Delta R.T.: 0.002 min
Response: 1041009
Conc: 0.50 ng/ml

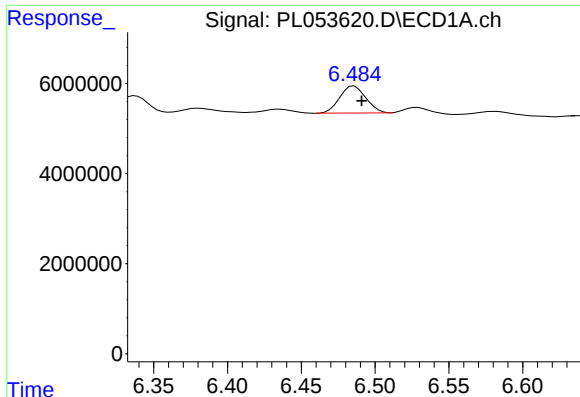

#17 4,4'-DDT


R.T.: 6.486 min
Delta R.T.: -0.005 min
Response: 7377181
Conc: 0.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

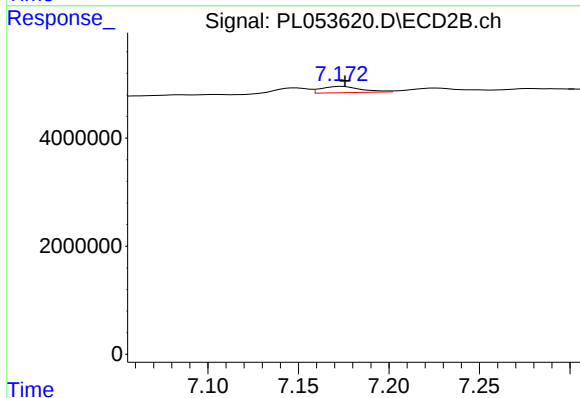


#17 4,4'-DDT

R.T.: 7.174 min
Delta R.T.: -0.001 min
Response: 1790663
Conc: 0.77 ng/ml

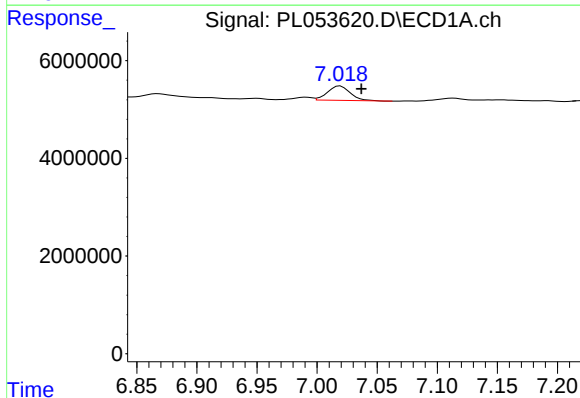


#20 Methoxychlor

R.T.: 7.019 min
Delta R.T.: -0.018 min
Response: 3900994
Conc: 0.79 ng/ml

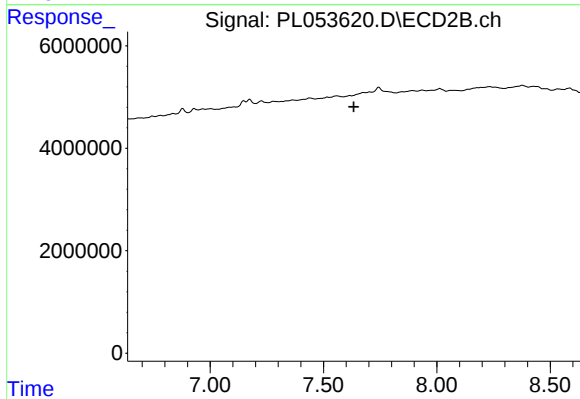

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.633 min
Response: 0
Conc: N.D.

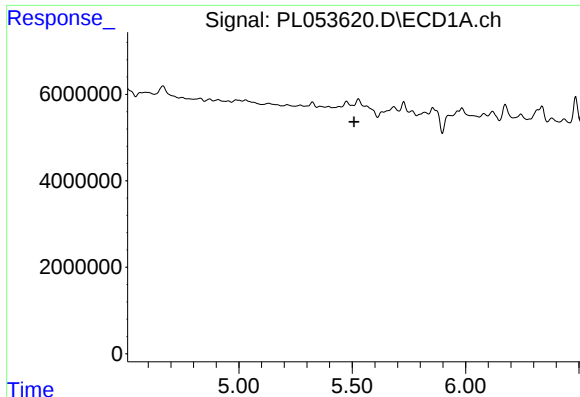

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

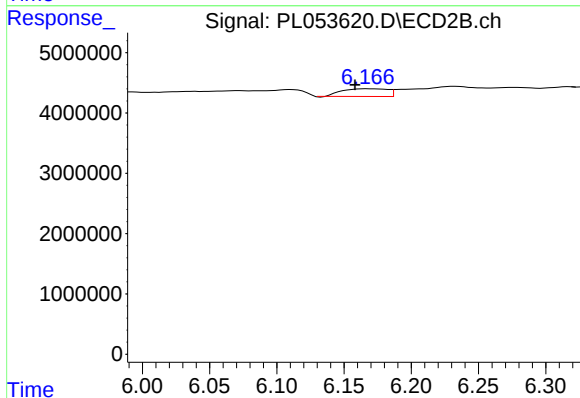


#25 Chlordane-3

R.T.: 6.167 min
Delta R.T.: 0.009 min
Response: 3045015
Conc: 8.34 ng/ml

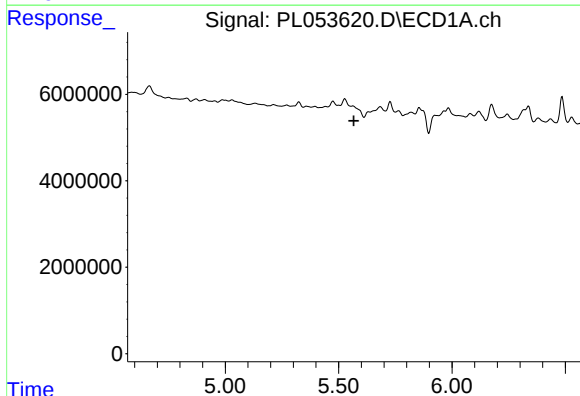


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.568 min
Response: 0
Conc: N.D.

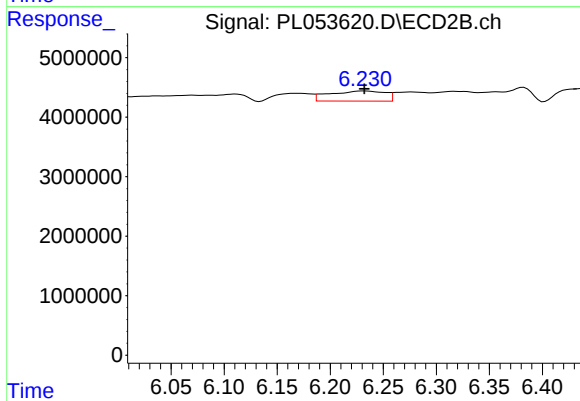

#26 Chlordane-4

R.T.: 6.232 min
Delta R.T.: 0.000 min
Response: 6234660
Conc: 13.89 ng/ml

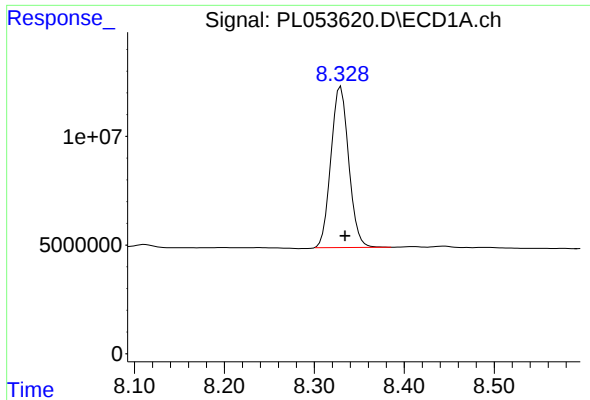

#28 Decachlorobiphenyl


R.T.: 8.329 min

Delta R.T.: -0.005 min

Response: 101812692

Conc: 10.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

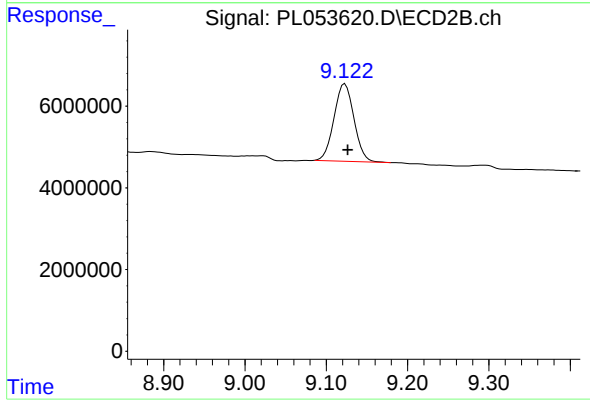

#28 Decachlorobiphenyl

R.T.: 9.123 min

Delta R.T.: -0.003 min

Response: 32311059

Conc: 11.47 ng/ml