

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
 Data File : PL053623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2019 19:31
 Operator : SG\AJ
 Sample : PB124213BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 22:39:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.044	205.2E6	50602532	18.935	20.222
28)	SA Decachlor...	8.330	9.122	168.9E6	51500582	17.210	18.288
Target Compounds							
15)	B Endosulfa...	0.000	6.972	0	4213815	N.D.	1.650 #
17)	MA 4,4'-DDT	0.000	7.153f	0	4564838	N.D.	1.974 #
20)	A Methoxychlor	7.034	0.000	4032422	0	0.818	N.D. #
27)	Chlordane-5	6.435f	0.000	44933002	0	122.921	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
Data File : PL053623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2019 19:31
Operator : SG\AJ
Sample : PB124213BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 22:39:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

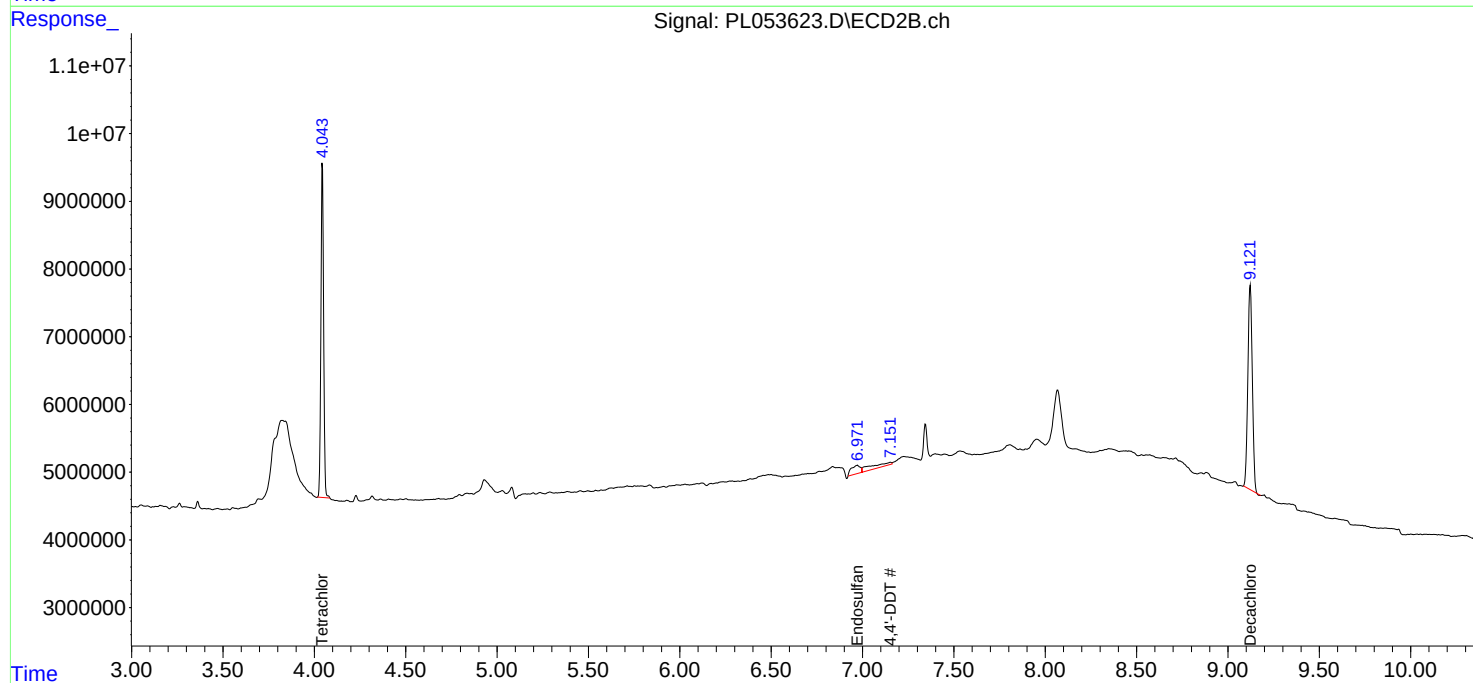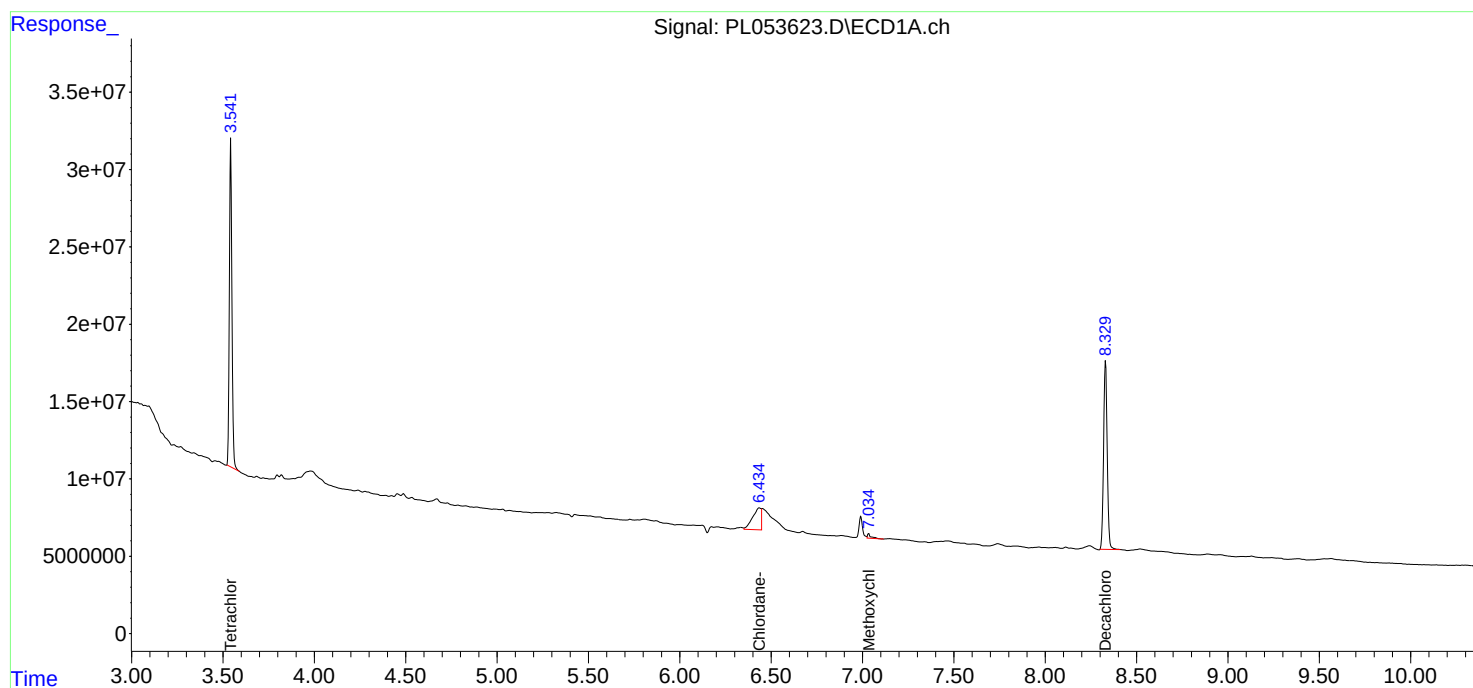


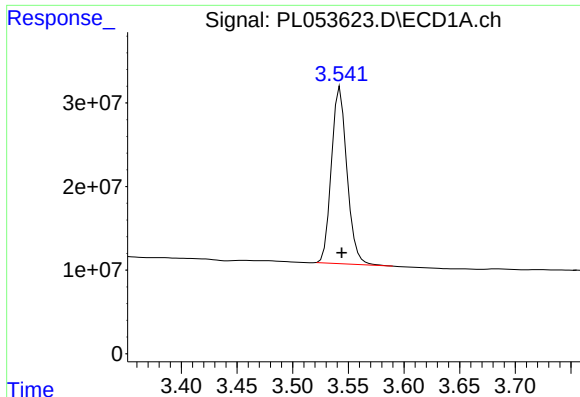

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 205239840
Conc: 18.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

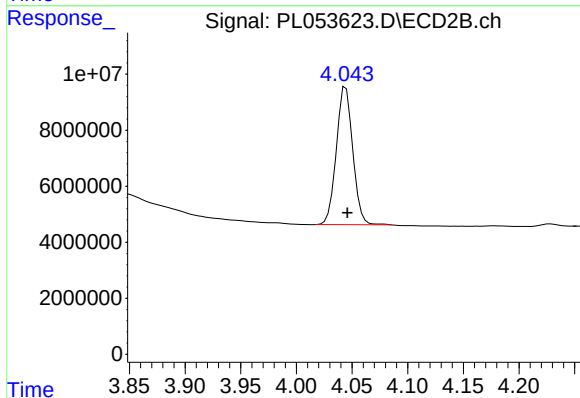


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.001 min
Response: 50602532
Conc: 20.22 ng/ml

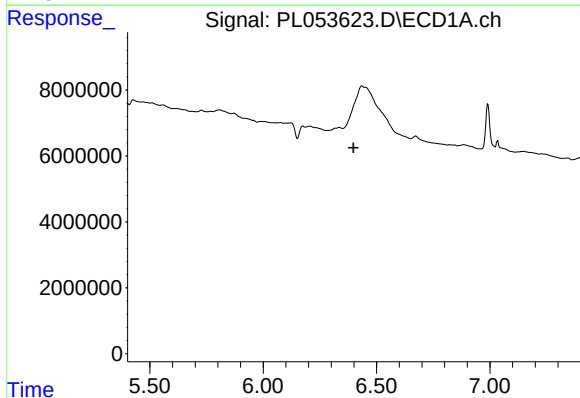


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

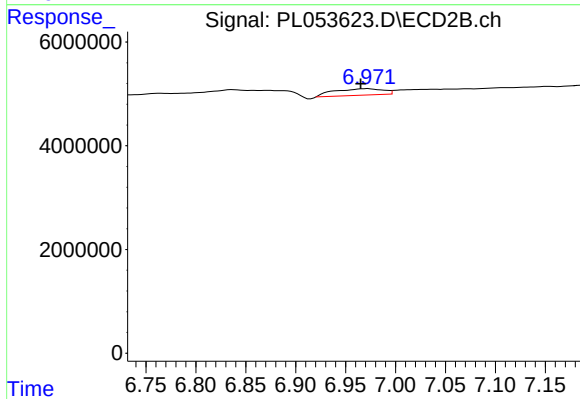

#15 Endosulfan II


R.T.: 6.972 min
Delta R.T.: 0.007 min
Response: 4213815
Conc: 1.65 ng/ml

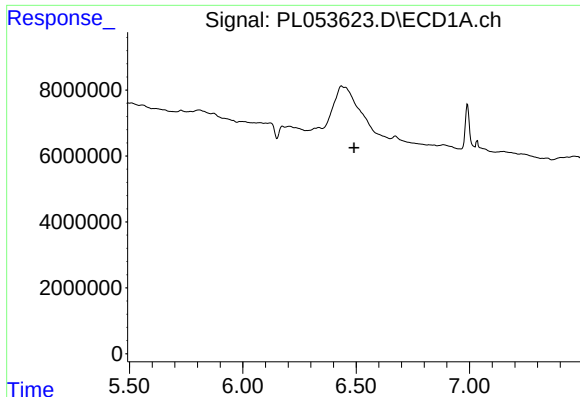

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

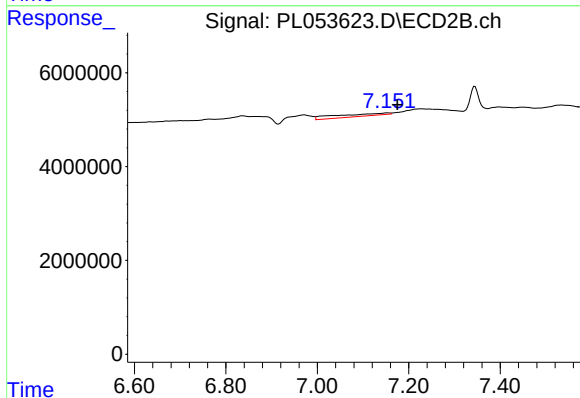


#17 4,4'-DDT

R.T.: 7.153 min
Delta R.T.: -0.023 min
Response: 4564838
Conc: 1.97 ng/ml

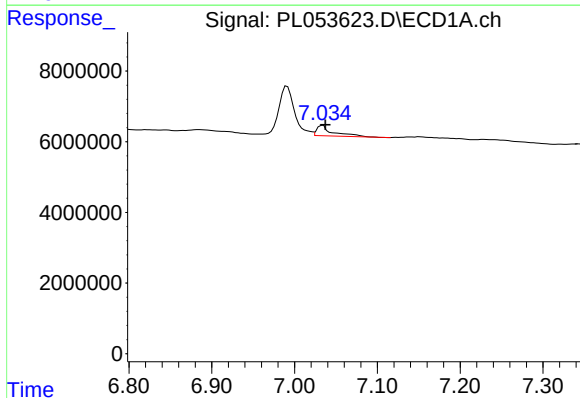


#20 Methoxychlor

R.T.: 7.034 min
Delta R.T.: -0.003 min
Response: 4032422
Conc: 0.82 ng/ml

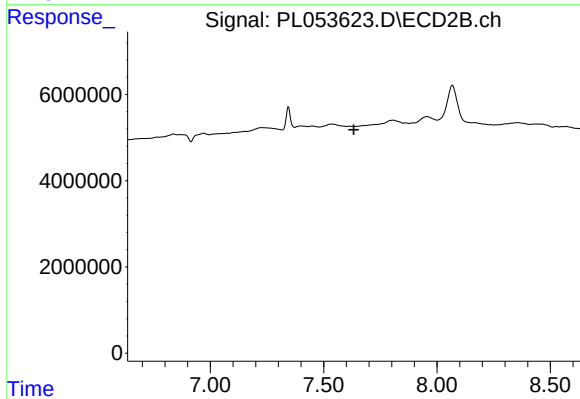

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.633 min
Response: 0
Conc: N.D.

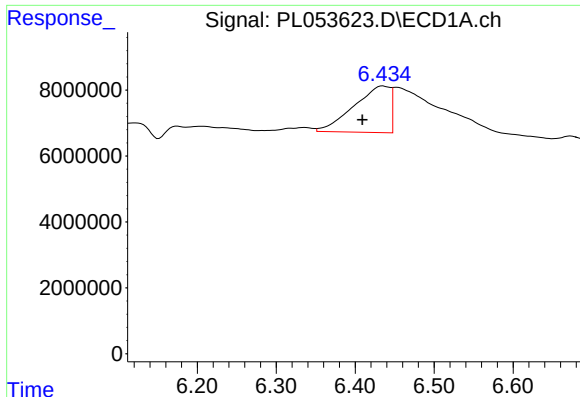

#27 Chlordane-5


R.T.: 6.435 min
Delta R.T.: 0.026 min
Response: 44933002
Conc: 122.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

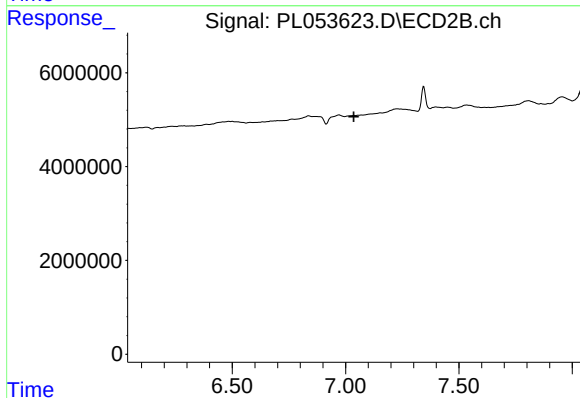


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.037 min
Response: 0
Conc: N.D.

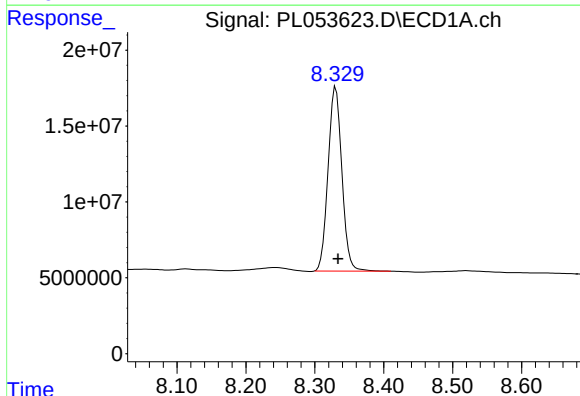

#28 Decachlorobiphenyl

R.T.: 8.330 min
Delta R.T.: -0.004 min
Response: 168855618
Conc: 17.21 ng/ml

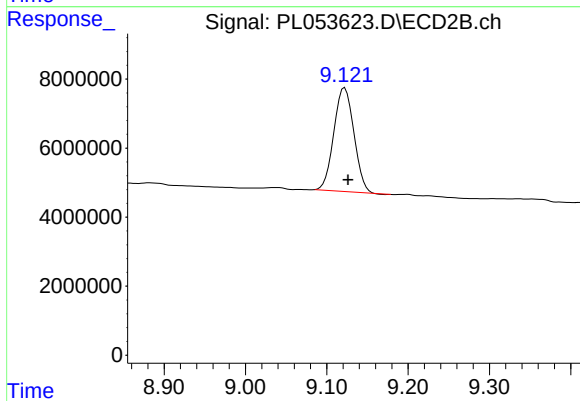

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.004 min
Response: 51500582
Conc: 18.29 ng/ml