

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
 Data File : PL053660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2019 05:17
 Operator : SG\AJ
 Sample : K5497-19 10X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 05:48:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.044	17772882	4538643	1.640	1.814
28)	SA Decachlor...	8.329	9.120	16464358	3281205	1.678	1.165 #
Target Compounds							
6)	B beta-BHC	4.524	0.000	2802126	0	0.425	N.D. #
10)	B gamma-Chl...	5.506	6.155	2933659	1404593	0.215	0.481 #
11)	B alpha-Chl...	0.000	6.230	0	2175970	N.D.	0.745 #
12)	B 4,4'-DDE	5.727	6.384	8098666	2534299	0.682	0.900 #
14)	MA Endrin	6.120	6.780f	6119014	554614	0.528	0.228 #
16)	A 4,4'-DDD	6.244	0.000	3117800	0	0.350	N.D. #
17)	MA 4,4'-DDT	6.487	7.173	19023487	5754555	1.920	2.488 #
25)	Chlordane-3	5.506	6.155	2933659	1404593	2.545	3.846 #
26)	Chlordane-4	0.000	6.230	0	2175970	N.D.	4.847 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
Data File : PL053660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2019 05:17
Operator : SG\AJ
Sample : K5497-19 10X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 05:48:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

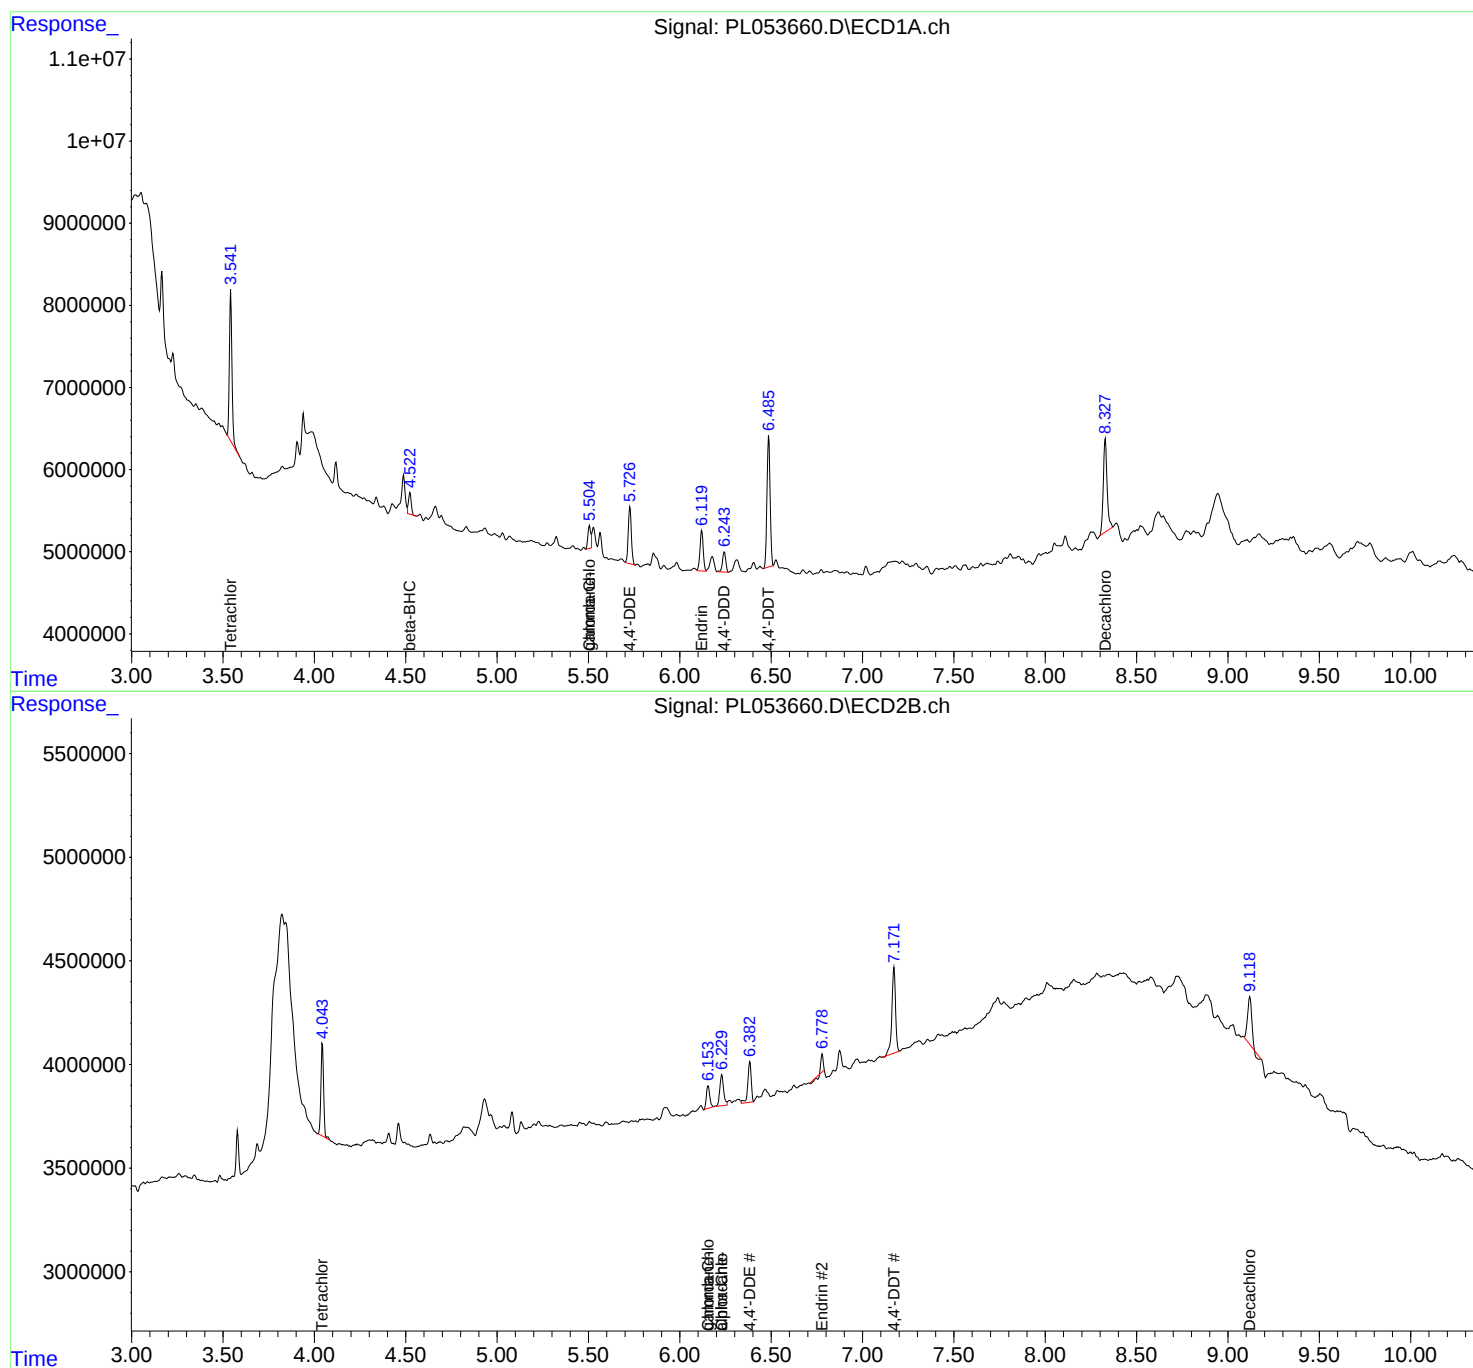


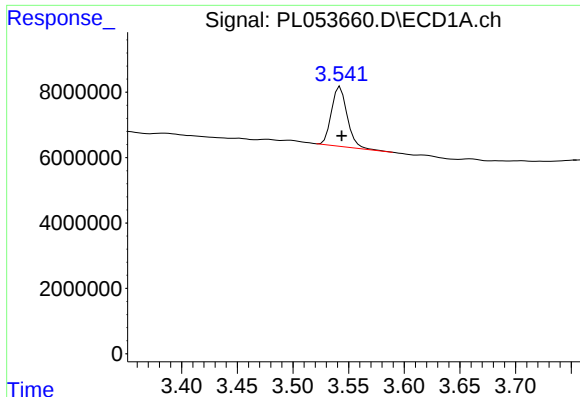

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 17772882
Conc: 1.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

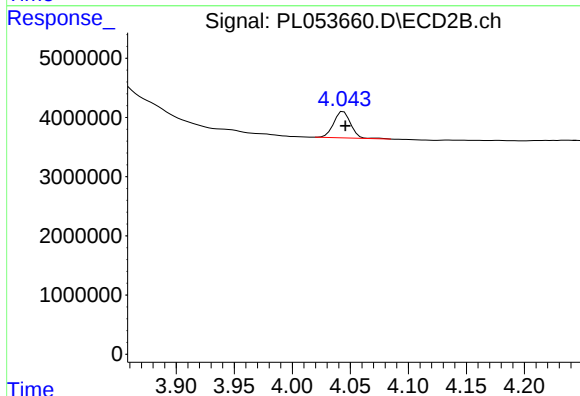


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 4538643
Conc: 1.81 ng/ml

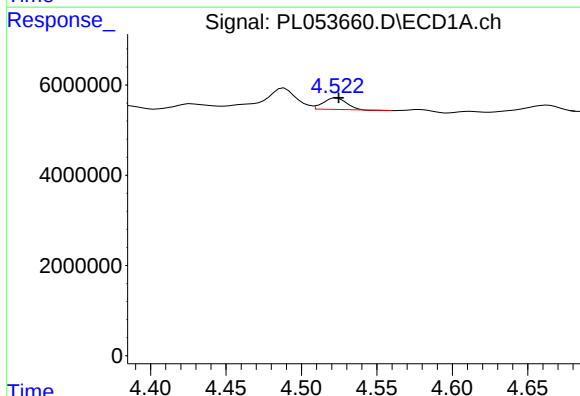


#6 beta-BHC

R.T.: 4.524 min
Delta R.T.: -0.001 min
Response: 2802126
Conc: 0.43 ng/ml

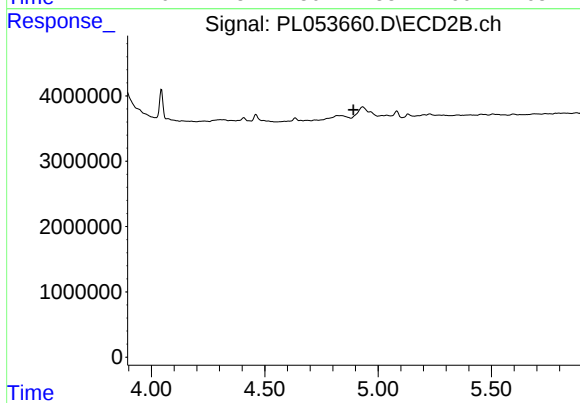

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.892 min
Response: 0
Conc: N.D.

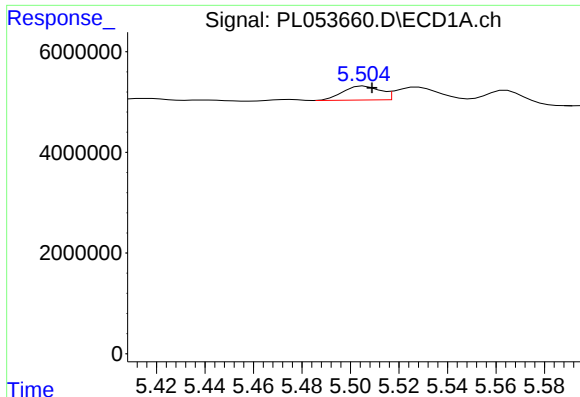

#10 gamma-Chlordane


R.T.: 5.506 min
Delta R.T.: -0.003 min
Response: 2933659
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

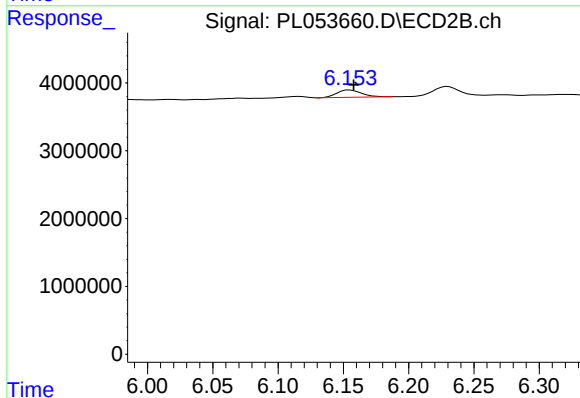


#10 gamma-Chlordane

R.T.: 6.155 min
Delta R.T.: -0.003 min
Response: 1404593
Conc: 0.48 ng/ml

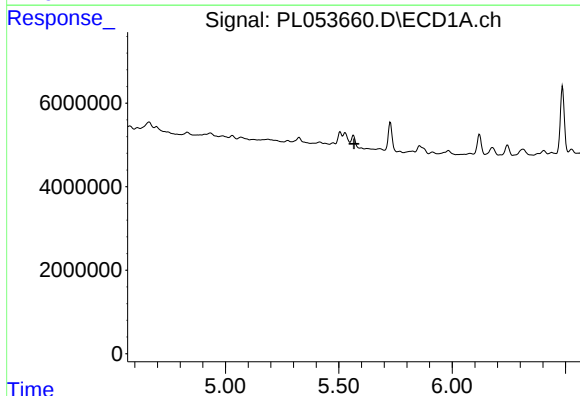


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.568 min
Response: 0
Conc: N.D.

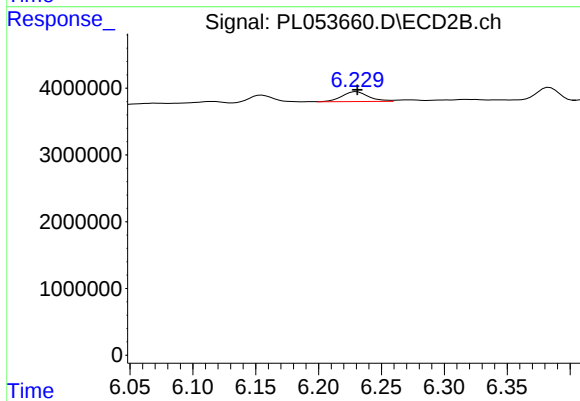

#11 alpha-Chlordane


R.T.: 6.230 min
Delta R.T.: 0.000 min
Response: 2175970
Conc: 0.75 ng/ml

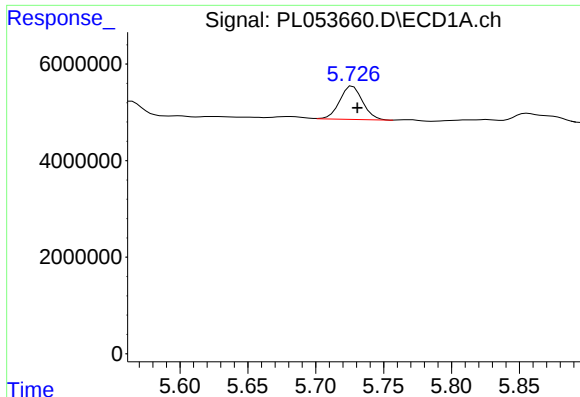

#12 4,4'-DDE


R.T.: 5.727 min
Delta R.T.: -0.004 min
Response: 8098666
Conc: 0.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

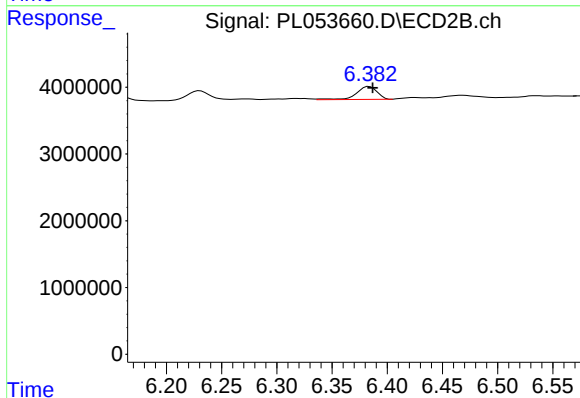


#12 4,4'-DDE

R.T.: 6.384 min
Delta R.T.: -0.003 min
Response: 2534299
Conc: 0.90 ng/ml

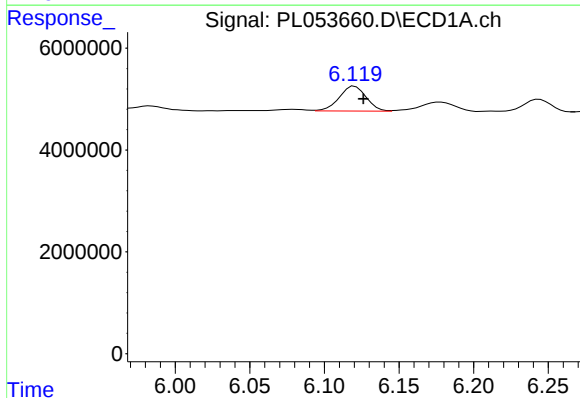


#14 Endrin

R.T.: 6.120 min
Delta R.T.: -0.006 min
Response: 6119014
Conc: 0.53 ng/ml

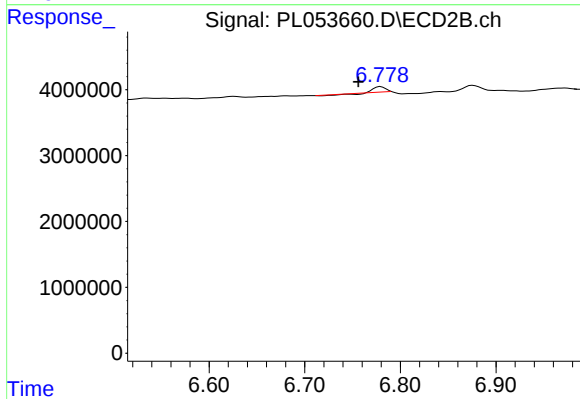

#14 Endrin


R.T.: 6.780 min
Delta R.T.: 0.023 min
Response: 554614
Conc: 0.23 ng/ml

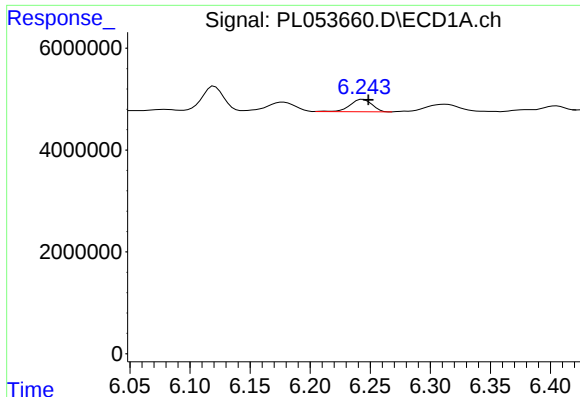

#16 4,4'-DDD


R.T.: 6.244 min
Delta R.T.: -0.004 min
Response: 3117800
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

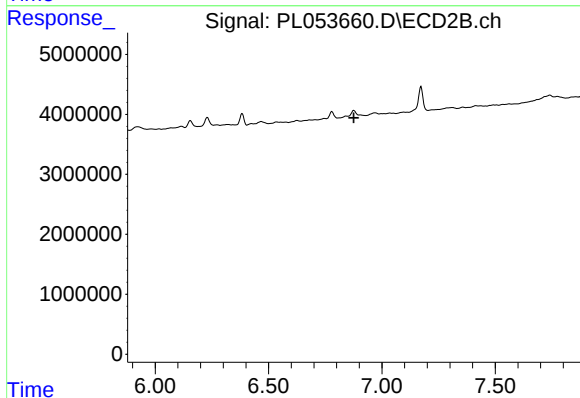


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.877 min
Response: 0
Conc: N.D.

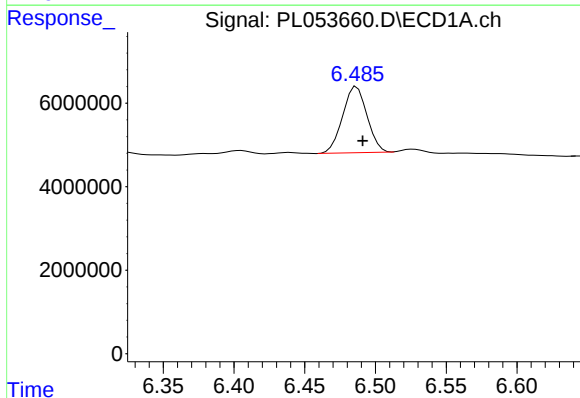


#17 4,4'-DDT

R.T.: 6.487 min
Delta R.T.: -0.004 min
Response: 19023487
Conc: 1.92 ng/ml

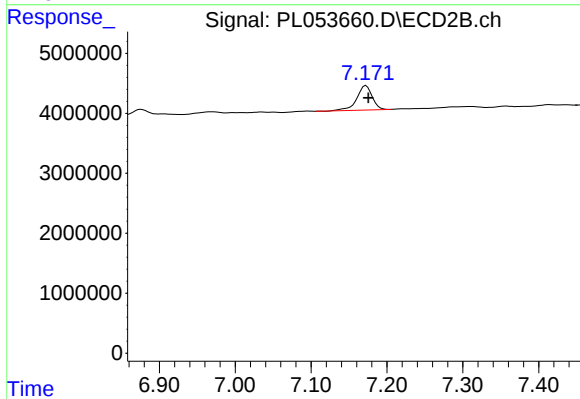

#17 4,4'-DDT


R.T.: 7.173 min
Delta R.T.: -0.003 min
Response: 5754555
Conc: 2.49 ng/ml

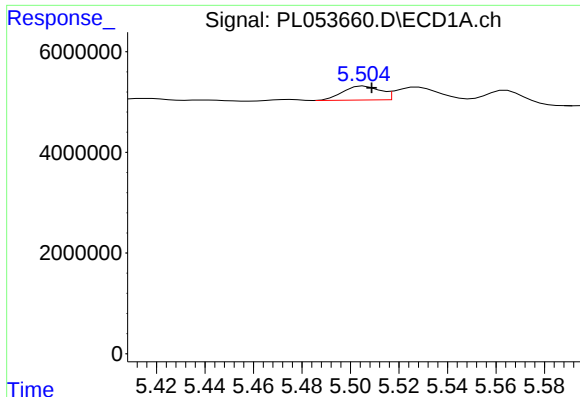

#25 Chlordane-3


R.T.: 5.506 min
Delta R.T.: -0.003 min
Response: 2933659
Conc: 2.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

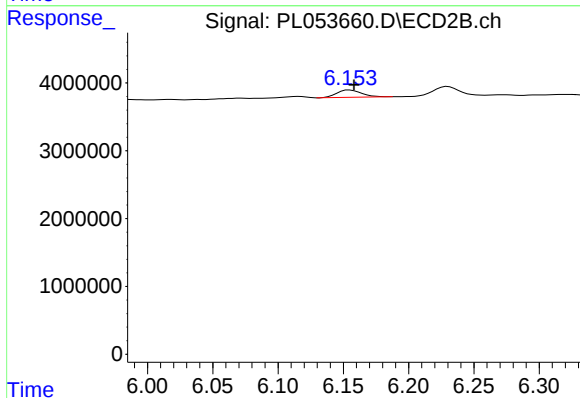


#25 Chlordane-3

R.T.: 6.155 min
Delta R.T.: -0.003 min
Response: 1404593
Conc: 3.85 ng/ml

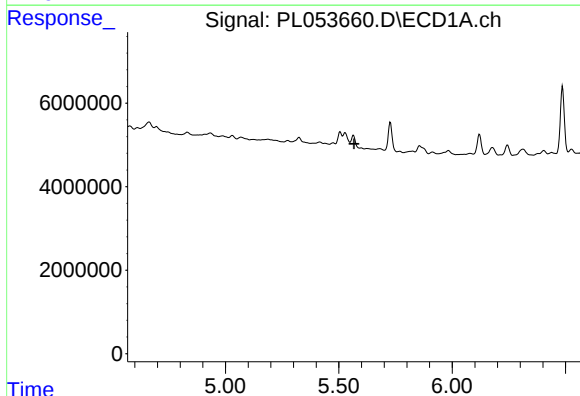


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.568 min
Response: 0
Conc: N.D.

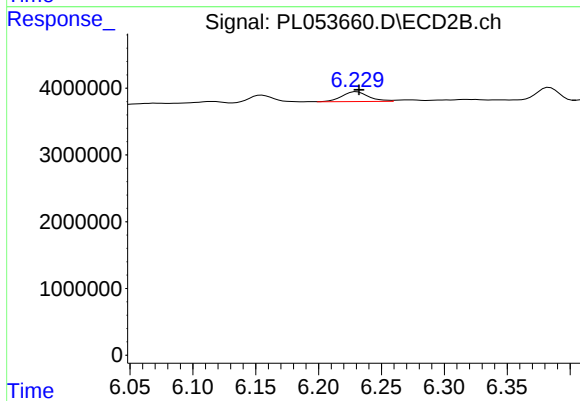

#26 Chlordane-4


R.T.: 6.230 min
Delta R.T.: -0.002 min
Response: 2175970
Conc: 4.85 ng/ml

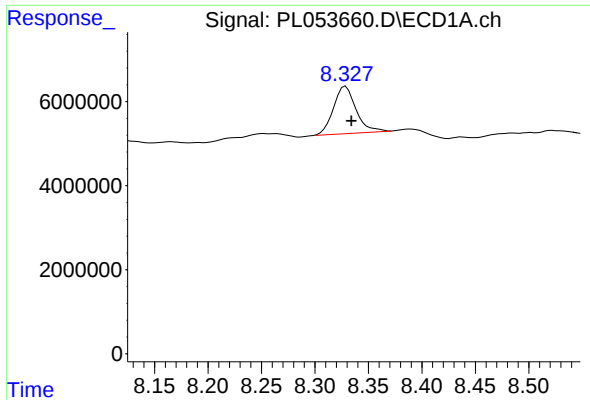

#28 Decachlorobiphenyl

R.T.: 8.329 min
Delta R.T.: -0.005 min
Response: 16464358
Conc: 1.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

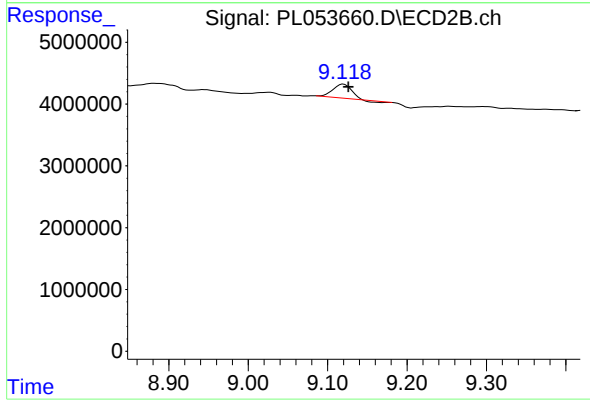

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: -0.006 min
Response: 3281205
Conc: 1.17 ng/ml