

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
 Data File : PL053596.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2019 13:14
 Operator : SG\AJ
 Sample : K5139-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BU-03-102119

Manual Integrations
 APPROVED

Ankita
 10/24/2019 1:59:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 22:35:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.045	130.2E6	30648175	12.015	12.248
28)	SA Decachlor...	8.331	9.124	89042955	27261890	9.075	9.681
Target Compounds							
12)	B 4,4'-DDE	5.729	6.385	16412754	5859154	1.381	2.080 #
17)	MA 4,4'-DDT	6.488	7.173	15199582	4699434	1.534m	2.032m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
Data File : PL053596.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2019 13:14
Operator : SG\AJ
Sample : K5139-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
BU-03-102119


Manual Integrations
APPROVED

Ankita
10/24/2019 1:59:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 22:35:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

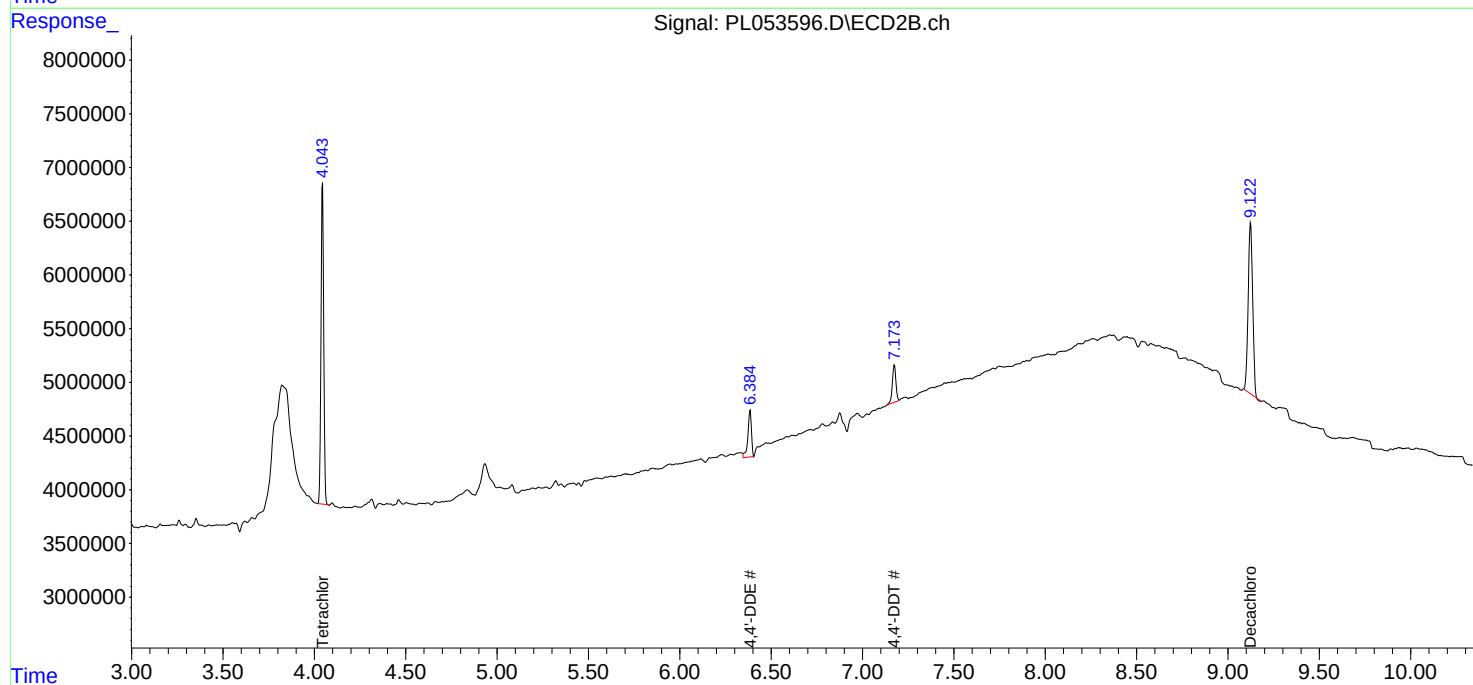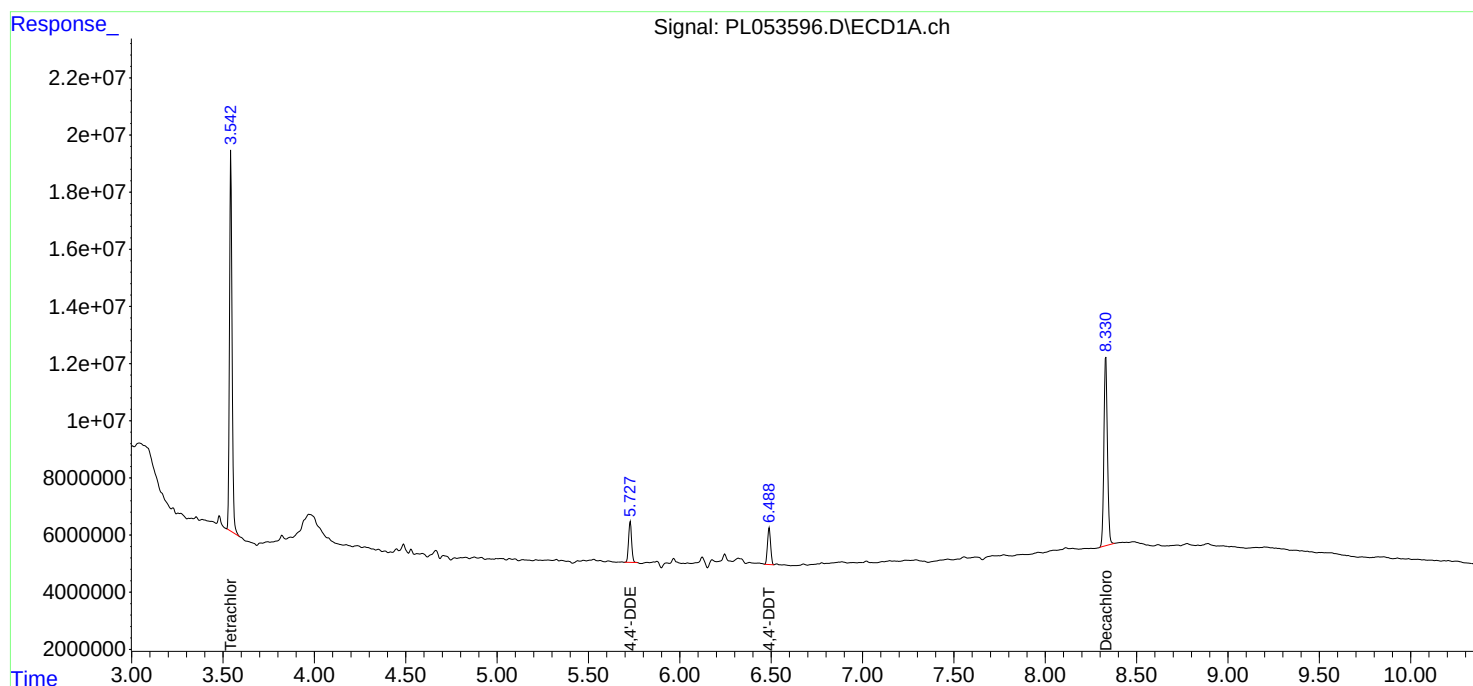

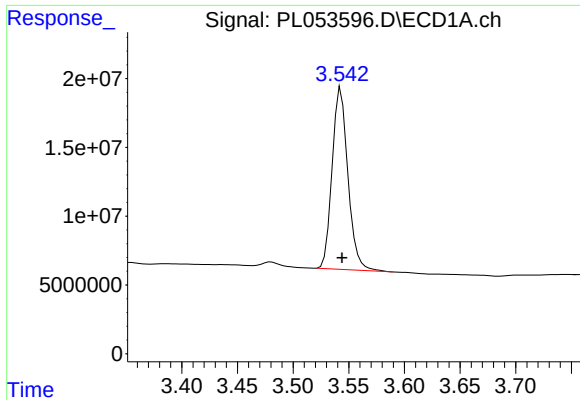


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 130231429
Conc: 12.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
BU-03-102119


Manual Integrations
APPROVED

Ankita
10/24/2019 1:59:14 PM

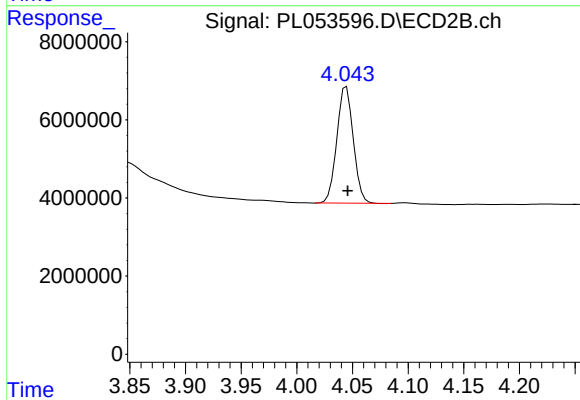


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: -0.001 min
Response: 30648175
Conc: 12.25 ng/ml

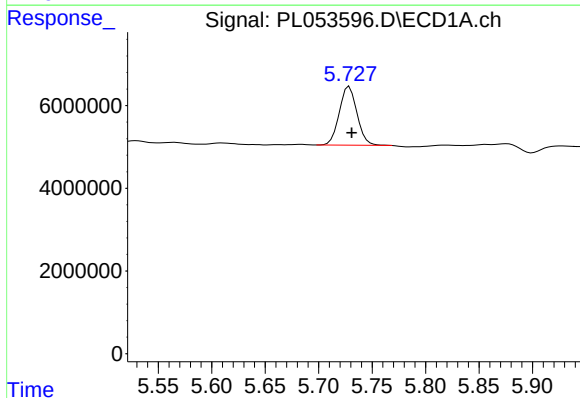


#12 4,4'-DDE

R.T.: 5.729 min
Delta R.T.: -0.002 min
Response: 16412754
Conc: 1.38 ng/ml

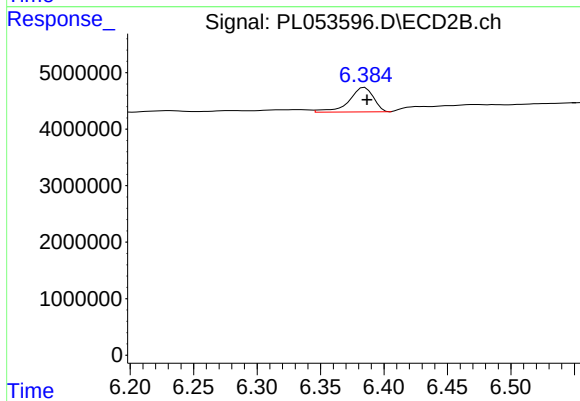

#12 4,4'-DDE

R.T.: 6.385 min
Delta R.T.: -0.002 min
Response: 5859154
Conc: 2.08 ng/ml

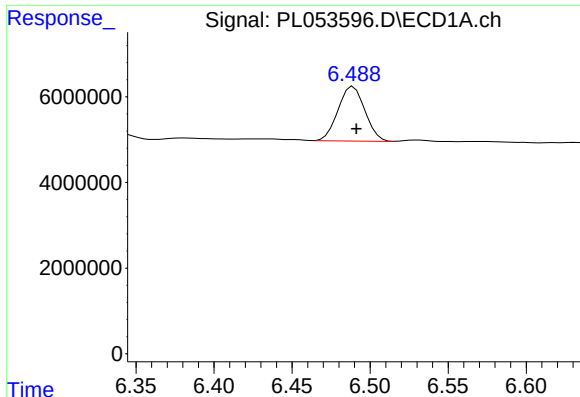


#17 4,4'-DDT

R.T.: 6.488 min
Delta R.T.: -0.003 min
Response: 15199582
Conc: 1.53 ng/ml m

Instrument :
ECD_L
ClientSampleId :
BU-03-102119


Manual Integrations
APPROVED

Ankita
10/24/2019 1:59:14 PM

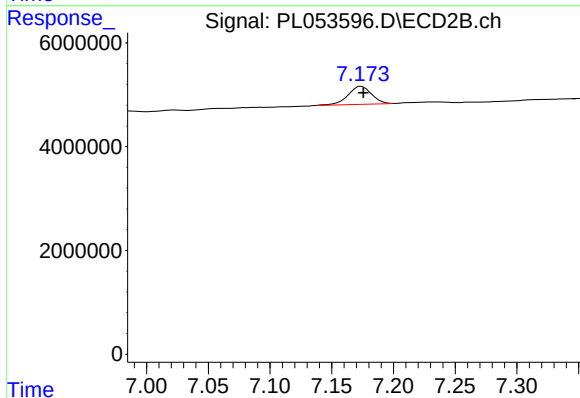


#17 4,4'-DDT

R.T.: 7.173 min
Delta R.T.: -0.003 min
Response: 4699434
Conc: 2.03 ng/ml m

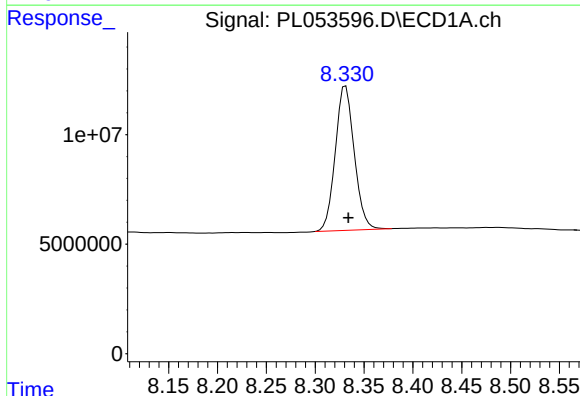

#28 Decachlorobiphenyl

R.T.: 8.331 min
Delta R.T.: -0.003 min
Response: 89042955
Conc: 9.08 ng/ml

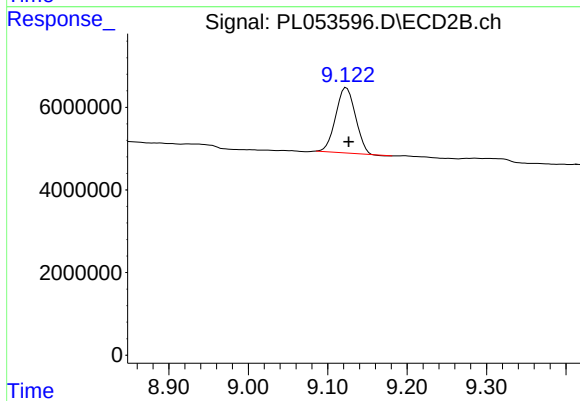

#28 Decachlorobiphenyl

R.T.: 9.124 min
Delta R.T.: -0.003 min
Response: 27261890
Conc: 9.68 ng/ml