

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
 Data File : PL053605.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2019 15:19
 Operator : SG\AJ
 Sample : K5494-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP1-2FT

Manual Integrations
 APPROVED

Ankita
 10/24/2019 2:00:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 22:36:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.045	257.6E6	59901853	23.762	23.938
28)	SA Decachlor...	8.330	9.125	173.2E6	52954043	17.654	18.805
Target Compounds							
16)	A 4,4'-DDD	6.247	6.874	6062843	4091467	0.681	1.963m#
17)	MA 4,4'-DDT	6.487	7.174	14114532	3422929	1.425	1.480m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
Data File : PL053605.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2019 15:19
Operator : SG\AJ
Sample : K5494-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP1-2FT


Manual Integrations
APPROVED

Ankita
10/24/2019 2:00:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 22:36:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

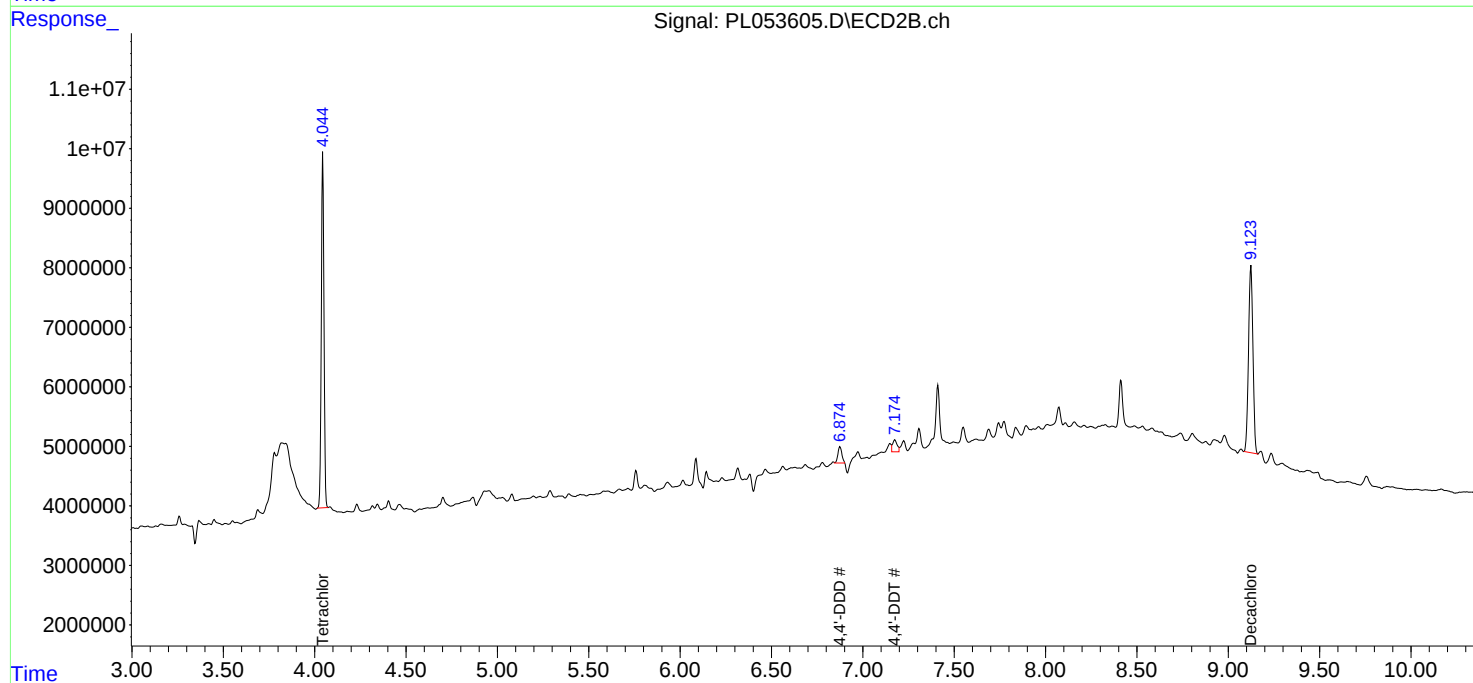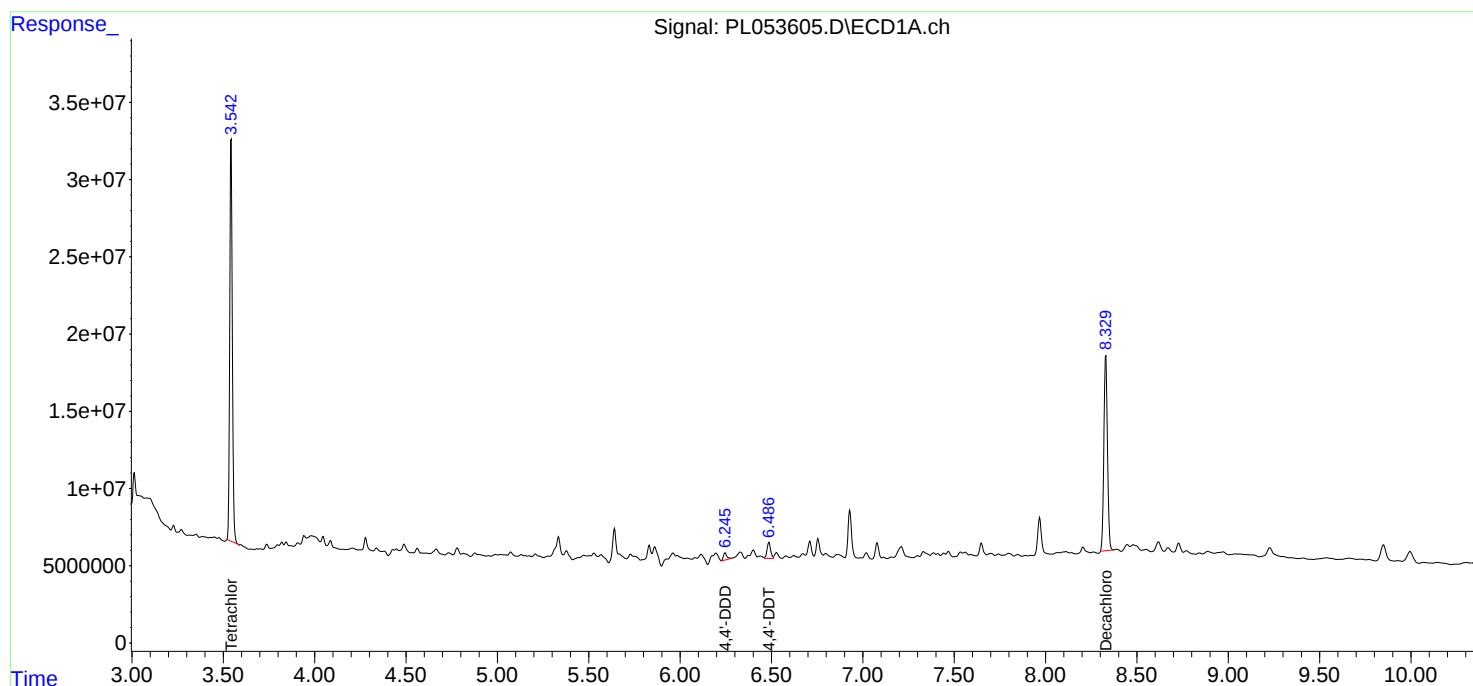

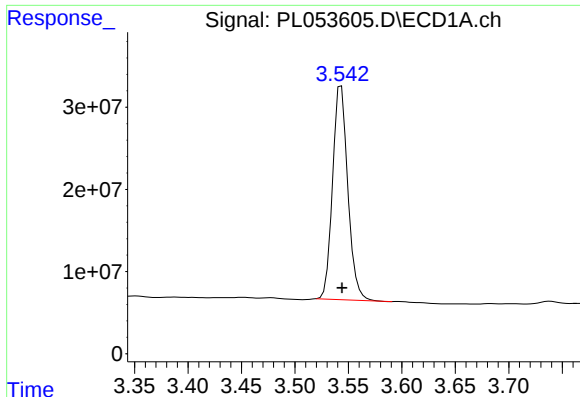


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 257561422
Conc: 23.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP1-2FT


Manual Integrations
APPROVED

Ankita
10/24/2019 2:00:46 PM

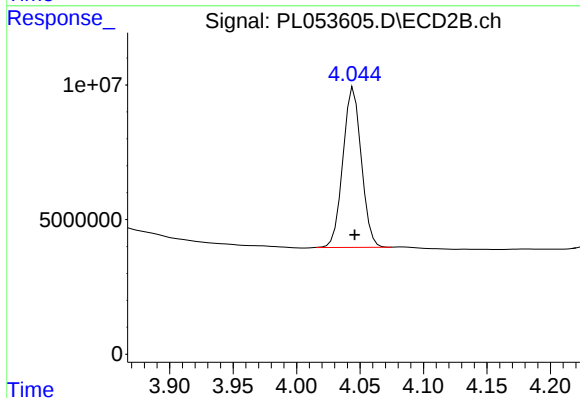


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 59901853
Conc: 23.94 ng/ml

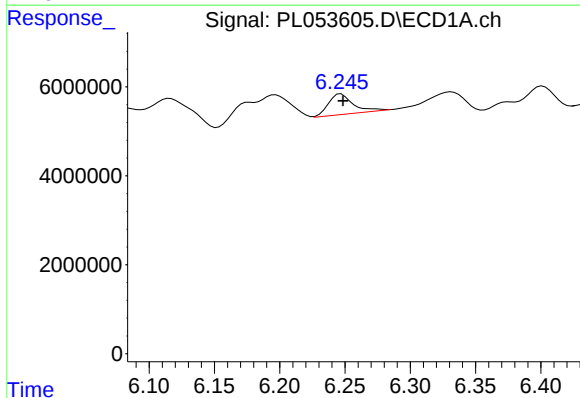


#16 4,4'-DDD

R.T.: 6.247 min
Delta R.T.: -0.002 min
Response: 6062843
Conc: 0.68 ng/ml

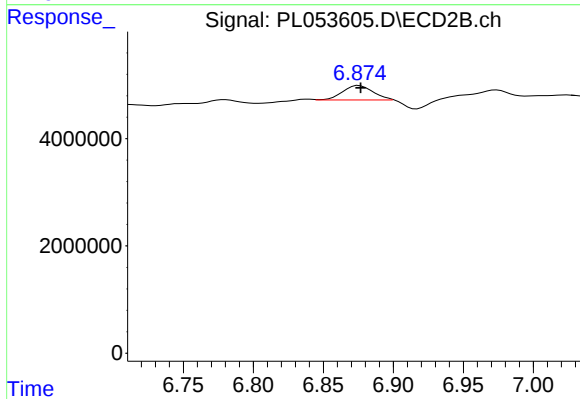

#16 4,4'-DDD

R.T.: 6.874 min
Delta R.T.: -0.003 min
Response: 4091467
Conc: 1.96 ng/ml m

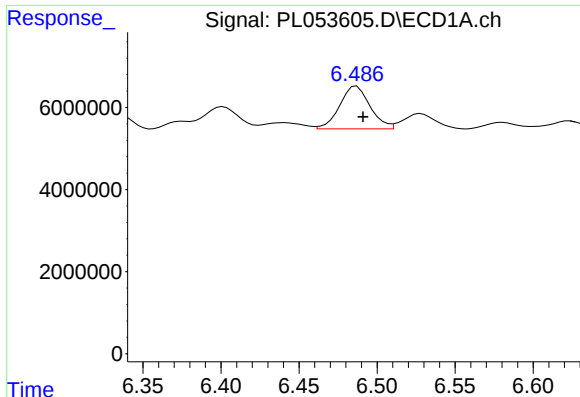


#17 4,4'-DDT

R.T.: 6.487 min
Delta R.T.: -0.004 min
Response: 14114532
Conc: 1.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP1-2FT


Manual Integrations
APPROVED

Ankita
10/24/2019 2:00:46 PM

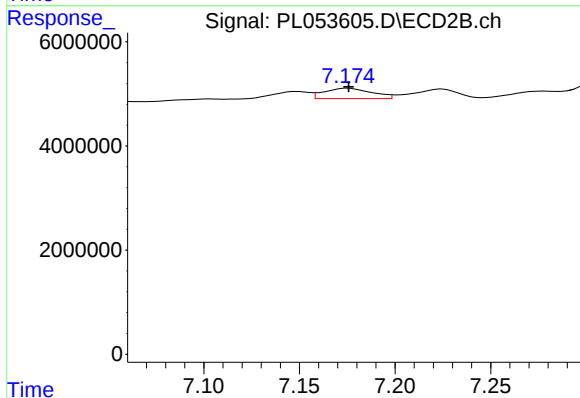


#17 4,4'-DDT

R.T.: 7.174 min
Delta R.T.: -0.002 min
Response: 3422929
Conc: 1.48 ng/ml m

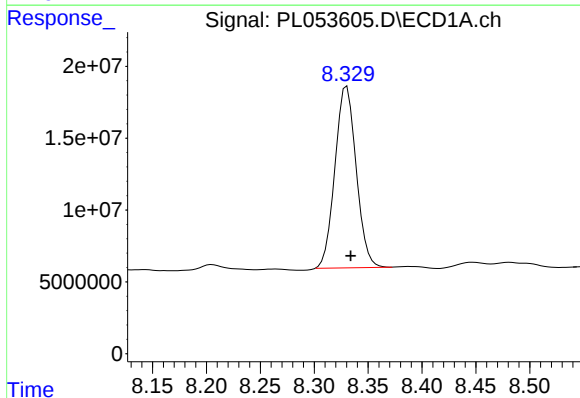

#28 Decachlorobiphenyl

R.T.: 8.330 min
Delta R.T.: -0.004 min
Response: 173213453
Conc: 17.65 ng/ml

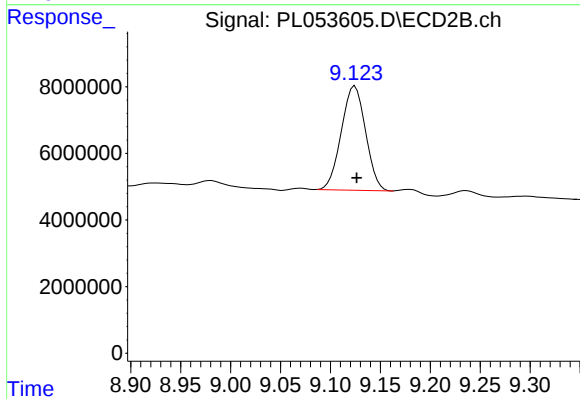

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: -0.002 min
Response: 52954043
Conc: 18.80 ng/ml