

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
 Data File : PL053624.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2019 20:12
 Operator : SG\AJ
 Sample : K5489-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MAIN-STOCKPILE-SLP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 22:40:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.044	202.2E6	49779734	18.654	19.893
28)	SA Decachlor...	8.330	9.121	128.6E6	40909314	13.112	14.527

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
Data File : PL053624.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2019 20:12
Operator : SG\AJ
Sample : K5489-03
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MAIN-STOCKPILE-SLP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 22:40:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

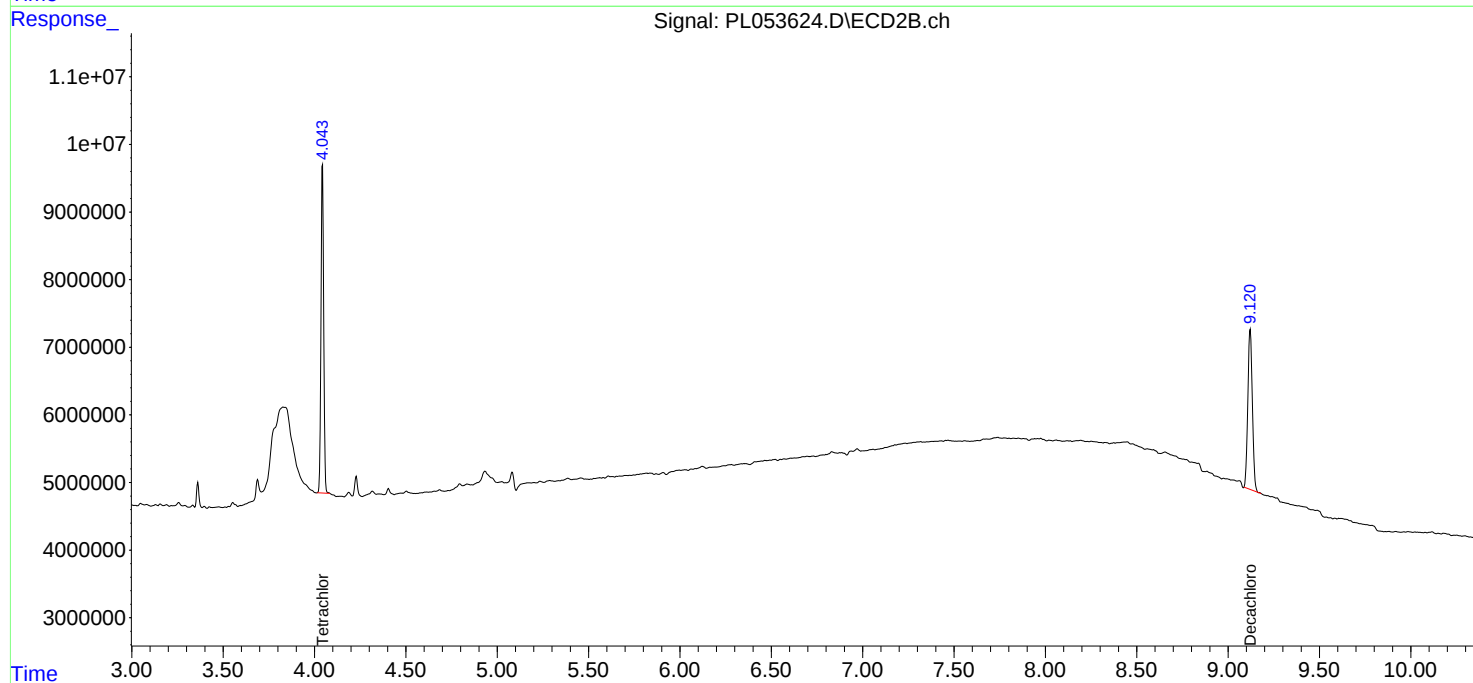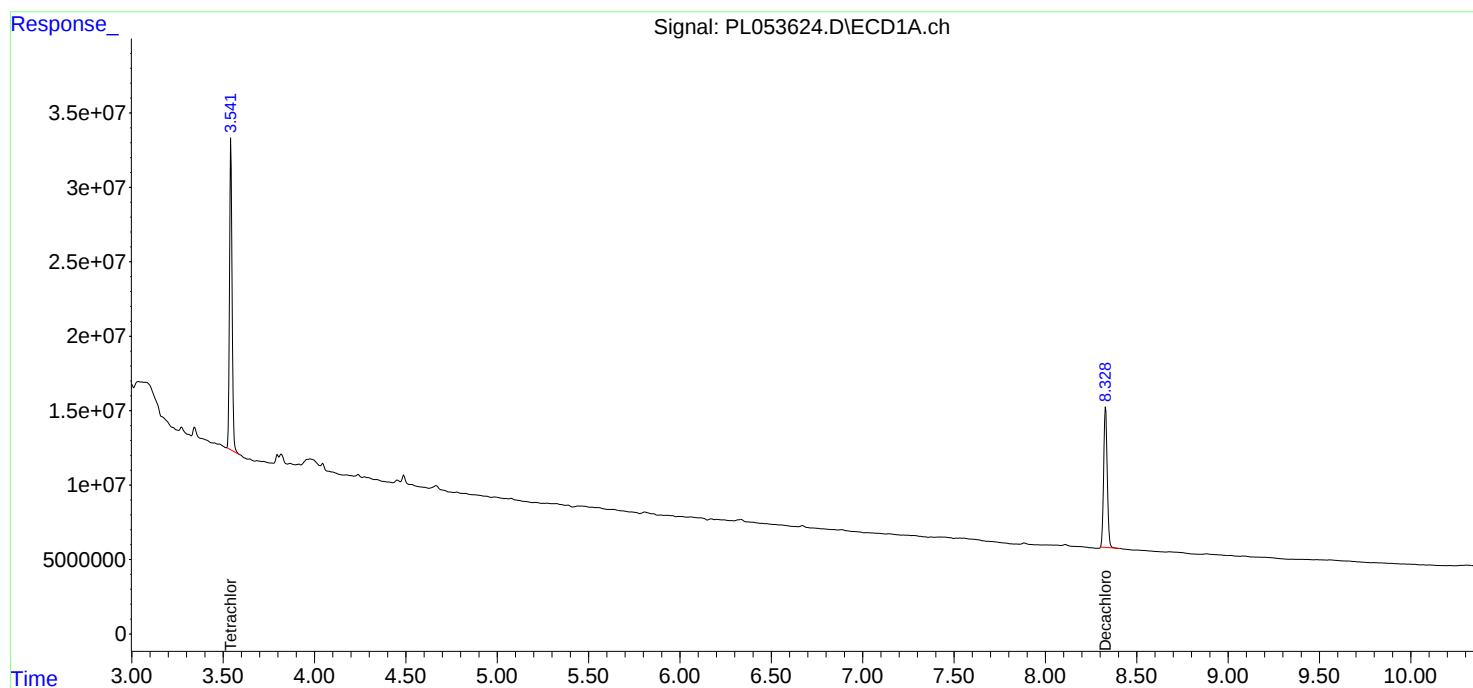


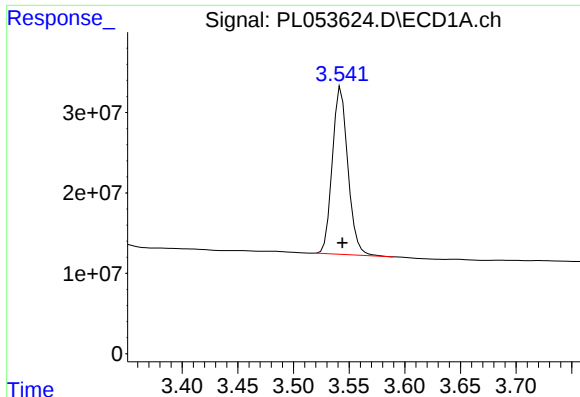

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 202196957
Conc: 18.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
MAIN-STOCKPILE-SLP

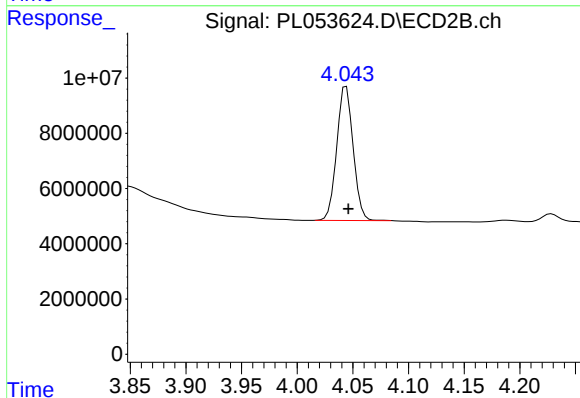


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 49779734
Conc: 19.89 ng/ml

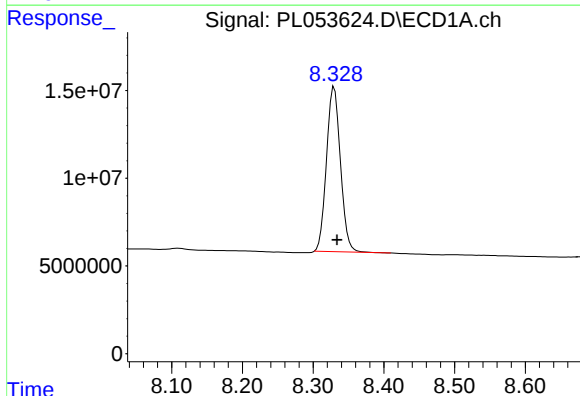

#28 Decachlorobiphenyl

R.T.: 8.330 min
Delta R.T.: -0.004 min
Response: 128649188
Conc: 13.11 ng/ml

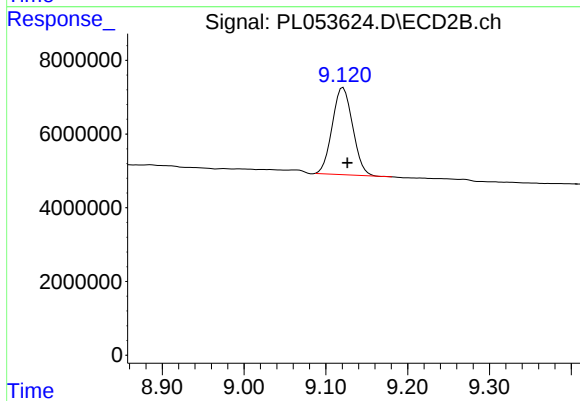

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.005 min
Response: 40909314
Conc: 14.53 ng/ml