

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
 Data File : PL053635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2019 23:00
 Operator : SG\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Manual Integrations
 APPROVED

Ankita
 10/24/2019 3:21:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 01:48:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.044	549.0E6	130.5E6	50.648	52.144
28)	SA Decachlor...	8.328	9.122	431.6E6	134.3E6	43.987	47.693
Target Compounds							
2)	A alpha-BHC	3.986	4.435	855.0E6	172.4E6	49.036	49.874
3)	MA gamma-BHC...	4.273	4.721	749.0E6	166.3E6	48.095	51.654
4)	MA Heptachlor	4.580	5.231	729.5E6	153.5E6	46.220	47.630
5)	MB Aldrin	4.832	5.536	672.9E6	141.5E6	47.073	47.458
6)	B beta-BHC	4.523	4.890	296.9E6	69262496	45.059	44.841
7)	B delta-BHC	4.732	5.108	716.6E6	154.7E6	47.079	51.202
8)	B Heptachlo...	5.277	5.922	626.4E6	135.7E6	46.402	46.524
9)	A Endosulfan I	5.620	6.279	563.1E6	122.7E6	45.814	45.249
10)	B gamma-Chl...	5.506	6.156	631.8E6	132.0E6	46.310	45.228
11)	B alpha-Chl...	5.565	6.229	604.0E6	131.8E6	45.403	45.142
12)	B 4,4'-DDE	5.728	6.385	560.0E6	125.3E6	47.132	44.478
13)	MA Dieldrin	5.864	6.536	591.4E6	131.5E6	45.372	46.067
14)	MA Endrin	6.123	6.754	521.3E6	106.2E6	44.975	43.768
15)	B Endosulfa...	6.395	6.963	484.7E6	117.9E6	43.354	46.154
16)	A 4,4'-DDD	6.245	6.875	435.1E6	91944887	48.892	44.120
17)	MA 4,4'-DDT	6.488	7.172	412.1E6	93406237	41.604	40.392m
18)	B Endrin al...	6.564	7.087	385.6E6	97730119	42.055	44.488
19)	B Endosulfa...	6.777	7.310	439.6E6	110.5E6	43.215	45.025
20)	A Methoxychlor	7.033	7.631	211.5E6	56002122	42.893	43.115
21)	B Endrin ke...	7.271	7.781	485.5E6	121.5E6	45.097	47.105
22)	Mirex	7.464	8.235	353.6E6	85932163	41.342	42.476

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
 Data File : PL053635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2019 23:00
 Operator : SG\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1



Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050


Manual Integrations
 APPROVED

Ankita
 10/24/2019 3:21:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 01:48:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

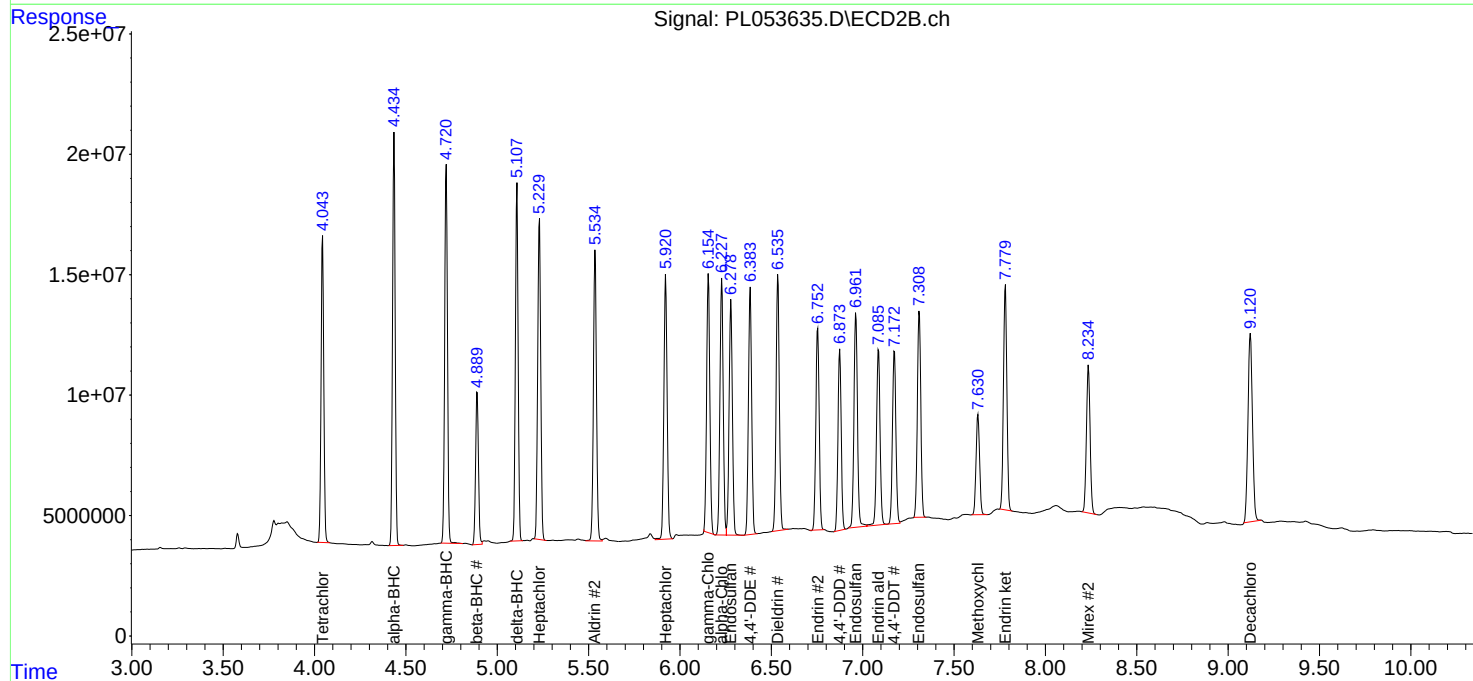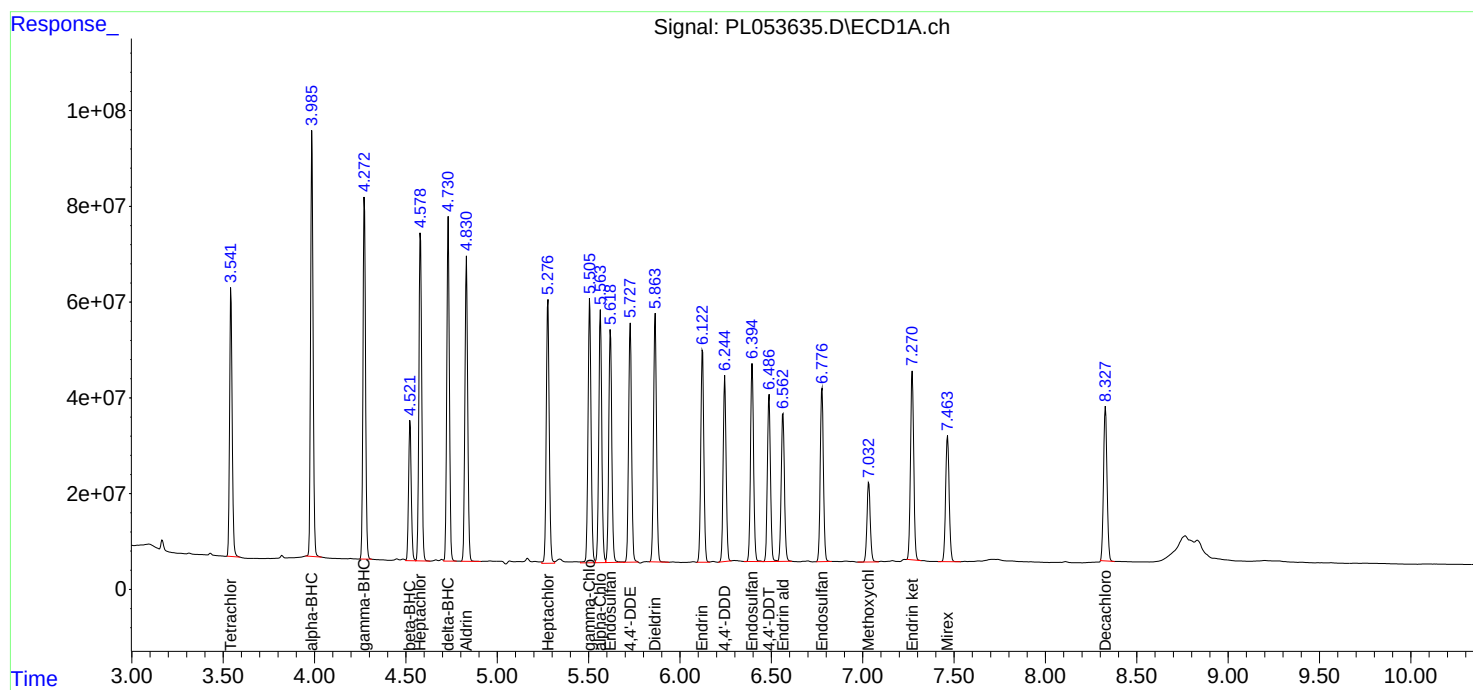

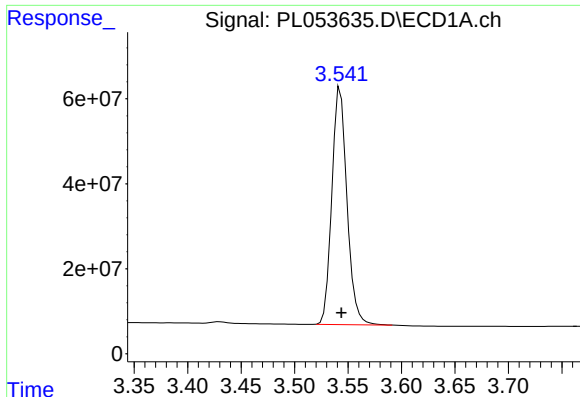


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 548993605
Conc: 50.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
10/24/2019 3:21:47 PM

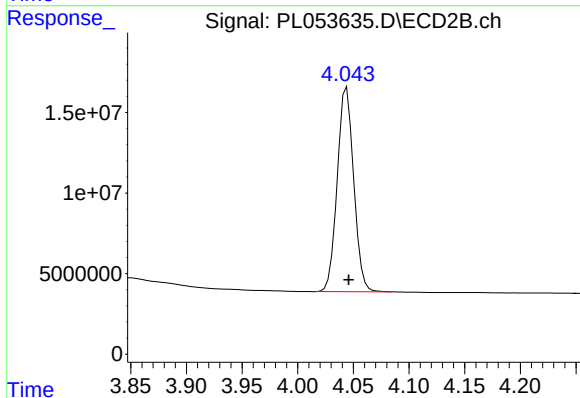


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 130483797
Conc: 52.14 ng/ml

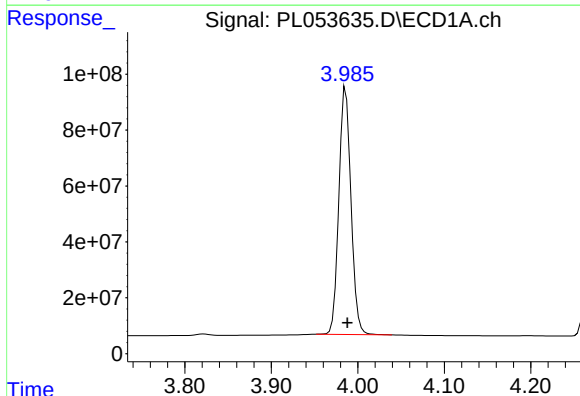


#2 alpha-BHC

R.T.: 3.986 min
Delta R.T.: -0.002 min
Response: 855008435
Conc: 49.04 ng/ml

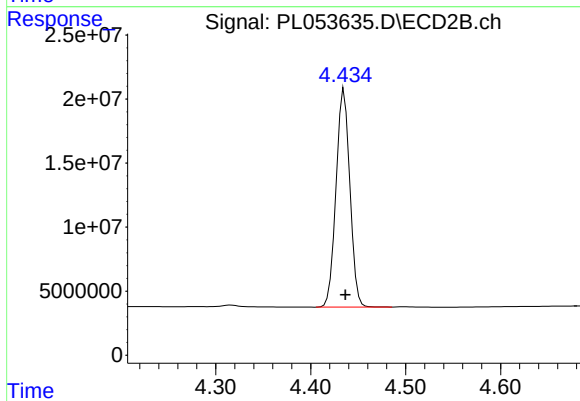

#2 alpha-BHC

R.T.: 4.435 min
Delta R.T.: -0.001 min
Response: 172417757
Conc: 49.87 ng/ml

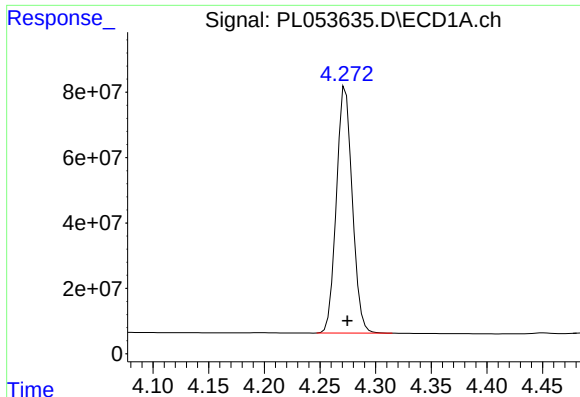


#3 gamma-BHC (Lindane)

R.T.: 4.273 min
Delta R.T.: -0.002 min
Response: 749006777
Conc: 48.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
10/24/2019 3:21:47 PM

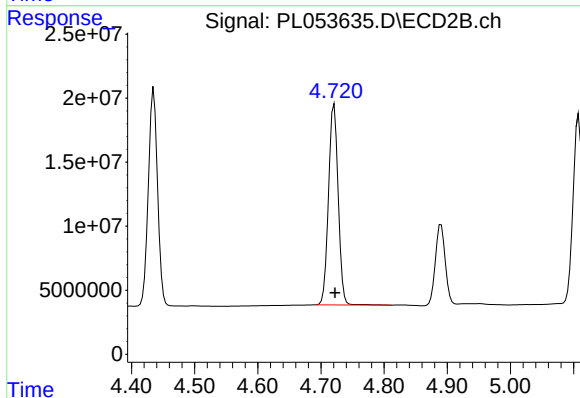


#3 gamma-BHC (Lindane)

R.T.: 4.721 min
Delta R.T.: -0.002 min
Response: 166347070
Conc: 51.65 ng/ml

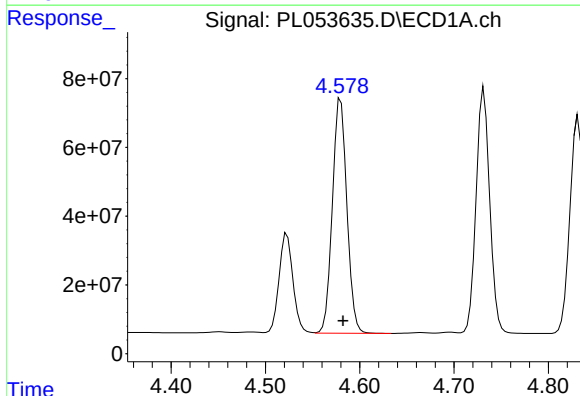


#4 Heptachlor

R.T.: 4.580 min
Delta R.T.: -0.002 min
Response: 729490050
Conc: 46.22 ng/ml

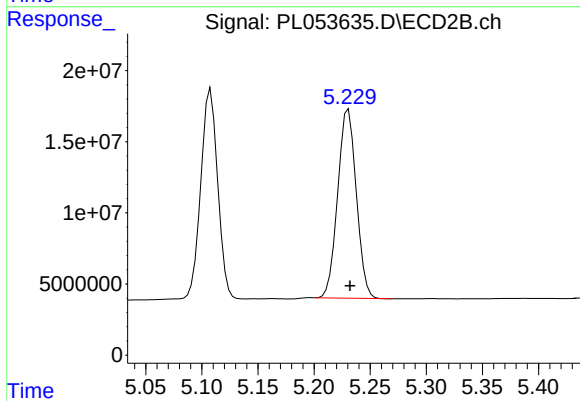

#4 Heptachlor

R.T.: 5.231 min
Delta R.T.: -0.002 min
Response: 153471353
Conc: 47.63 ng/ml

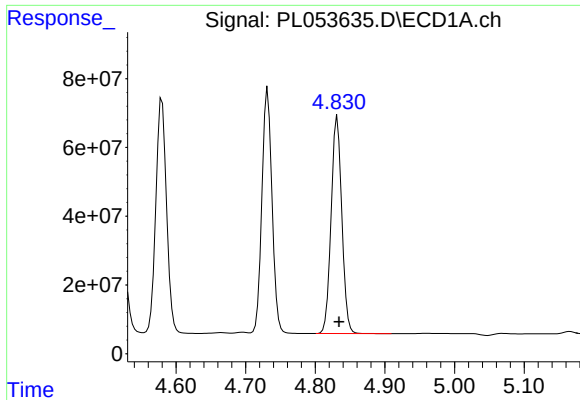


#5 Aldrin

R.T.: 4.832 min
Delta R.T.: -0.003 min
Response: 672944978
Conc: 47.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
10/24/2019 3:21:47 PM

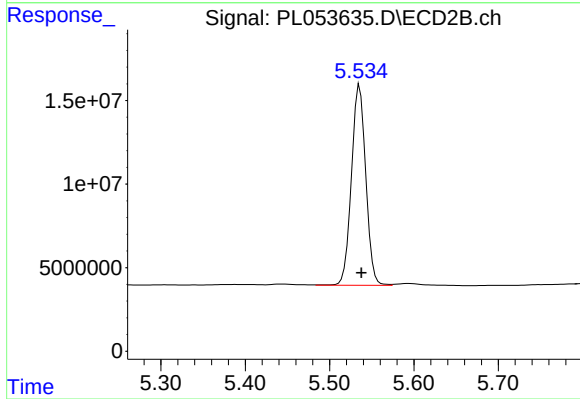


#5 Aldrin

R.T.: 5.536 min
Delta R.T.: -0.002 min
Response: 141497676
Conc: 47.46 ng/ml

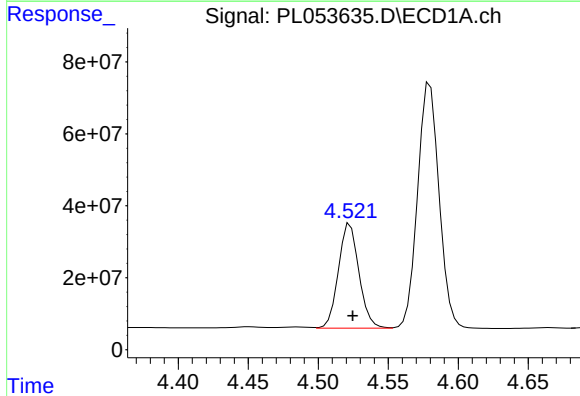


#6 beta-BHC

R.T.: 4.523 min
Delta R.T.: -0.002 min
Response: 296931773
Conc: 45.06 ng/ml

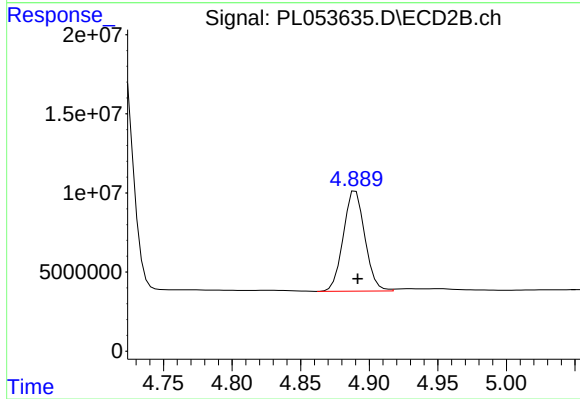

#6 beta-BHC

R.T.: 4.890 min
Delta R.T.: -0.001 min
Response: 69262496
Conc: 44.84 ng/ml

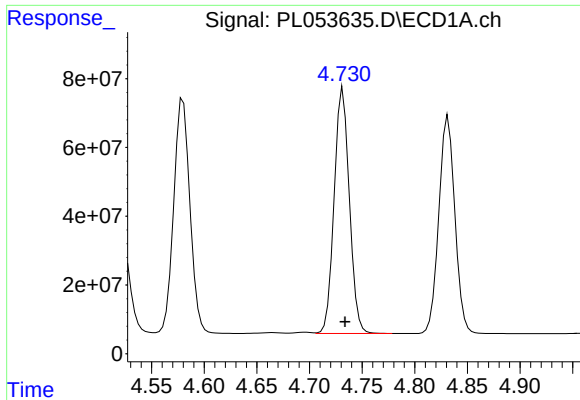


#7 delta-BHC

R.T.: 4.732 min
Delta R.T.: -0.002 min
Response: 716595435
Conc: 47.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
10/24/2019 3:21:47 PM

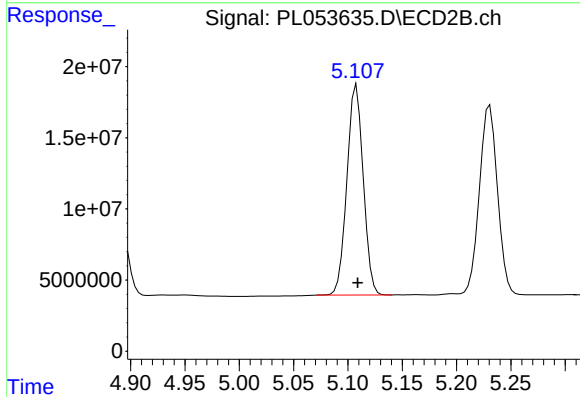


#7 delta-BHC

R.T.: 5.108 min
Delta R.T.: -0.001 min
Response: 154659240
Conc: 51.20 ng/ml

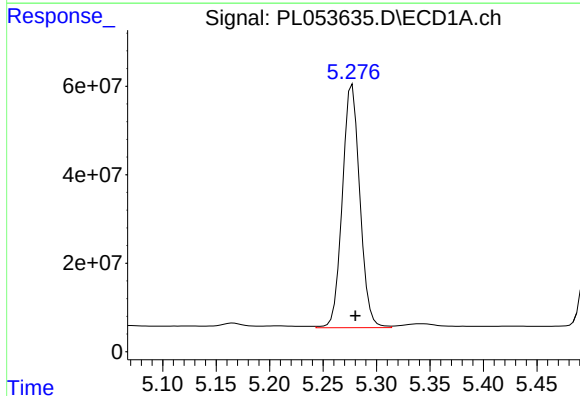


#8 Heptachlor epoxide

R.T.: 5.277 min
Delta R.T.: -0.003 min
Response: 626393259
Conc: 46.40 ng/ml

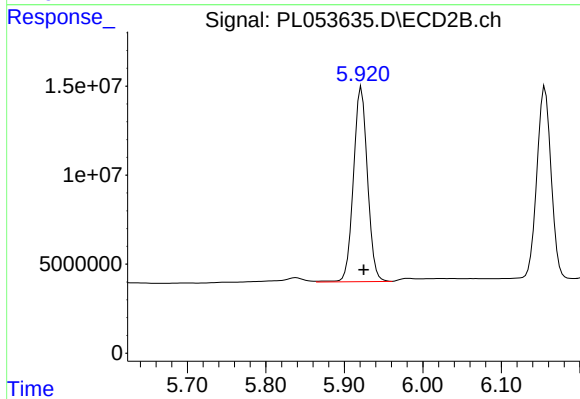

#8 Heptachlor epoxide

R.T.: 5.922 min
Delta R.T.: -0.003 min
Response: 135681762
Conc: 46.52 ng/ml

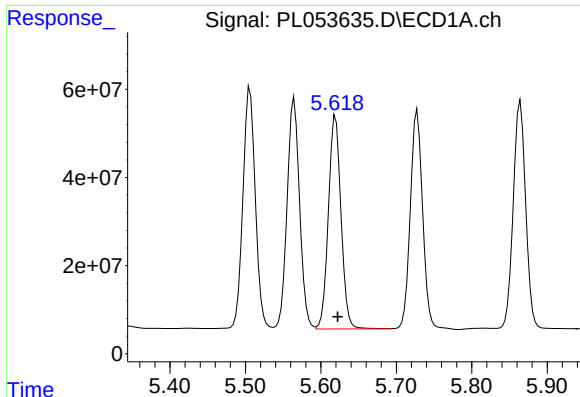


#9 Endosulfan I

R.T.: 5.620 min
Delta R.T.: -0.003 min
Response: 563143805
Conc: 45.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
10/24/2019 3:21:47 PM

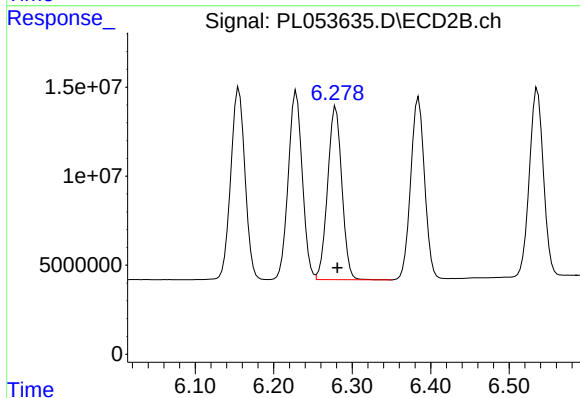


#9 Endosulfan I

R.T.: 6.279 min
Delta R.T.: -0.002 min
Response: 122681195
Conc: 45.25 ng/ml

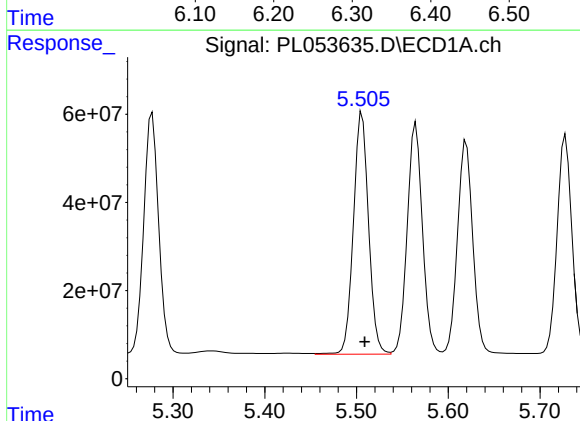


#10 gamma-Chlordane

R.T.: 5.506 min
Delta R.T.: -0.003 min
Response: 631832764
Conc: 46.31 ng/ml

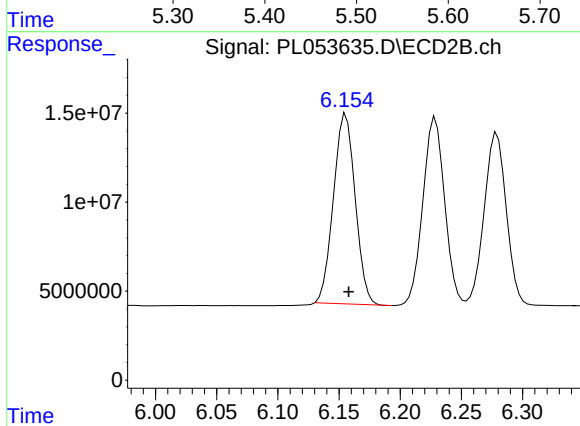

#10 gamma-Chlordane

R.T.: 6.156 min
Delta R.T.: -0.002 min
Response: 131965444
Conc: 45.23 ng/ml

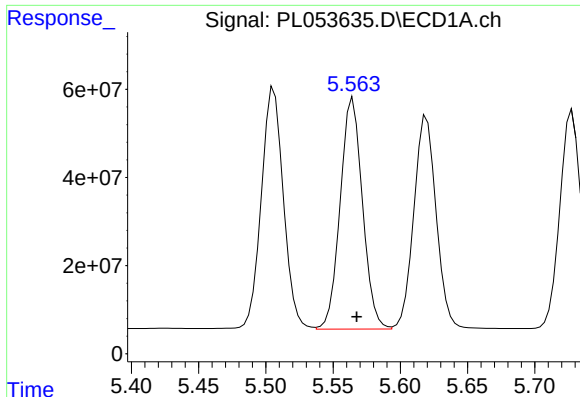


#11 alpha-Chlordane

R.T.: 5.565 min
Delta R.T.: -0.003 min
Response: 604023398
Conc: 45.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
10/24/2019 3:21:47 PM

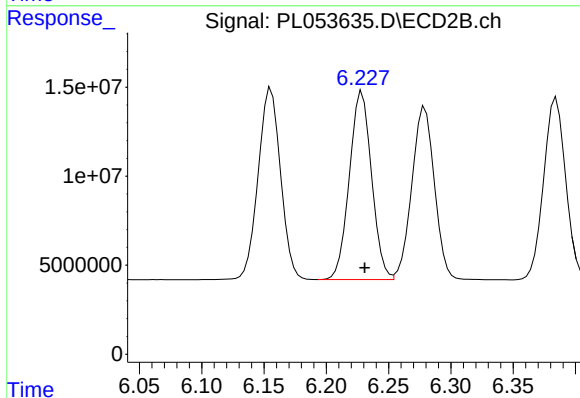


#11 alpha-Chlordane

R.T.: 6.229 min
Delta R.T.: -0.002 min
Response: 131779713
Conc: 45.14 ng/ml

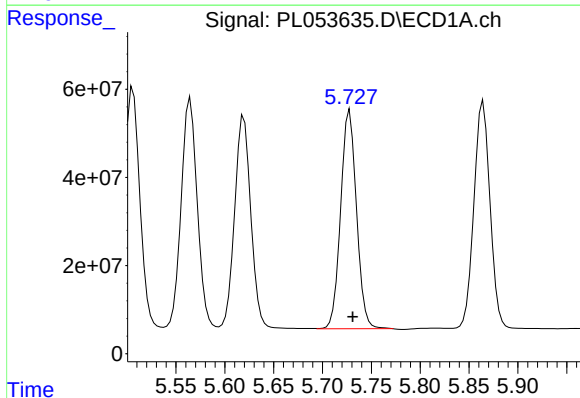


#12 4,4'-DDE

R.T.: 5.728 min
Delta R.T.: -0.003 min
Response: 560029493
Conc: 47.13 ng/ml

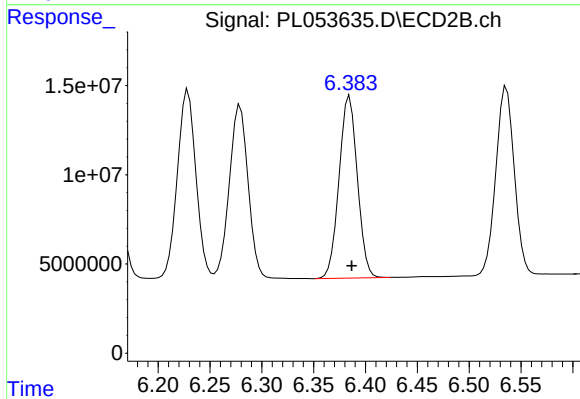

#12 4,4'-DDE

R.T.: 6.385 min
Delta R.T.: -0.002 min
Response: 125264799
Conc: 44.48 ng/ml

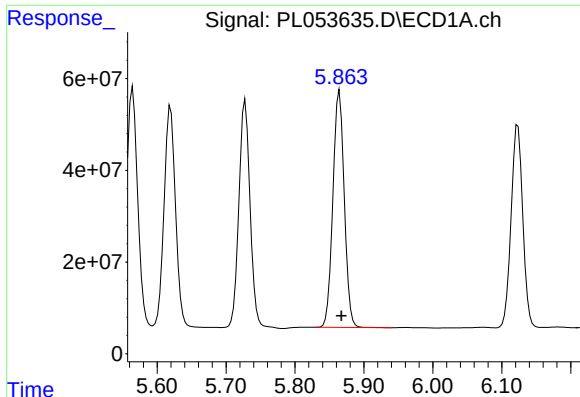


#13 Dieldrin

R.T.: 5.864 min
Delta R.T.: -0.003 min
Response: 591356745
Conc: 45.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
10/24/2019 3:21:47 PM

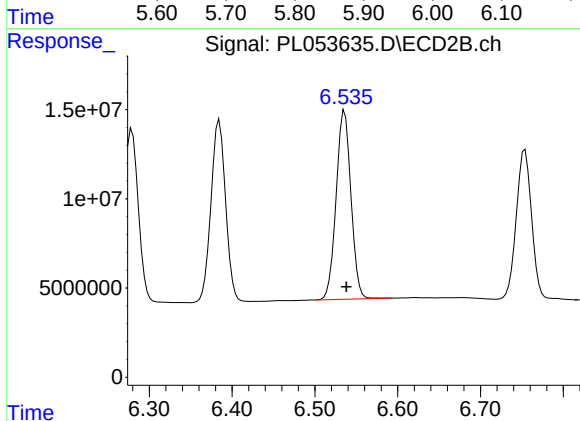


#13 Dieldrin

R.T.: 6.536 min
Delta R.T.: -0.002 min
Response: 131458927
Conc: 46.07 ng/ml

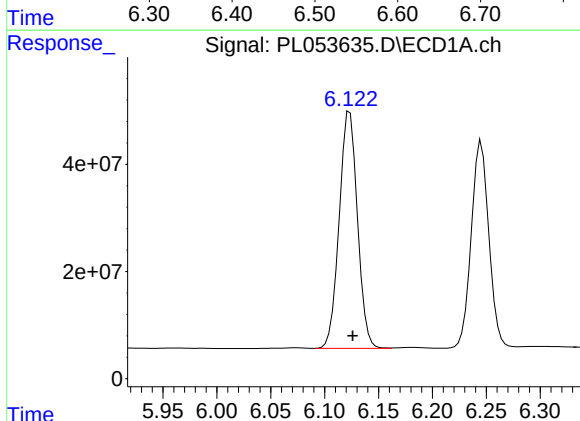


#14 Endrin

R.T.: 6.123 min
Delta R.T.: -0.003 min
Response: 521314660
Conc: 44.98 ng/ml

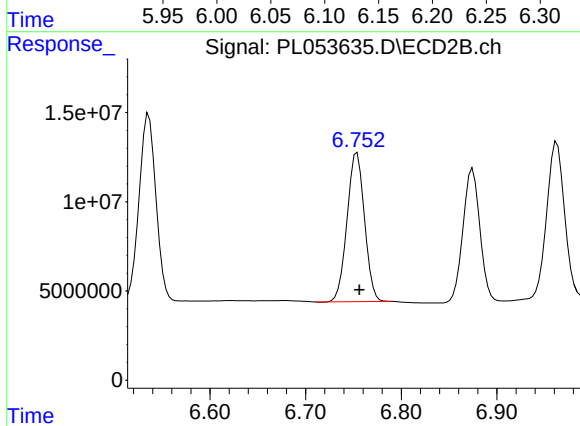

#14 Endrin

R.T.: 6.754 min
Delta R.T.: -0.002 min
Response: 106232751
Conc: 43.77 ng/ml

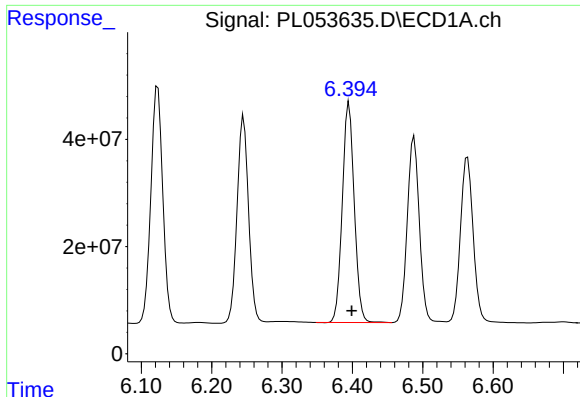


#15 Endosulfan II

R.T.: 6.395 min
Delta R.T.: -0.004 min
Response: 484709260
Conc: 43.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
10/24/2019 3:21:47 PM

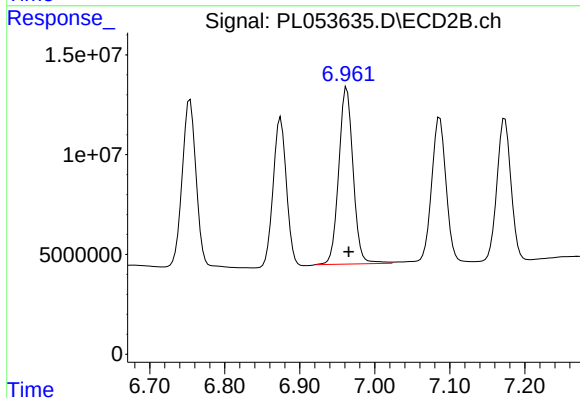


#15 Endosulfan II

R.T.: 6.963 min
Delta R.T.: -0.002 min
Response: 117900503
Conc: 46.15 ng/ml

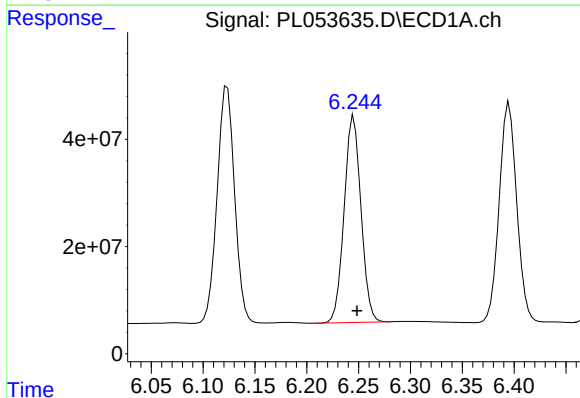


#16 4,4'-DDD

R.T.: 6.245 min
Delta R.T.: -0.003 min
Response: 435130508
Conc: 48.89 ng/ml

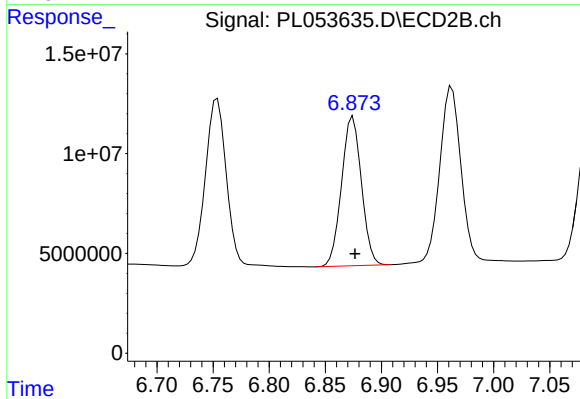

#16 4,4'-DDD

R.T.: 6.875 min
Delta R.T.: -0.002 min
Response: 91944887
Conc: 44.12 ng/ml

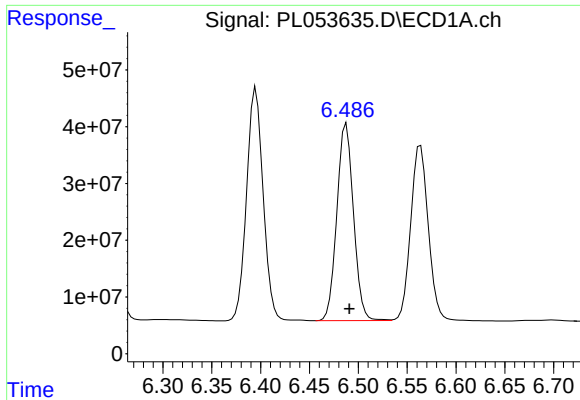


#17 4,4'-DDT

R.T.: 6.488 min
Delta R.T.: -0.003 min
Response: 412142606
Conc: 41.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
10/24/2019 3:21:47 PM

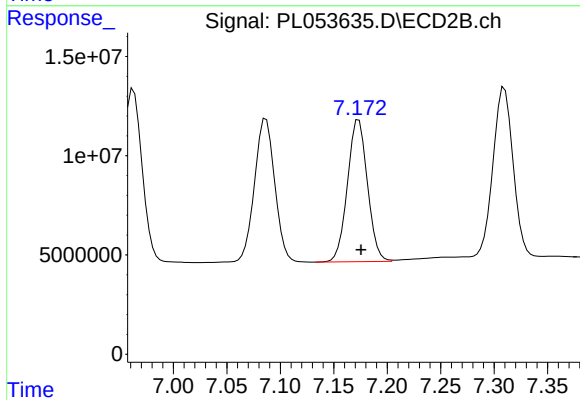


#17 4,4'-DDT

R.T.: 7.172 min
Delta R.T.: -0.004 min
Response: 93406237
Conc: 40.39 ng/ml m

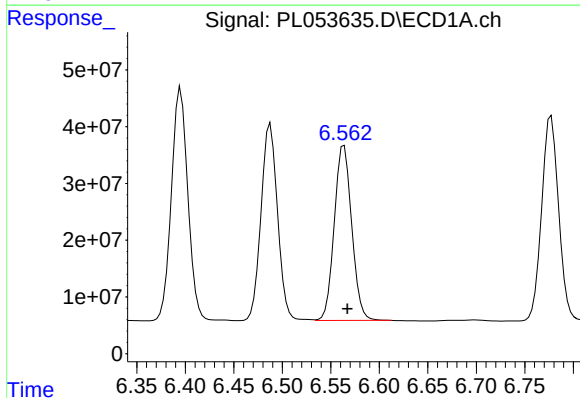


#18 Endrin aldehyde

R.T.: 6.564 min
Delta R.T.: -0.003 min
Response: 385610334
Conc: 42.05 ng/ml

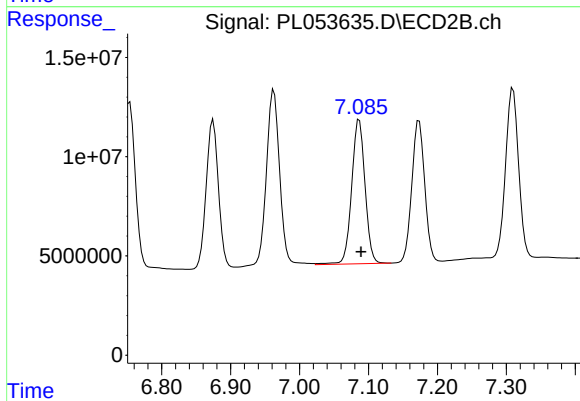

#18 Endrin aldehyde

R.T.: 7.087 min
Delta R.T.: -0.002 min
Response: 97730119
Conc: 44.49 ng/ml

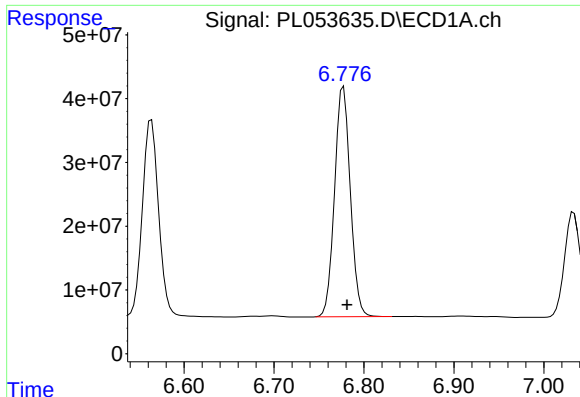


#19 Endosulfan Sulfate

R.T.: 6.777 min
Delta R.T.: -0.004 min
Response: 439570762
Conc: 43.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
10/24/2019 3:21:47 PM

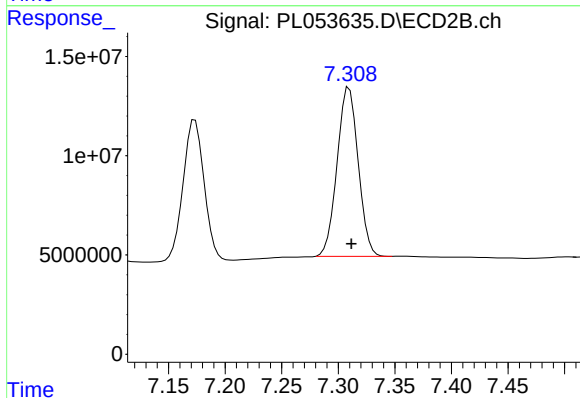


#19 Endosulfan Sulfate

R.T.: 7.310 min
Delta R.T.: -0.002 min
Response: 110472504
Conc: 45.02 ng/ml

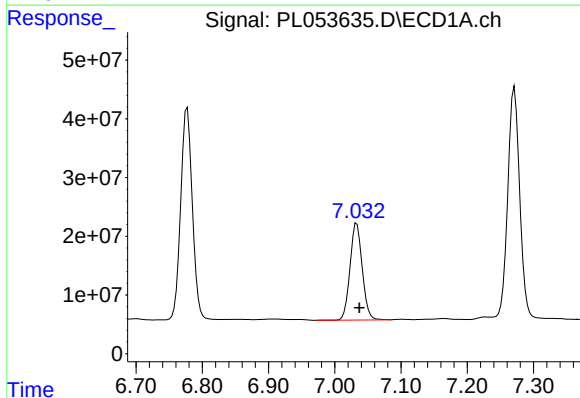


#20 Methoxychlor

R.T.: 7.033 min
Delta R.T.: -0.004 min
Response: 211476922
Conc: 42.89 ng/ml

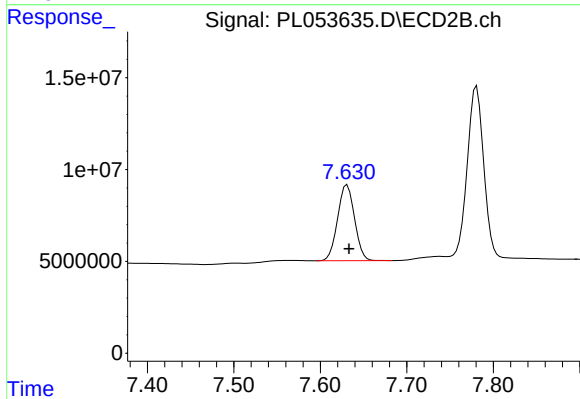

#20 Methoxychlor

R.T.: 7.631 min
Delta R.T.: -0.002 min
Response: 56002122
Conc: 43.11 ng/ml

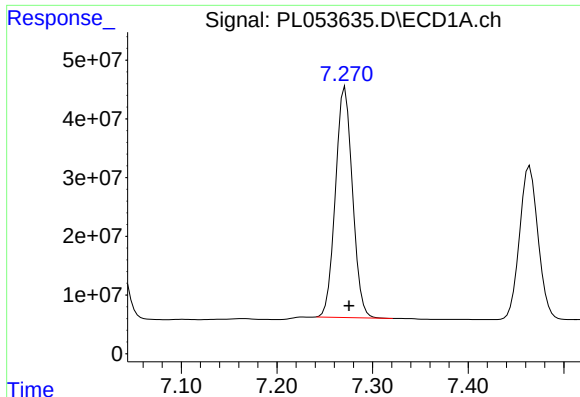


#21 Endrin ketone

R.T.: 7.271 min
Delta R.T.: -0.004 min
Response: 485471923
Conc: 45.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
10/24/2019 3:21:47 PM

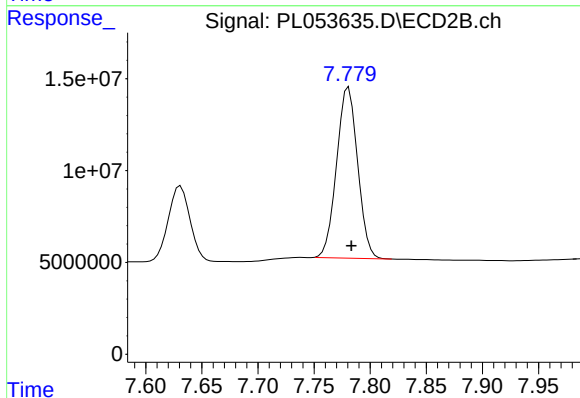


#21 Endrin ketone

R.T.: 7.781 min
Delta R.T.: -0.002 min
Response: 121457864
Conc: 47.10 ng/ml

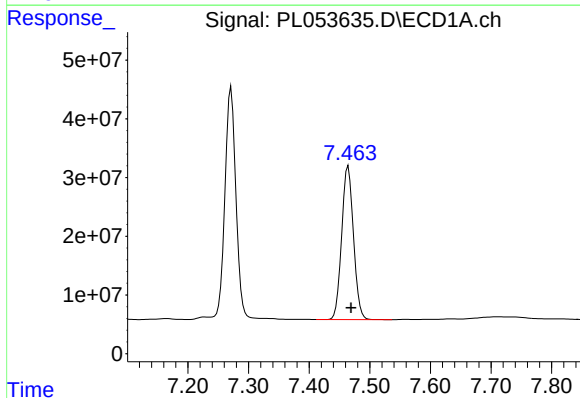


#22 Mirex

R.T.: 7.464 min
Delta R.T.: -0.005 min
Response: 353595341
Conc: 41.34 ng/ml

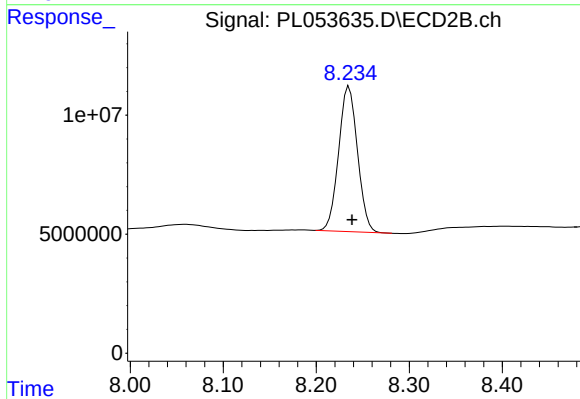

#22 Mirex

R.T.: 8.235 min
Delta R.T.: -0.003 min
Response: 85932163
Conc: 42.48 ng/ml

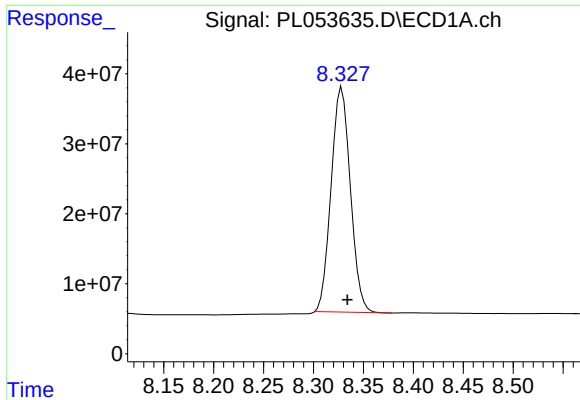


#28 Decachlorobiphenyl

R.T.: 8.328 min
Delta R.T.: -0.006 min
Response: 431580249
Conc: 43.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Manual Integrations
APPROVED

Ankita
10/24/2019 3:21:47 PM

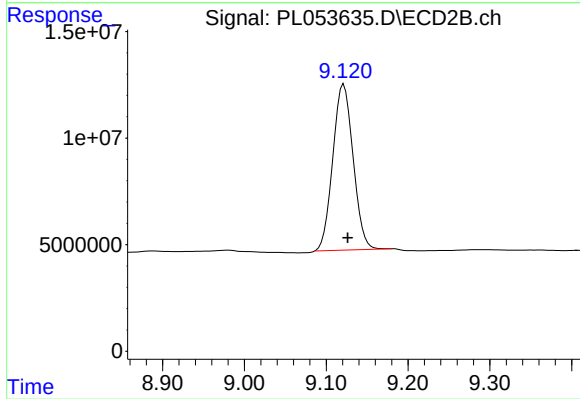

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.005 min
Response: 134305153
Conc: 47.69 ng/ml