

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
 Data File : PL053654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2019 03:39
 Operator : SG\AJ
 Sample : K5498-17
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 193-10-(0-1)

Manual Integrations
 APPROVED

Ankita
 10/24/2019 3:22:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 04:23:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	4.045	129.0E6	31210480	11.897	12.472
28) SA Decachlor...	8.329	9.121	83938916	24577820	8.555	8.728
Target Compounds						
10) B gamma-Chl...	5.504	6.154	39654687	11830909	2.906m	4.055m#
11) B alpha-Chl...	5.563	6.228	42804115	17064411	3.218m	5.846m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102319\
Data File : PL053654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2019 03:39
Operator : SG\AJ
Sample : K5498-17
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
193-10-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 3:22:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 04:23:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

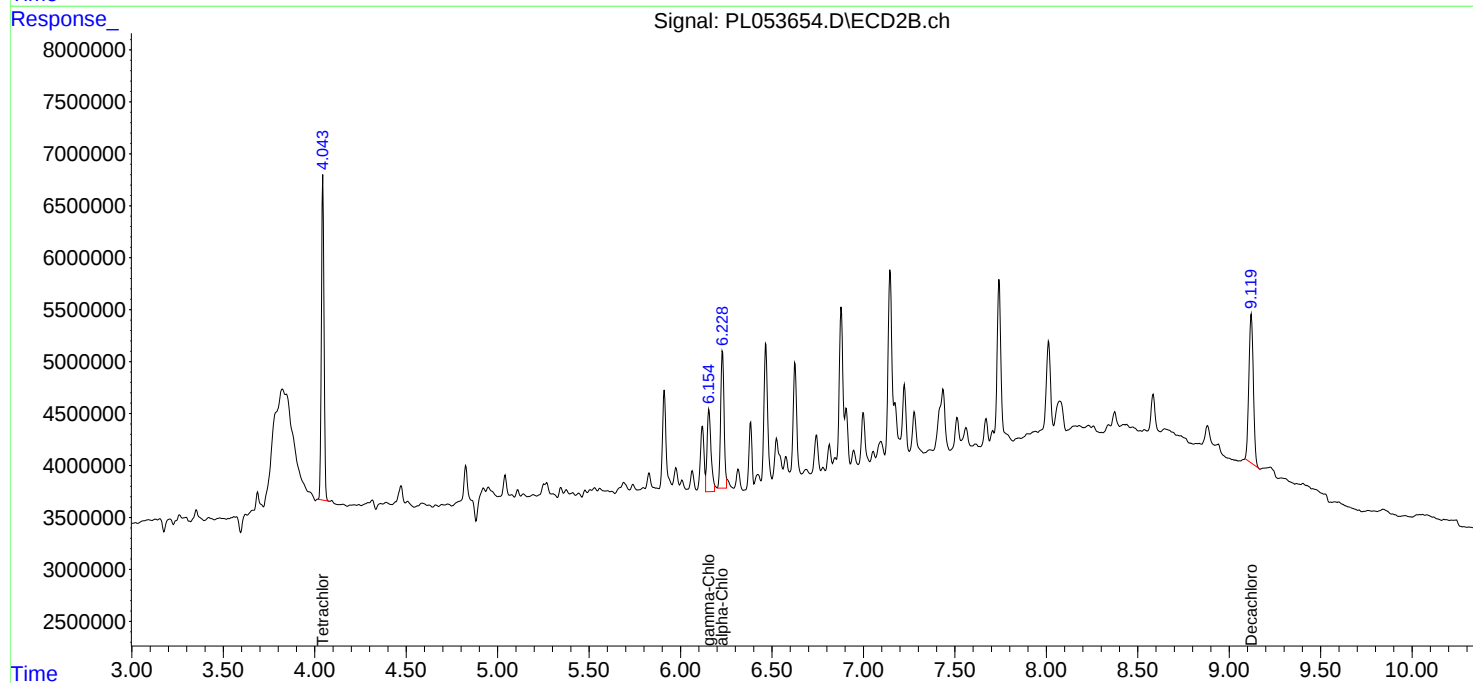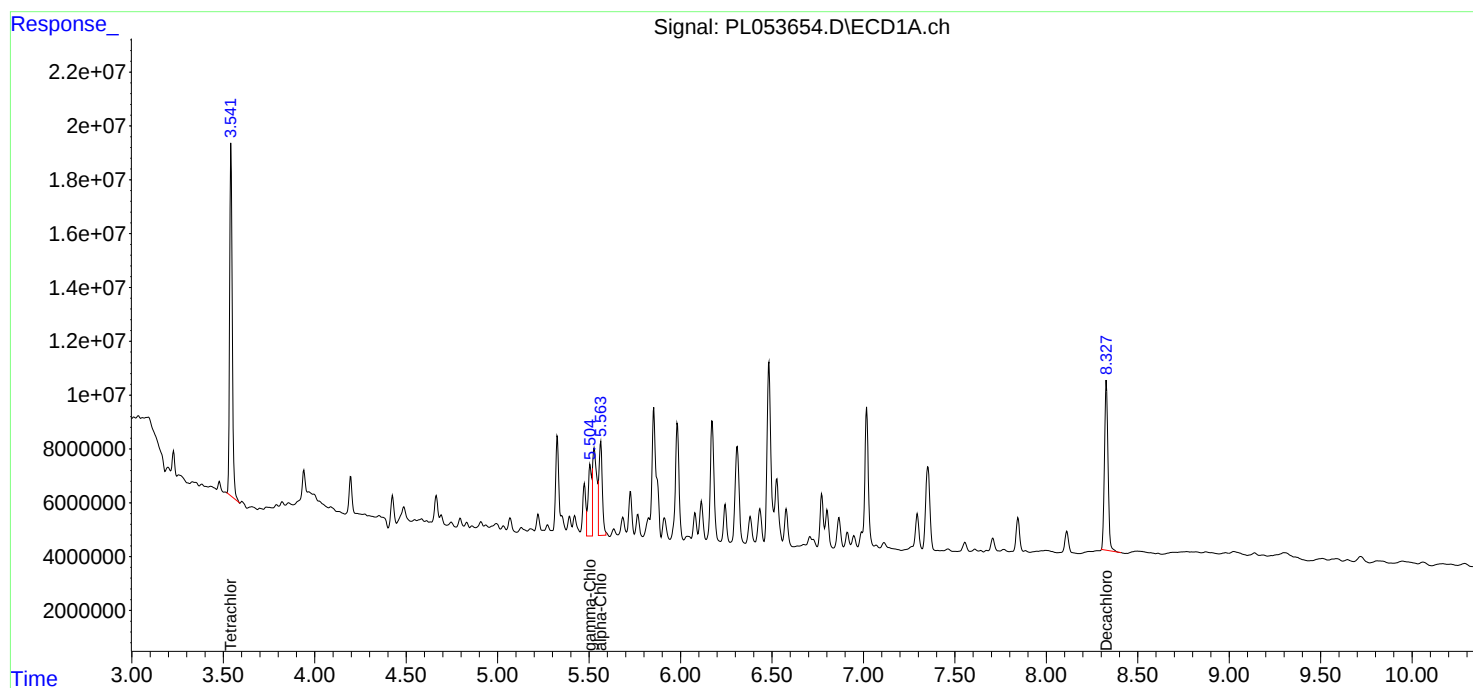

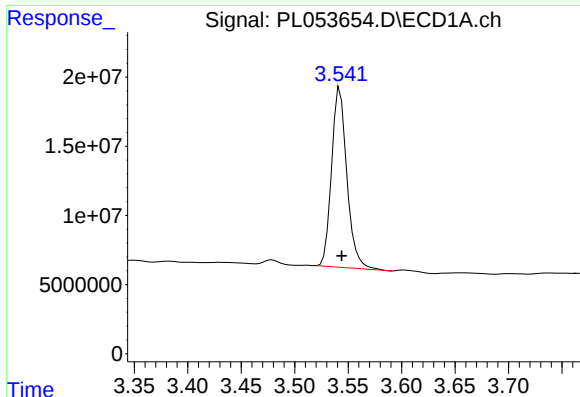


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 128952860
Conc: 11.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
193-10-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 3:22:07 PM

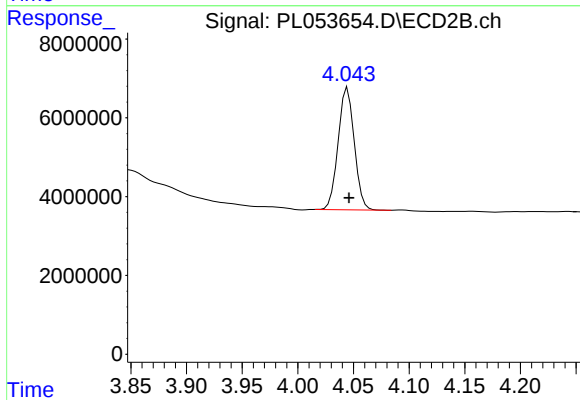


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: -0.001 min
Response: 31210480
Conc: 12.47 ng/ml

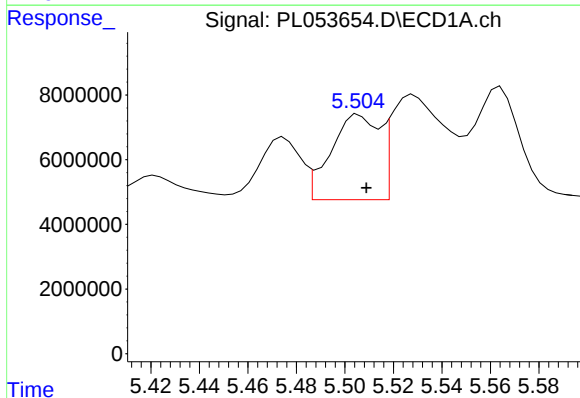


#10 gamma-Chlordane

R.T.: 5.504 min
Delta R.T.: -0.005 min
Response: 39654687
Conc: 2.91 ng/ml m

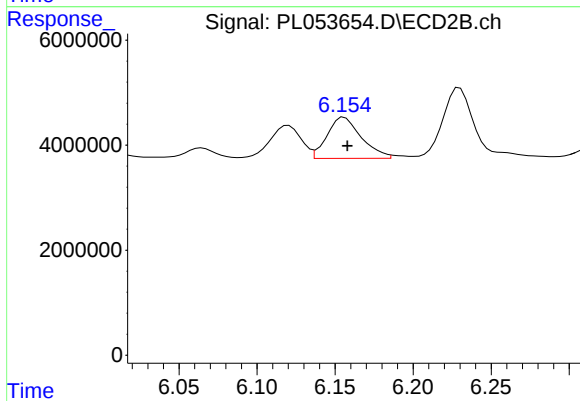

#10 gamma-Chlordane

R.T.: 6.154 min
Delta R.T.: -0.003 min
Response: 11830909
Conc: 4.05 ng/ml m

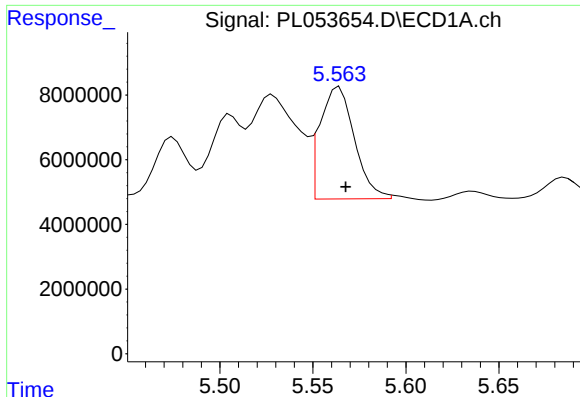


#11 alpha-Chlordane

R.T.: 5.563 min
Delta R.T.: -0.005 min
Response: 42804115
Conc: 3.22 ng/ml m

Instrument :
ECD_L
ClientSampleId :
193-10-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 3:22:07 PM

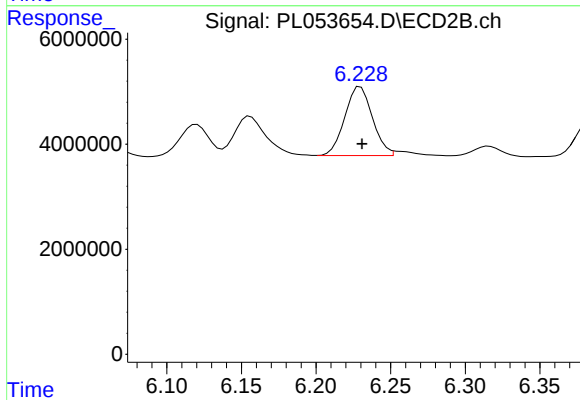


#11 alpha-Chlordane

R.T.: 6.228 min
Delta R.T.: -0.002 min
Response: 17064411
Conc: 5.85 ng/ml m

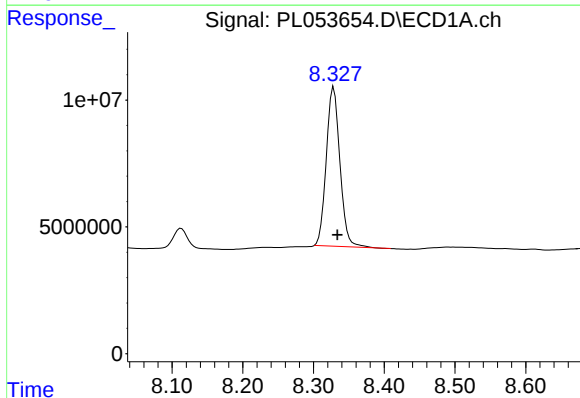

#28 Decachlorobiphenyl

R.T.: 8.329 min
Delta R.T.: -0.005 min
Response: 83938916
Conc: 8.56 ng/ml

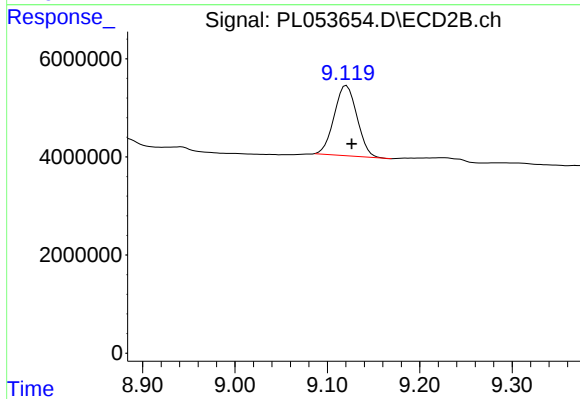

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.005 min
Response: 24577820
Conc: 8.73 ng/ml