

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102320\
 Data File : PL062567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2020 16:49
 Operator : DD\AJ
 Sample : L4494-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 18:28:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	36317142	63692620	21.114	21.674
28)	SA Decachlor...	8.127	8.991	33499367	46989448	20.881	22.451
Target Compounds							
7)	B delta-BHC	0.000	4.983f	0	1801923	N.D.	0.515 #
8)	B Heptachlo...	5.105	0.000	684369	0	0.375	N.D. #
11)	B alpha-Chl...	5.375	0.000	624097	0	0.345	N.D. #
15)	B Endosulfa...	0.000	6.867	0	2771180	N.D.	0.969 #
23)	Chlordane-1	4.279	0.000	895902	0	17.379	N.D. #
26)	Chlordane-4	5.375	0.000	624097	0	4.791	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102320\
Data File : PL062567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2020 16:49
Operator : DD\AJ
Sample : L4494-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 18:28:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

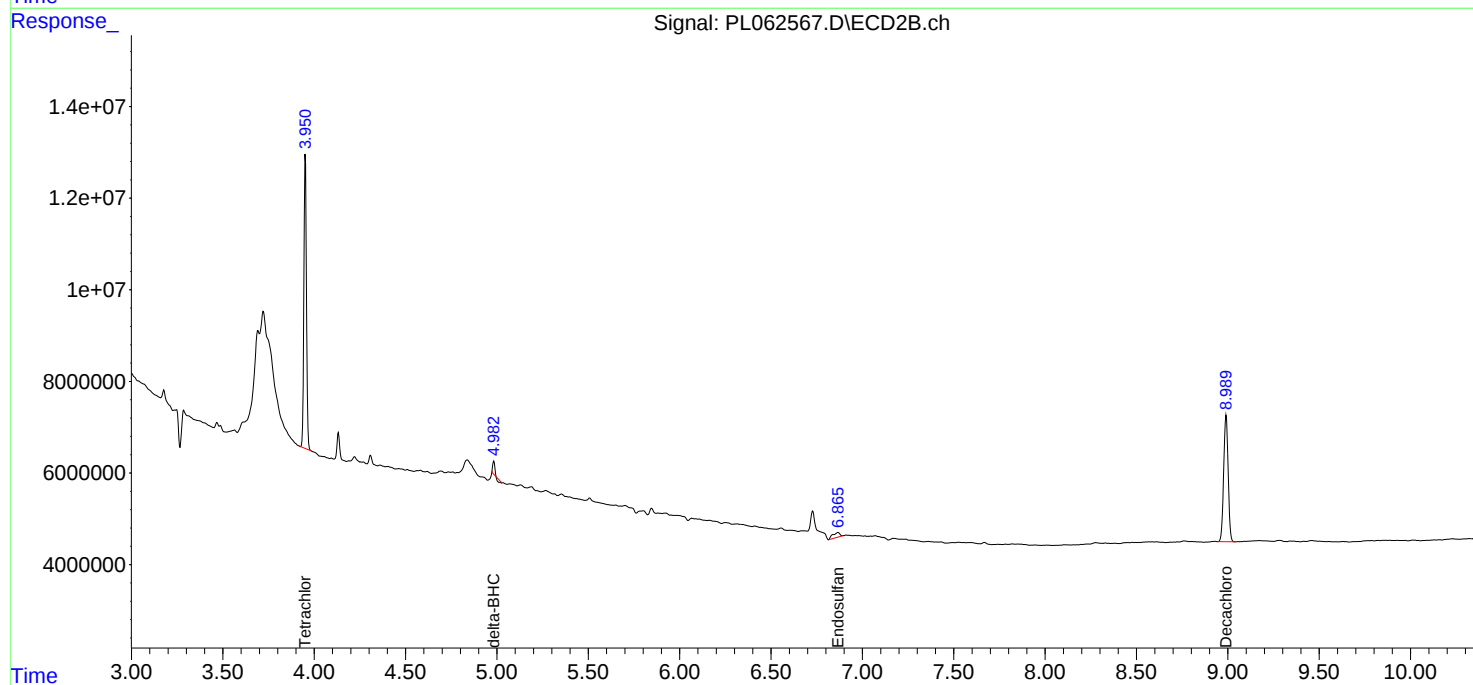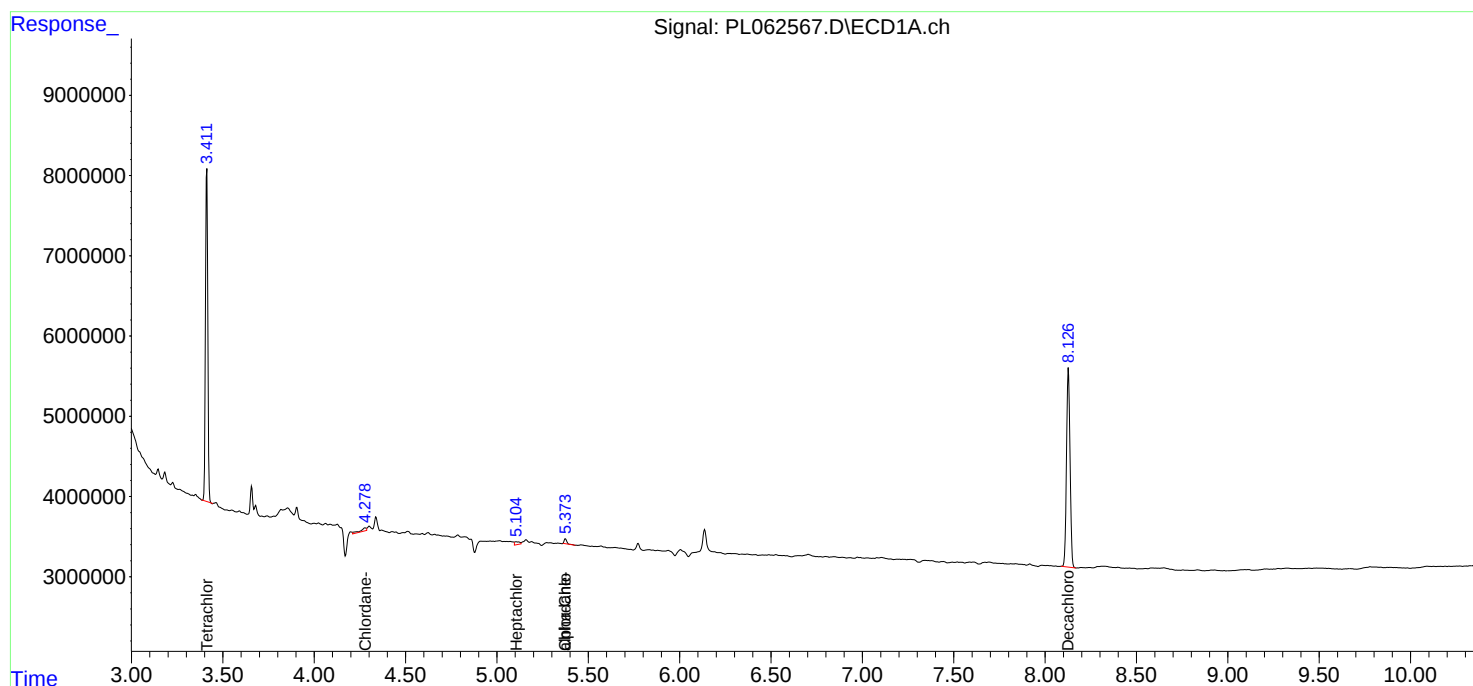


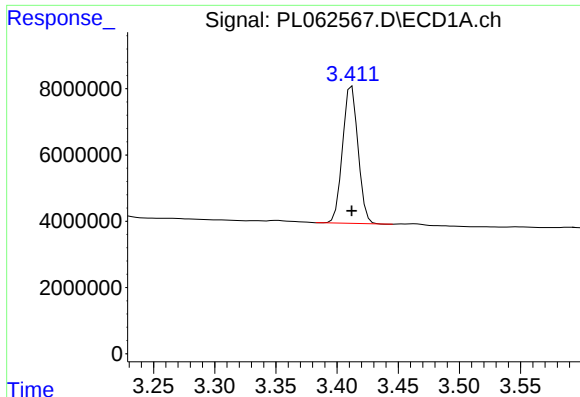

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 36317142
Conc: 21.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

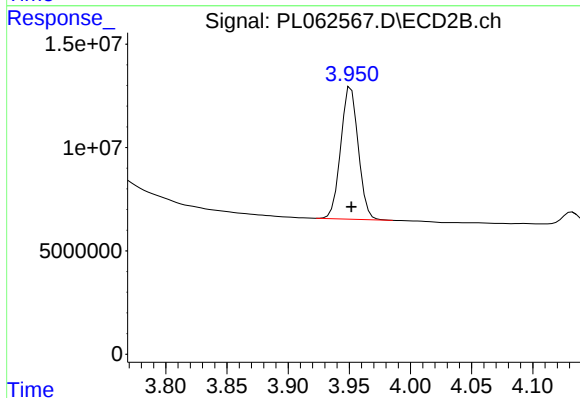


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 63692620
Conc: 21.67 ng/ml

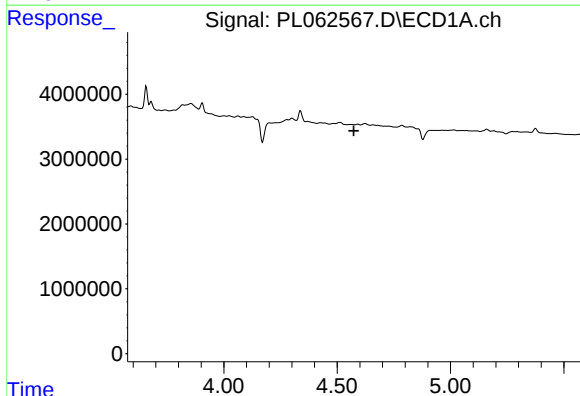


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

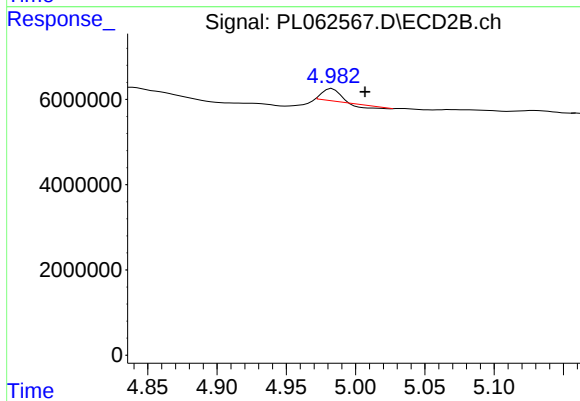

#7 delta-BHC


R.T.: 4.983 min
Delta R.T.: -0.024 min
Response: 1801923
Conc: 0.51 ng/ml

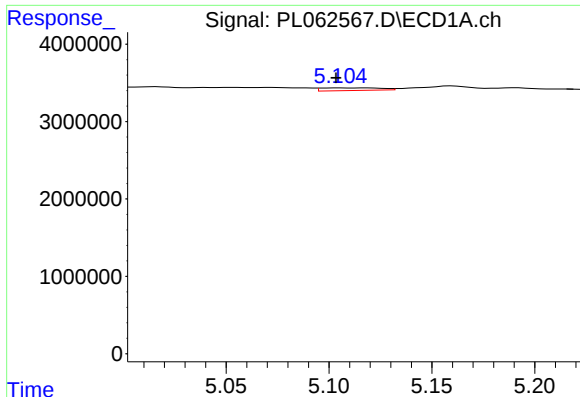

#8 Heptachlor epoxide


R.T.: 5.105 min
Delta R.T.: 0.002 min
Response: 684369
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

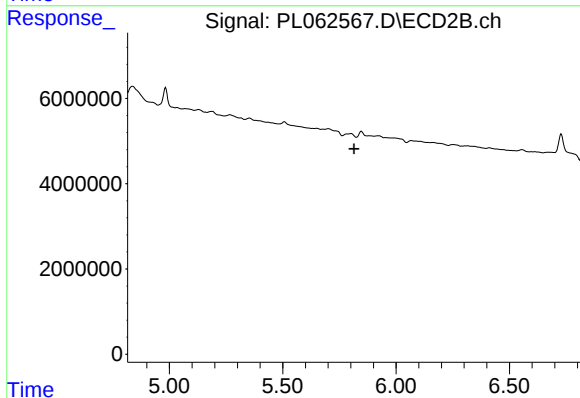


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.815 min
Response: 0
Conc: N.D.

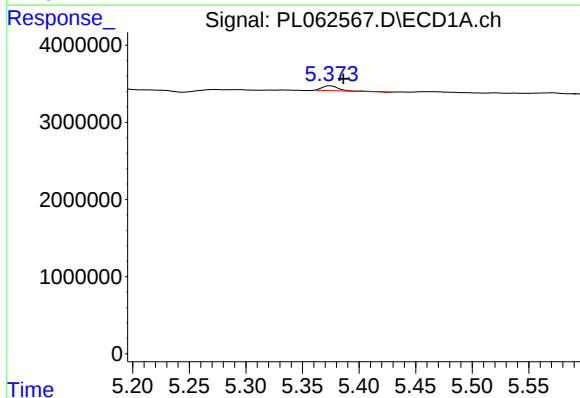


#11 alpha-Chlordane

R.T.: 5.375 min
Delta R.T.: -0.011 min
Response: 624097
Conc: 0.35 ng/ml

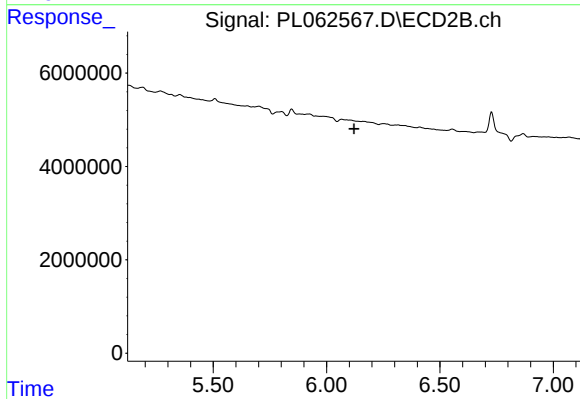

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.121 min
Response: 0
Conc: N.D.

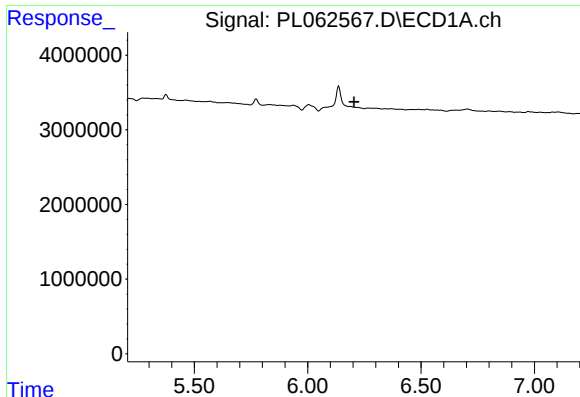

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

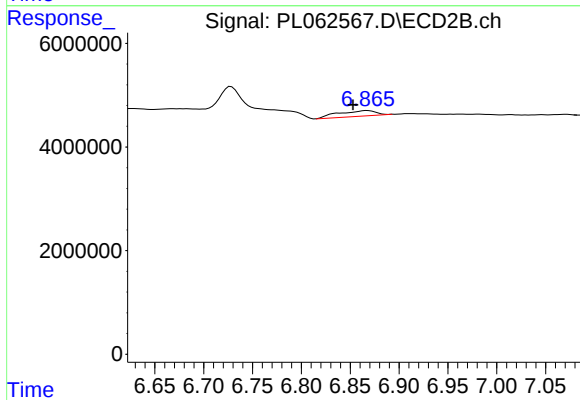


#15 Endosulfan II

R.T.: 6.867 min
Delta R.T.: 0.015 min
Response: 2771180
Conc: 0.97 ng/ml

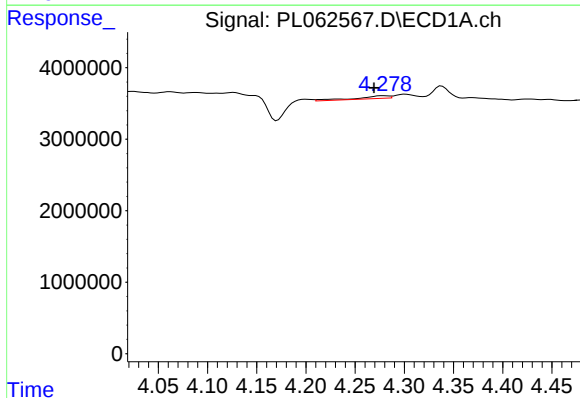


#23 Chlordane-1

R.T.: 4.279 min
Delta R.T.: 0.010 min
Response: 895902
Conc: 17.38 ng/ml

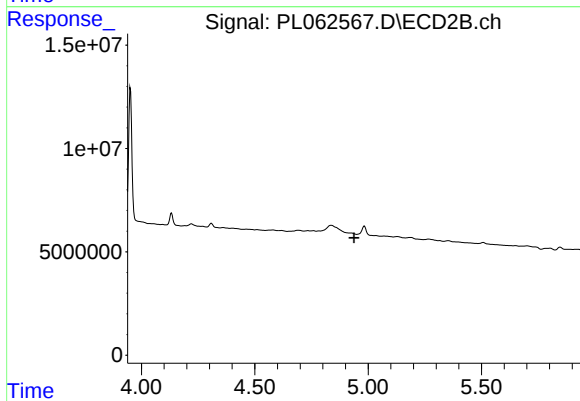

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.938 min
Response: 0
Conc: N.D.

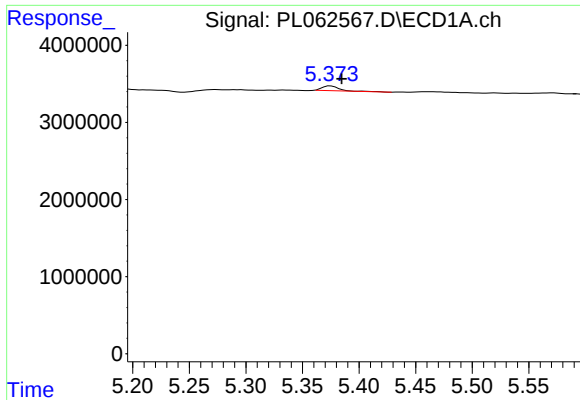

#26 Chlordane-4


R.T.: 5.375 min
Delta R.T.: -0.010 min
Response: 624097
Conc: 4.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

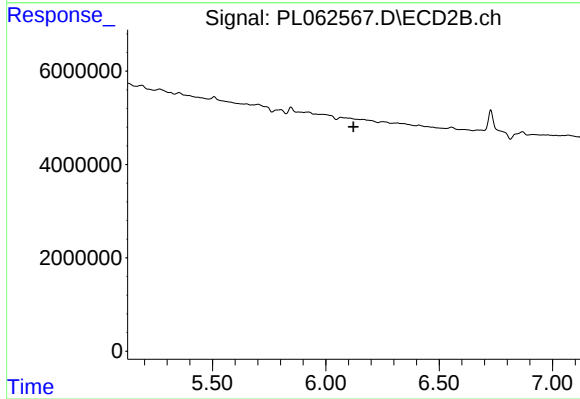


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.123 min
Response: 0
Conc: N.D.

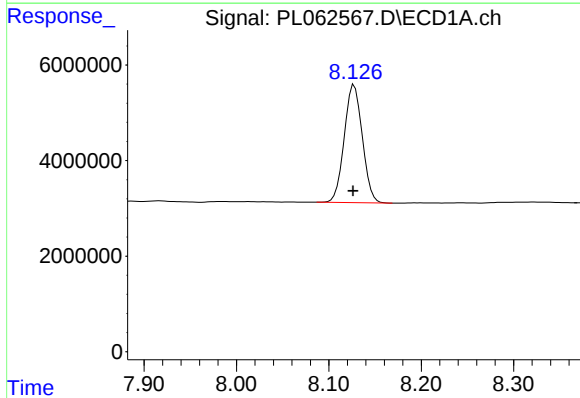

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.001 min
Response: 33499367
Conc: 20.88 ng/ml

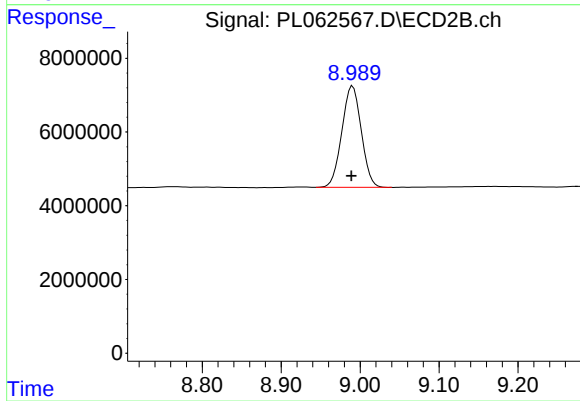

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: 0.002 min
Response: 46989448
Conc: 22.45 ng/ml