

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102418\
 Data File : PL041283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2018 11:46
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 01:04:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) A	alpha-BHC	3.886f	0.000	20307424	0	2.563	N.D. #
3) MA	gamma-BHC...	4.222	0.000	501785	0	0.069	N.D. #
5) MB	Aldrin	0.000	5.637	0	6714301	N.D.	2.225 #
6) B	beta-BHC	4.420f	4.911f	2287633	956766	0.721	0.597
7) B	delta-BHC	4.683	0.000	700721	0	0.105	N.D. #
10) B	gamma-Chl...	5.375f	0.000	4797985	0	0.730	N.D. #
14) MA	Endrin	6.072f	0.000	93577	0	0.016	N.D. #
19) B	Endosulfa...	6.719	0.000	10924089	0	2.147	N.D. #
23)	Chlordane-1	4.420	0.000	2287633	0	8.964	N.D. #
24)	Chlordane-2	4.899	5.637	2288890	6714301	8.481	54.292 #
25)	Chlordane-3	5.375	0.000	4797985	0	6.269	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102418\
Data File : PL041283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2018 11:46
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 01:04:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

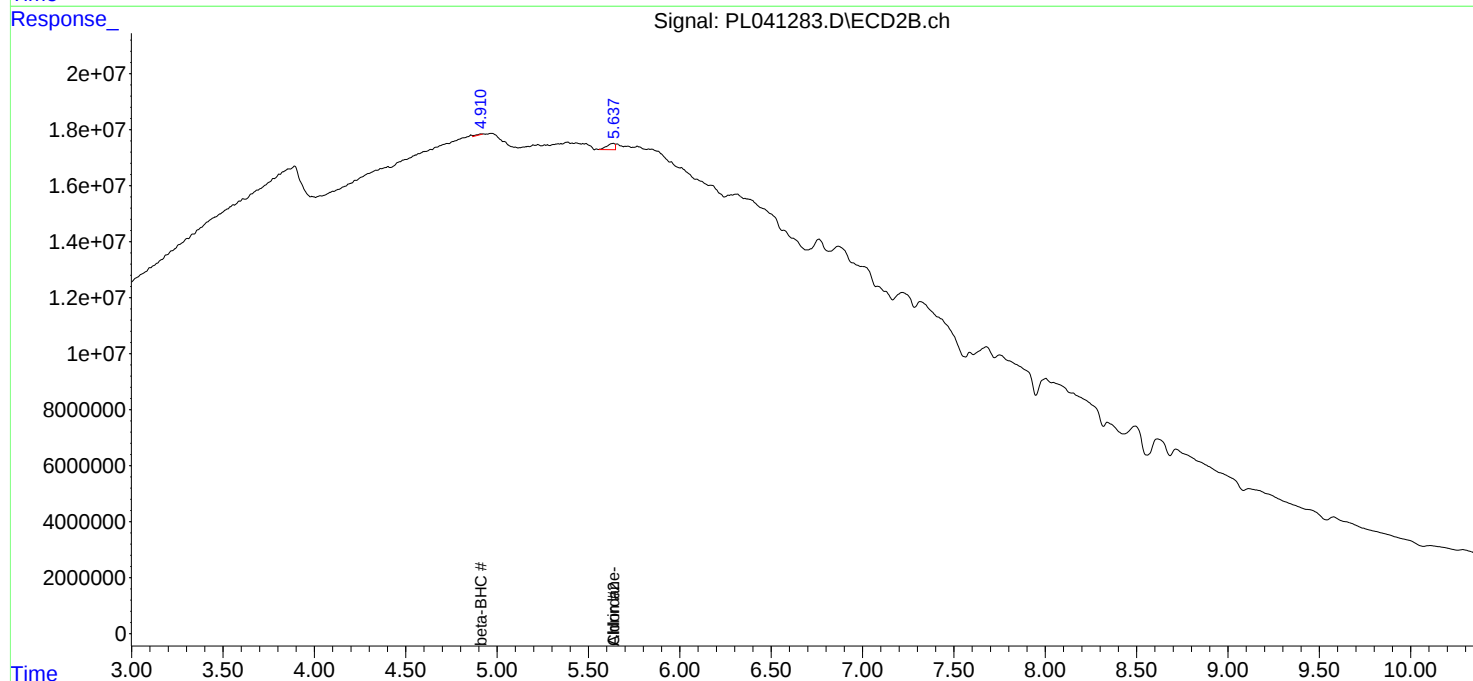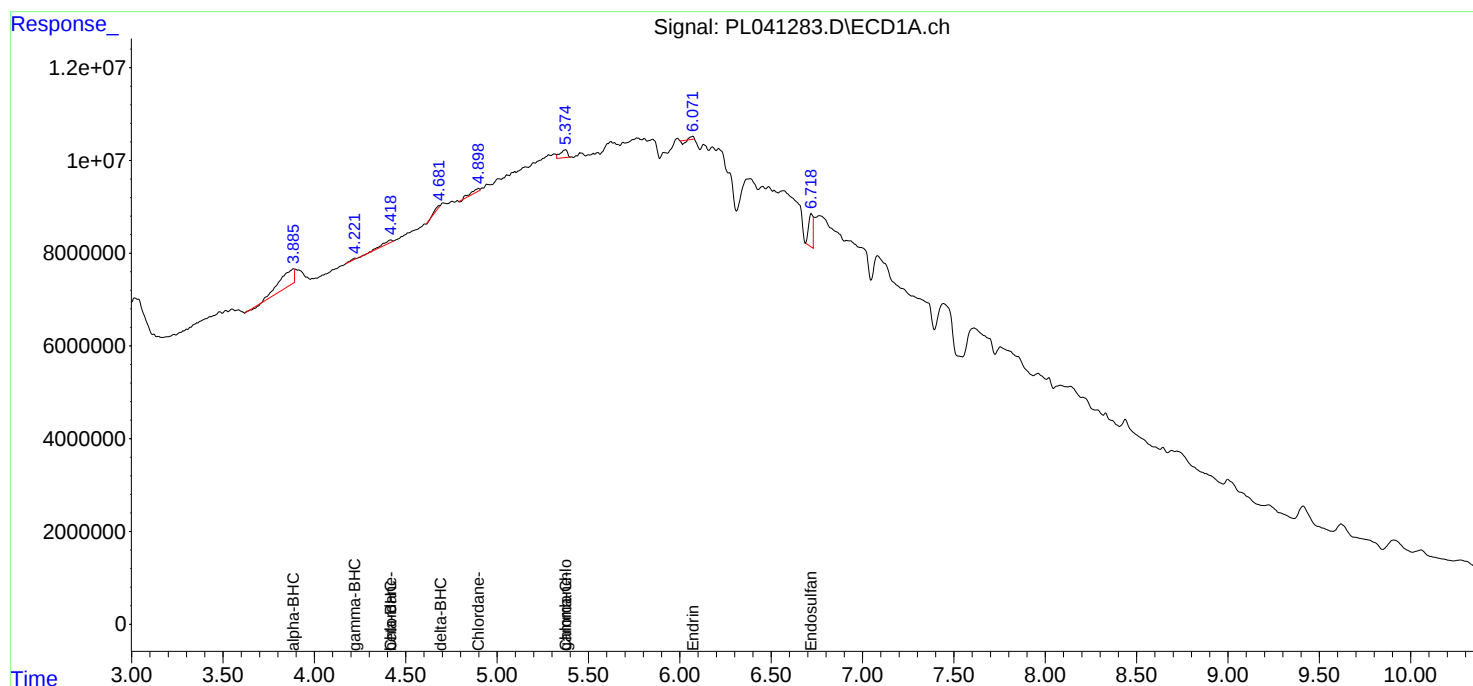


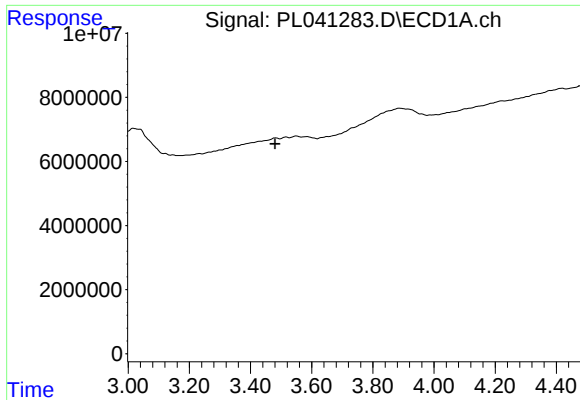

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

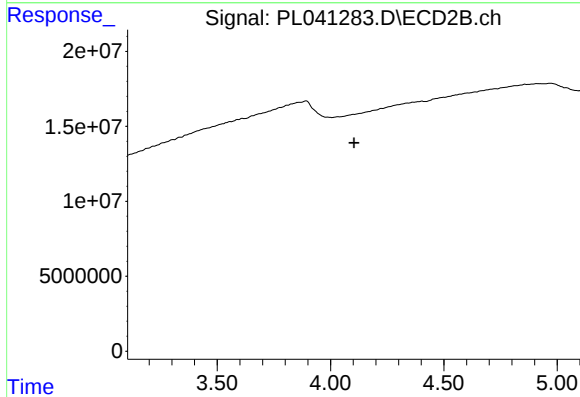


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.104 min
Response: 0
Conc: N.D.

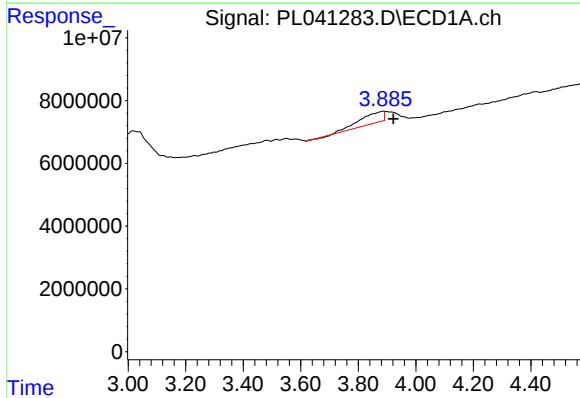


#2 alpha-BHC

R.T.: 3.886 min
Delta R.T.: -0.036 min
Response: 20307424
Conc: 2.56 ng/ml

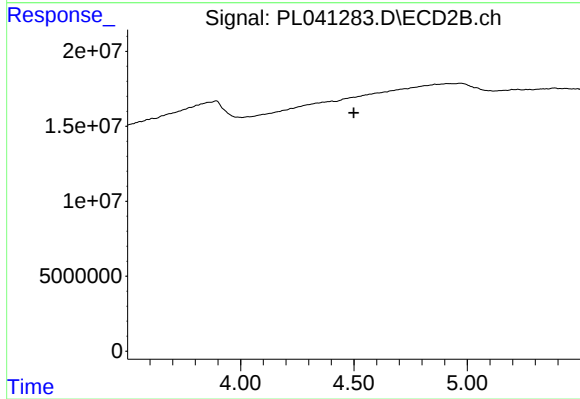

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.499 min
Response: 0
Conc: N.D.

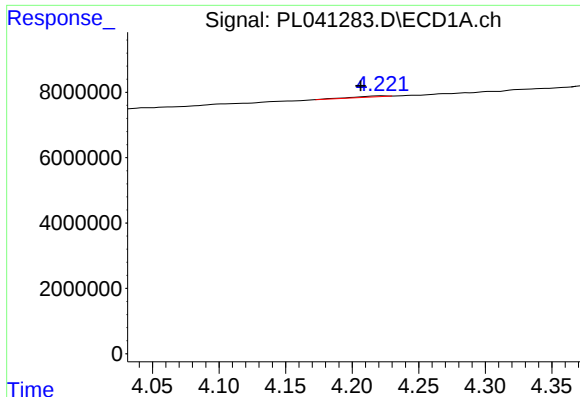

#3 gamma-BHC (Lindane)


R.T.: 4.222 min
Delta R.T.: 0.016 min
Response: 501785
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

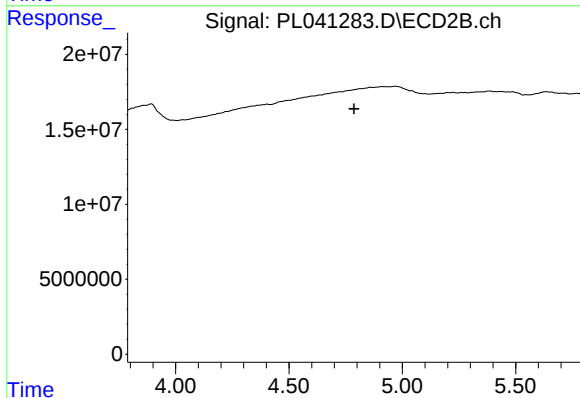


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.788 min
Response: 0
Conc: N.D.

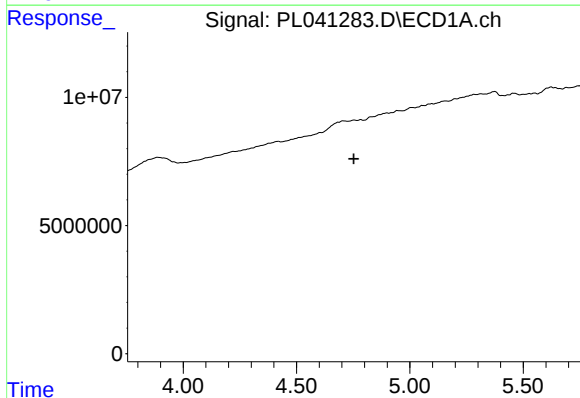


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.752 min
Response: 0
Conc: N.D.

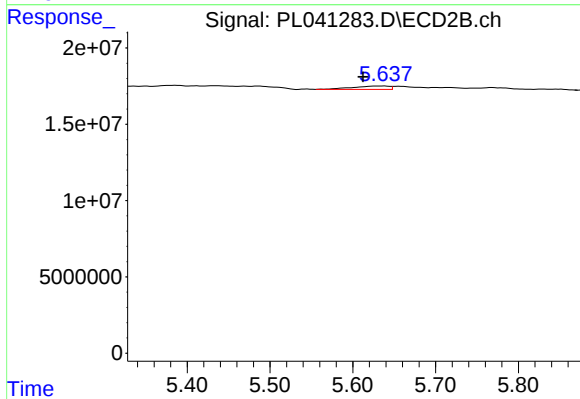

#5 Aldrin


R.T.: 5.637 min
Delta R.T.: 0.025 min
Response: 6714301
Conc: 2.22 ng/ml

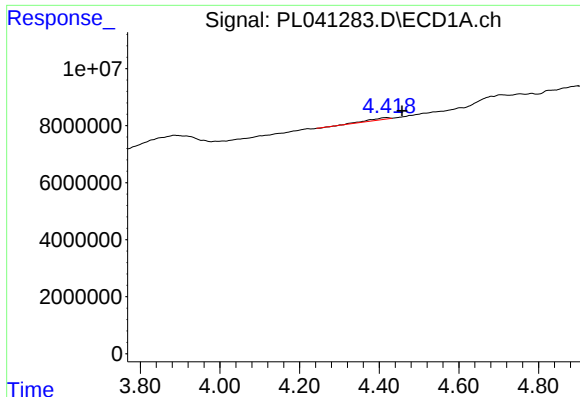

#6 beta-BHC


R.T.: 4.420 min
Delta R.T.: -0.038 min
Response: 2287633
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

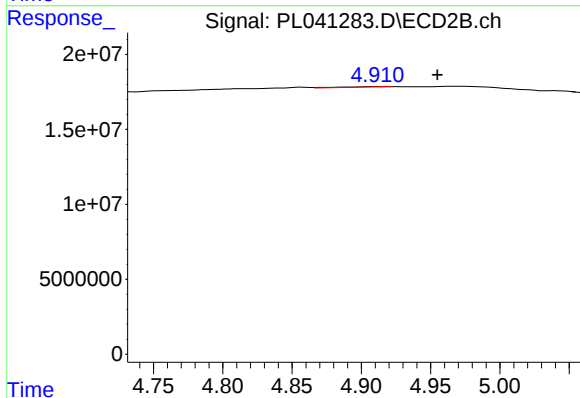


#6 beta-BHC

R.T.: 4.911 min
Delta R.T.: -0.044 min
Response: 956766
Conc: 0.60 ng/ml

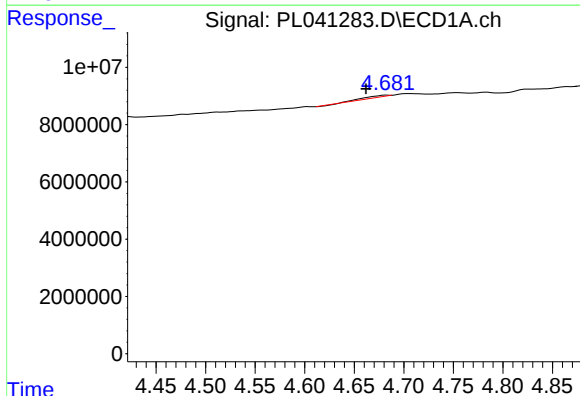


#7 delta-BHC

R.T.: 4.683 min
Delta R.T.: 0.021 min
Response: 700721
Conc: 0.11 ng/ml

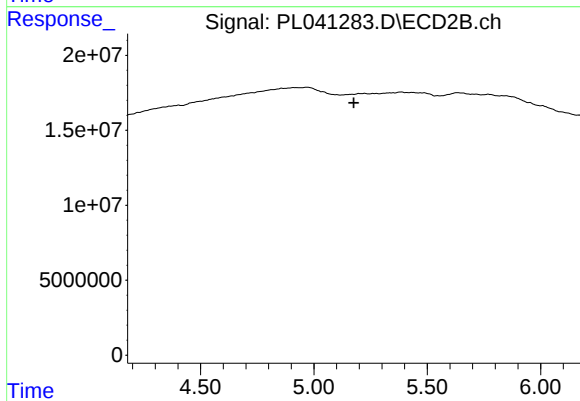

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 5.176 min
Response: 0
Conc: N.D.

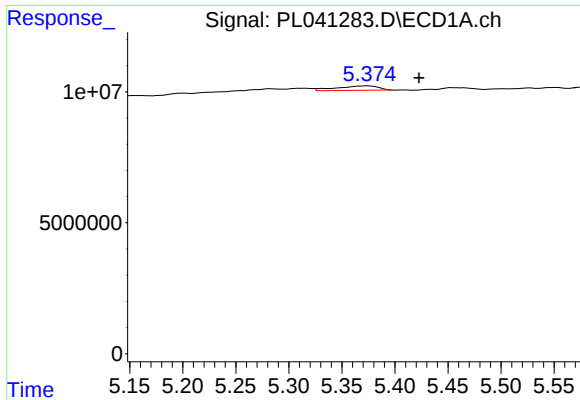

#10 gamma-Chlordane


R.T.: 5.375 min
Delta R.T.: -0.048 min
Response: 4797985
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

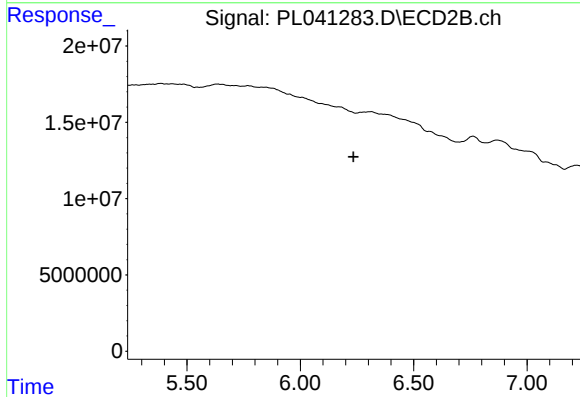


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.235 min
Response: 0
Conc: N.D.

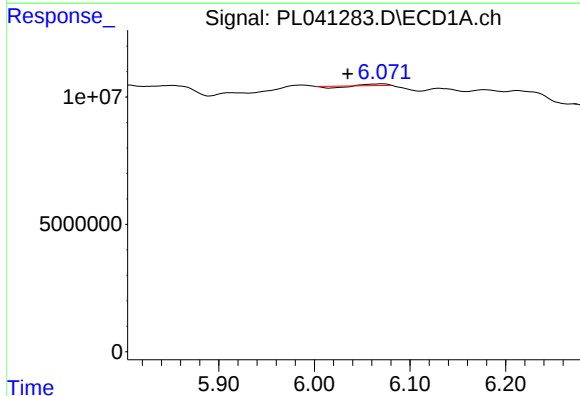


#14 Endrin

R.T.: 6.072 min
Delta R.T.: 0.037 min
Response: 93577
Conc: 0.02 ng/ml

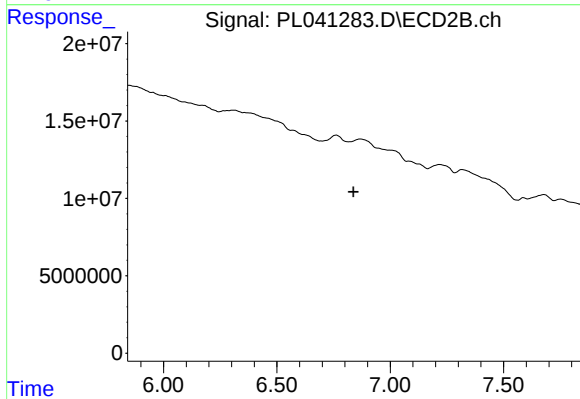

#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.838 min
Response: 0
Conc: N.D.

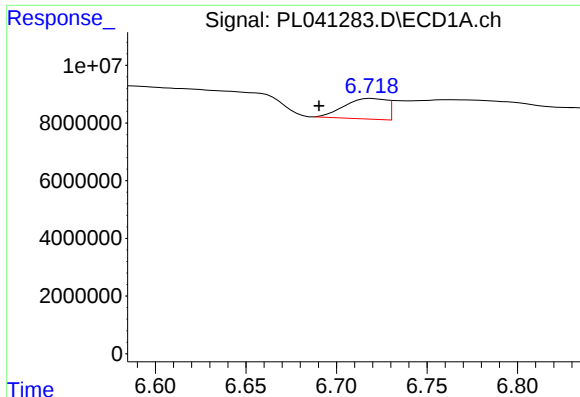

#19 Endosulfan Sulfate


R.T.: 6.719 min

Delta R.T.: 0.029 min

Response: 10924089

Conc: 2.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

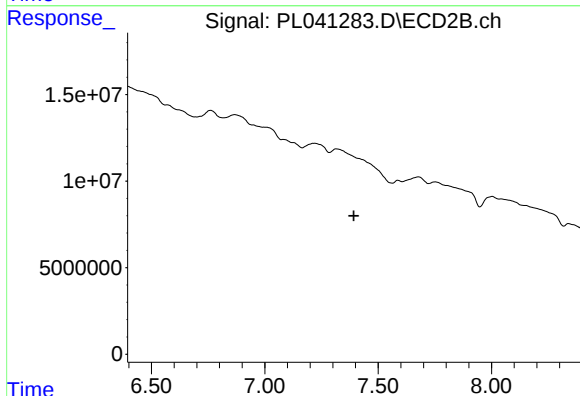


#19 Endosulfan Sulfate

R.T.: 0.000 min

Exp R.T. : 7.392 min

Response: 0

Conc: N.D.

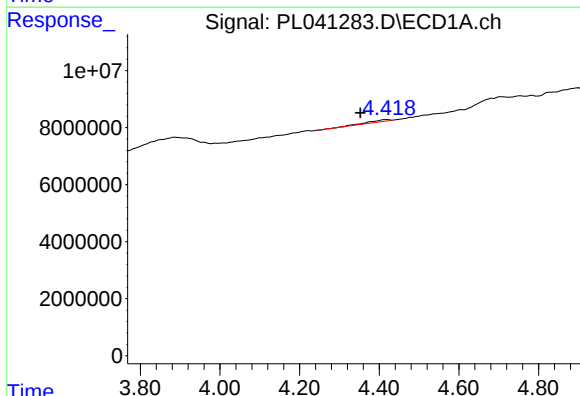


#23 Chlordane-1

R.T.: 4.420 min

Delta R.T.: 0.067 min

Response: 2287633

Conc: 8.96 ng/ml

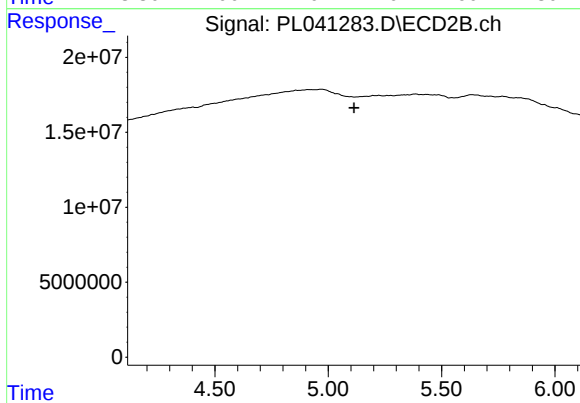


#23 Chlordane-1

R.T.: 0.000 min

Exp R.T. : 5.114 min

Response: 0


Conc: N.D.

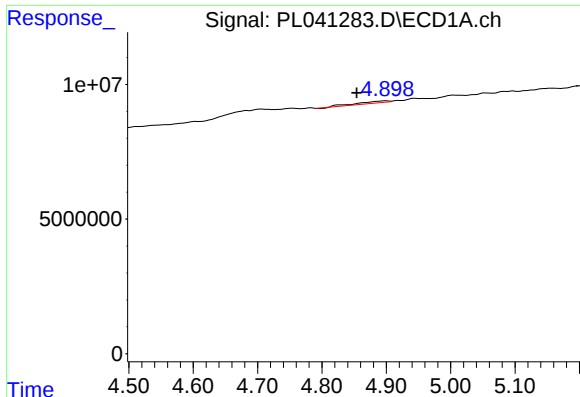

#24 Chlordane-2


R.T.: 4.899 min
Delta R.T.: 0.045 min
Response: 2288890
Conc: 8.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

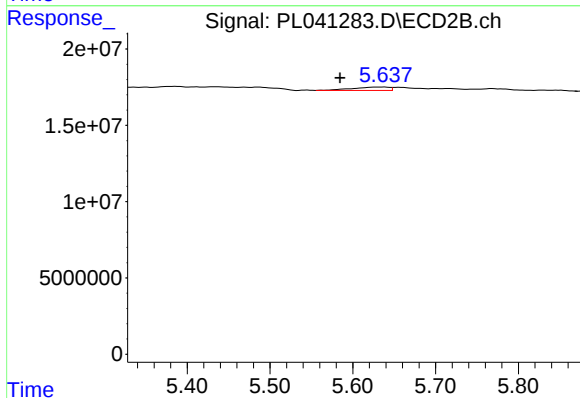


#24 Chlordane-2

R.T.: 5.637 min
Delta R.T.: 0.052 min
Response: 6714301
Conc: 54.29 ng/ml

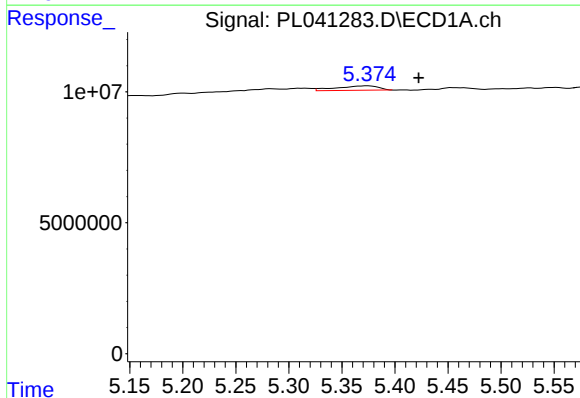


#25 Chlordane-3

R.T.: 5.375 min
Delta R.T.: -0.048 min
Response: 4797985
Conc: 6.27 ng/ml

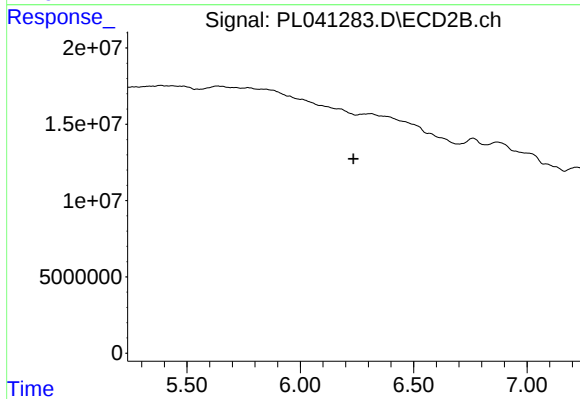

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.235 min
Response: 0
Conc: N.D.

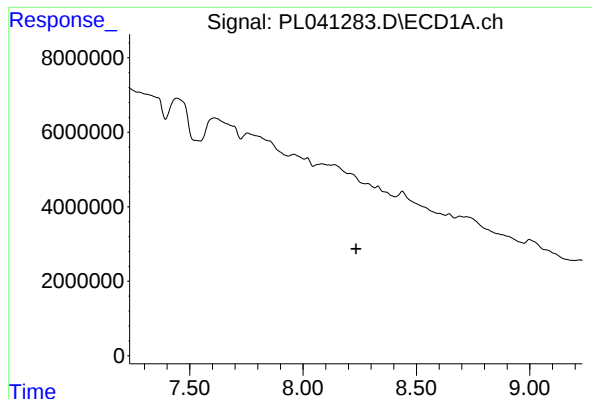

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.234 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

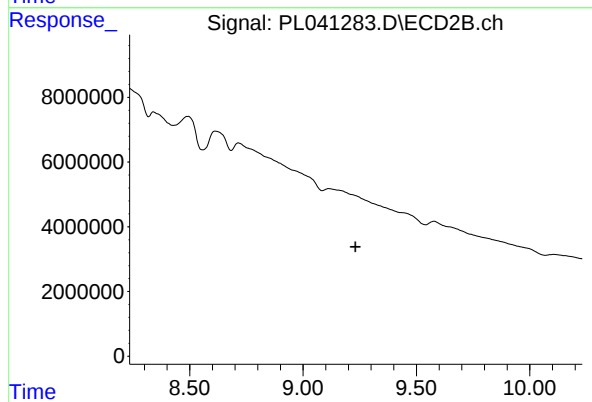

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.231 min
Response: 0
Conc: N.D.