

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102418\
 Data File : PL041312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2018 19:53
 Operator : AJ\SJ
 Sample : J5625-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 01:11:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.103	54220143	28894964	9.893	10.363
28)	SA Decachlor...	8.219	9.233	60926806	27062022	11.718	10.465
Target Compounds							
6)	B beta-BHC	4.412f	4.995f	6469026	3308446	2.039	2.064
12)	B 4,4'-DDE	5.636	0.000	2040178	0	0.359	N.D. #
15)	B Endosulfa...	6.241f	0.000	5169490	0	0.922	N.D. #
17)	MA 4,4'-DDT	6.387	0.000	2638481	0	0.579	N.D. #
18)	B Endrin al...	6.429f	0.000	838816	0	0.200	N.D. #
19)	B Endosulfa...	6.701	0.000	795305	0	0.156	N.D. #
20)	A Methoxychlor	6.917f	0.000	1206080	0	0.464	N.D. #
21)	B Endrin ke...	0.000	7.826f	0	3096608	N.D.	1.317 #
23)	Chlordane-1	4.348	0.000	1407895	0	5.517	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102418\
Data File : PL041312.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2018 19:53
Operator : AJ\SJ
Sample : J5625-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 01:11:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

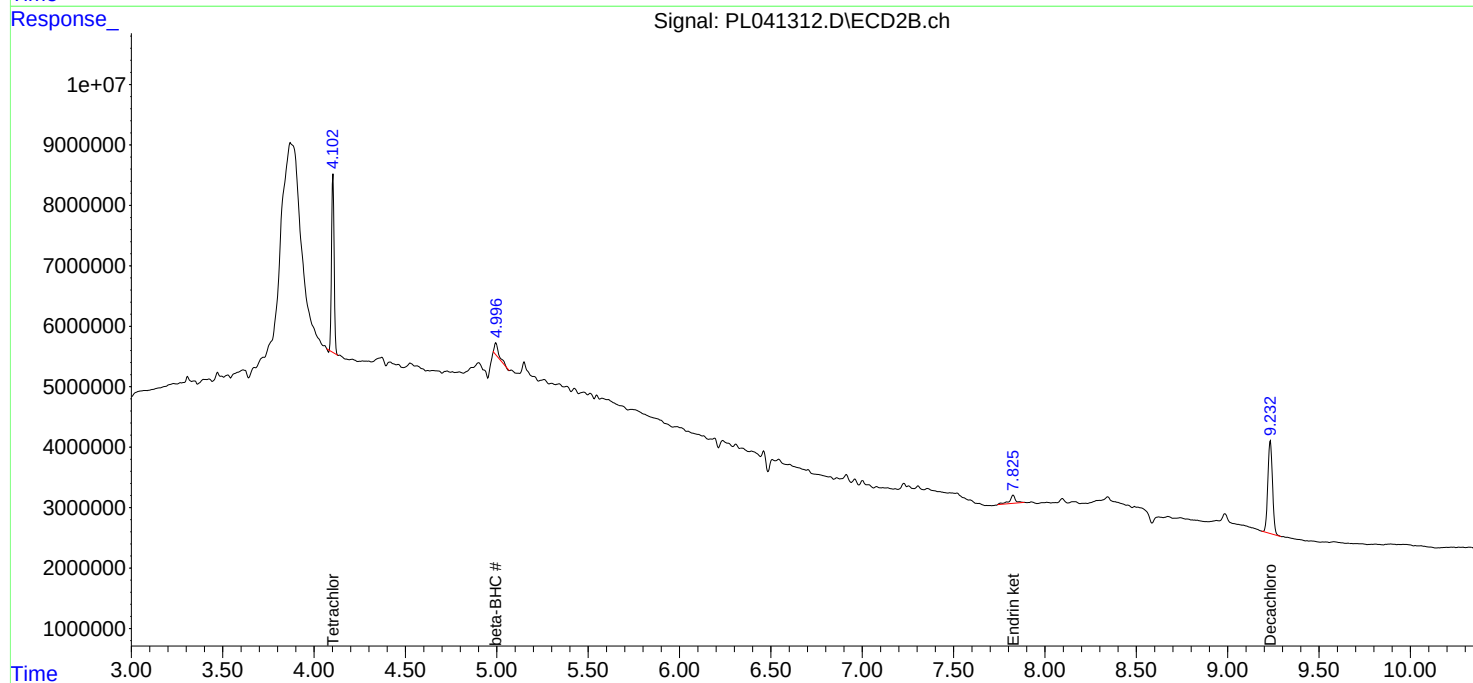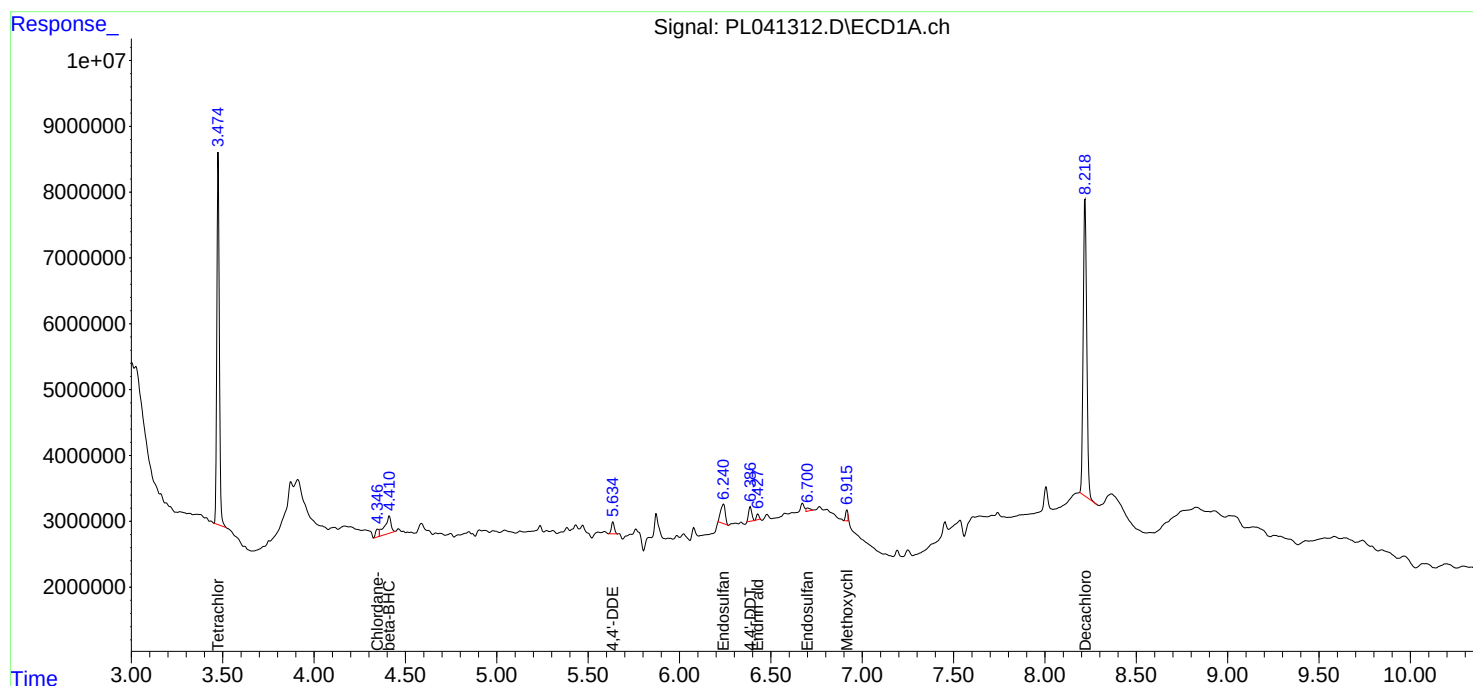


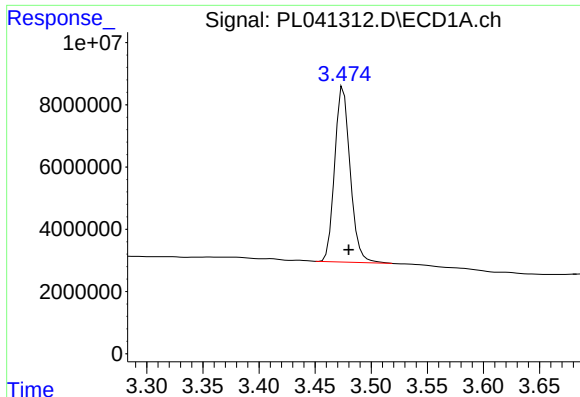

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: -0.005 min
Response: 54220143
Conc: 9.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

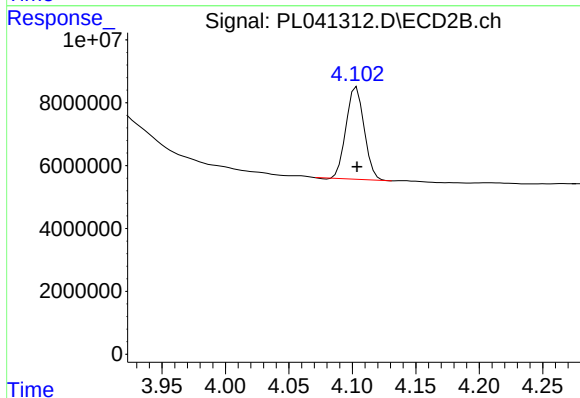


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.000 min
Response: 28894964
Conc: 10.36 ng/ml

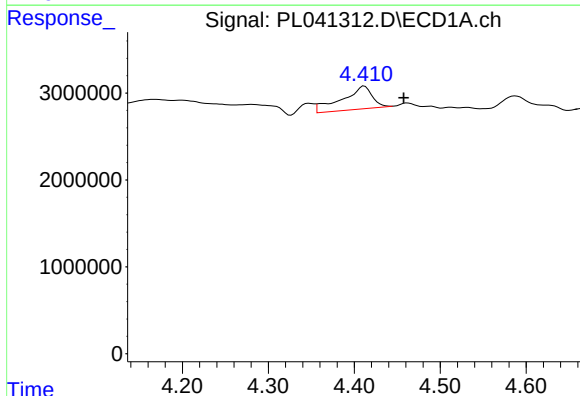


#6 beta-BHC

R.T.: 4.412 min
Delta R.T.: -0.046 min
Response: 6469026
Conc: 2.04 ng/ml

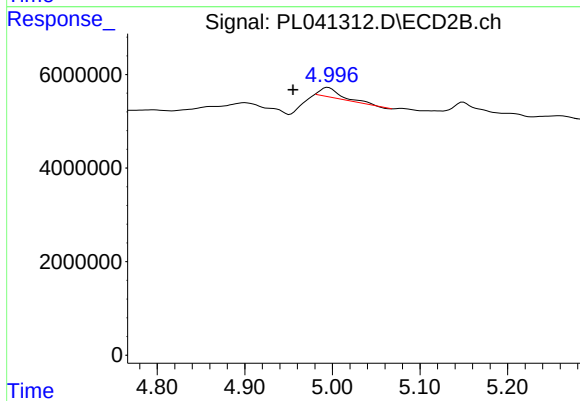

#6 beta-BHC


R.T.: 4.995 min
Delta R.T.: 0.040 min
Response: 3308446
Conc: 2.06 ng/ml

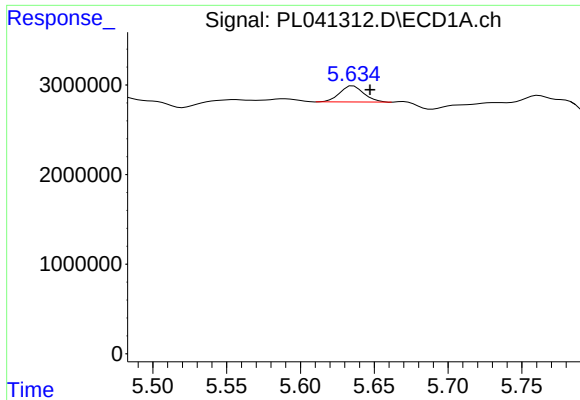

#12 4,4'-DDE


R.T.: 5.636 min
Delta R.T.: -0.011 min
Response: 2040178
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

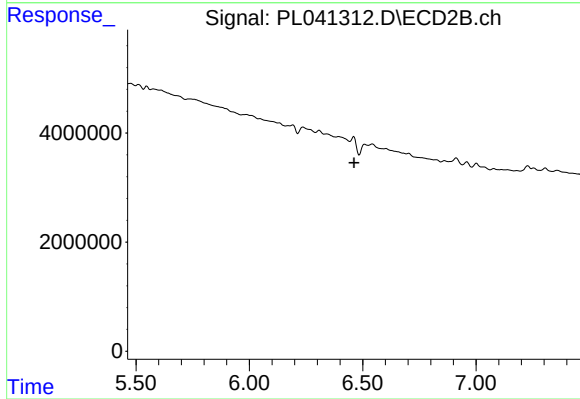


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.462 min
Response: 0
Conc: N.D.

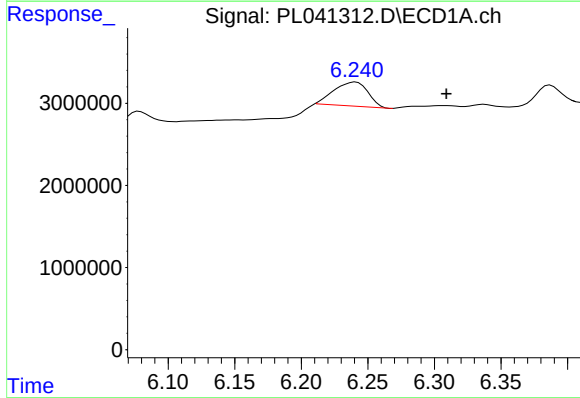


#15 Endosulfan II

R.T.: 6.241 min
Delta R.T.: -0.068 min
Response: 5169490
Conc: 0.92 ng/ml

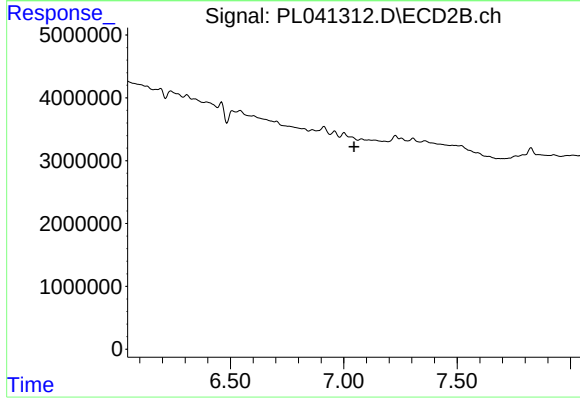

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.045 min
Response: 0
Conc: N.D.

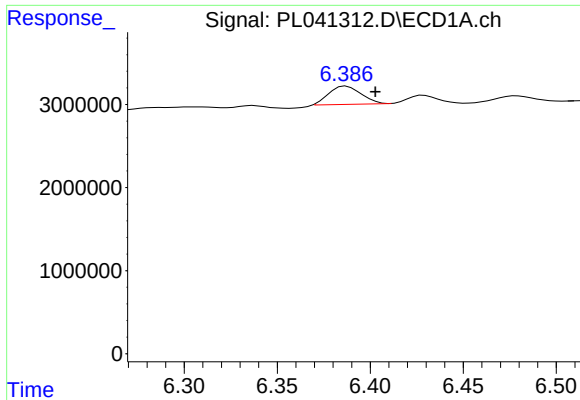

#17 4,4'-DDT


R.T.: 6.387 min
Delta R.T.: -0.016 min
Response: 2638481
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

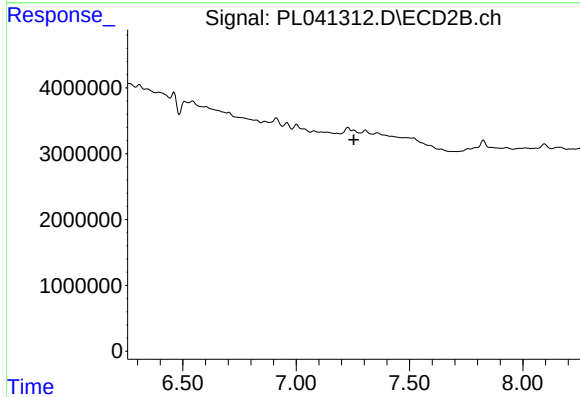


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.254 min
Response: 0
Conc: N.D.

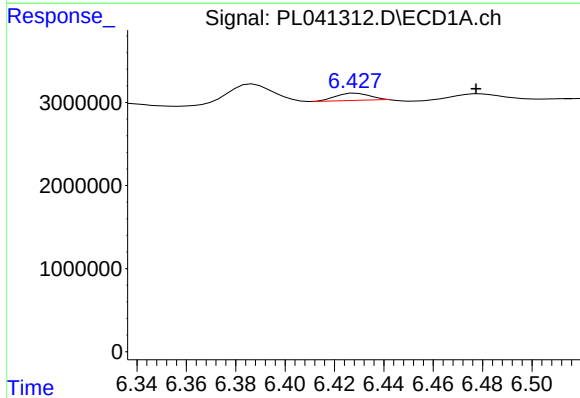


#18 Endrin aldehyde

R.T.: 6.429 min
Delta R.T.: -0.048 min
Response: 838816
Conc: 0.20 ng/ml

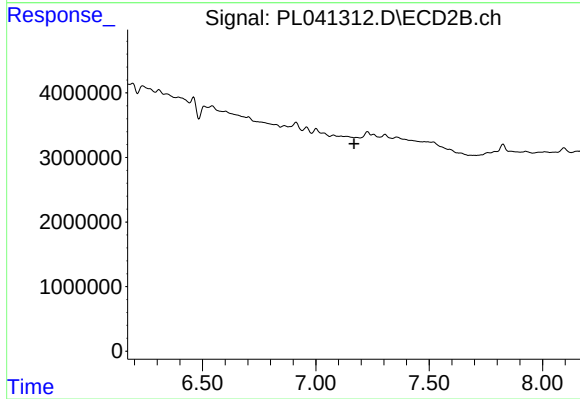

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.169 min
Response: 0
Conc: N.D.

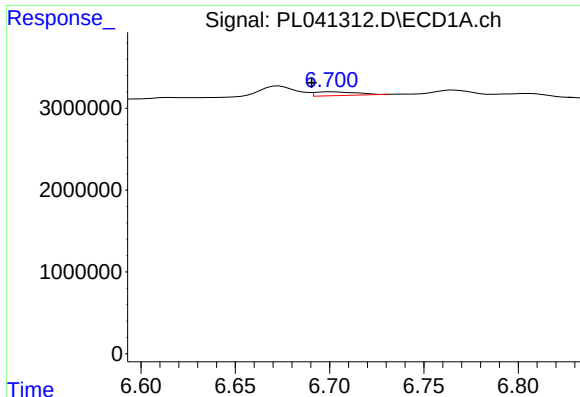

#19 Endosulfan Sulfate


R.T.: 6.701 min
Delta R.T.: 0.011 min
Response: 795305
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

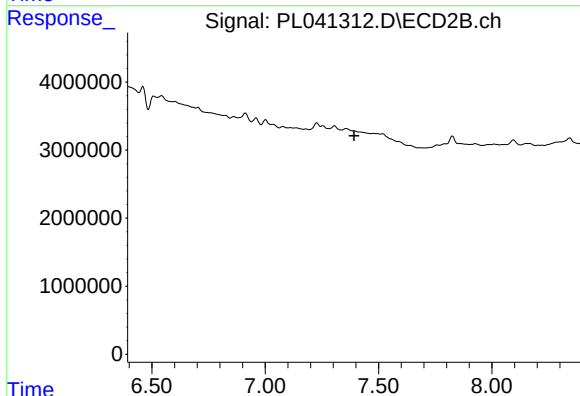


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

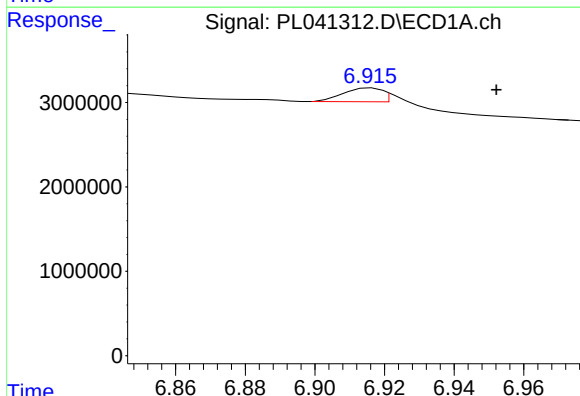


#20 Methoxychlor

R.T.: 6.917 min
Delta R.T.: -0.036 min
Response: 1206080
Conc: 0.46 ng/ml

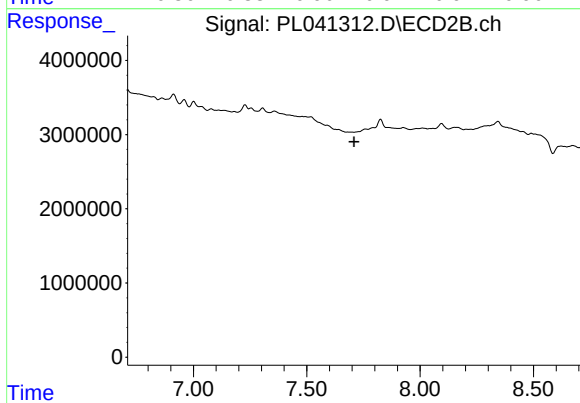

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

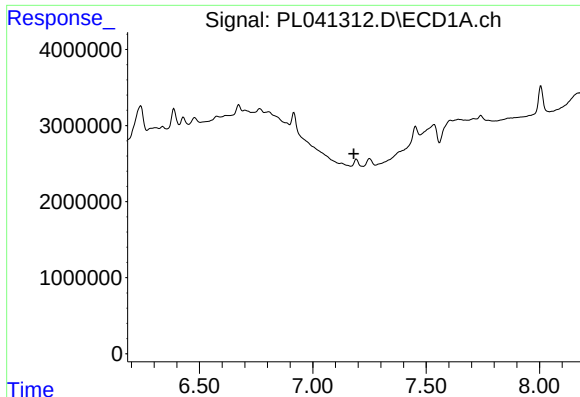

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.181 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

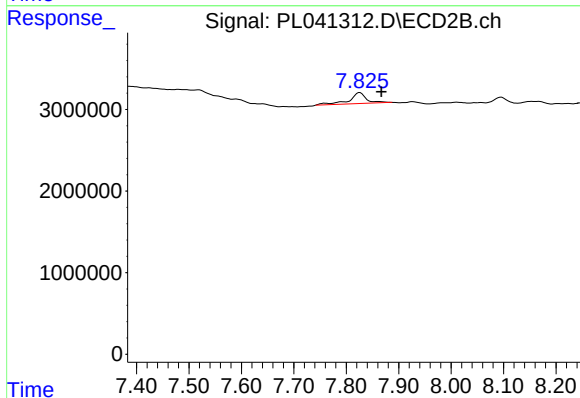


#21 Endrin ketone

R.T.: 7.826 min
Delta R.T.: -0.041 min
Response: 3096608
Conc: 1.32 ng/ml

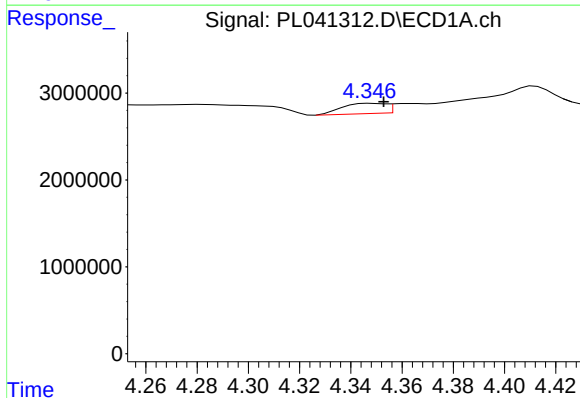


#23 Chlordane-1

R.T.: 4.348 min
Delta R.T.: -0.005 min
Response: 1407895
Conc: 5.52 ng/ml

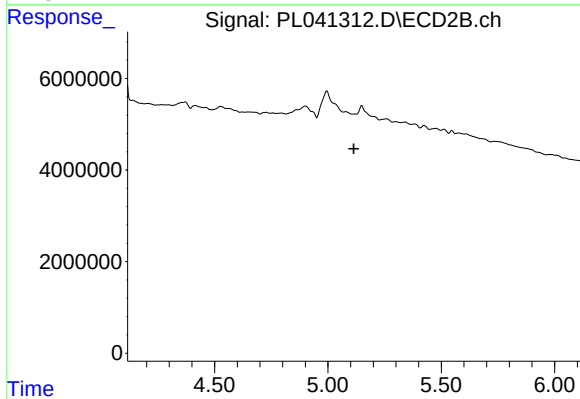

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.114 min
Response: 0
Conc: N.D.

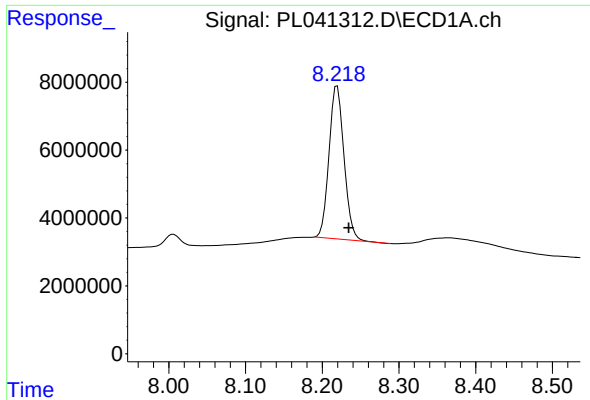

#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: -0.015 min
Response: 60926806
Conc: 11.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

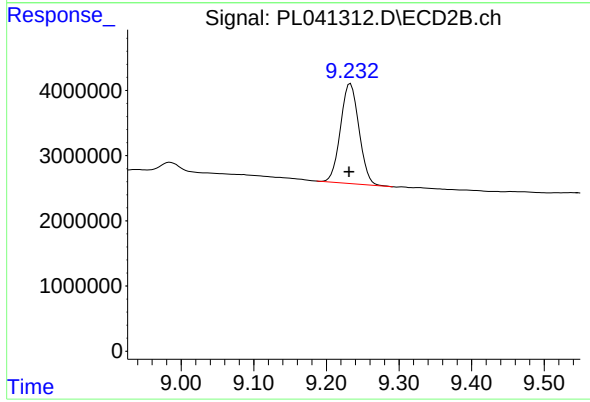

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.002 min
Response: 27062022
Conc: 10.47 ng/ml