

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102418\
 Data File : PL041320.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2018 22:14
 Operator : AJ\SJ
 Sample : J5642-02
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 04:36:39 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.104	112.5E6	59990965	20.518	21.515
28)	SA Decachlor...	8.220	9.234	100.6E6	44622593	19.346	17.256
Target Compounds							
2)	A alpha-BHC	3.883f	0.000	1943150	0	0.245	N.D. #
6)	B beta-BHC	4.414f	4.995f	8478376	1632916	2.672	1.019 #
7)	B delta-BHC	0.000	5.150f	0	1828241	N.D.	0.557 #
23)	Chlordane-1	4.388	5.150	4191424	1828241	16.423	14.802



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102418\
Data File : PL041320.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2018 22:14
Operator : AJ\SJ
Sample : J5642-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 04:36:39 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

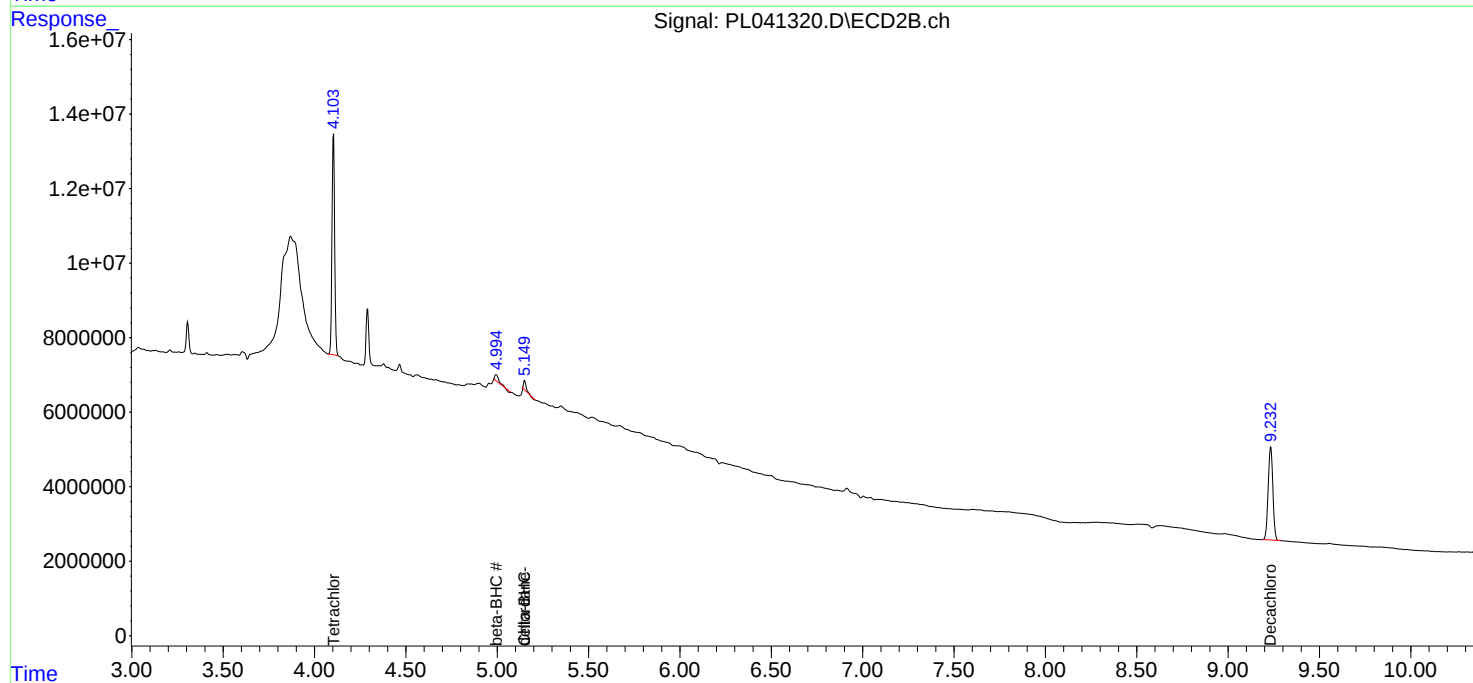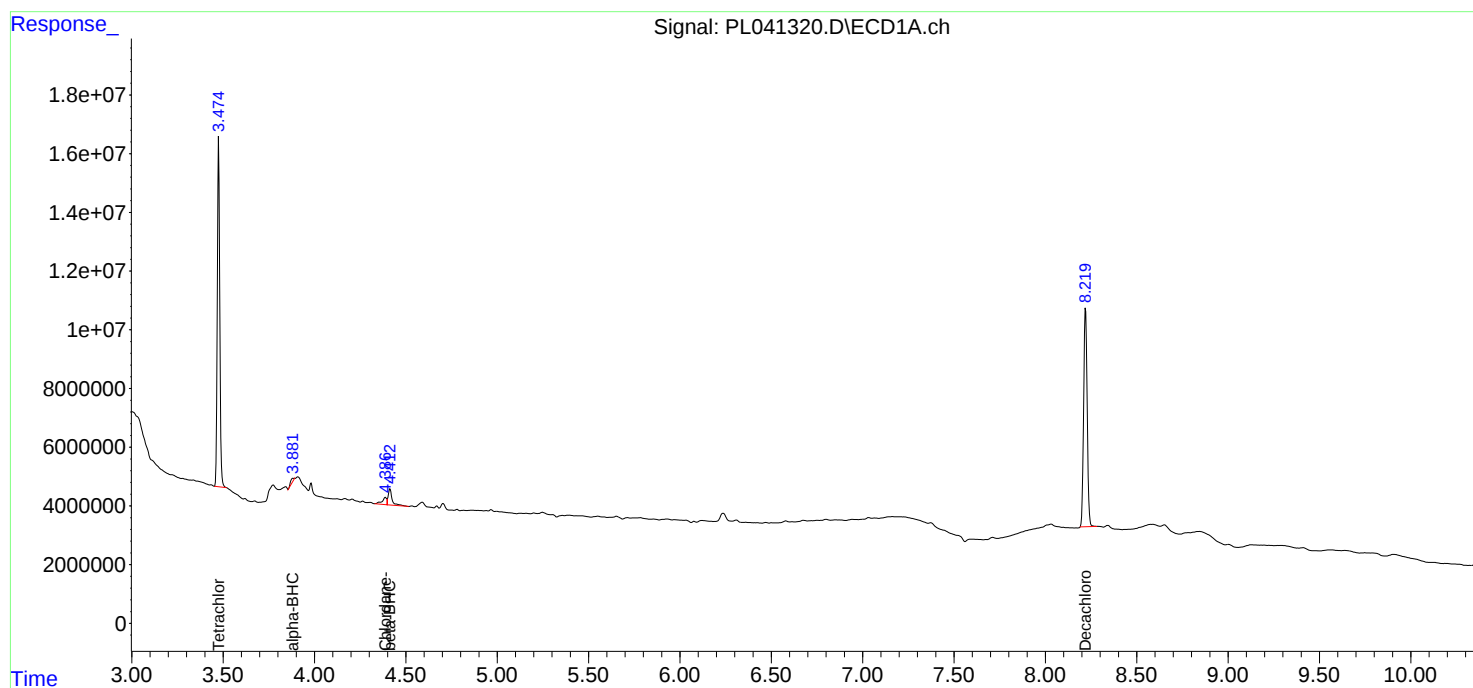


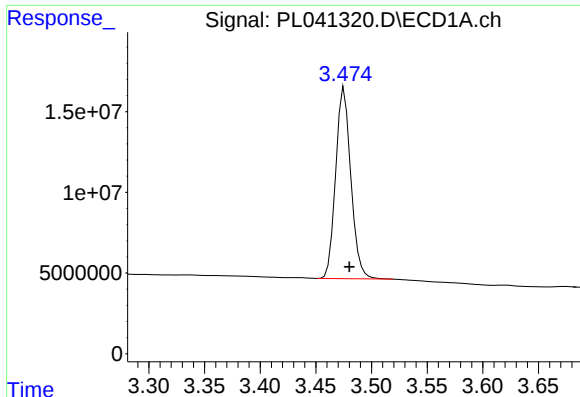

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: -0.004 min
Response: 112455361
Conc: 20.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

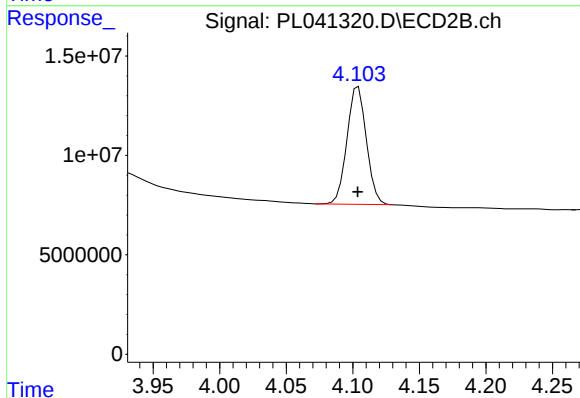


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 59990965
Conc: 21.52 ng/ml

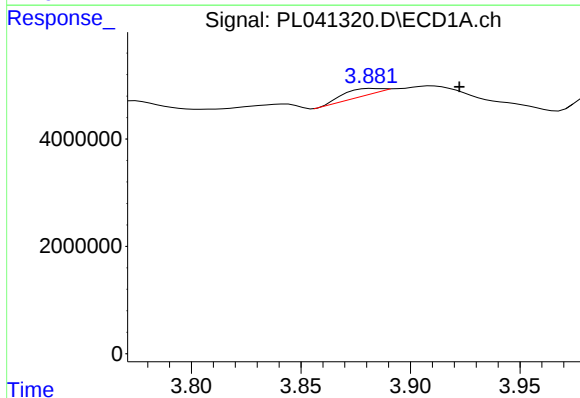


#2 alpha-BHC

R.T.: 3.883 min
Delta R.T.: -0.040 min
Response: 1943150
Conc: 0.25 ng/ml

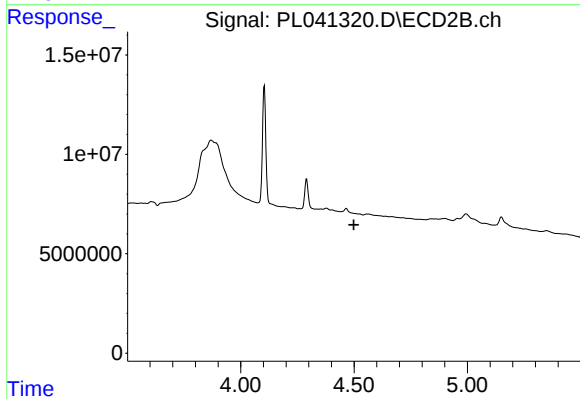

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.499 min
Response: 0
Conc: N.D.

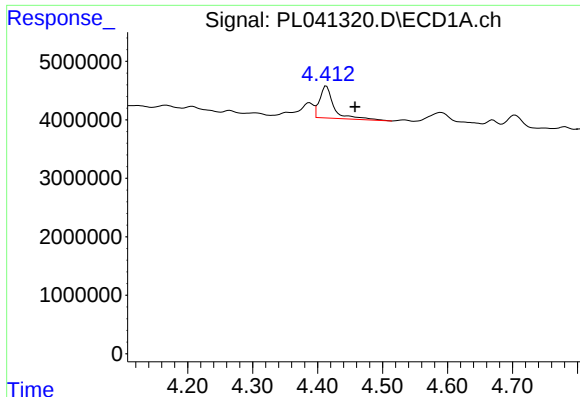

#6 beta-BHC


R.T.: 4.414 min
Delta R.T.: -0.044 min
Response: 8478376
Conc: 2.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

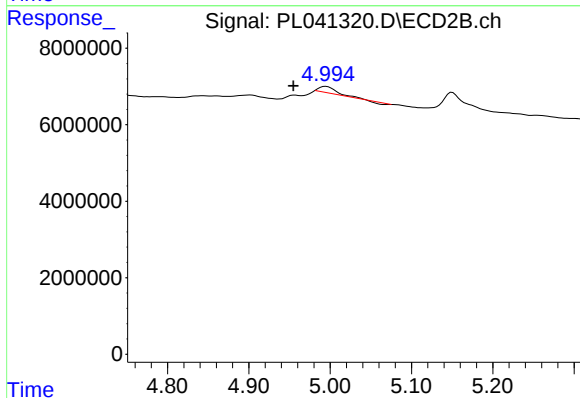


#6 beta-BHC

R.T.: 4.995 min
Delta R.T.: 0.040 min
Response: 1632916
Conc: 1.02 ng/ml

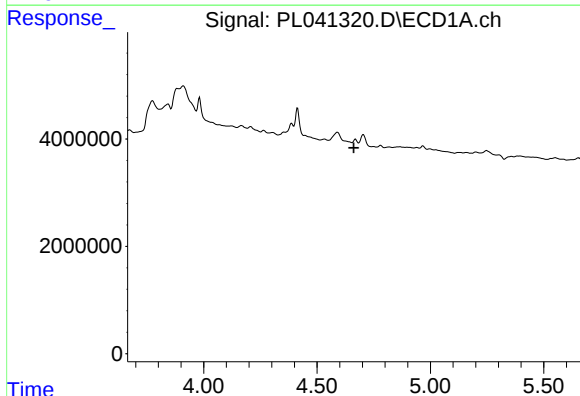


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.662 min
Response: 0
Conc: N.D.

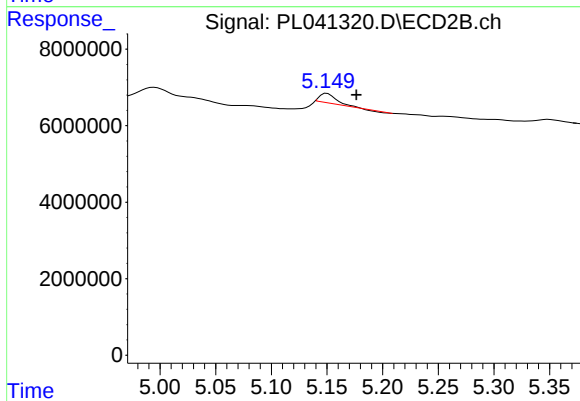

#7 delta-BHC


R.T.: 5.150 min
Delta R.T.: -0.026 min
Response: 1828241
Conc: 0.56 ng/ml

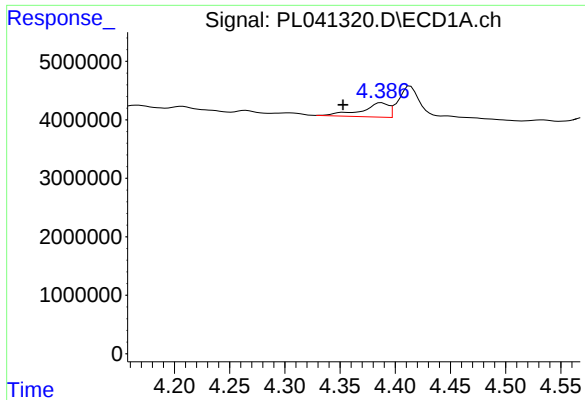

#23 Chlordane-1


R.T.: 4.388 min
Delta R.T.: 0.035 min
Response: 4191424
Conc: 16.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

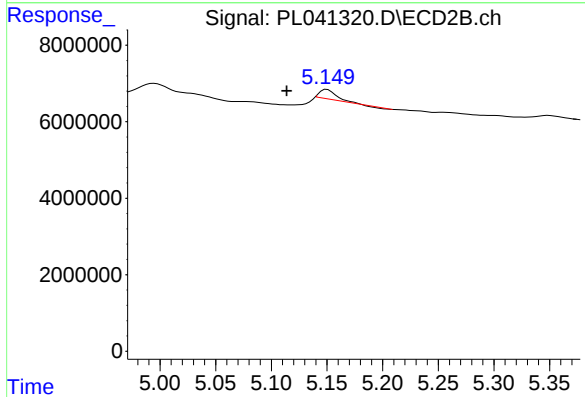


#23 Chlordane-1

R.T.: 5.150 min
Delta R.T.: 0.036 min
Response: 1828241
Conc: 14.80 ng/ml

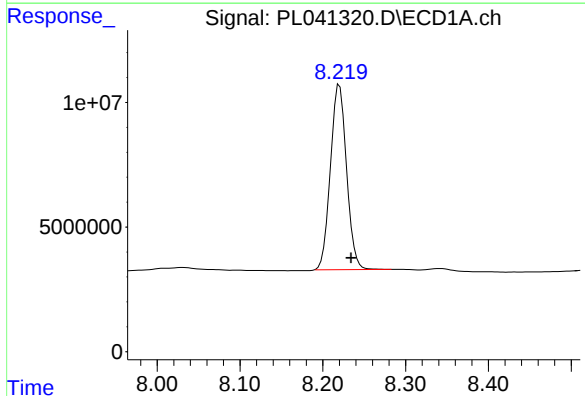

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: -0.014 min
Response: 100587436
Conc: 19.35 ng/ml

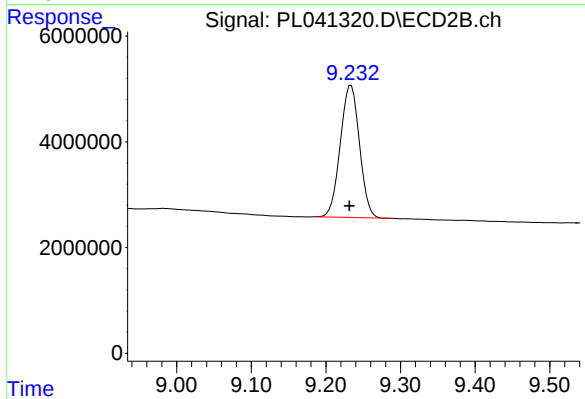

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.002 min
Response: 44622593
Conc: 17.26 ng/ml