

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102418\
 Data File : PL041321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2018 22:28
 Operator : AJ\SJ
 Sample : J5647-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 04:36:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.104	110.5E6	59061961	20.165	21.182
28)	SA Decachlor...	8.220	9.233	96800558	39842783	18.617	15.408
Target Compounds							
3)	MA gamma-BHC...	4.208	4.769	11664477	4091129	1.597	1.149 #
6)	B beta-BHC	4.414f	4.994f	5462617	3216527	1.722	2.007
7)	B delta-BHC	0.000	5.151f	0	1318528	N.D.	0.402 #
8)	B Heptachlo...	5.252f	0.000	5683929	0	0.867	N.D. #
9)	A Endosulfan I	5.551	0.000	1599384	0	0.267	N.D. #
10)	B gamma-Chl...	0.000	6.220	0	8152516	N.D.	2.907 #
16)	A 4,4'-DDD	6.109f	0.000	1574238	0	0.349	N.D. #
23)	Chlordane-1	4.387	5.151	2275524	1318528	8.916	10.675
25)	Chlordane-3	0.000	6.220	0	8152516	N.D.	20.223 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102418\
Data File : PL041321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2018 22:28
Operator : AJ\SJ
Sample : J5647-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 04:36:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

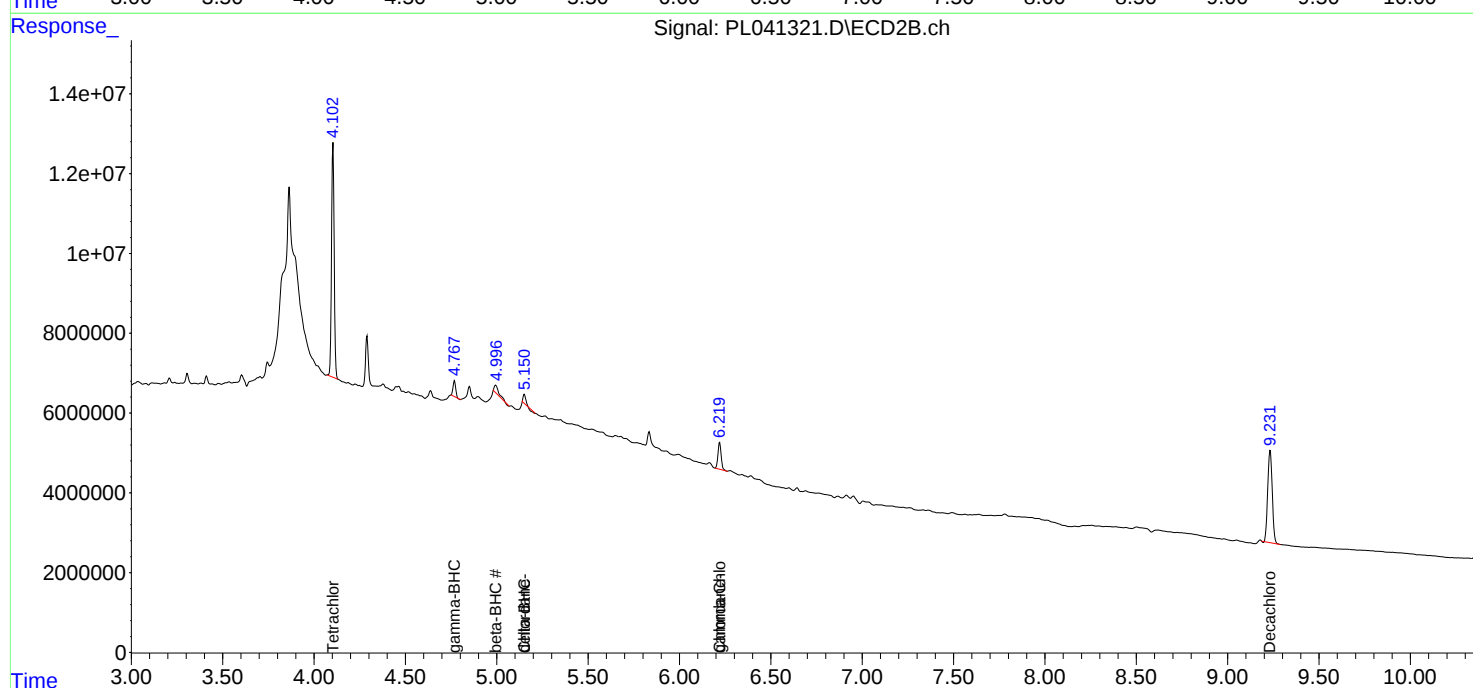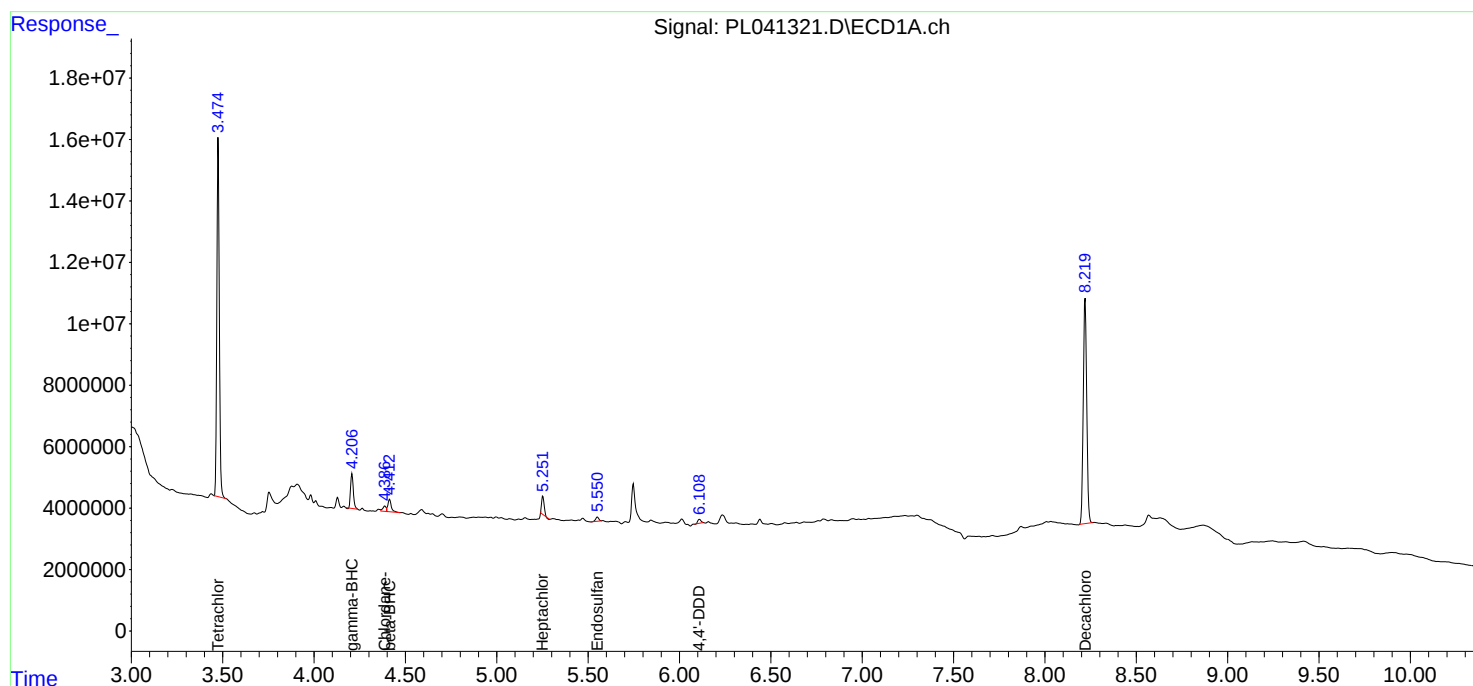


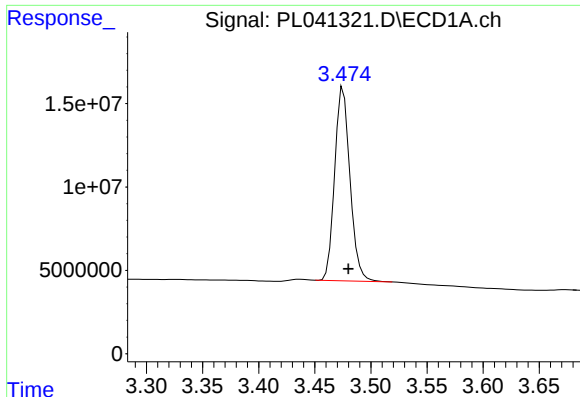

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: -0.004 min
Response: 110518987
Conc: 20.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

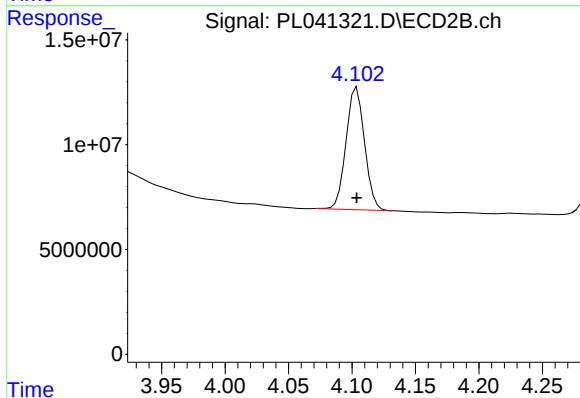


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 59061961
Conc: 21.18 ng/ml

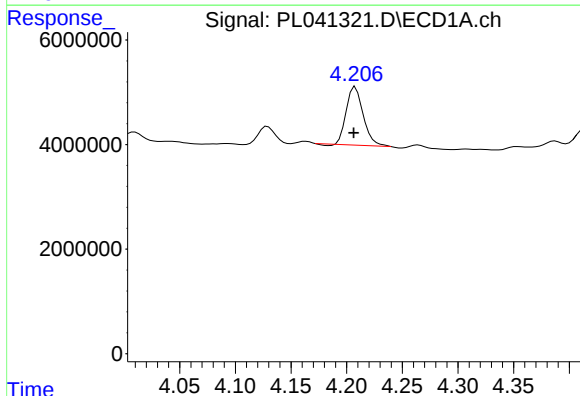


#3 gamma-BHC (Lindane)

R.T.: 4.208 min
Delta R.T.: 0.002 min
Response: 11664477
Conc: 1.60 ng/ml

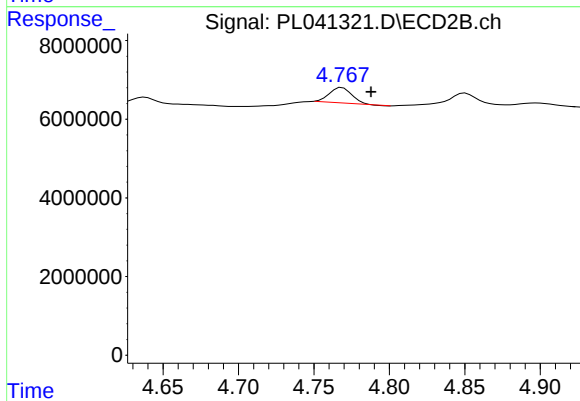

#3 gamma-BHC (Lindane)


R.T.: 4.769 min
Delta R.T.: -0.019 min
Response: 4091129
Conc: 1.15 ng/ml

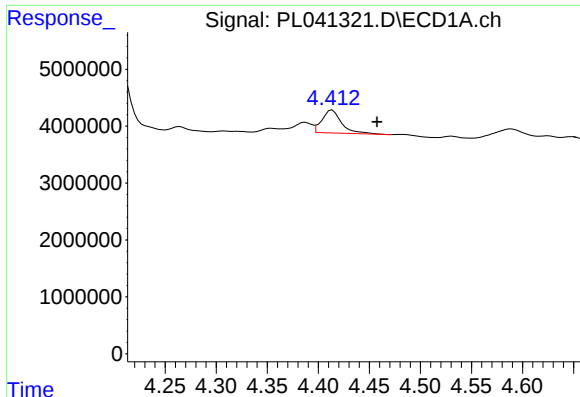

#6 beta-BHC


R.T.: 4.414 min
Delta R.T.: -0.044 min
Response: 5462617
Conc: 1.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

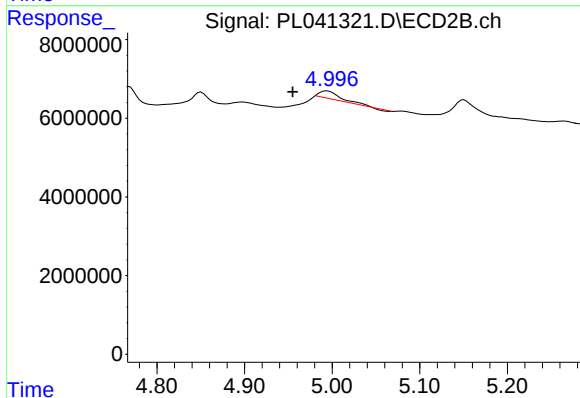


#6 beta-BHC

R.T.: 4.994 min
Delta R.T.: 0.039 min
Response: 3216527
Conc: 2.01 ng/ml

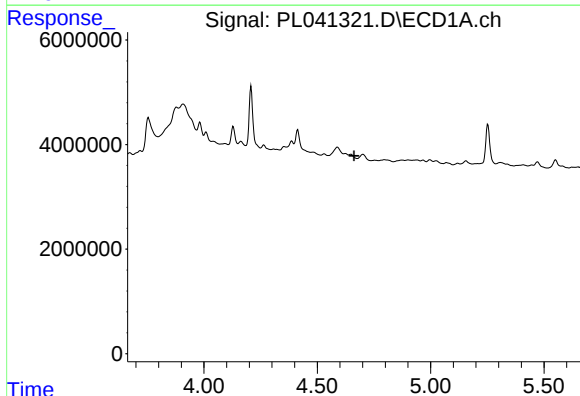


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.662 min
Response: 0
Conc: N.D.

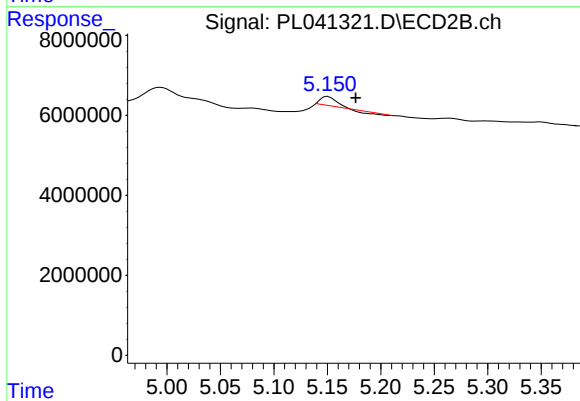

#7 delta-BHC


R.T.: 5.151 min
Delta R.T.: -0.026 min
Response: 1318528
Conc: 0.40 ng/ml

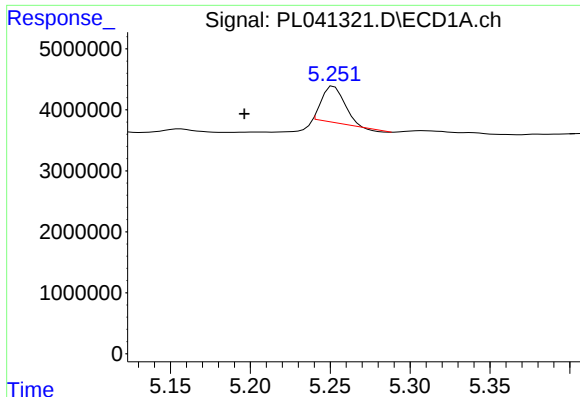

#8 Heptachlor epoxide


R.T.: 5.252 min
Delta R.T.: 0.056 min
Response: 5683929
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

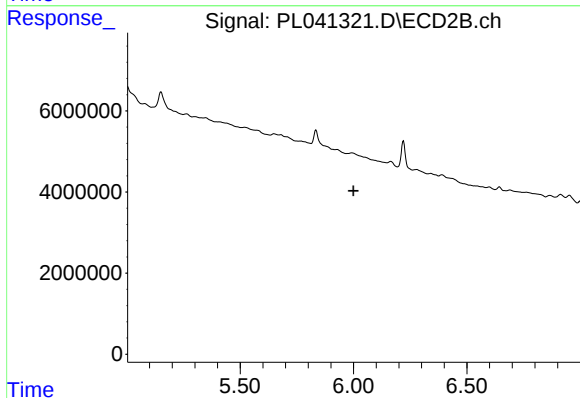


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.000 min
Response: 0
Conc: N.D.

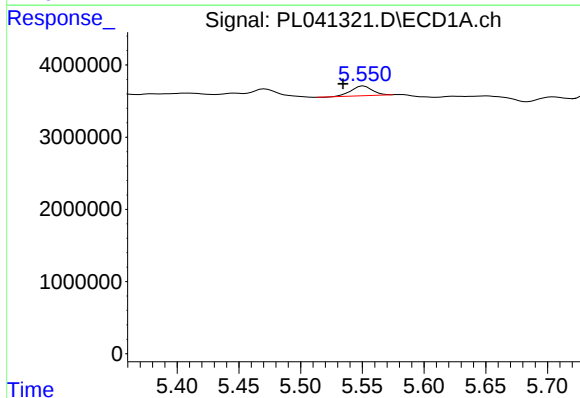


#9 Endosulfan I

R.T.: 5.551 min
Delta R.T.: 0.017 min
Response: 1599384
Conc: 0.27 ng/ml

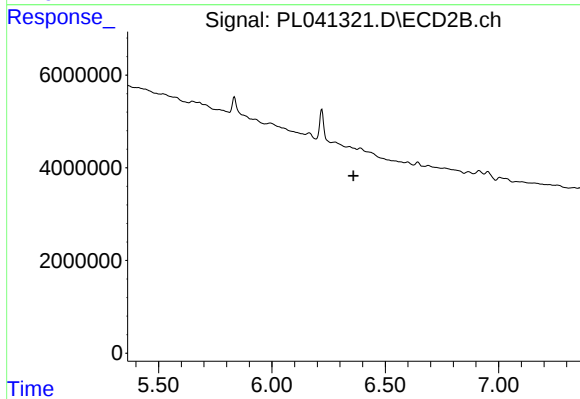

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.360 min
Response: 0
Conc: N.D.

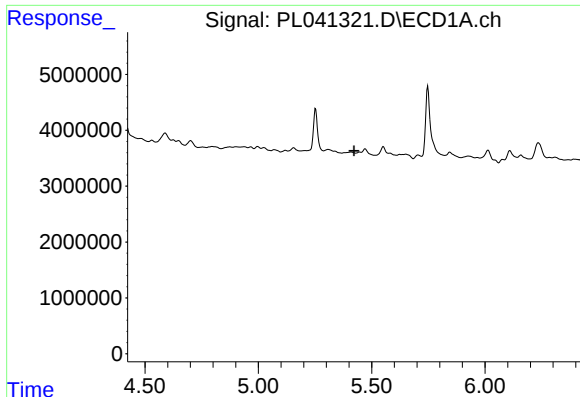

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.423 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

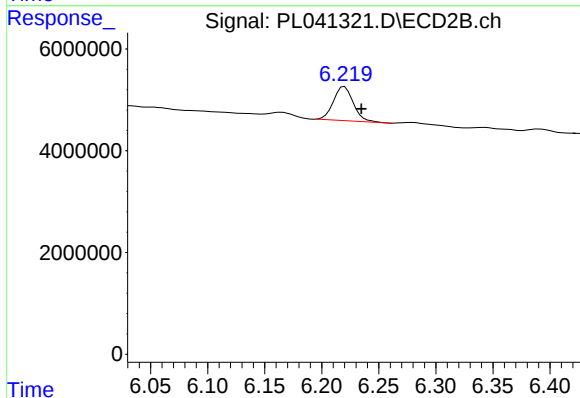


#10 gamma-Chlordane

R.T.: 6.220 min
Delta R.T.: -0.015 min
Response: 8152516
Conc: 2.91 ng/ml

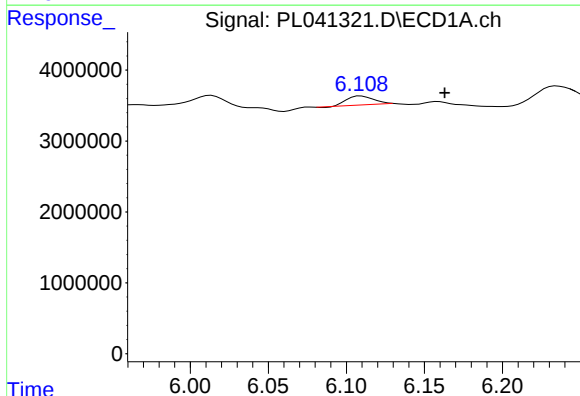


#16 4,4'-DDD

R.T.: 6.109 min
Delta R.T.: -0.054 min
Response: 1574238
Conc: 0.35 ng/ml

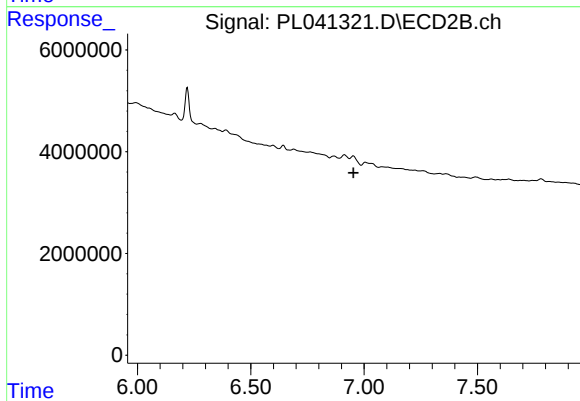

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.954 min
Response: 0
Conc: N.D.

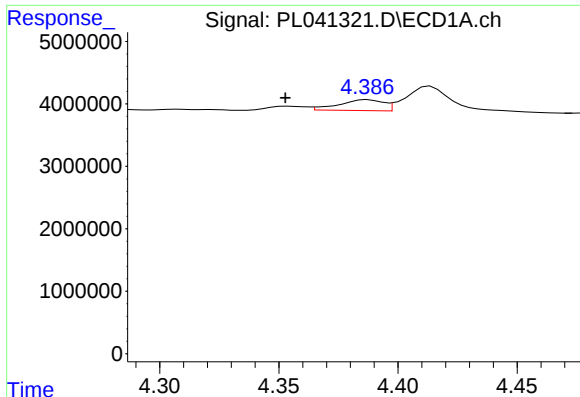

#23 Chlordane-1


R.T.: 4.387 min
Delta R.T.: 0.035 min
Response: 2275524
Conc: 8.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

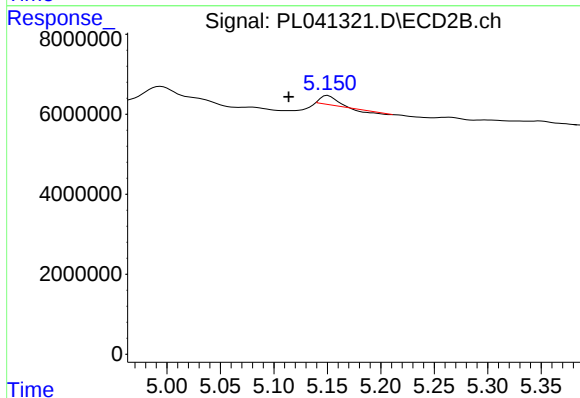


#23 Chlordane-1

R.T.: 5.151 min
Delta R.T.: 0.037 min
Response: 1318528
Conc: 10.68 ng/ml

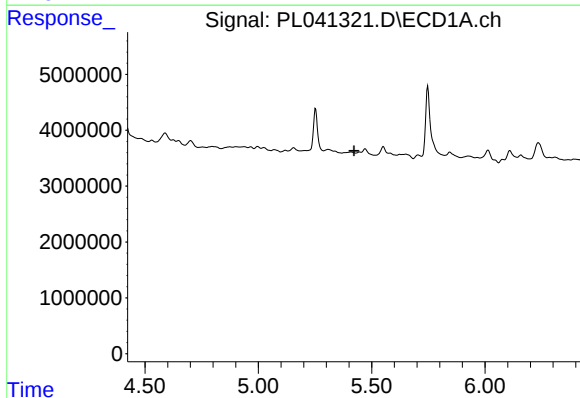


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.423 min
Response: 0
Conc: N.D.

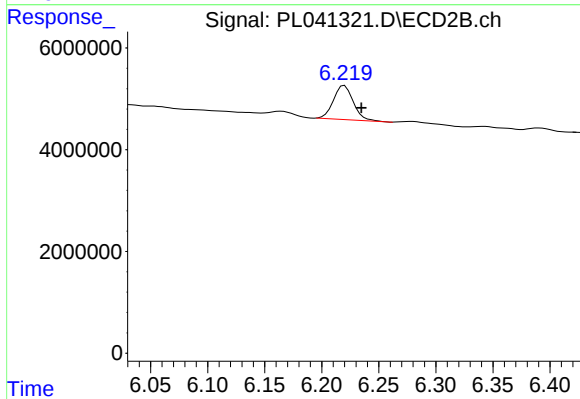

#25 Chlordane-3


R.T.: 6.220 min
Delta R.T.: -0.015 min
Response: 8152516
Conc: 20.22 ng/ml

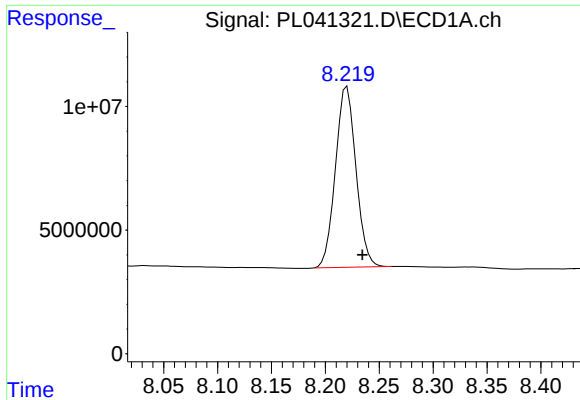

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: -0.014 min
Response: 96800558
Conc: 18.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

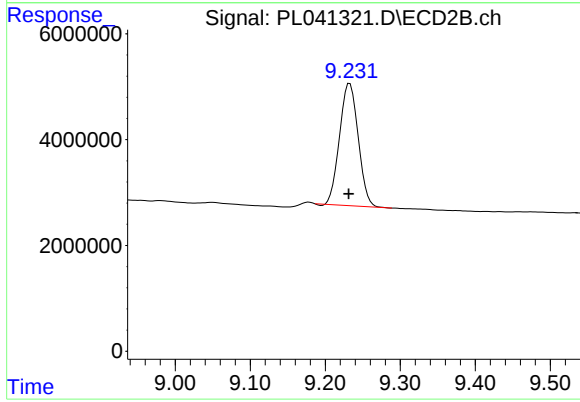

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.001 min
Response: 39842783
Conc: 15.41 ng/ml