

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102418\
 Data File : PL041328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2018 00:07
 Operator : AJ\SJ
 Sample : J5200-14
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 01:12:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.104	120.6E6	63598604	21.996	22.809
28)	SA Decachlor...	8.220	9.233	113.2E6	48416281	21.780	18.724
Target Compounds							
2)	A alpha-BHC	3.876f	0.000	489024	0	0.062	N.D. #
3)	MA gamma-BHC...	4.236f	0.000	2017803	0	0.276	N.D. #
6)	B beta-BHC	4.413f	4.994f	12925423	1679918	4.074	1.048 #
7)	B delta-BHC	0.000	5.150f	0	1310861	N.D.	0.399 #
8)	B Heptachlo...	5.252f	0.000	1848673	0	0.282	N.D. #
9)	A Endosulfan I	5.557	0.000	3121319	0	0.521	N.D. #
16)	A 4,4'-DDD	6.232f	0.000	4176725	0	0.925	N.D. #
23)	Chlordane-1	4.413	5.150	12925423	1310861	50.645	10.613 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102418\
Data File : PL041328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2018 00:07
Operator : AJ\SJ
Sample : J5200-14
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 01:12:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

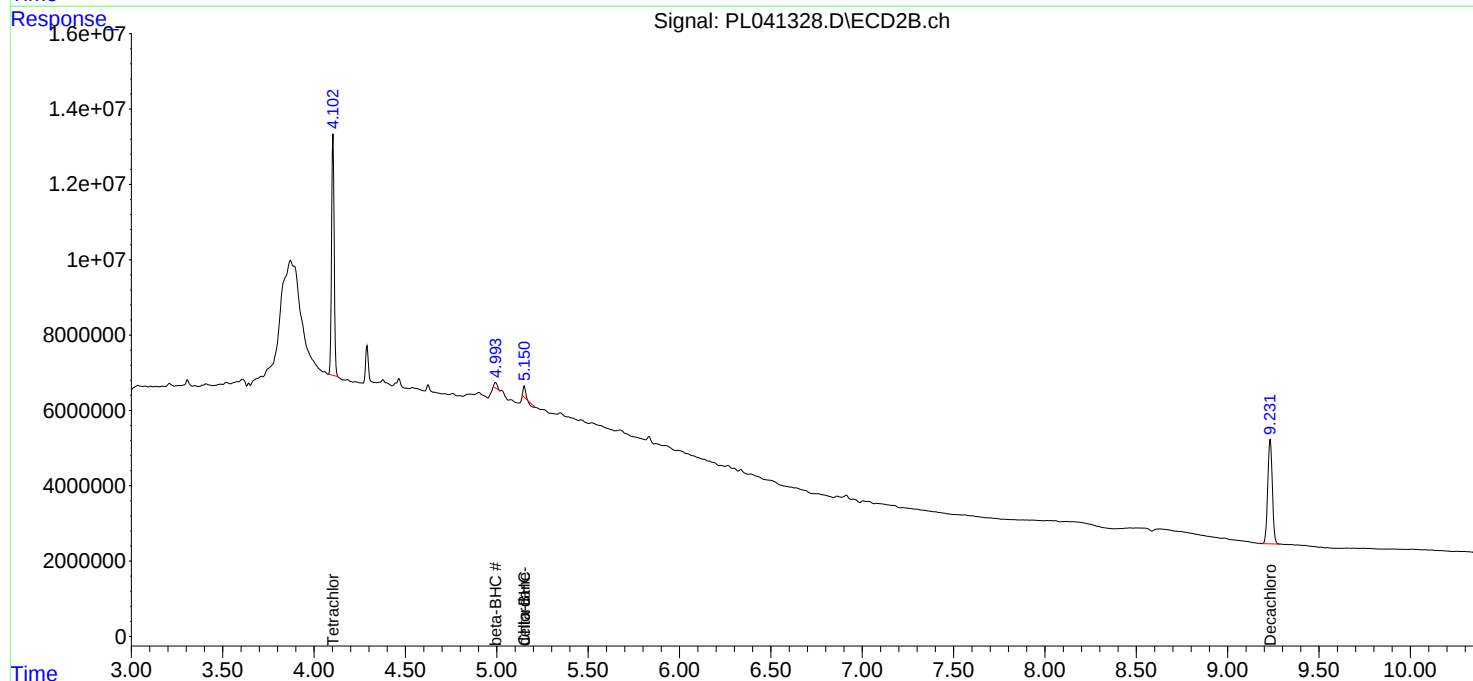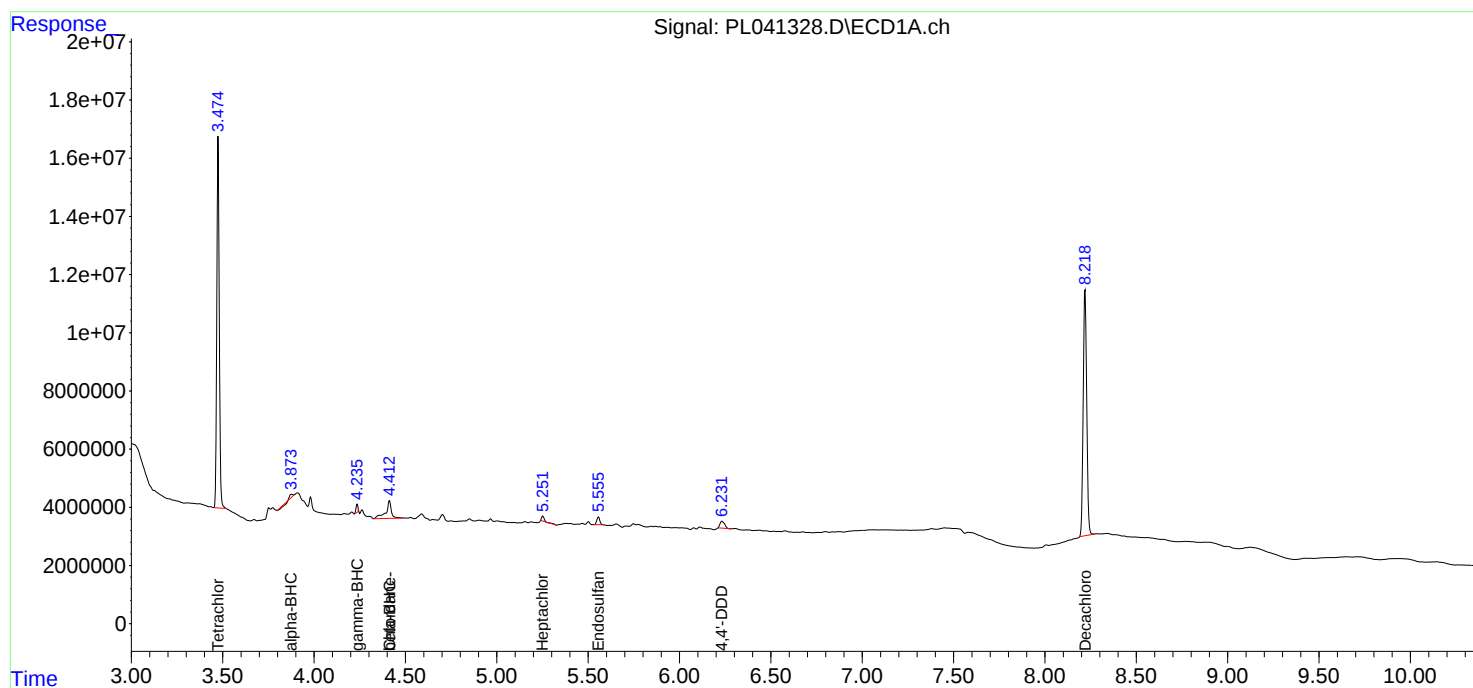


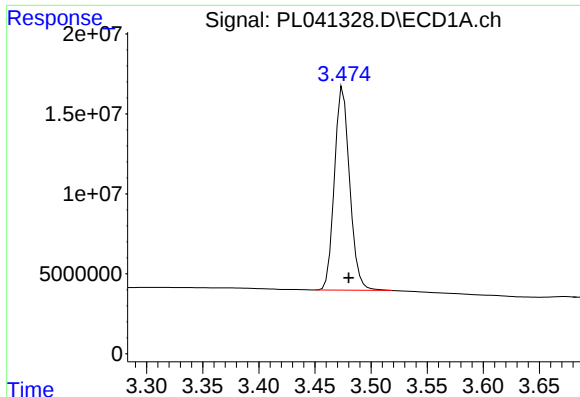

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: -0.005 min
Response: 120552052
Conc: 22.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

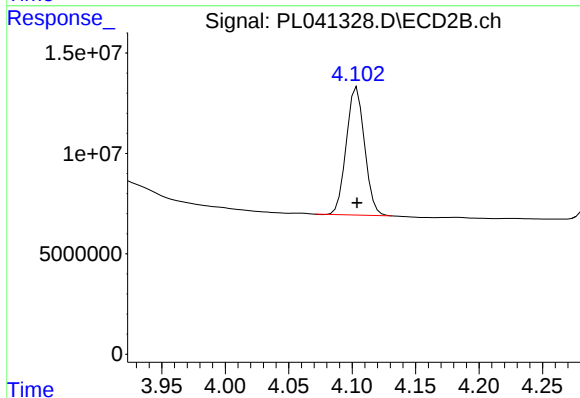


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 63598604
Conc: 22.81 ng/ml

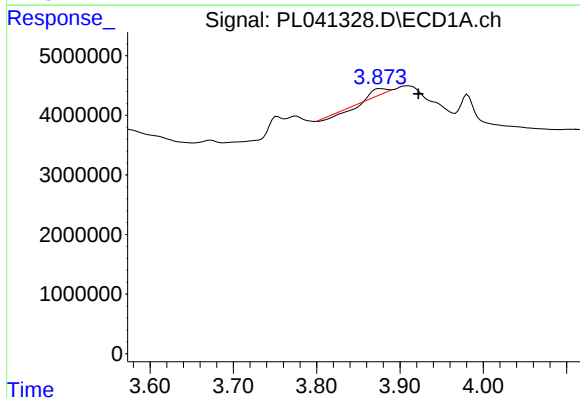


#2 alpha-BHC

R.T.: 3.876 min
Delta R.T.: -0.046 min
Response: 489024
Conc: 0.06 ng/ml

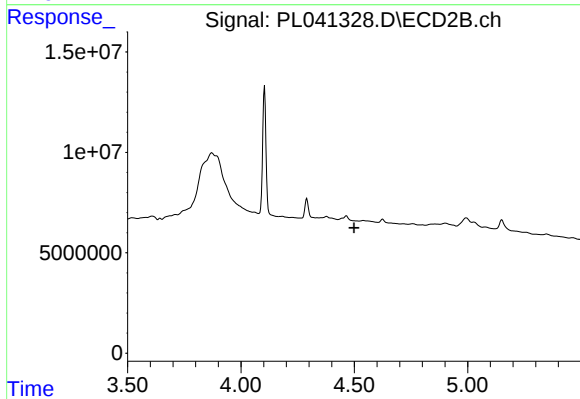

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.499 min
Response: 0
Conc: N.D.

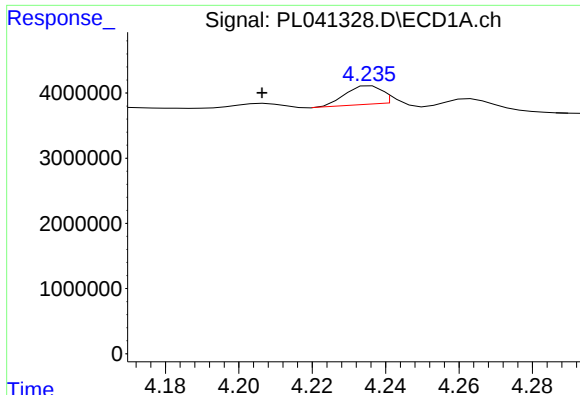

#3 gamma-BHC (Lindane)


R.T.: 4.236 min
Delta R.T.: 0.030 min
Response: 2017803
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

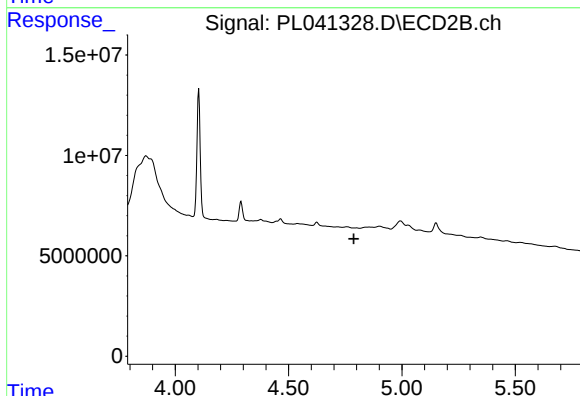


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.788 min
Response: 0
Conc: N.D.

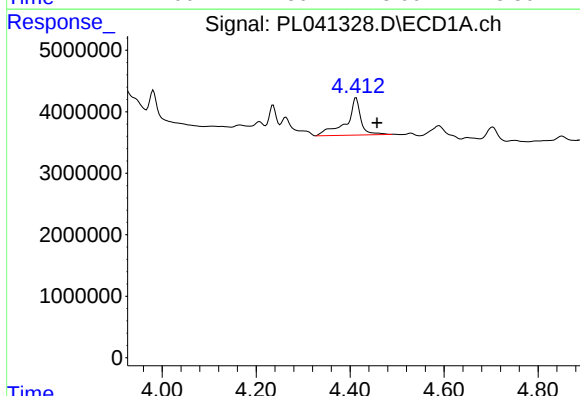


#6 beta-BHC

R.T.: 4.413 min
Delta R.T.: -0.045 min
Response: 12925423
Conc: 4.07 ng/ml

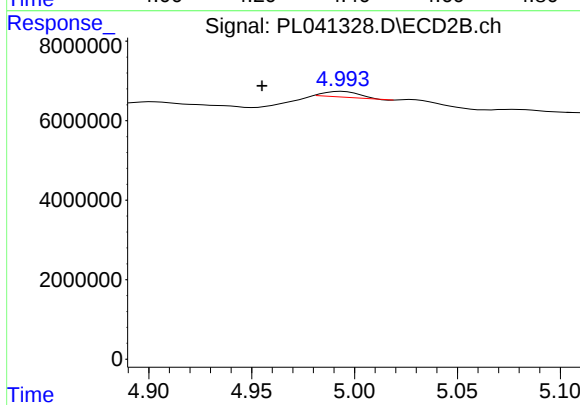

#6 beta-BHC


R.T.: 4.994 min
Delta R.T.: 0.039 min
Response: 1679918
Conc: 1.05 ng/ml

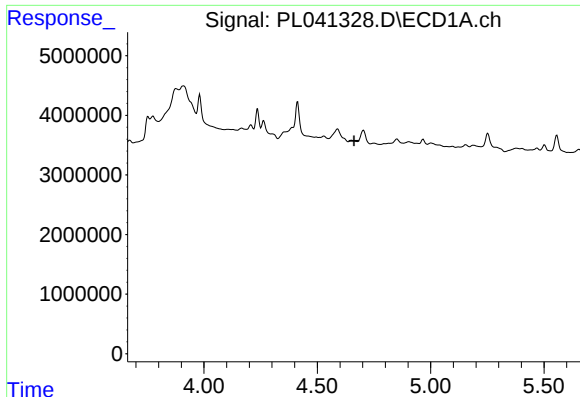

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.662 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

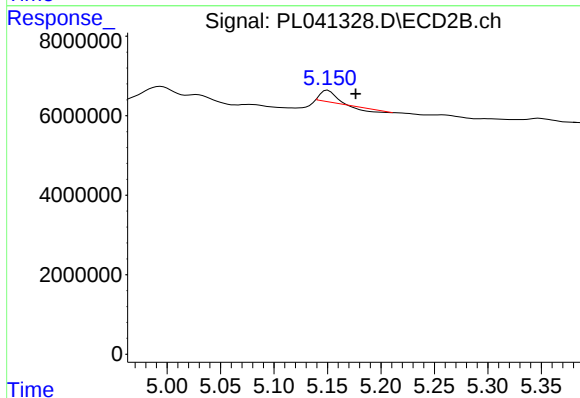


#7 delta-BHC

R.T.: 5.150 min
Delta R.T.: -0.026 min
Response: 1310861
Conc: 0.40 ng/ml

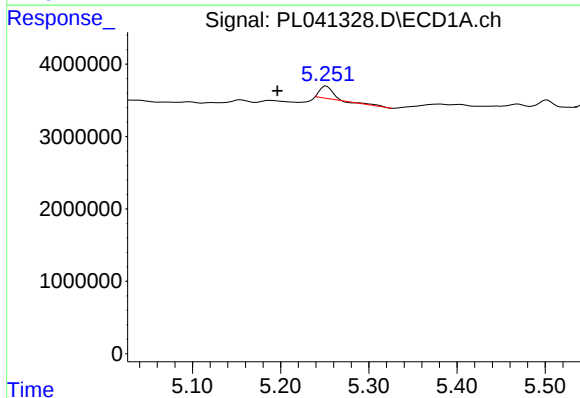


#8 Heptachlor epoxide

R.T.: 5.252 min
Delta R.T.: 0.056 min
Response: 1848673
Conc: 0.28 ng/ml

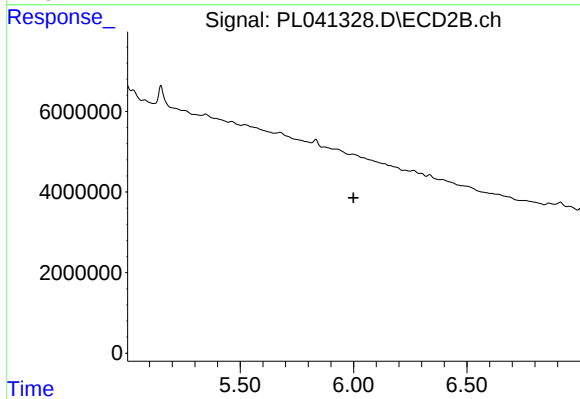

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.000 min
Response: 0
Conc: N.D.

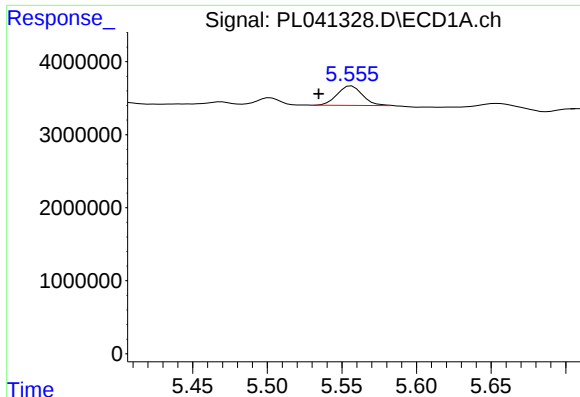

#9 Endosulfan I


R.T.: 5.557 min
Delta R.T.: 0.022 min
Response: 3121319
Conc: 0.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

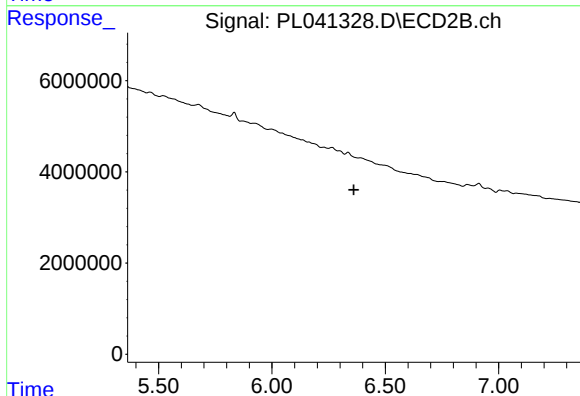


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.360 min
Response: 0
Conc: N.D.

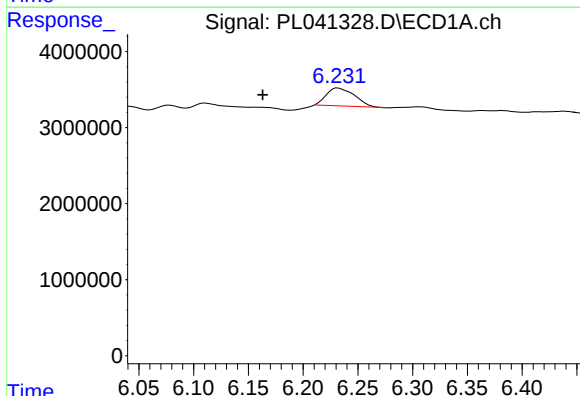


#16 4,4'-DDD

R.T.: 6.232 min
Delta R.T.: 0.069 min
Response: 4176725
Conc: 0.92 ng/ml

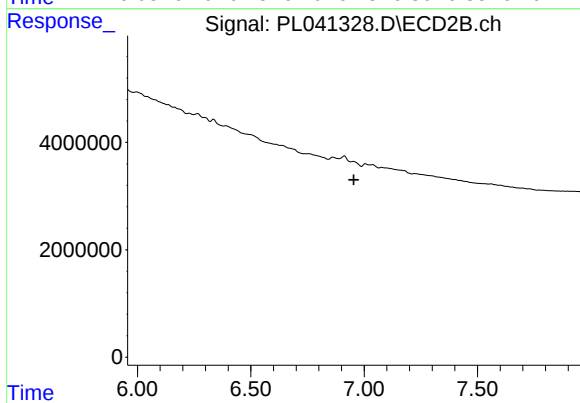

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.954 min
Response: 0
Conc: N.D.

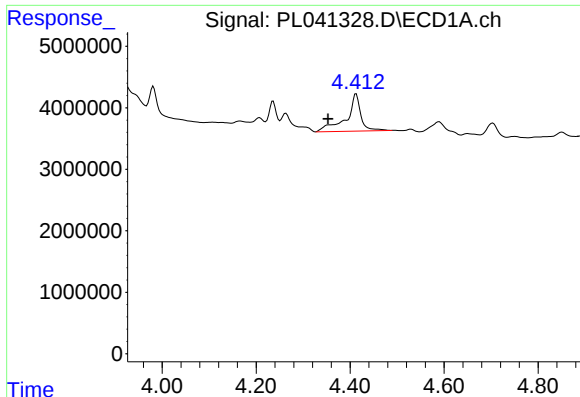

#23 Chlordane-1


R.T.: 4.413 min
Delta R.T.: 0.060 min
Response: 12925423
Conc: 50.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

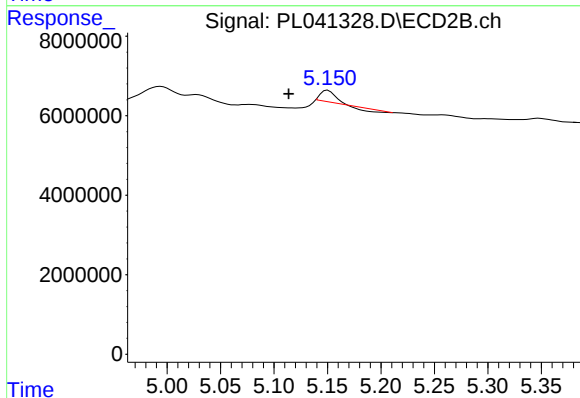


#23 Chlordane-1

R.T.: 5.150 min
Delta R.T.: 0.037 min
Response: 1310861
Conc: 10.61 ng/ml

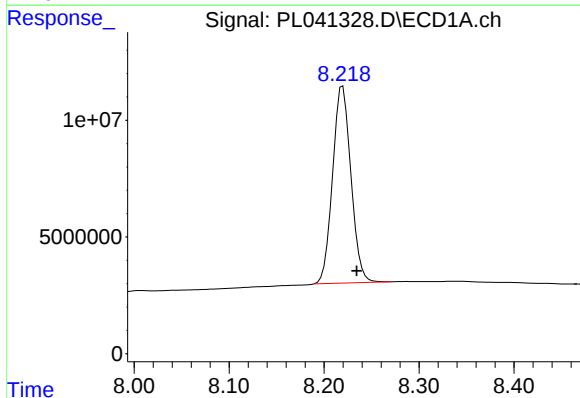

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: -0.015 min
Response: 113247608
Conc: 21.78 ng/ml

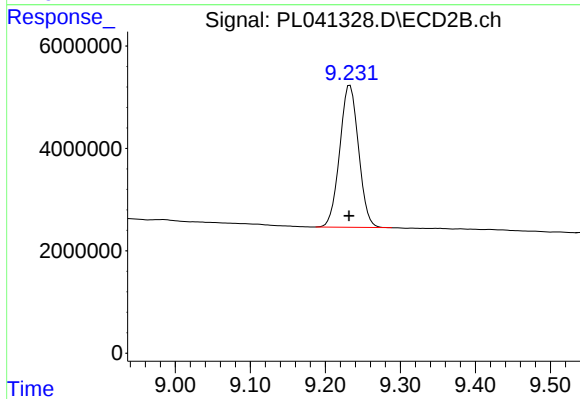

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.002 min
Response: 48416281
Conc: 18.72 ng/ml